

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082025\
 Data File : PS031524.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2025 14:47
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 16:46:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
 Quant Title : 8080.M
 QLast Update : Fri Aug 08 03:17:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.287	7.742	1704.6E6	483.1E6	537.051	571.526
Target Compounds							
1) T	Dalapon	0.000	2.654f	0	76438923	N.D.	28.726
2) T	3,5-DICHL...	6.463	0.000	589170	0	<MDL	N.D. #
5) T	DICAMBA	7.472	0.000	1049212	0	<MDL	N.D. #
7) T	MCPA	7.825	8.246f	950457	37753471	<MDL	13.457 #
8) T	DICHLORPROP	8.207	8.671	278349	2163027	<MDL	1.620 #
10) T	Pentachlo...	8.714	9.511	6820947	45682816	<MDL	1.312 #
11) T	2,4,5-TP ...	9.290	9.899	9421617	31592160	<MDL	2.409 #
12) T	2,4,5-T	9.601	0.000	4028164	0	<MDL	N.D. #
13) T	2,4-DB	10.175	10.910	2542367	6865461	1.323	7.116 #
14) T	DINOSEB	11.370	0.000	3990565	0	<MDL	N.D. #
15) T	Picloram	11.202	0.000	1447466	0	<MDL	N.D. #
16) T	DCPA	11.660	0.000	5954727	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082025\
Data File : PS031524.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 14:47
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 16:46:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
Quant Title : 8080.M
QLast Update : Fri Aug 08 03:17:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

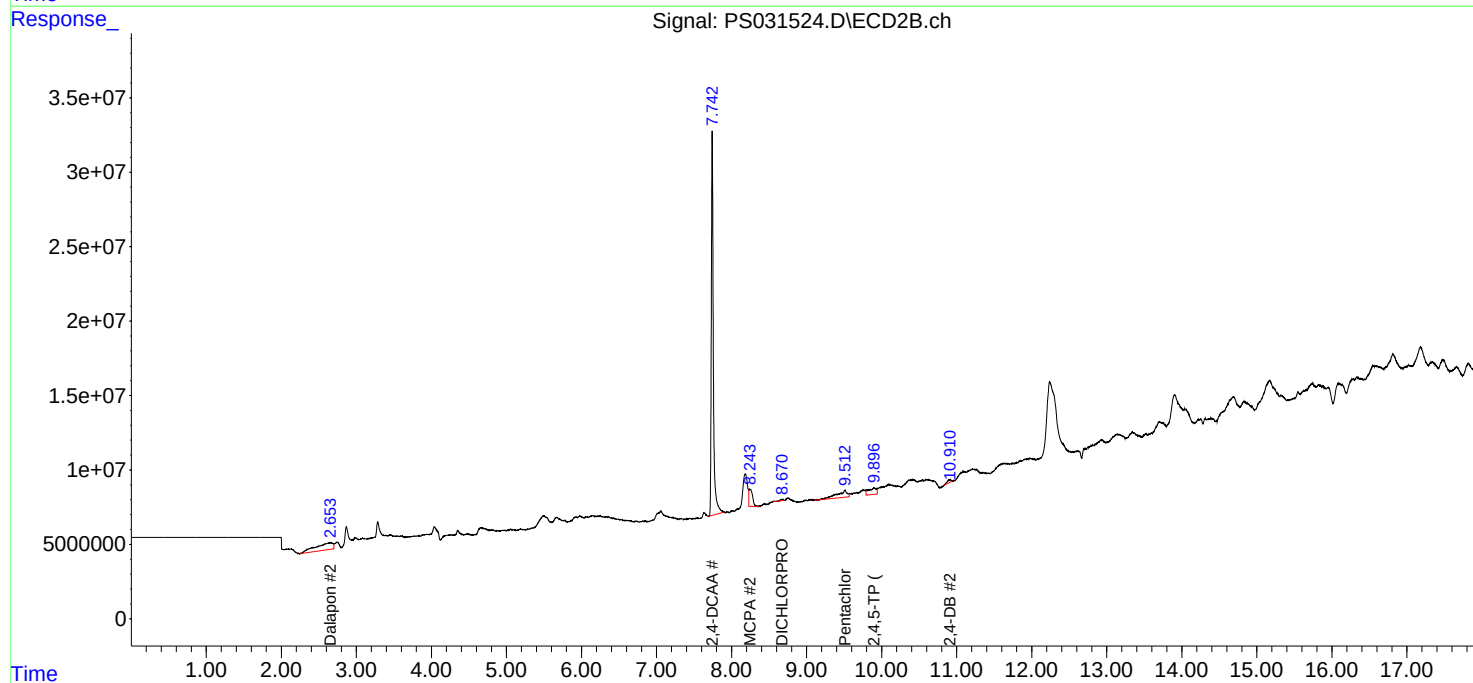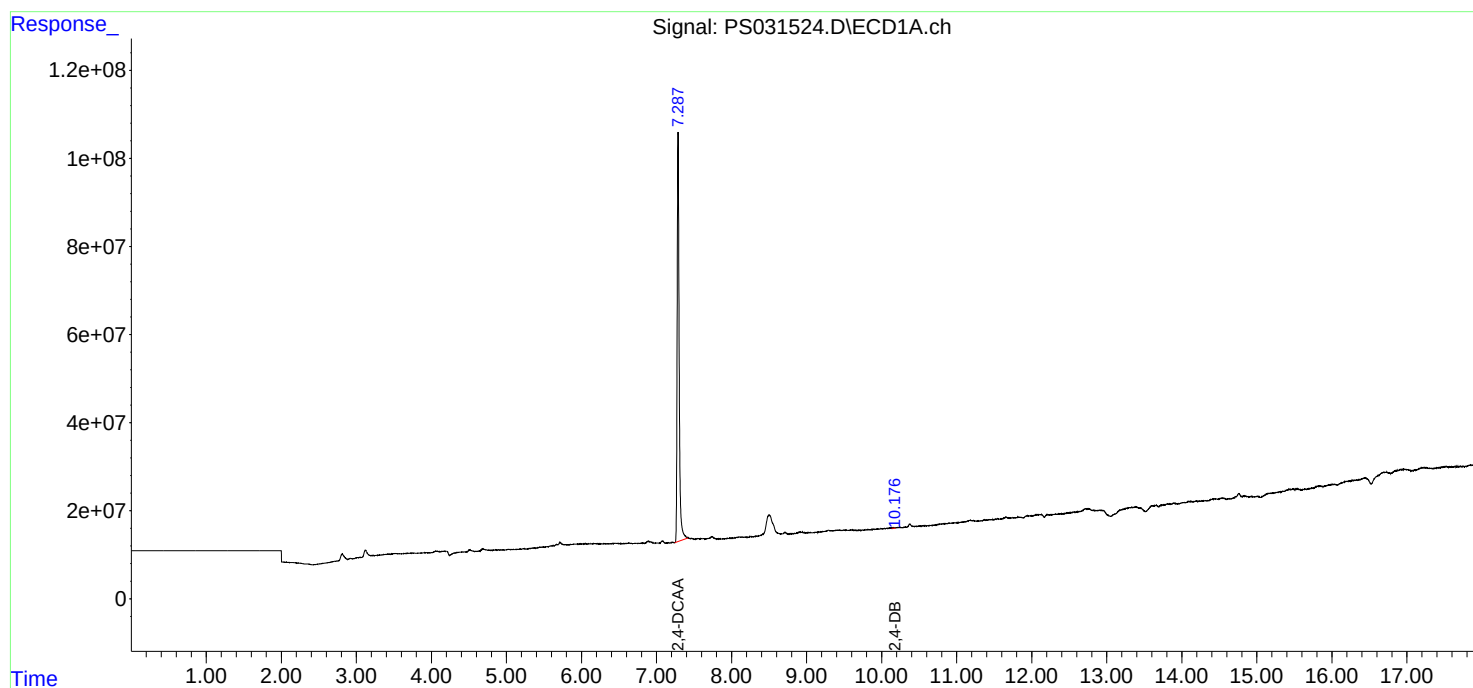


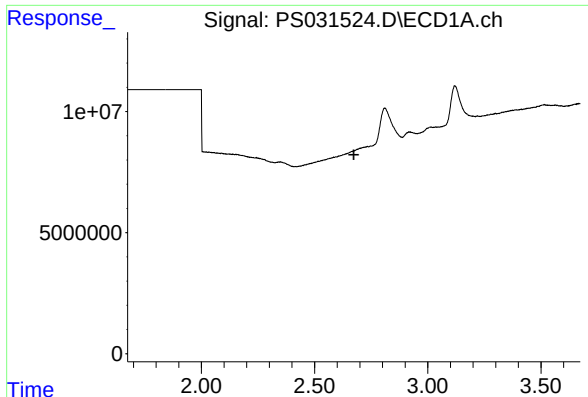

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

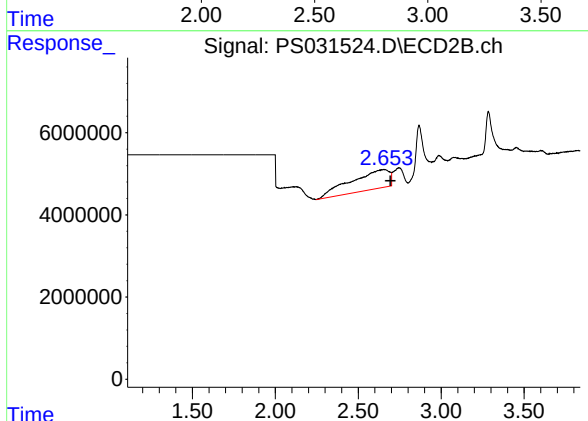


#1 Dalapon

R.T.: 2.654 min
Delta R.T.: -0.041 min
Response: 76438923
Conc: 28.73 ng/ml

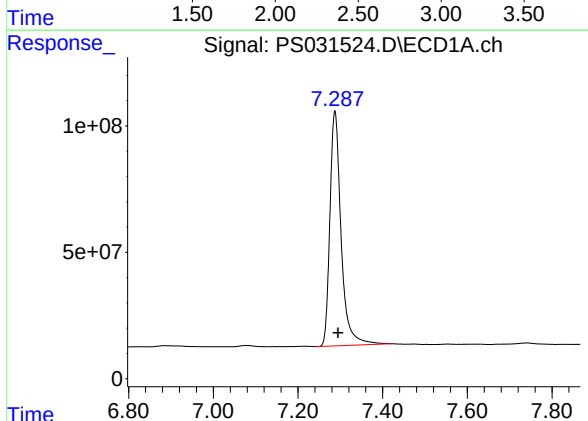


#4 2,4-DCAA

R.T.: 7.287 min
Delta R.T.: -0.008 min
Response: 1704594358
Conc: 537.05 ng/ml

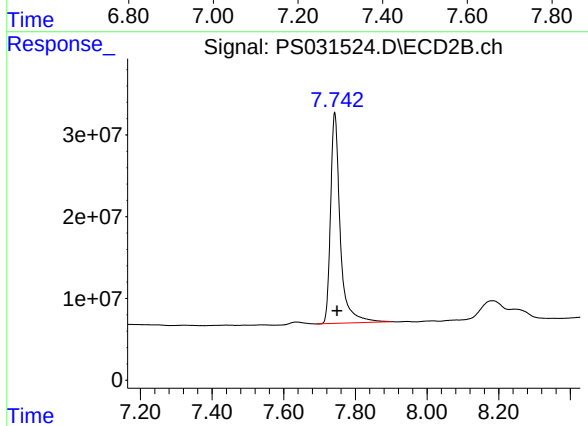

#4 2,4-DCAA


R.T.: 7.742 min
Delta R.T.: -0.007 min
Response: 483133317
Conc: 571.53 ng/ml

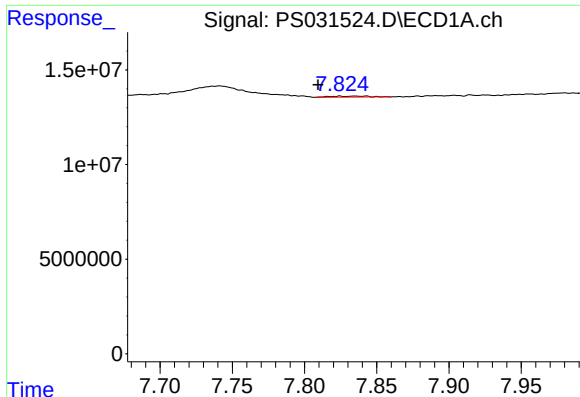

#7 MCPA


R.T.: 7.825 min
Delta R.T.: 0.015 min
Response: 950457
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

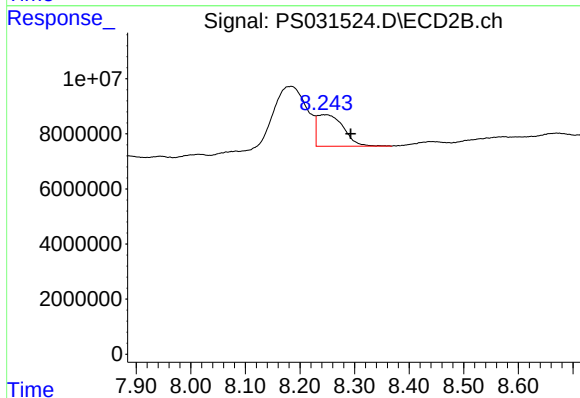


#7 MCPA

R.T.: 8.246 min
Delta R.T.: -0.048 min
Response: 37753471
Conc: 13.46 ug/ml

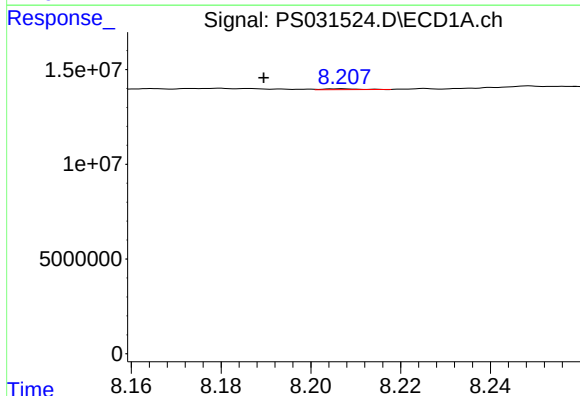


#8 DICHLORPROP

R.T.: 8.207 min
Delta R.T.: 0.017 min
Response: 278349
Conc: N.D.

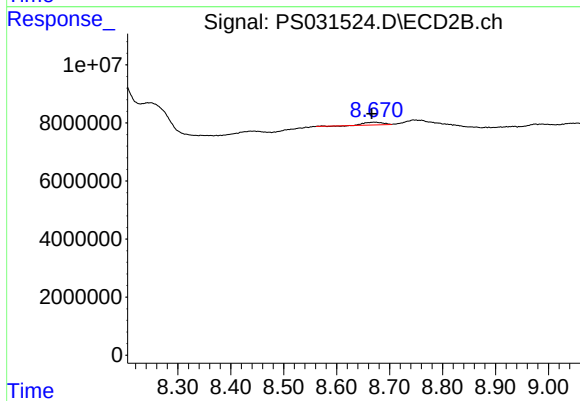

#8 DICHLORPROP


R.T.: 8.671 min
Delta R.T.: 0.005 min
Response: 2163027
Conc: 1.62 ng/ml

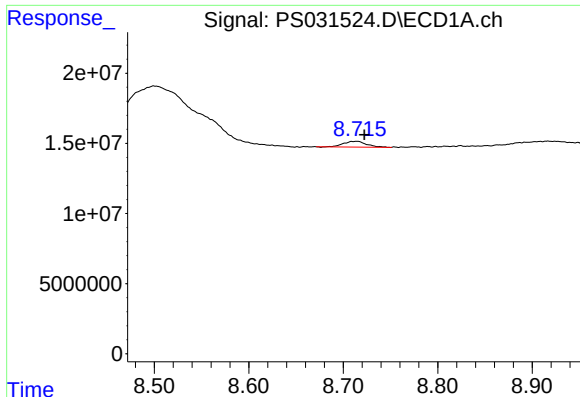

#10 Pentachlorophenol


R.T.: 8.714 min
Delta R.T.: -0.008 min
Response: 6820947
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

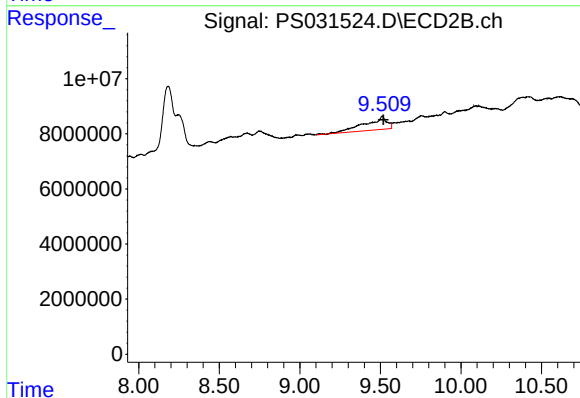


#10 Pentachlorophenol

R.T.: 9.511 min
Delta R.T.: -0.007 min
Response: 45682816
Conc: 1.31 ng/ml

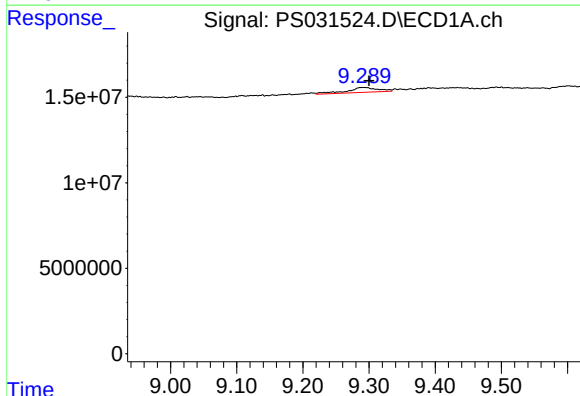


#11 2,4,5-TP (SILVEX)

R.T.: 9.290 min
Delta R.T.: -0.010 min
Response: 9421617
Conc: N.D.

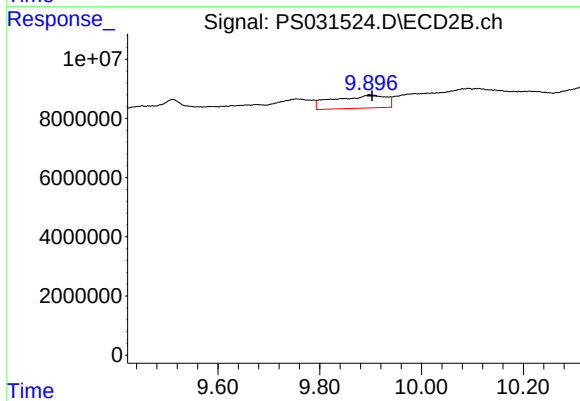

#11 2,4,5-TP (SILVEX)


R.T.: 9.899 min
Delta R.T.: -0.003 min
Response: 31592160
Conc: 2.41 ng/ml

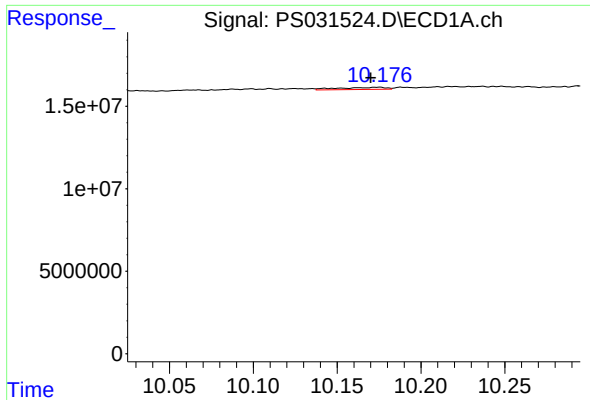

#13 2,4-DB

R.T.: 10.175 min
Delta R.T.: 0.004 min
Response: 2542367
Conc: 1.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

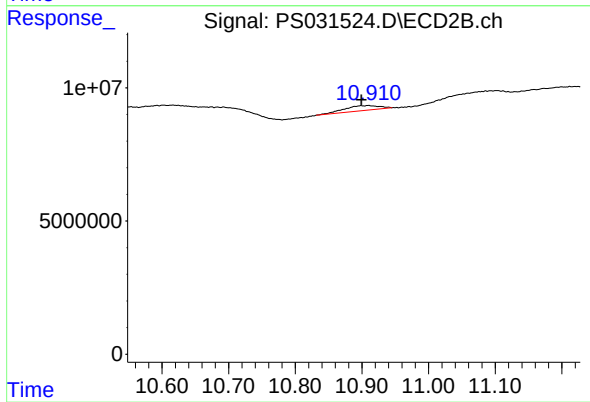

#13 2,4-DB

R.T.: 10.910 min
Delta R.T.: 0.010 min
Response: 6865461
Conc: 7.12 ng/ml