

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082025\
 Data File : PS031520.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2025 10:45
 Operator : AR\AJ
 Sample : Q2879-13RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 OU4-TS-GRILLO-TSCP09-081425RE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/21/2025
 Supervised By :mohammad ahmed 08/25/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 11:04:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
 Quant Title : 8080.M
 QLast Update : Fri Aug 08 03:17:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.272	7.749	159.5E6	122.6E6	50.268m	144.978m#

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082025\
Data File : PS031520.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 10:45
Operator : AR\AJ
Sample : Q2879-13RE
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
OU4-TS-GRILLO-TSCP09-081425RE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/21/2025
Supervised By : mohammad ahmed 08/25/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 11:04:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
Quant Title : 8080.M
QLast Update : Fri Aug 08 03:17:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

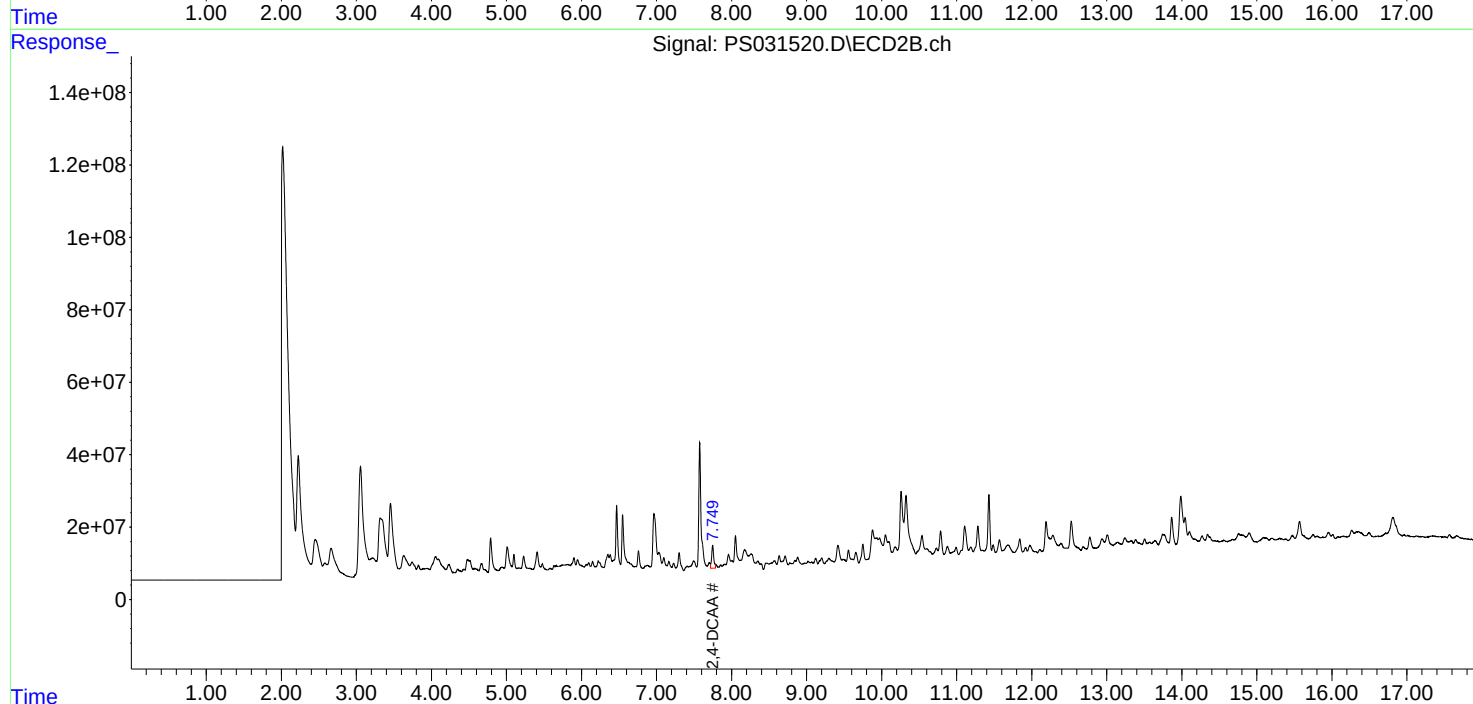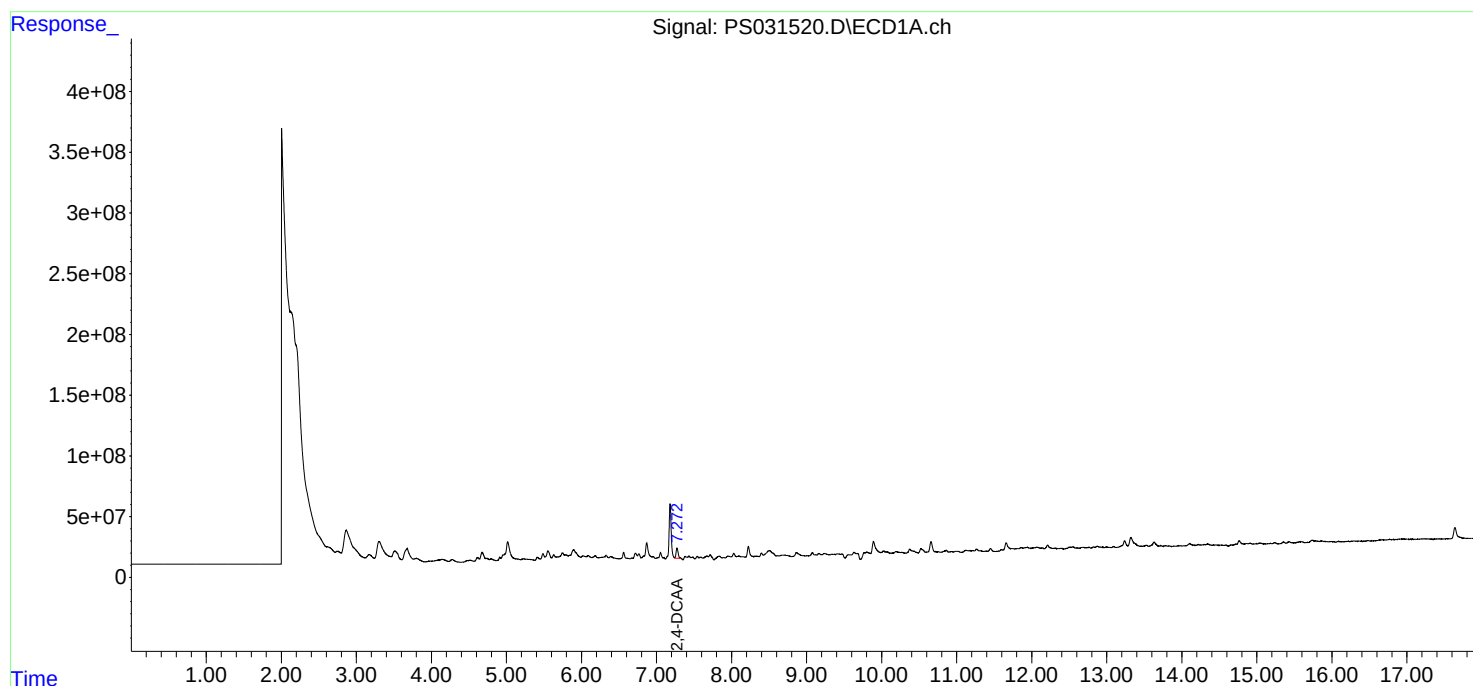

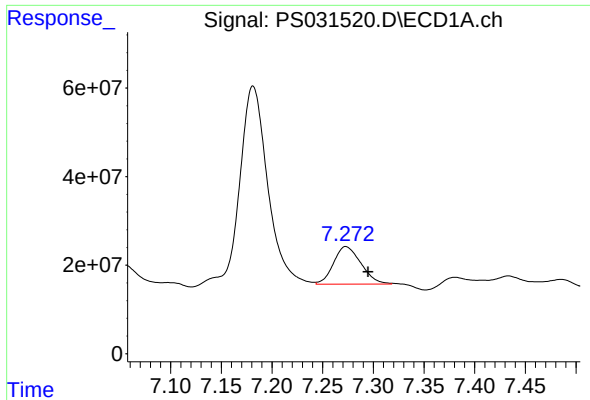


#4 2,4-DCAA

R.T.: 7.272 min
Delta R.T.: -0.023 min
Response: 159548668
Conc: 50.27 ng/ml

Instrument :
ECD_S
ClientSampleId :
OU4-TS-GRILLO-TSCP09-081425RE

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/21/2025
Supervised By :mohammad ahmed 08/25/2025

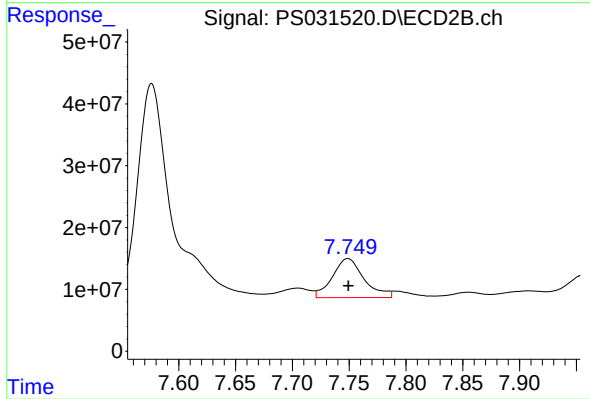

#4 2,4-DCAA

R.T.: 7.749 min
Delta R.T.: 0.000 min
Response: 122555726
Conc: 144.98 ng/ml m