

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082120\
 Data File : PS011876.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2020 18:18
 Operator : DD\AJ
 Sample : L3506-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 00:49:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.220	6.916	219.5E6	140.5E6	201.247	262.649 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	43064198	N.D.	52.350
3) T	4-Nitroph...	6.986	0.000	1981539	0	3.364	N.D. #
5) T	DICAMBA	7.481	7.049	9175730	8356621	2.240	3.868 #
6) T	MCP	7.629	0.000	5783503	0	1.810	N.D. #
7) T	MCPA	7.699	0.000	123.3E6	0	27.112	N.D. #
8) T	DICHLORPROP	0.000	7.740	0	22282306	N.D.	39.463
9) T	2,4-D	8.400	0.000	121.3E6	0	107.474	N.D. #
11) T	2,4,5-TP ...	0.000	8.765	0	8982051	N.D.	3.072
12) T	2,4,5-T	9.412	0.000	11518133	0	1.944	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081120\
Data File : PS011876.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2020 18:18
Operator : DD\AJ
Sample : L3506-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 00:49:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

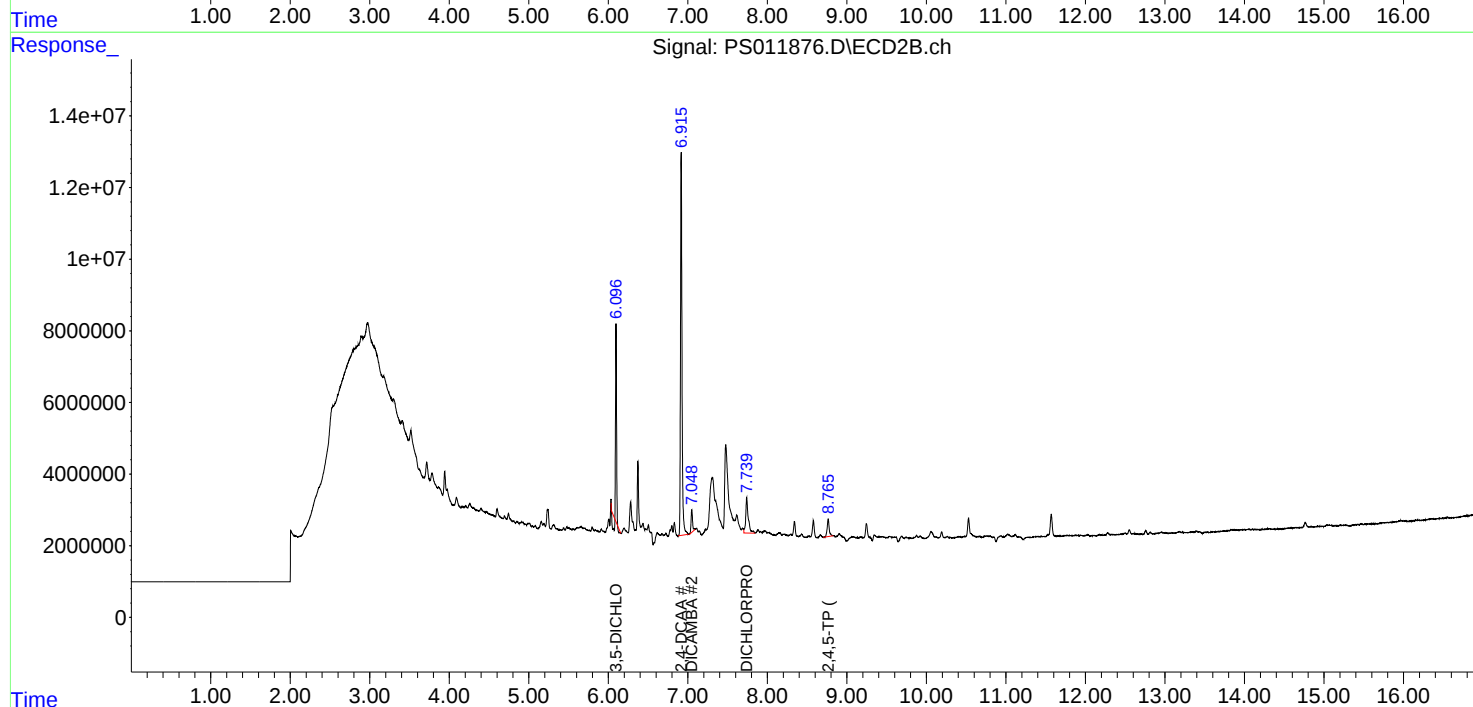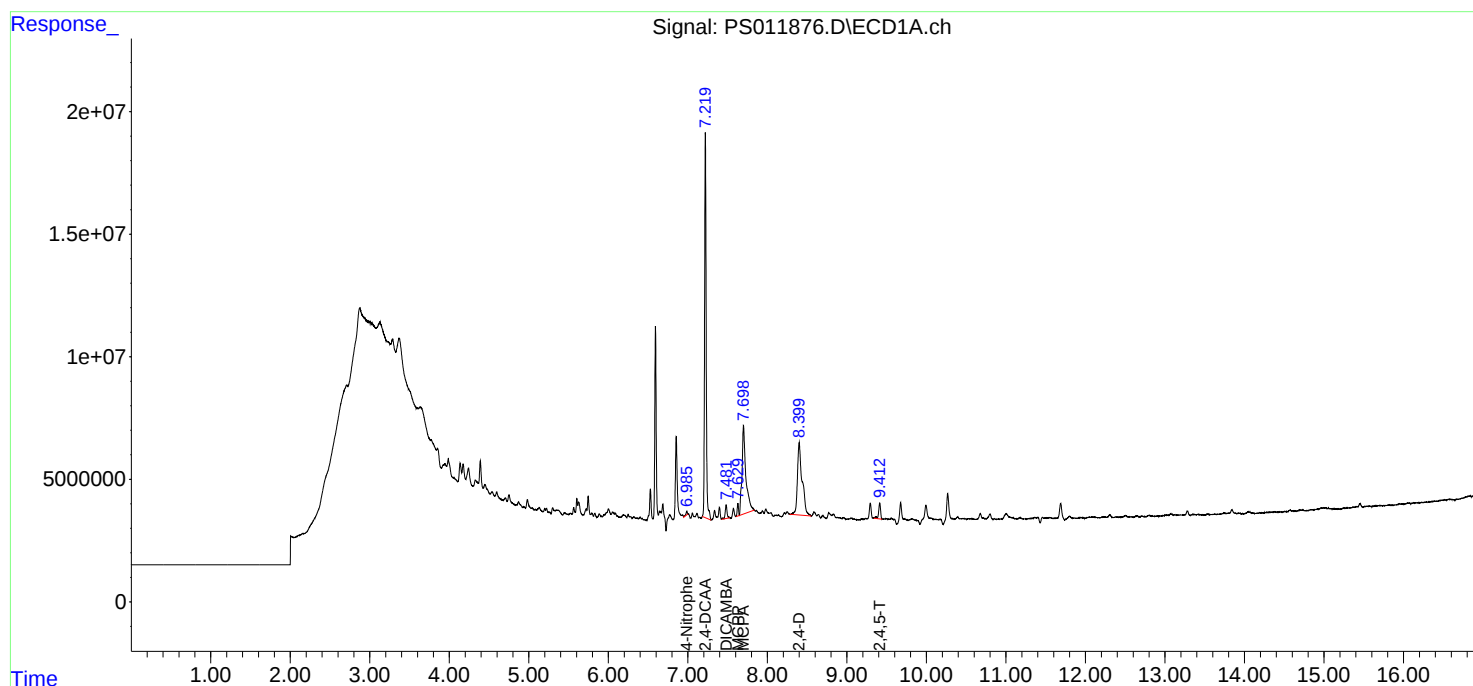


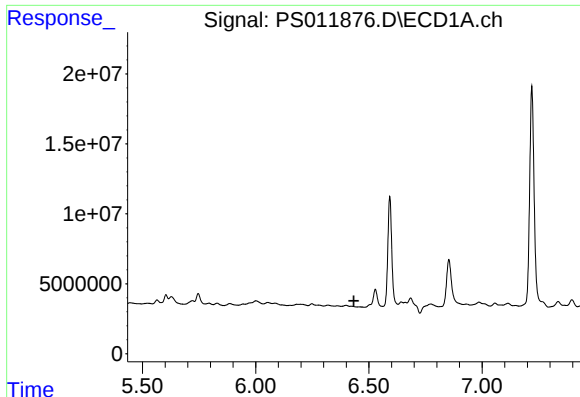

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

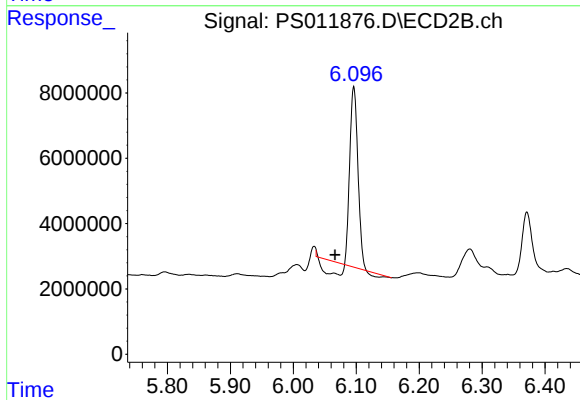


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.030 min
Response: 43064198
Conc: 52.35 ng/ml

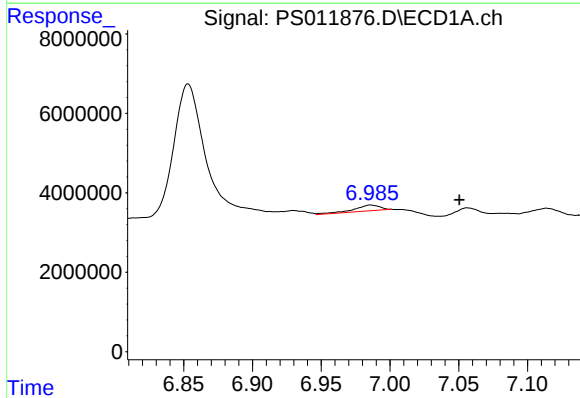


#3 4-Nitrophenol

R.T.: 6.986 min
Delta R.T.: -0.064 min
Response: 1981539
Conc: 3.36 ng/ml

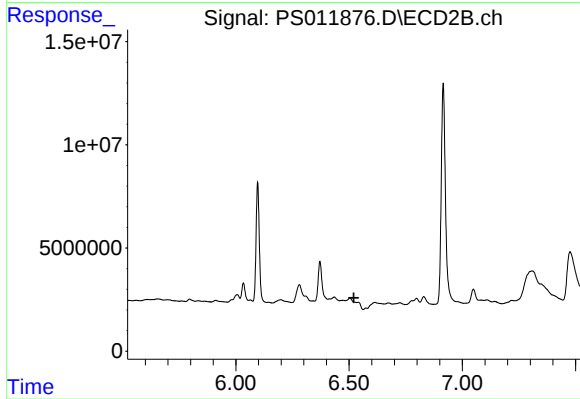

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

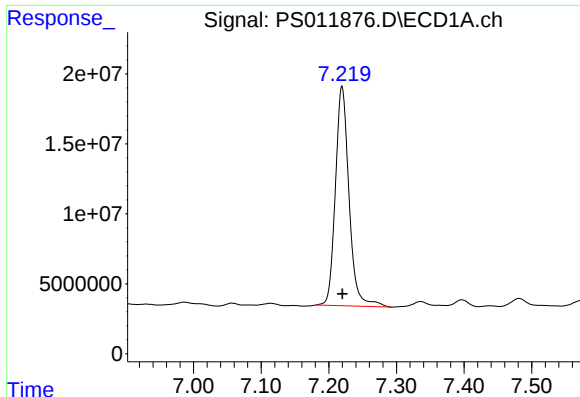

#4 2,4-DCAA


R.T.: 7.220 min
Delta R.T.: 0.000 min
Response: 219513375
Conc: 201.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

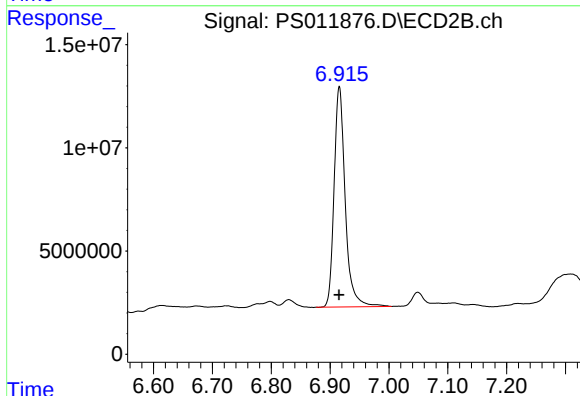


#4 2,4-DCAA

R.T.: 6.916 min
Delta R.T.: 0.000 min
Response: 140461247
Conc: 262.65 ng/ml

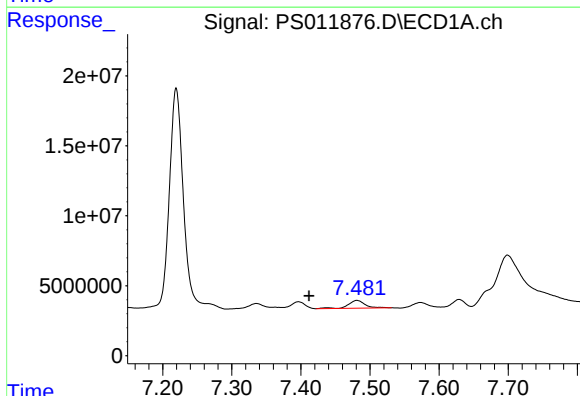


#5 DICAMBA

R.T.: 7.481 min
Delta R.T.: 0.070 min
Response: 9175730
Conc: 2.24 ng/ml

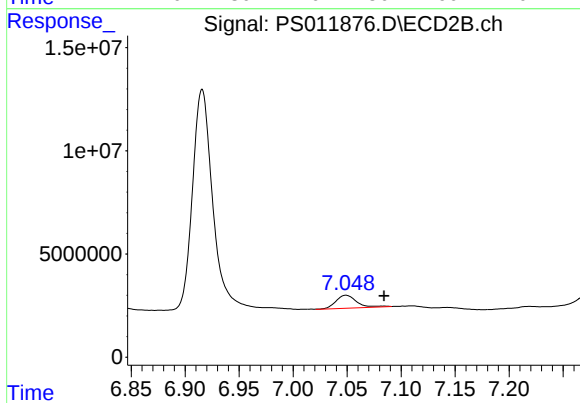

#5 DICAMBA


R.T.: 7.049 min
Delta R.T.: -0.035 min
Response: 8356621
Conc: 3.87 ng/ml

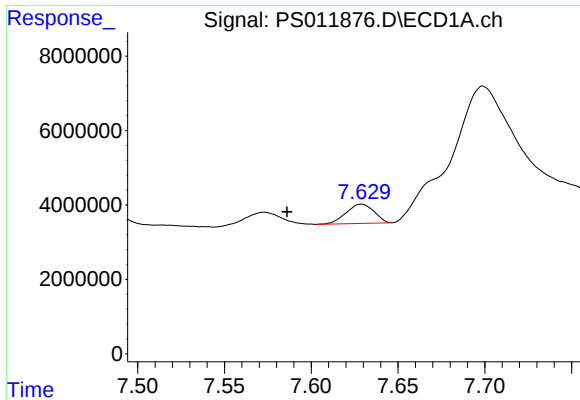

#6 MCPP


R.T.: 7.629 min
Delta R.T.: 0.043 min
Response: 5783503
Conc: 1.81 ug/ml

Instrument :
ECD_S
ClientSampleId :

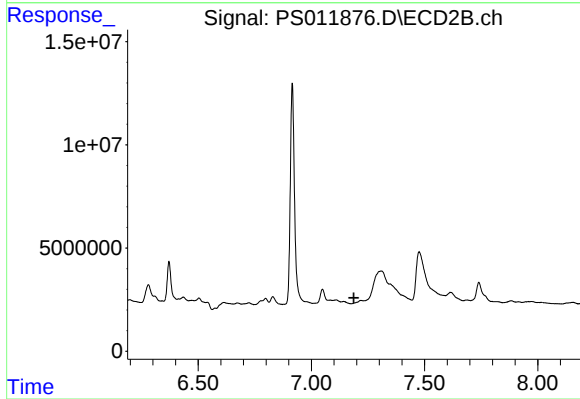


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

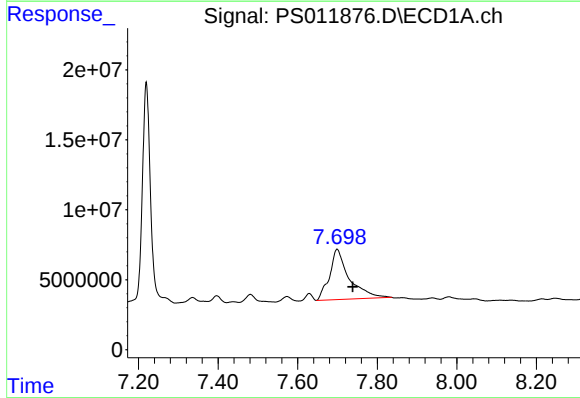


#7 MCPA

R.T.: 7.699 min
Delta R.T.: -0.039 min
Response: 123320501
Conc: 27.11 ug/ml

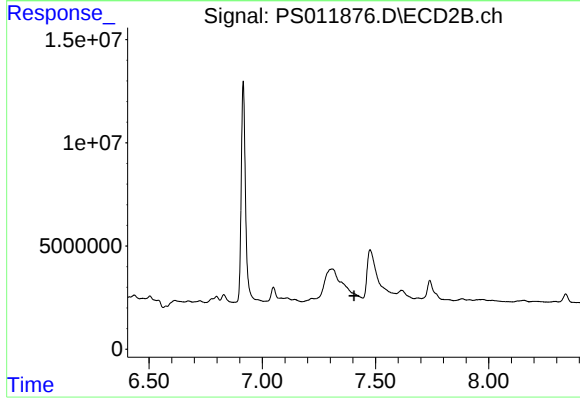

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.405 min
Response: 0
Conc: N.D.

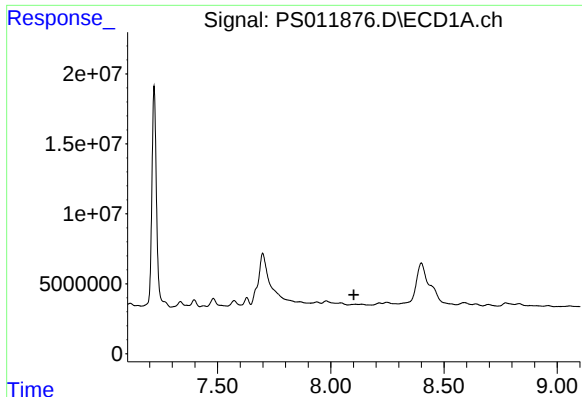

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

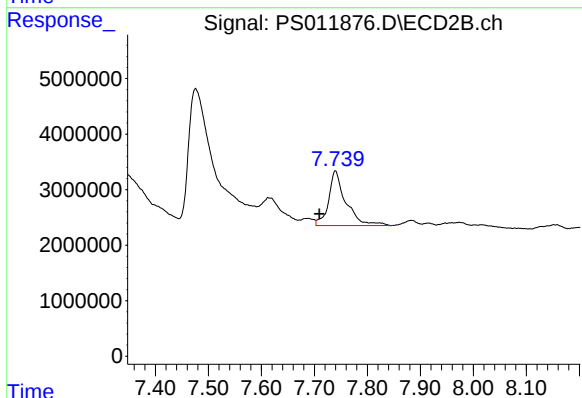


#8 DICHLORPROP

R.T.: 7.740 min
Delta R.T.: 0.030 min
Response: 22282306
Conc: 39.46 ng/ml

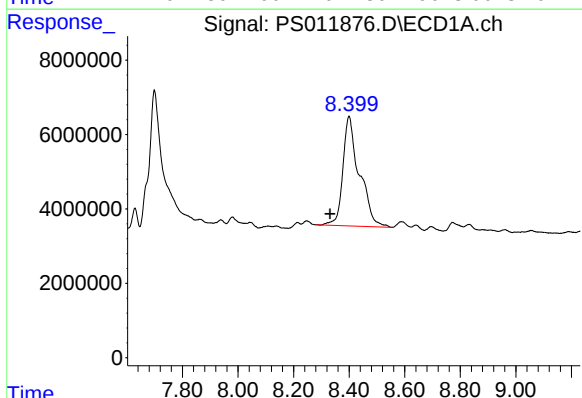


#9 2,4-D

R.T.: 8.400 min
Delta R.T.: 0.067 min
Response: 121348317
Conc: 107.47 ng/ml

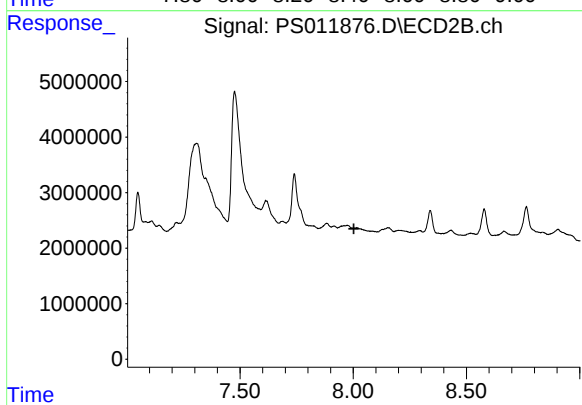

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

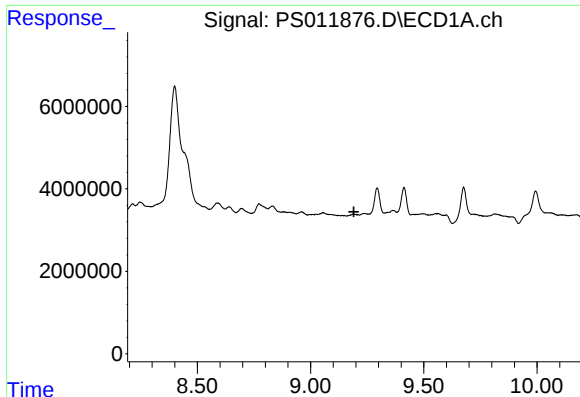

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

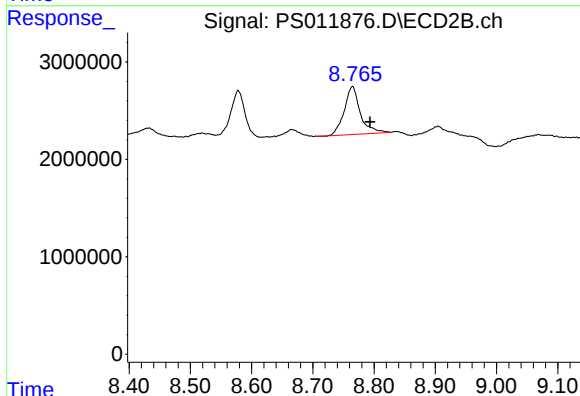


#11 2,4,5-TP (SILVEX)

R.T.: 8.765 min
Delta R.T.: -0.029 min
Response: 8982051
Conc: 3.07 ng/ml

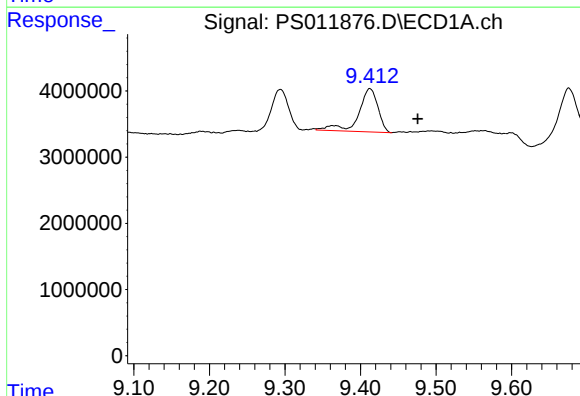

#12 2,4,5-T

R.T.: 9.412 min
Delta R.T.: -0.063 min
Response: 11518133
Conc: 1.94 ng/ml

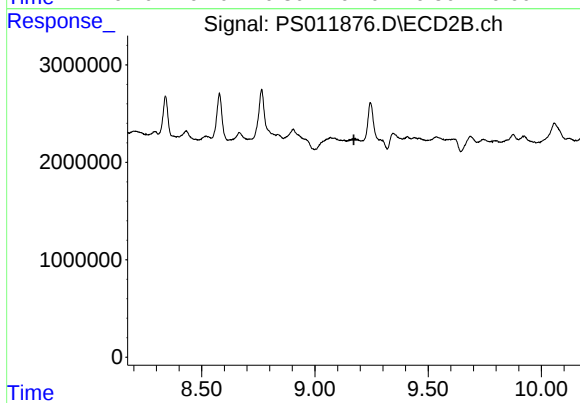

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.