

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082319\
 Data File : PS006298.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2019 12:25
 Operator : SM\AJ
 Sample : K4089-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 OK-01-082119

Manual Integrations
 APPROVED

Ankita
 8/26/2019 3:17:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 02:06:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	5.474	5.204	300.7E6	193.0E6	348.376m	392.436

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082319\
Data File : PS006298.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2019 12:25
Operator : SM\AJ
Sample : K4089-05
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
OK-01-082119


Manual Integrations
APPROVED

Ankita
8/26/2019 3:17:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 02:06:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

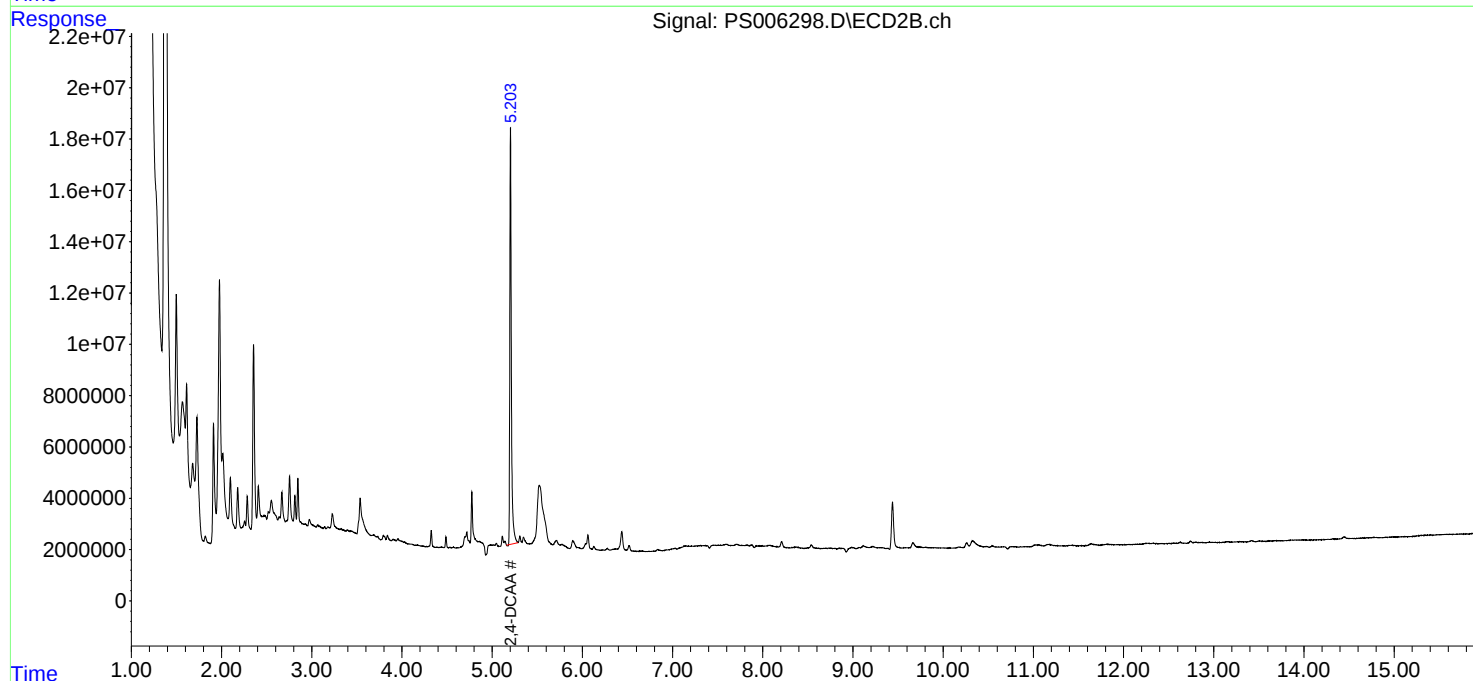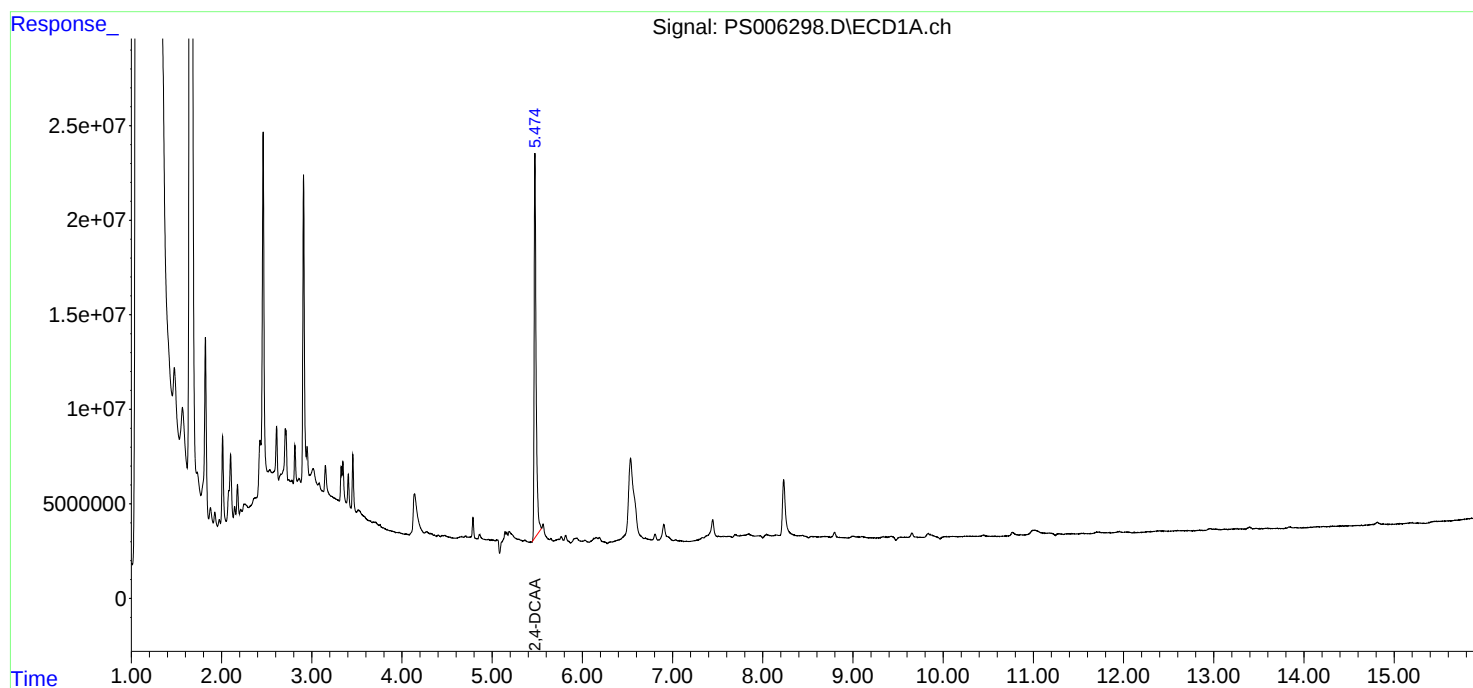

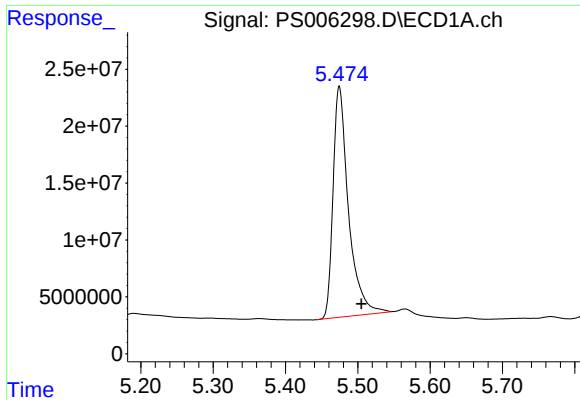


#4 2,4-DCAA

R.T.: 5.474 min
Delta R.T.: -0.031 min
Response: 300718096
Conc: 348.38 ng/ml m

Instrument :
ECD_S
ClientSampleId :
OK-01-082119

Manual Integrations
APPROVED

Ankita
8/26/2019 3:17:15 PM

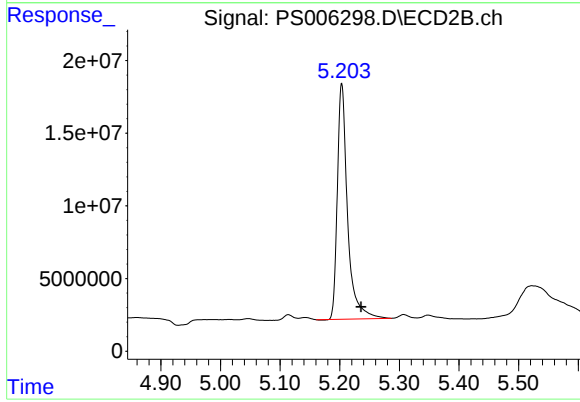

#4 2,4-DCAA

R.T.: 5.204 min
Delta R.T.: -0.032 min
Response: 193020537
Conc: 392.44 ng/ml