

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082321\
 Data File : PS016592.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Aug 2021 09:02
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 13:18:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 02 14:10:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.182	6.764	628.1E6	267.5E6	426.936	512.732
Target Compounds							
3) T	4-Nitroph...	6.984	0.000	3101951	0	3.881	N.D. #
7) T	MCPA	7.636f	0.000	18033602	0	2.927	N.D. #
10) T	Pentachlo...	8.642	0.000	1974394	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.201f	0.000	17835194	0	2.467	N.D. #
12) T	2,4,5-T	9.414	0.000	3494036	0	<MDL	N.D. #
13) T	2,4-DB	9.965	0.000	2694502	0	1.854	N.D. #
14) T	DINOSEB	11.182	0.000	4728839	0	<MDL	N.D. #
15) T	Picloram	10.985	10.824	14360933	2711016	1.439	<MDL #
16) T	DCPA	11.423	10.824f	32403798	2711016	3.066	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082321\
Data File : PS016592.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Aug 2021 09:02
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 13:18:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
Quant Title : 8080.M
QLast Update : Mon Aug 02 14:10:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

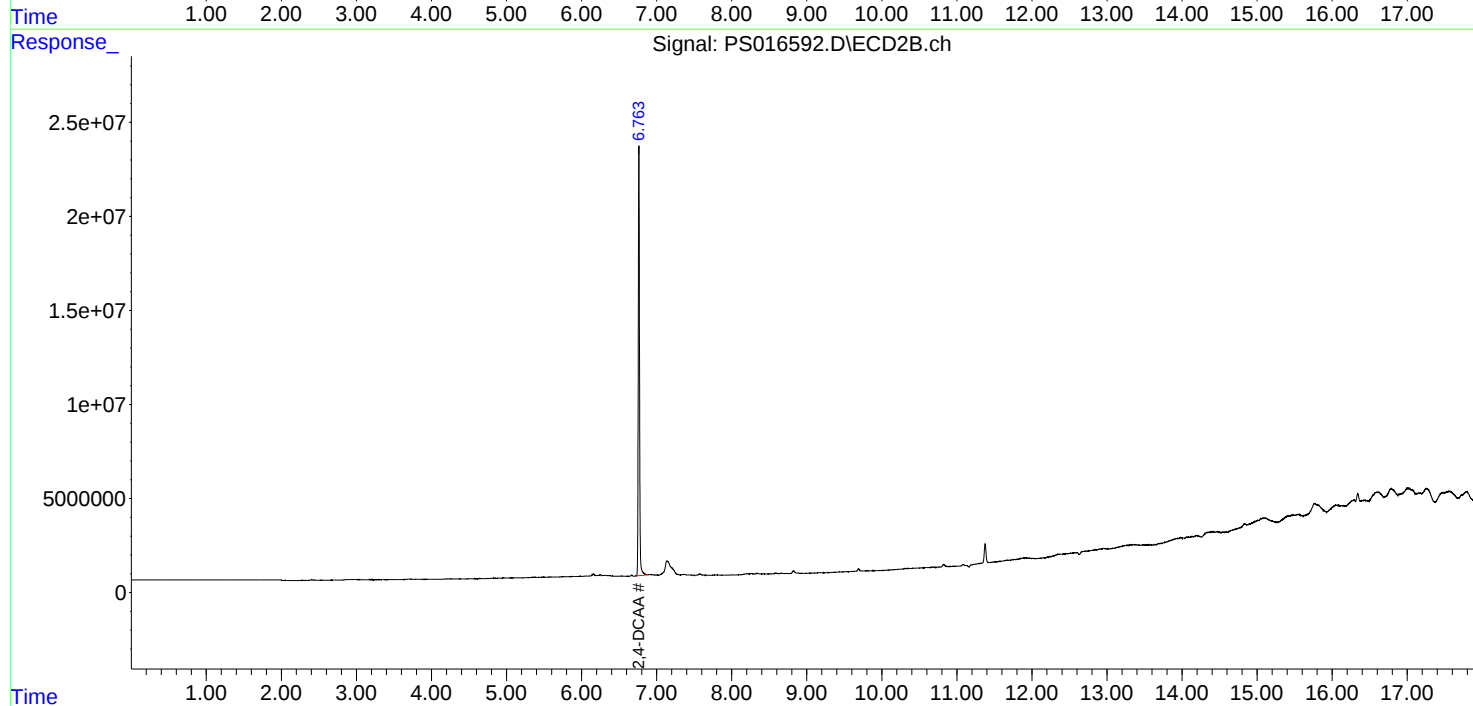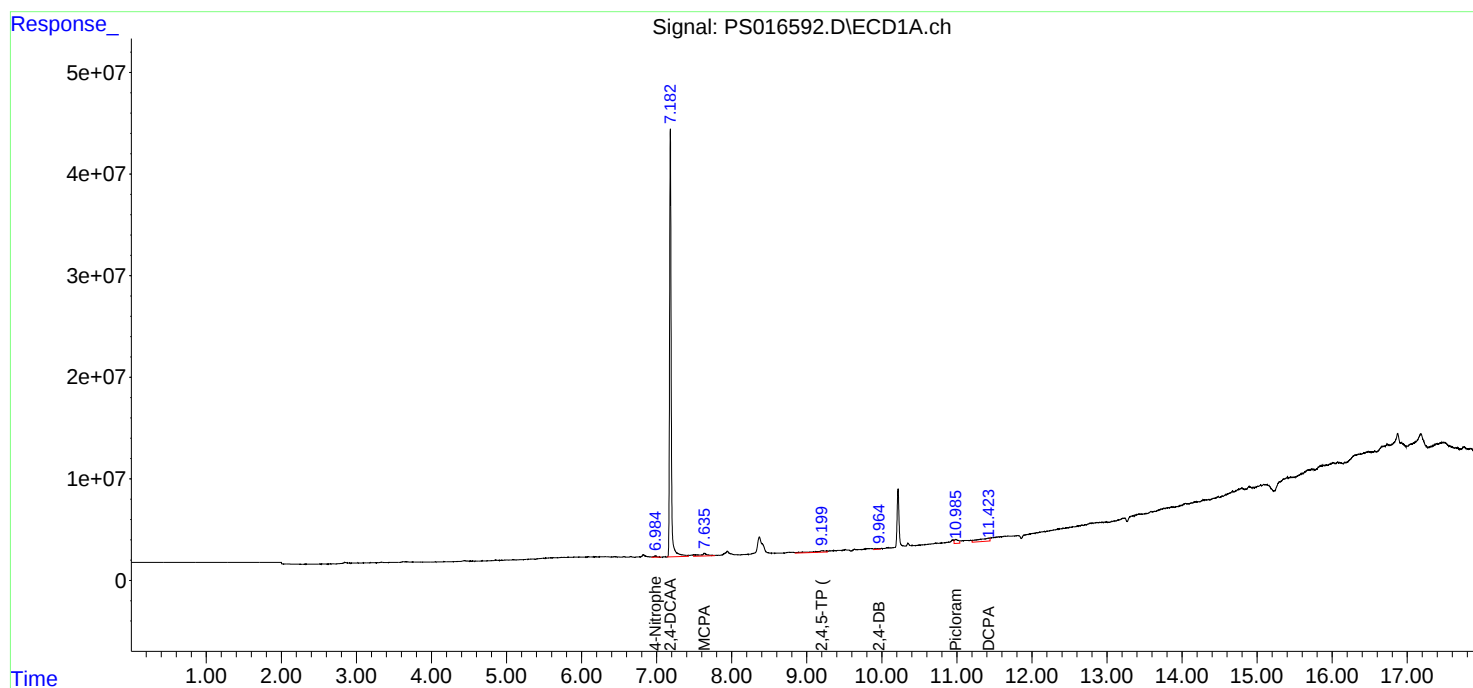


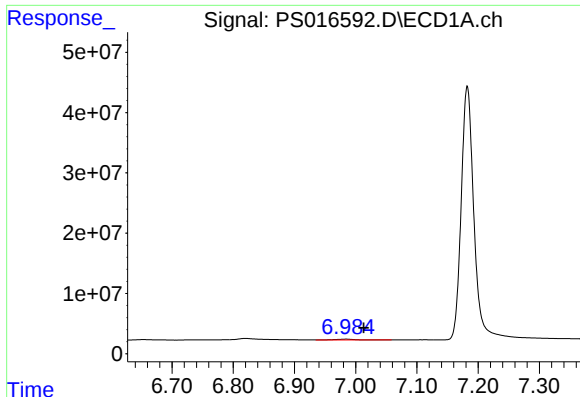

#3 4-Nitrophenol


R.T.: 6.984 min
Delta R.T.: -0.029 min
Response: 3101951
Conc: 3.88 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

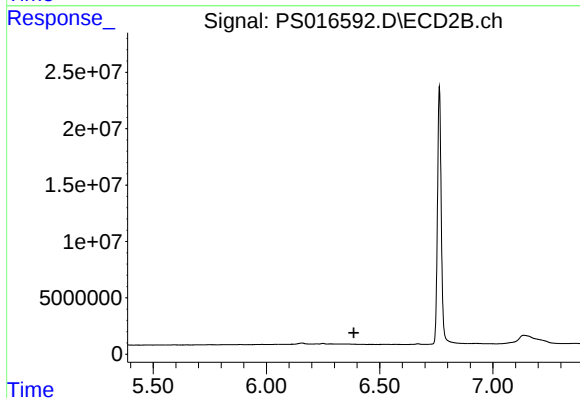


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.386 min
Response: 0
Conc: N.D.

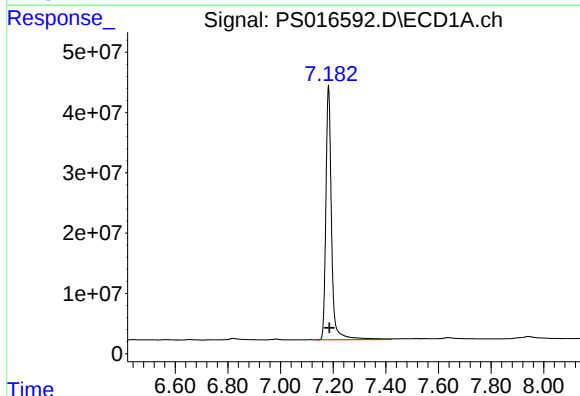


#4 2,4-DCAA

R.T.: 7.182 min
Delta R.T.: -0.003 min
Response: 628067750
Conc: 426.94 ng/ml

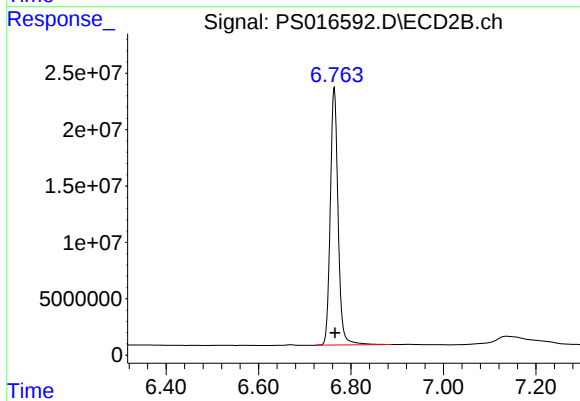

#4 2,4-DCAA


R.T.: 6.764 min
Delta R.T.: -0.002 min
Response: 267453793
Conc: 512.73 ng/ml

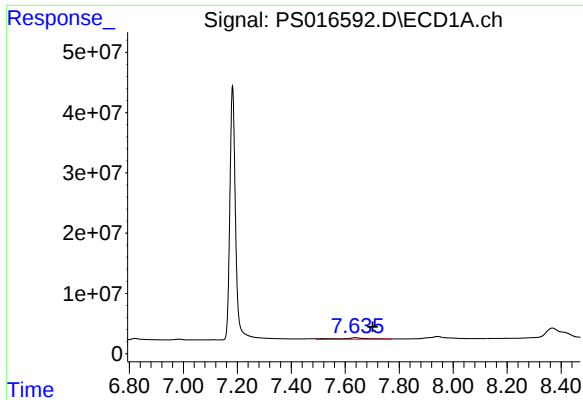

#7 MCPA


R.T.: 7.636 min
Delta R.T.: -0.067 min
Response: 18033602
Conc: 2.93 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

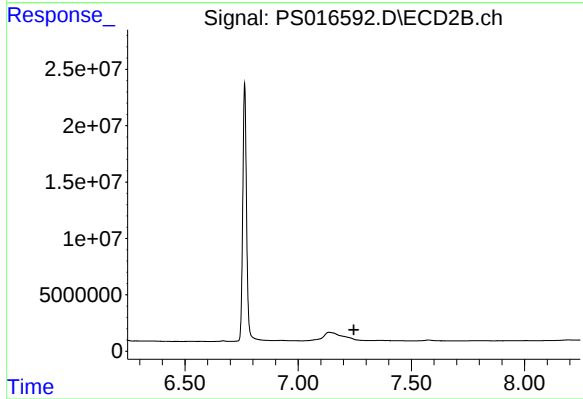


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 7.246 min
Response: 0
Conc: N.D.

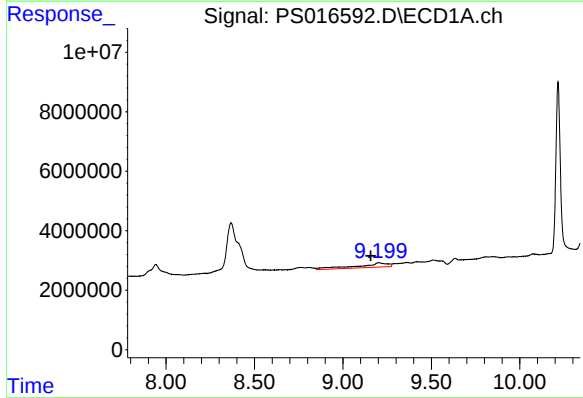


#11 2,4,5-TP (SILVEX)

R.T.: 9.201 min
Delta R.T.: 0.044 min
Response: 17835194
Conc: 2.47 ng/ml

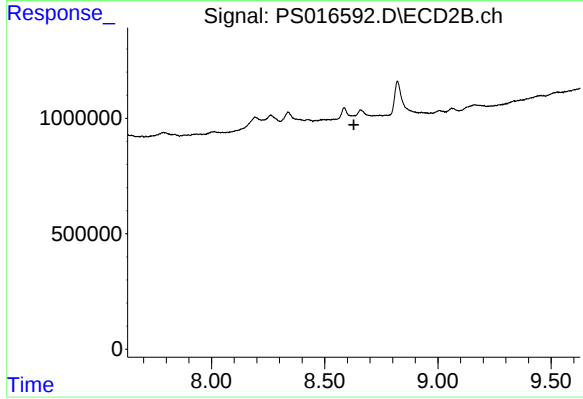

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 8.629 min
Response: 0
Conc: N.D.

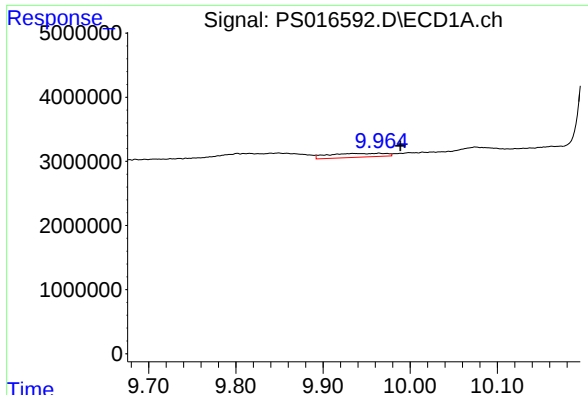

#13 2,4-DB


R.T.: 9.965 min
Delta R.T.: -0.024 min
Response: 2694502
Conc: 1.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

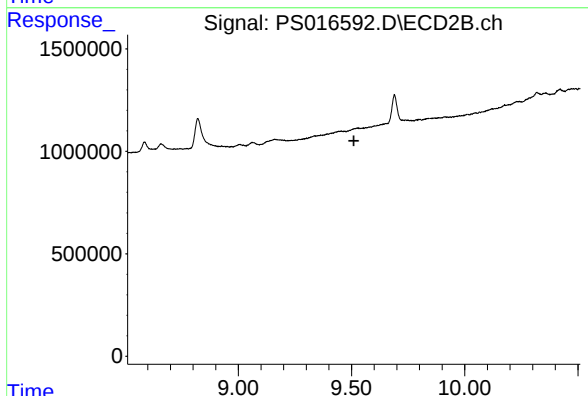


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.510 min
Response: 0
Conc: N.D.

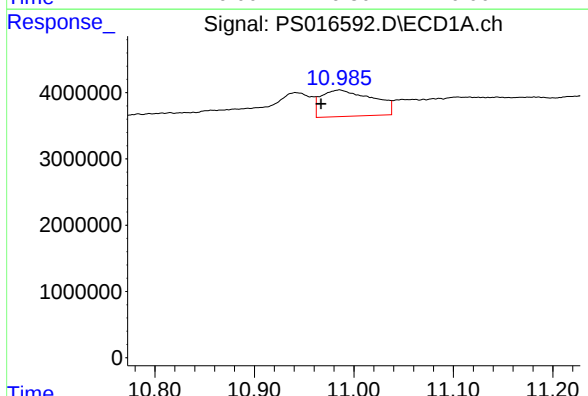


#15 Picloram

R.T.: 10.985 min
Delta R.T.: 0.018 min
Response: 14360933
Conc: 1.44 ng/ml

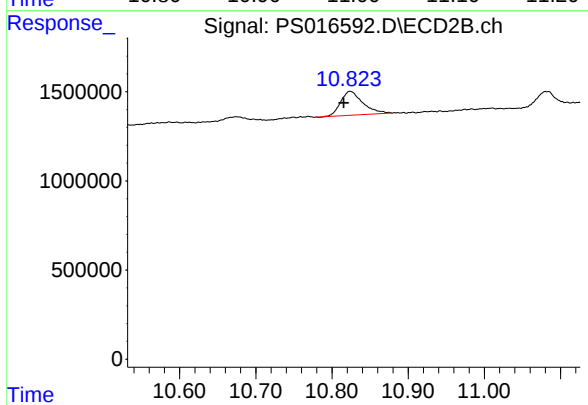

#15 Picloram


R.T.: 10.824 min
Delta R.T.: 0.008 min
Response: 2711016
Conc: N.D.

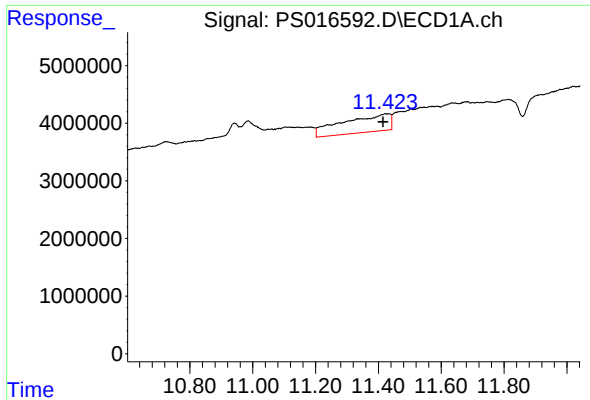

#16 DCPA

R.T.: 11.423 min
Delta R.T.: 0.008 min
Response: 32403798
Conc: 3.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

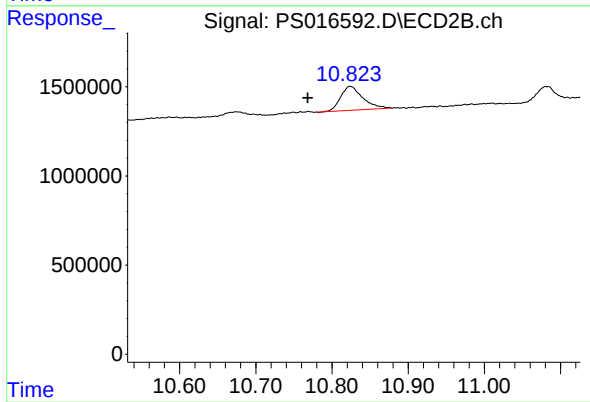

#16 DCPA

R.T.: 10.824 min
Delta R.T.: 0.055 min
Response: 2711016
Conc: N.D.