

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082322\
 Data File : PS020326.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2022 09:47
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 23:42:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.172	0.000	2592109	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	3.037	0.000	1387936	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.391	6.011f	1635863	607157	<MDL	<MDL #
3) T	4-Nitroph...	7.031	6.455f	518485	1030884	<MDL	2.099 #
5) T	DICAMBA	7.378	0.000	485335	0	<MDL	N.D. #
6) T	MCP	7.521	7.048	2119627	549354	<MDL	<MDL #
7) T	MCPA	7.679	0.000	1797104	0	<MDL	N.D. #
8) T	DICHLORPROP	8.078	0.000	2695129	0	<MDL	N.D. #
9) T	2,4-D	8.273	0.000	371133	0	<MDL	N.D. #
10) T	Pentachlo...	8.598	0.000	1199936	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.156	0.000	4081513	0	<MDL	N.D. #
12) T	2,4,5-T	9.408	0.000	12279406	0	<MDL	N.D. #
13) T	2,4-DB	10.011	0.000	195197	0	<MDL	N.D. #
14) T	DINOSEB	11.105	0.000	5042089	0	<MDL	N.D. #
15) T	Picloram	10.946	10.821	20177544	11689505	<MDL	1.549 #
16) T	DCPA	11.409	0.000	441951	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082322\
Data File : PS020326.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2022 09:47
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 23:42:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

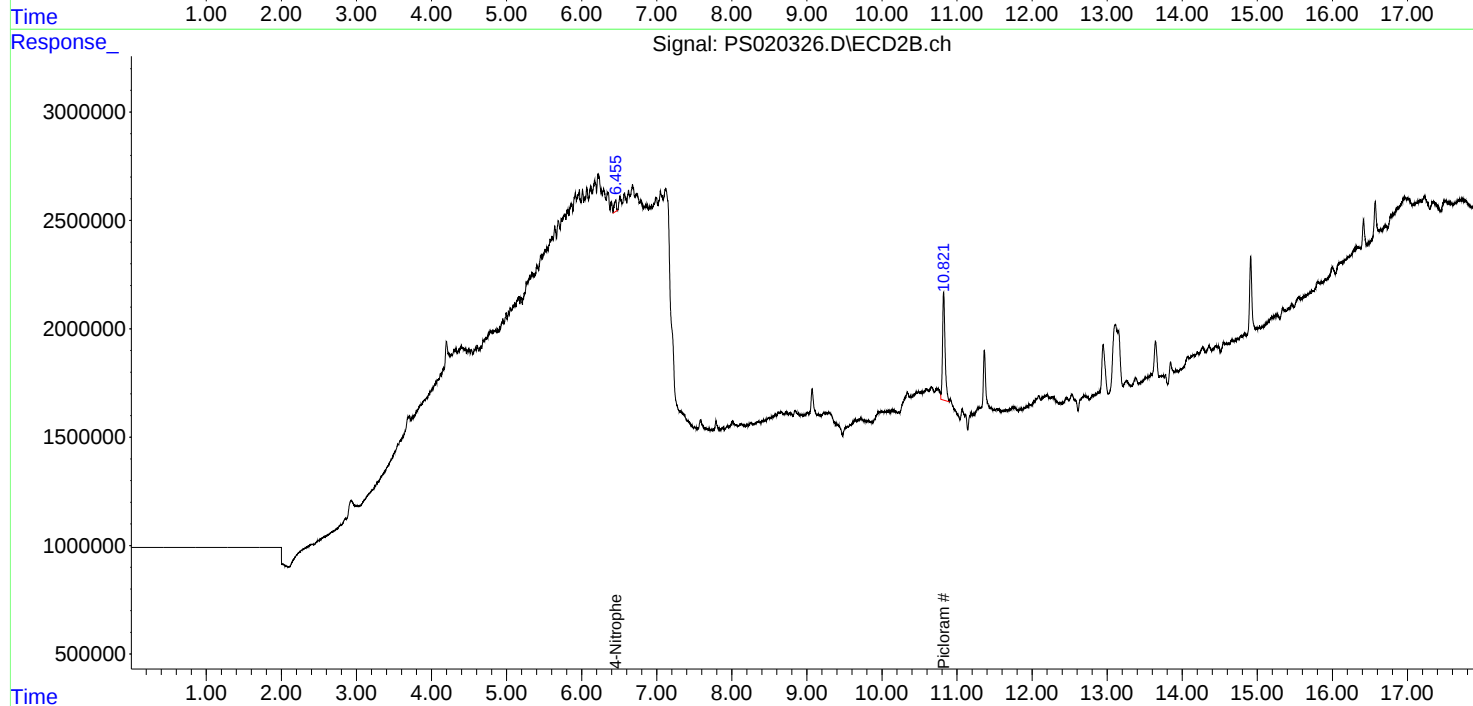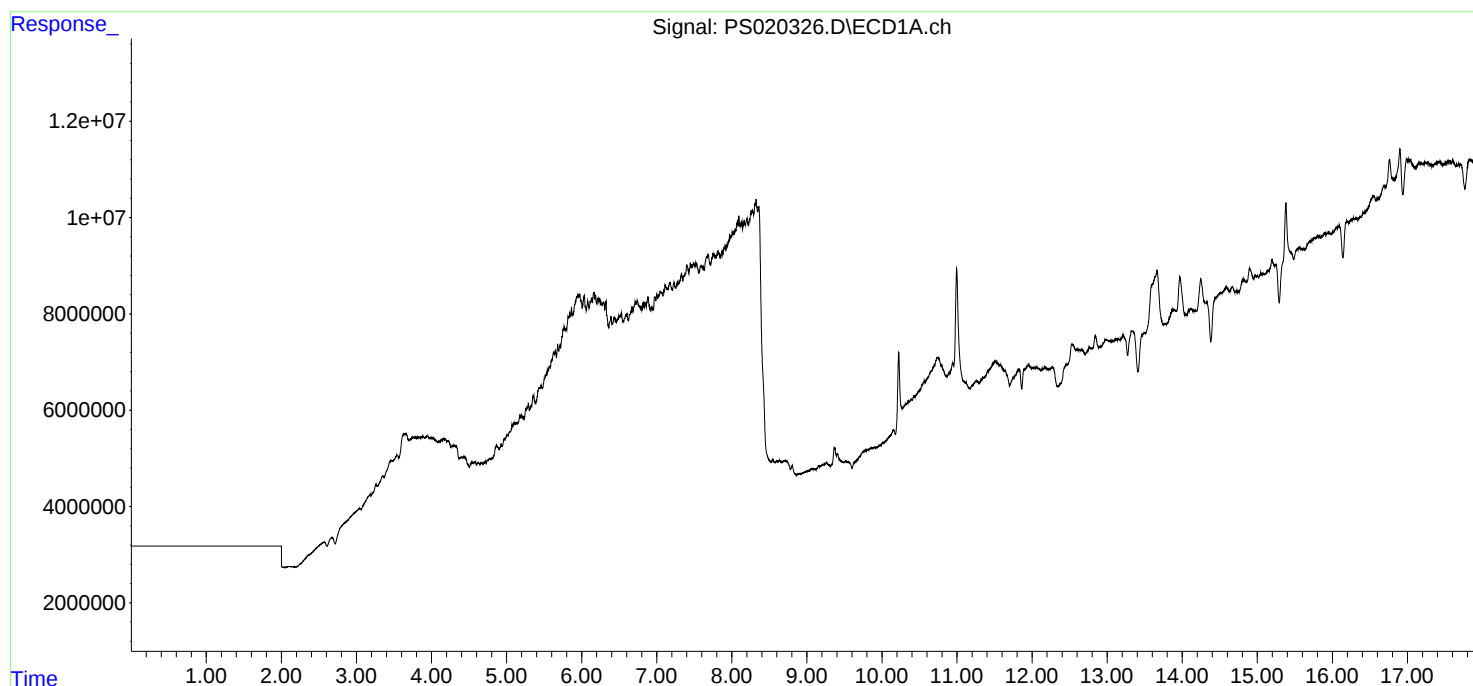


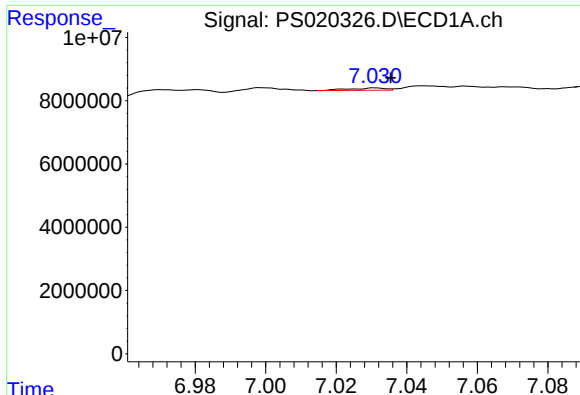

#3 4-Nitrophenol


R.T.: 7.031 min
Delta R.T.: -0.004 min
Response: 518485
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

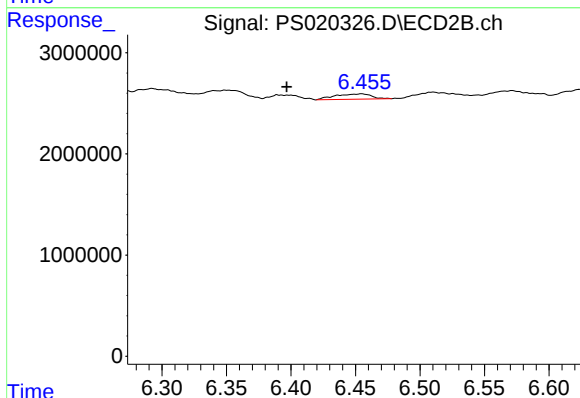


#3 4-Nitrophenol

R.T.: 6.455 min
Delta R.T.: 0.058 min
Response: 1030884
Conc: 2.10 ng/ml

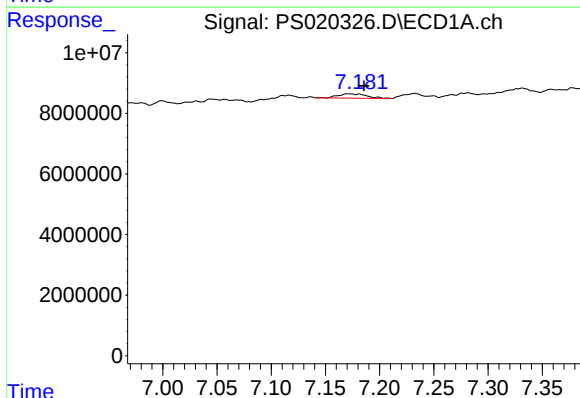


#4 2,4-DCAA

R.T.: 7.172 min
Delta R.T.: -0.014 min
Response: 2592109
Conc: N.D.

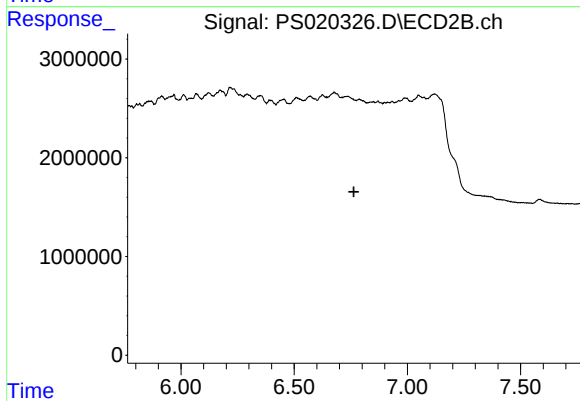

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.763 min
Response: 0
Conc: N.D.

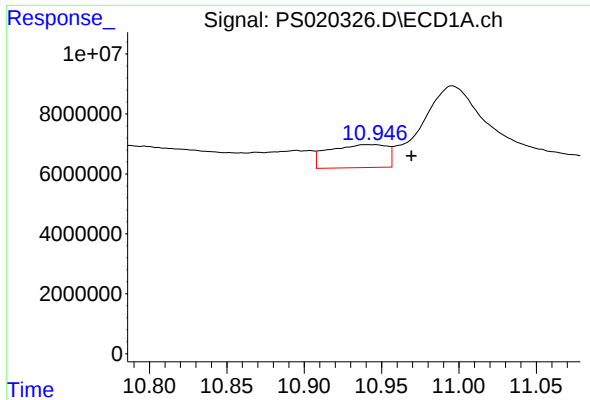

#15 Picloram

R.T.: 10.946 min
Delta R.T.: -0.024 min
Response: 20177544
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

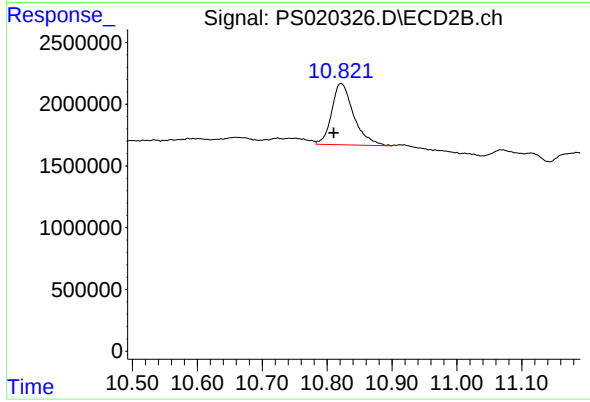

#15 Picloram

R.T.: 10.821 min
Delta R.T.: 0.011 min
Response: 11689505
Conc: 1.55 ng/ml