

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082322\
 Data File : PS020344.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2022 21:14
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 23:58:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.181	6.760	1442.5E6	441.0E6	489.201	541.181
Target Compounds							
2) T	3,5-DICHL...	6.418	5.968	153911	1200301	<MDL	<MDL #
3) T	4-Nitroph...	6.989f	0.000	609387	0	<MDL	N.D. #
7) T	MCPA	7.686	7.153f	4627529	47688007	<MDL	11.328 #
8) T	DICHLORPROP	0.000	7.610f	0	1529312	N.D.	1.635
11) T	2,4,5-TP ...	9.109	8.680f	6165145	1454758	<MDL	<MDL #
12) T	2,4,5-T	9.414	0.000	19844658	0	1.093	N.D. #
13) T	2,4-DB	10.024	9.437f	5455761	2524020	1.495	3.711 #
14) T	DINOSEB	11.090f	0.000	13117641	0	<MDL	N.D. #
15) T	Picloram	10.961	10.856f	7528823	7535358	<MDL	<MDL #
16) T	DCPA	11.415	0.000	5750013	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082322\
Data File : PS020344.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2022 21:14
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 23:58:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

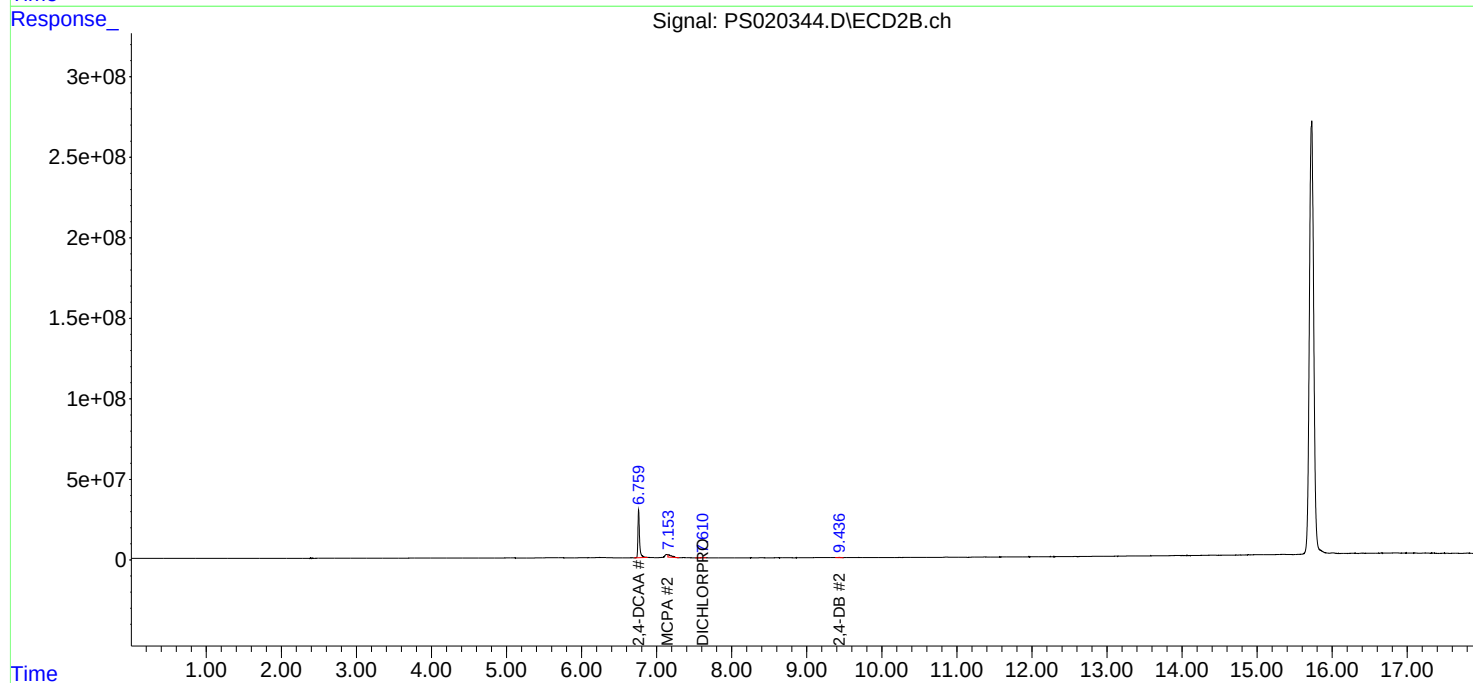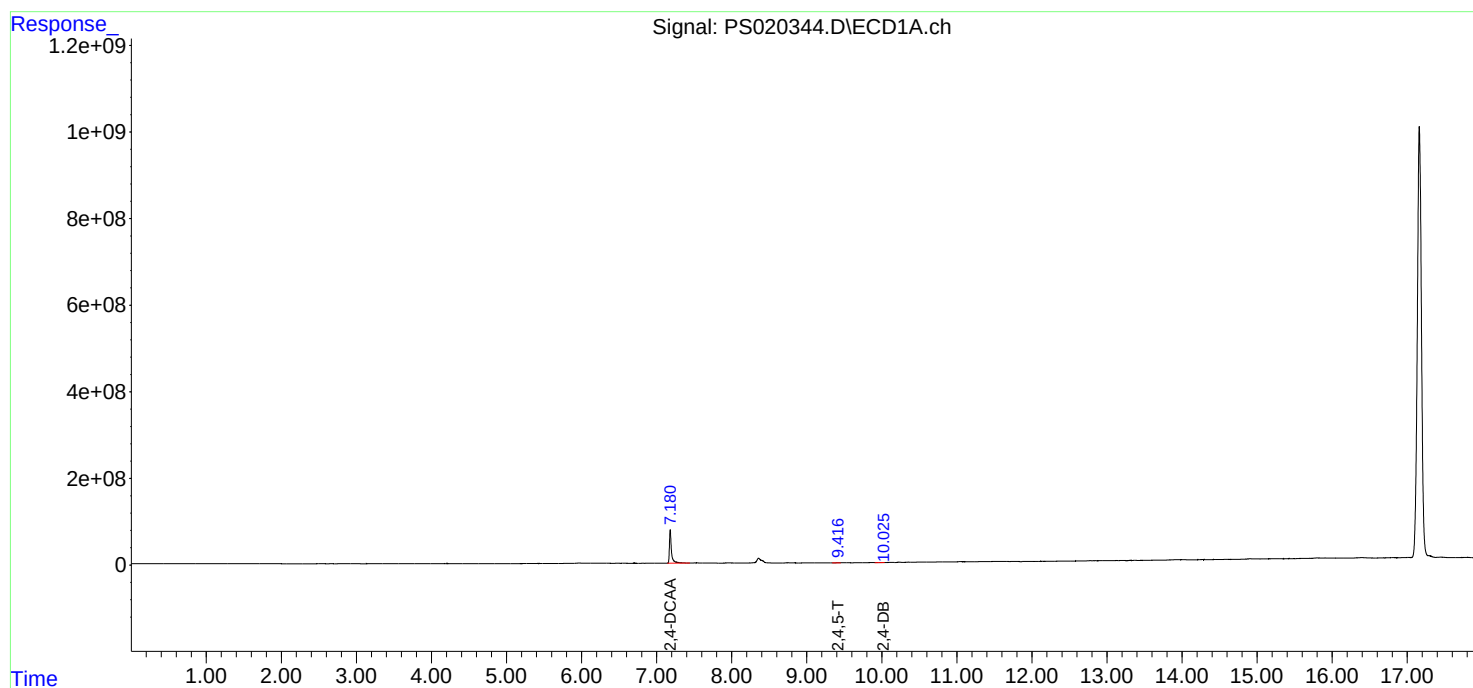


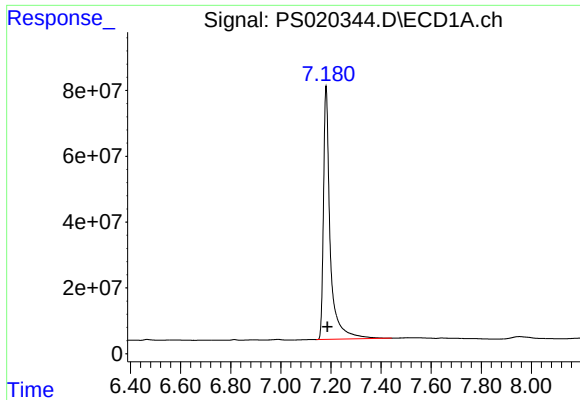

#4 2,4-DCAA


R.T.: 7.181 min
Delta R.T.: -0.005 min
Response: 1442518538
Conc: 489.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

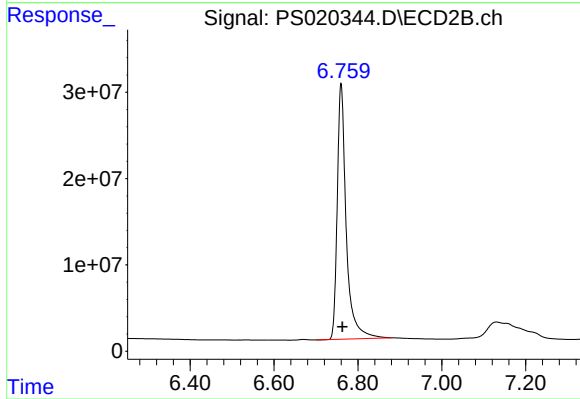


#4 2,4-DCAA

R.T.: 6.760 min
Delta R.T.: -0.004 min
Response: 441038929
Conc: 541.18 ng/ml

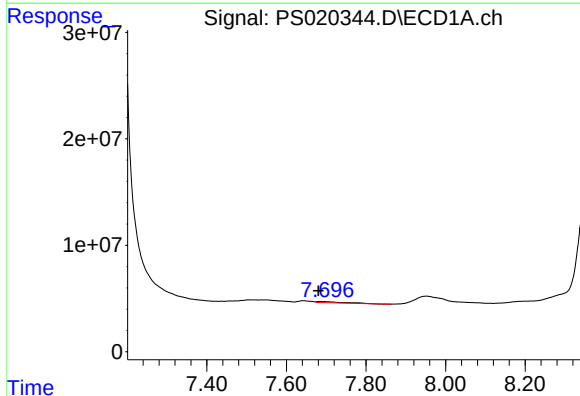


#7 MCPA

R.T.: 7.686 min
Delta R.T.: 0.005 min
Response: 4627529
Conc: N.D.

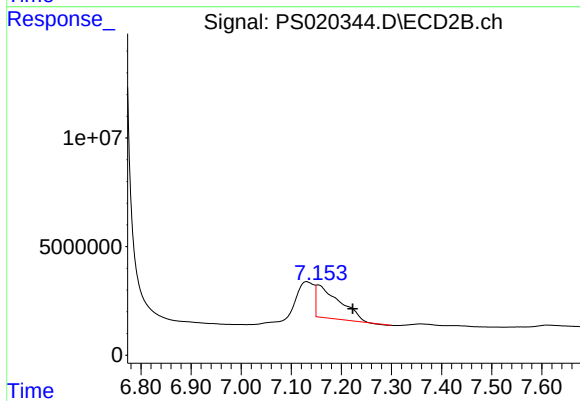

#7 MCPA


R.T.: 7.153 min
Delta R.T.: -0.069 min
Response: 47688007
Conc: 11.33 ug/ml

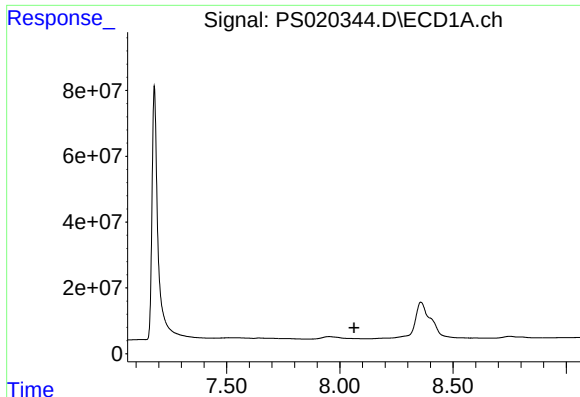

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

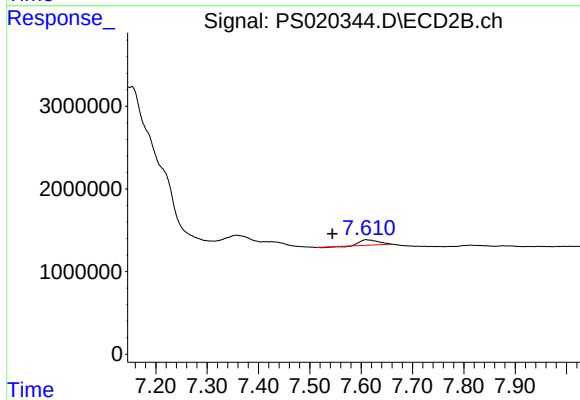


#8 DICHLORPROP

R.T.: 7.610 min
Delta R.T.: 0.066 min
Response: 1529312
Conc: 1.64 ng/ml

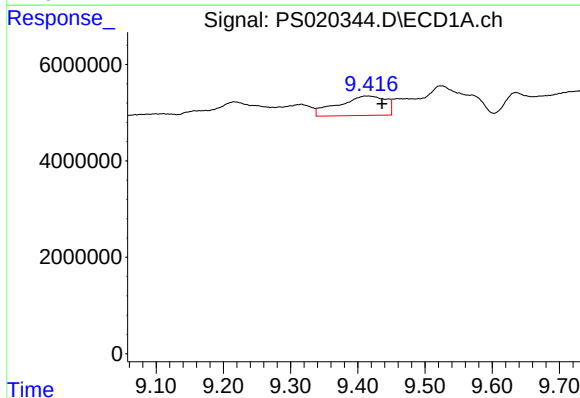


#12 2,4,5-T

R.T.: 9.414 min
Delta R.T.: -0.022 min
Response: 19844658
Conc: 1.09 ng/ml

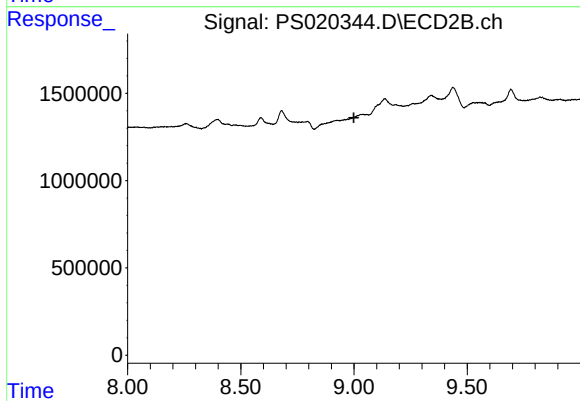

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 8.999 min
Response: 0
Conc: N.D.

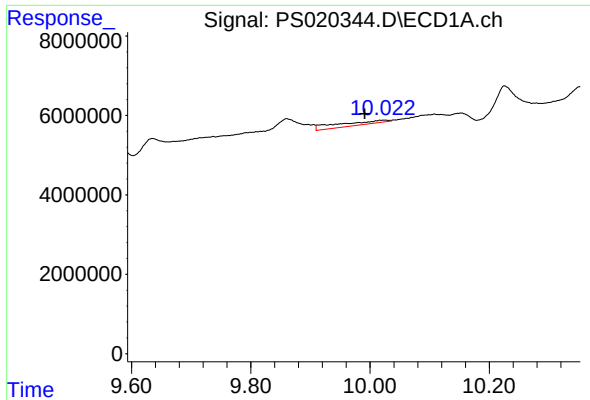

#13 2,4-DB

R.T.: 10.024 min
Delta R.T.: 0.033 min
Response: 5455761
Conc: 1.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

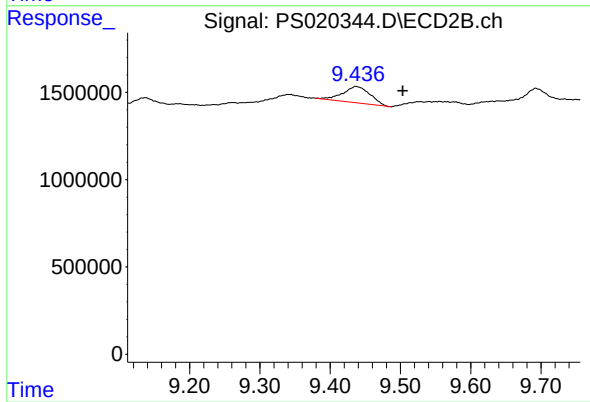

#13 2,4-DB

R.T.: 9.437 min
Delta R.T.: -0.067 min
Response: 2524020
Conc: 3.71 ng/ml