

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082323\
 Data File : PS024115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2023 08:40
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 13:08:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080823.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 08 13:26:17 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.335	6.786	8185417	420301	4.133	<MDL #
Target Compounds							
1) T	Dalapon	2.518	2.572	5708140	3805025	2.601	3.480 #
3) T	4-Nitroph...	6.203	0.000	18541308	0	16.752	N.D. #
5) T	DICAMBA	6.497	7.001	1332338	13678688	<MDL	4.664 #
6) T	MCP	6.686	7.078	6827991	-338760	1.095	N.D. #
7) T	MCPA	6.825	7.204f	1039836	5907320	<MDL	2.019 #
8) T	DICHLORPROP	7.084	7.583	2000069	3723284	<MDL	5.093 #
9) T	2,4-D	7.260	7.800f	130.4E6	917590	52.611	1.077 #
10) T	Pentachlo...	7.523	0.000	1255236	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.059	8.637	197590	944339	<MDL	<MDL #
12) T	2,4,5-T	8.314	9.055	1088127	1423759	<MDL	<MDL #
14) T	DINOSEB	9.872	0.000	486329	0	<MDL	N.D. #
15) T	Picloram	9.691	10.801	29899476	23830826	2.313	4.783 #
16) T	DCPA	0.000	10.801	0	23830826	N.D.	4.635



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082323\
Data File : PS024115.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2023 08:40
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 13:08:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080823.M
Quant Title : 8080.M
QLast Update : Tue Aug 08 13:26:17 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

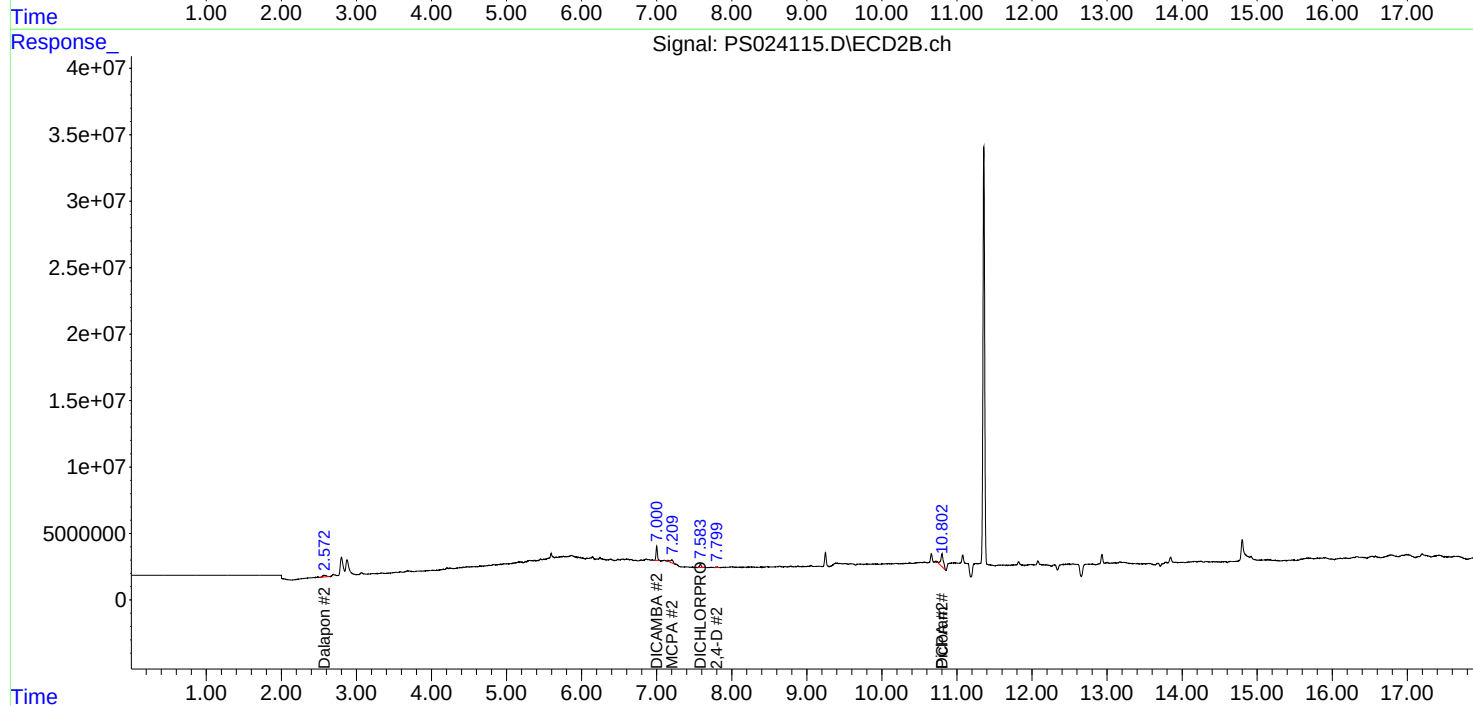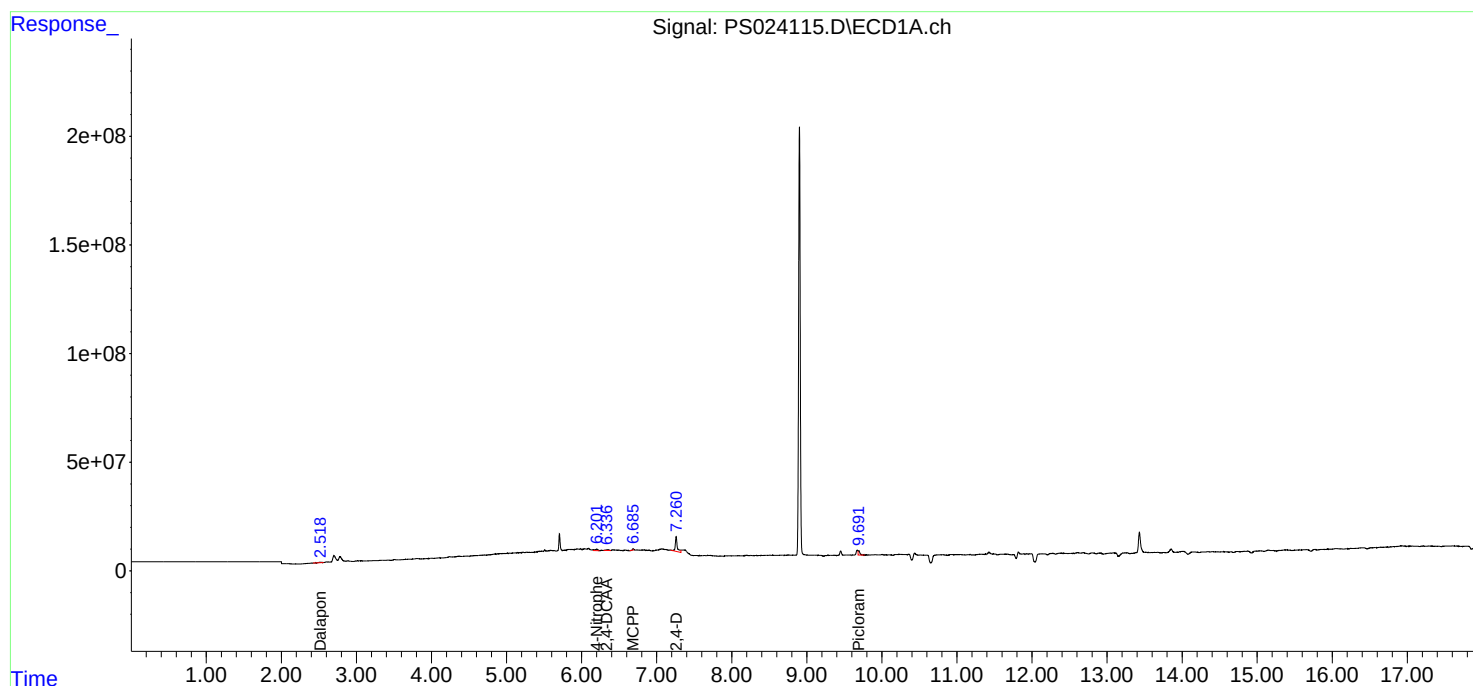


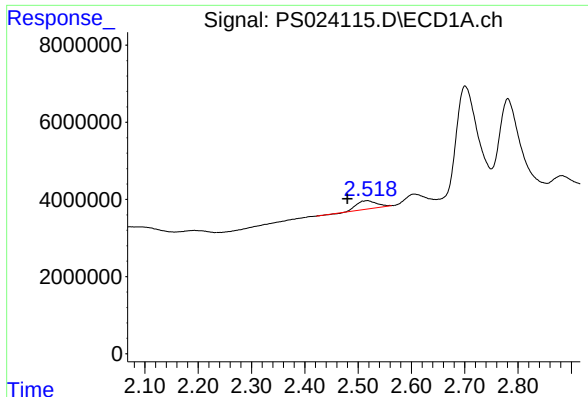

#1 Dalapon


R.T.: 2.518 min
Delta R.T.: 0.038 min
Response: 5708140
Conc: 2.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

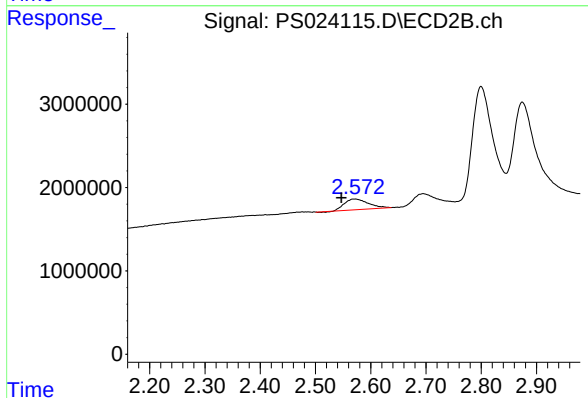


#1 Dalapon

R.T.: 2.572 min
Delta R.T.: 0.025 min
Response: 3805025
Conc: 3.48 ng/ml

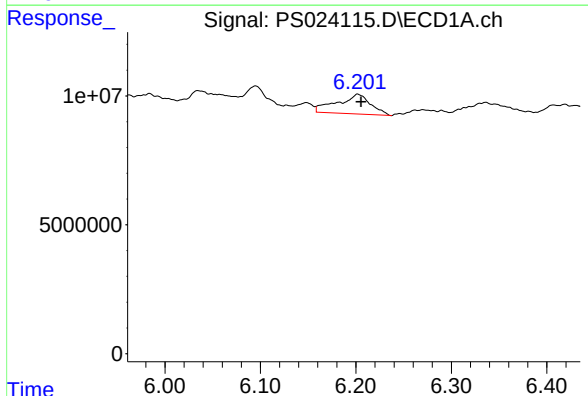


#3 4-Nitrophenol

R.T.: 6.203 min
Delta R.T.: -0.003 min
Response: 18541308
Conc: 16.75 ng/ml

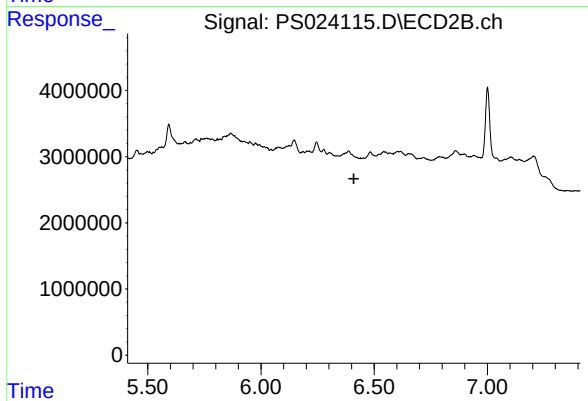

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.410 min
Response: 0
Conc: N.D.

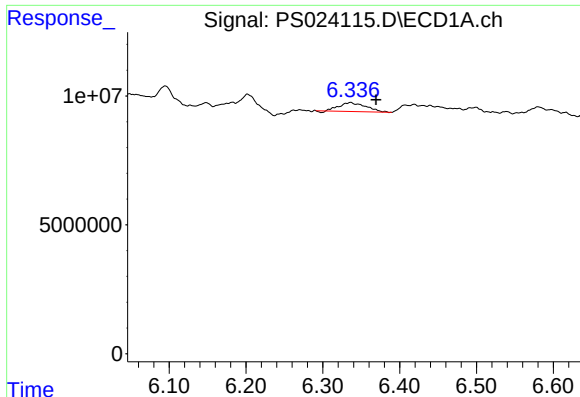

#4 2,4-DCAA


R.T.: 6.335 min
Delta R.T.: -0.034 min
Response: 8185417
Conc: 4.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

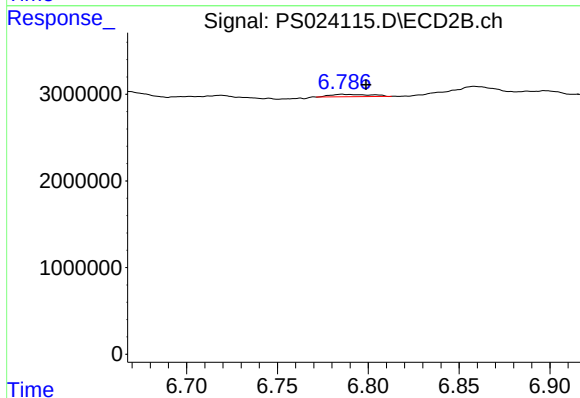


#4 2,4-DCAA

R.T.: 6.786 min
Delta R.T.: -0.013 min
Response: 420301
Conc: N.D.

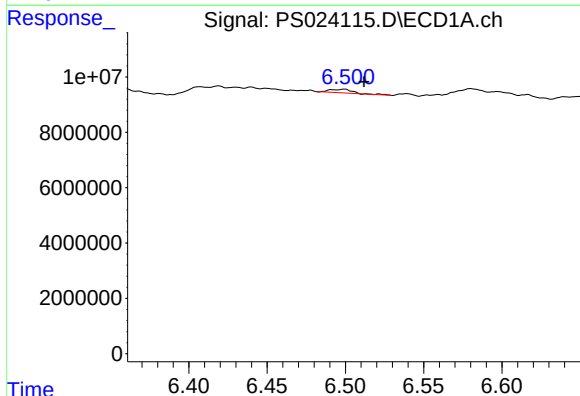


#5 DICAMBA

R.T.: 6.497 min
Delta R.T.: -0.015 min
Response: 1332338
Conc: N.D.

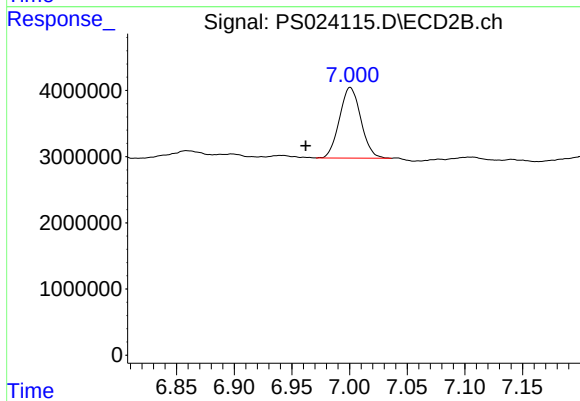

#5 DICAMBA


R.T.: 7.001 min
Delta R.T.: 0.039 min
Response: 13678688
Conc: 4.66 ng/ml

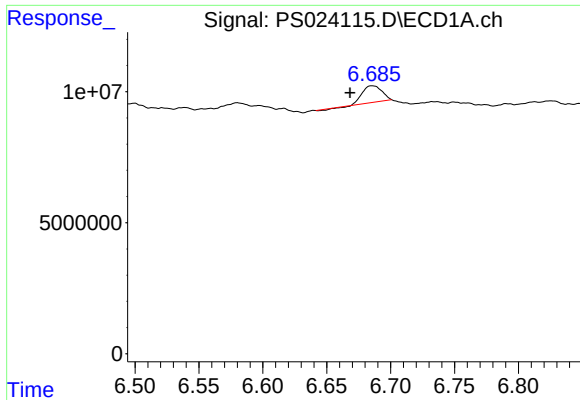

#6 MCPP


R.T.: 6.686 min
Delta R.T.: 0.018 min
Response: 6827991
Conc: 1.09 ug/ml

Instrument :
ECD_S
ClientSampleId :

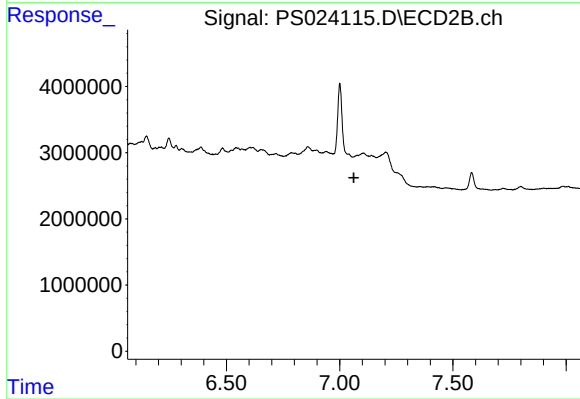


#6 MCPP

R.T.: 7.078 min
Delta R.T.: 0.015 min
Response: -338760
Conc: N.D.

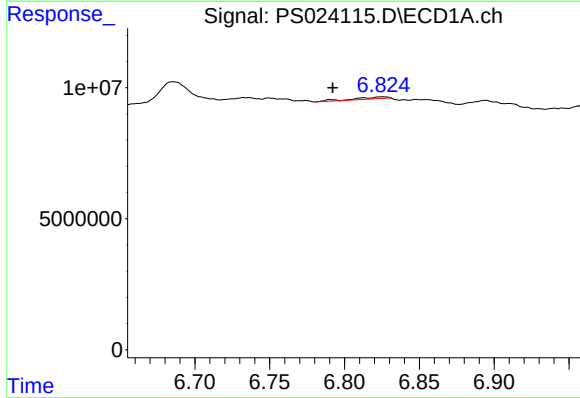


#7 MCPA

R.T.: 6.825 min
Delta R.T.: 0.033 min
Response: 1039836
Conc: N.D.

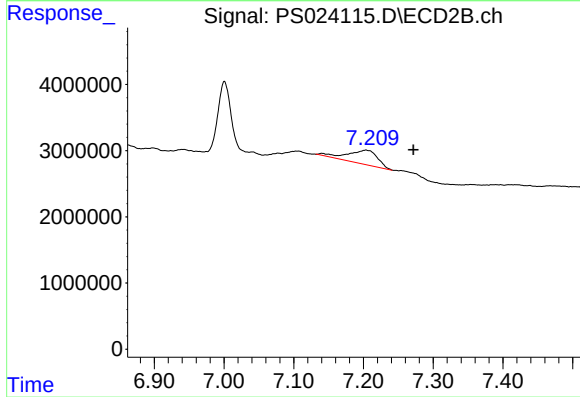

#7 MCPA


R.T.: 7.204 min
Delta R.T.: -0.068 min
Response: 5907320
Conc: 2.02 ug/ml

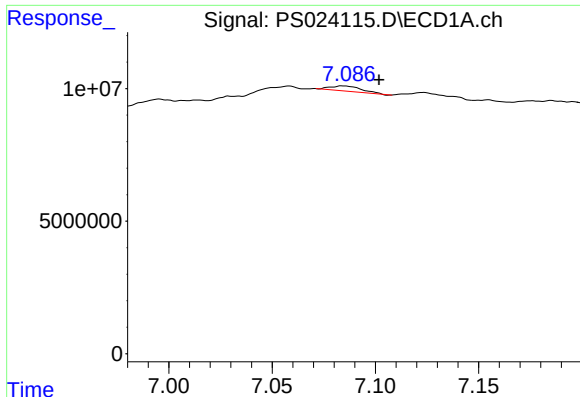

#8 DICHLORPROP


R.T.: 7.084 min
Delta R.T.: -0.017 min
Response: 2000069
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

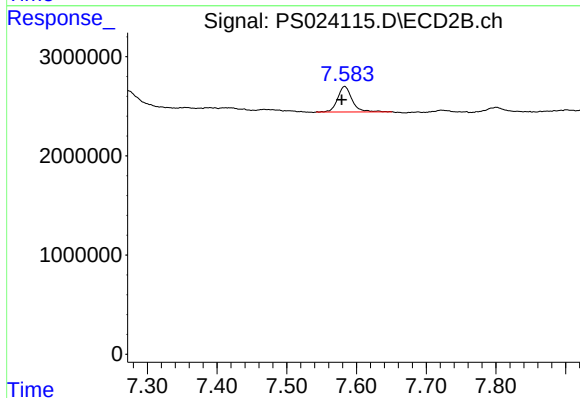


#8 DICHLORPROP

R.T.: 7.583 min
Delta R.T.: 0.004 min
Response: 3723284
Conc: 5.09 ng/ml

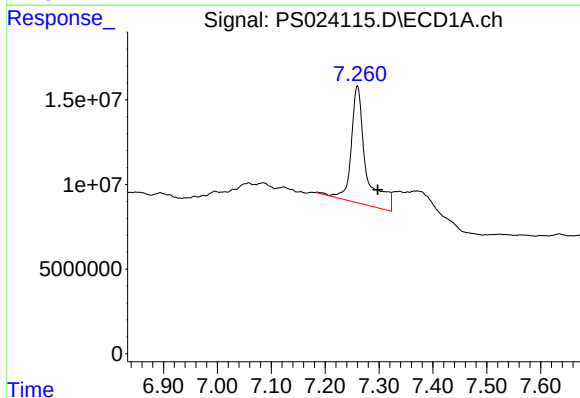


#9 2,4-D

R.T.: 7.260 min
Delta R.T.: -0.038 min
Response: 130372051
Conc: 52.61 ng/ml

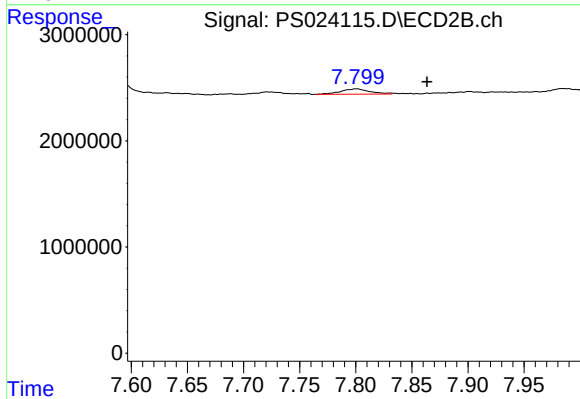

#9 2,4-D


R.T.: 7.800 min
Delta R.T.: -0.063 min
Response: 917590
Conc: 1.08 ng/ml

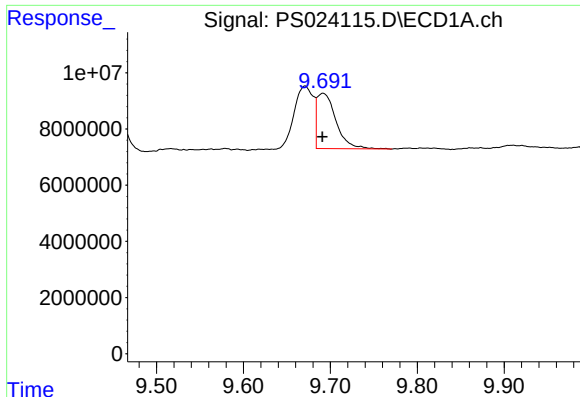

#15 Picloram


R.T.: 9.691 min
Delta R.T.: 0.000 min
Response: 29899476
Conc: 2.31 ng/ml

Instrument :
ECD_S
ClientSampleId :

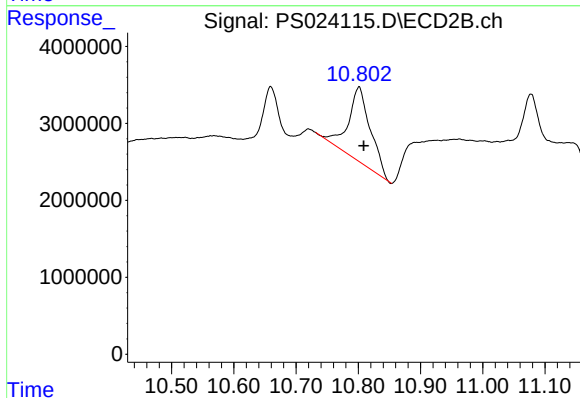


#15 Picloram

R.T.: 10.801 min
Delta R.T.: -0.008 min
Response: 23830826
Conc: 4.78 ng/ml

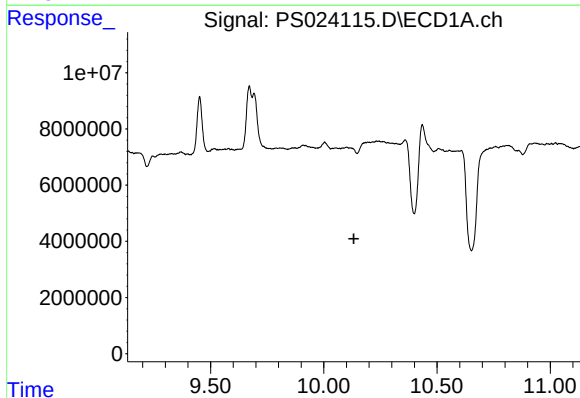

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.133 min
Response: 0
Conc: N.D.

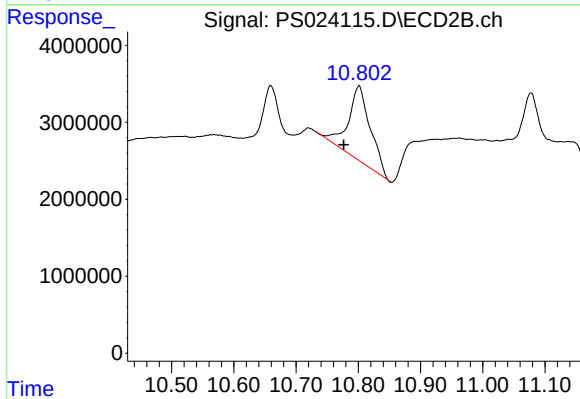

#16 DCPA

R.T.: 10.801 min
Delta R.T.: 0.024 min
Response: 23830826
Conc: 4.64 ng/ml