

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082323\
 Data File : PS024132.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2023 17:38
 Operator : AR\AJ
 Sample : PB154957BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 04:27:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080823.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 08 13:26:17 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.367	6.796	154.4E6	48986363	77.972	72.828
Target Compounds							
1) T	Dalapon	2.468	0.000	2819913	0	1.285	N.D. #
3) T	4-Nitroph...	6.202	6.397	19031171	604662	17.194	1.528 #
5) T	DICAMBA	6.460f	6.948	8003787	709166	<MDL	<MDL #
6) T	MCP	6.686	7.003f	15528675	10060766	2.490	5.200 #
7) T	MCPA	6.774	7.267	-1878786	6150043	N.D.	2.102
8) T	DICHLORPROP	7.045f	7.587	9174657	13605470	4.077	18.610 #
9) T	2,4-D	7.258	7.802f	29249534	871162	11.803	1.023 #
10) T	Pentachlo...	7.519	8.272	25395423	969358	<MDL	<MDL #
11) T	2,4,5-TP ...	8.048	8.595f	1068947	462798	<MDL	<MDL #
12) T	2,4,5-T	8.286	9.057	9543764	2727926	<MDL	<MDL #
13) T	2,4-DB	8.822	0.000	1666452	0	<MDL	N.D. #
14) T	DINOSEB	9.899	9.857	955412	1458769	<MDL	<MDL #
15) T	Picloram	9.663	10.802	99916335	22378022	7.728	4.491 #
16) T	DCPA	10.120	10.802	3865059	22378022	<MDL	4.353 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082323\
Data File : PS024132.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2023 17:38
Operator : AR\AJ
Sample : PB154957BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 04:27:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080823.M
Quant Title : 8080.M
QLast Update : Tue Aug 08 13:26:17 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

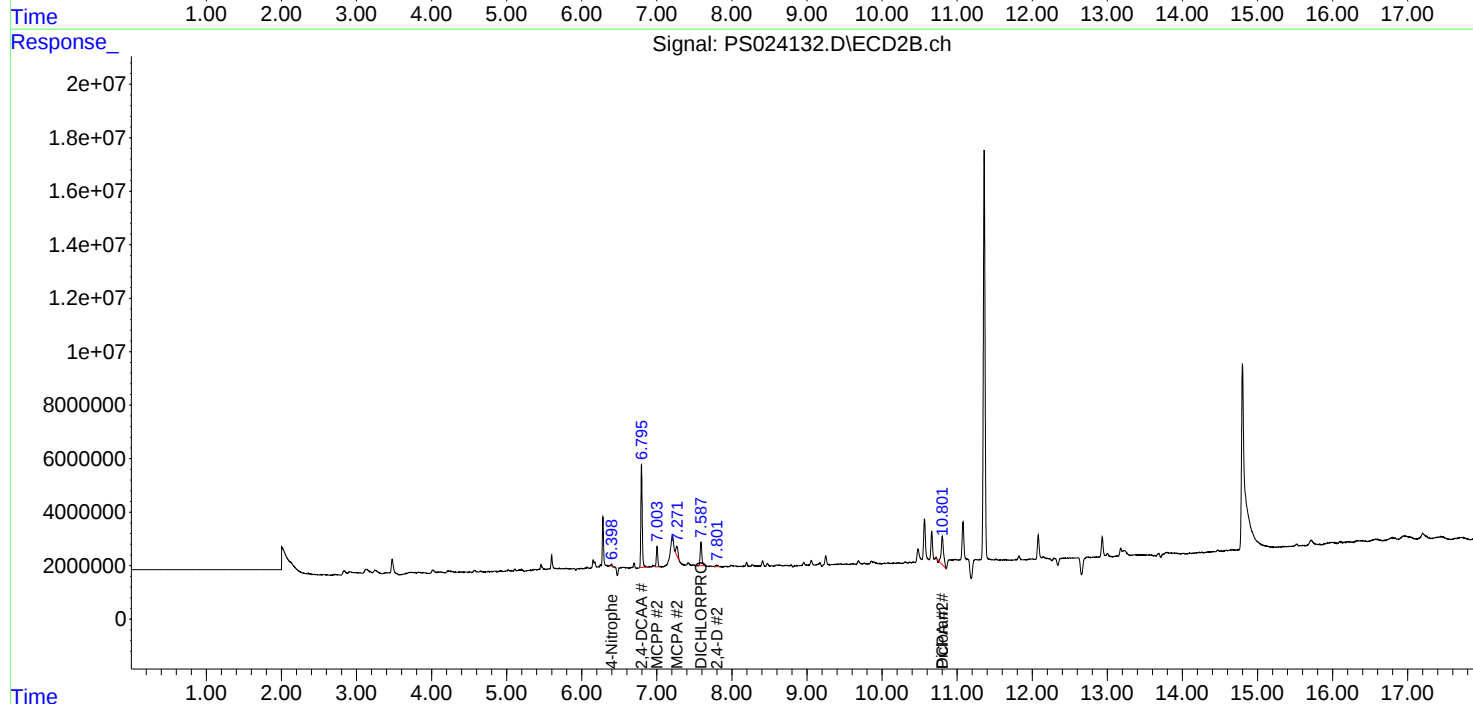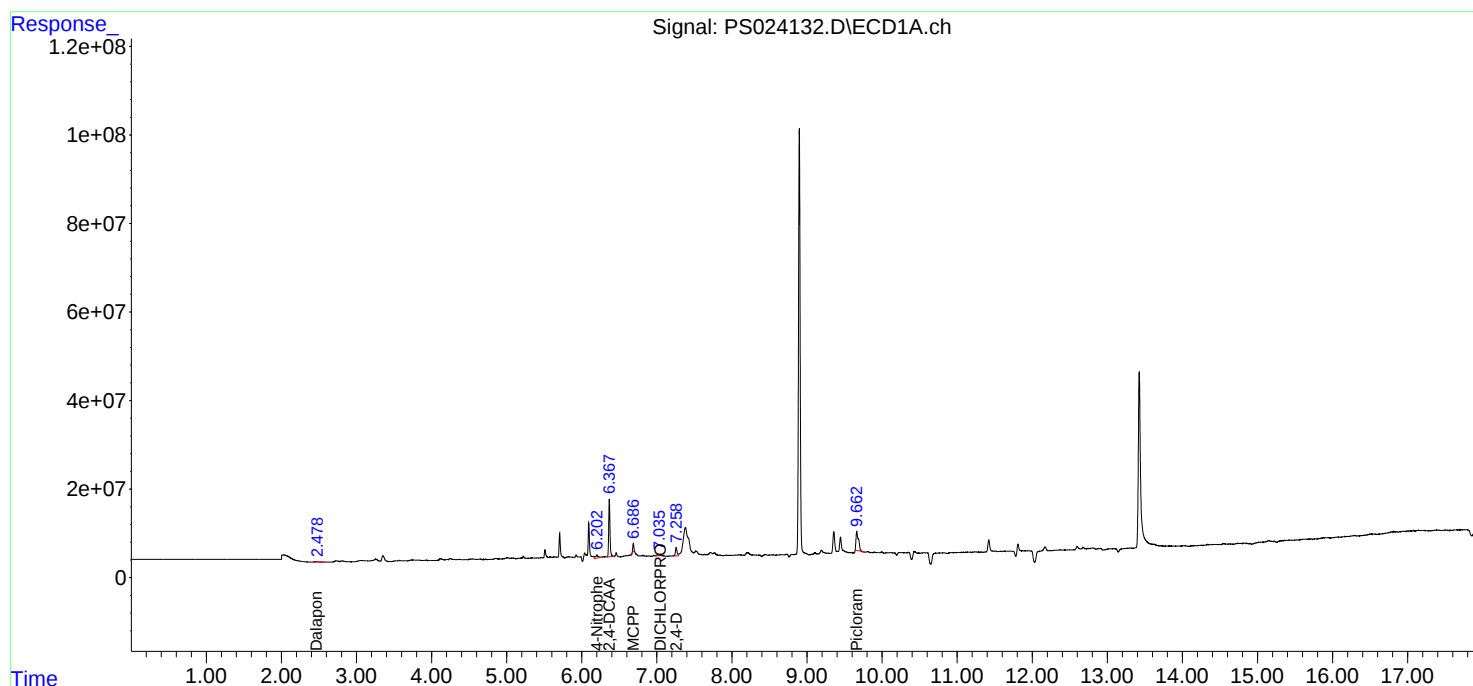


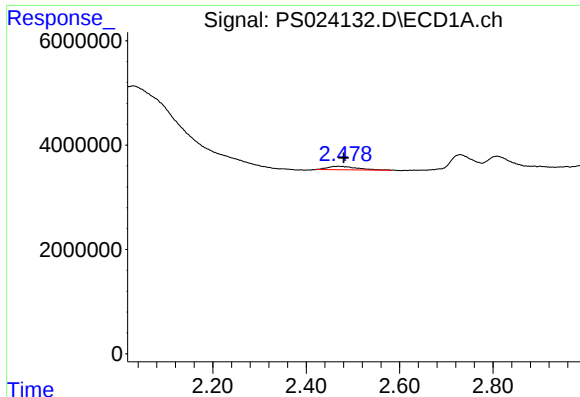

#1 Dalapon


R.T.: 2.468 min
Delta R.T.: -0.012 min
Response: 2819913
Conc: 1.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

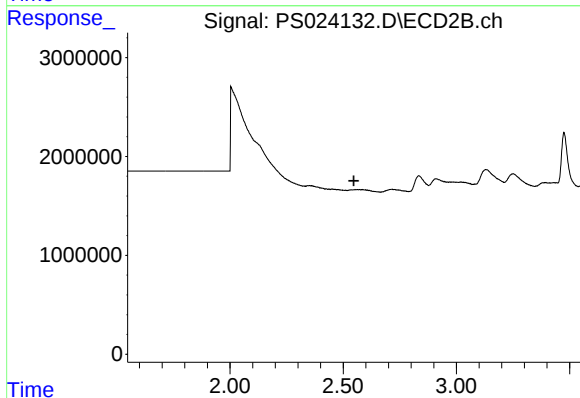


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.547 min
Response: 0
Conc: N.D.

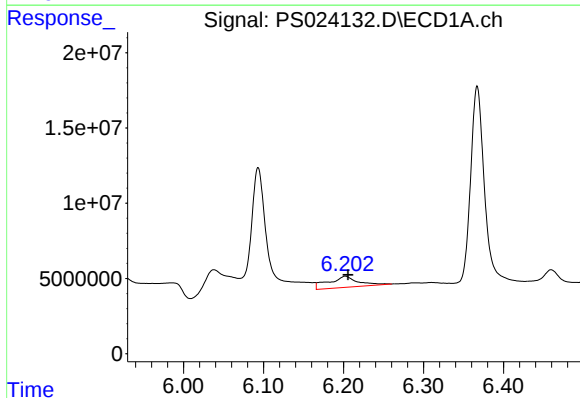


#3 4-Nitrophenol

R.T.: 6.202 min
Delta R.T.: -0.003 min
Response: 19031171
Conc: 17.19 ng/ml

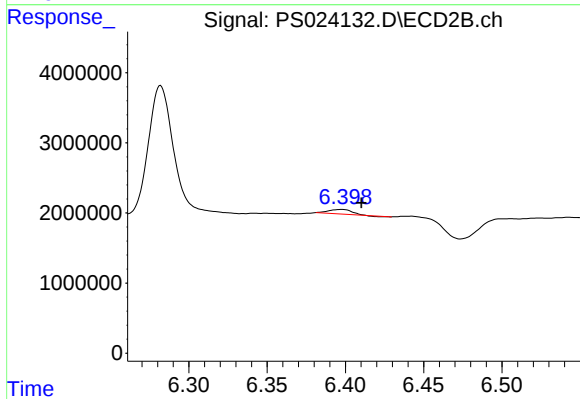

#3 4-Nitrophenol


R.T.: 6.397 min
Delta R.T.: -0.013 min
Response: 604662
Conc: 1.53 ng/ml

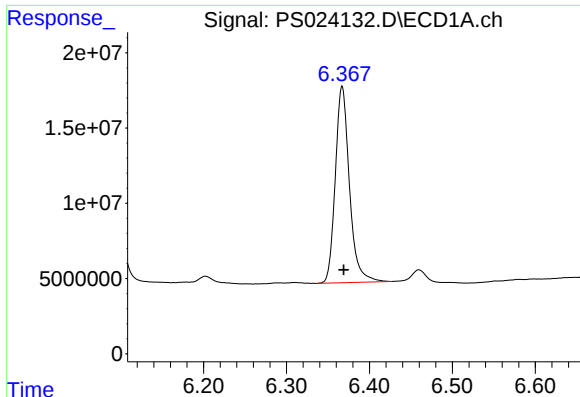

#4 2,4-DCAA


R.T.: 6.367 min
Delta R.T.: -0.002 min
Response: 154428423
Conc: 77.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

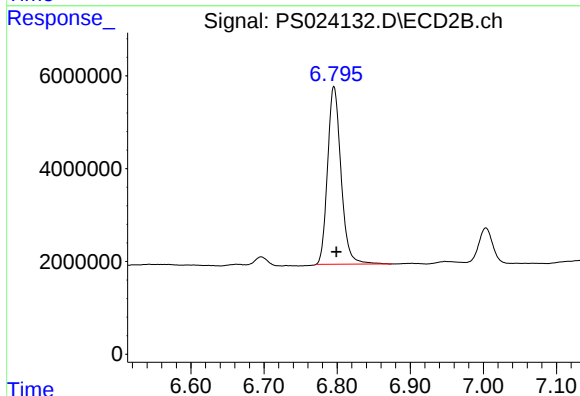


#4 2,4-DCAA

R.T.: 6.796 min
Delta R.T.: -0.003 min
Response: 48986363
Conc: 72.83 ng/ml

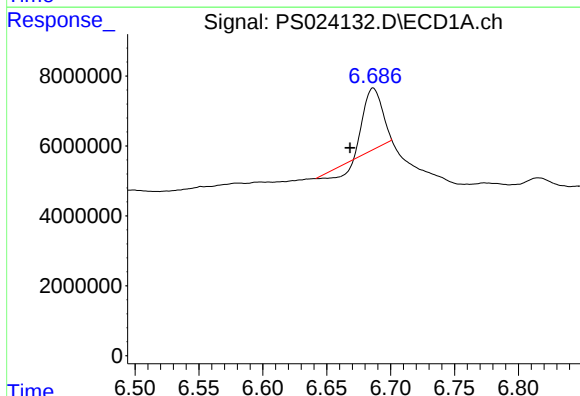


#6 MCP

R.T.: 6.686 min
Delta R.T.: 0.018 min
Response: 15528675
Conc: 2.49 ug/ml

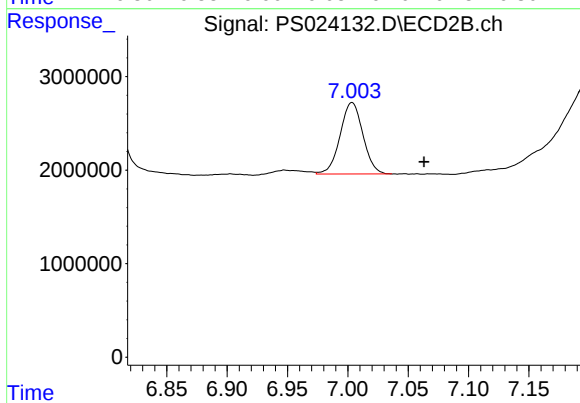

#6 MCP


R.T.: 7.003 min
Delta R.T.: -0.060 min
Response: 10060766
Conc: 5.20 ug/ml

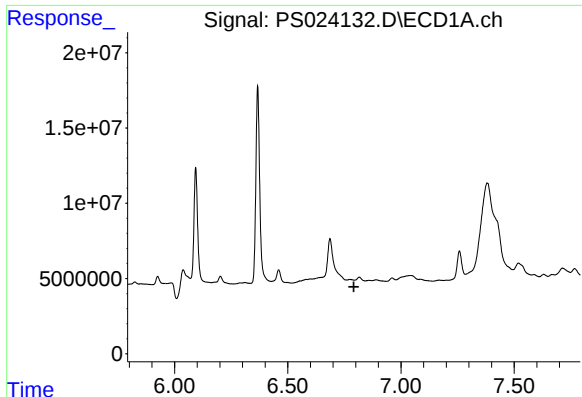

#7 MCPA


R.T.: 6.774 min
Delta R.T.: -0.018 min
Response: -1878786
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

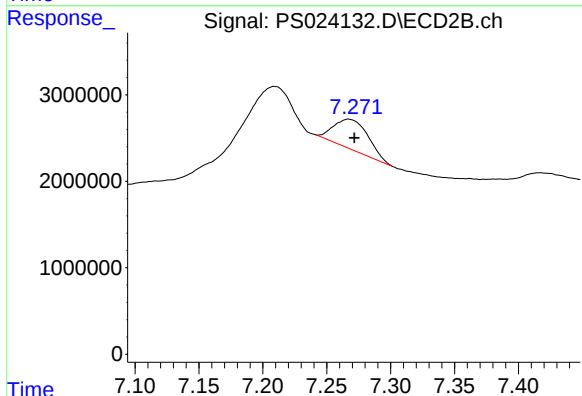


#7 MCPA

R.T.: 7.267 min
Delta R.T.: -0.005 min
Response: 6150043
Conc: 2.10 ug/ml

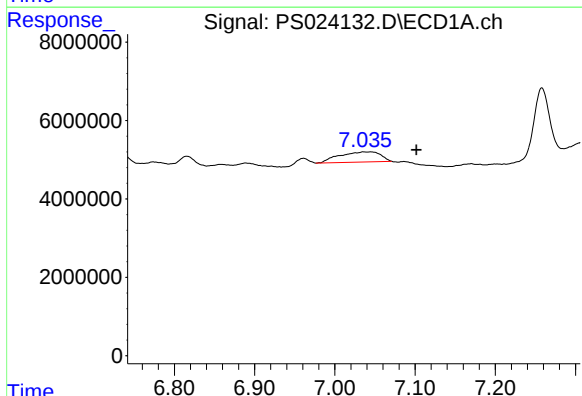


#8 DICHLORPROP

R.T.: 7.045 min
Delta R.T.: -0.057 min
Response: 9174657
Conc: 4.08 ng/ml

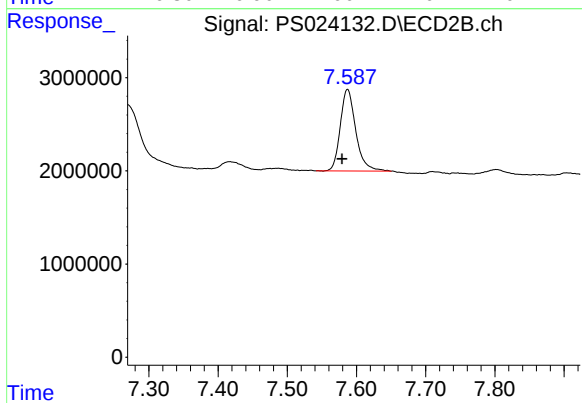

#8 DICHLORPROP


R.T.: 7.587 min
Delta R.T.: 0.008 min
Response: 13605470
Conc: 18.61 ng/ml

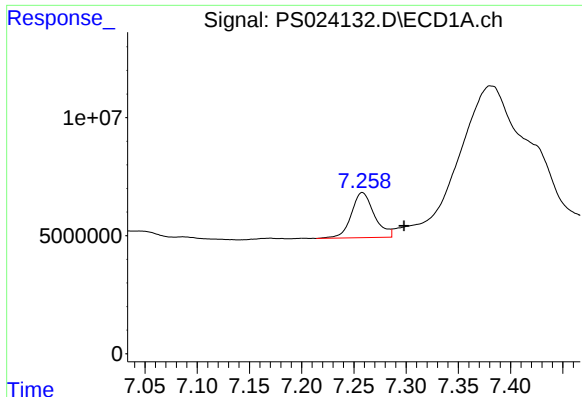

#9 2,4-D


R.T.: 7.258 min
Delta R.T.: -0.040 min
Response: 29249534
Conc: 11.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

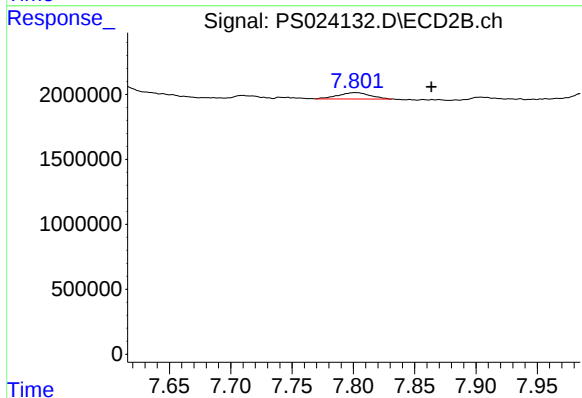


#9 2,4-D

R.T.: 7.802 min
Delta R.T.: -0.062 min
Response: 871162
Conc: 1.02 ng/ml

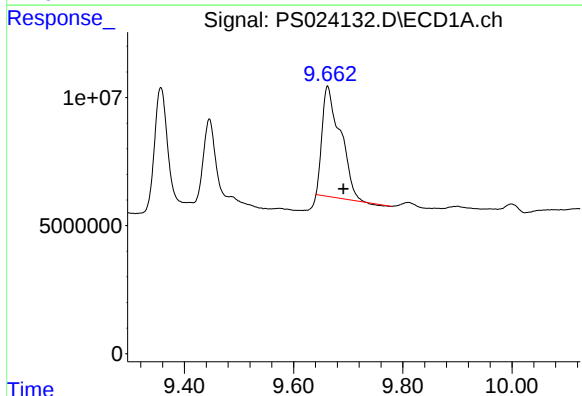


#15 Picloram

R.T.: 9.663 min
Delta R.T.: -0.029 min
Response: 99916335
Conc: 7.73 ng/ml

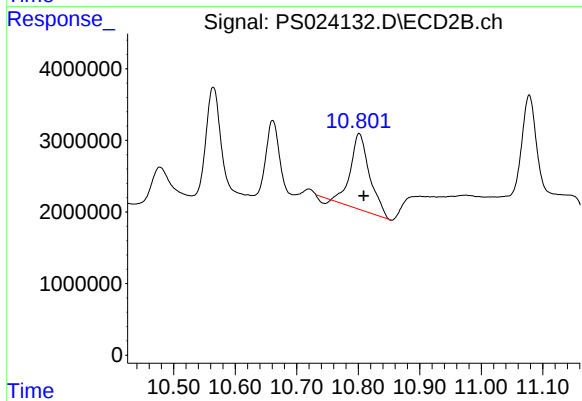

#15 Picloram


R.T.: 10.802 min
Delta R.T.: -0.007 min
Response: 22378022
Conc: 4.49 ng/ml

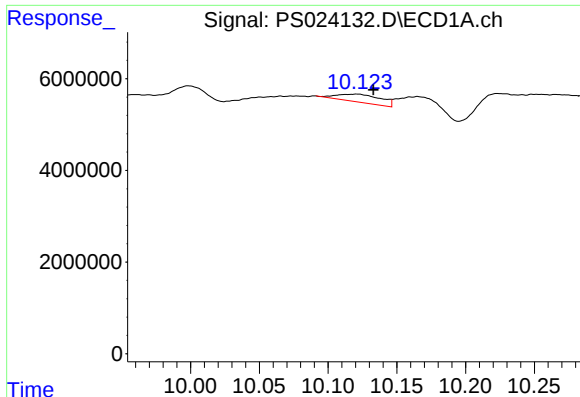

#16 DCPA

R.T.: 10.120 min
Delta R.T.: -0.013 min
Response: 3865059
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

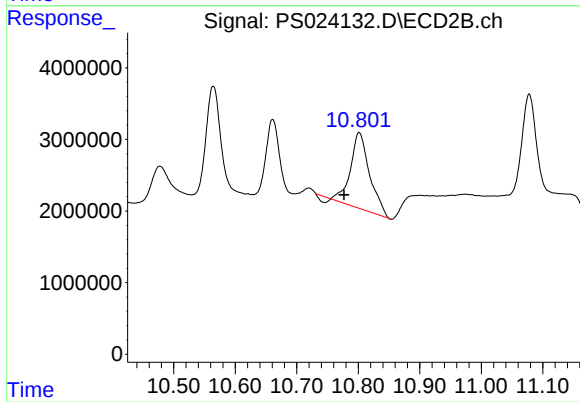

#16 DCPA

R.T.: 10.802 min
Delta R.T.: 0.025 min
Response: 22378022
Conc: 4.35 ng/ml