

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082323\
 Data File : PS024134.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2023 18:27
 Operator : AR\AJ
 Sample : 04042-01MS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 04:28:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080823.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 08 13:26:17 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.366	0.000	434249	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.413f	0.000	466805	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.747	0.000	422068	0	<MDL	N.D. #
3) T	4-Nitroph...	6.205	0.000	4607003	0	4.162	N.D. #
5) T	DICAMBA	6.511	6.959	749796	1746870	<MDL	<MDL #
6) T	MCPD	6.692	0.000	473986	0	<MDL	N.D. #
7) T	MCPA	0.000	7.252	0	4044479	N.D.	1.383
8) T	DICHLORPROP	0.000	7.589	0	1314979	N.D.	1.799
9) T	2,4-D	7.366f	7.804f	447.2E6	468064	180.449	<MDL #
11) T	2,4,5-TP ...	8.045	0.000	480295	0	<MDL	N.D. #
12) T	2,4,5-T	8.301	0.000	670537	0	<MDL	N.D. #
14) T	DINOSEB	9.849	0.000	462496	0	<MDL	N.D. #
15) T	Picloram	9.673	10.774	643618	2538993	<MDL	<MDL #
16) T	DCPA	10.124	10.774	2525243	2538993	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082323\
Data File : PS024134.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2023 18:27
Operator : AR\AJ
Sample : 04042-01MS
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 04:28:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080823.M
Quant Title : 8080.M
QLast Update : Tue Aug 08 13:26:17 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

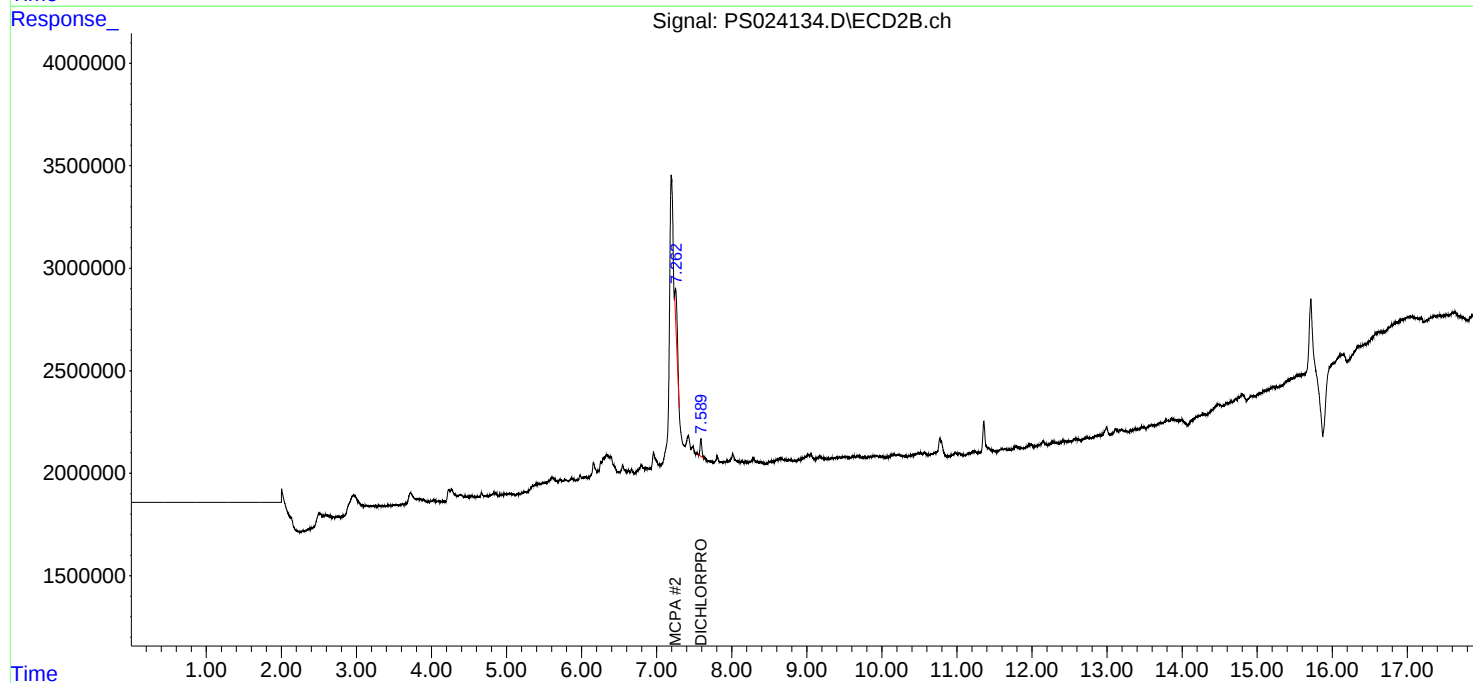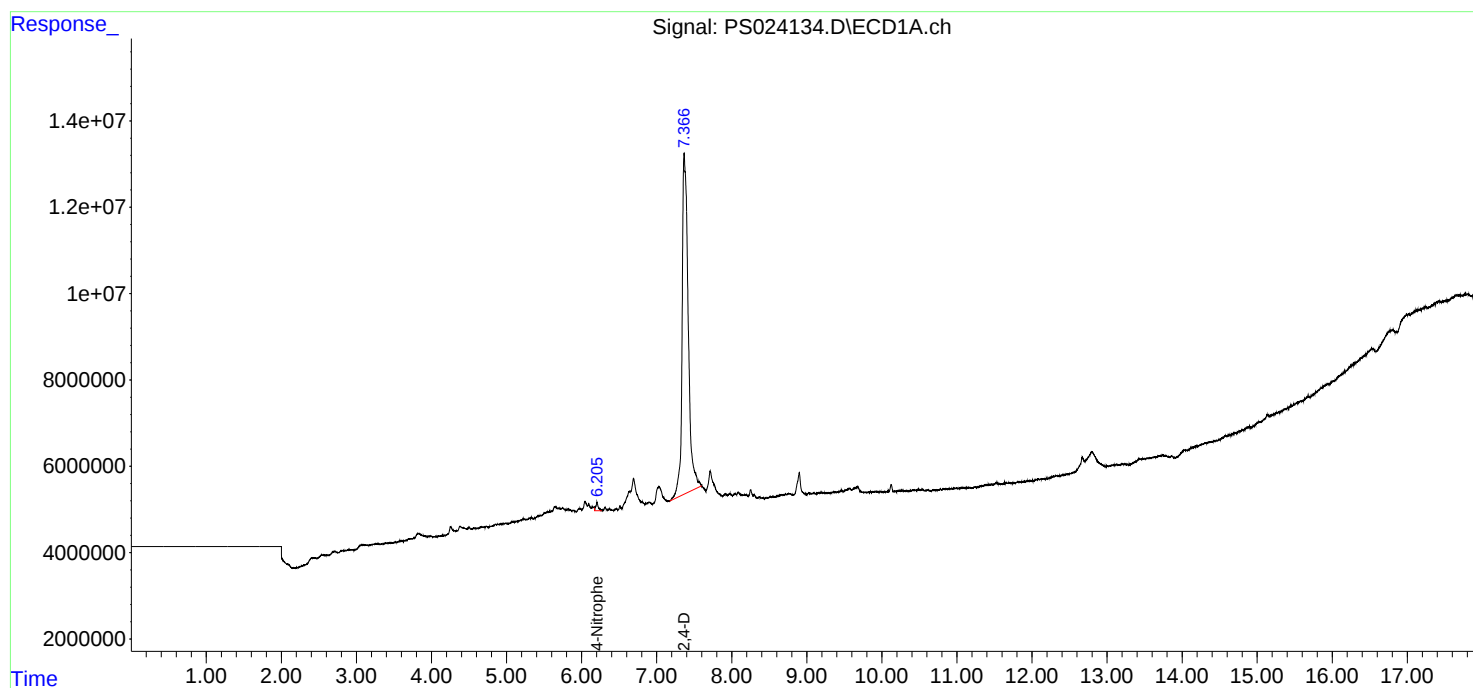


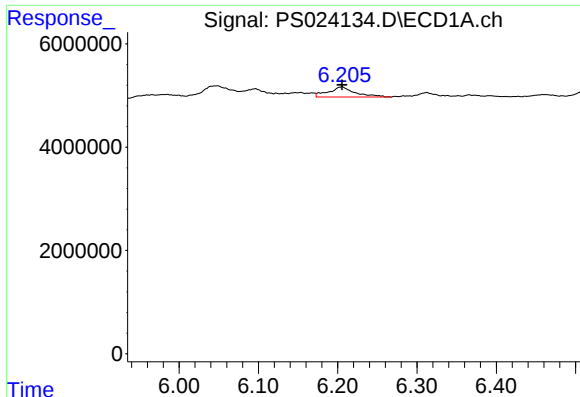

#3 4-Nitrophenol


R.T.: 6.205 min
Delta R.T.: 0.000 min
Response: 4607003
Conc: 4.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

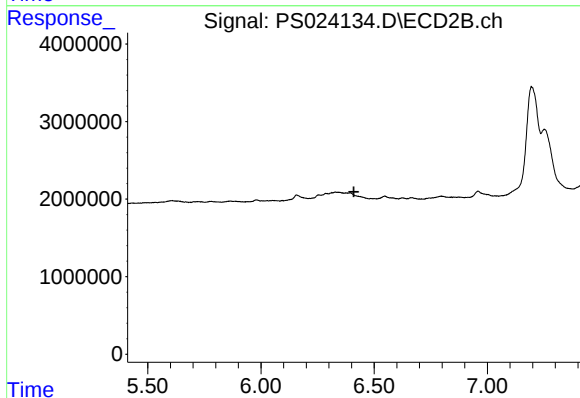


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.410 min
Response: 0
Conc: N.D.

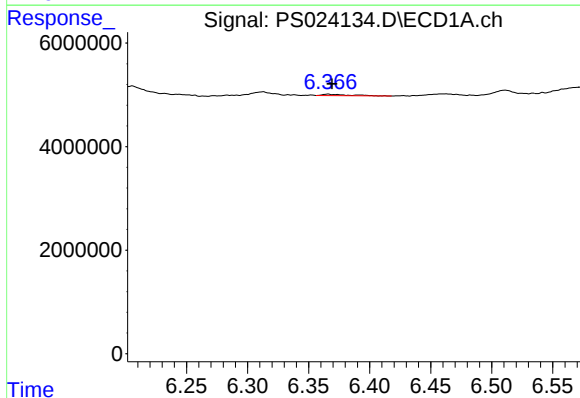


#4 2,4-DCAA

R.T.: 6.366 min
Delta R.T.: -0.003 min
Response: 434249
Conc: N.D.

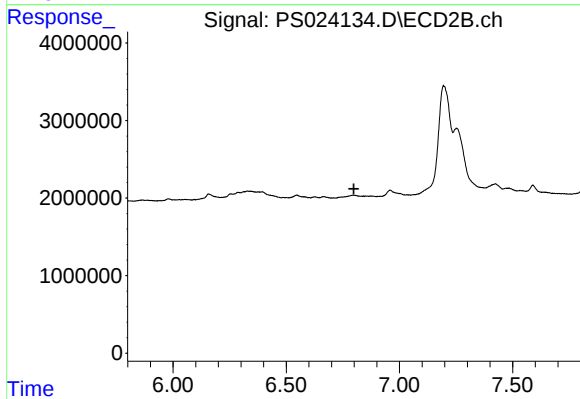

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.799 min
Response: 0
Conc: N.D.

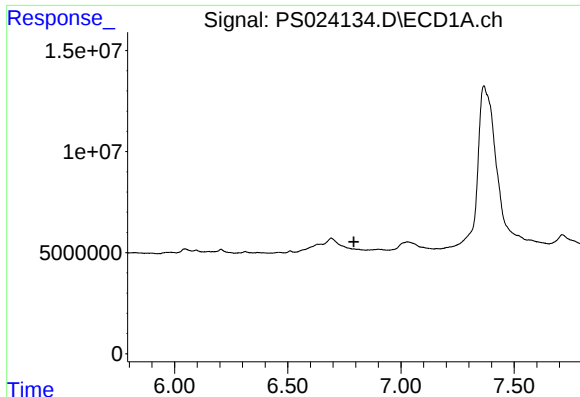

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.792 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

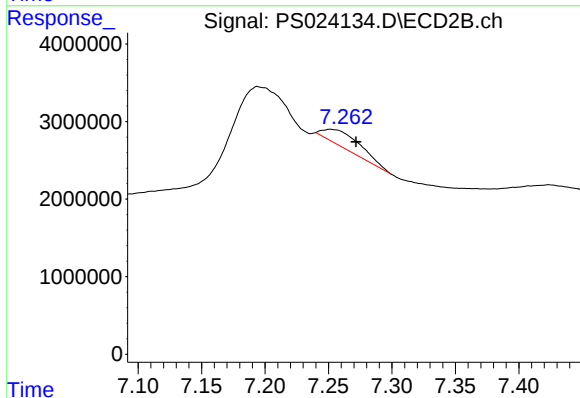


#7 MCPA

R.T.: 7.252 min
Delta R.T.: -0.020 min
Response: 4044479
Conc: 1.38 ug/ml

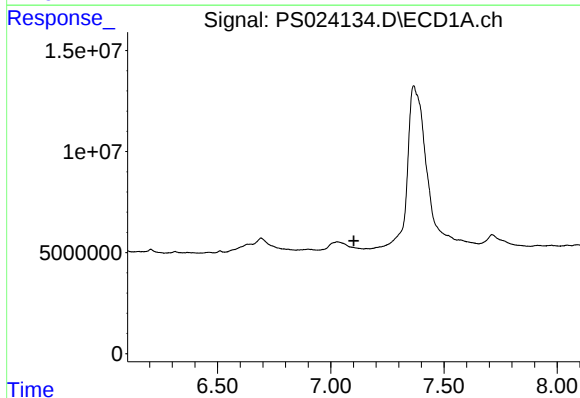


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.102 min
Response: 0
Conc: N.D.

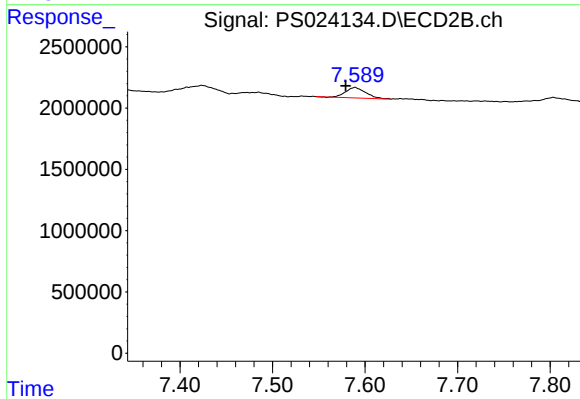

#8 DICHLORPROP


R.T.: 7.589 min
Delta R.T.: 0.010 min
Response: 1314979
Conc: 1.80 ng/ml

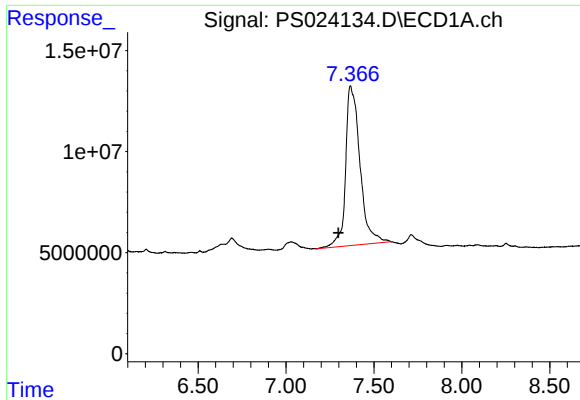

#9 2,4-D

R.T.: 7.366 min
Delta R.T.: 0.068 min
Response: 447161771
Conc: 180.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

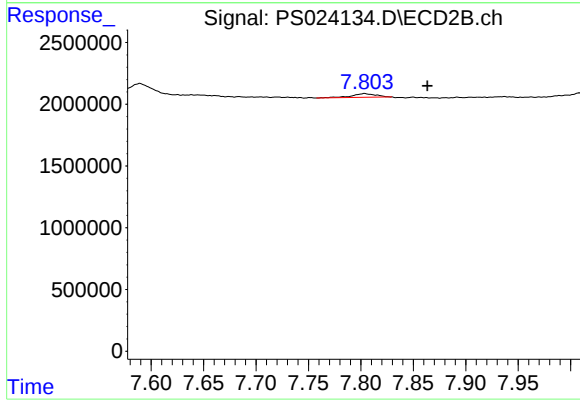

#9 2,4-D

R.T.: 7.804 min
Delta R.T.: -0.060 min
Response: 468064
Conc: N.D.