

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082324\
 Data File : PS027515.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2024 14:08
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 09:08:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081924.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 19 14:50:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.157	7.736	1270.1E6	1011.1E6	491.095	512.161
Target Compounds							
1) T	Dalapon	0.000	2.705	0	2201575	N.D.	<MDL
2) T	3,5-DICHL...	0.000	6.697	0	1741491	N.D.	<MDL
3) T	4-Nitroph...	6.948	0.000	28496951	0	18.300	N.D. #
5) T	DICAMBA	0.000	7.931	0	6025294	N.D.	<MDL
6) T	MCP	0.000	8.036	0	4933285	N.D.	<MDL
8) T	DICHLORPROP	8.058	8.697f	2667395	13946586	<MDL	6.272 #
9) T	2,4-D	8.269	0.000	51831102	0	17.783	N.D. #
10) T	Pentachlo...	8.576	9.496	7253181	1167078	<MDL	<MDL #
11) T	2,4,5-TP ...	9.091f	9.891	4402182	2059211	<MDL	<MDL #
12) T	2,4,5-T	9.414	10.296	4325578	3645914	<MDL	<MDL #
13) T	2,4-DB	0.000	10.884	0	141119	N.D.	<MDL
14) T	DINOSEB	11.151	0.000	1137918	0	<MDL	N.D. #
15) T	Picloram	10.955f	12.331	85067834	64655269	4.234	3.303
16) T	DCPA	0.000	12.238f	0	13112695	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082324\
Data File : PS027515.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2024 14:08
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 09:08:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081924.M
Quant Title : 8080.M
QLast Update : Mon Aug 19 14:50:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

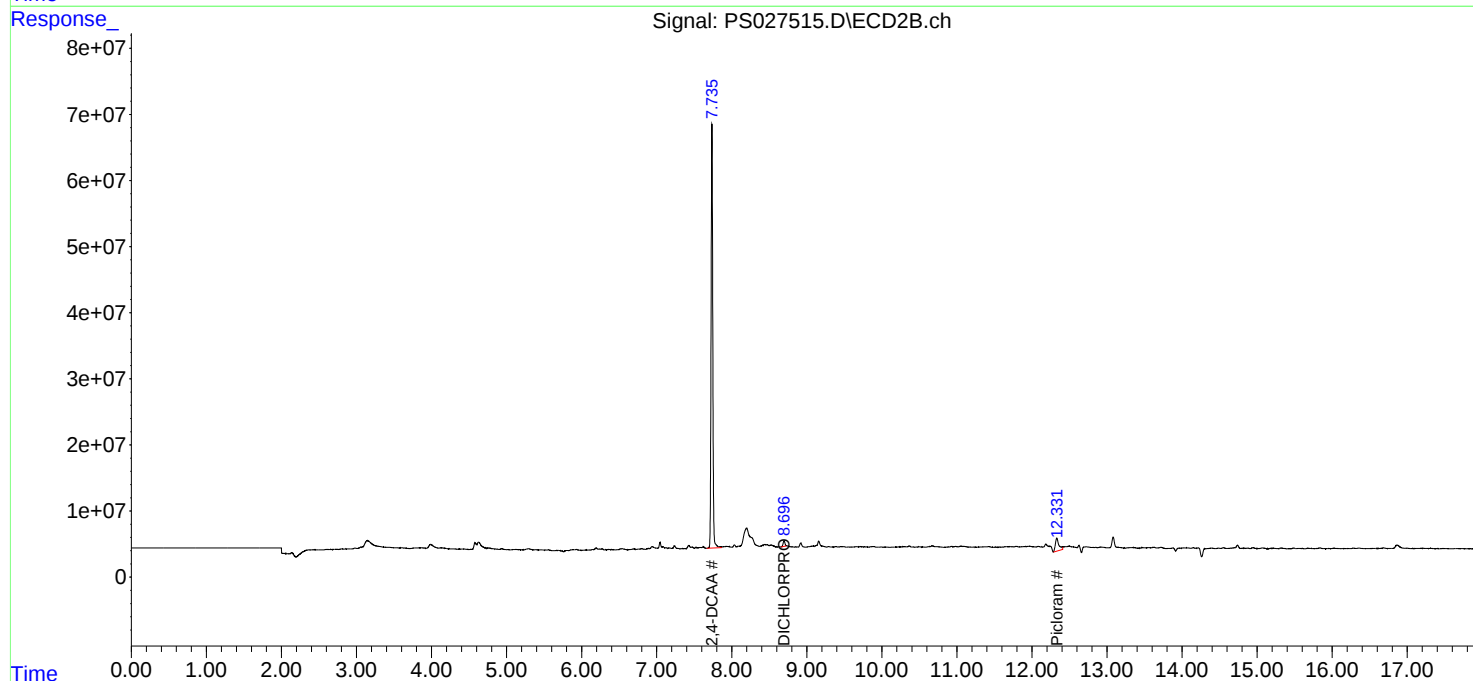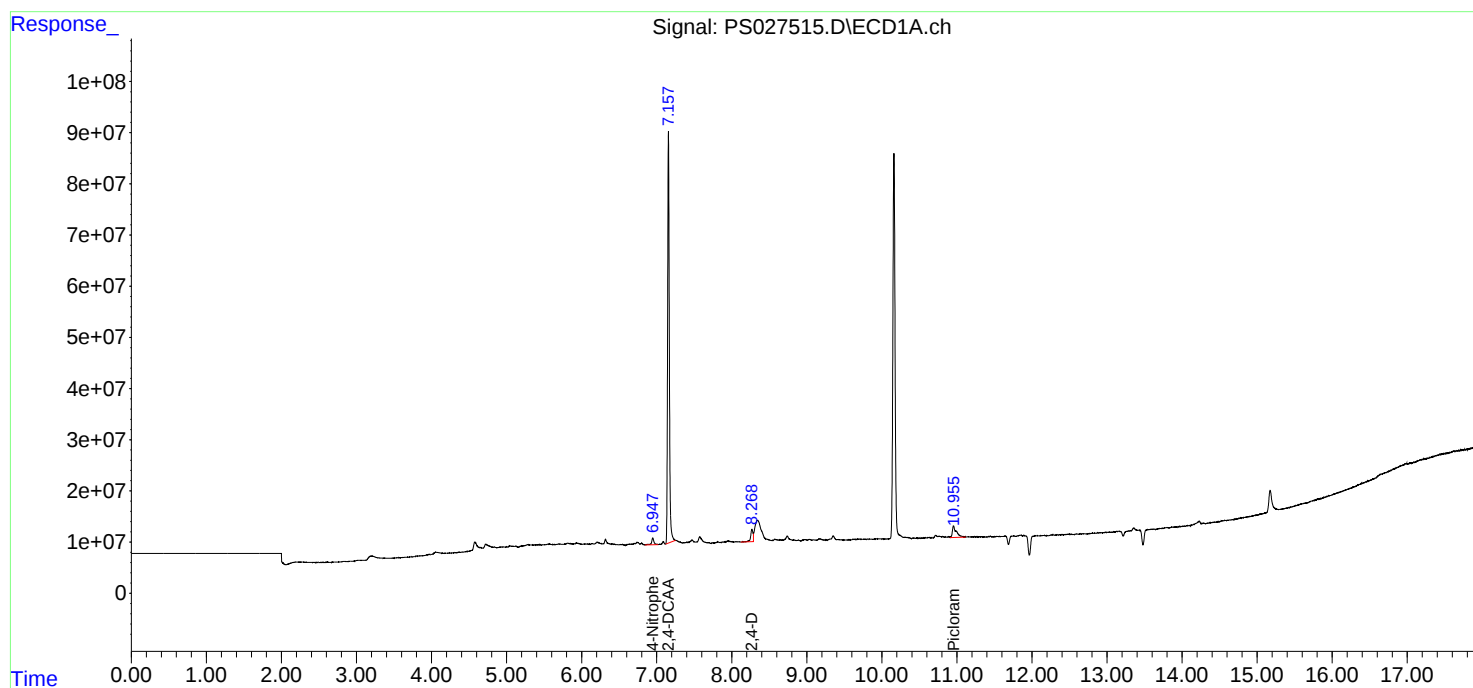


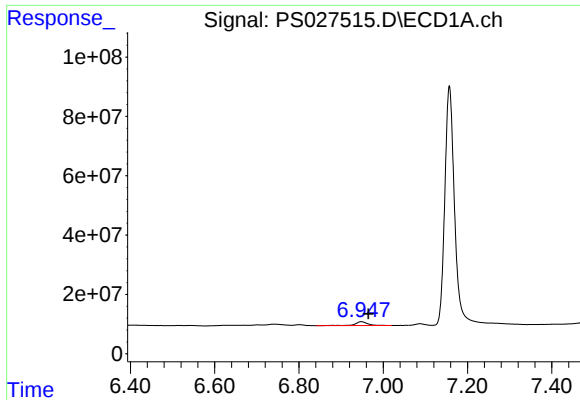

#3 4-Nitrophenol


R.T.: 6.948 min
Delta R.T.: -0.016 min
Response: 28496951
Conc: 18.30 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

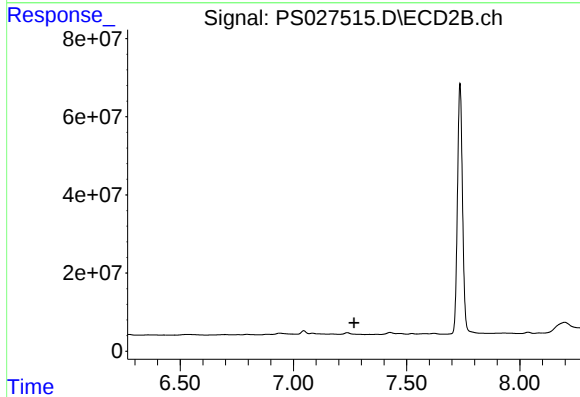


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 7.267 min
Response: 0
Conc: N.D.

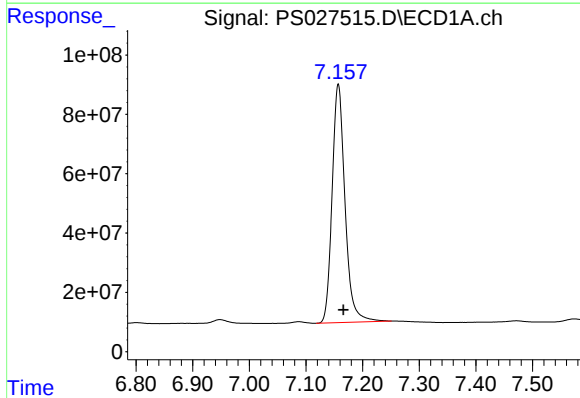


#4 2,4-DCAA

R.T.: 7.157 min
Delta R.T.: -0.009 min
Response: 1270098353
Conc: 491.09 ng/ml

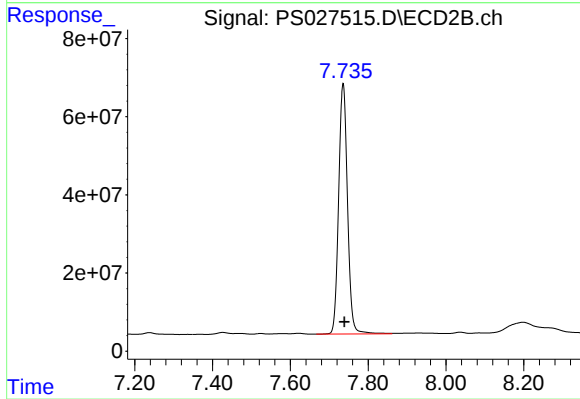

#4 2,4-DCAA


R.T.: 7.736 min
Delta R.T.: -0.003 min
Response: 1011124921
Conc: 512.16 ng/ml

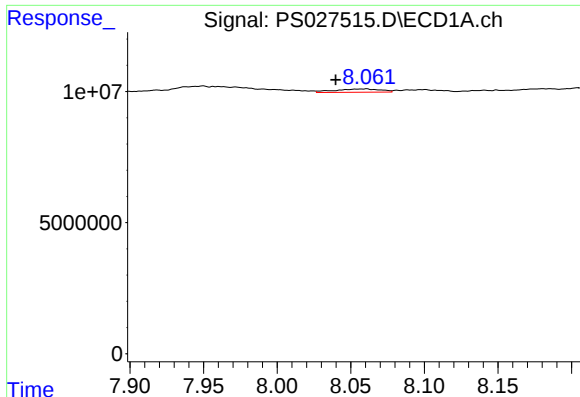

#8 DICHLORPROP


R.T.: 8.058 min
Delta R.T.: 0.018 min
Response: 2667395
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

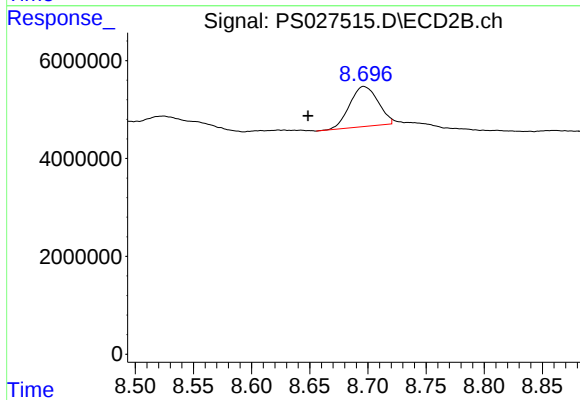


#8 DICHLORPROP

R.T.: 8.697 min
Delta R.T.: 0.048 min
Response: 13946586
Conc: 6.27 ng/ml

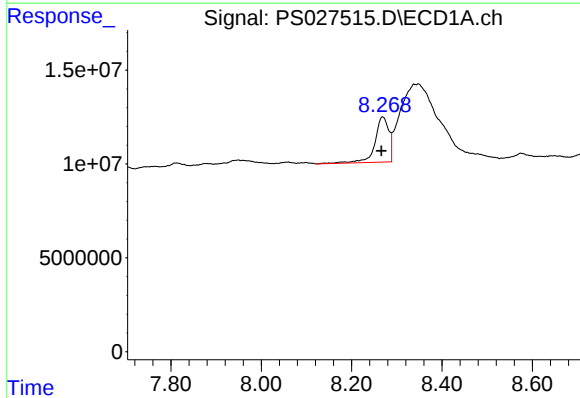


#9 2,4-D

R.T.: 8.269 min
Delta R.T.: 0.003 min
Response: 51831102
Conc: 17.78 ng/ml

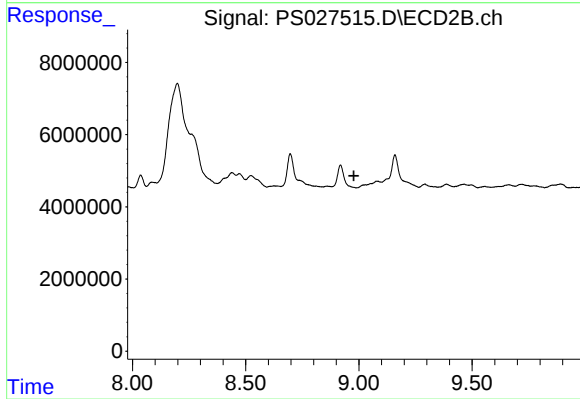

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.978 min
Response: 0
Conc: N.D.

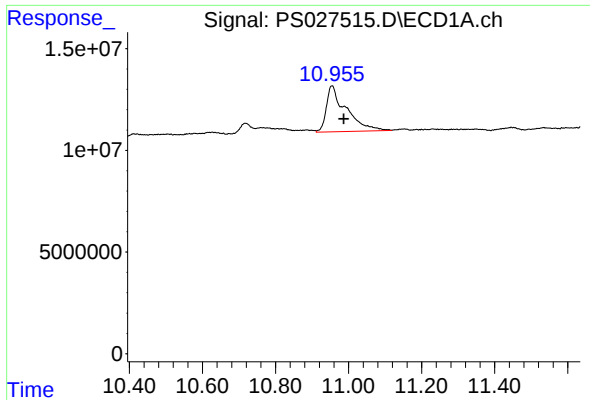

#15 Picloram

R.T.: 10.955 min
Delta R.T.: -0.032 min
Response: 85067834
Conc: 4.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

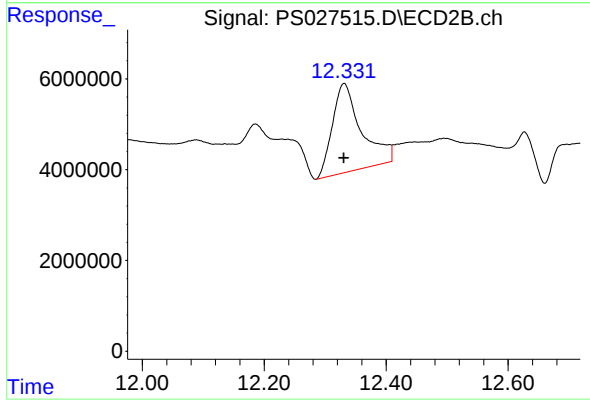

#15 Picloram

R.T.: 12.331 min
Delta R.T.: 0.000 min
Response: 64655269
Conc: 3.30 ng/ml