

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS082418\  
 Data File : PS001602.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 24 Aug 2018 18:16  
 Operator : UA  
 Sample : J4621-05  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Aug 25 02:00:34 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS082218.M  
 Quant Title : 8080.M  
 QLast Update : Thu Aug 23 02:55:24 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1   | RT#2   | Resp#1   | Resp#2   | ng/ml   | ng/ml    |
|-----------------------------|--------------|--------|--------|----------|----------|---------|----------|
| -----                       |              |        |        |          |          |         |          |
| System Monitoring Compounds |              |        |        |          |          |         |          |
| 4) S                        | 2,4-DCAA     | 11.486 | 10.984 | 61330229 | 58524601 | 332.232 | 288.968  |
| Target Compounds            |              |        |        |          |          |         |          |
| 1) T                        | Dalapon      | 0.000  | 2.386  | 0        | 10548389 | N.D.    | 44.075 # |
| 6) T                        | MCP          | 12.175 | 0.000  | 10013507 | 0        | 19.901  | N.D. #   |
| 10) T                       | Pentachlo... | 13.731 | 0.000  | 2885925  | 0        | 1.157   | N.D. #   |
| 12) T                       | 2,4,5-T      | 0.000  | 14.645 | 0        | 2175312  | N.D.    | 2.518 #  |
| 15) T                       | Picloram     | 16.981 | 16.916 | 8810923  | 6139335  | 6.291   | 4.708 #  |
| 16) T                       | DCPA         | 0.000  | 16.916 | 0        | 6139335  | N.D.    | 4.300 #  |
| -----                       |              |        |        |          |          |         |          |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS082418\  
Data File : PS001602.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 24 Aug 2018 18:16  
Operator : UA  
Sample : J4621-05  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Aug 25 02:00:34 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS082218.M  
Quant Title : 8080.M  
QLast Update : Thu Aug 23 02:55:24 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

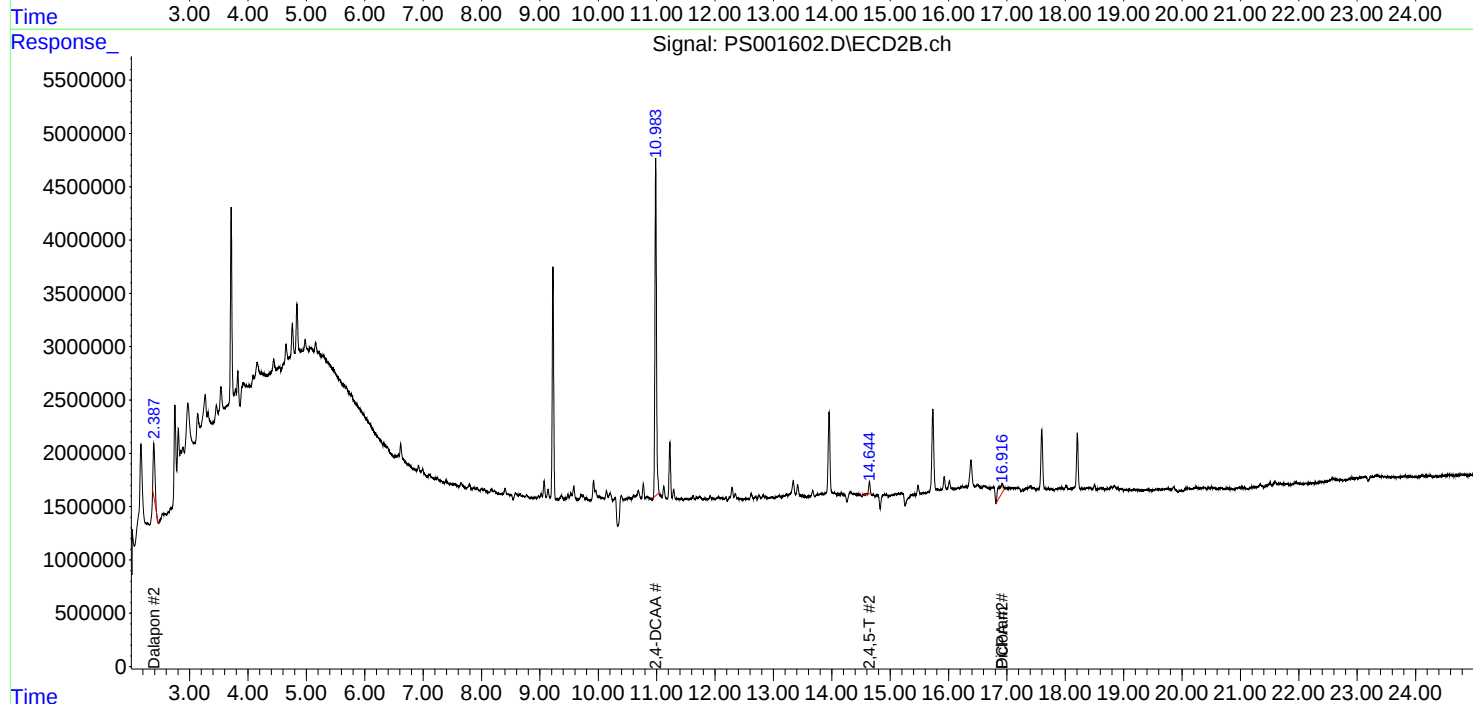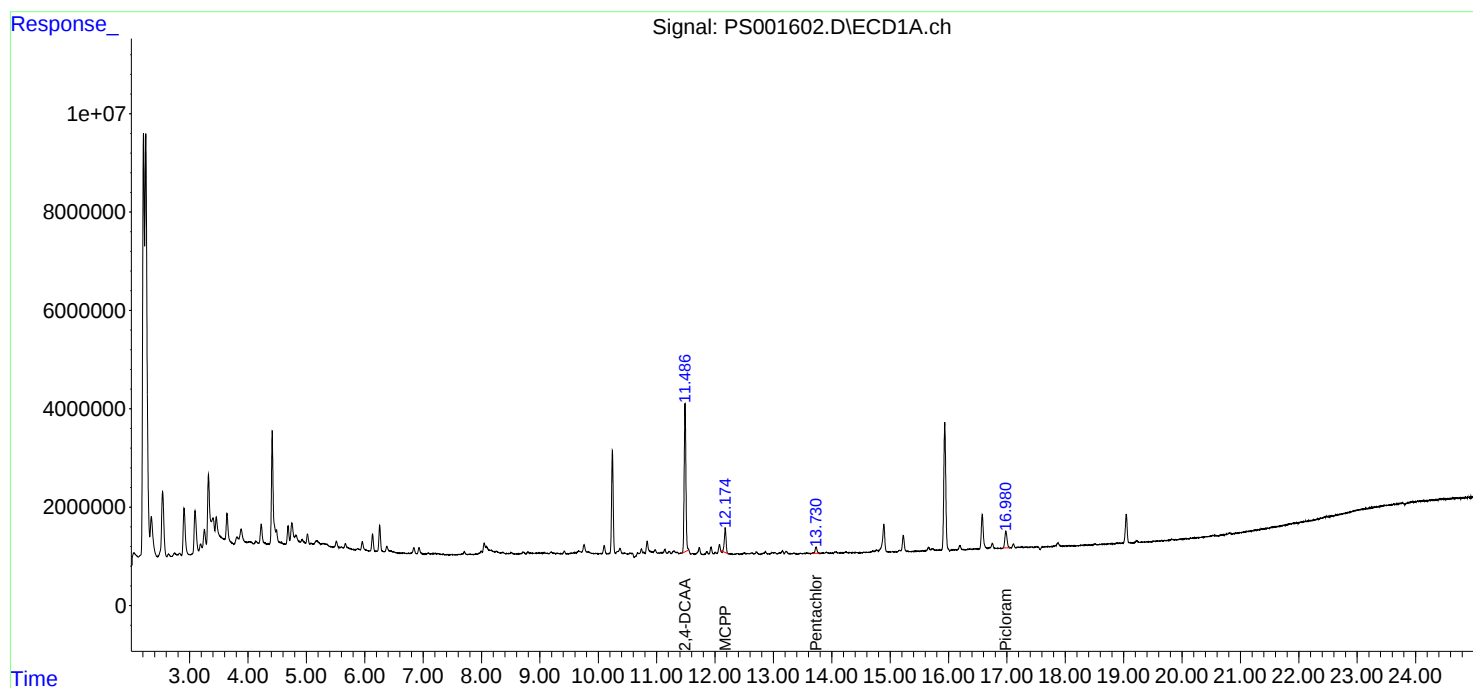


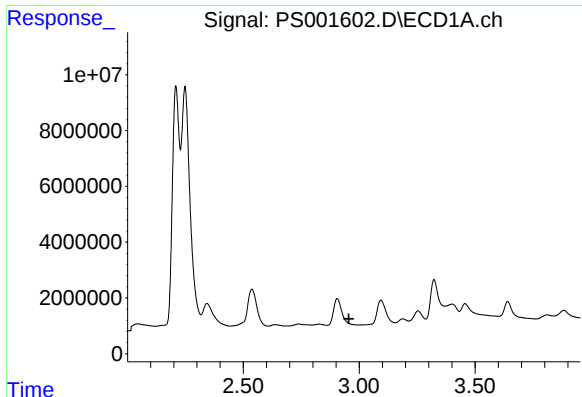

#1 Dalapon


R.T.: 0.000 min  
Exp R.T.: 2.954 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

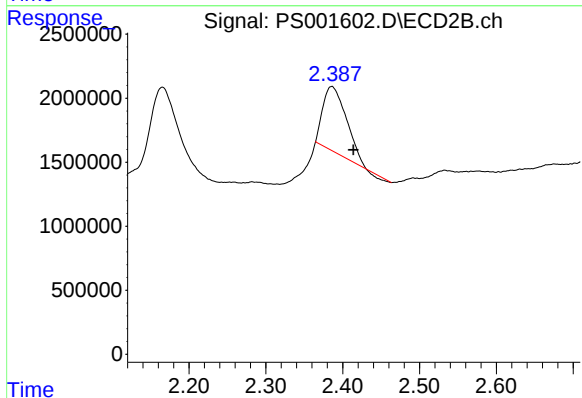


#1 Dalapon

R.T.: 2.386 min  
Delta R.T.: -0.028 min  
Response: 10548389  
Conc: 44.07 ng/ml

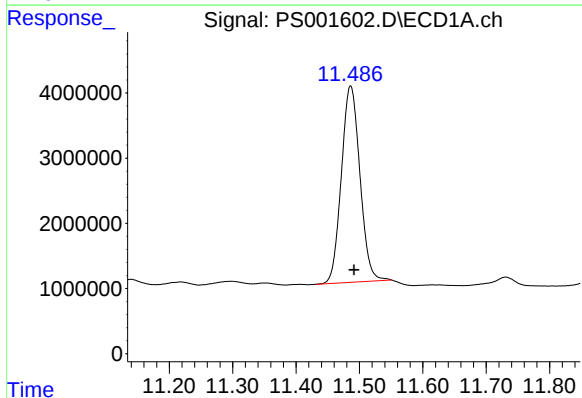


#4 2,4-DCAA

R.T.: 11.486 min  
Delta R.T.: -0.006 min  
Response: 61330229  
Conc: 332.23 ng/ml

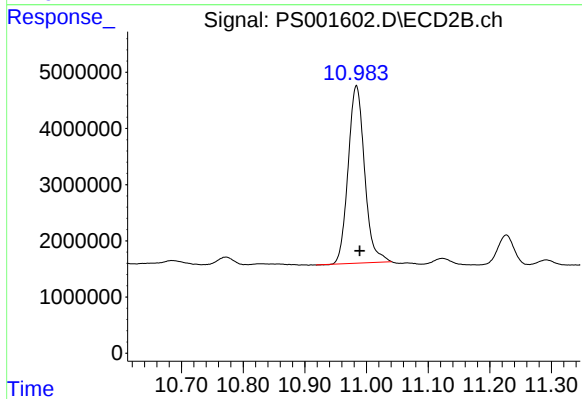

#4 2,4-DCAA


R.T.: 10.984 min  
Delta R.T.: -0.005 min  
Response: 58524601  
Conc: 288.97 ng/ml

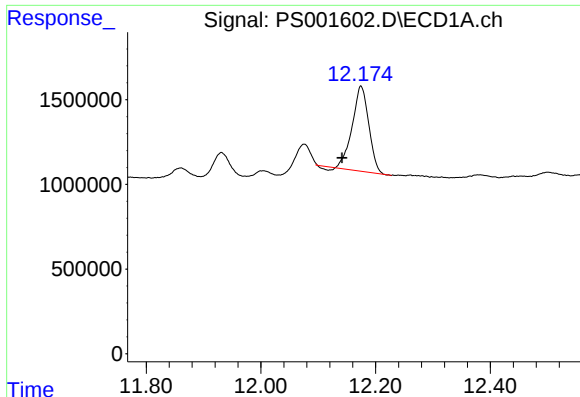

#6 MCP


R.T.: 12.175 min  
Delta R.T.: 0.033 min  
Response: 10013507  
Conc: 19.90 ug/ml

Instrument :  
ECD\_S  
ClientSampleId :

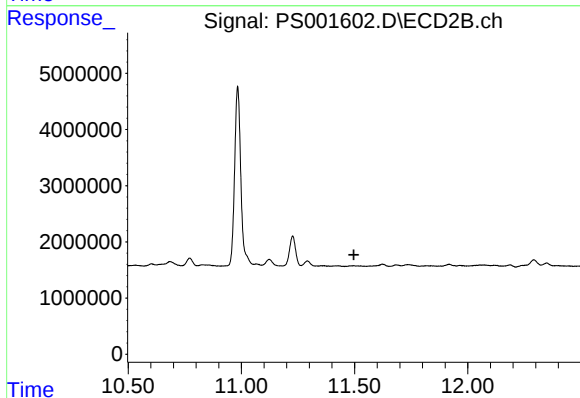


#6 MCP

R.T.: 0.000 min  
Exp R.T. : 11.497 min  
Response: 0  
Conc: N.D.

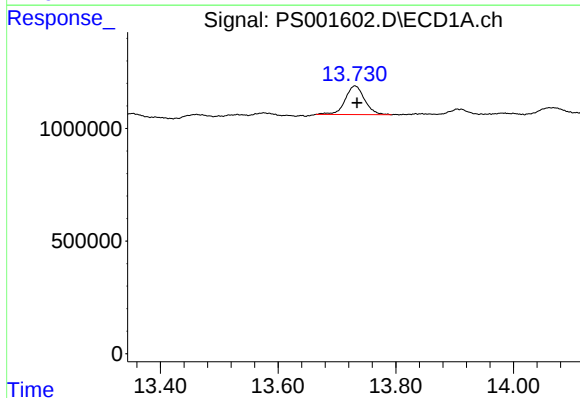


#10 Pentachlorophenol

R.T.: 13.731 min  
Delta R.T.: -0.003 min  
Response: 2885925  
Conc: 1.16 ng/ml

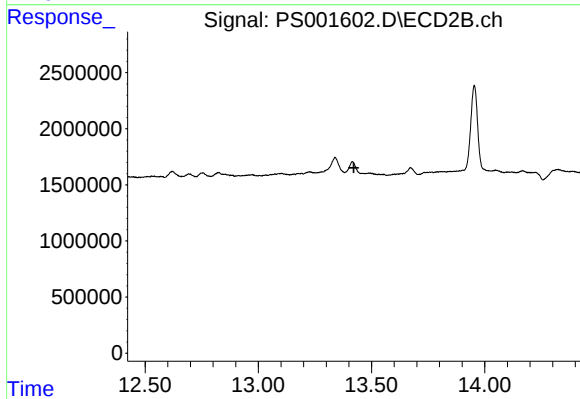

#10 Pentachlorophenol


R.T.: 0.000 min  
Exp R.T. : 13.422 min  
Response: 0  
Conc: N.D.

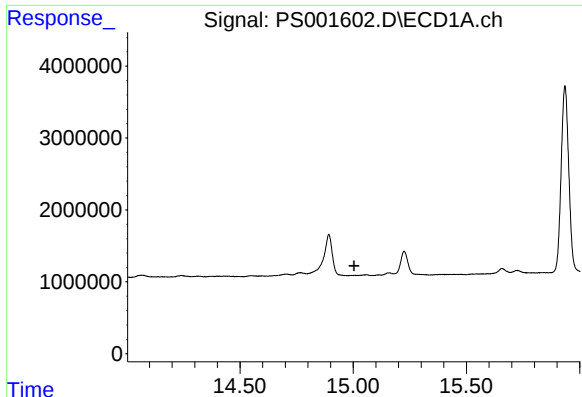

#12 2,4,5-T


R.T.: 0.000 min  
Exp R.T.: 15.003 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

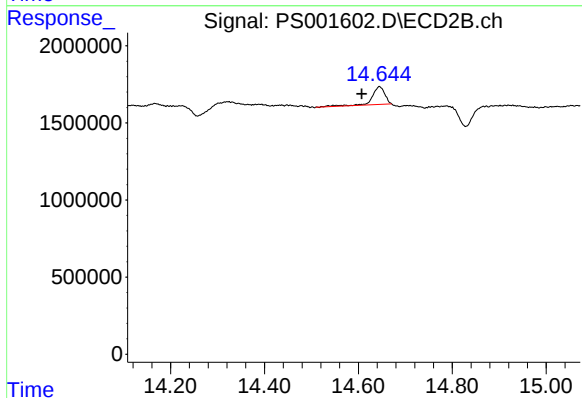


#12 2,4,5-T

R.T.: 14.645 min  
Delta R.T.: 0.038 min  
Response: 2175312  
Conc: 2.52 ng/ml

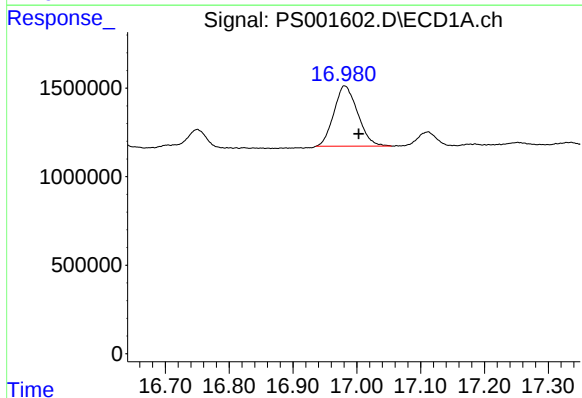


#15 Picloram

R.T.: 16.981 min  
Delta R.T.: -0.022 min  
Response: 8810923  
Conc: 6.29 ng/ml

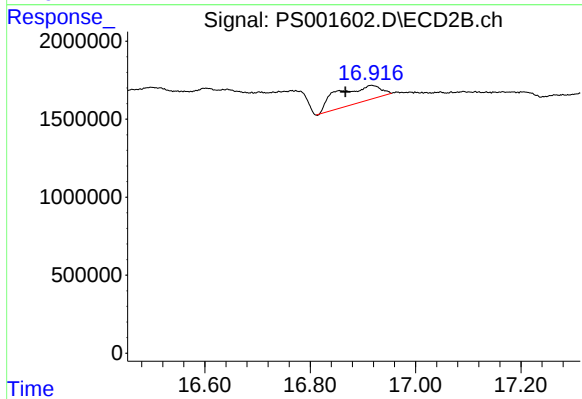

#15 Picloram


R.T.: 16.916 min  
Delta R.T.: 0.049 min  
Response: 6139335  
Conc: 4.71 ng/ml

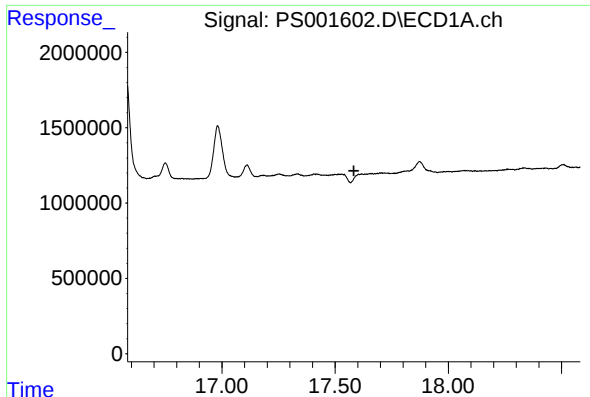

#16 DCPA

R.T.: 0.000 min  
Exp R.T.: 17.583 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

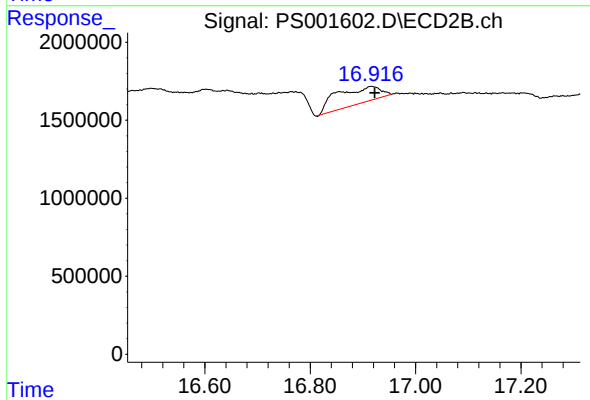

#16 DCPA

R.T.: 16.916 min  
Delta R.T.: -0.006 min  
Response: 6139335  
Conc: 4.30 ng/ml