

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082418\
 Data File : PS001603.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Aug 2018 18:47
 Operator : UA
 Sample : J4621-09
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 02:00:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.489	10.987	66025567	61830495	357.667	305.291
Target Compounds							
1) T	Dalapon	0.000	2.389	0	12501263	N.D.	52.235 #
5) T	DICAMBA	0.000	11.230	0	2543030	N.D.	3.626 #
6) T	MCPD	12.178	0.000	10867332	0	21.598	N.D. #
15) T	Picloram	16.981	16.922	6802413	5873620	4.857	4.504
16) T	DCPA	0.000	16.922	0	5873620	N.D.	4.114 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082418\
Data File : PS001603.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Aug 2018 18:47
Operator : UA
Sample : J4621-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 02:00:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

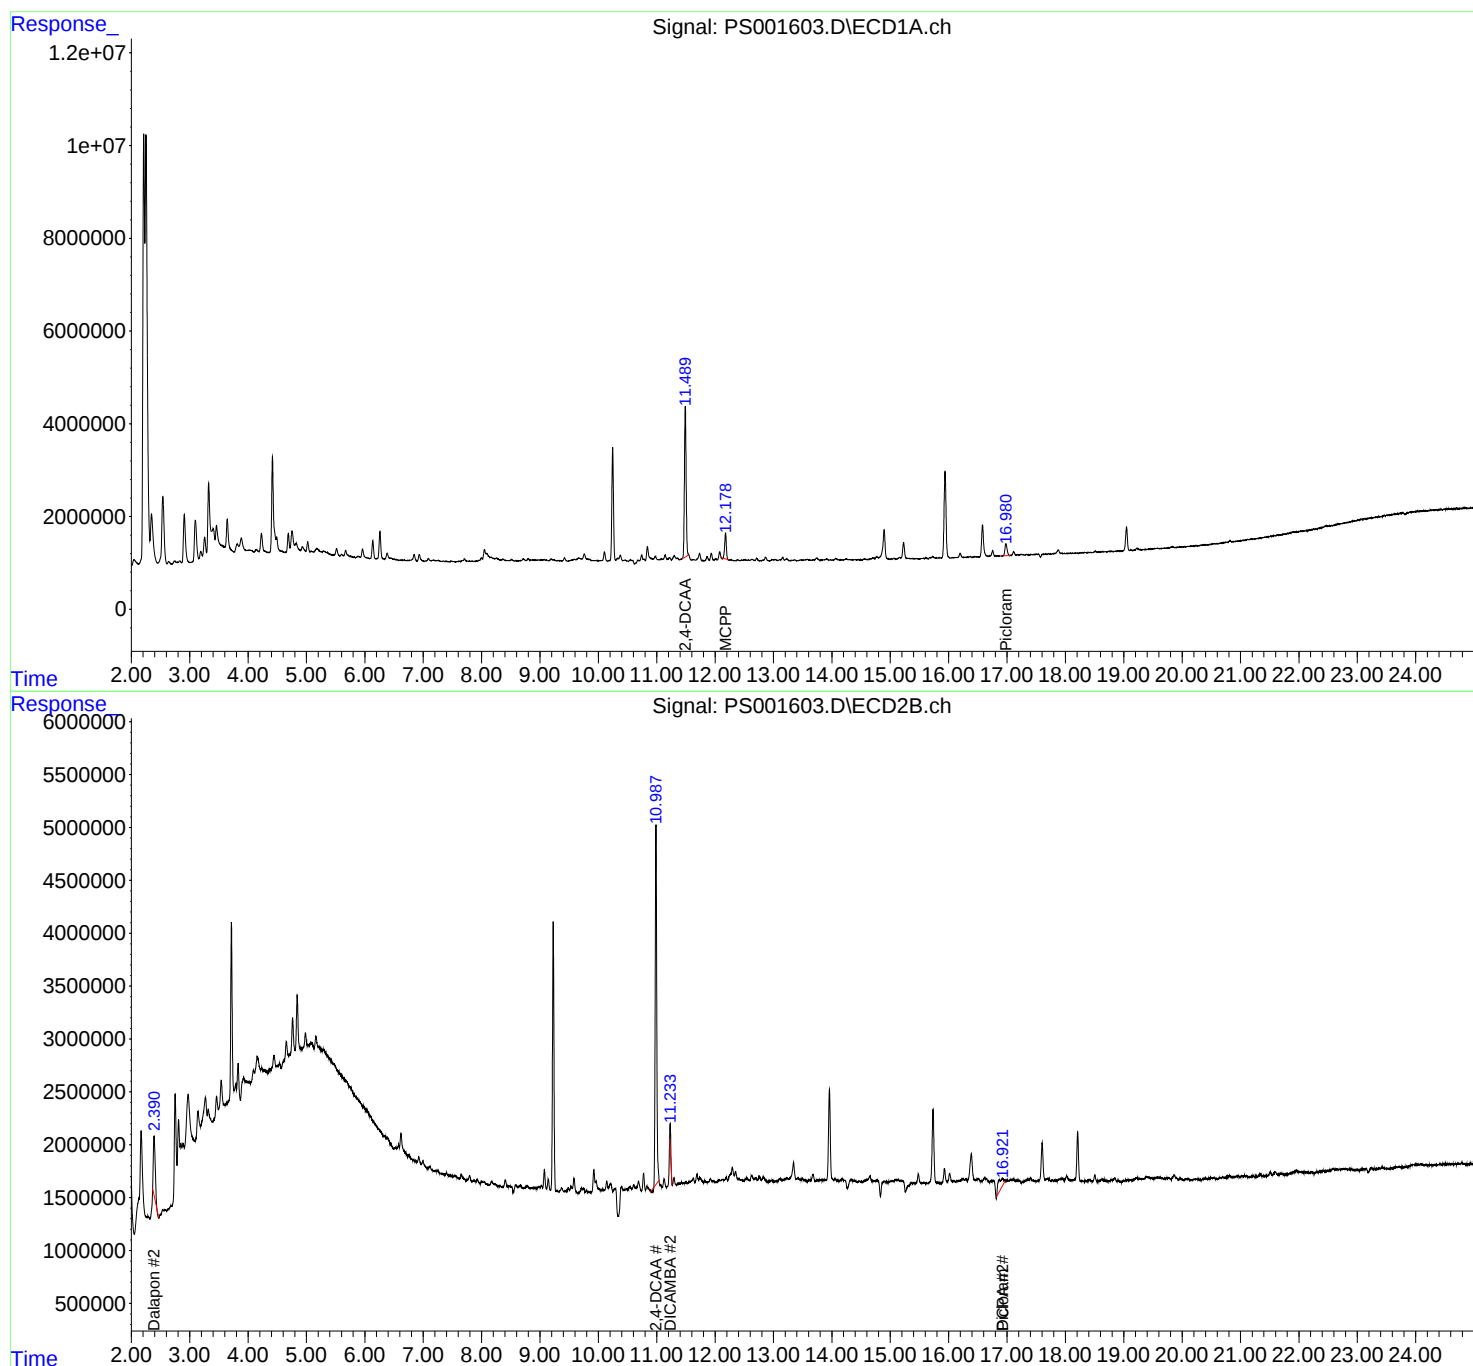


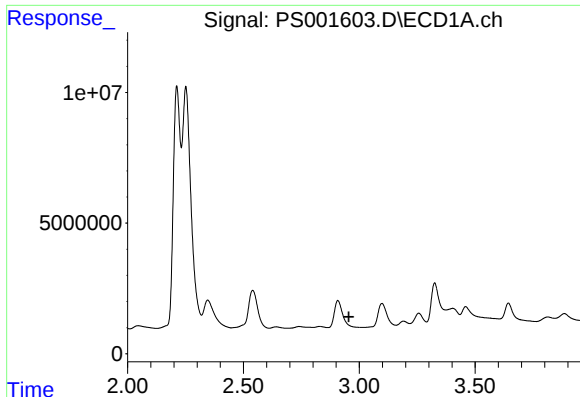

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.954 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

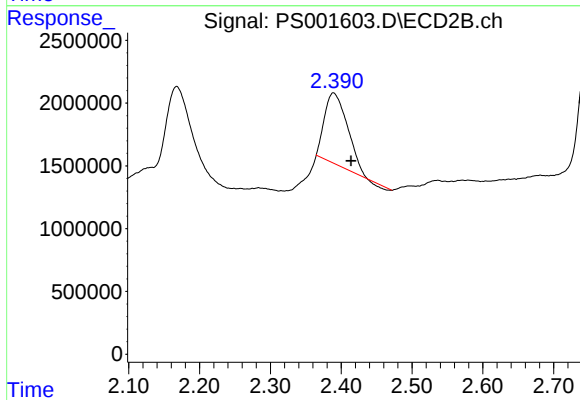


#1 Dalapon

R.T.: 2.389 min
Delta R.T.: -0.025 min
Response: 12501263
Conc: 52.23 ng/ml

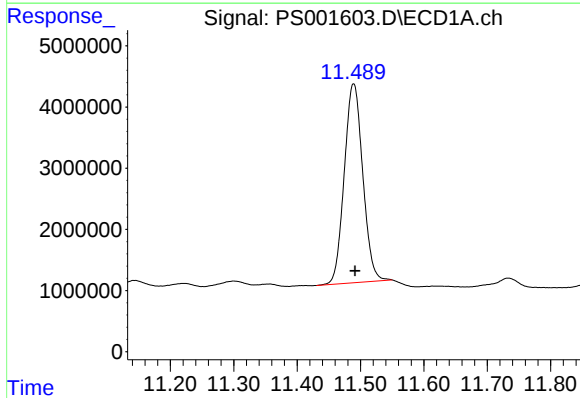


#4 2,4-DCAA

R.T.: 11.489 min
Delta R.T.: -0.003 min
Response: 66025567
Conc: 357.67 ng/ml

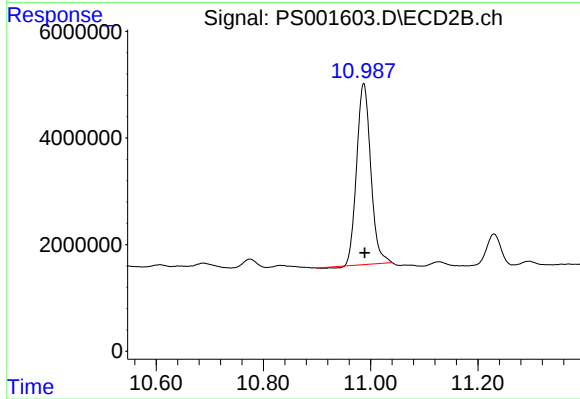

#4 2,4-DCAA


R.T.: 10.987 min
Delta R.T.: -0.002 min
Response: 61830495
Conc: 305.29 ng/ml

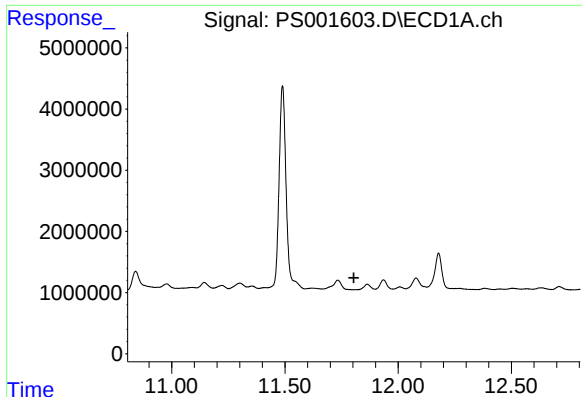

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.805 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

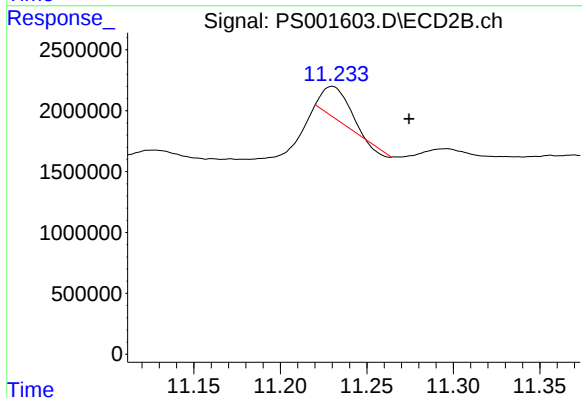


#5 DICAMBA

R.T.: 11.230 min
Delta R.T.: -0.044 min
Response: 2543030
Conc: 3.63 ng/ml

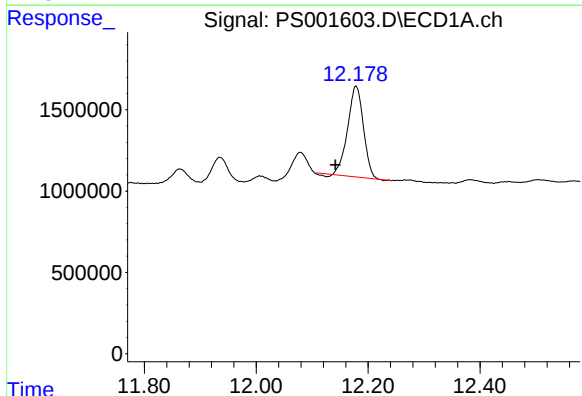


#6 MCP

R.T.: 12.178 min
Delta R.T.: 0.037 min
Response: 10867332
Conc: 21.60 ug/ml

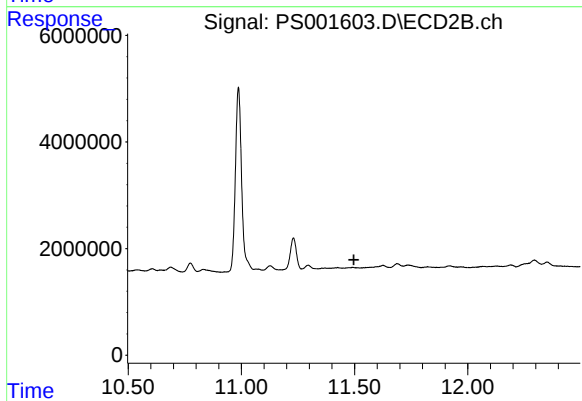

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.497 min
Response: 0
Conc: N.D.

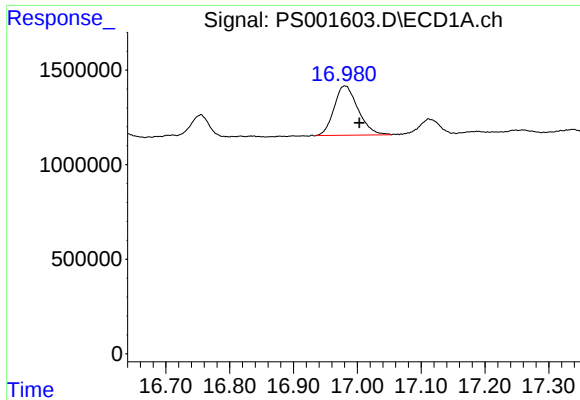

#15 Picloram


R.T.: 16.981 min
Delta R.T.: -0.022 min
Response: 6802413
Conc: 4.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

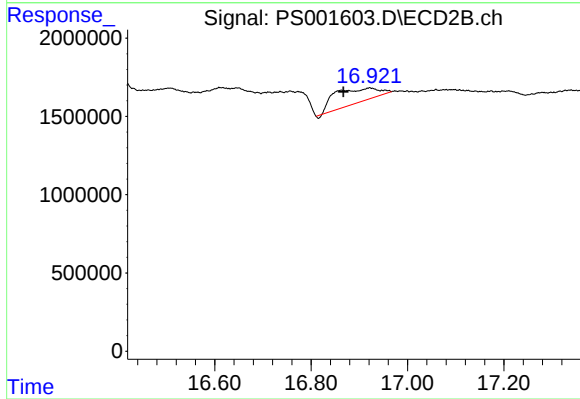


#15 Picloram

R.T.: 16.922 min
Delta R.T.: 0.054 min
Response: 5873620
Conc: 4.50 ng/ml

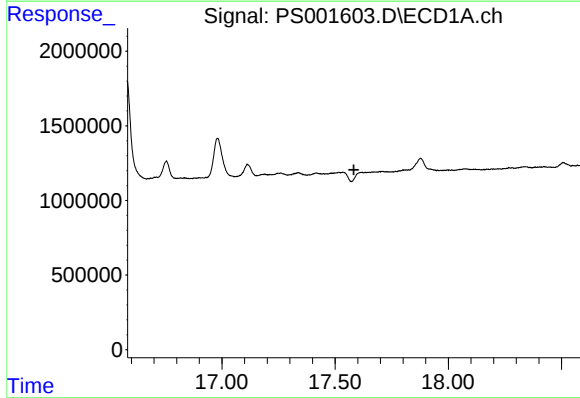

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.583 min
Response: 0
Conc: N.D.

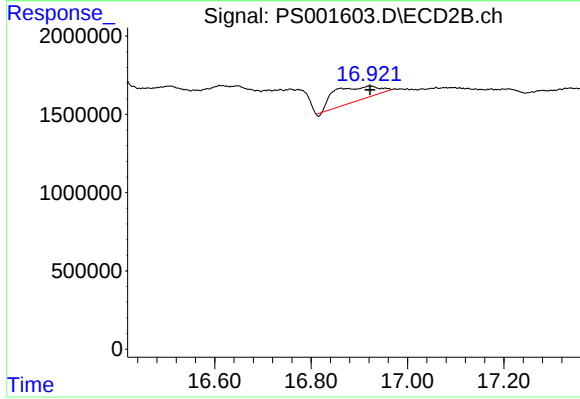

#16 DCPA

R.T.: 16.922 min
Delta R.T.: 0.000 min
Response: 5873620
Conc: 4.11 ng/ml