

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082420\
 Data File : PS011884.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Aug 2020 11:50
 Operator : DD\AJ
 Sample : L3506-10RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 13:15:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.221	6.912	842.3E6	505.2E6	772.236	944.595
Target Compounds							
2) T	3,5-DICHL...	6.476	6.093	4788311	55952487	3.303	68.017 #
5) T	DICAMBA	0.000	7.048	0	12936284	N.D.	5.988
6) T	MCP	7.633	0.000	5882431	0	1.841	N.D. #
7) T	MCPA	7.702	0.000	44581868	0	9.801	N.D. #
8) T	DICHLORPROP	0.000	7.735	0	45541946	N.D.	80.657
9) T	2,4-D	0.000	7.941	0	24397523	N.D.	33.209
11) T	2,4,5-TP ...	0.000	8.761	0	16455936	N.D.	5.629
12) T	2,4,5-T	9.416	9.240	22533204	12978704	3.803	4.385
15) T	Picloram	11.029	11.006	43460313	29292839	5.561	6.463
16) T	DCPA	11.460	11.006	6190569	29292839	<MDL	7.967 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082420\
Data File : PS011884.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Aug 2020 11:50
Operator : DD\AJ
Sample : L3506-10RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 13:15:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

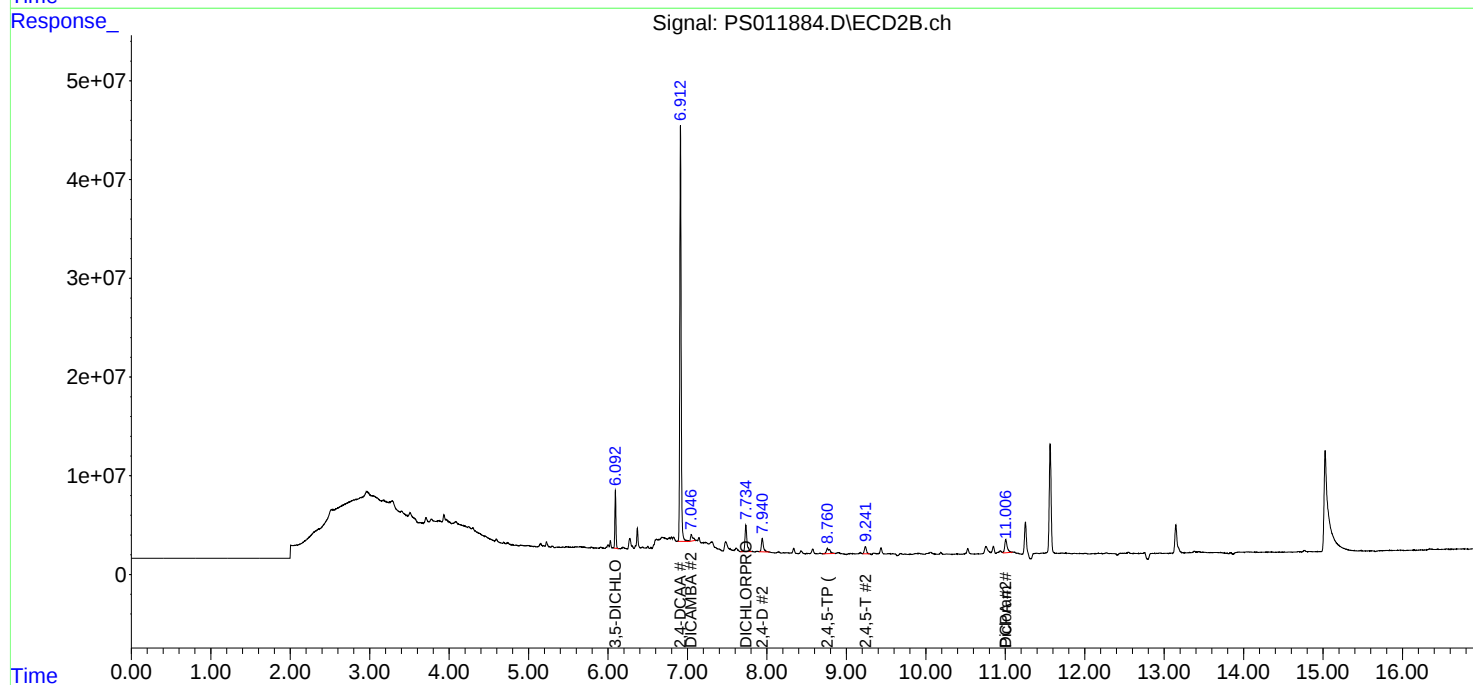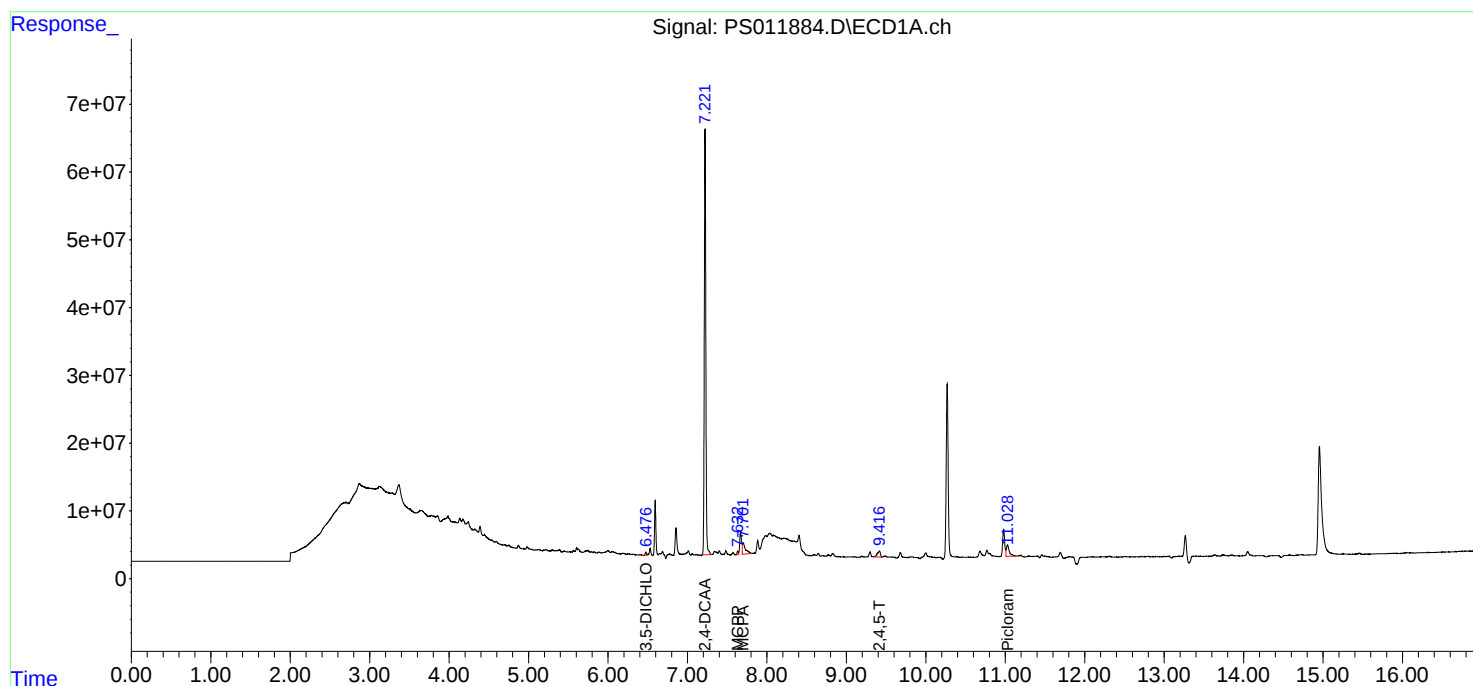


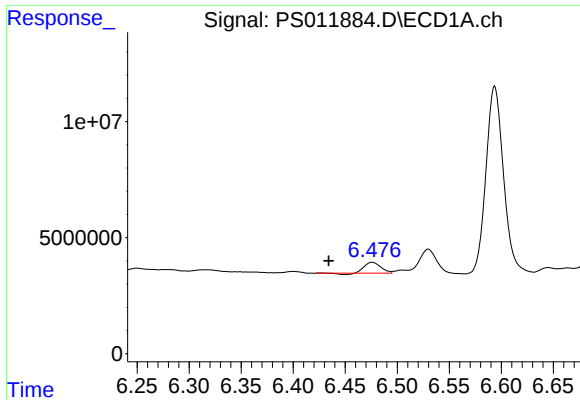

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.476 min
Delta R.T.: 0.042 min
Response: 4788311
Conc: 3.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

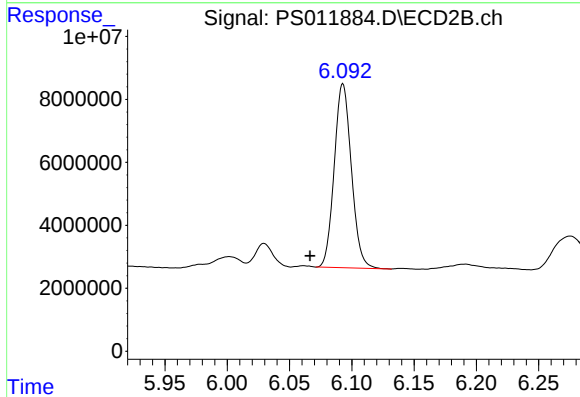


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.093 min
Delta R.T.: 0.026 min
Response: 55952487
Conc: 68.02 ng/ml

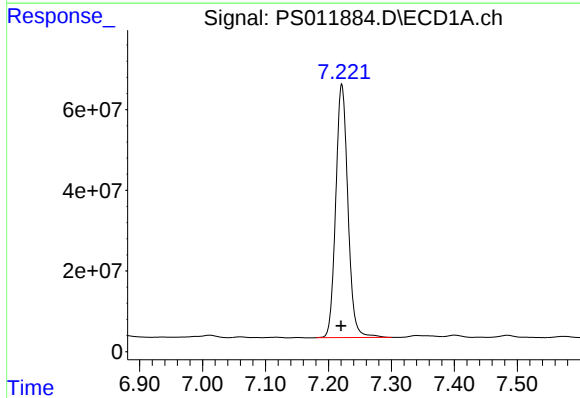


#4 2,4-DCAA

R.T.: 7.221 min
Delta R.T.: 0.001 min
Response: 842330845
Conc: 772.24 ng/ml

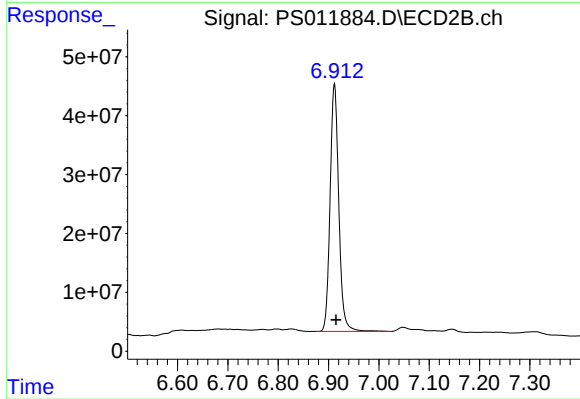

#4 2,4-DCAA


R.T.: 6.912 min
Delta R.T.: -0.003 min
Response: 505156734
Conc: 944.59 ng/ml

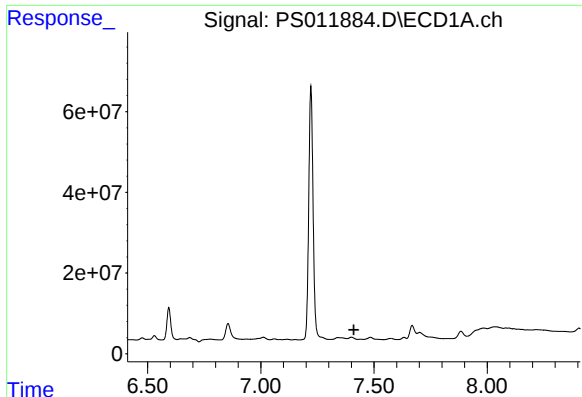

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

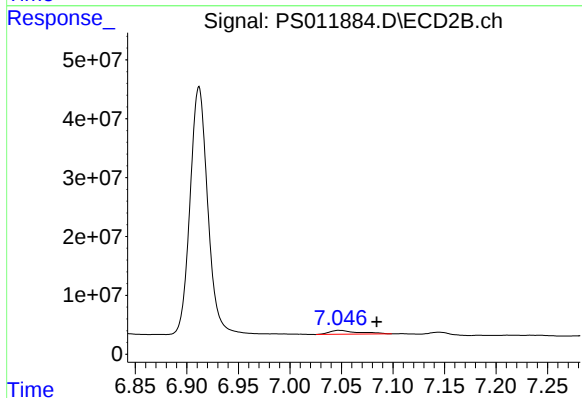


#5 DICAMBA

R.T.: 7.048 min
Delta R.T.: -0.036 min
Response: 12936284
Conc: 5.99 ng/ml

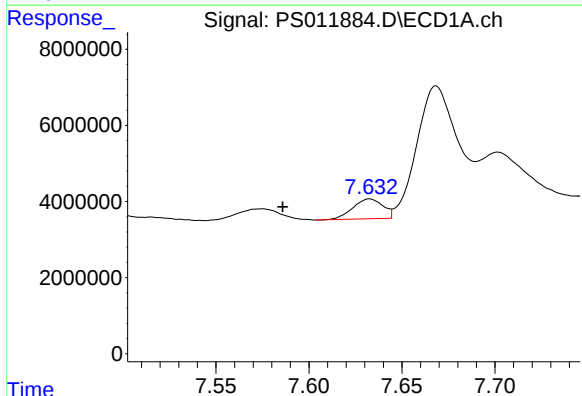


#6 MCP

R.T.: 7.633 min
Delta R.T.: 0.047 min
Response: 5882431
Conc: 1.84 ug/ml

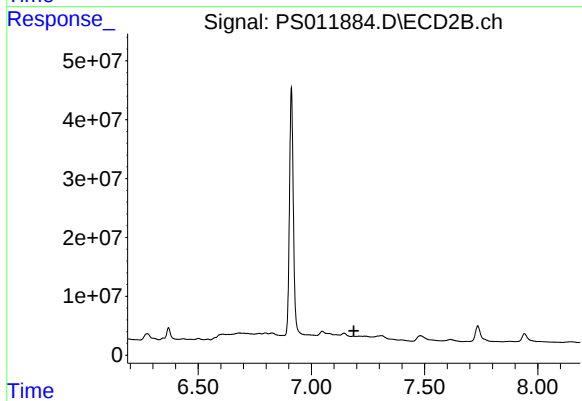

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.188 min
Response: 0
Conc: N.D.

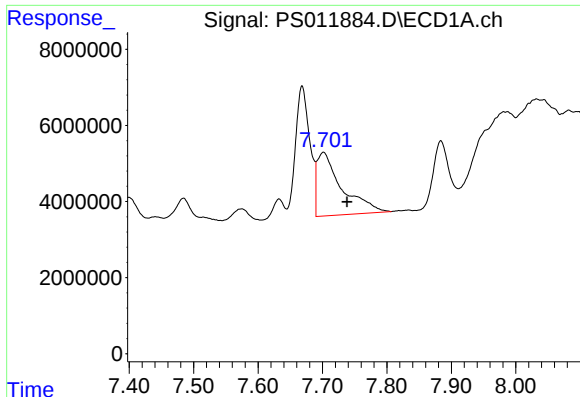

#7 MCPA


R.T.: 7.702 min
Delta R.T.: -0.037 min
Response: 44581868
Conc: 9.80 ug/ml

Instrument :
ECD_S
ClientSampleId :

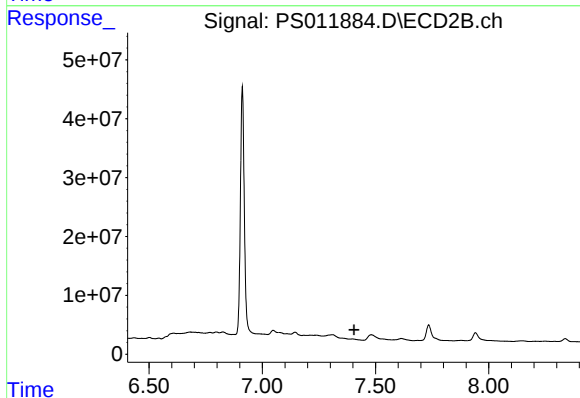


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.405 min
Response: 0
Conc: N.D.

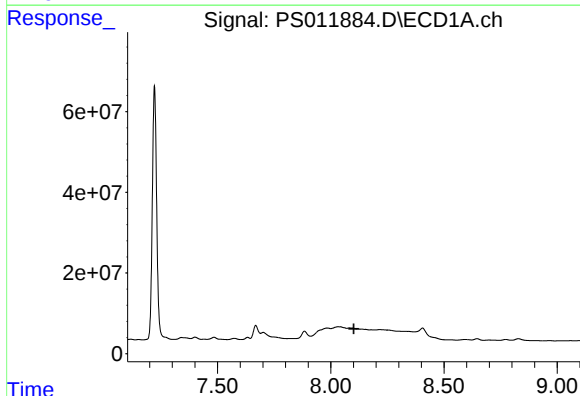


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.102 min
Response: 0
Conc: N.D.

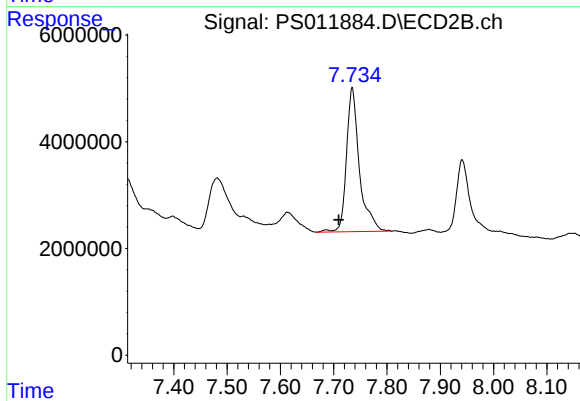

#8 DICHLORPROP


R.T.: 7.735 min
Delta R.T.: 0.025 min
Response: 45541946
Conc: 80.66 ng/ml

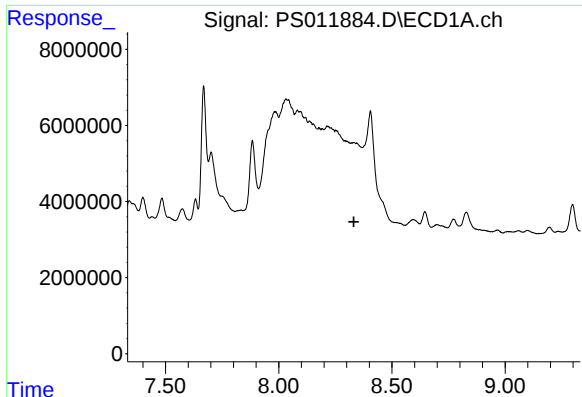

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.332 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

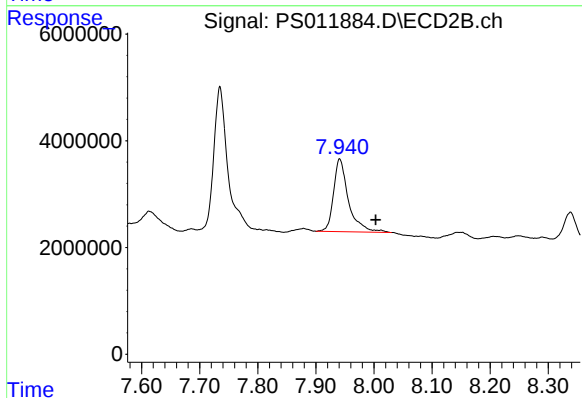


#9 2,4-D

R.T.: 7.941 min
Delta R.T.: -0.062 min
Response: 24397523
Conc: 33.21 ng/ml

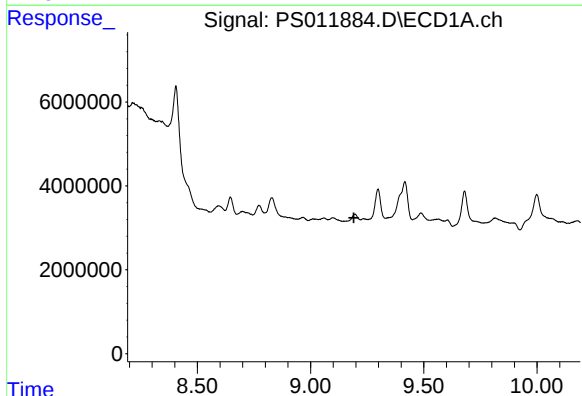


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

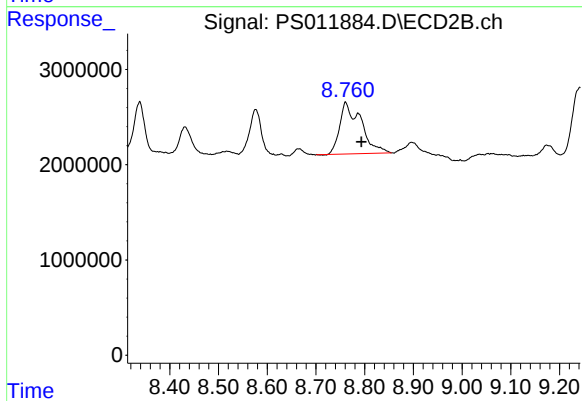

#11 2,4,5-TP (SILVEX)


R.T.: 8.761 min
Delta R.T.: -0.032 min
Response: 16455936
Conc: 5.63 ng/ml

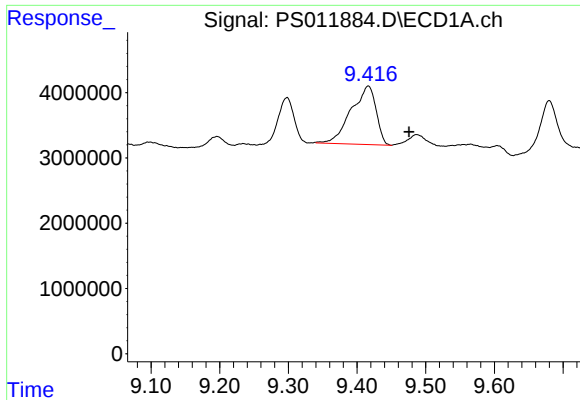

#12 2,4,5-T


R.T.: 9.416 min
Delta R.T.: -0.060 min
Response: 22533204
Conc: 3.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

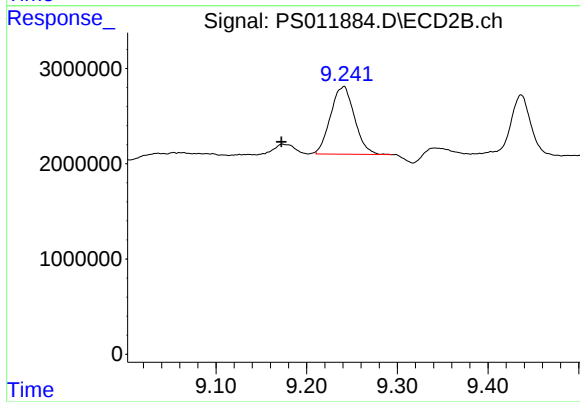


#12 2,4,5-T

R.T.: 9.240 min
Delta R.T.: 0.068 min
Response: 12978704
Conc: 4.38 ng/ml

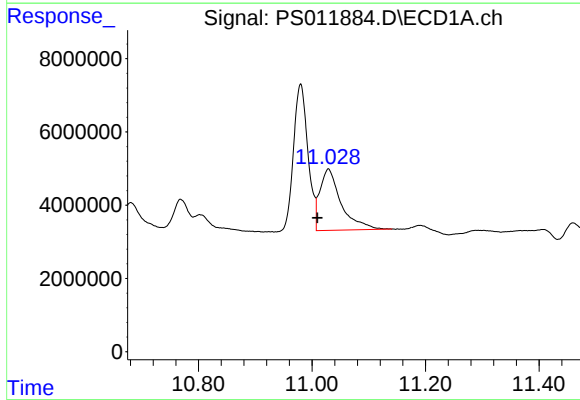


#15 Picloram

R.T.: 11.029 min
Delta R.T.: 0.019 min
Response: 43460313
Conc: 5.56 ng/ml

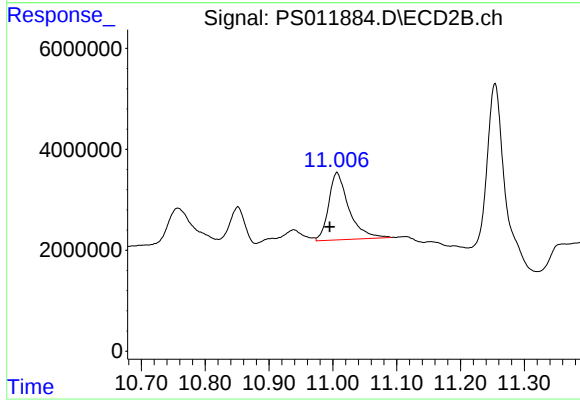

#15 Picloram


R.T.: 11.006 min
Delta R.T.: 0.011 min
Response: 29292839
Conc: 6.46 ng/ml

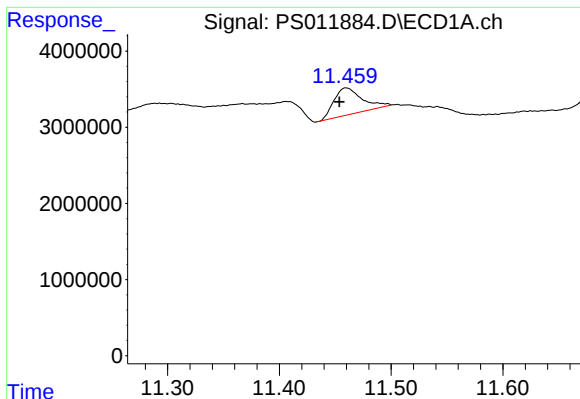

#16 DCPA

R.T.: 11.460 min
Delta R.T.: 0.006 min
Response: 6190569
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

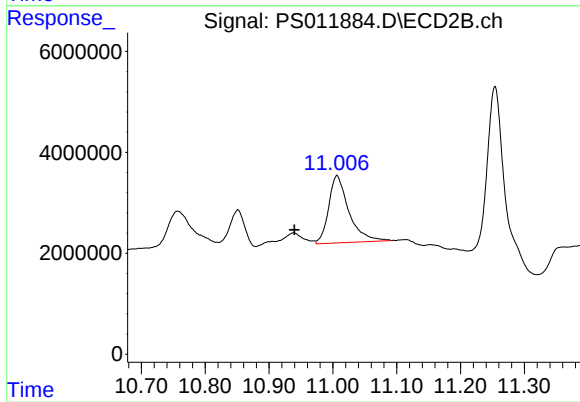

#16 DCPA

R.T.: 11.006 min
Delta R.T.: 0.067 min
Response: 29292839
Conc: 7.97 ng/ml