

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082421\
 Data File : PS016604.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Aug 2021 13:27
 Operator : DD\AJ
 Sample : M3434-07
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SWCS-11-1015

Manual Integrations
 APPROVED

mohammad
 8/25/2021 4:56:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 07:01:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 02 14:10:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.181	6.763	619.4E6	237.5E6	421.047	455.252m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082421\
Data File : PS016604.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Aug 2021 13:27
Operator : DD\AJ
Sample : M3434-07
Misc :
ALS Vial : 50 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
SWCS-11-1015


Manual Integrations
APPROVED

mohammad
8/25/2021 4:56:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 07:01:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
Quant Title : 8080.M
QLast Update : Mon Aug 02 14:10:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

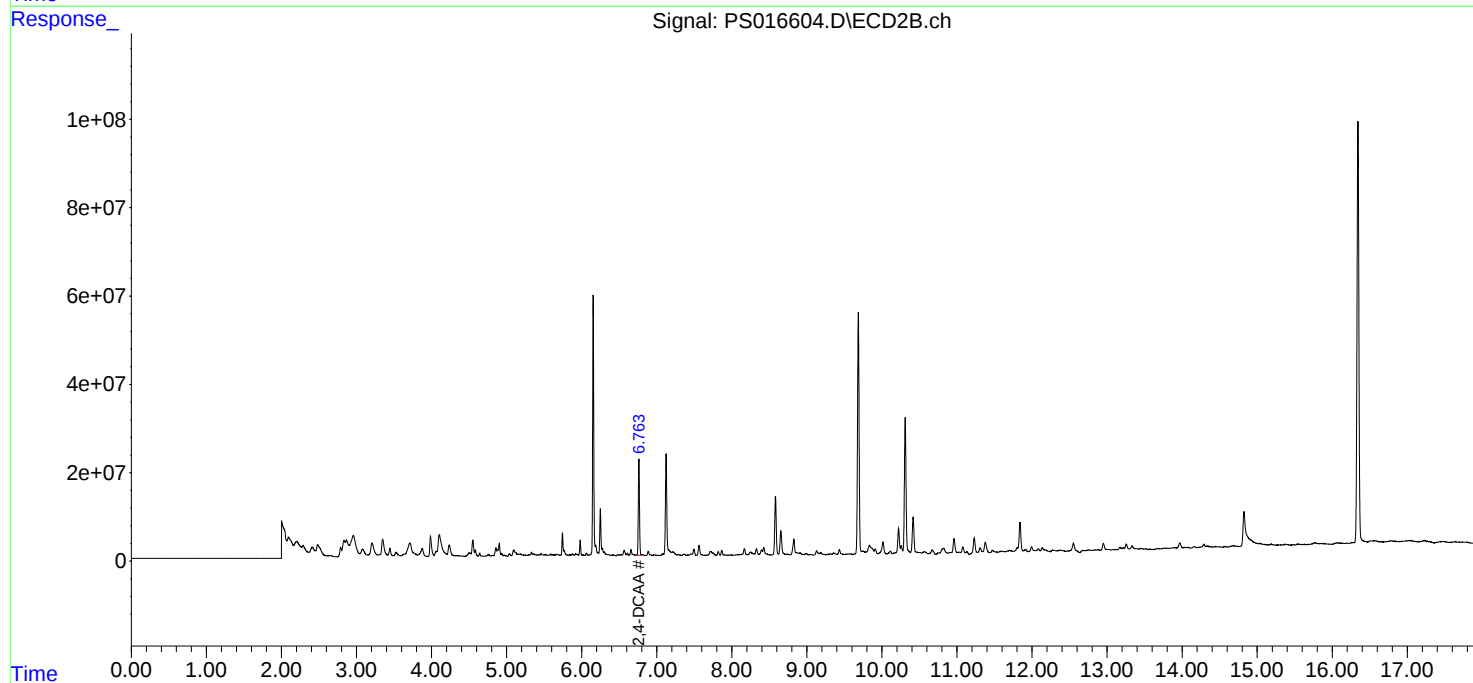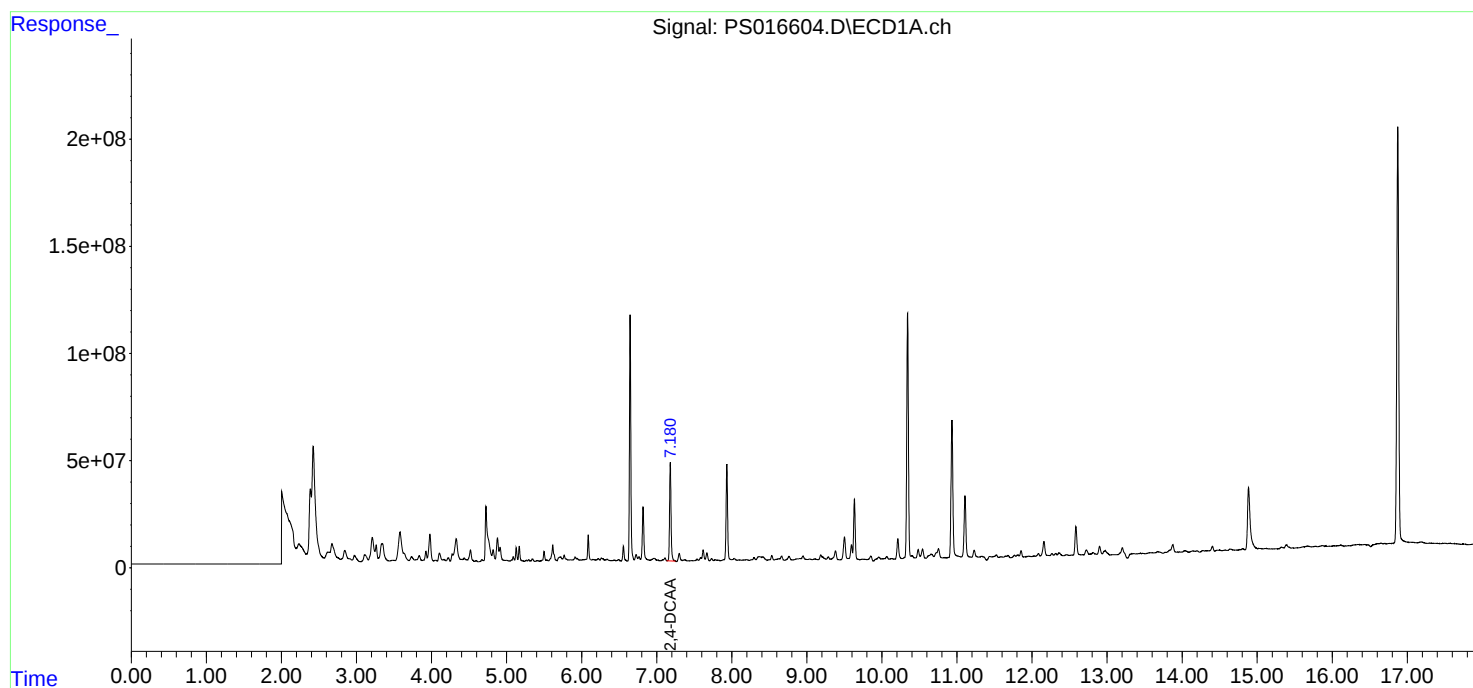

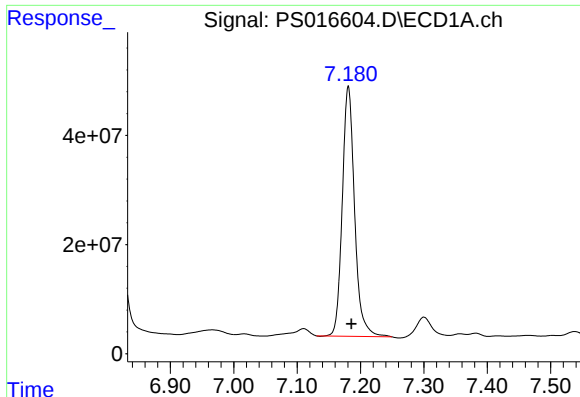


#4 2,4-DCAA

R.T.: 7.181 min
Delta R.T.: -0.005 min
Response: 619405522
Conc: 421.05 ng/ml

Instrument :
ECD_S
ClientSampleId :
SWCS-11-1015

Manual Integrations
APPROVED

mohammad
8/25/2021 4:56:52 PM

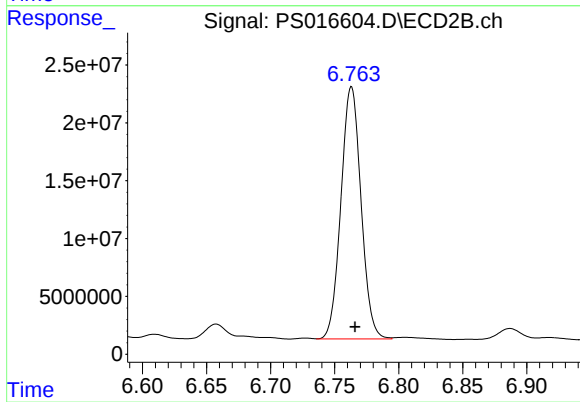

#4 2,4-DCAA

R.T.: 6.763 min
Delta R.T.: -0.003 min
Response: 237470707
Conc: 455.25 ng/ml m