

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS082422\  
 Data File : PS020346.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 24 Aug 2022 08:32  
 Operator : AJ\MA  
 Sample : HEXANE  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Aug 24 23:51:23 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS080322.M  
 Quant Title : 8080.M  
 QLast Update : Thu Aug 04 02:05:37 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1   | RT#2   | Resp#1   | Resp#2   | ng/ml | ng/ml  |
|-----------------------------|--------------|--------|--------|----------|----------|-------|--------|
| -----                       |              |        |        |          |          |       |        |
| System Monitoring Compounds |              |        |        |          |          |       |        |
| 4) S                        | 2,4-DCAA     | 7.174  | 0.000  | 856190   | 0        | <MDL  | N.D. # |
| Target Compounds            |              |        |        |          |          |       |        |
| 1) T                        | Dalapon      | 3.042  | 0.000  | 1684308  | 0        | <MDL  | N.D. # |
| 2) T                        | 3,5-DICHL... | 0.000  | 5.902f | 0        | 383080   | N.D.  | <MDL   |
| 5) T                        | DICAMBA      | 7.387  | 0.000  | 4077705  | 0        | <MDL  | N.D. # |
| 6) T                        | MCP          | 7.520  | 7.025  | 1057556  | 238166   | <MDL  | <MDL # |
| 7) T                        | MCPA         | 7.650  | 0.000  | 2806671  | 0        | <MDL  | N.D. # |
| 8) T                        | DICHLORPROP  | 8.047  | 0.000  | 666550   | 0        | <MDL  | N.D. # |
| 9) T                        | 2,4-D        | 8.306  | 0.000  | 389024   | 0        | <MDL  | N.D. # |
| 10) T                       | Pentachlo... | 8.601  | 0.000  | 1362694  | 0        | <MDL  | N.D. # |
| 12) T                       | 2,4,5-T      | 9.374f | 0.000  | 25346014 | 0        | 1.396 | N.D. # |
| 13) T                       | 2,4-DB       | 10.021 | 0.000  | 5663515  | 0        | 1.552 | N.D. # |
| 15) T                       | Picloram     | 10.999 | 10.823 | 257.9E6  | 46372591 | 8.157 | 6.146  |
| 16) T                       | DCPA         | 11.401 | 10.753 | 1640044  | 2640908  | <MDL  | <MDL # |
| -----                       |              |        |        |          |          |       |        |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS082422\  
Data File : PS020346.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 24 Aug 2022 08:32  
Operator : AJ\MA  
Sample : HEXANE  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Aug 24 23:51:23 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS080322.M  
Quant Title : 8080.M  
QLast Update : Thu Aug 04 02:05:37 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

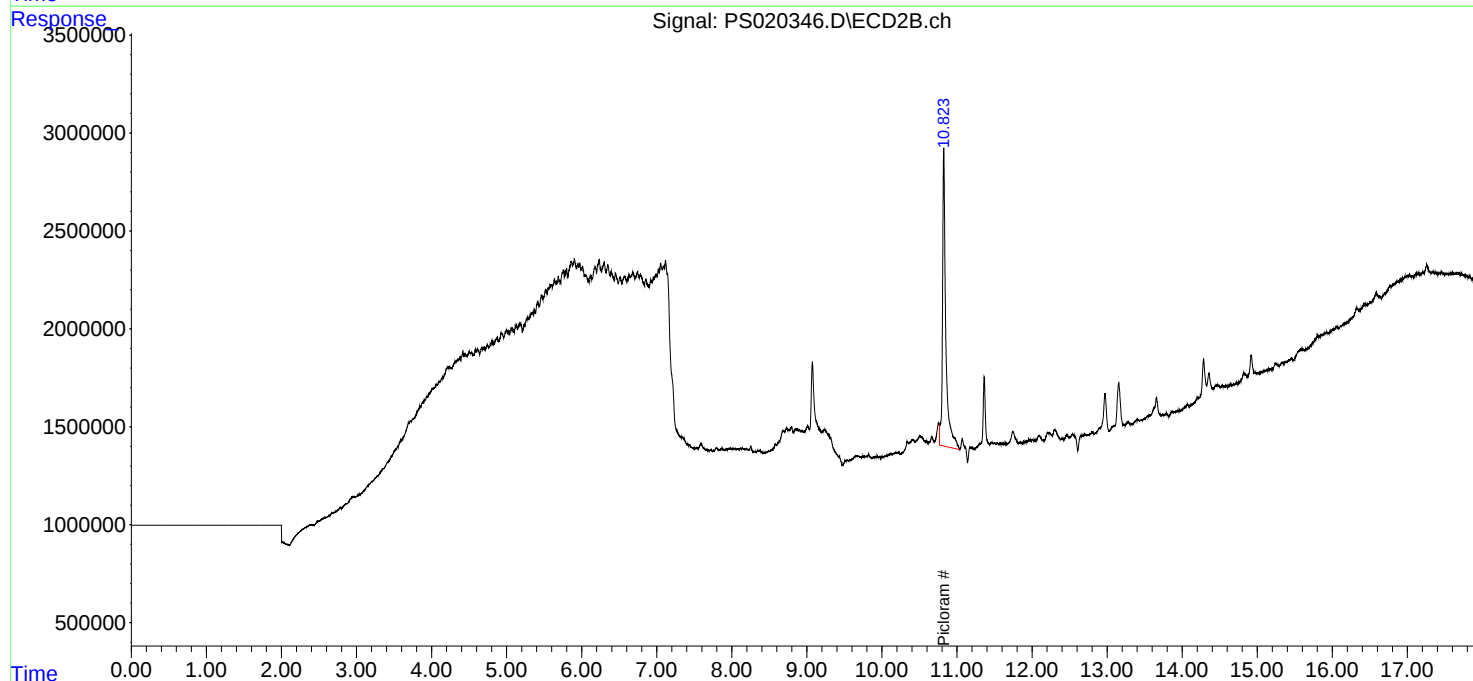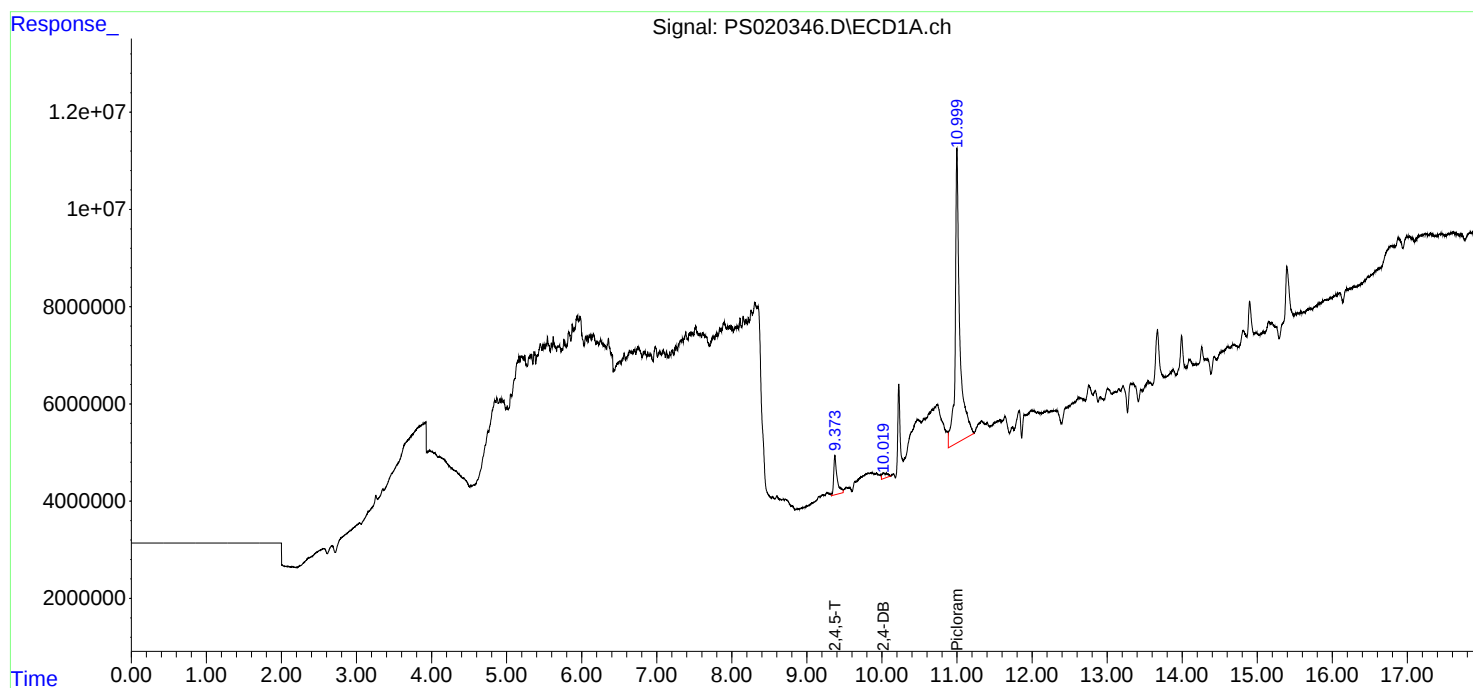


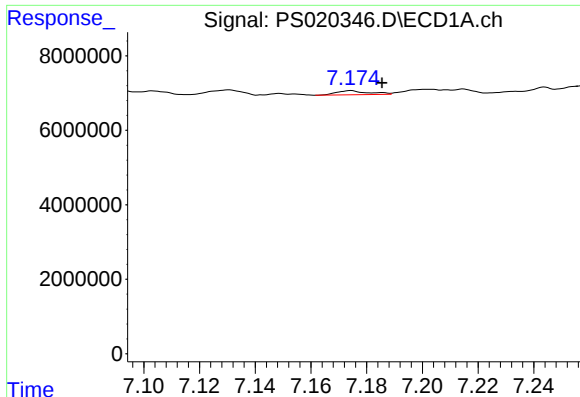

#4 2,4-DCAA


R.T.: 7.174 min  
Delta R.T.: -0.011 min  
Response: 856190  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

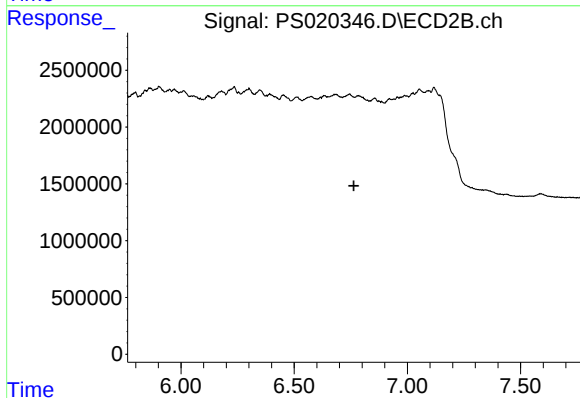


#4 2,4-DCAA

R.T.: 0.000 min  
Exp R.T. : 6.763 min  
Response: 0  
Conc: N.D.

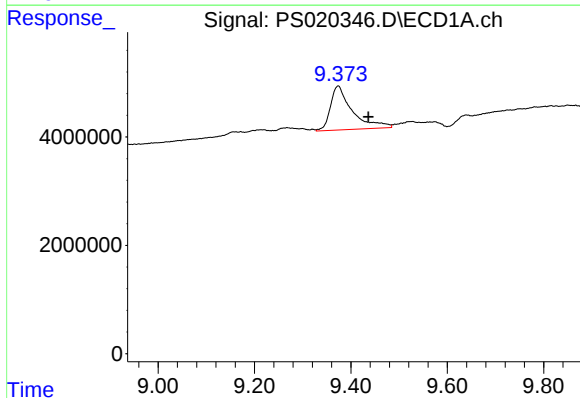


#12 2,4,5-T

R.T.: 9.374 min  
Delta R.T.: -0.062 min  
Response: 25346014  
Conc: 1.40 ng/ml

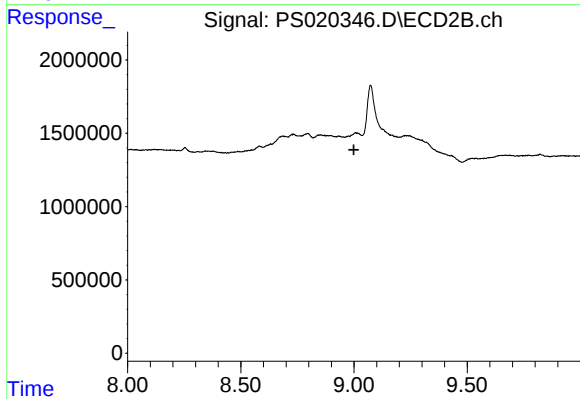

#12 2,4,5-T


R.T.: 0.000 min  
Exp R.T. : 8.999 min  
Response: 0  
Conc: N.D.

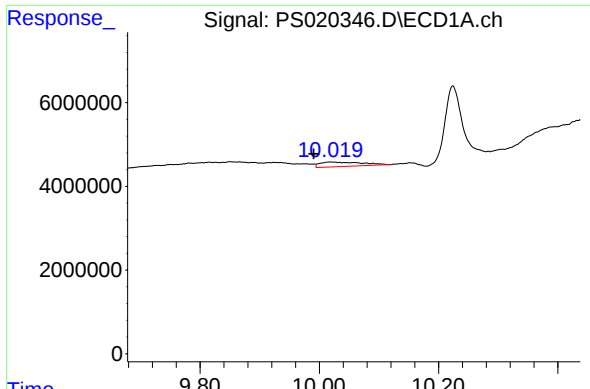

#13 2,4-DB


R.T.: 10.021 min  
Delta R.T.: 0.030 min  
Response: 5663515  
Conc: 1.55 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

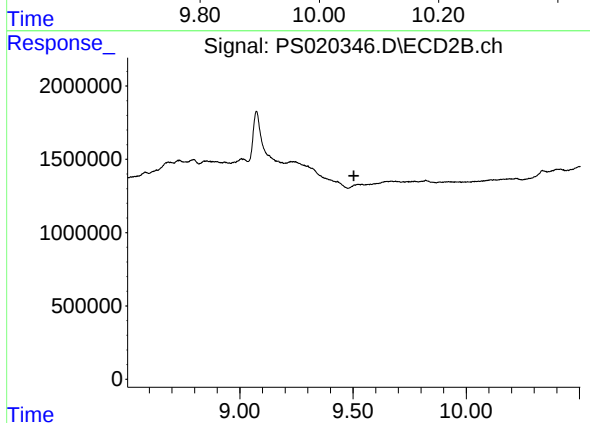


#13 2,4-DB

R.T.: 0.000 min  
Exp R.T. : 9.503 min  
Response: 0  
Conc: N.D.

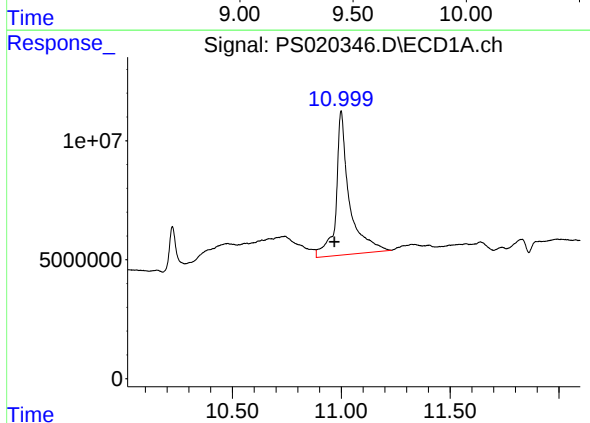

#15 Picloram

R.T.: 10.999 min  
Delta R.T.: 0.030 min  
Response: 257912244  
Conc: 8.16 ng/ml

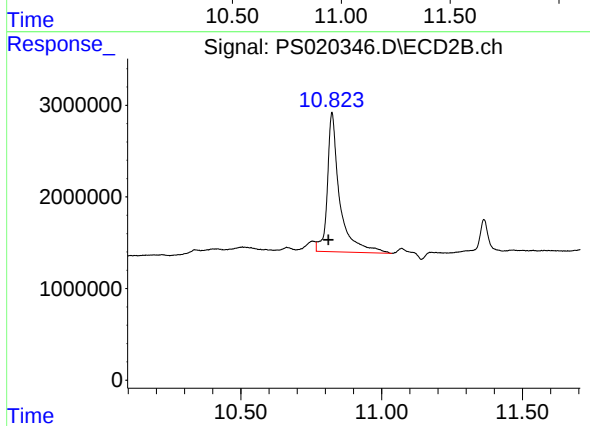

#15 Picloram

R.T.: 10.823 min  
Delta R.T.: 0.013 min  
Response: 46372591  
Conc: 6.15 ng/ml