

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082520\
 Data File : PS011917.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Aug 2020 19:22
 Operator : DD\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 26 01:52:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.218	6.914	822.3E6	439.1E6	753.895	821.042
Target Compounds							
1) T	Dalapon	3.035	2.624	893.0E6	514.6E6	716.859	680.822
2) T	3,5-DICHL...	6.432	6.066	1052.3E6	618.1E6	725.873	751.347
3) T	4-Nitroph...	7.049	6.523	360.6E6	247.7E6	612.105	679.467
5) T	DICAMBA	7.408	7.082	3096.5E6	1703.4E6	755.978	788.424
6) T	MCPD	7.578	7.180	244.8E6	141.1E6	76.613	79.824
7) T	MCPA	7.728	7.396	335.6E6	211.4E6	73.782	77.133
8) T	DICHLORPROP	8.100	7.708	746.1E6	443.2E6	742.582	784.994
9) T	2,4-D	8.330	8.002	809.5E6	573.8E6	716.949	781.055
10) T	Pentachlo...	8.640	8.432	10727.5E6	5233.6E6	745.922	770.243
11) T	2,4,5-TP ...	9.189	8.792	4312.7E6	2294.3E6	741.677	784.740
12) T	2,4,5-T	9.474	9.172	4383.0E6	2277.7E6	739.650	769.484
13) T	2,4-DB	10.027	9.679	543.7E6	322.9E6	684.239	772.180
14) T	DINOSEB	11.186	10.010	3340.2E6	1677.9E6	711.631	789.270
15) T	Picloram	11.012	10.997	4644.0E6	3018.6E6	594.191	665.999
16) T	DCPA	11.452	10.939	5338.5E6	2894.7E6	702.122	787.265



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082520\
Data File : PS011917.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Aug 2020 19:22
Operator : DD\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 26 01:52:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

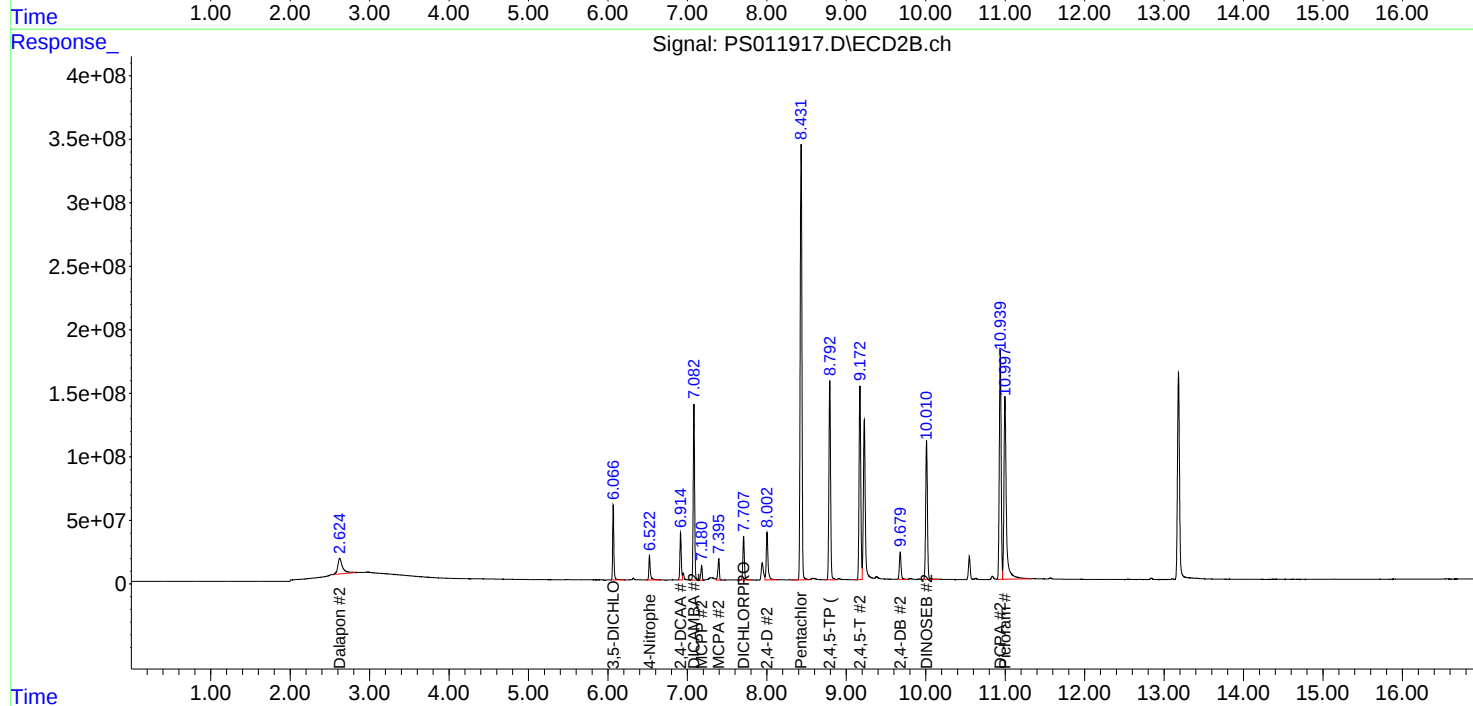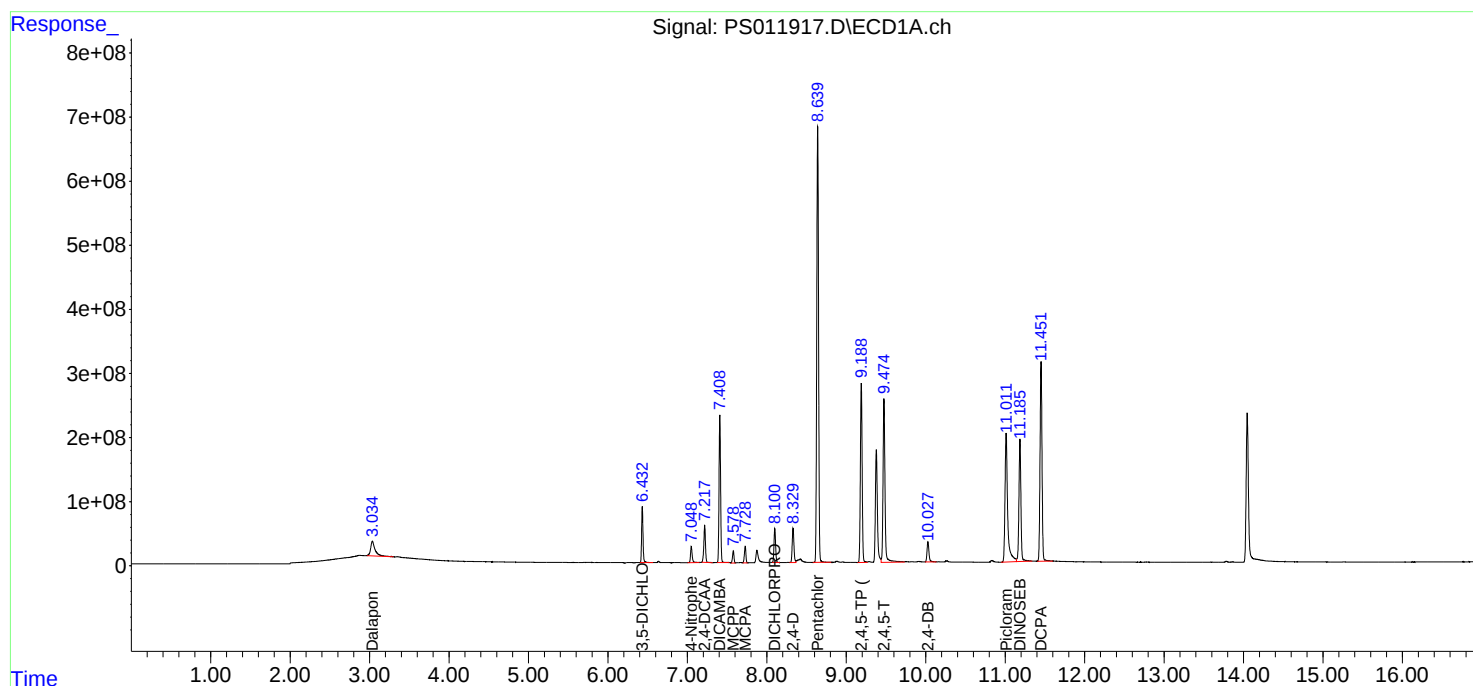


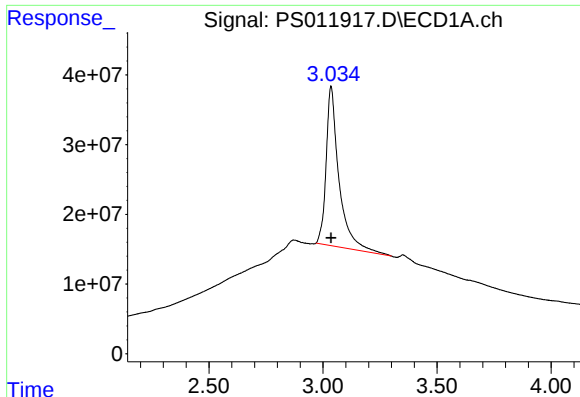

#1 Dalapon


R.T.: 3.035 min
Delta R.T.: 0.000 min
Response: 892960775
Conc: 716.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

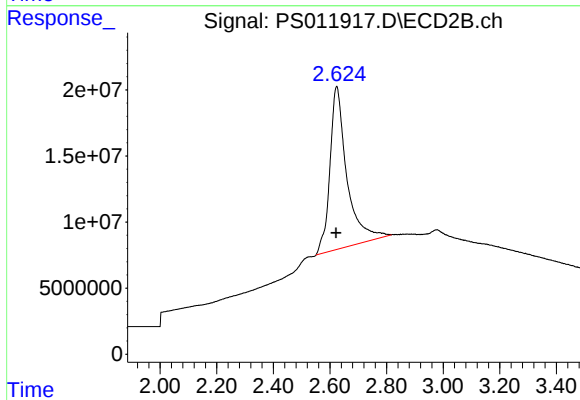


#1 Dalapon

R.T.: 2.624 min
Delta R.T.: 0.003 min
Response: 514597728
Conc: 680.82 ng/ml

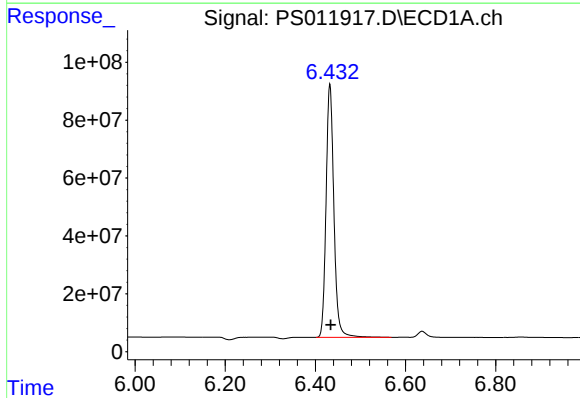


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.432 min
Delta R.T.: -0.002 min
Response: 1052326624
Conc: 725.87 ng/ml

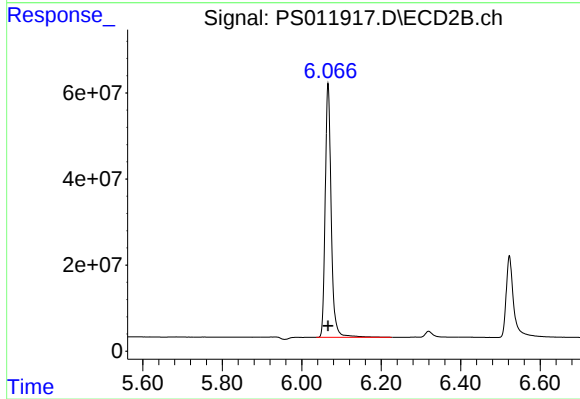

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.066 min
Delta R.T.: 0.000 min
Response: 618073121
Conc: 751.35 ng/ml

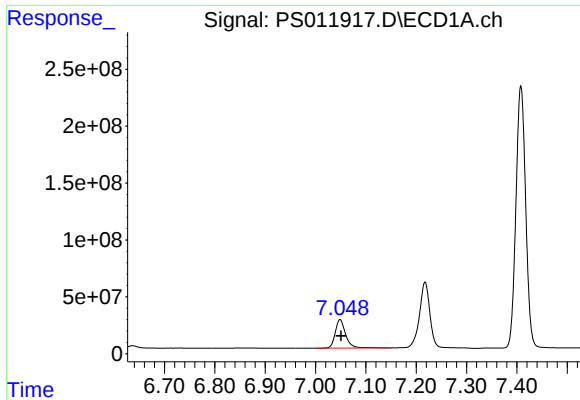

#3 4-Nitrophenol


R.T.: 7.049 min
Delta R.T.: -0.002 min
Response: 360555811
Conc: 612.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

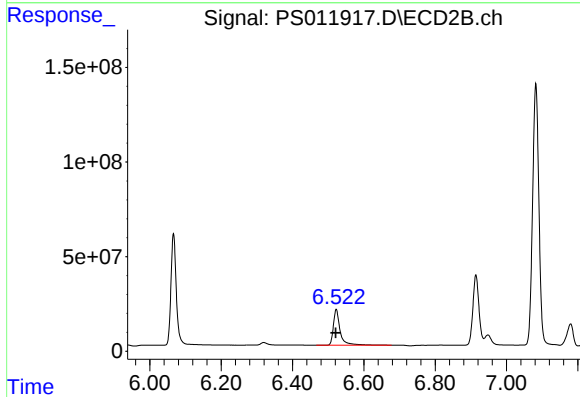


#3 4-Nitrophenol

R.T.: 6.523 min
Delta R.T.: 0.001 min
Response: 247740076
Conc: 679.47 ng/ml

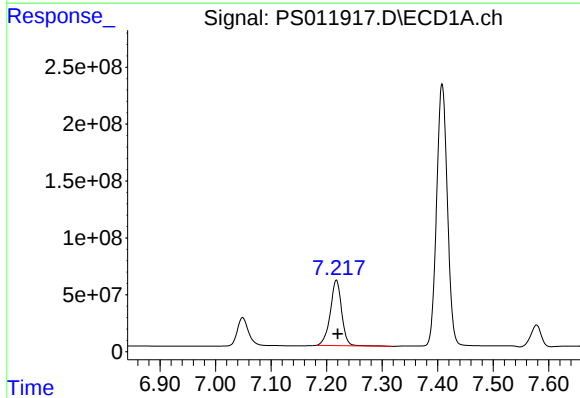


#4 2,4-DCAA

R.T.: 7.218 min
Delta R.T.: -0.002 min
Response: 822324997
Conc: 753.90 ng/ml

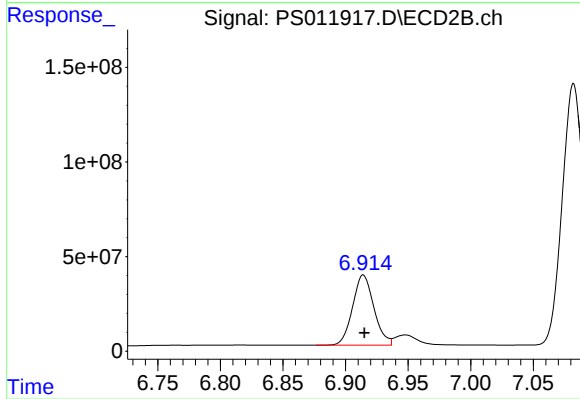

#4 2,4-DCAA


R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 439082532
Conc: 821.04 ng/ml

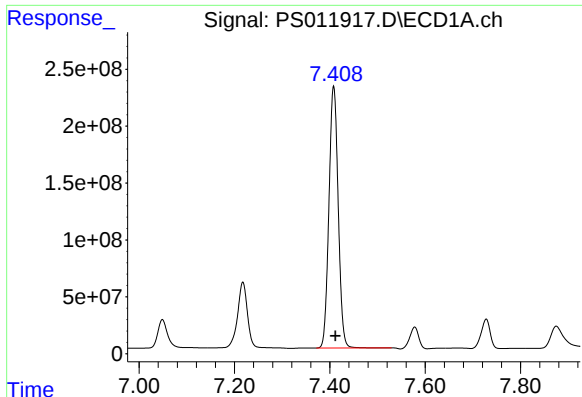

#5 DICAMBA


R.T.: 7.408 min
Delta R.T.: -0.004 min
Response: 3096469844
Conc: 755.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

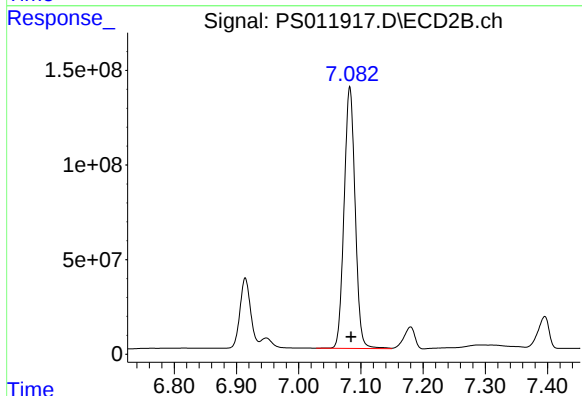


#5 DICAMBA

R.T.: 7.082 min
Delta R.T.: -0.002 min
Response: 1703393969
Conc: 788.42 ng/ml

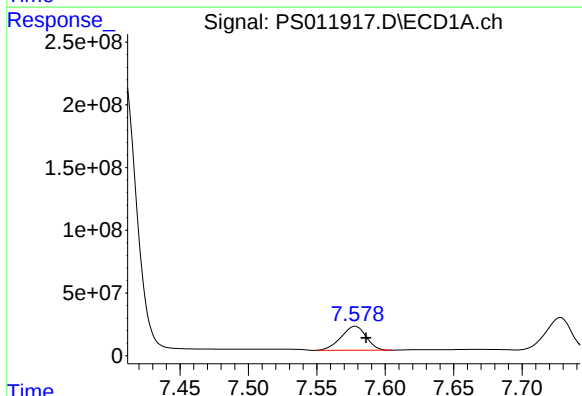


#6 MCP

R.T.: 7.578 min
Delta R.T.: -0.008 min
Response: 244783709
Conc: 76.61 ug/ml

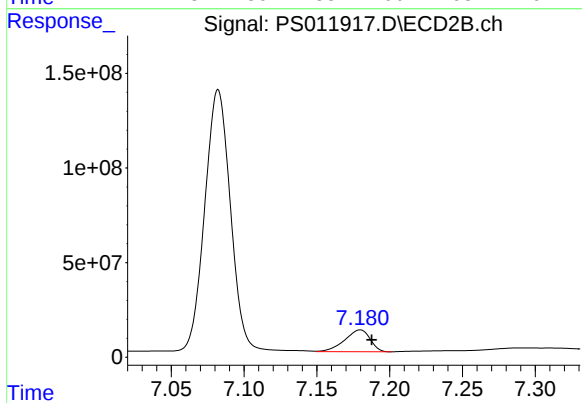

#6 MCP


R.T.: 7.180 min
Delta R.T.: -0.008 min
Response: 141083779
Conc: 79.82 ug/ml

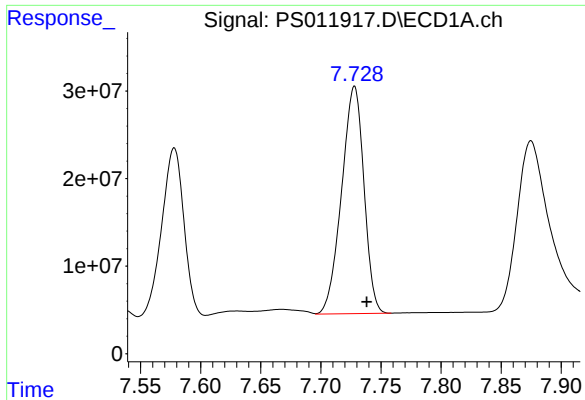

#7 MCPA


R.T.: 7.728 min
Delta R.T.: -0.010 min
Response: 335596903
Conc: 73.78 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

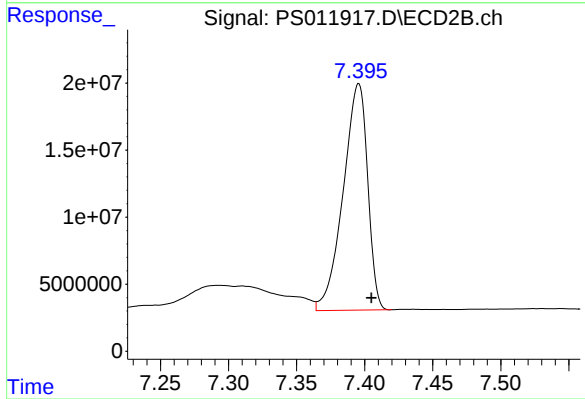


#7 MCPA

R.T.: 7.396 min
Delta R.T.: -0.009 min
Response: 211356164
Conc: 77.13 ug/ml

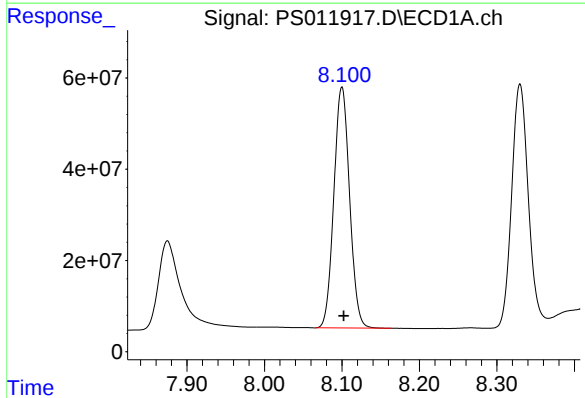


#8 DICHLORPROP

R.T.: 8.100 min
Delta R.T.: -0.002 min
Response: 746055636
Conc: 742.58 ng/ml

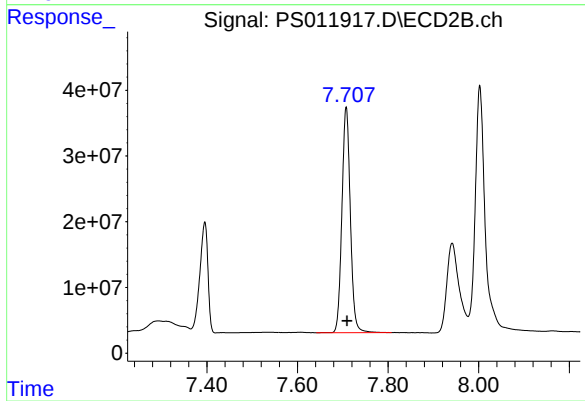

#8 DICHLORPROP


R.T.: 7.708 min
Delta R.T.: -0.002 min
Response: 443236147
Conc: 784.99 ng/ml

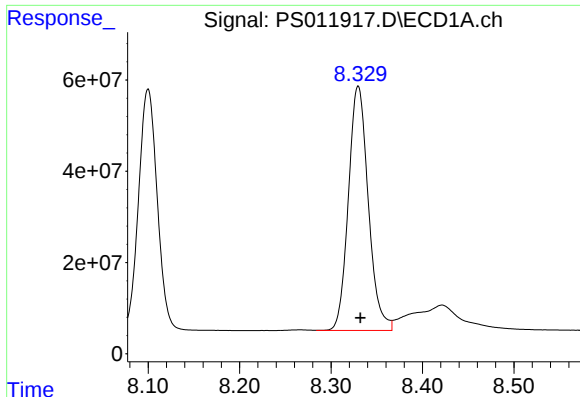

#9 2,4-D


R.T.: 8.330 min
Delta R.T.: -0.002 min
Response: 809501452
Conc: 716.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

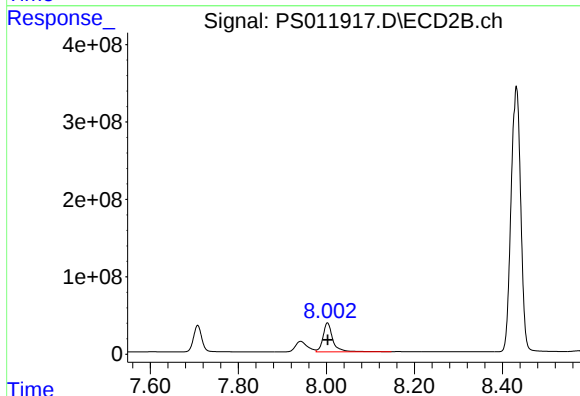


#9 2,4-D

R.T.: 8.002 min
Delta R.T.: 0.000 min
Response: 573812772
Conc: 781.06 ng/ml

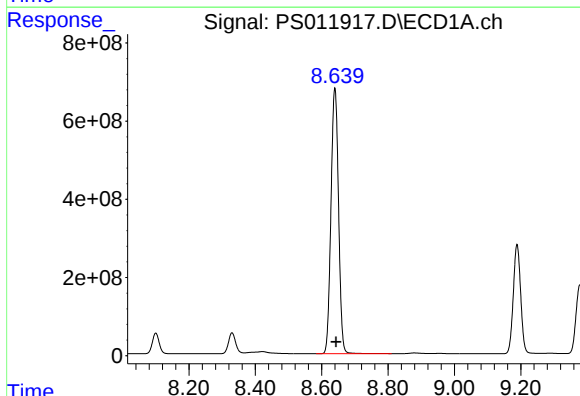


#10 Pentachlorophenol

R.T.: 8.640 min
Delta R.T.: -0.003 min
Response: 10727499855
Conc: 745.92 ng/ml

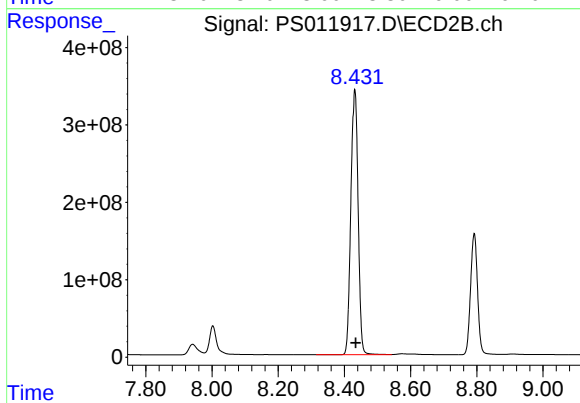

#10 Pentachlorophenol


R.T.: 8.432 min
Delta R.T.: -0.002 min
Response: 5233629025
Conc: 770.24 ng/ml

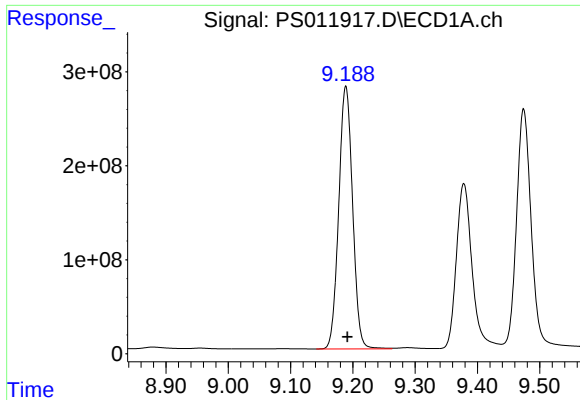

#11 2,4,5-TP (SILVEX)


R.T.: 9.189 min
Delta R.T.: -0.003 min
Response: 4312700943
Conc: 741.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

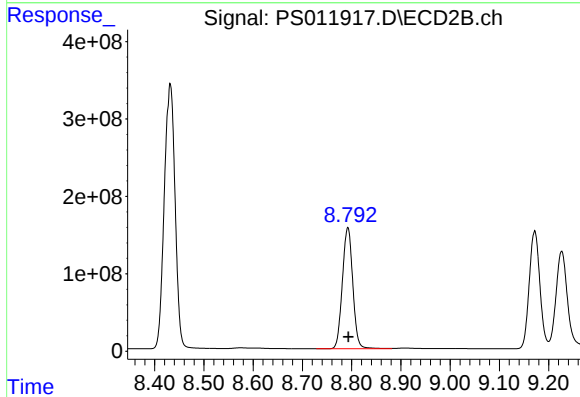


#11 2,4,5-TP (SILVEX)

R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 2294303765
Conc: 784.74 ng/ml

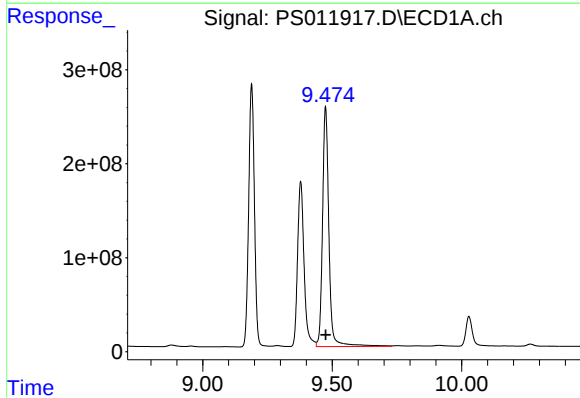


#12 2,4,5-T

R.T.: 9.474 min
Delta R.T.: -0.002 min
Response: 4383036181
Conc: 739.65 ng/ml

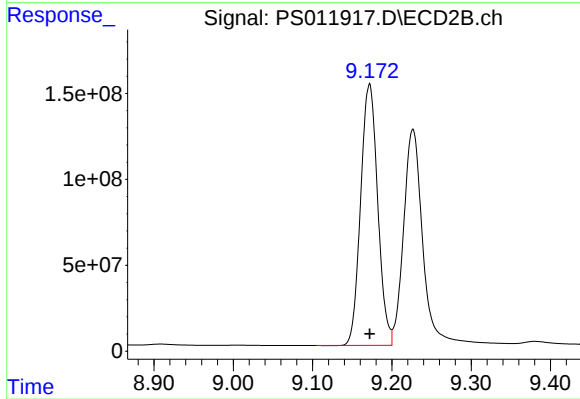

#12 2,4,5-T


R.T.: 9.172 min
Delta R.T.: 0.000 min
Response: 2277735159
Conc: 769.48 ng/ml

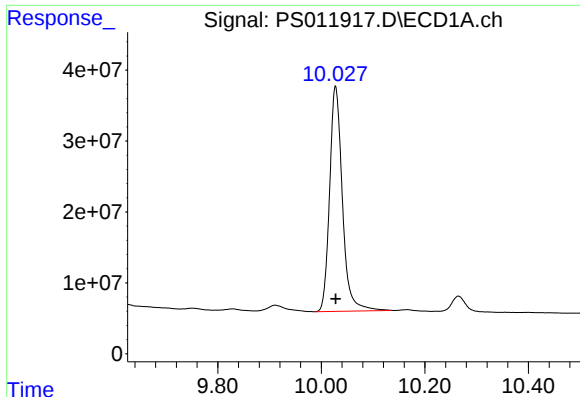

#13 2,4-DB


R.T.: 10.027 min
Delta R.T.: 0.000 min
Response: 543680725
Conc: 684.24 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

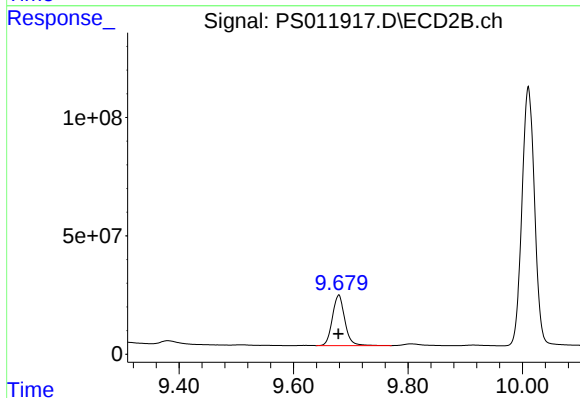


#13 2,4-DB

R.T.: 9.679 min
Delta R.T.: 0.000 min
Response: 322942431
Conc: 772.18 ng/ml

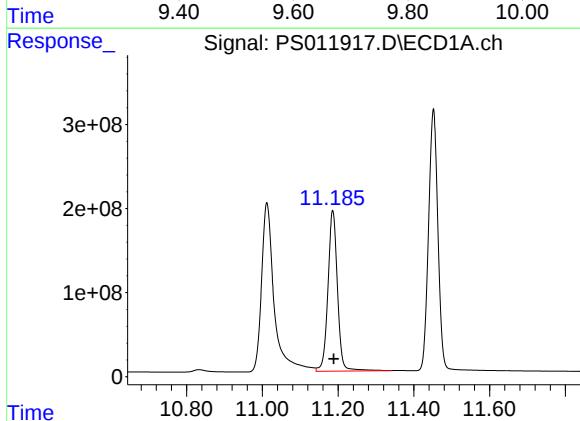


#14 DINOSEB

R.T.: 11.186 min
Delta R.T.: -0.003 min
Response: 3340165769
Conc: 711.63 ng/ml

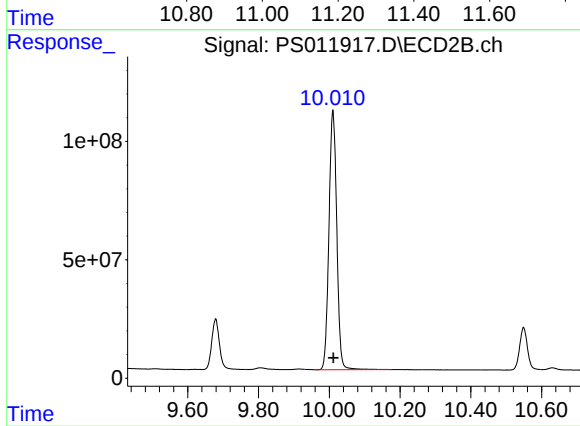

#14 DINOSEB


R.T.: 10.010 min
Delta R.T.: -0.002 min
Response: 1677928286
Conc: 789.27 ng/ml

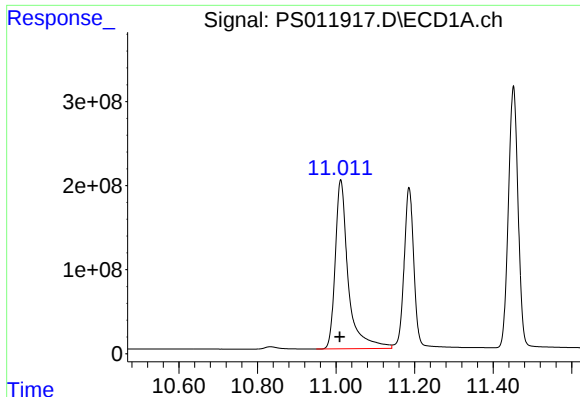

#15 Picloram


R.T.: 11.012 min
Delta R.T.: 0.002 min
Response: 4643970660
Conc: 594.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

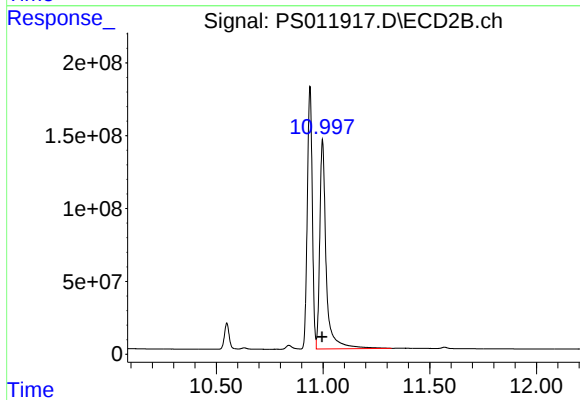


#15 Picloram

R.T.: 10.997 min
Delta R.T.: 0.002 min
Response: 3018608110
Conc: 666.00 ng/ml

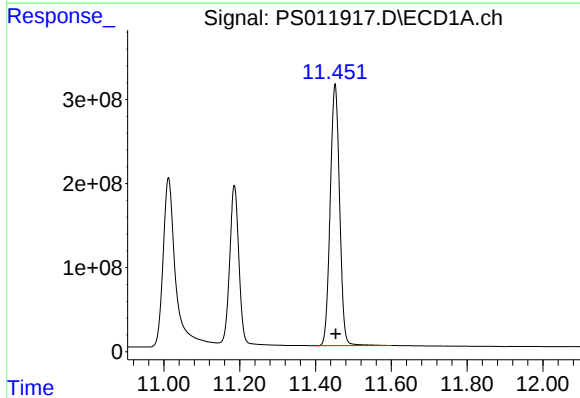

#16 DCPA

R.T.: 11.452 min
Delta R.T.: -0.002 min
Response: 5338545960
Conc: 702.12 ng/ml

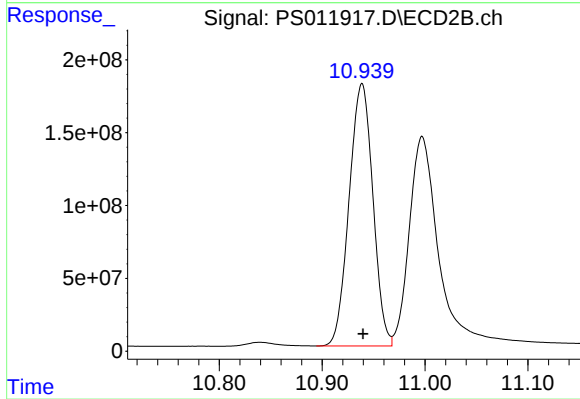

#16 DCPA

R.T.: 10.939 min
Delta R.T.: -0.001 min
Response: 2894712682
Conc: 787.27 ng/ml