

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082521\
 Data File : PS016701.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Aug 2021 04:52
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 26 05:40:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 02 14:10:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.182	6.763	627.6E6	262.9E6	426.593	504.092
Target Compounds							
8) T	DICHLORPROP	0.000	7.574	0	2744254	N.D.	5.065
9) T	2,4-D	8.365f	0.000	89563762	0	59.228	N.D. #
10) T	Pentachlo...	8.602	8.263	11457805	5577891	<MDL	<MDL #
12) T	2,4,5-T	0.000	9.064f	0	3176833	N.D.	1.097
15) T	Picloram	10.986	10.823	33403299	15699685	3.347	3.899
16) T	DCPA	0.000	10.763	0	1914204	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082521\
Data File : PS016701.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2021 04:52
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 26 05:40:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
Quant Title : 8080.M
QLast Update : Mon Aug 02 14:10:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

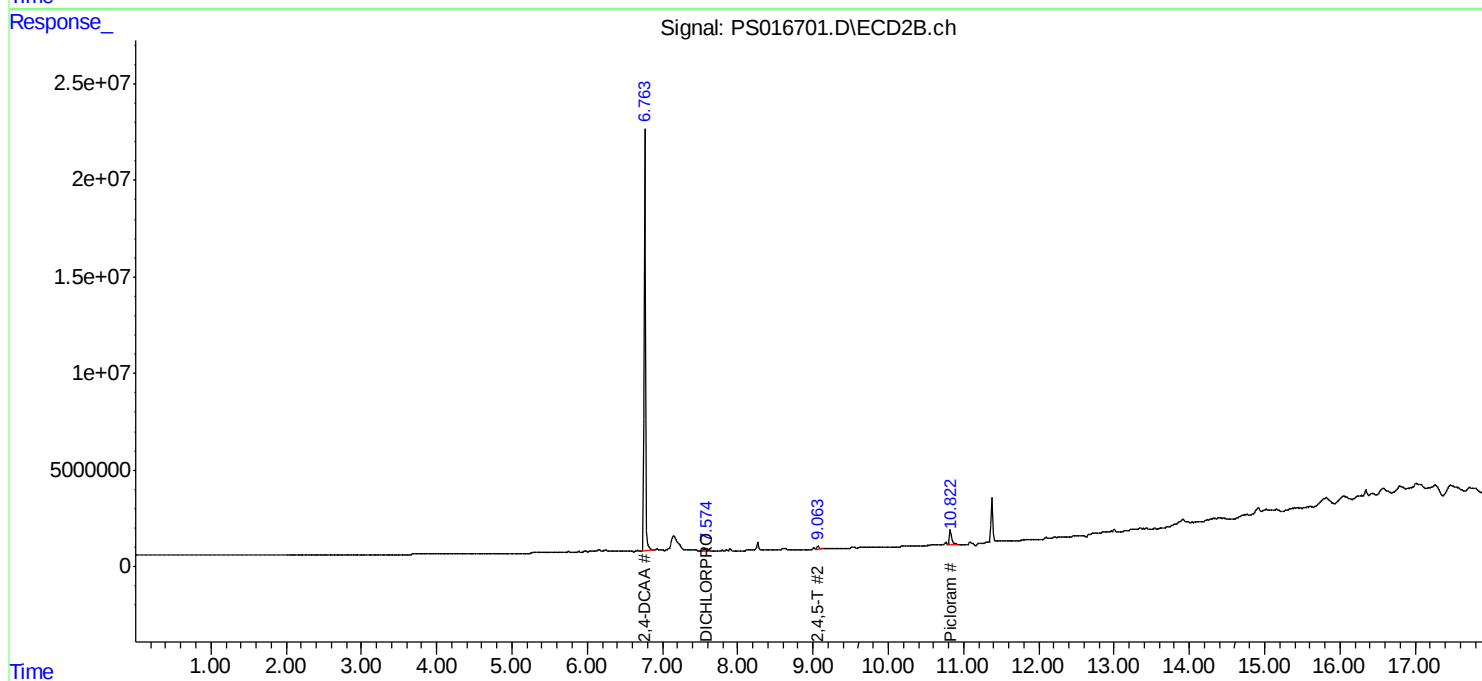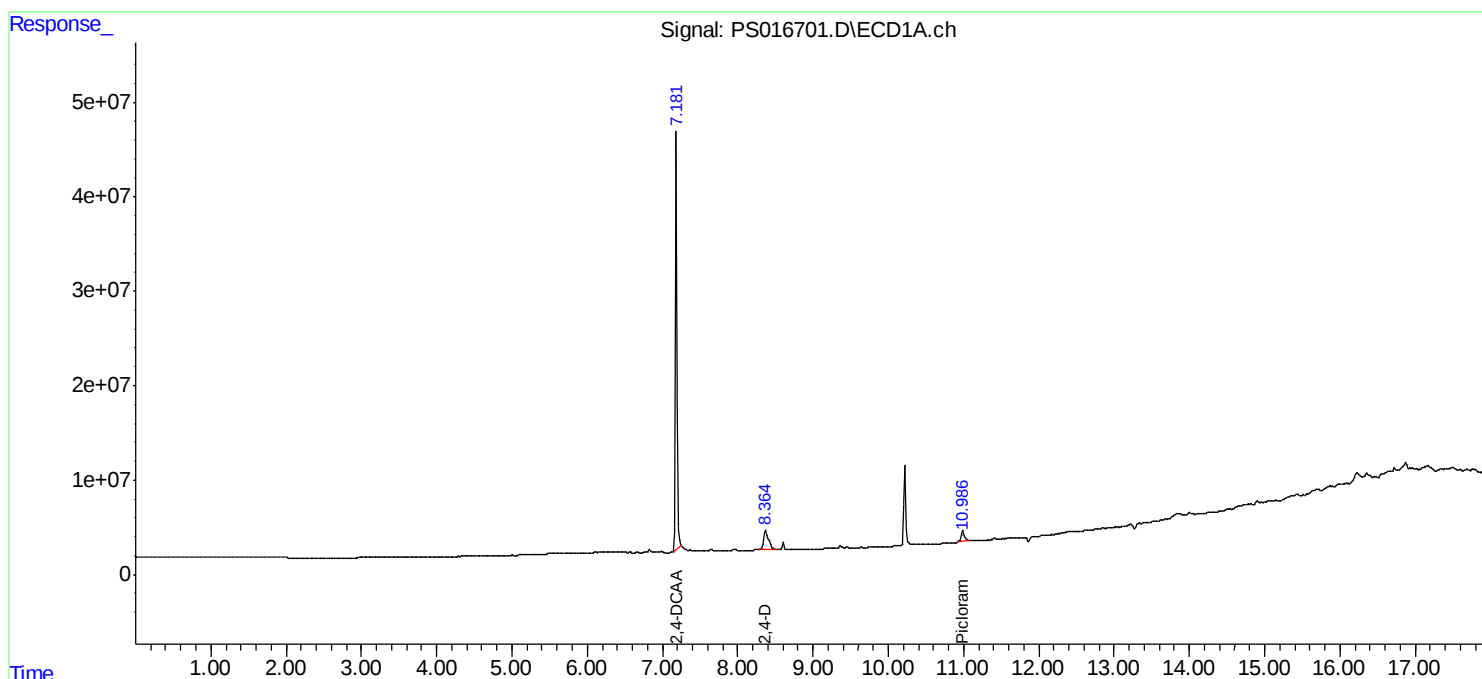


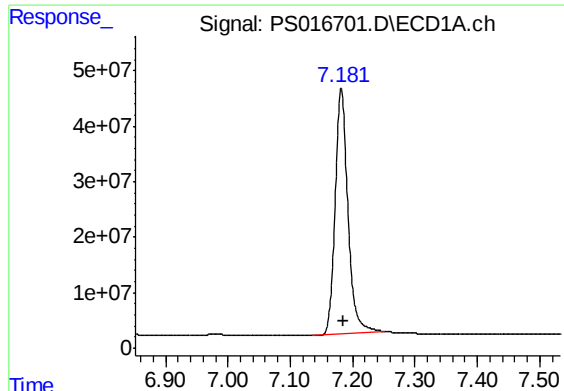

#4 2,4-DCAA


R.T.: 7.182 min
Delta R.T.: -0.004 min
Response: 627563192
Conc: 426.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

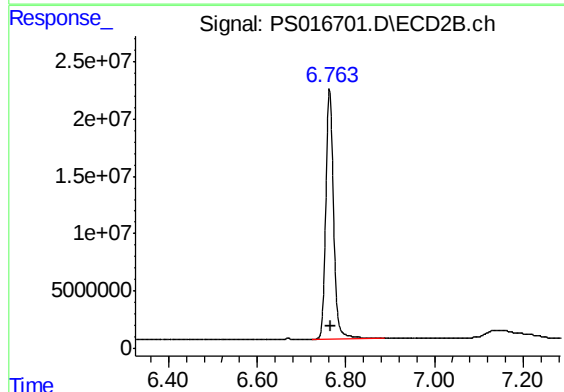


#4 2,4-DCAA

R.T.: 6.763 min
Delta R.T.: -0.003 min
Response: 262946528
Conc: 504.09 ng/ml

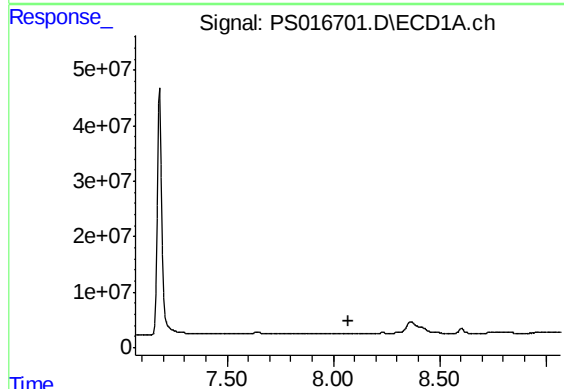


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.069 min
Response: 0
Conc: N.D.

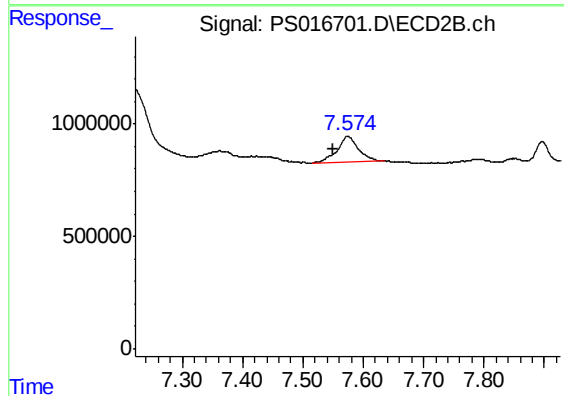

#8 DICHLORPROP


R.T.: 7.574 min
Delta R.T.: 0.025 min
Response: 2744254
Conc: 5.07 ng/ml

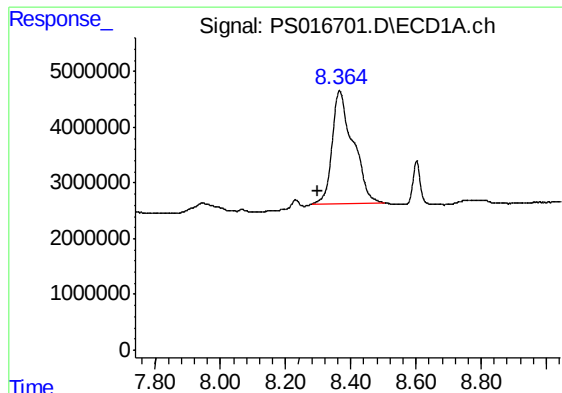

#9 2,4-D


R.T.: 8.365 min
Delta R.T.: 0.068 min
Response: 89563762
Conc: 59.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

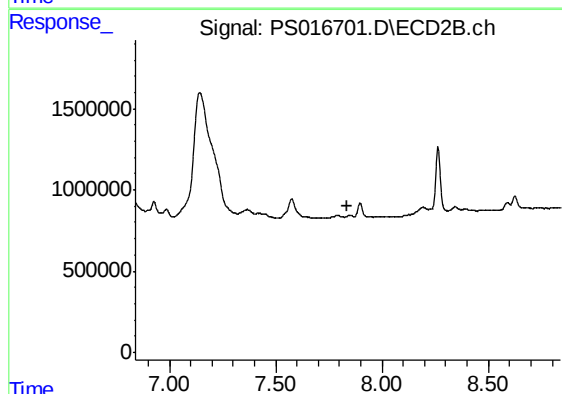


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.839 min
Response: 0
Conc: N.D.

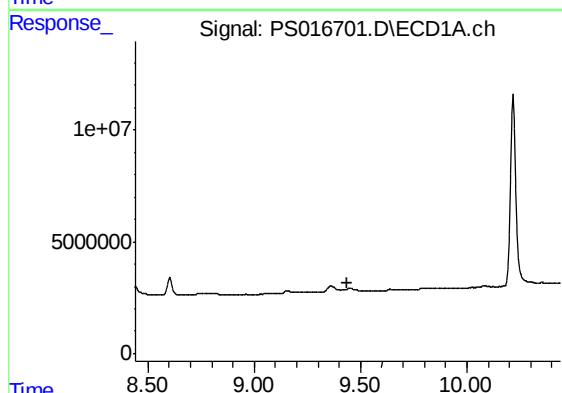


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.440 min
Response: 0
Conc: N.D.

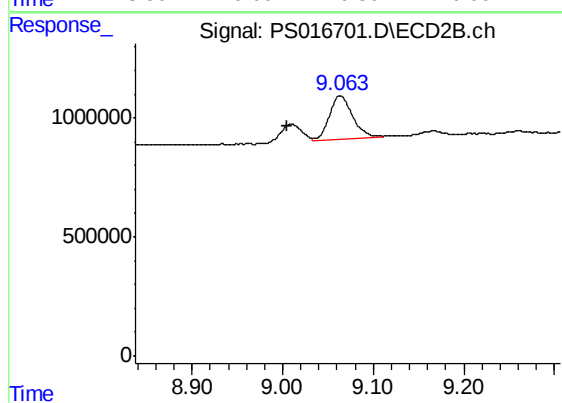

#12 2,4,5-T


R.T.: 9.064 min
Delta R.T.: 0.058 min
Response: 3176833
Conc: 1.10 ng/ml

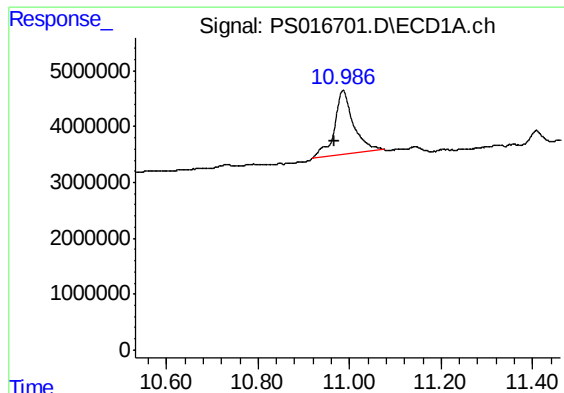

#15 Picloram

R.T.: 10.986 min
Delta R.T.: 0.019 min
Response: 33403299
Conc: 3.35 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

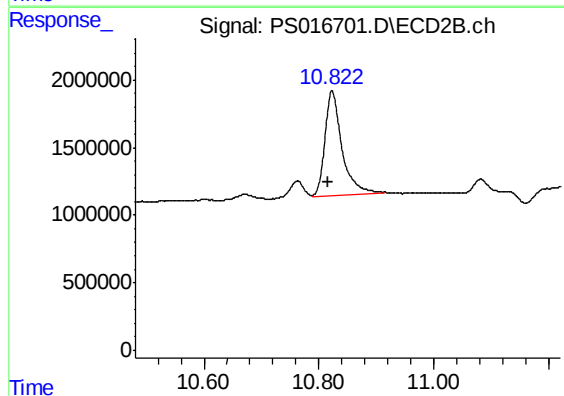

#15 Picloram

R.T.: 10.823 min
Delta R.T.: 0.007 min
Response: 15699685
Conc: 3.90 ng/ml