

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082521\
 Data File : PS016710.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Aug 2021 09:22
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 26 13:05:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 02 14:10:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.181	6.763	636.7E6	264.4E6	432.822	506.889
Target Compounds							
7) T	MCPA	7.638f	0.000	10975179	0	1.782	N.D. #
8) T	DICHLORPROP	0.000	7.574	0	5821708	N.D.	10.746
9) T	2,4-D	8.366f	0.000	91061871	0	60.219	N.D. #
12) T	2,4,5-T	0.000	9.062f	0	1892209	N.D.	<MDL
15) T	Picloram	10.983	10.823	10877727	6535555	1.090	1.623 #
16) T	DCPA	0.000	10.823f	0	6535555	N.D.	1.454



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082521\
Data File : PS016710.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2021 09:22
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 26 13:05:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
Quant Title : 8080.M
QLast Update : Mon Aug 02 14:10:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

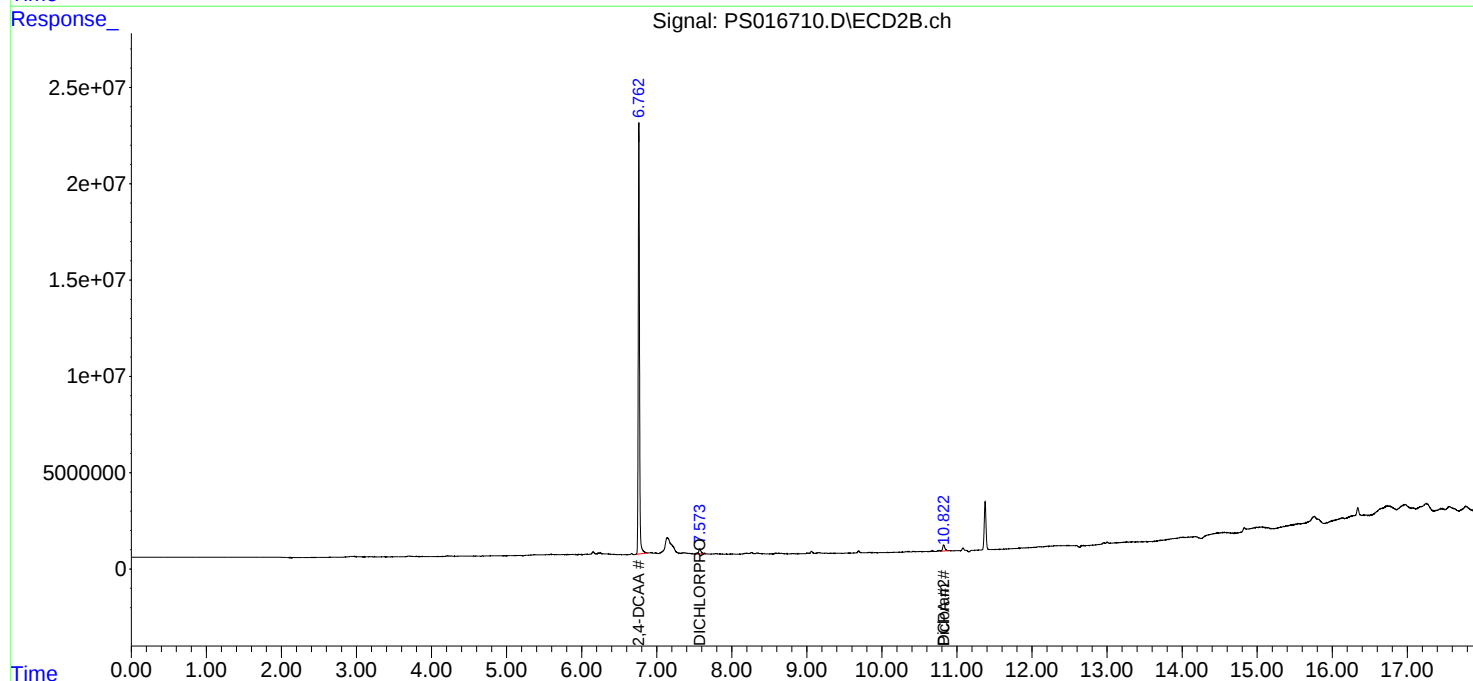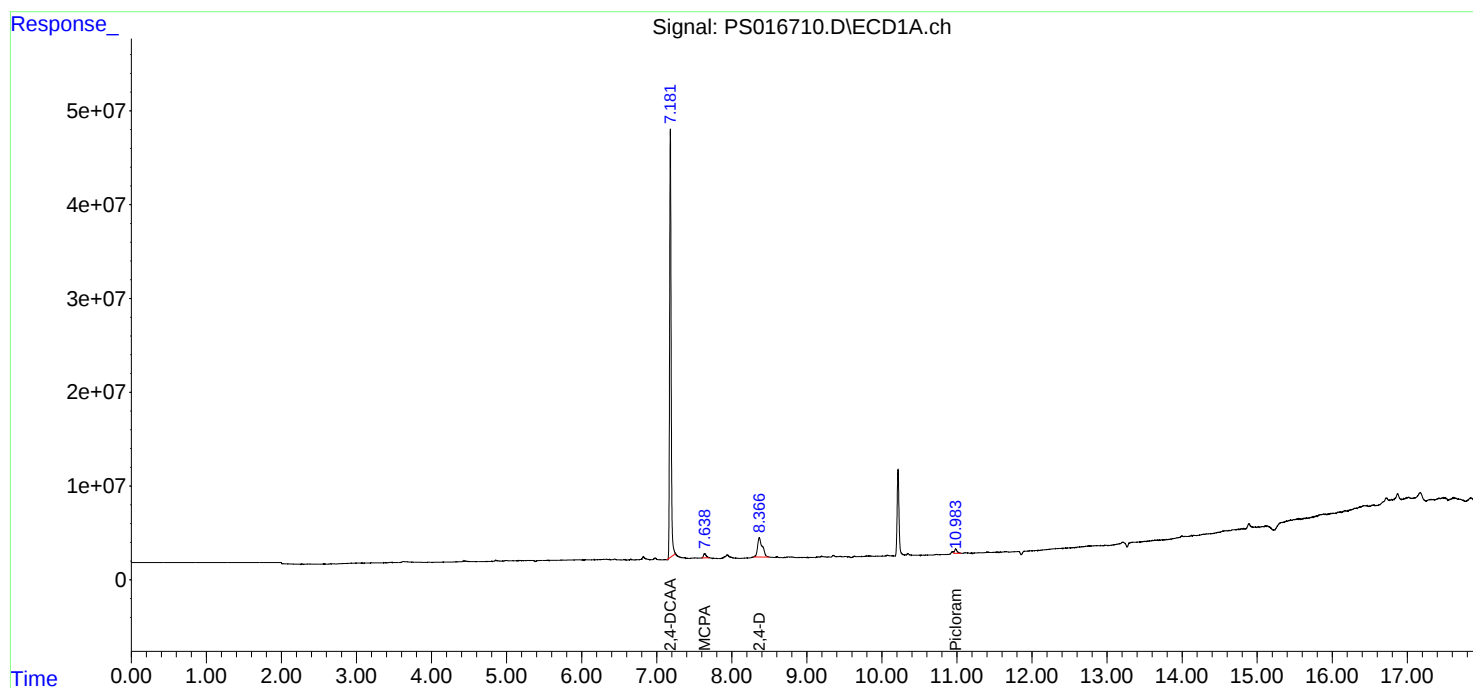


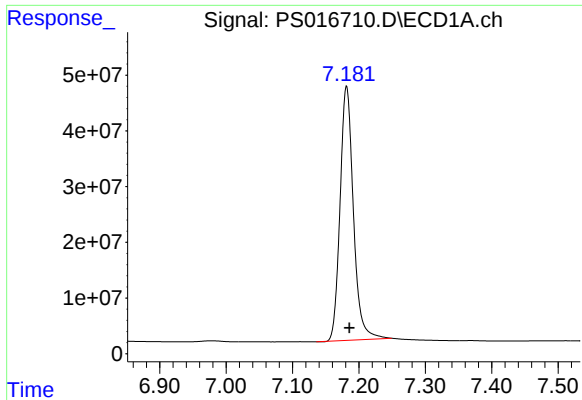

#4 2,4-DCAA


R.T.: 7.181 min
Delta R.T.: -0.004 min
Response: 636726794
Conc: 432.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

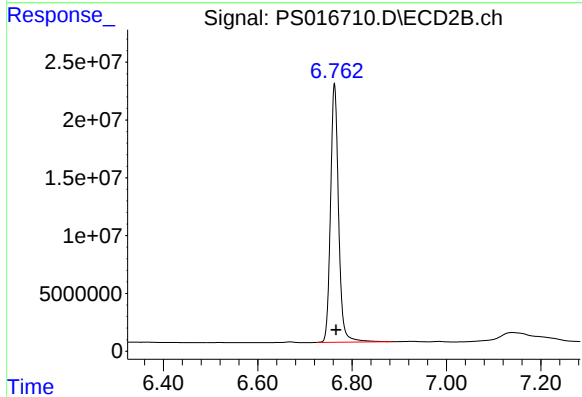


#4 2,4-DCAA

R.T.: 6.763 min
Delta R.T.: -0.003 min
Response: 264405657
Conc: 506.89 ng/ml

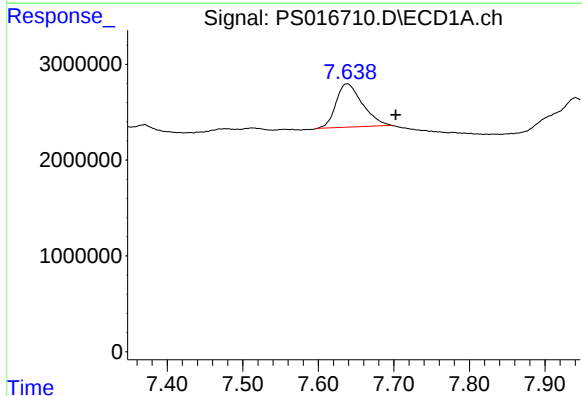


#7 MCPA

R.T.: 7.638 min
Delta R.T.: -0.064 min
Response: 10975179
Conc: 1.78 ug/ml

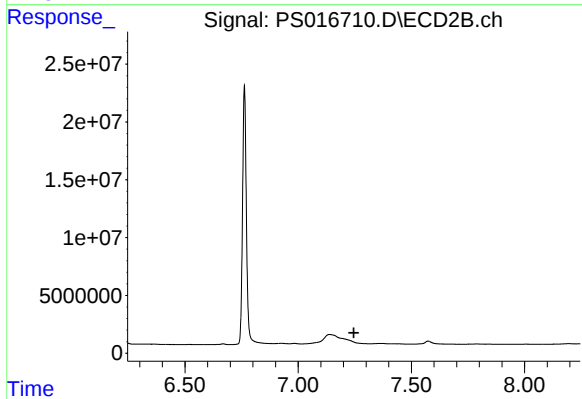

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.246 min
Response: 0
Conc: N.D.

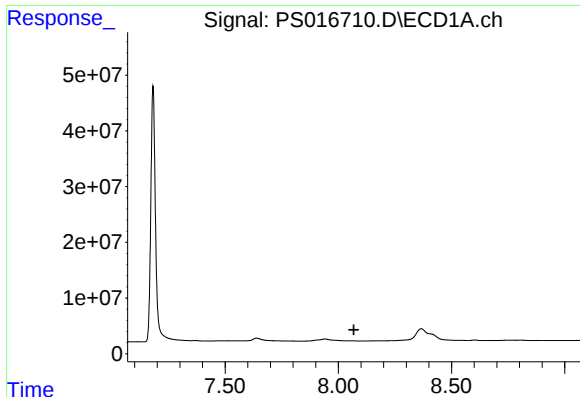

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.069 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

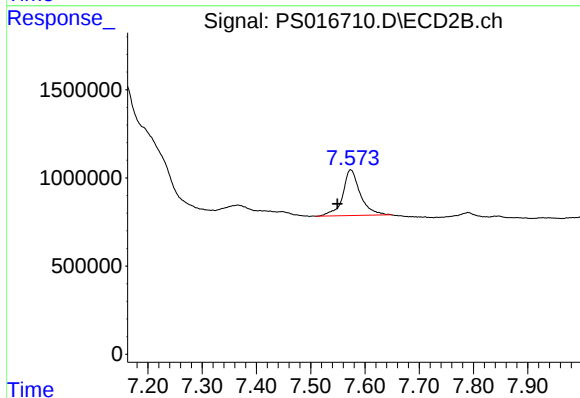


#8 DICHLORPROP

R.T.: 7.574 min
Delta R.T.: 0.024 min
Response: 5821708
Conc: 10.75 ng/ml

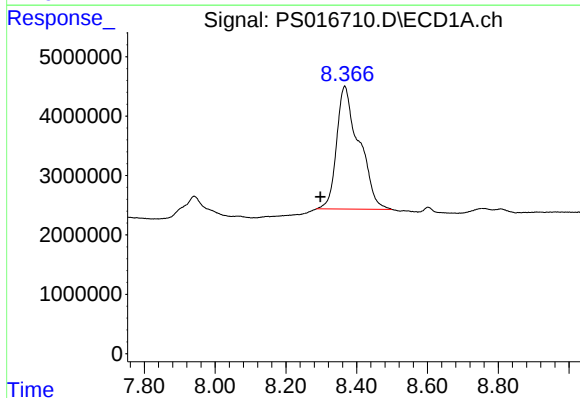


#9 2,4-D

R.T.: 8.366 min
Delta R.T.: 0.069 min
Response: 91061871
Conc: 60.22 ng/ml

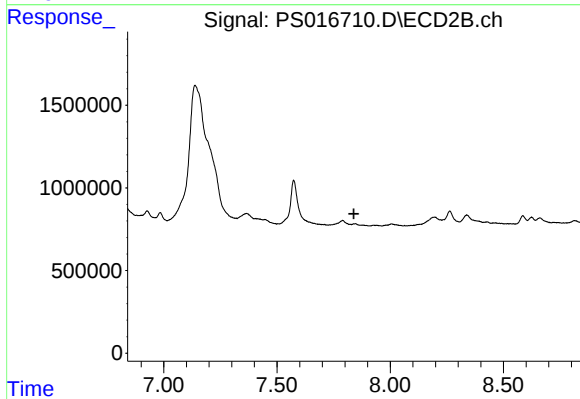

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.839 min
Response: 0
Conc: N.D.

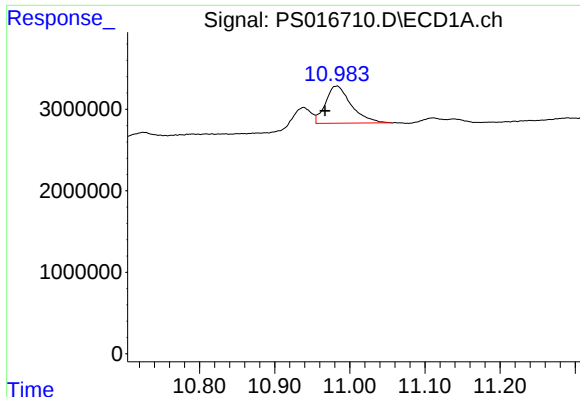

#15 Picloram


R.T.: 10.983 min
Delta R.T.: 0.016 min
Response: 10877727
Conc: 1.09 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

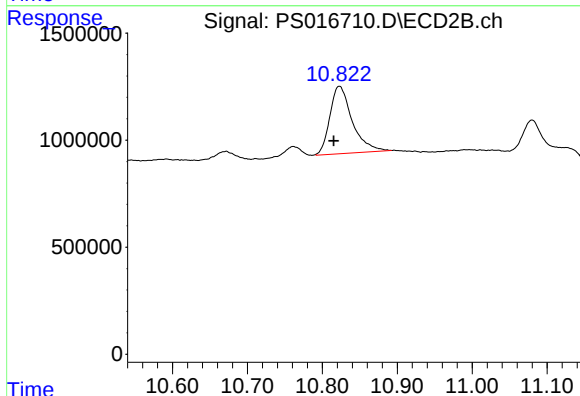


#15 Picloram

R.T.: 10.823 min
Delta R.T.: 0.007 min
Response: 6535555
Conc: 1.62 ng/ml

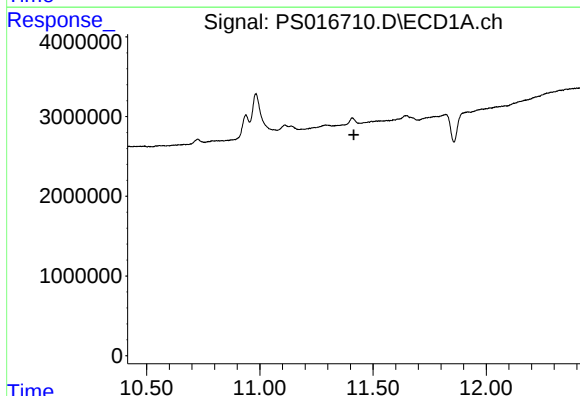

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.415 min
Response: 0
Conc: N.D.

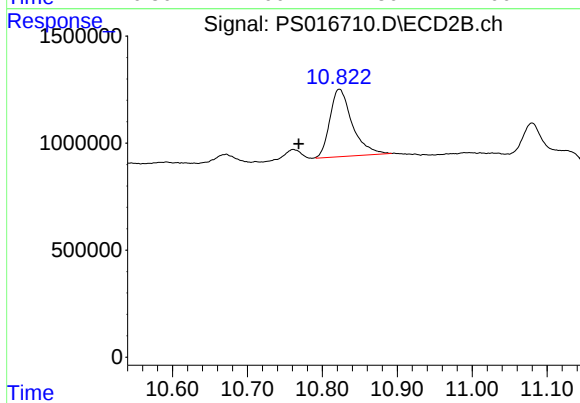

#16 DCPA

R.T.: 10.823 min
Delta R.T.: 0.054 min
Response: 6535555
Conc: 1.45 ng/ml