

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082522\
 Data File : PS020362.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Aug 2022 09:15
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 22:30:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.184	6.761	1499.9E6	448.4E6	508.672	550.179
Target Compounds							
1) T	Dalapon	3.004	0.000	308776	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.465f	0.000	1485160	0	<MDL	N.D. #
7) T	MCPA	7.657	0.000	1498037	0	<MDL	N.D. #
10) T	Pentachlo...	8.605	0.000	196448	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.174	0.000	1569149	0	<MDL	N.D. #
12) T	2,4,5-T	9.457	0.000	24892466	0	1.371	N.D. #
13) T	2,4-DB	9.962	0.000	197758	0	<MDL	N.D. #
14) T	DINOSEB	11.076f	0.000	135.5E6	0	8.515	N.D. #
15) T	Picloram	10.987	10.875f	9635042	29683858	<MDL	3.934 #
16) T	DCPA	11.406	0.000	1141893	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082522\
Data File : PS020362.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Aug 2022 09:15
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 22:30:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

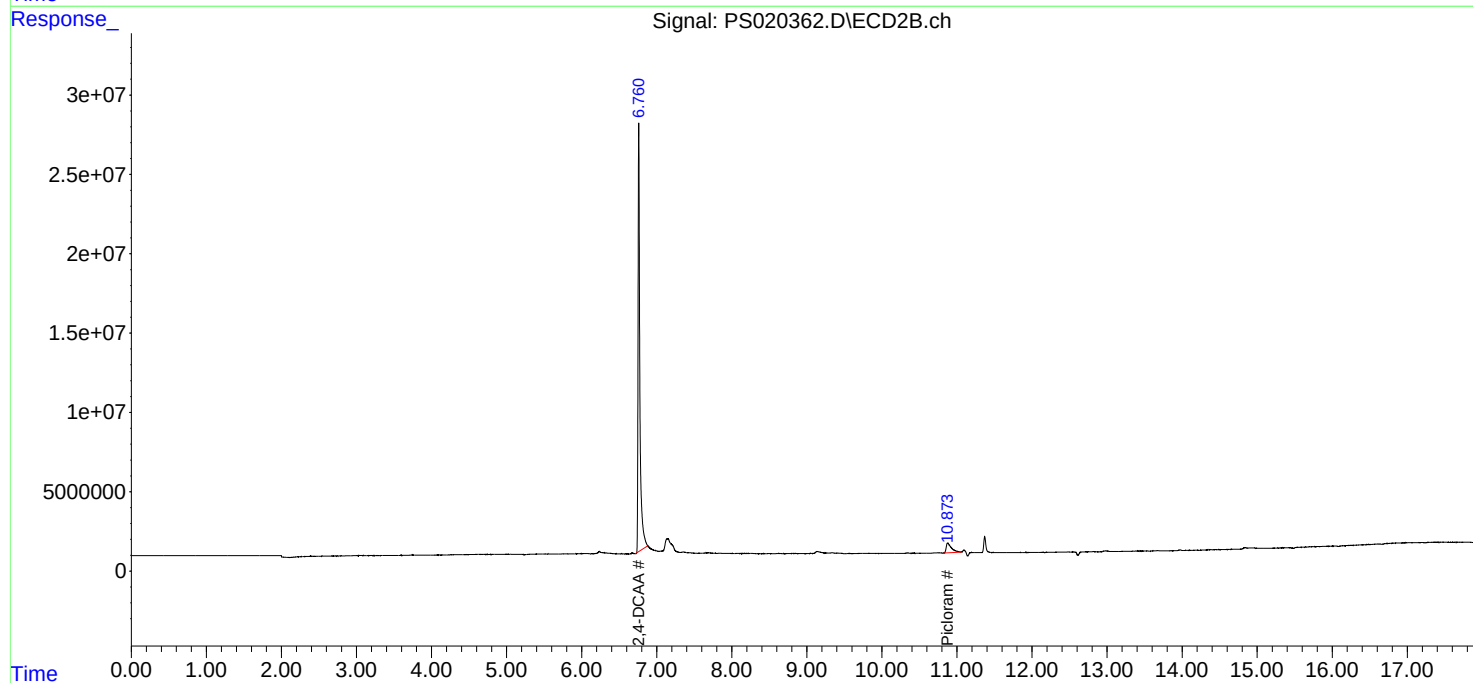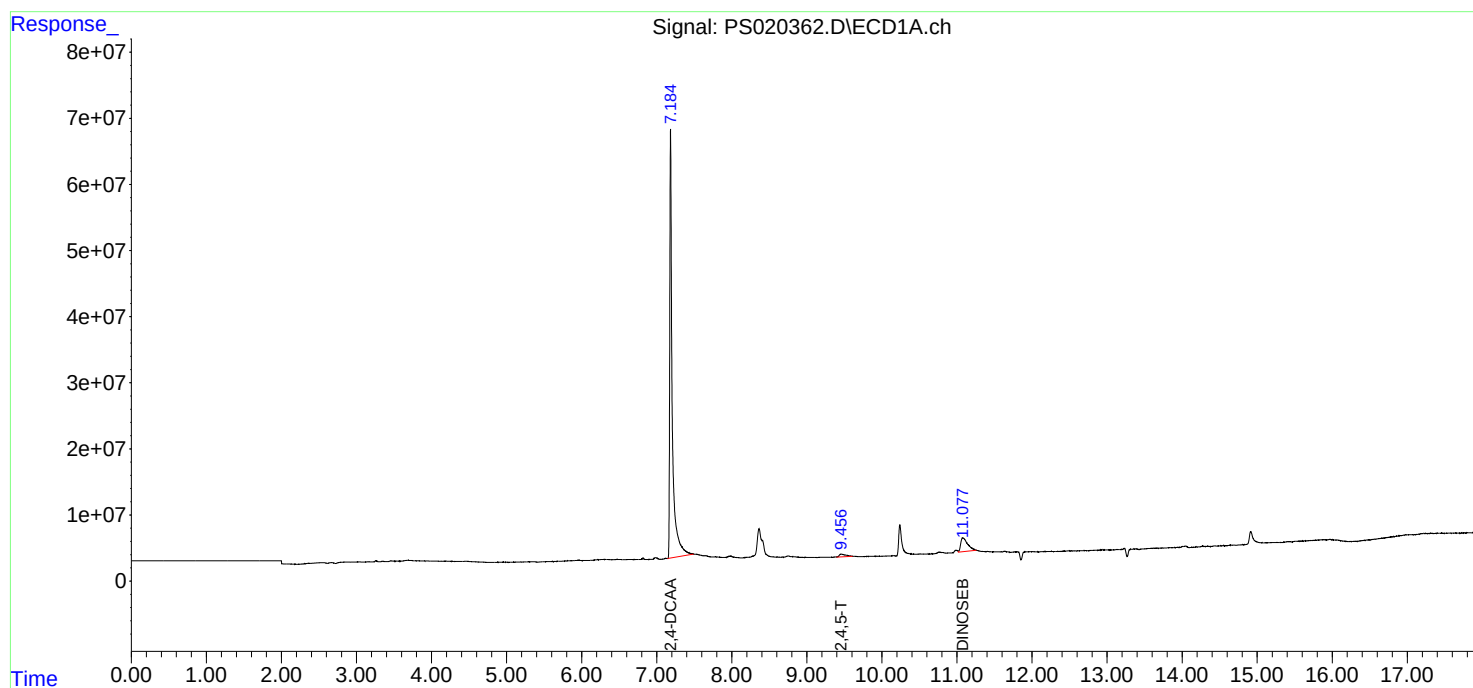


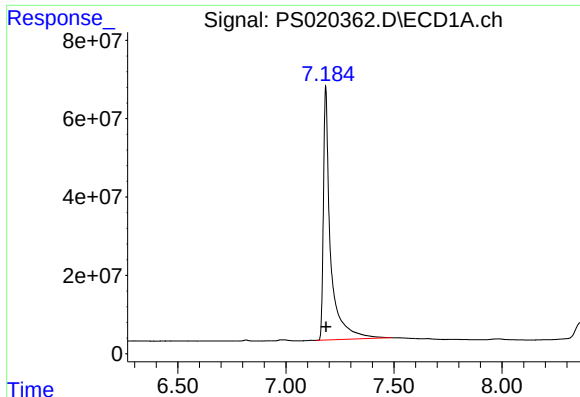

#4 2,4-DCAA


R.T.: 7.184 min
Delta R.T.: -0.001 min
Response: 1499933501
Conc: 508.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

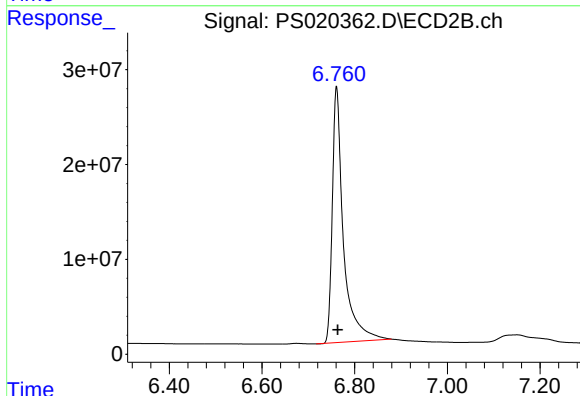


#4 2,4-DCAA

R.T.: 6.761 min
Delta R.T.: -0.003 min
Response: 448371463
Conc: 550.18 ng/ml

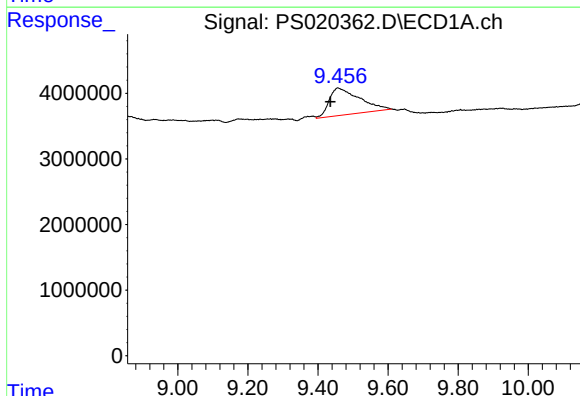


#12 2,4,5-T

R.T.: 9.457 min
Delta R.T.: 0.021 min
Response: 24892466
Conc: 1.37 ng/ml

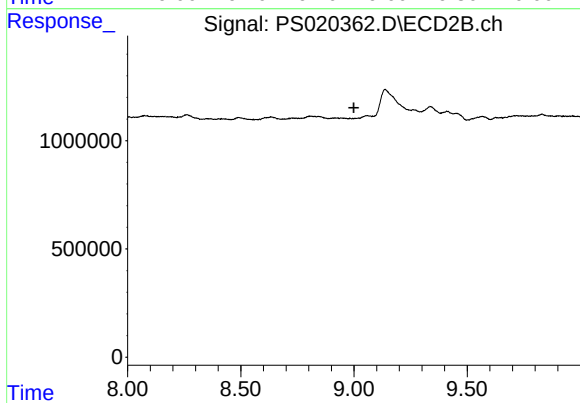

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 8.999 min
Response: 0
Conc: N.D.

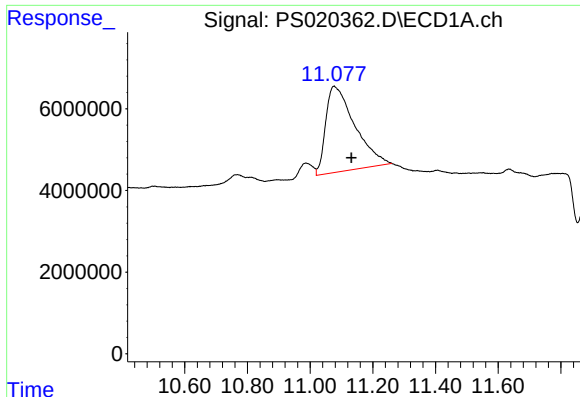

#14 DINOSEB


R.T.: 11.076 min
Delta R.T.: -0.056 min
Response: 135468856
Conc: 8.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

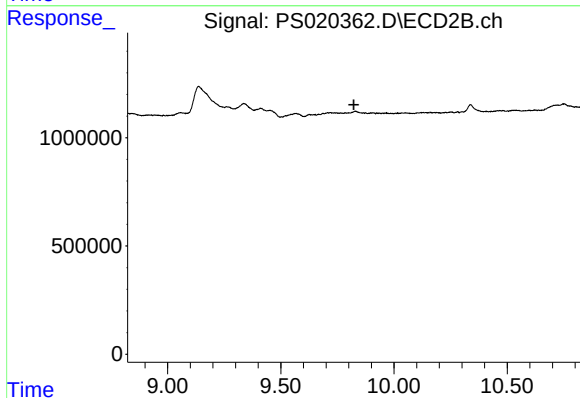


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.823 min
Response: 0
Conc: N.D.

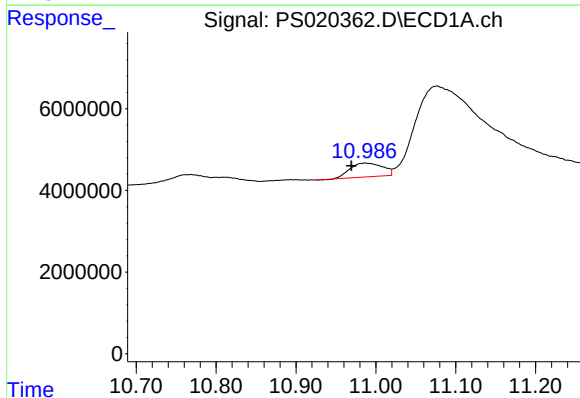

#15 Picloram

R.T.: 10.987 min
Delta R.T.: 0.017 min
Response: 9635042
Conc: N.D.

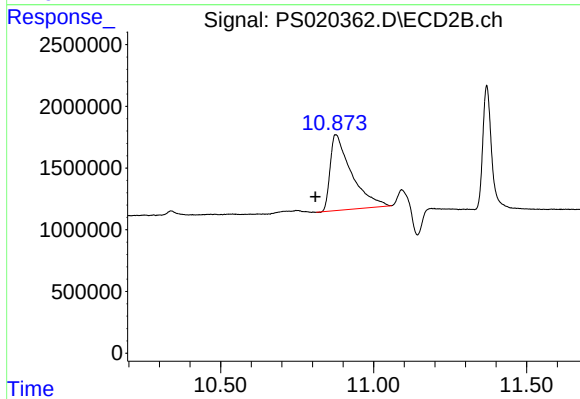

#15 Picloram

R.T.: 10.875 min
Delta R.T.: 0.064 min
Response: 29683858
Conc: 3.93 ng/ml