

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082522\
 Data File : PS020365.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Aug 2022 11:24
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 22:31:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.187	6.760	1441.6E6	416.5E6	488.877	511.065
Target Compounds							
2) T	3,5-DICHL...	6.423	0.000	298248	0	<MDL	N.D. #
5) T	DICAMBA	0.000	6.926	0	1017356	N.D.	<MDL
6) T	MCP	0.000	6.973f	0	21717944	N.D.	7.961
7) T	MCPA	7.654	0.000	2892886	0	<MDL	N.D. #
10) T	Pentachlo...	8.663f	0.000	10002761	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.167	0.000	5376854	0	<MDL	N.D. #
12) T	2,4,5-T	9.434	0.000	17977883	0	<MDL	N.D. #
13) T	2,4-DB	9.929f	0.000	1405798	0	<MDL	N.D. #
14) T	DINOSEB	11.127	0.000	19908063	0	1.251	N.D. #
15) T	Picloram	10.973	10.868f	16258880	14654836	<MDL	1.942 #
16) T	DCPA	11.403	10.743	6542368	928710	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082522\
Data File : PS020365.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Aug 2022 11:24
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 22:31:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

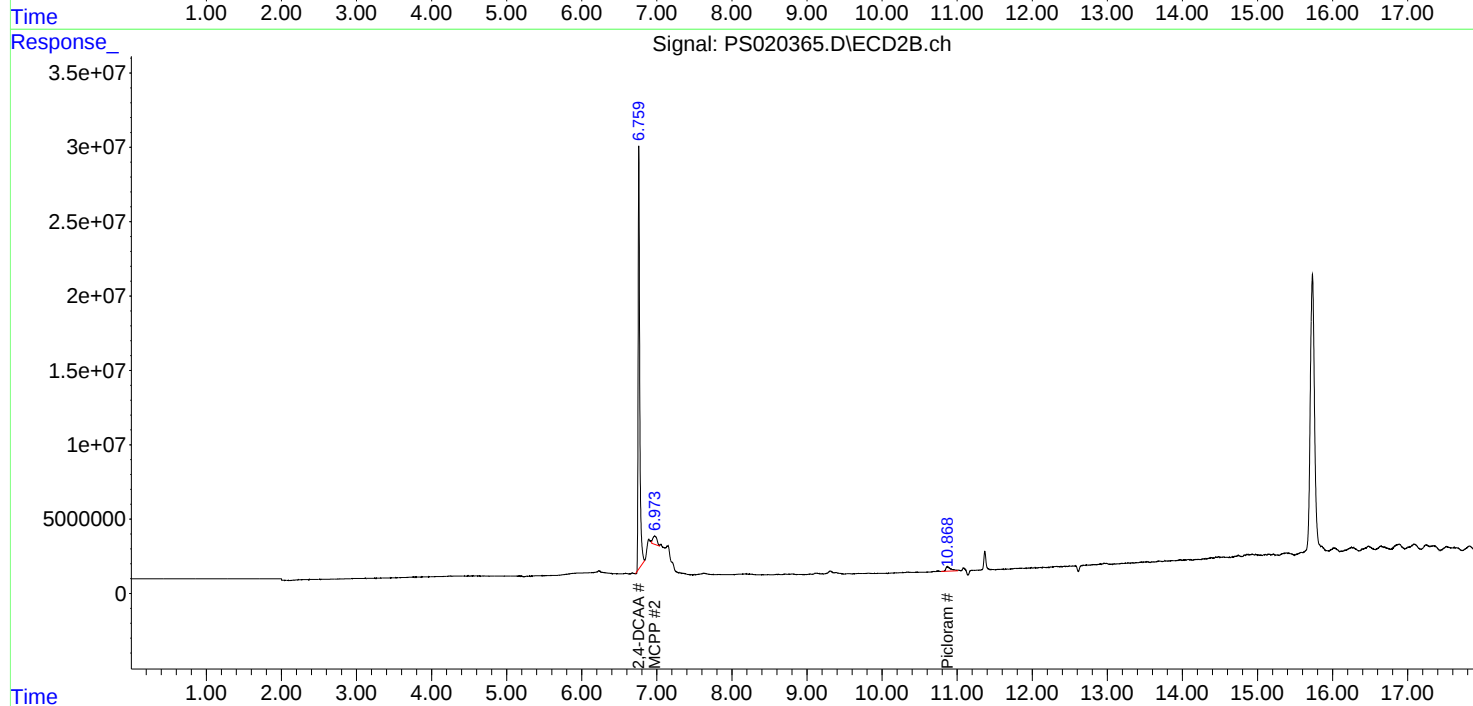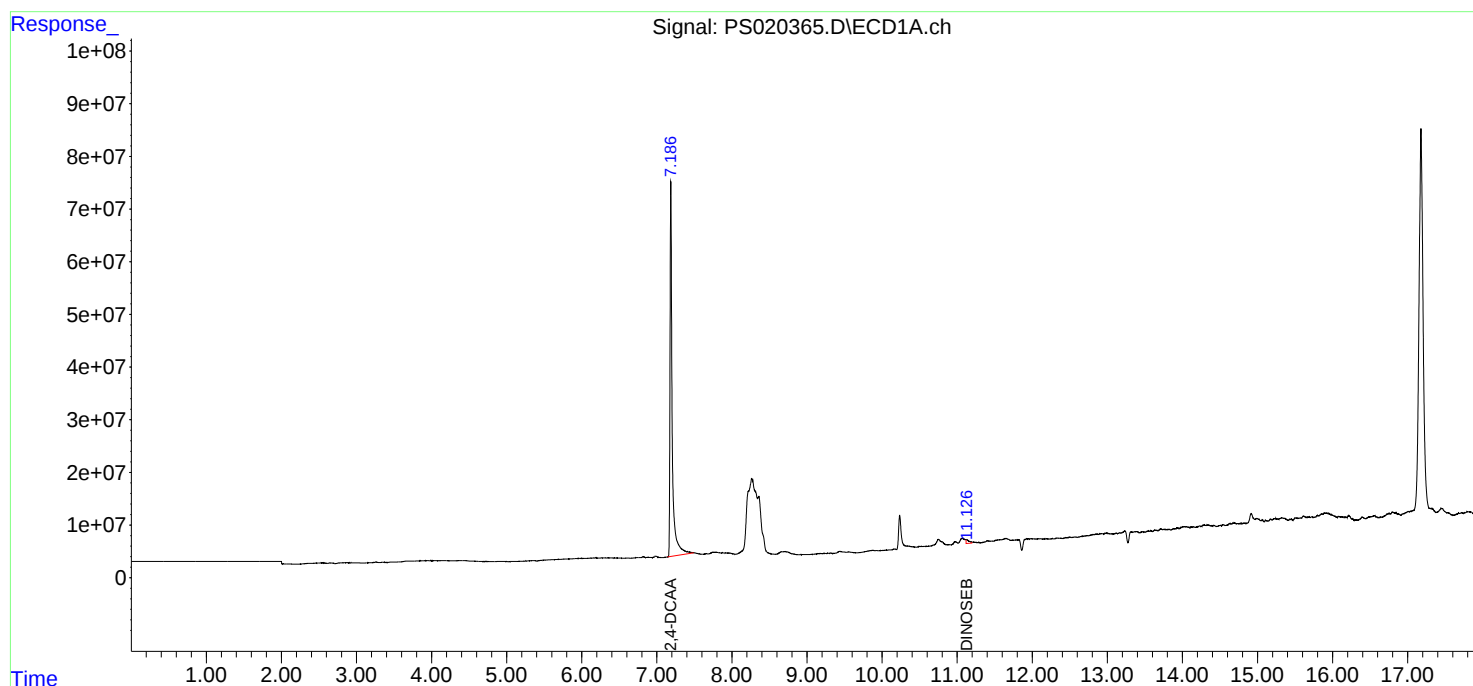


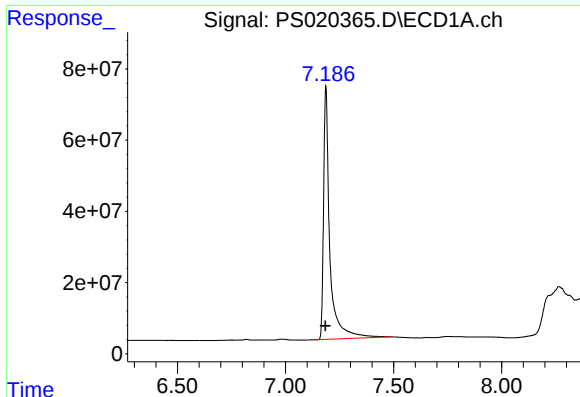

#4 2,4-DCAA


R.T.: 7.187 min
Delta R.T.: 0.000 min
Response: 1441562581
Conc: 488.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

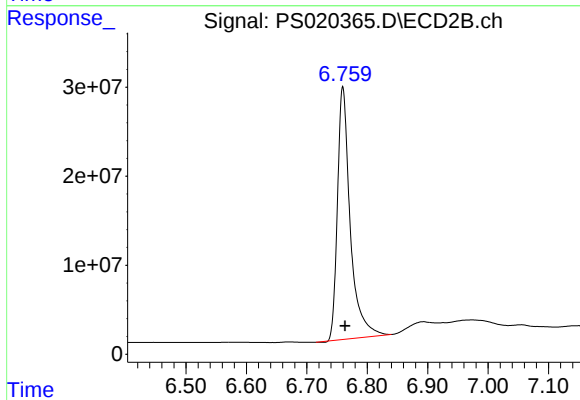


#4 2,4-DCAA

R.T.: 6.760 min
Delta R.T.: -0.004 min
Response: 416495398
Conc: 511.06 ng/ml

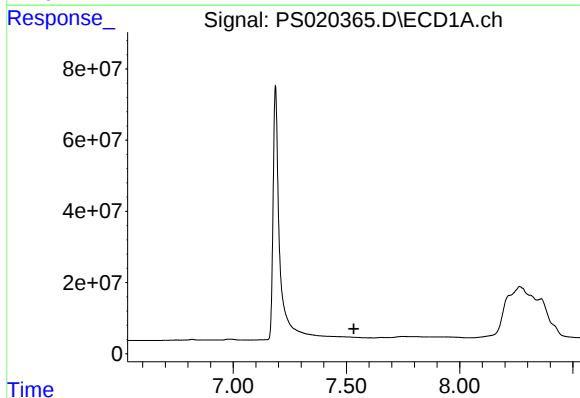


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.533 min
Response: 0
Conc: N.D.

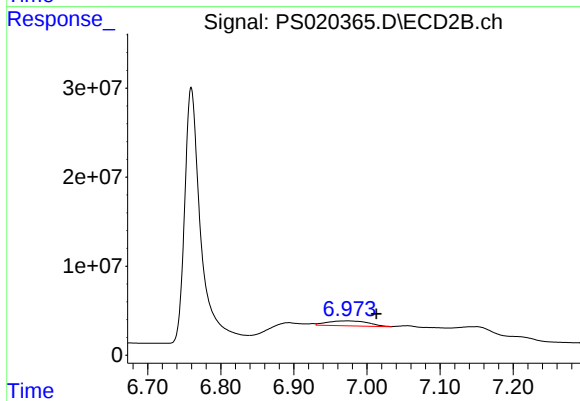

#6 MCPP


R.T.: 6.973 min
Delta R.T.: -0.040 min
Response: 21717944
Conc: 7.96 ug/ml

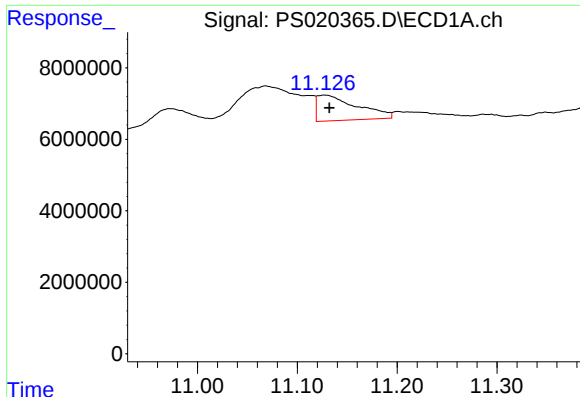

#14 DINOSEB


R.T.: 11.127 min
Delta R.T.: -0.005 min
Response: 19908063
Conc: 1.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

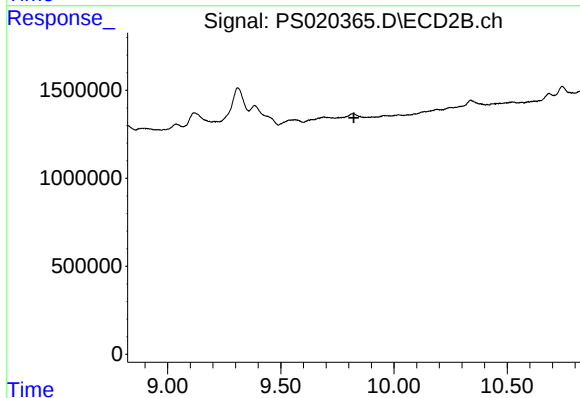


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.823 min
Response: 0
Conc: N.D.

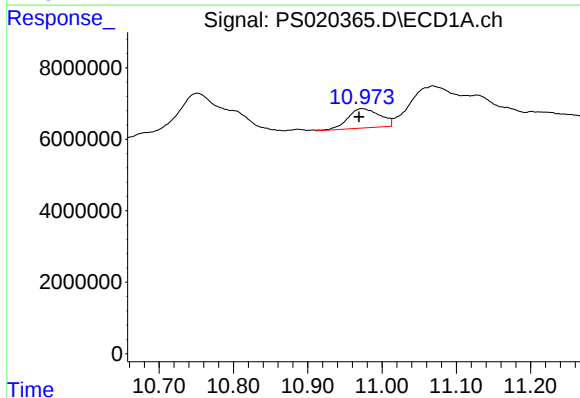

#15 Picloram

R.T.: 10.973 min
Delta R.T.: 0.004 min
Response: 16258880
Conc: N.D.

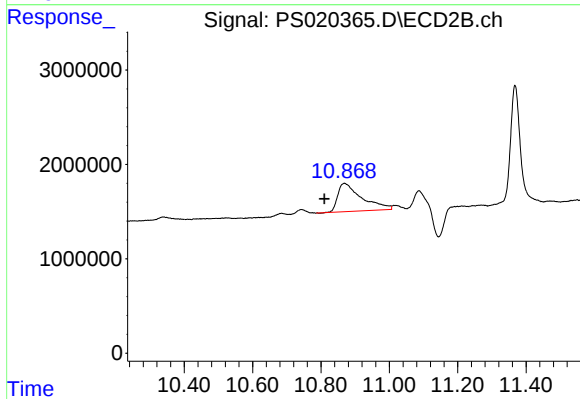

#15 Picloram

R.T.: 10.868 min
Delta R.T.: 0.058 min
Response: 14654836
Conc: 1.94 ng/ml