

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082620\
 Data File : PS011921.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Aug 2020 11:49
 Operator : DD\AJ
 Sample : PB131190BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 26 12:44:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.223	6.913	515.7E6	300.8E6	472.772	562.379
Target Compounds							
1) T	Dalapon	2.992	2.579	14102085	9772822	11.321	12.930
2) T	3,5-DICHL...	0.000	6.094	0	78978503	N.D.	96.008
5) T	DICAMBA	7.401	7.047	7763085	11913485	1.895	5.514 #
6) T	MCP	7.577	0.000	6642365	0	2.079	N.D. #
7) T	MCPA	7.770	7.375	62783607	16222296	13.803	5.920 #
10) T	Pentachlo...	8.702	0.000	13112353	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.766	0	8608352	N.D.	2.944
12) T	2,4,5-T	9.419	0.000	37325312	0	6.299	N.D. #
15) T	Picloram	11.045	11.022	36692684	77937547	4.695	17.195 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082620\
Data File : PS011921.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2020 11:49
Operator : DD\AJ
Sample : PB131190BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 26 12:44:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

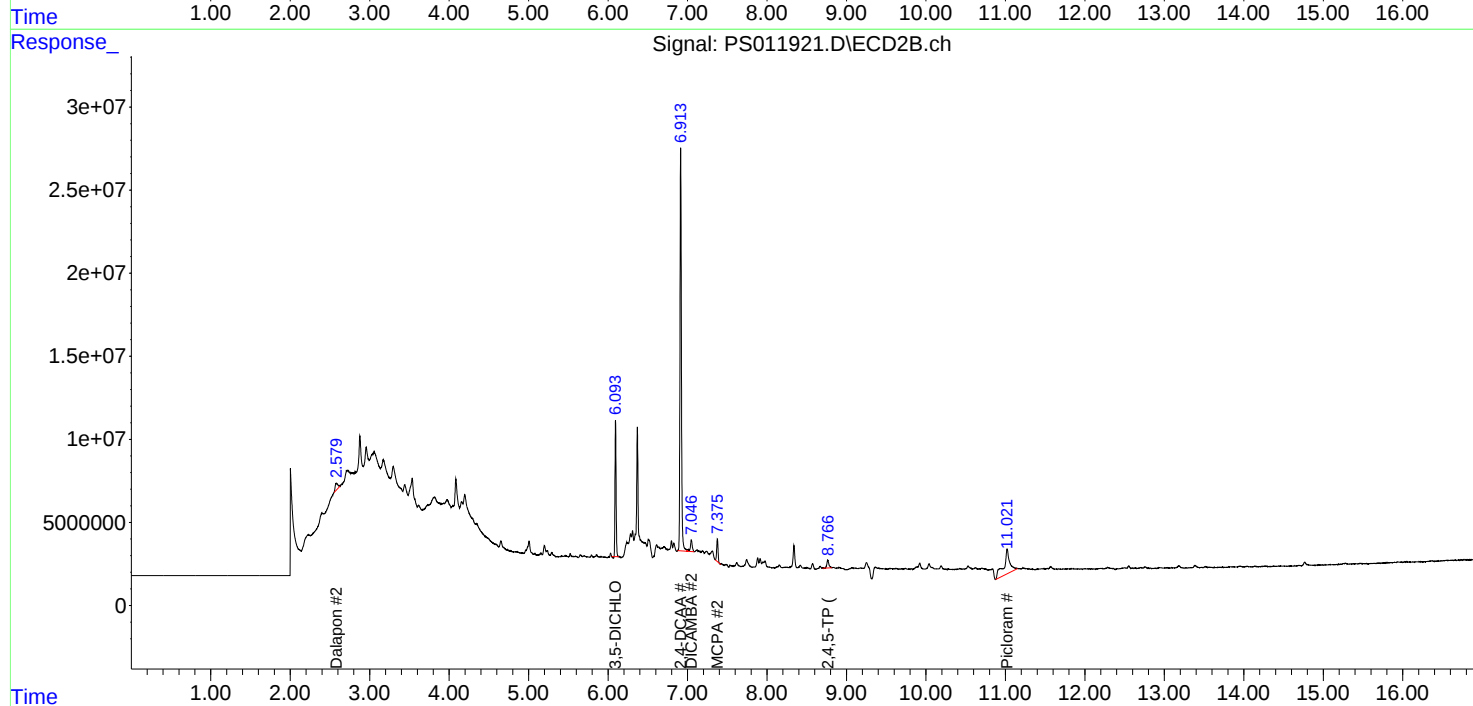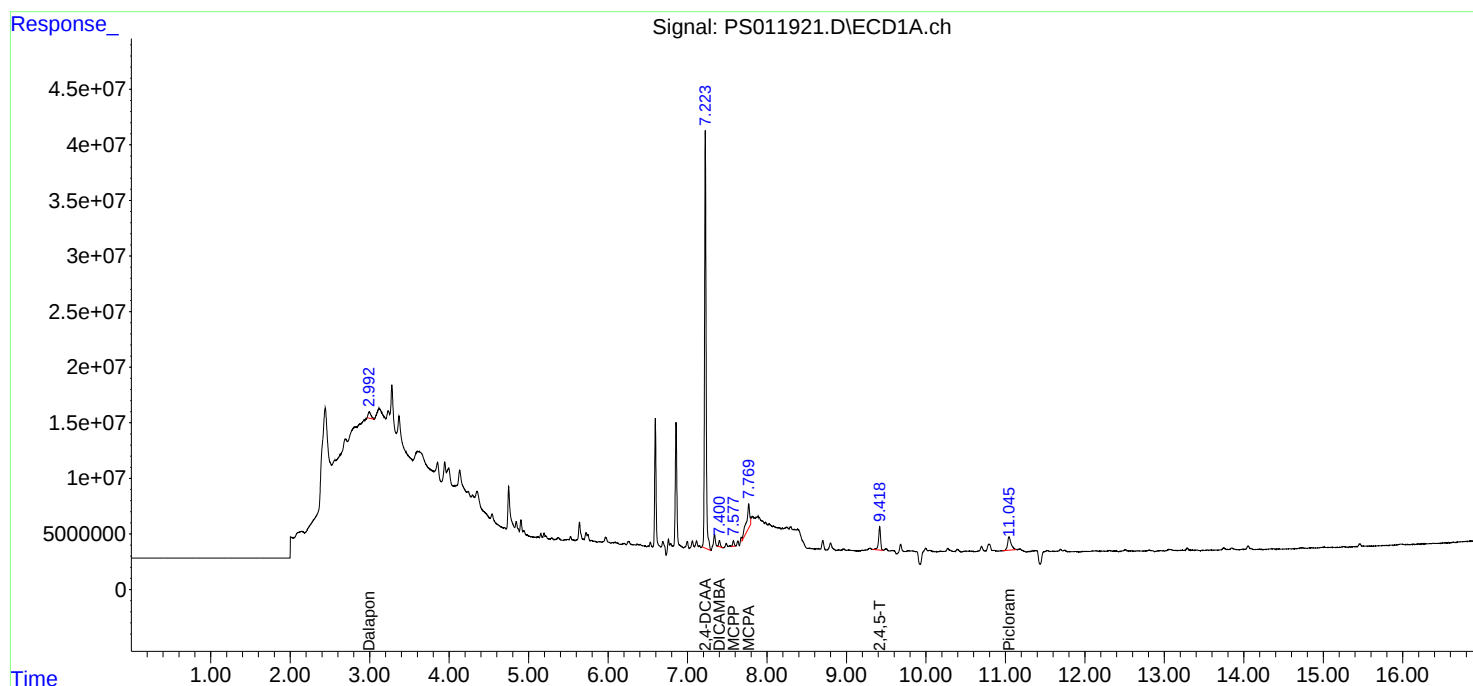


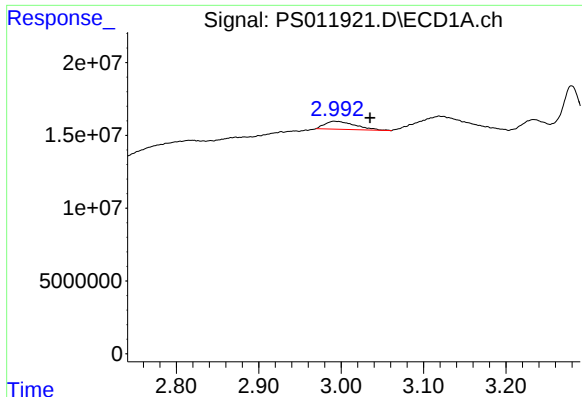

#1 Dalapon


R.T.: 2.992 min
Delta R.T.: -0.043 min
Response: 14102085
Conc: 11.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

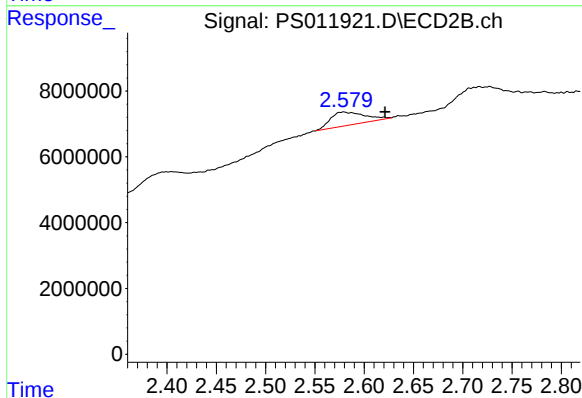


#1 Dalapon

R.T.: 2.579 min
Delta R.T.: -0.042 min
Response: 9772822
Conc: 12.93 ng/ml

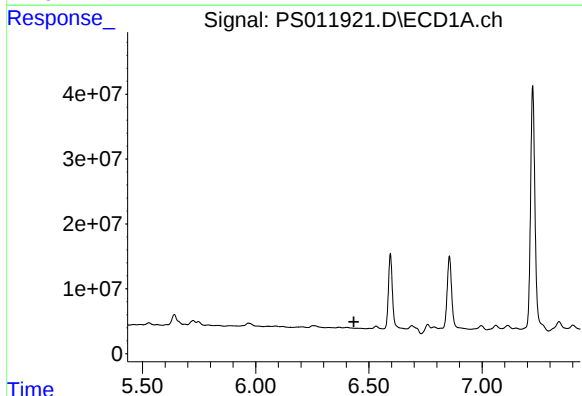


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

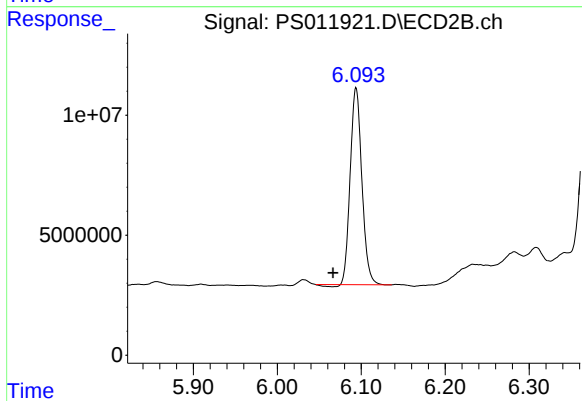

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.094 min
Delta R.T.: 0.027 min
Response: 78978503
Conc: 96.01 ng/ml

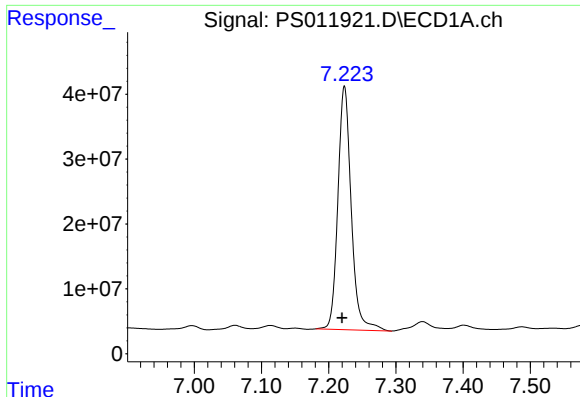

#4 2,4-DCAA


R.T.: 7.223 min
Delta R.T.: 0.003 min
Response: 515684416
Conc: 472.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

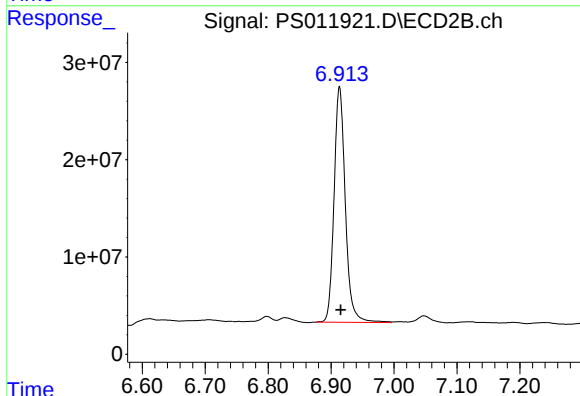


#4 2,4-DCAA

R.T.: 6.913 min
Delta R.T.: -0.002 min
Response: 300752891
Conc: 562.38 ng/ml

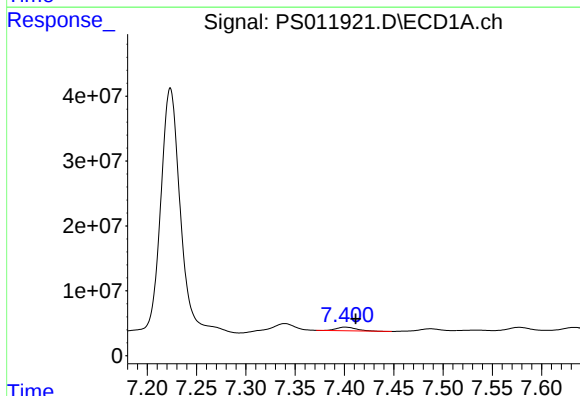


#5 DICAMBA

R.T.: 7.401 min
Delta R.T.: -0.011 min
Response: 7763085
Conc: 1.90 ng/ml

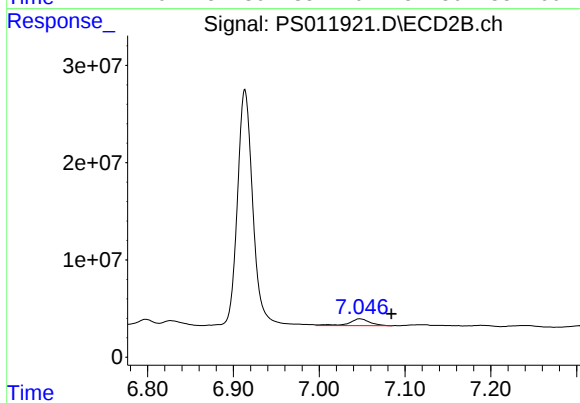

#5 DICAMBA


R.T.: 7.047 min
Delta R.T.: -0.037 min
Response: 11913485
Conc: 5.51 ng/ml

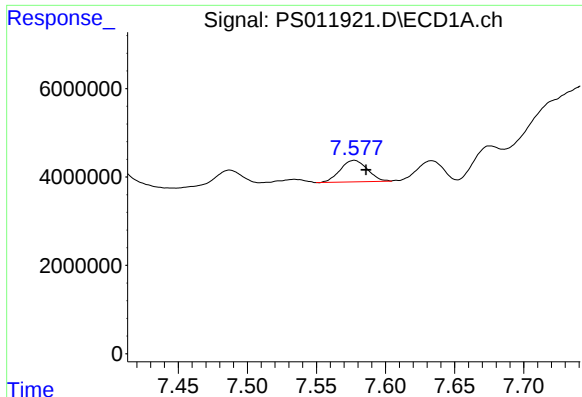

#6 MCPP


R.T.: 7.577 min
Delta R.T.: -0.009 min
Response: 6642365
Conc: 2.08 ug/ml

Instrument :
ECD_S
ClientSampleId :

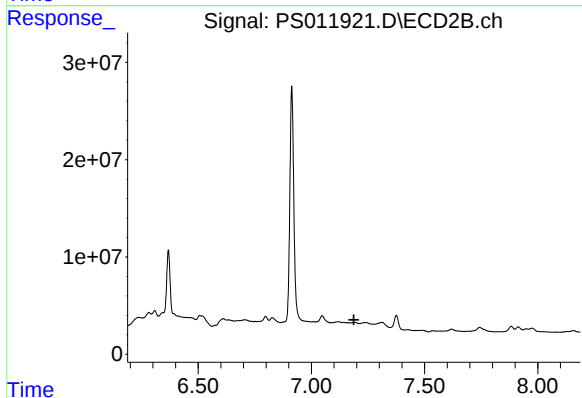


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

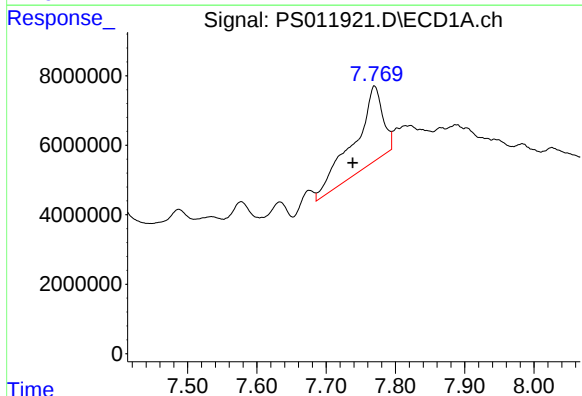


#7 MCPA

R.T.: 7.770 min
Delta R.T.: 0.032 min
Response: 62783607
Conc: 13.80 ug/ml

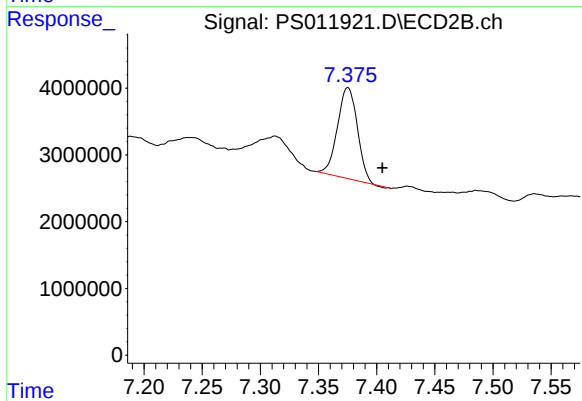

#7 MCPA


R.T.: 7.375 min
Delta R.T.: -0.030 min
Response: 16222296
Conc: 5.92 ug/ml

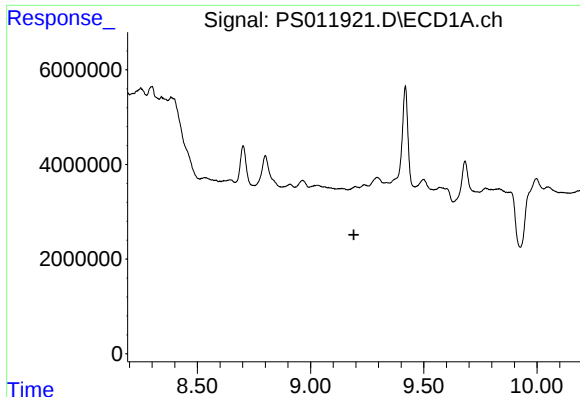

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

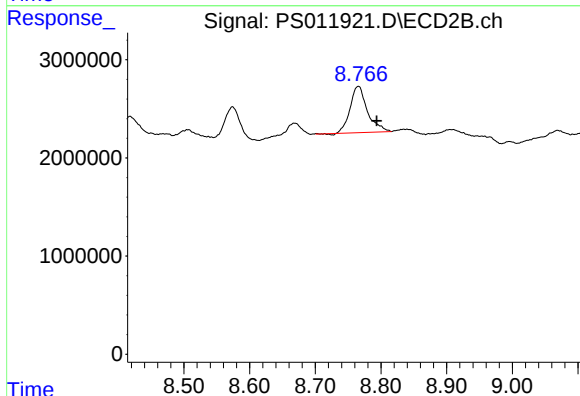


#11 2,4,5-TP (SILVEX)

R.T.: 8.766 min
Delta R.T.: -0.028 min
Response: 8608352
Conc: 2.94 ng/ml

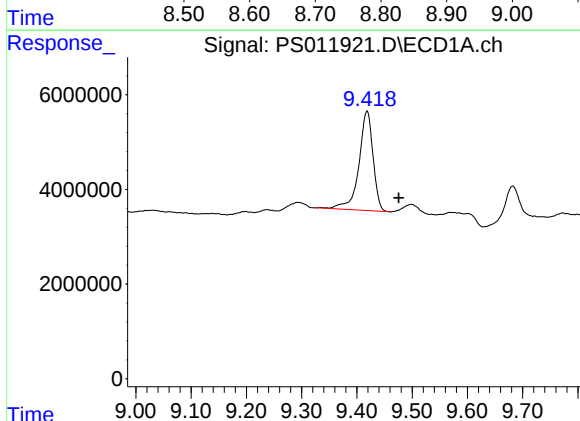


#12 2,4,5-T

R.T.: 9.419 min
Delta R.T.: -0.057 min
Response: 37325312
Conc: 6.30 ng/ml

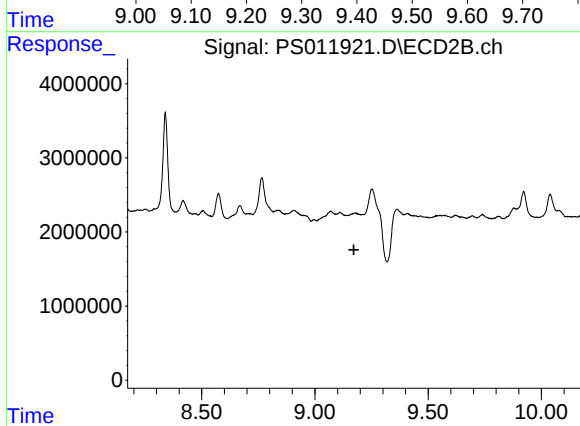

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.

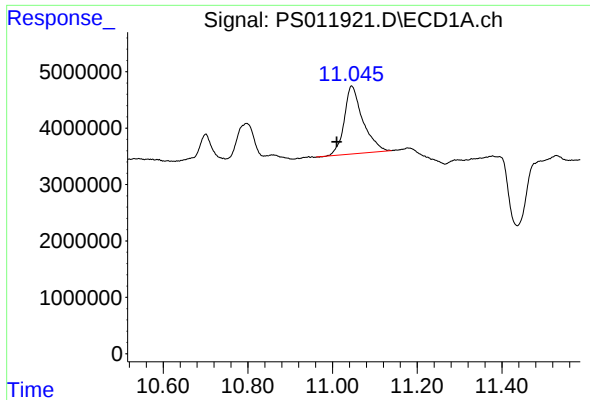

#15 Picloram

R.T.: 11.045 min
Delta R.T.: 0.036 min
Response: 36692684
Conc: 4.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

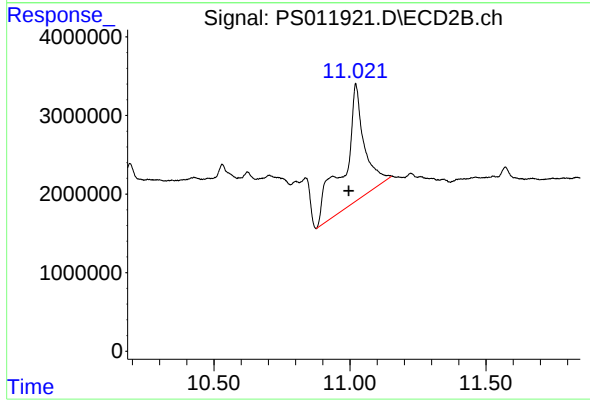

#15 Picloram

R.T.: 11.022 min
Delta R.T.: 0.026 min
Response: 77937547
Conc: 17.20 ng/ml