

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082620\
 Data File : PS011947.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Aug 2020 21:45
 Operator : DD\AJ
 Sample : L3784-08
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 RO-23

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 02:12:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.218	6.914	221.1E6	148.8E6	202.688	278.298 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.095	0	93712932	N.D.	113.920
3) T	4-Nitroph...	7.055	6.505	6971341	26119721	11.835	71.637 #
5) T	DICAMBA	7.396	7.048	9853577	16202317	2.406	7.499 #
6) T	MCP	7.629	0.000	10459493	0	3.274	N.D. #
7) T	MCPA	7.689	7.462	244.5E6	175.2E6	53.749	63.921
8) T	DICHLORPROP	0.000	7.736	0	23299326	N.D.	41.264
9) T	2,4-D	8.399	0.000	91008152	0	80.603	N.D. #
11) T	2,4,5-TP ...	0.000	8.786	0	15918259	N.D.	5.445
12) T	2,4,5-T	9.411	0.000	23442920	0	3.956	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082620\
Data File : PS011947.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2020 21:45
Operator : DD\AJ
Sample : L3784-08
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
RO-23

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 02:12:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

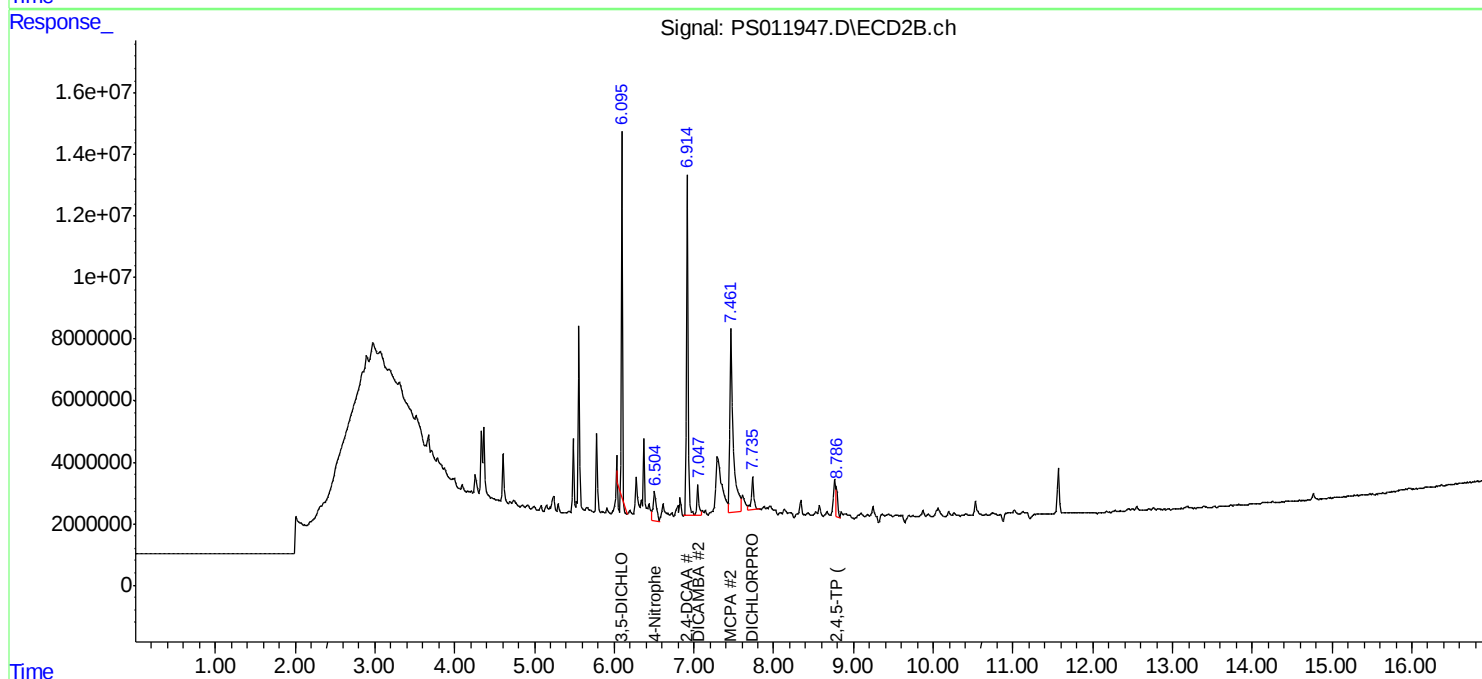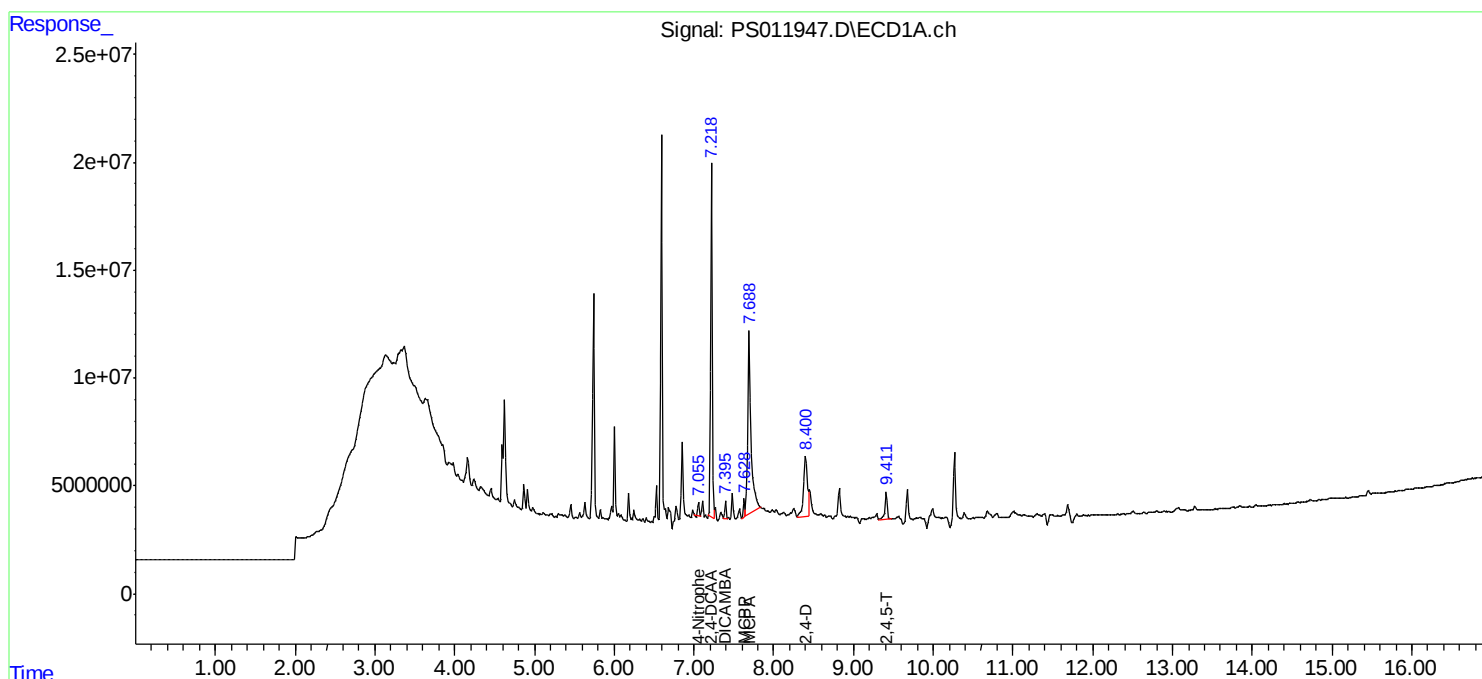


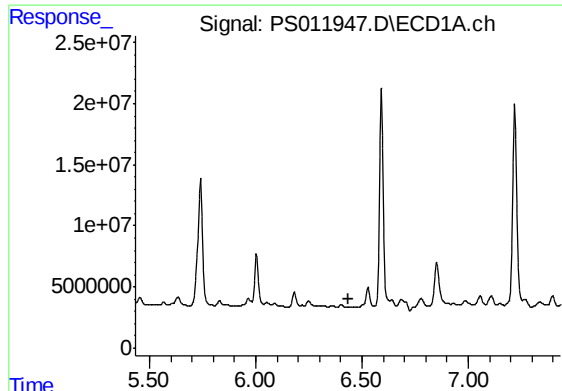

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RO-23

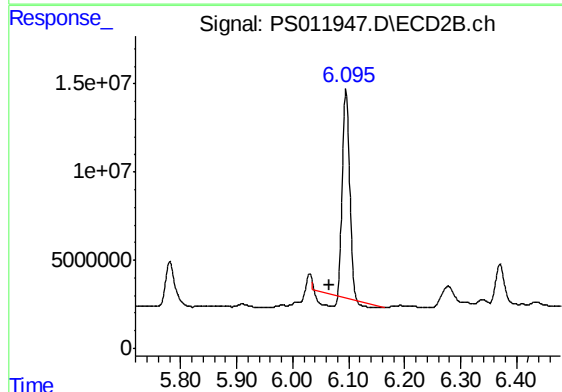


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.095 min
Delta R.T.: 0.029 min
Response: 93712932
Conc: 113.92 ng/ml

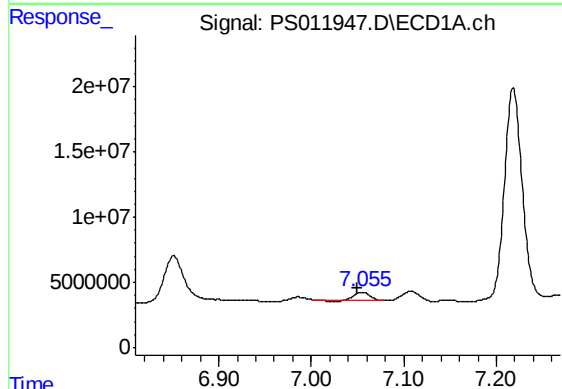


#3 4-Nitrophenol

R.T.: 7.055 min
Delta R.T.: 0.005 min
Response: 6971341
Conc: 11.84 ng/ml

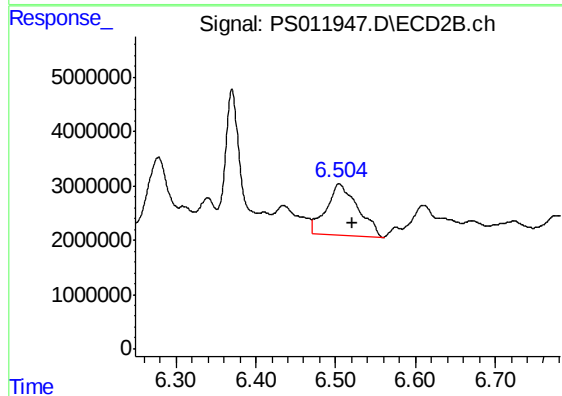

#3 4-Nitrophenol


R.T.: 6.505 min
Delta R.T.: -0.016 min
Response: 26119721
Conc: 71.64 ng/ml

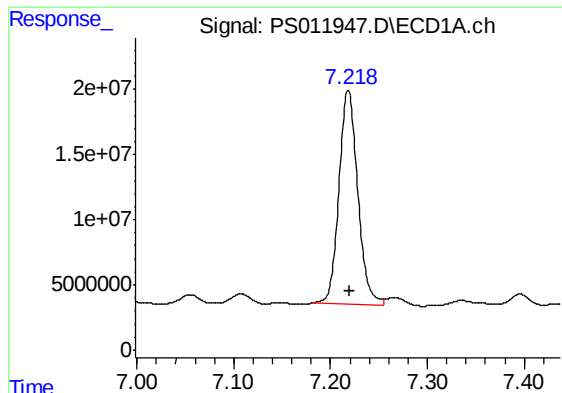

#4 2,4-DCAA


R.T.: 7.218 min
Delta R.T.: -0.002 min
Response: 221086081
Conc: 202.69 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-23

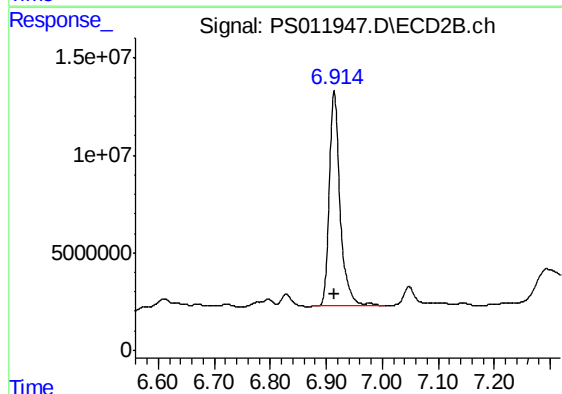


#4 2,4-DCAA

R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 148829848
Conc: 278.30 ng/ml

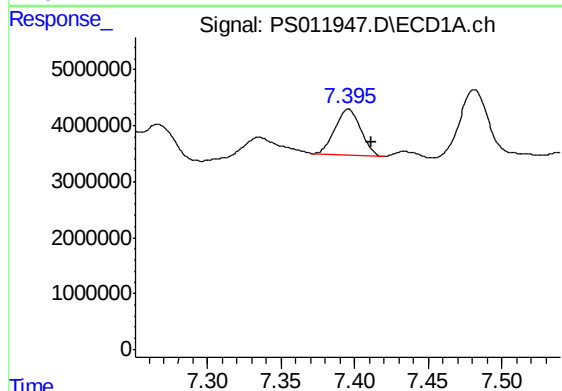


#5 DICAMBA

R.T.: 7.396 min
Delta R.T.: -0.016 min
Response: 9853577
Conc: 2.41 ng/ml

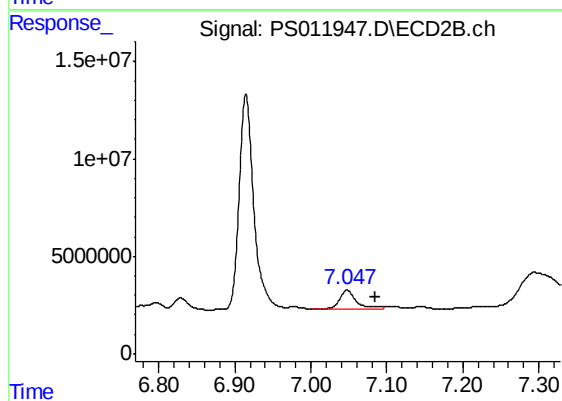

#5 DICAMBA


R.T.: 7.048 min
Delta R.T.: -0.036 min
Response: 16202317
Conc: 7.50 ng/ml

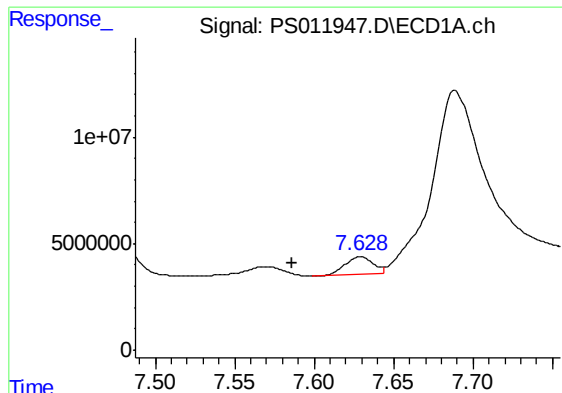

#6 MCPP


R.T.: 7.629 min
Delta R.T.: 0.043 min
Response: 10459493
Conc: 3.27 ug/ml

Instrument :
ECD_S
ClientSampleId :
RO-23

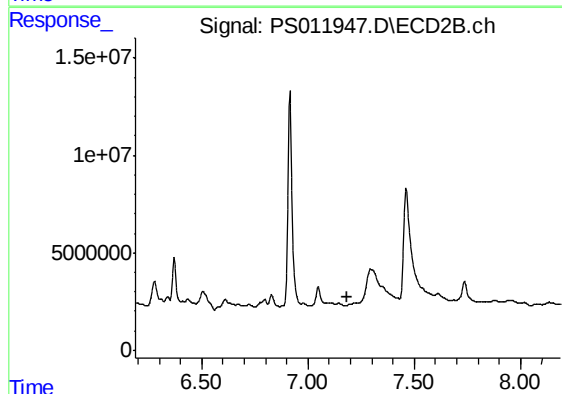


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

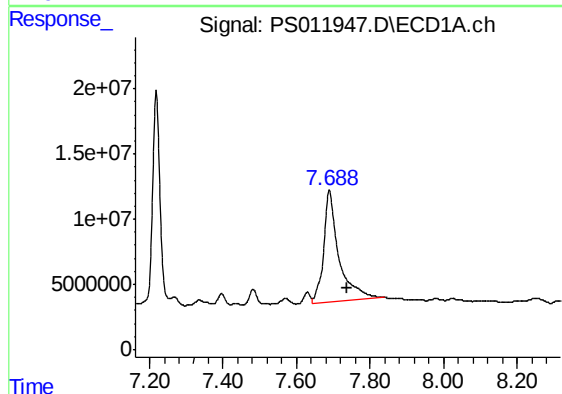


#7 MCPA

R.T.: 7.689 min
Delta R.T.: -0.049 min
Response: 244476668
Conc: 53.75 ug/ml

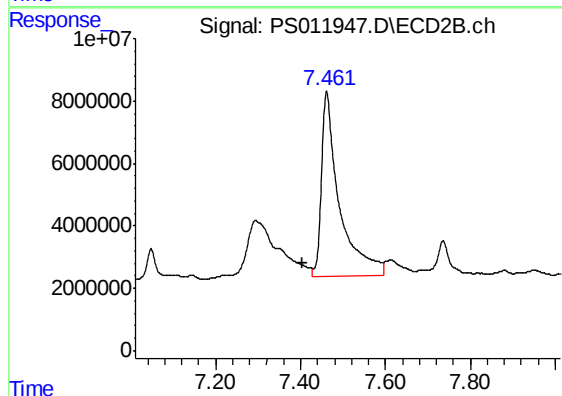

#7 MCPA


R.T.: 7.462 min
Delta R.T.: 0.057 min
Response: 175152385
Conc: 63.92 ug/ml

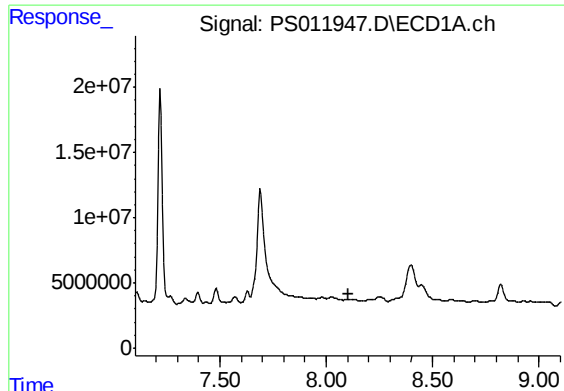

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RO-23

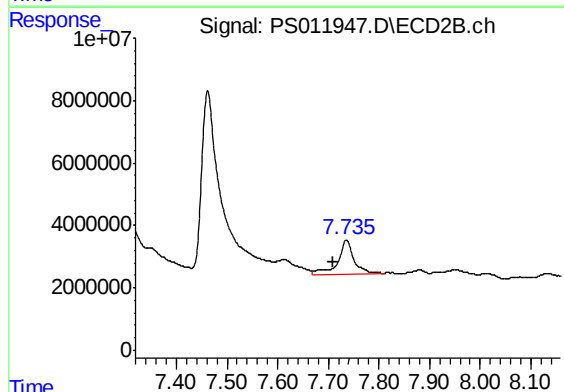


#8 DICHLORPROP

R.T.: 7.736 min
Delta R.T.: 0.026 min
Response: 23299326
Conc: 41.26 ng/ml

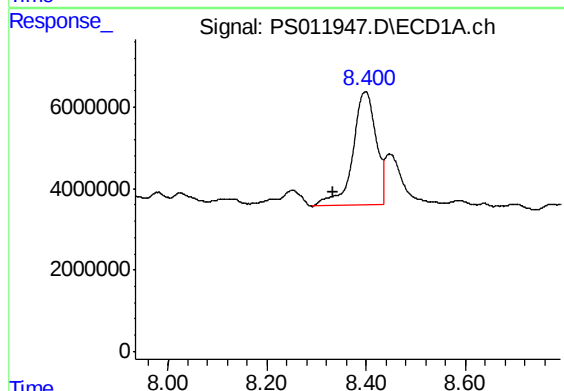


#9 2,4-D

R.T.: 8.399 min
Delta R.T.: 0.067 min
Response: 91008152
Conc: 80.60 ng/ml

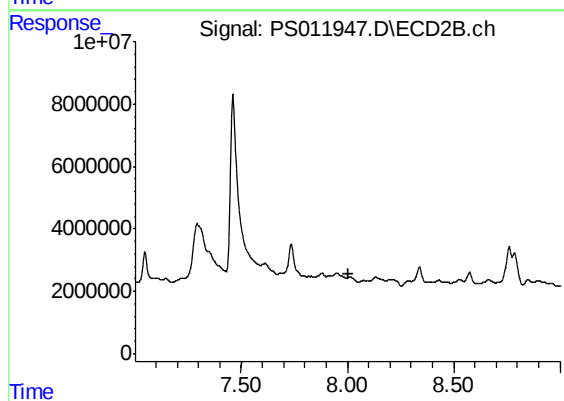

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 8.003 min
Response: 0
Conc: N.D.

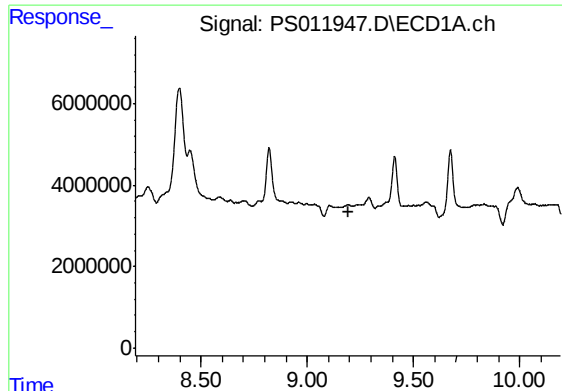

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RO-23

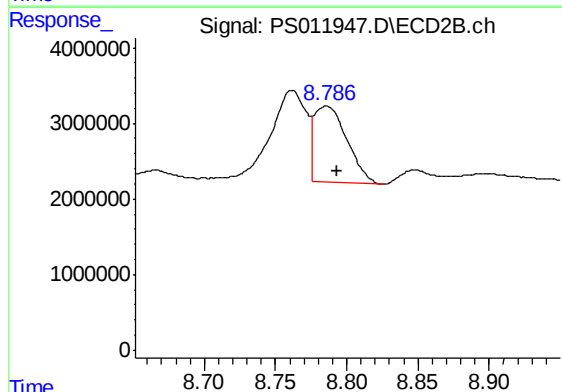


#11 2,4,5-TP (SILVEX)

R.T.: 8.786 min
Delta R.T.: -0.008 min
Response: 15918259
Conc: 5.44 ng/ml

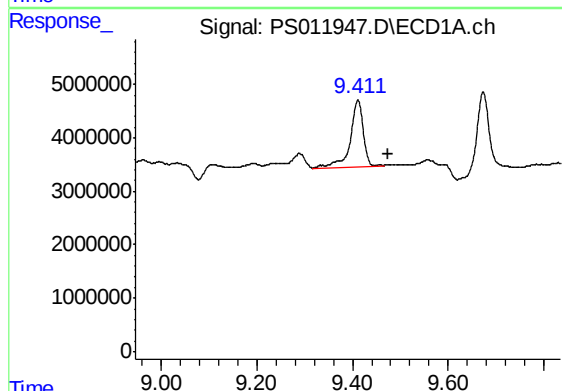

#12 2,4,5-T

R.T.: 9.411 min
Delta R.T.: -0.065 min
Response: 23442920
Conc: 3.96 ng/ml

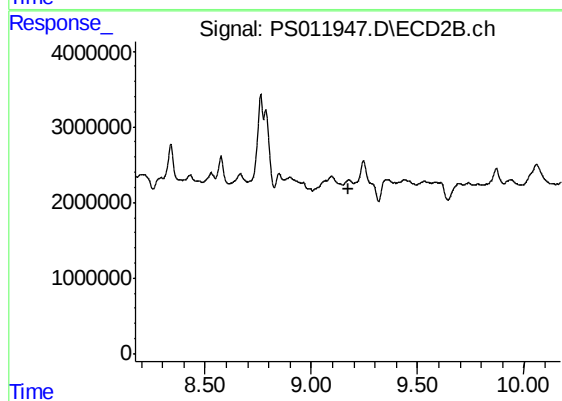

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.