

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082620\
 Data File : PS011948.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Aug 2020 22:08
 Operator : DD\AJ
 Sample : L378411
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 RO-24

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 02:12:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.218	6.915	227.6E6	150.6E6	208.704	281.588 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	105.1E6	N.D.	127.755
3) T	4-Nitroph...	7.055	6.506	4485025	16927515	7.614	46.426 #
5) T	DICAMBA	7.396	7.048	9597366	18339858	2.343	8.489 #
6) T	MCP	7.629	0.000	10040411	0	3.142	N.D. #
7) T	MCPA	7.690	7.462	253.5E6	199.3E6	55.737	72.744 #
8) T	DICHLORPROP	0.000	7.737	0	19343895	N.D.	34.259
9) T	2,4-D	8.400	0.000	115.4E6	0	102.184	N.D. #
11) T	2,4,5-TP ...	0.000	8.762	0	27088191	N.D.	9.265
12) T	2,4,5-T	9.411	0.000	20534689	0	3.465	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082620\
Data File : PS011948.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2020 22:08
Operator : DD\AJ
Sample : L378411
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
RO-24

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 02:12:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

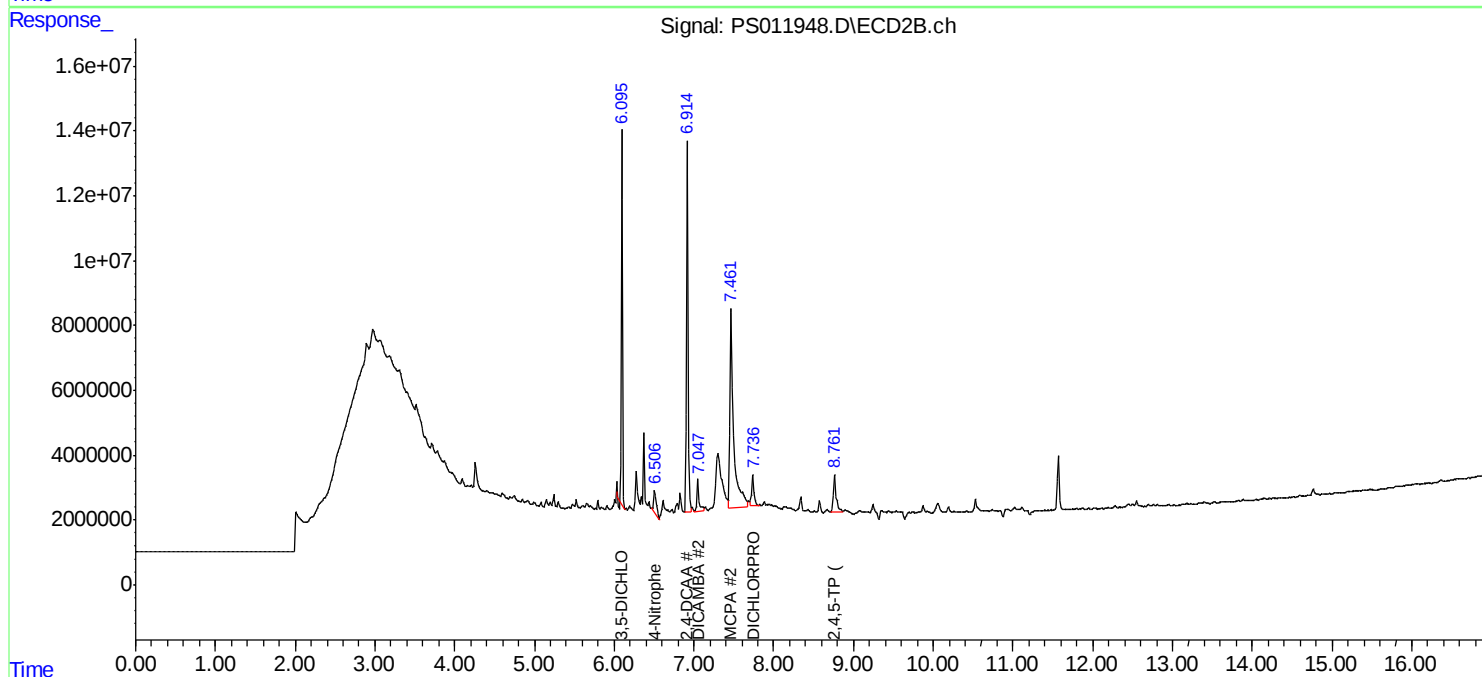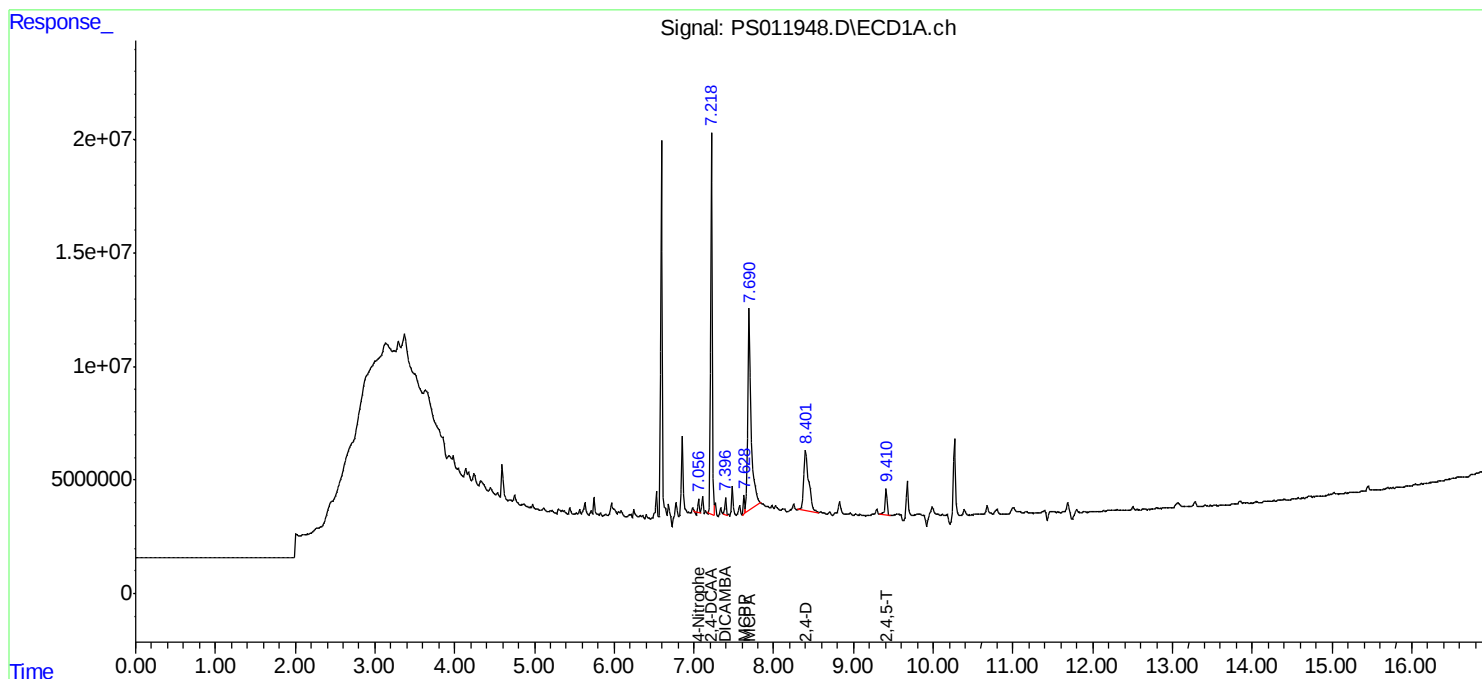


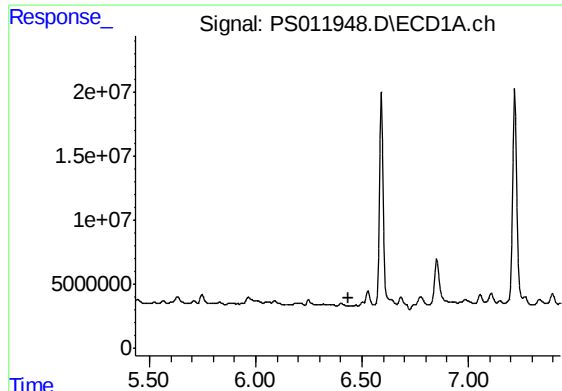

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RO-24

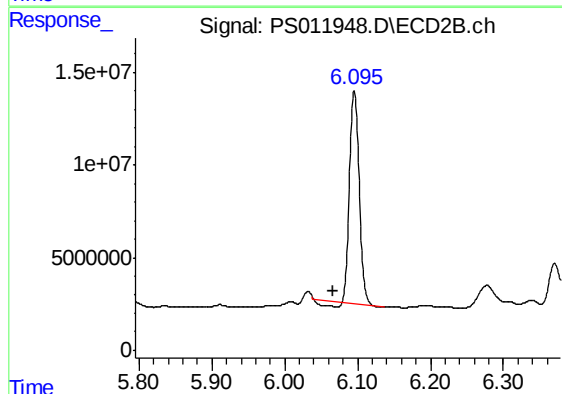


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.029 min
Response: 105093943
Conc: 127.76 ng/ml

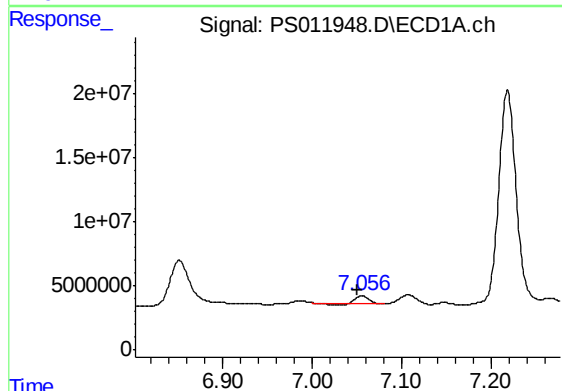


#3 4-Nitrophenol

R.T.: 7.055 min
Delta R.T.: 0.005 min
Response: 4485025
Conc: 7.61 ng/ml

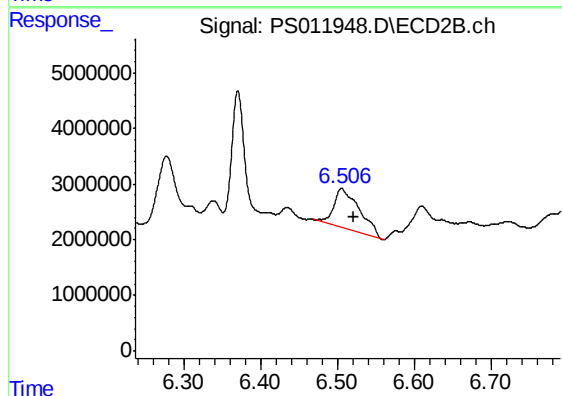

#3 4-Nitrophenol


R.T.: 6.506 min
Delta R.T.: -0.015 min
Response: 16927515
Conc: 46.43 ng/ml

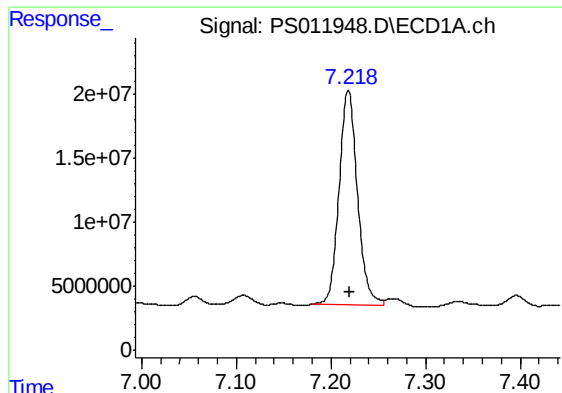

#4 2,4-DCAA


R.T.: 7.218 min
Delta R.T.: -0.002 min
Response: 227647784
Conc: 208.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-24

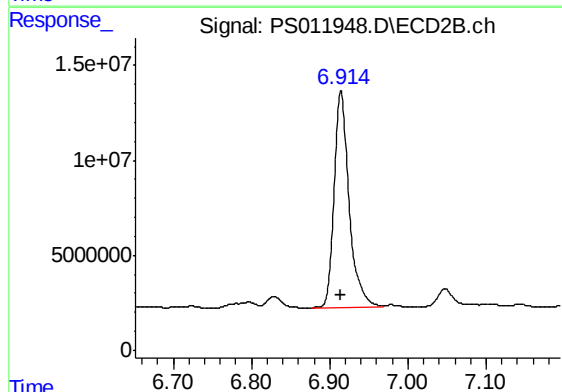


#4 2,4-DCAA

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 150589269
Conc: 281.59 ng/ml

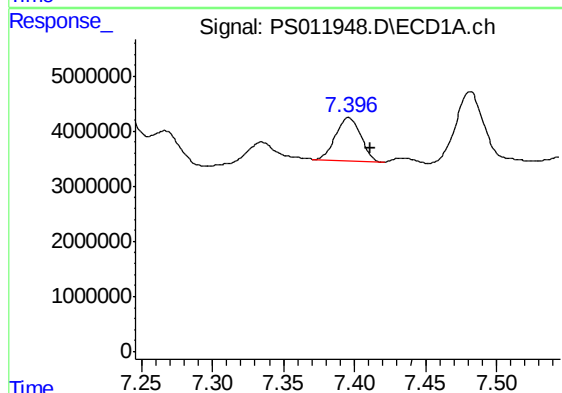


#5 DICAMBA

R.T.: 7.396 min
Delta R.T.: -0.016 min
Response: 9597366
Conc: 2.34 ng/ml

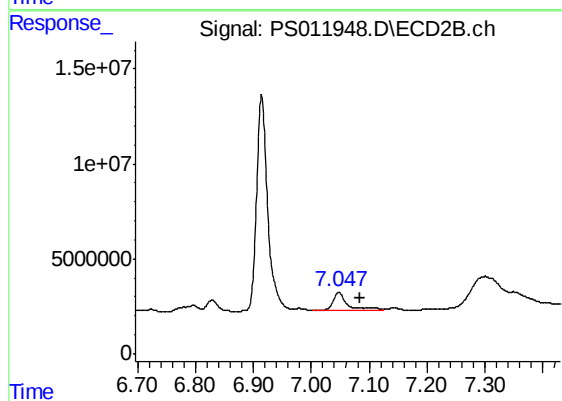

#5 DICAMBA


R.T.: 7.048 min
Delta R.T.: -0.036 min
Response: 18339858
Conc: 8.49 ng/ml

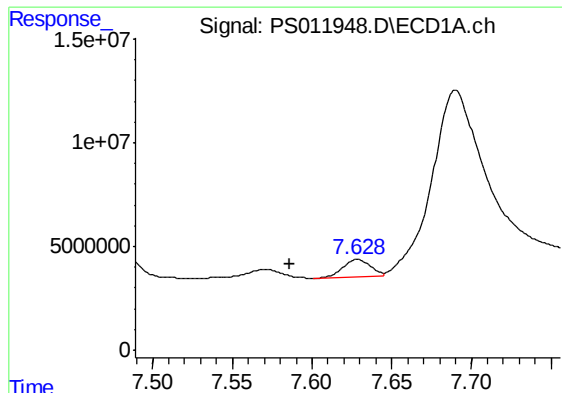

#6 MCPP


R.T.: 7.629 min
Delta R.T.: 0.043 min
Response: 10040411
Conc: 3.14 ug/ml

Instrument :
ECD_S
ClientSampleId :
RO-24

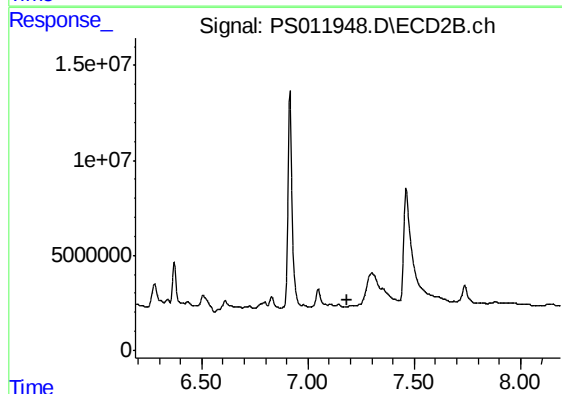


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

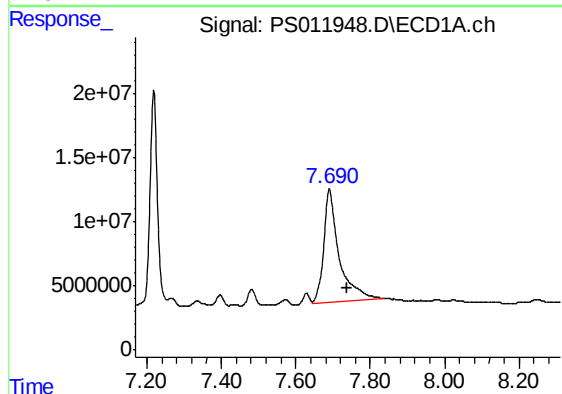


#7 MCPA

R.T.: 7.690 min
Delta R.T.: -0.048 min
Response: 253519286
Conc: 55.74 ug/ml

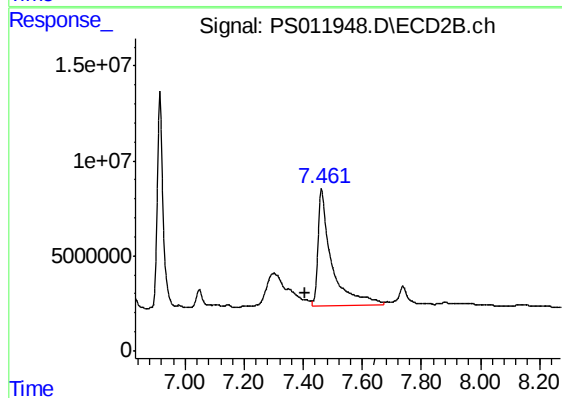

#7 MCPA


R.T.: 7.462 min
Delta R.T.: 0.057 min
Response: 199327758
Conc: 72.74 ug/ml

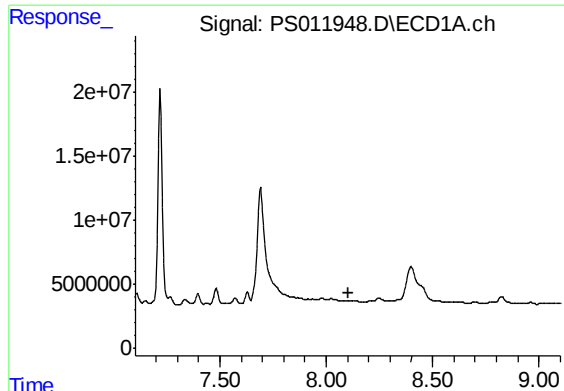

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RO-24

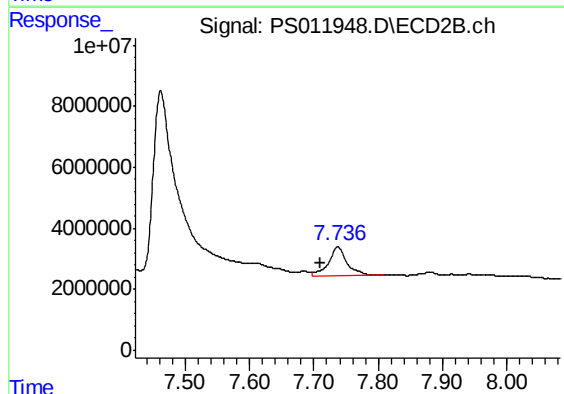


#8 DICHLORPROP

R.T.: 7.737 min
Delta R.T.: 0.028 min
Response: 19343895
Conc: 34.26 ng/ml

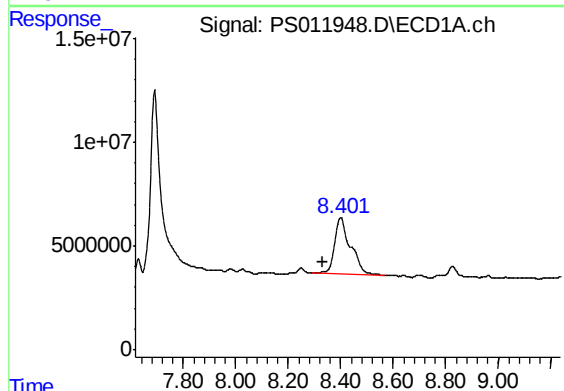


#9 2,4-D

R.T.: 8.400 min
Delta R.T.: 0.068 min
Response: 115375244
Conc: 102.18 ng/ml

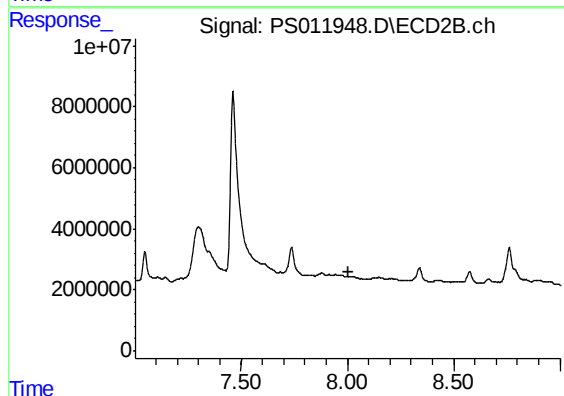

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 8.003 min
Response: 0
Conc: N.D.

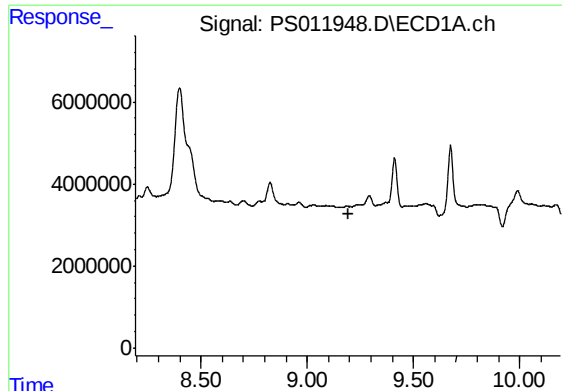

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RO-24

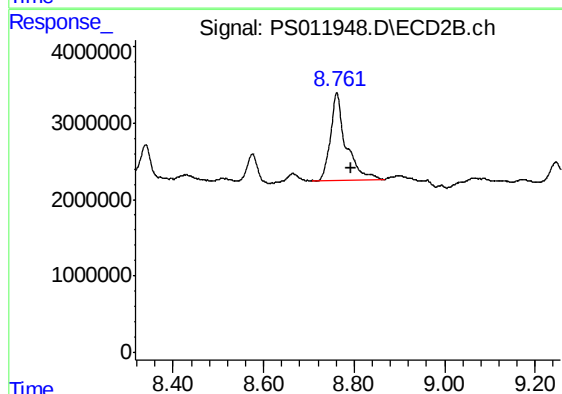


#11 2,4,5-TP (SILVEX)

R.T.: 8.762 min
Delta R.T.: -0.032 min
Response: 27088191
Conc: 9.27 ng/ml

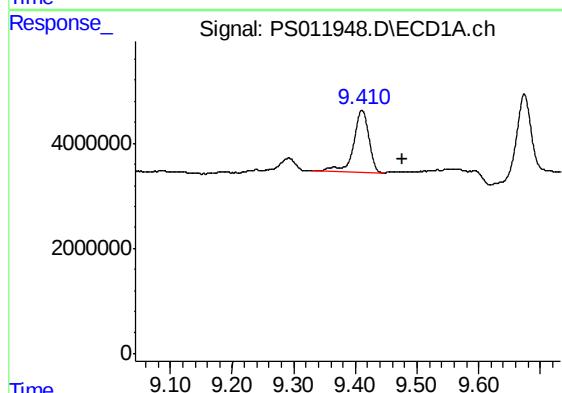

#12 2,4,5-T

R.T.: 9.411 min
Delta R.T.: -0.065 min
Response: 20534689
Conc: 3.47 ng/ml

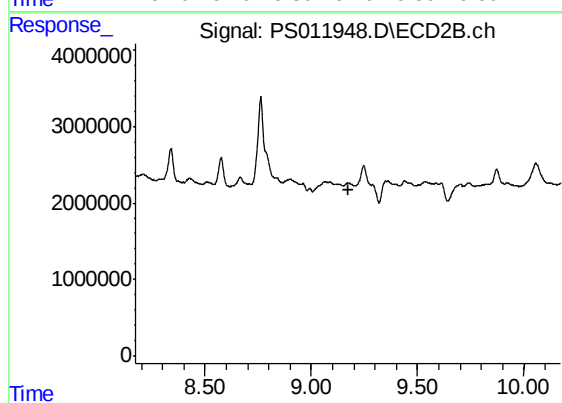

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.