

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082620\
 Data File : PS011949.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Aug 2020 22:31
 Operator : DD\AJ
 Sample : L3784-14
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 RO-06

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 02:13:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.915	209.8E6	146.3E6	192.331	273.657 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	93903987	N.D.	114.152
3) T	4-Nitroph...	7.056	6.506	4435576	15892487	7.530	43.588 #
5) T	DICAMBA	7.396	7.048	9178389	13002321	2.241	6.018 #
6) T	MCPD	7.629	0.000	8520463	0	2.667	N.D. #
7) T	MCPA	7.691	7.463	257.4E6	186.9E6	56.595	68.204
8) T	DICHLORPROP	0.000	7.738	0	21473273	N.D.	38.030
9) T	2,4-D	8.397	0.000	108.8E6	0	96.323	N.D. #
11) T	2,4,5-TP ...	0.000	8.762	0	25769312	N.D.	8.814
12) T	2,4,5-T	9.411	0.000	19105257	0	3.224	N.D. #
15) T	Picloram	11.006	0.000	9606945	0	1.229	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082620\
Data File : PS011949.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2020 22:31
Operator : DD\AJ
Sample : L3784-14
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
RO-06

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 02:13:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

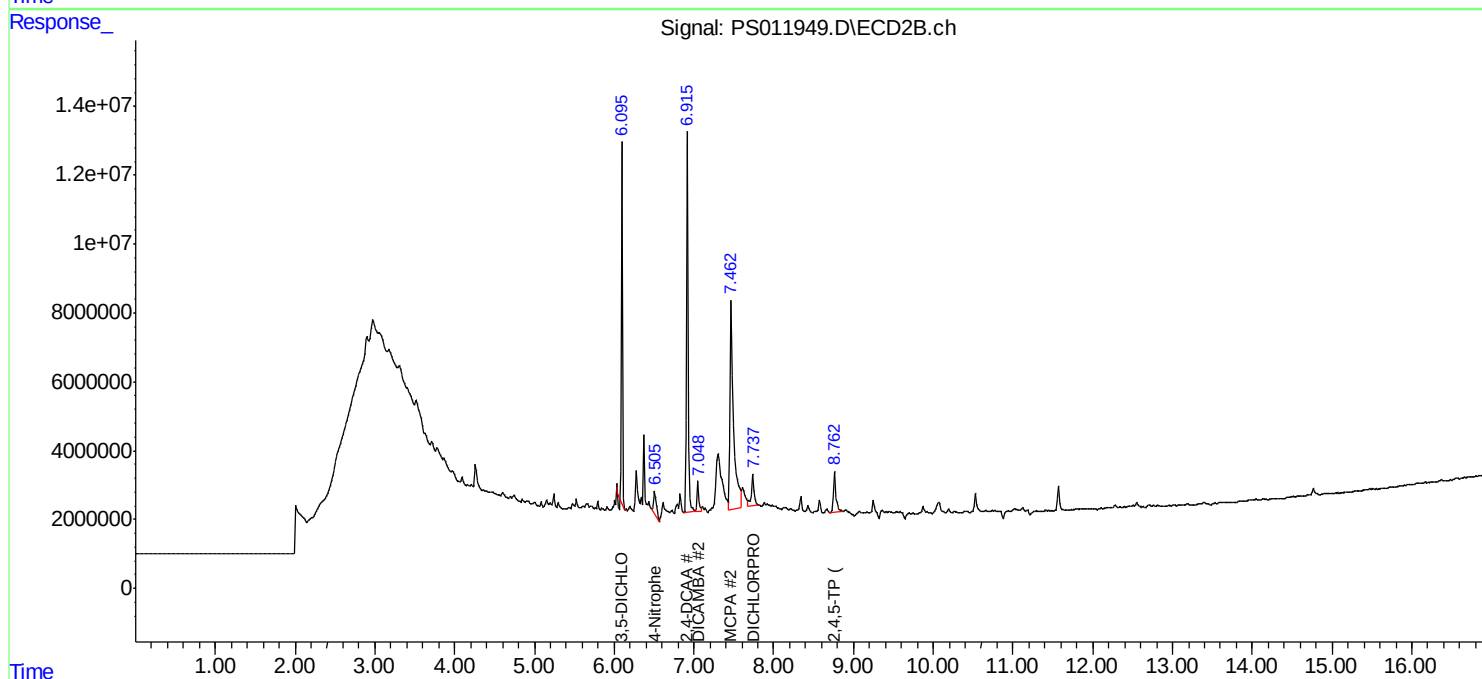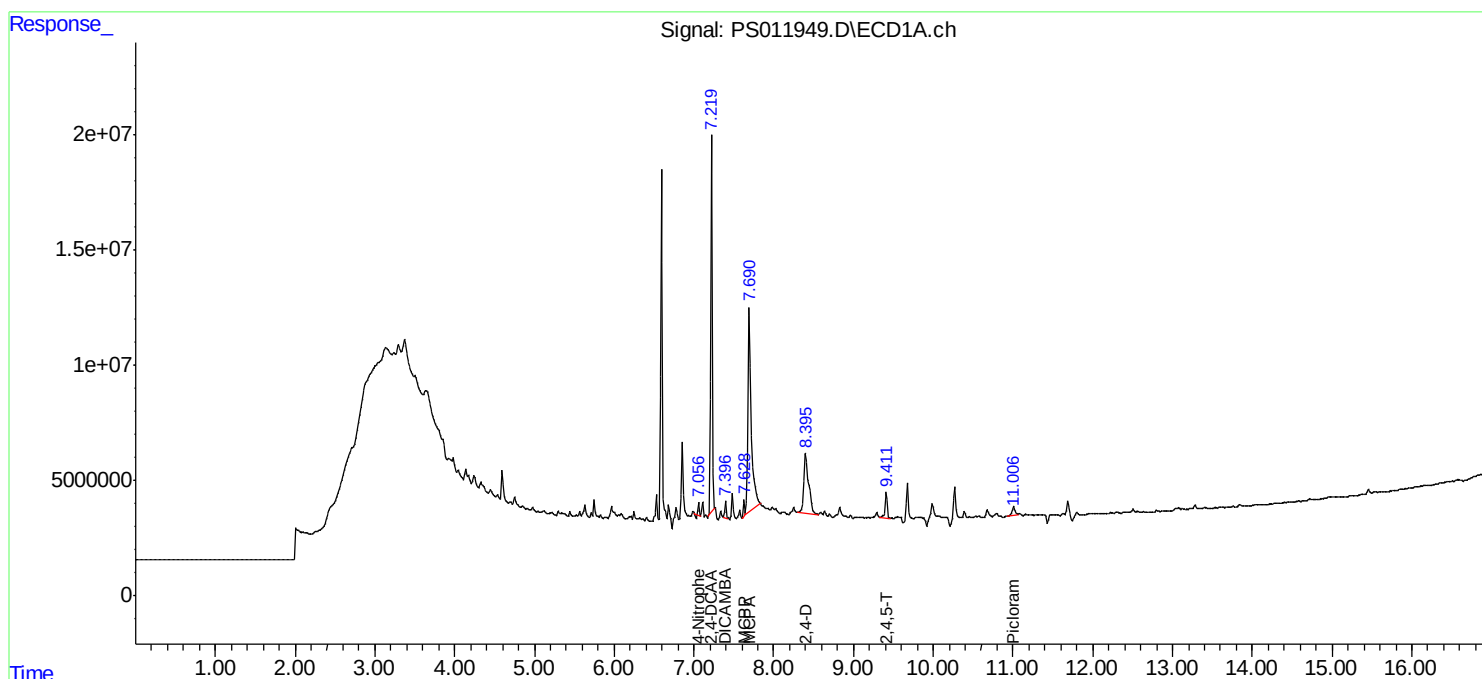


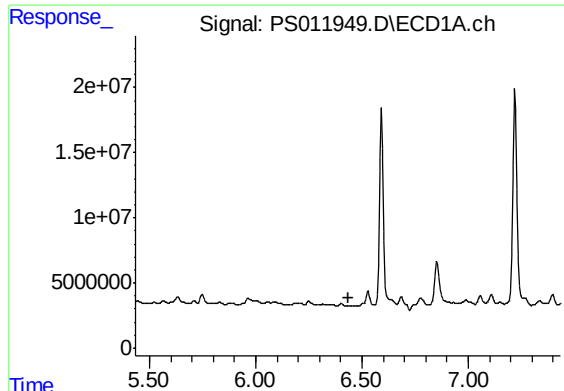

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RO-06

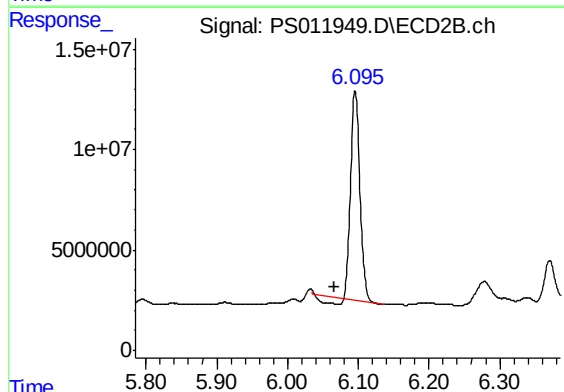


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.029 min
Response: 93903987
Conc: 114.15 ng/ml

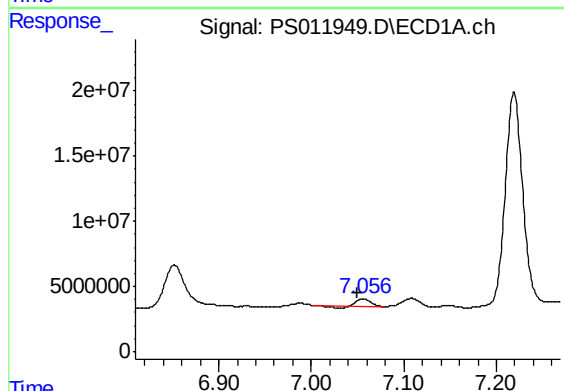


#3 4-Nitrophenol

R.T.: 7.056 min
Delta R.T.: 0.006 min
Response: 4435576
Conc: 7.53 ng/ml

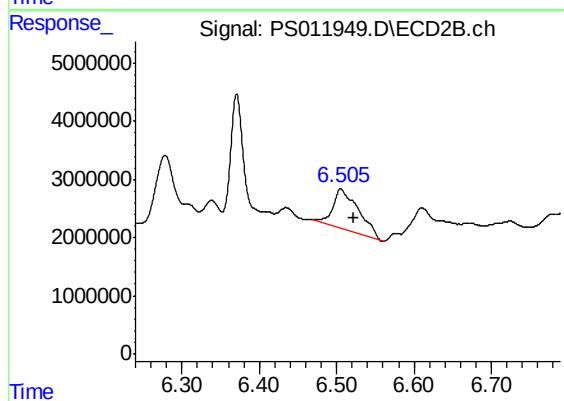

#3 4-Nitrophenol


R.T.: 6.506 min
Delta R.T.: -0.015 min
Response: 15892487
Conc: 43.59 ng/ml

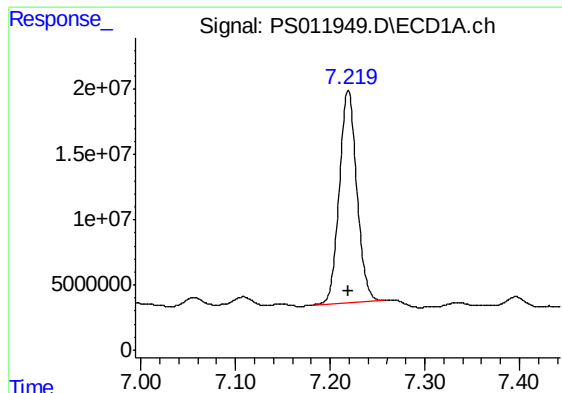

#4 2,4-DCAA


R.T.: 7.219 min
Delta R.T.: 0.000 min
Response: 209788955
Conc: 192.33 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-06

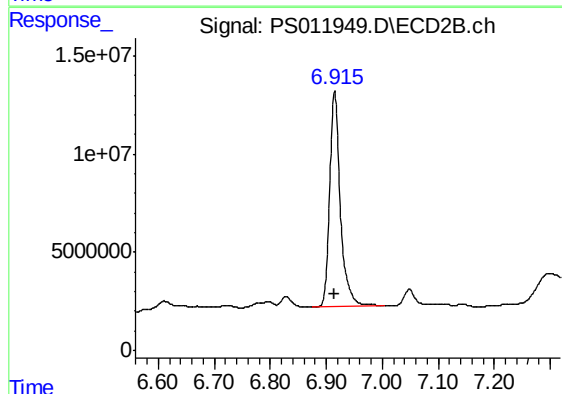


#4 2,4-DCAA

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 146348377
Conc: 273.66 ng/ml

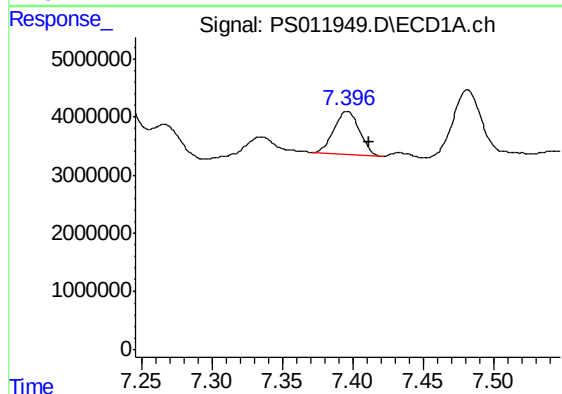


#5 DICAMBA

R.T.: 7.396 min
Delta R.T.: -0.015 min
Response: 9178389
Conc: 2.24 ng/ml

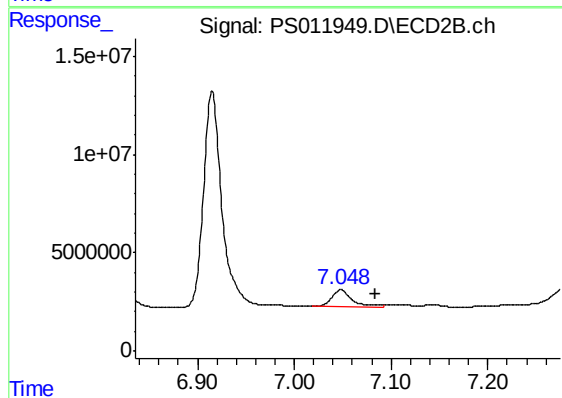

#5 DICAMBA


R.T.: 7.048 min
Delta R.T.: -0.036 min
Response: 13002321
Conc: 6.02 ng/ml

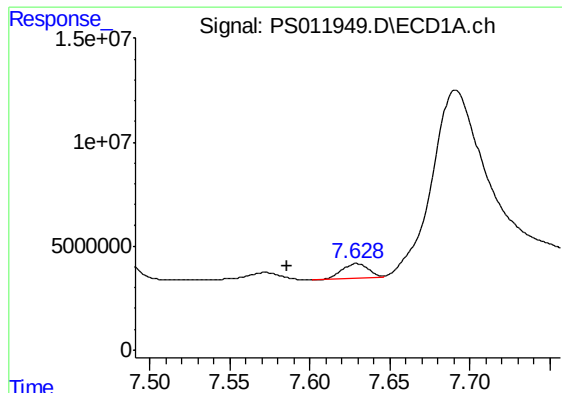

#6 MCPP


R.T.: 7.629 min
Delta R.T.: 0.043 min
Response: 8520463
Conc: 2.67 ug/ml

Instrument :
ECD_S
ClientSampleId :
RO-06

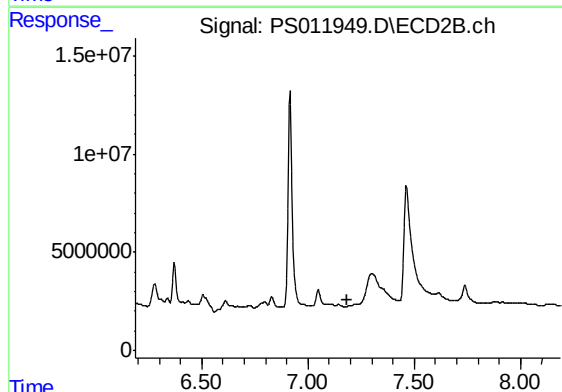


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

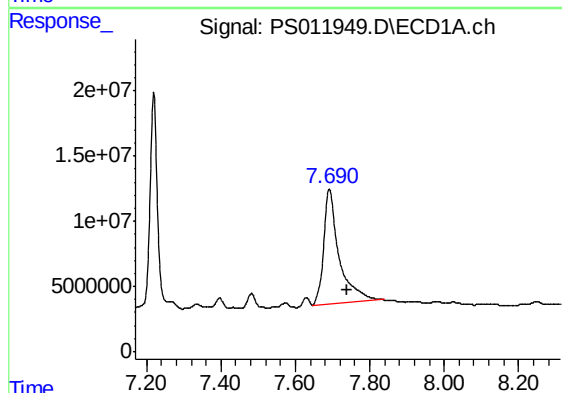


#7 MCPA

R.T.: 7.691 min
Delta R.T.: -0.047 min
Response: 257421975
Conc: 56.60 ug/ml

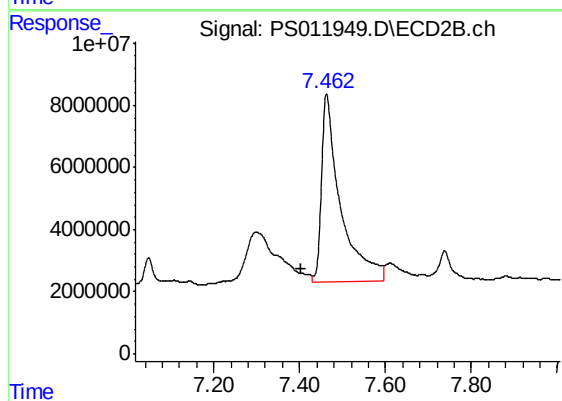

#7 MCPA


R.T.: 7.463 min
Delta R.T.: 0.058 min
Response: 186888135
Conc: 68.20 ug/ml

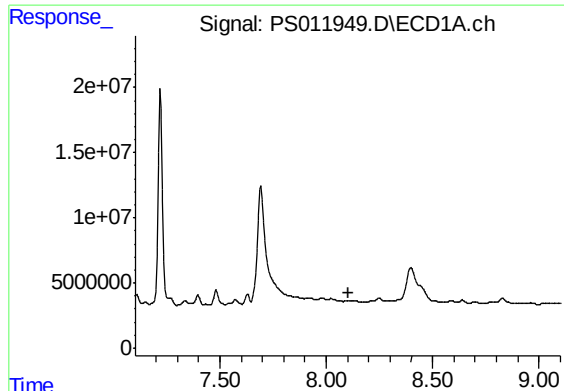

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RO-06

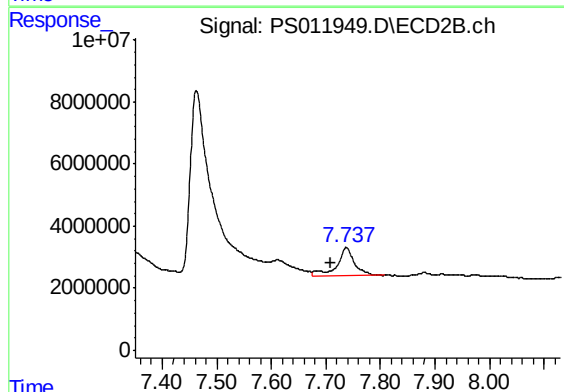


#8 DICHLORPROP

R.T.: 7.738 min
Delta R.T.: 0.028 min
Response: 21473273
Conc: 38.03 ng/ml

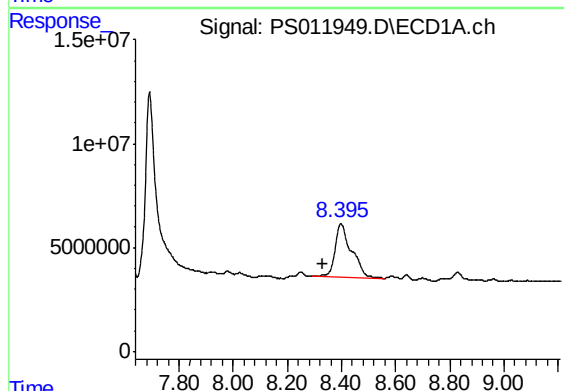


#9 2,4-D

R.T.: 8.397 min
Delta R.T.: 0.065 min
Response: 108757968
Conc: 96.32 ng/ml

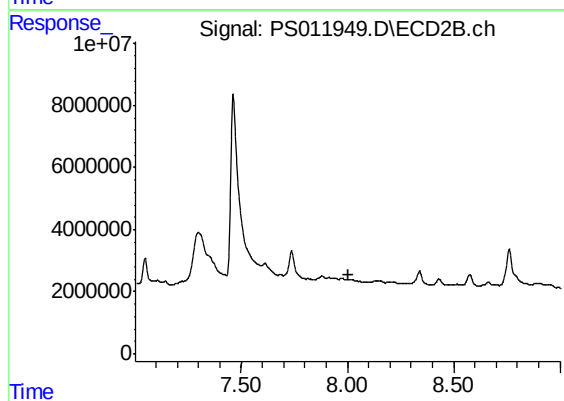

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 8.003 min
Response: 0
Conc: N.D.

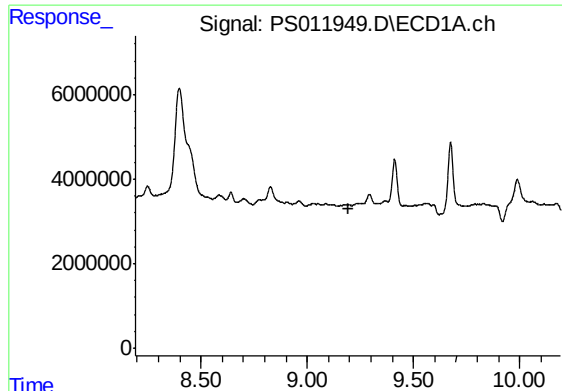

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RO-06

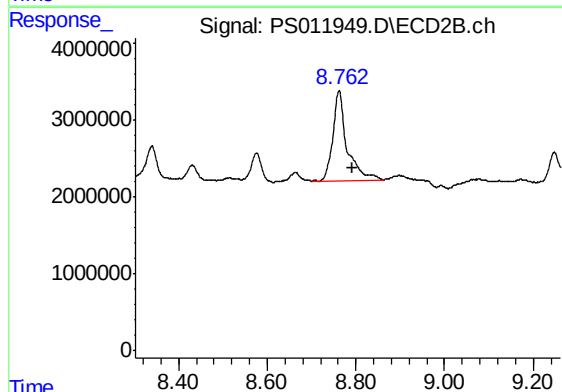


#11 2,4,5-TP (SILVEX)

R.T.: 8.762 min
Delta R.T.: -0.031 min
Response: 25769312
Conc: 8.81 ng/ml

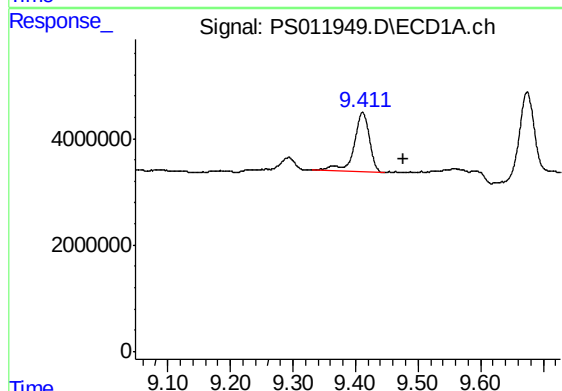


#12 2,4,5-T

R.T.: 9.411 min
Delta R.T.: -0.064 min
Response: 19105257
Conc: 3.22 ng/ml

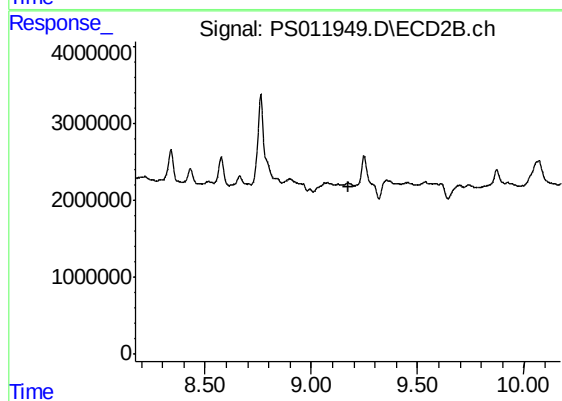

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.

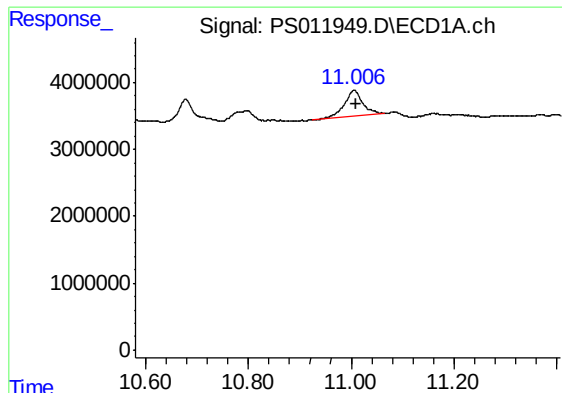

#15 Picloram

R.T.: 11.006 min
Delta R.T.: -0.004 min
Response: 9606945
Conc: 1.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-06

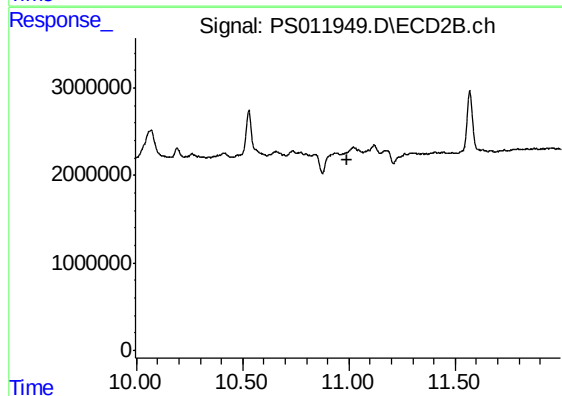

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.