

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082620\
 Data File : PS011950.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Aug 2020 22:54
 Operator : DD\AJ
 Sample : L3784-17
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 RO-04

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 02:13:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.915	214.8E6	143.8E6	196.960	268.893 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	99370799	N.D.	120.798
3) T	4-Nitroph...	7.056	6.506	3824728	16591503	6.493	45.505 #
5) T	DICAMBA	7.396	7.048	9327135	15003034	2.277	6.944 #
6) T	MCP	7.630	0.000	9288092	0	2.907	N.D. #
7) T	MCPA	7.690	7.462	268.4E6	198.7E6	59.016	72.496
8) T	DICHLORPROP	0.000	7.739	0	20720277	N.D.	36.697
9) T	2,4-D	8.398	0.000	105.9E6	0	93.787	N.D. #
11) T	2,4,5-TP ...	0.000	8.762	0	22044224	N.D.	7.540
12) T	2,4,5-T	9.412	0.000	19867919	0	3.353	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082620\
Data File : PS011950.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2020 22:54
Operator : DD\AJ
Sample : L3784-17
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
RO-04

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 02:13:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

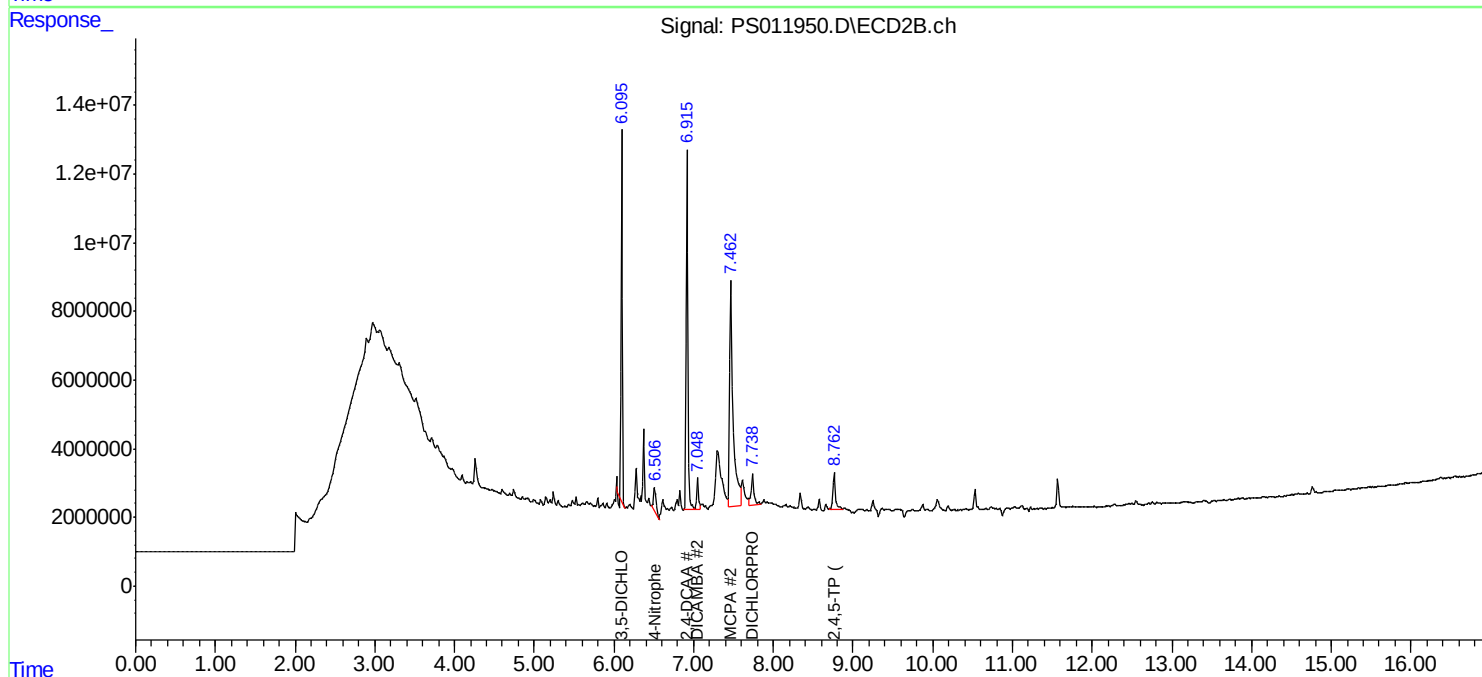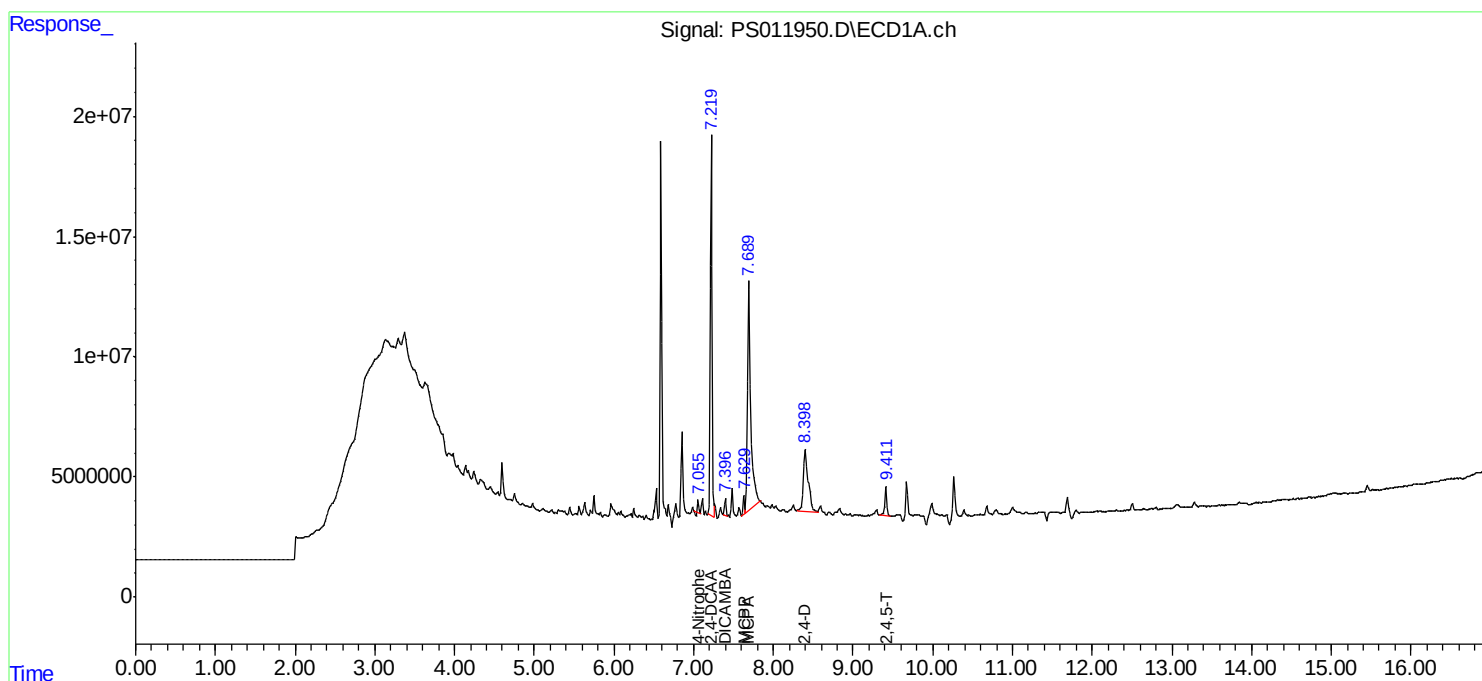


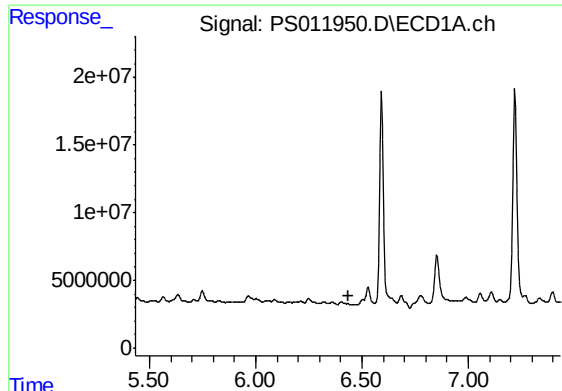

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RO-04

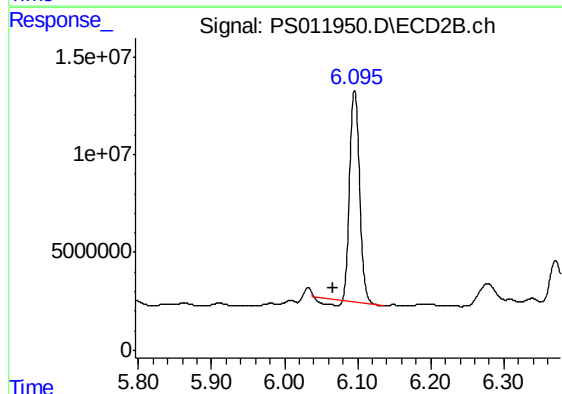


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.029 min
Response: 99370799
Conc: 120.80 ng/ml

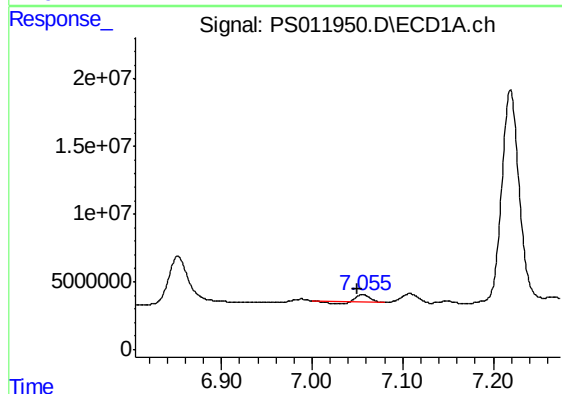


#3 4-Nitrophenol

R.T.: 7.056 min
Delta R.T.: 0.006 min
Response: 3824728
Conc: 6.49 ng/ml

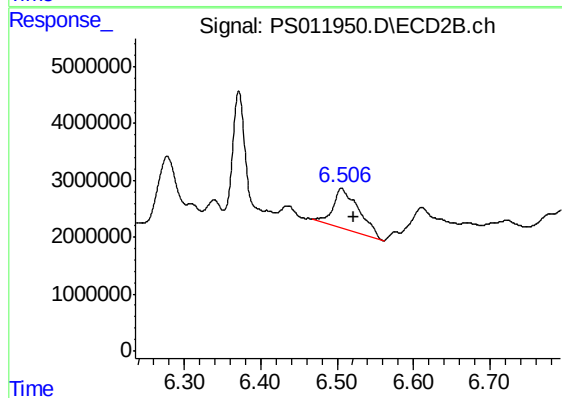

#3 4-Nitrophenol


R.T.: 6.506 min
Delta R.T.: -0.016 min
Response: 16591503
Conc: 45.50 ng/ml

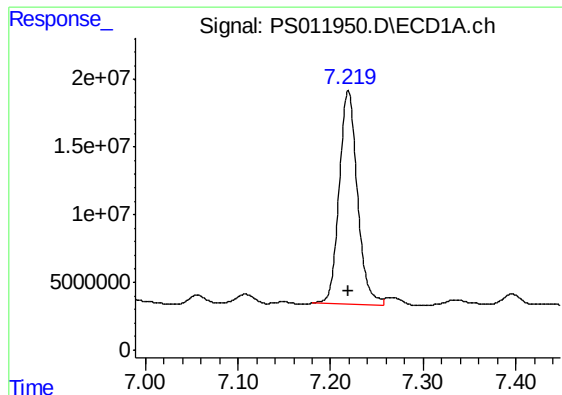

#4 2,4-DCAA


R.T.: 7.219 min
Delta R.T.: 0.000 min
Response: 214838010
Conc: 196.96 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-04

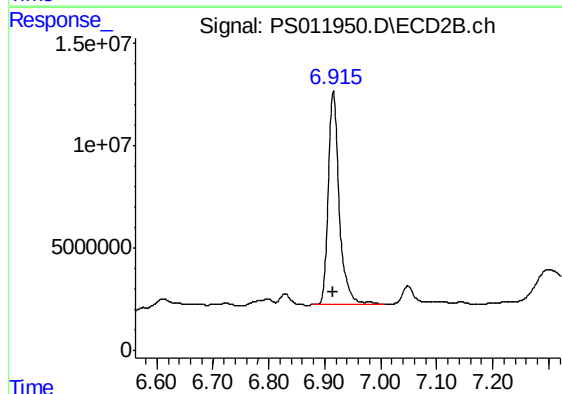


#4 2,4-DCAA

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 143800664
Conc: 268.89 ng/ml

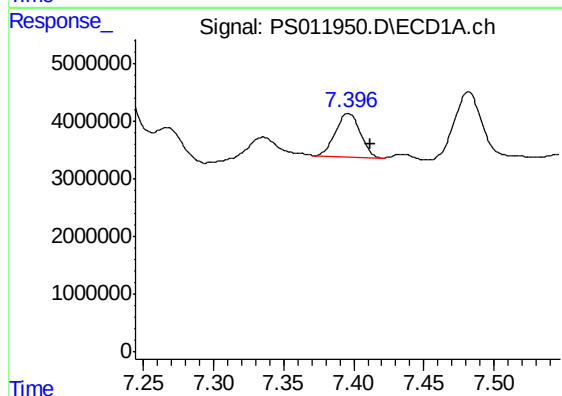


#5 DICAMBA

R.T.: 7.396 min
Delta R.T.: -0.015 min
Response: 9327135
Conc: 2.28 ng/ml

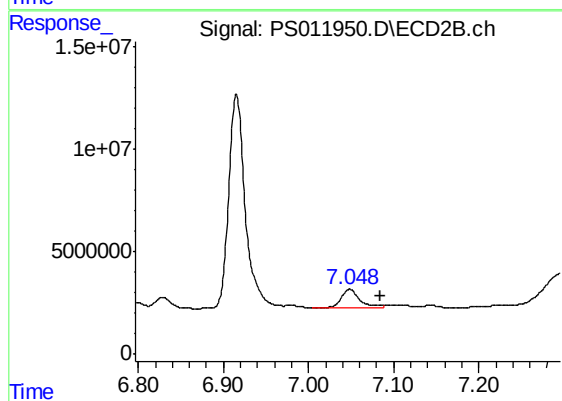

#5 DICAMBA


R.T.: 7.048 min
Delta R.T.: -0.036 min
Response: 15003034
Conc: 6.94 ng/ml

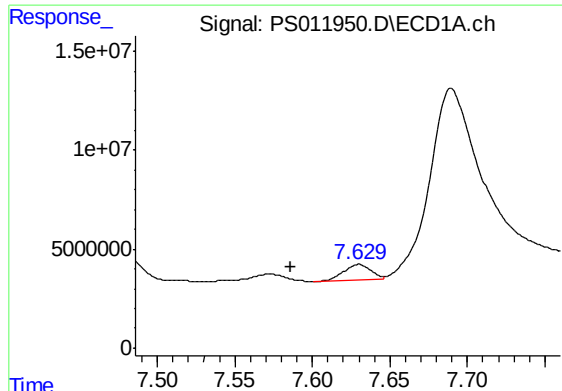

#6 MCPP


R.T.: 7.630 min
Delta R.T.: 0.044 min
Response: 9288092
Conc: 2.91 ug/ml

Instrument :
ECD_S
ClientSampleId :
RO-04

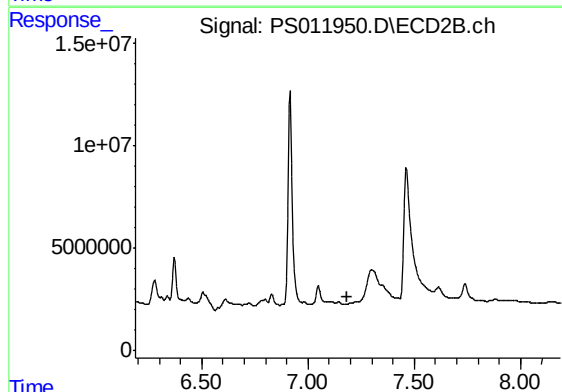


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

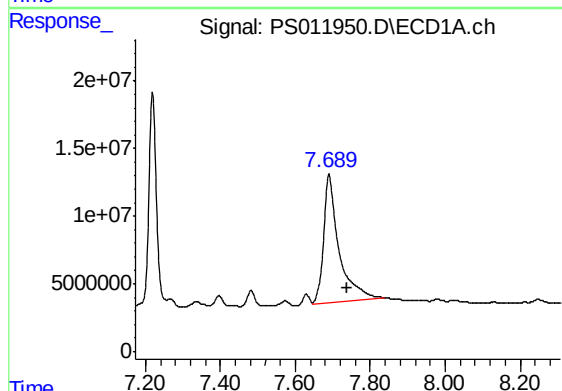


#7 MCPA

R.T.: 7.690 min
Delta R.T.: -0.048 min
Response: 268434346
Conc: 59.02 ug/ml

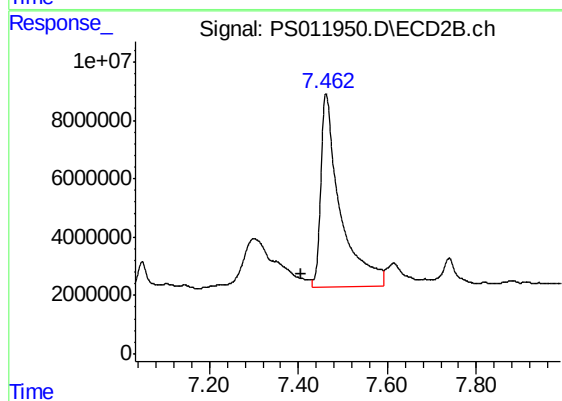

#7 MCPA


R.T.: 7.462 min
Delta R.T.: 0.057 min
Response: 198650260
Conc: 72.50 ug/ml

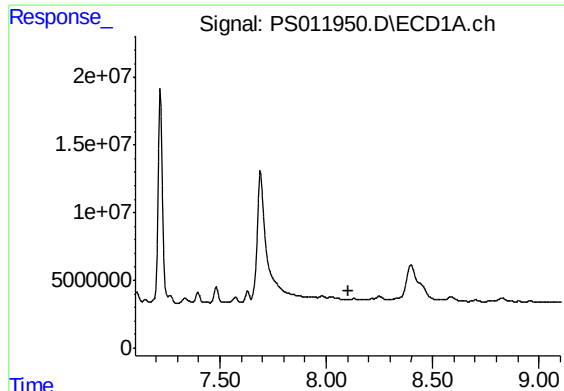

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RO-04

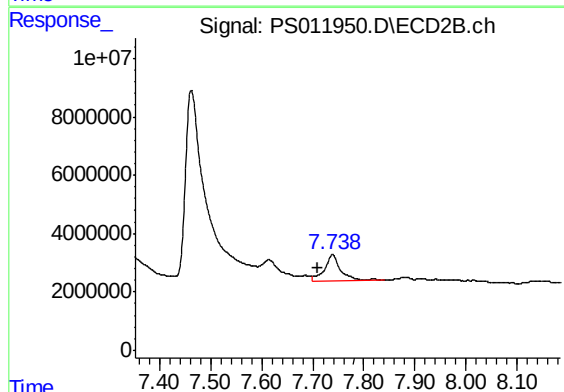


#8 DICHLORPROP

R.T.: 7.739 min
Delta R.T.: 0.029 min
Response: 20720277
Conc: 36.70 ng/ml

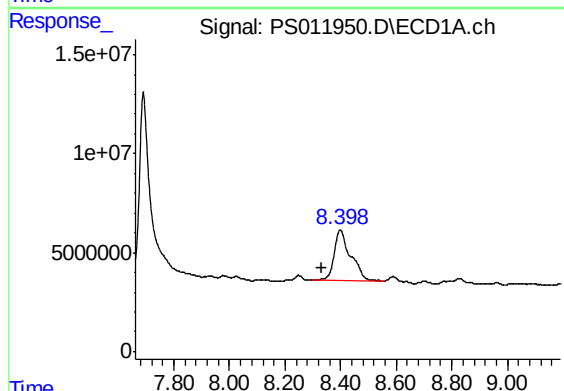


#9 2,4-D

R.T.: 8.398 min
Delta R.T.: 0.066 min
Response: 105894446
Conc: 93.79 ng/ml

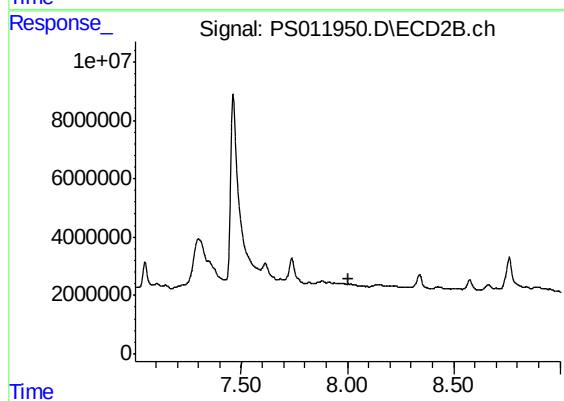

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 8.003 min
Response: 0
Conc: N.D.

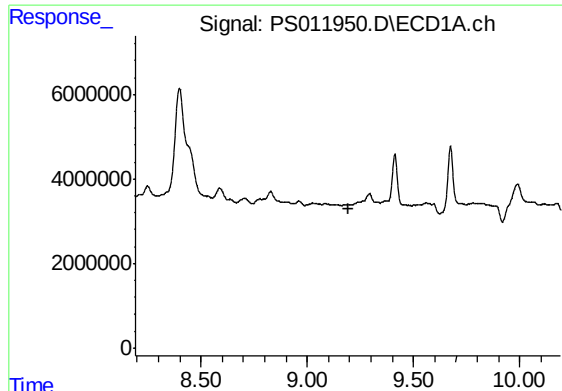

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RO-04

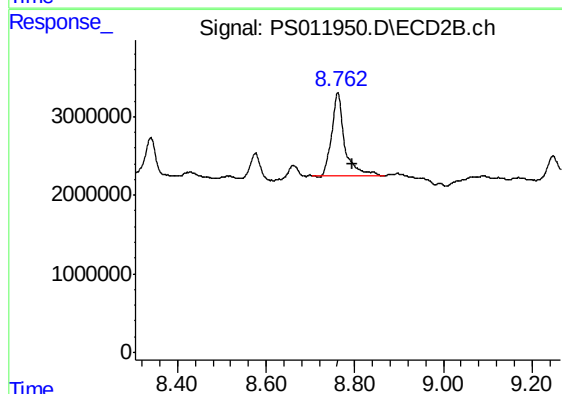


#11 2,4,5-TP (SILVEX)

R.T.: 8.762 min
Delta R.T.: -0.032 min
Response: 22044224
Conc: 7.54 ng/ml

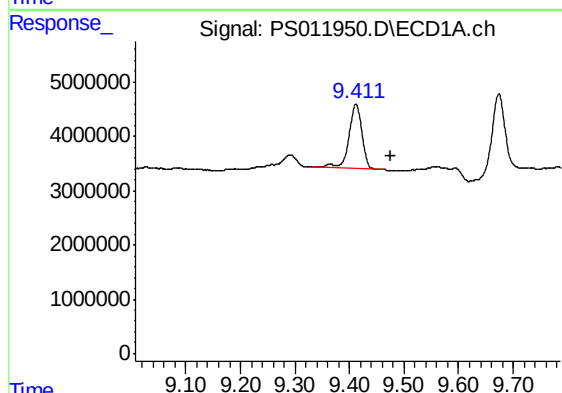

#12 2,4,5-T

R.T.: 9.412 min
Delta R.T.: -0.064 min
Response: 19867919
Conc: 3.35 ng/ml

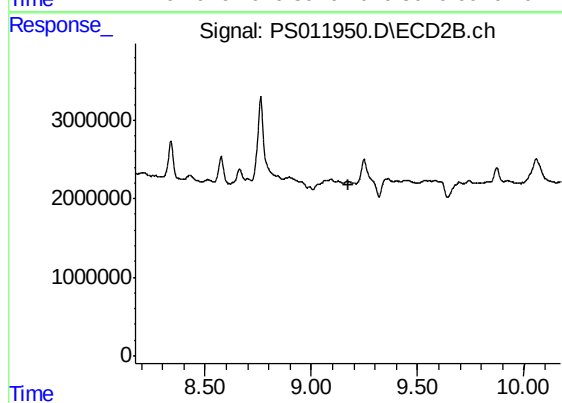

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.