

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082620\
 Data File : PS011951.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Aug 2020 23:17
 Operator : DD\AJ
 Sample : L3785-02
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CHRT-09

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 02:13:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.218	6.915	286.2E6	177.0E6	262.422	330.982 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	105.3E6	N.D.	127.953
3) T	4-Nitroph...	7.056	6.506	5516308	16251082	9.365	44.571 #
5) T	DICAMBA	7.396	7.048	10036893	14272186	2.450	6.606 #
6) T	MCP	7.629	0.000	10825307	0	3.388	N.D. #
7) T	MCPA	7.691	7.463	233.3E6	169.3E6	51.300	61.794
8) T	DICHLORPROP	0.000	7.738	0	20233679	N.D.	35.835
9) T	2,4-D	8.399	0.000	109.7E6	0	97.153	N.D. #
11) T	2,4,5-TP ...	0.000	8.762	0	20422783	N.D.	6.985
12) T	2,4,5-T	9.411	0.000	18602670	0	3.139	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082620\
Data File : PS011951.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2020 23:17
Operator : DD\AJ
Sample : L3785-02
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CHRT-09

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 02:13:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

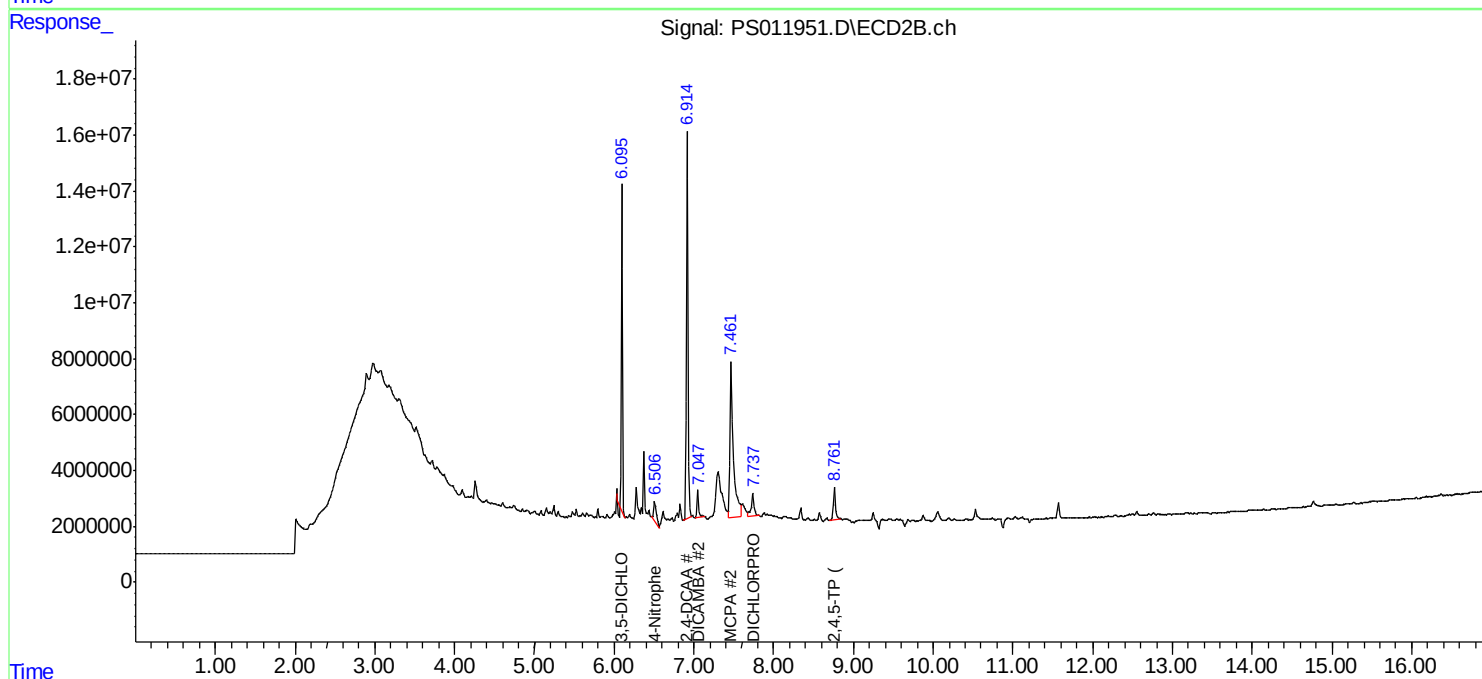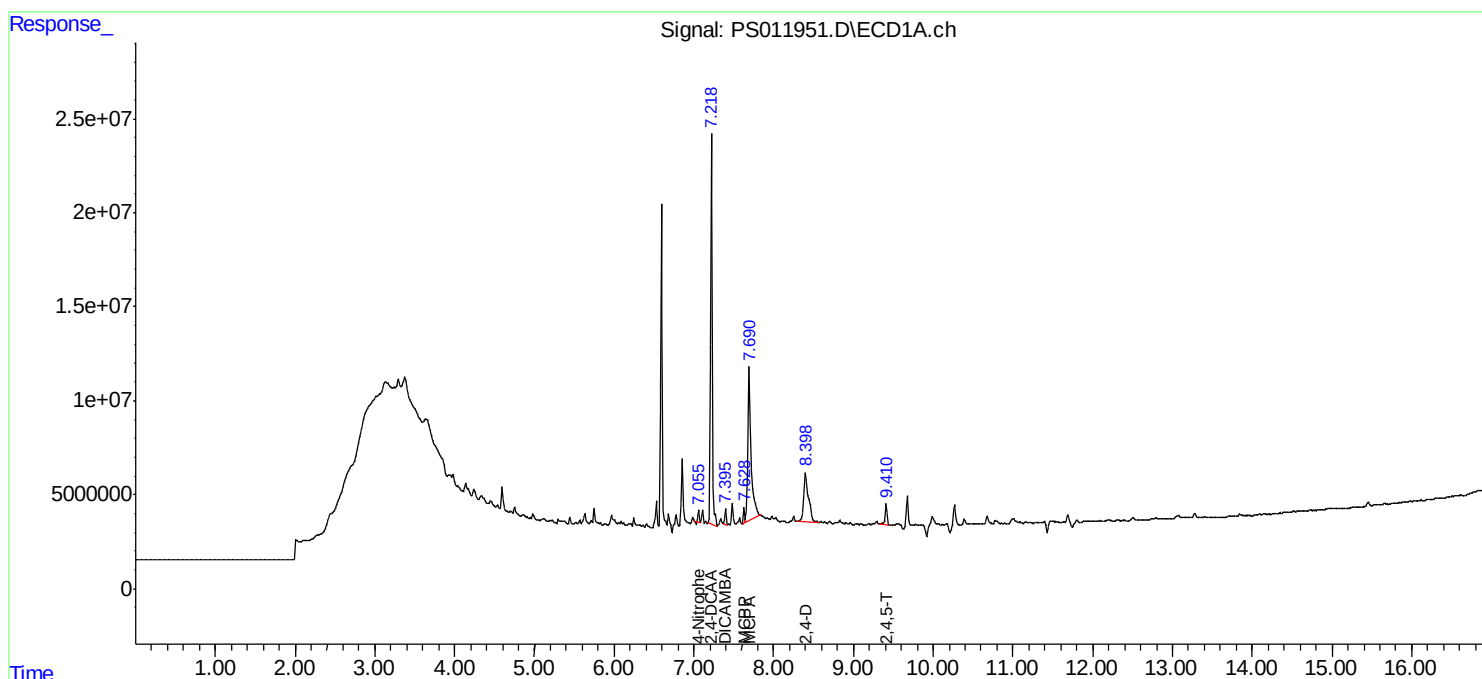


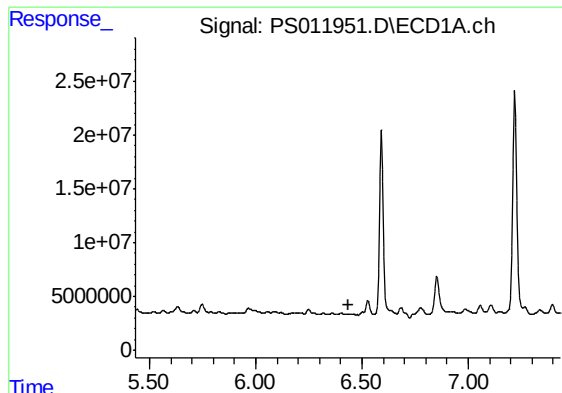

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CHRT-09

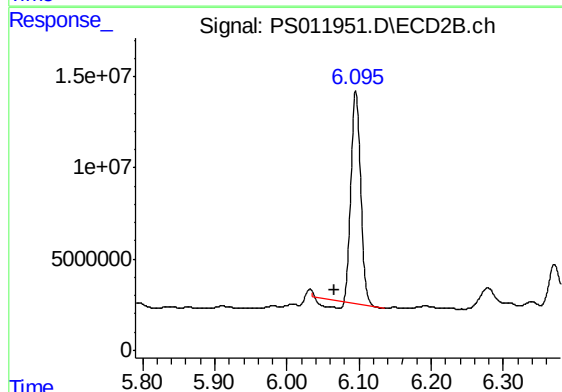


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.029 min
Response: 105256477
Conc: 127.95 ng/ml

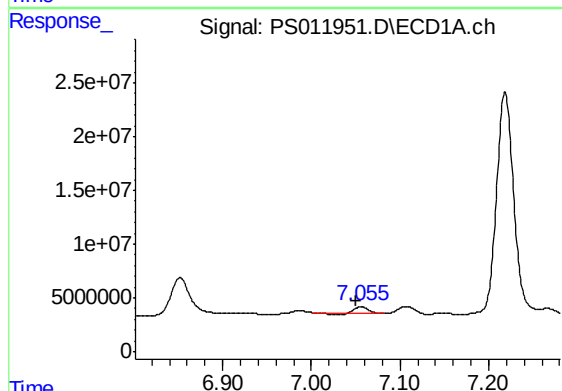


#3 4-Nitrophenol

R.T.: 7.056 min
Delta R.T.: 0.006 min
Response: 5516308
Conc: 9.36 ng/ml

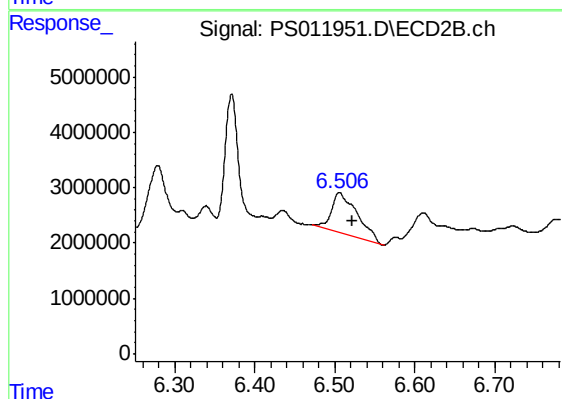

#3 4-Nitrophenol


R.T.: 6.506 min
Delta R.T.: -0.015 min
Response: 16251082
Conc: 44.57 ng/ml

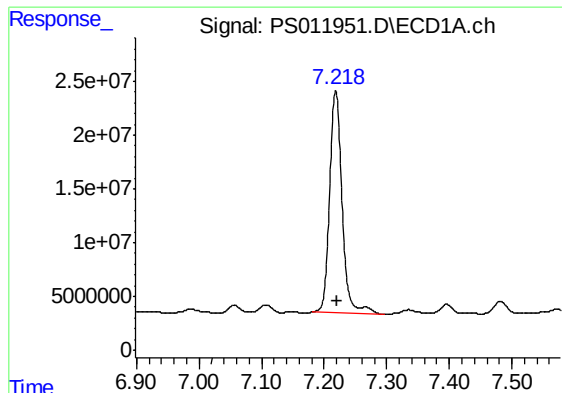

#4 2,4-DCAA


R.T.: 7.218 min
Delta R.T.: -0.002 min
Response: 286241254
Conc: 262.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
CHRT-09

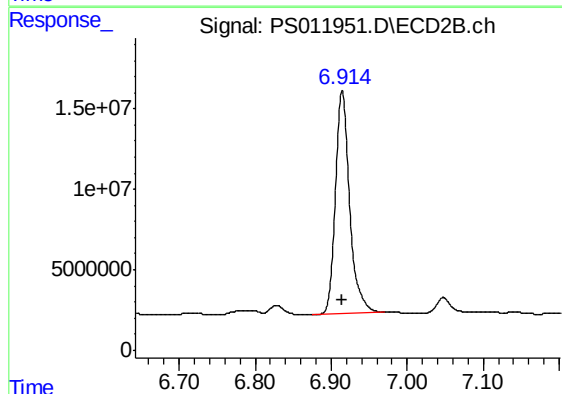


#4 2,4-DCAA

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 177004783
Conc: 330.98 ng/ml

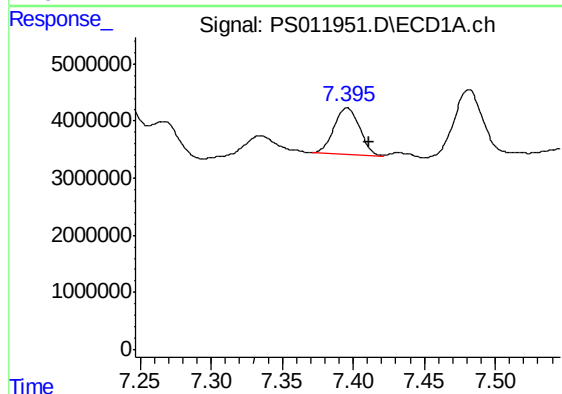


#5 DICAMBA

R.T.: 7.396 min
Delta R.T.: -0.016 min
Response: 10036893
Conc: 2.45 ng/ml

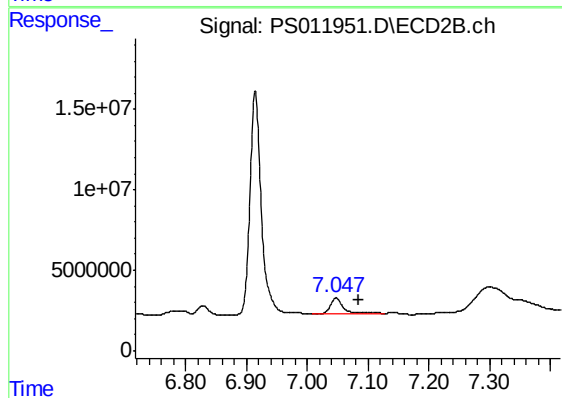

#5 DICAMBA


R.T.: 7.048 min
Delta R.T.: -0.036 min
Response: 14272186
Conc: 6.61 ng/ml

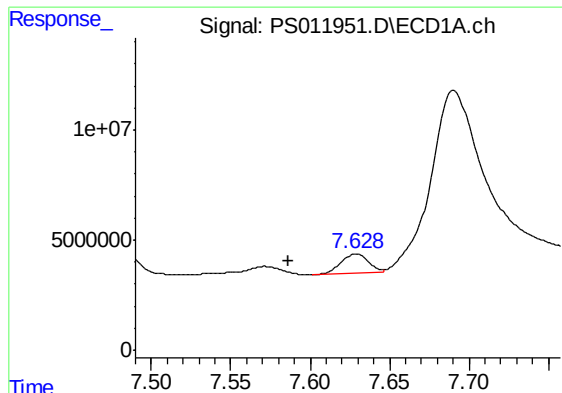

#6 MCPP


R.T.: 7.629 min
Delta R.T.: 0.043 min
Response: 10825307
Conc: 3.39 ug/ml

Instrument :
ECD_S
ClientSampleId :
CHRT-09

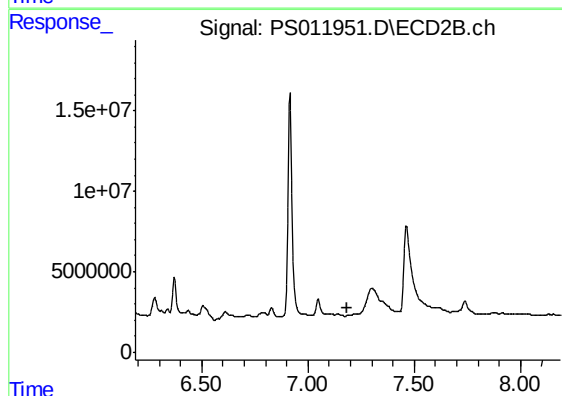


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

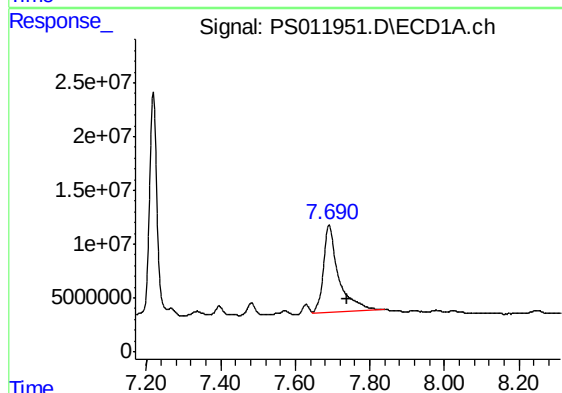


#7 MCPA

R.T.: 7.691 min
Delta R.T.: -0.048 min
Response: 233335272
Conc: 51.30 ug/ml

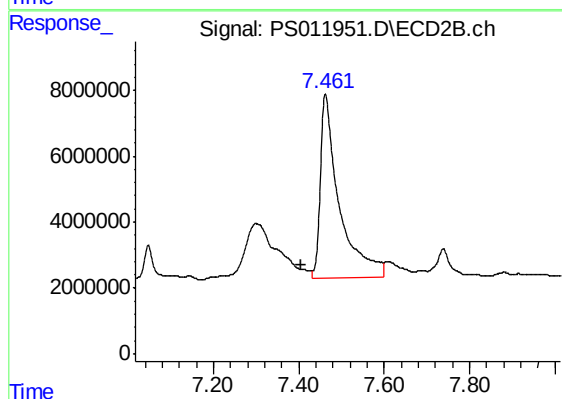

#7 MCPA


R.T.: 7.463 min
Delta R.T.: 0.058 min
Response: 169323207
Conc: 61.79 ug/ml

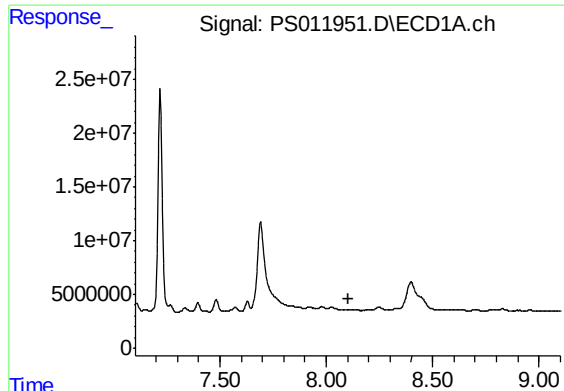

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CHRT-09

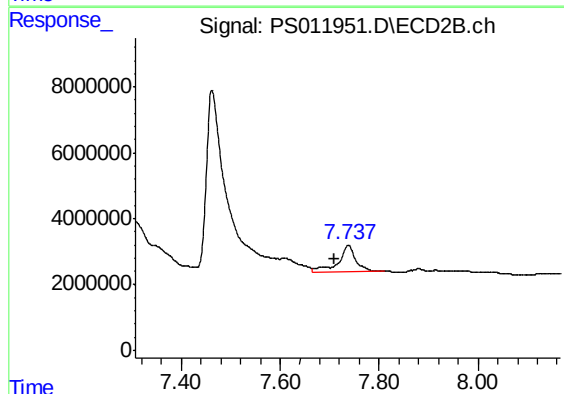


#8 DICHLORPROP

R.T.: 7.738 min
Delta R.T.: 0.029 min
Response: 20233679
Conc: 35.83 ng/ml

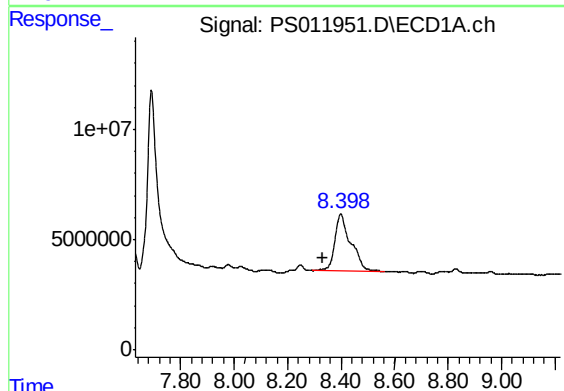


#9 2,4-D

R.T.: 8.399 min
Delta R.T.: 0.067 min
Response: 109695097
Conc: 97.15 ng/ml

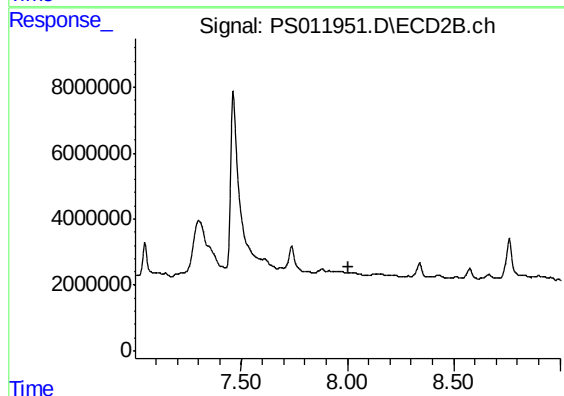

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 8.003 min
Response: 0
Conc: N.D.

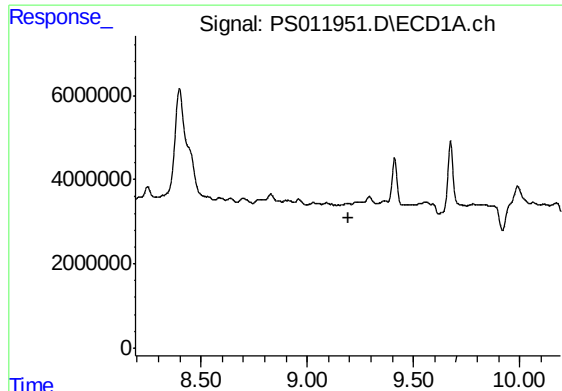

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CHRT-09

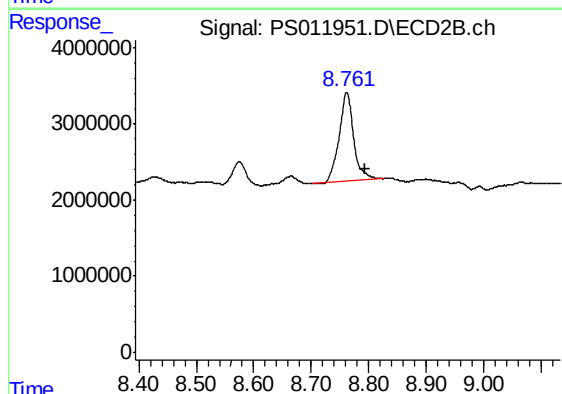


#11 2,4,5-TP (SILVEX)

R.T.: 8.762 min
Delta R.T.: -0.032 min
Response: 20422783
Conc: 6.99 ng/ml

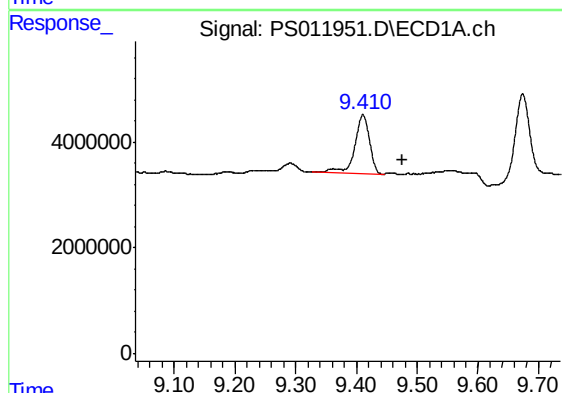

#12 2,4,5-T

R.T.: 9.411 min
Delta R.T.: -0.065 min
Response: 18602670
Conc: 3.14 ng/ml

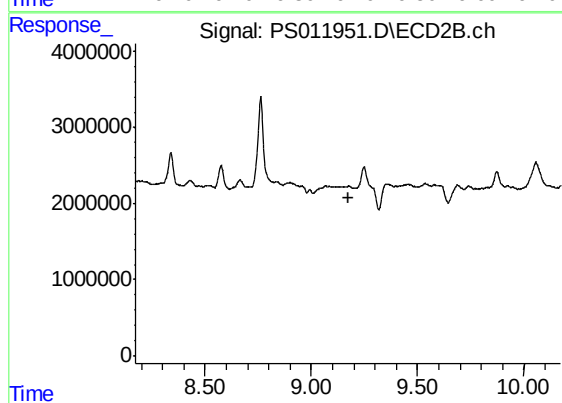

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.