

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082621\
 Data File : PS016722.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Aug 2021 20:20
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 01:03:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 02 14:10:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.182	6.764	644.8E6	271.1E6	438.281	519.657
Target Compounds							
8) T	DICHLORPROP	0.000	7.577	0	2929916	N.D.	5.408
11) T	2,4,5-TP ...	0.000	8.625	0	2279400	N.D.	<MDL
12) T	2,4,5-T	0.000	9.067f	0	3596776	N.D.	1.242
15) T	Picloram	10.995	10.828	23761155	13293761	2.381	3.301 #
16) T	DCPA	0.000	10.763	0	1661464	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082621\
Data File : PS016722.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2021 20:20
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 01:03:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
Quant Title : 8080.M
QLast Update : Mon Aug 02 14:10:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

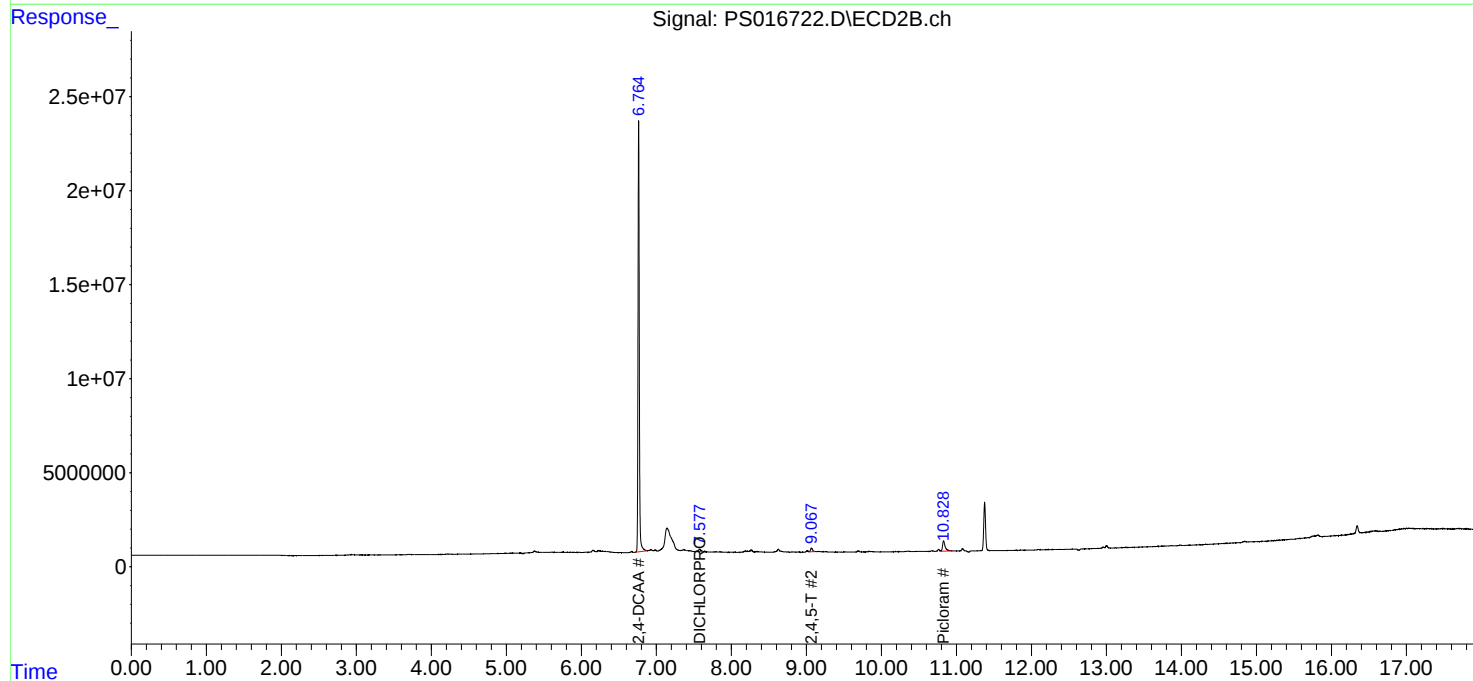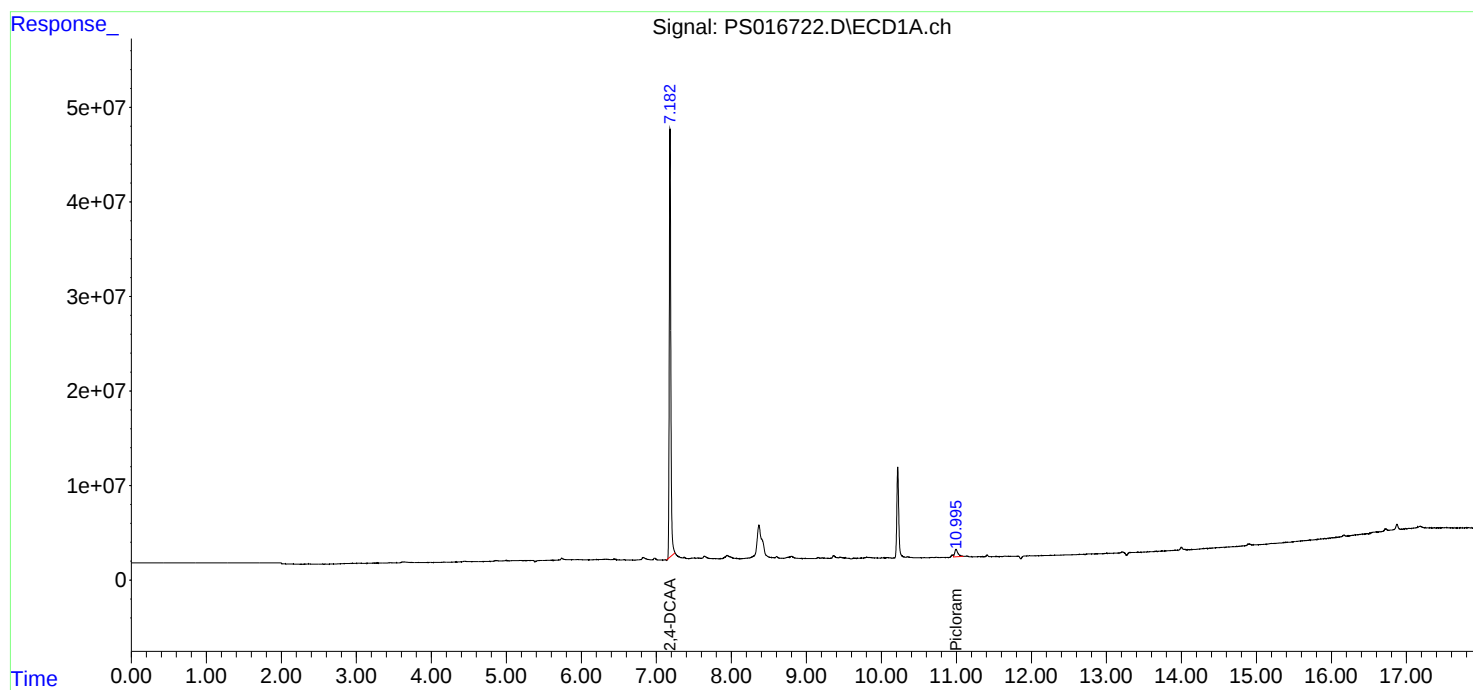


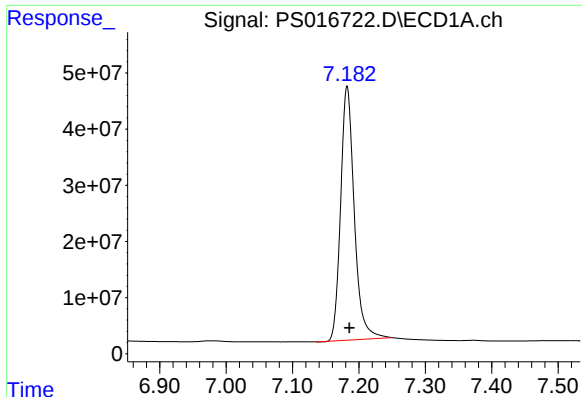

#4 2,4-DCAA


R.T.: 7.182 min
Delta R.T.: -0.003 min
Response: 644758813
Conc: 438.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

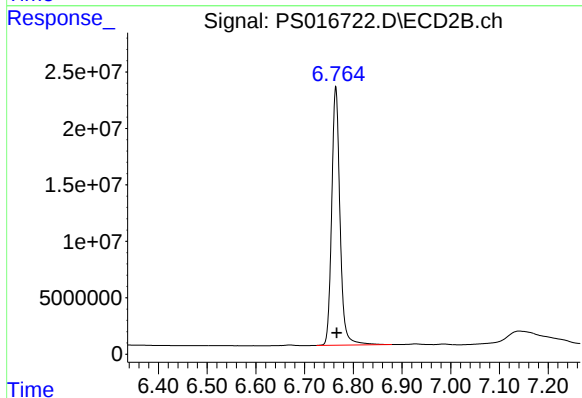


#4 2,4-DCAA

R.T.: 6.764 min
Delta R.T.: -0.002 min
Response: 271065694
Conc: 519.66 ng/ml

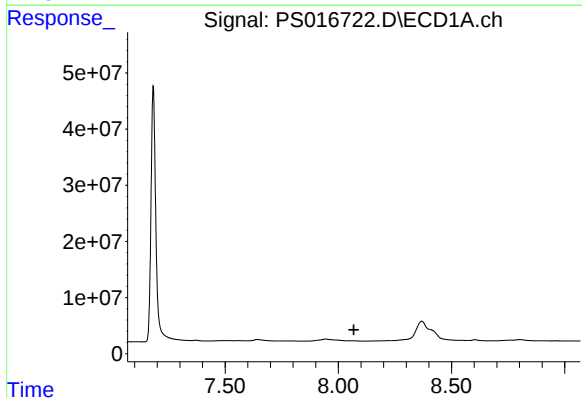


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.069 min
Response: 0
Conc: N.D.

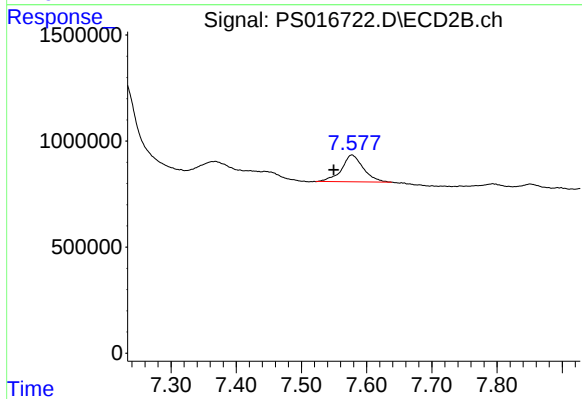

#8 DICHLORPROP


R.T.: 7.577 min
Delta R.T.: 0.028 min
Response: 2929916
Conc: 5.41 ng/ml

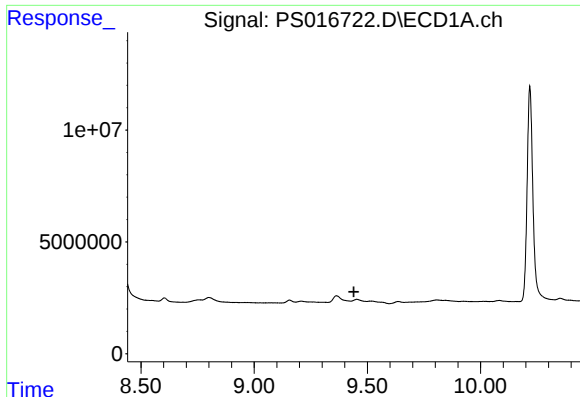

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.440 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

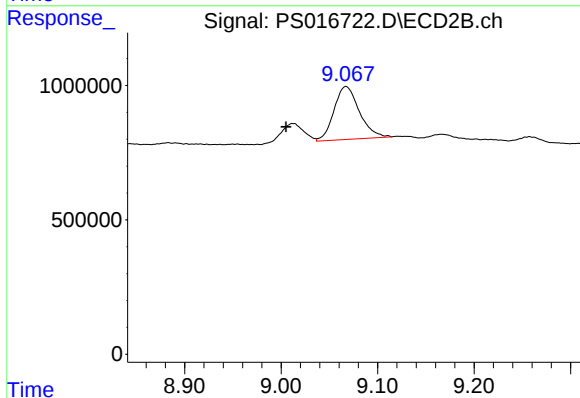


#12 2,4,5-T

R.T.: 9.067 min
Delta R.T.: 0.062 min
Response: 3596776
Conc: 1.24 ng/ml

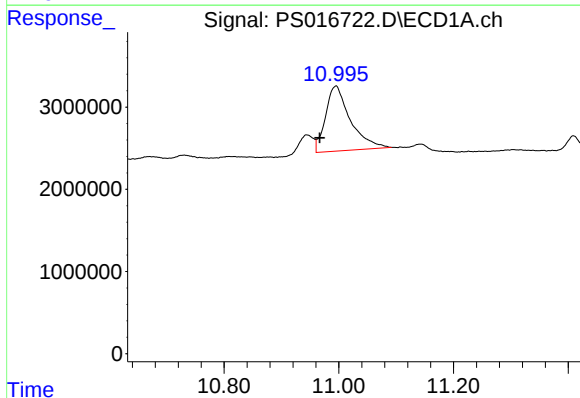

#15 Picloram

R.T.: 10.995 min
Delta R.T.: 0.028 min
Response: 23761155
Conc: 2.38 ng/ml

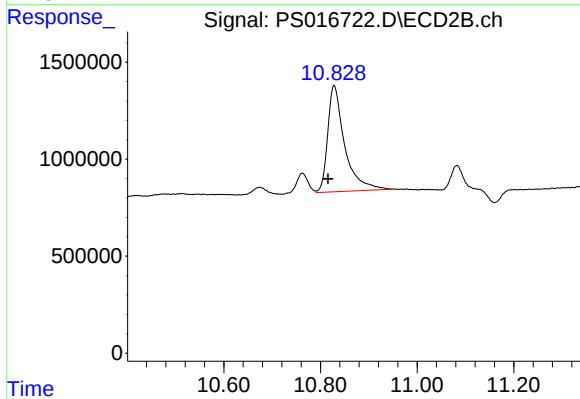

#15 Picloram

R.T.: 10.828 min
Delta R.T.: 0.013 min
Response: 13293761
Conc: 3.30 ng/ml