

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082625\
 Data File : PS031548.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Aug 2025 17:09
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 01:35:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
 Quant Title : 8080.M
 QLast Update : Fri Aug 08 03:17:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.287	7.744	1685.7E6	462.4E6	531.109	547.051
Target Compounds							
1) T	Dalapon	2.712f	2.669f	27355667	53262568	5.212	20.016 #
2) T	3,5-DICHL...	6.462	0.000	5059028	0	1.072	N.D. #
5) T	DICAMBA	7.473	7.943	9003463	3124736	<MDL	<MDL #
7) T	MCPA	7.823	0.000	141524	0	<MDL	N.D. #
8) T	DICHLORPROP	8.184	8.682	5050083	967109	1.592	<MDL #
10) T	Pentachlo...	8.712	9.514	43970379	34551635	<MDL	<MDL #
11) T	2,4,5-TP ...	9.296	9.907	19256339	14458318	1.074	1.102
12) T	2,4,5-T	9.610	10.374f	16170374	11699847	1.104	<MDL #
13) T	2,4-DB	10.177	10.896	1551677	3494935	<MDL	3.622 #
14) T	DINOSEB	11.360	11.273	28336452	5001281	2.235	<MDL #
15) T	Picloram	11.171f	0.000	2257814	0	<MDL	N.D. #
16) T	DCPA	11.659	0.000	17162853	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082625\
Data File : PS031548.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2025 17:09
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 01:35:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
Quant Title : 8080.M
QLast Update : Fri Aug 08 03:17:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

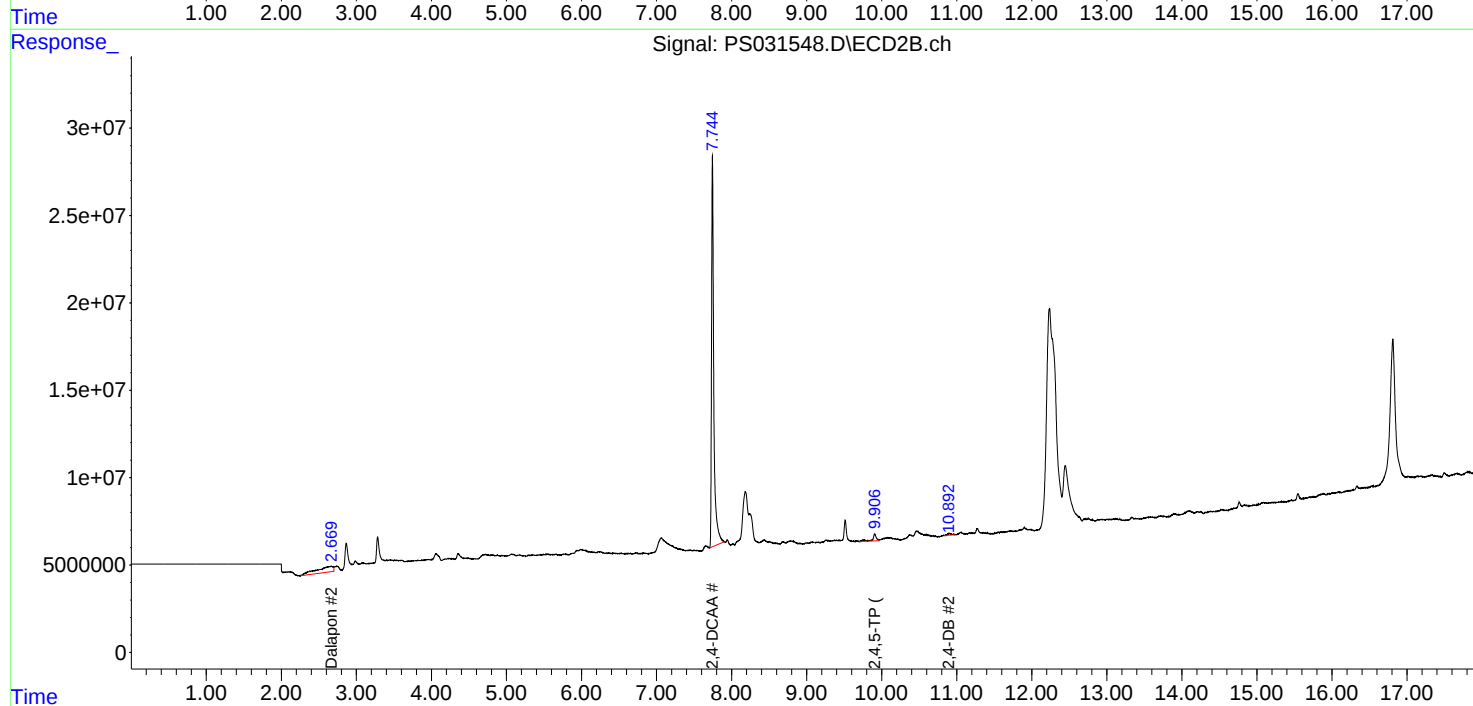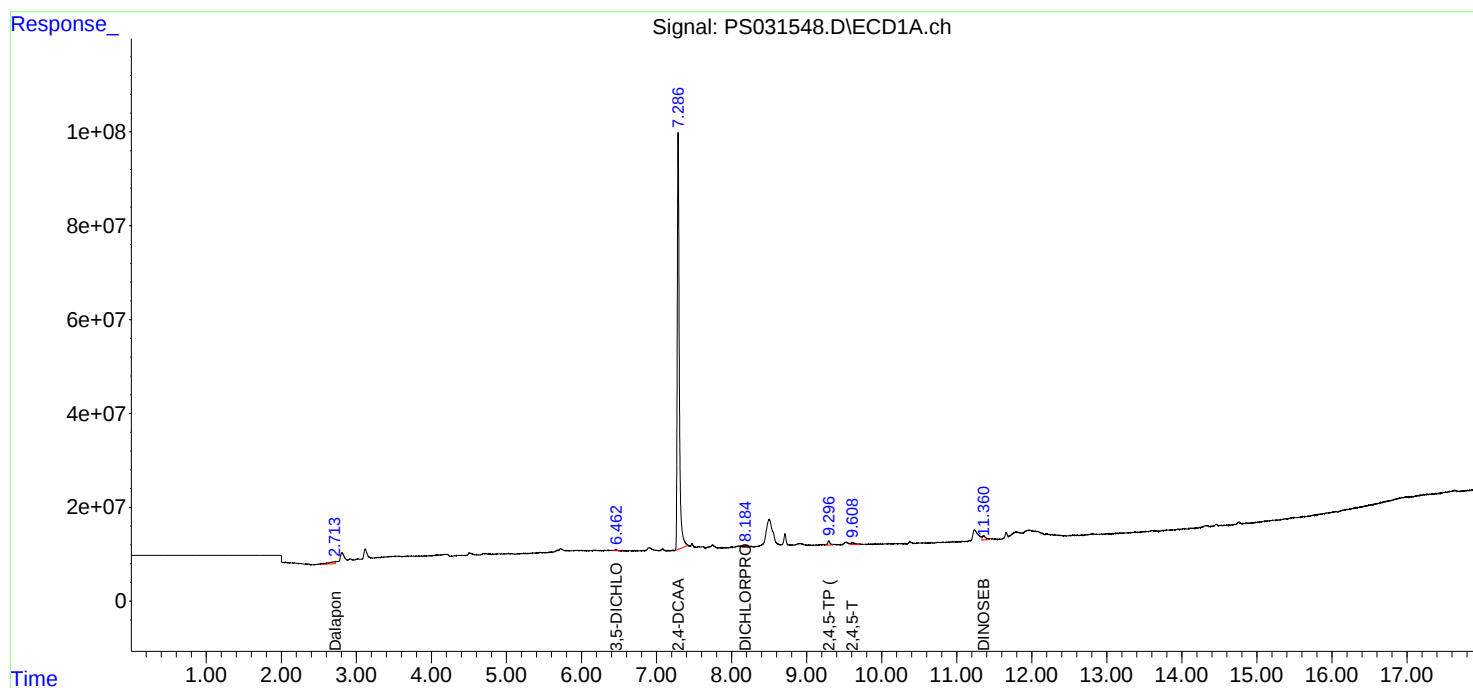


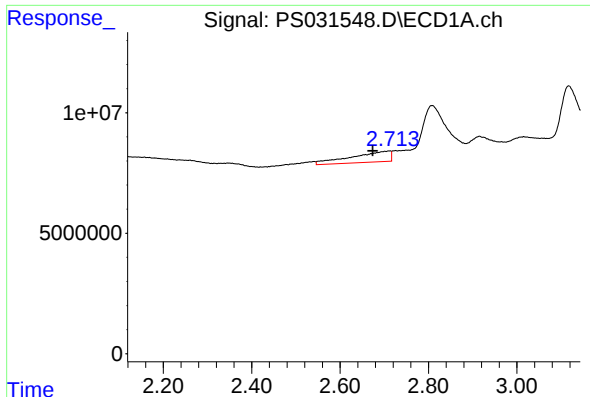

#1 Dalapon


R.T.: 2.712 min
Delta R.T.: 0.038 min
Response: 27355667
Conc: 5.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

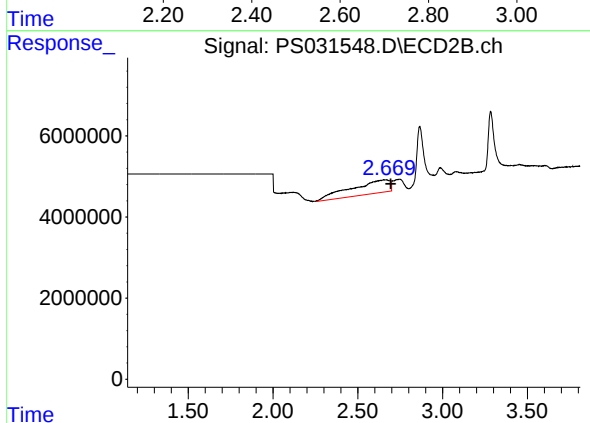


#1 Dalapon

R.T.: 2.669 min
Delta R.T.: -0.026 min
Response: 53262568
Conc: 20.02 ng/ml

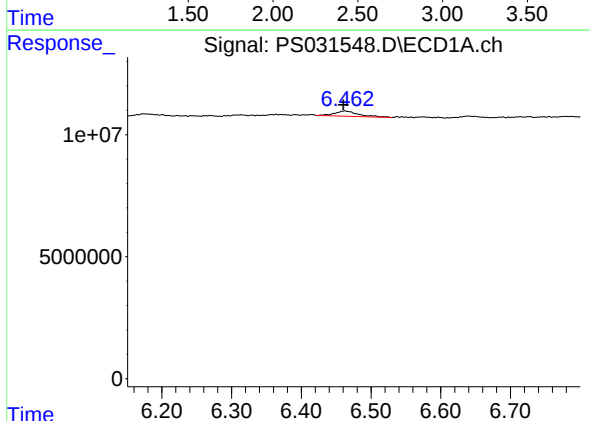


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.462 min
Delta R.T.: 0.002 min
Response: 5059028
Conc: 1.07 ng/ml

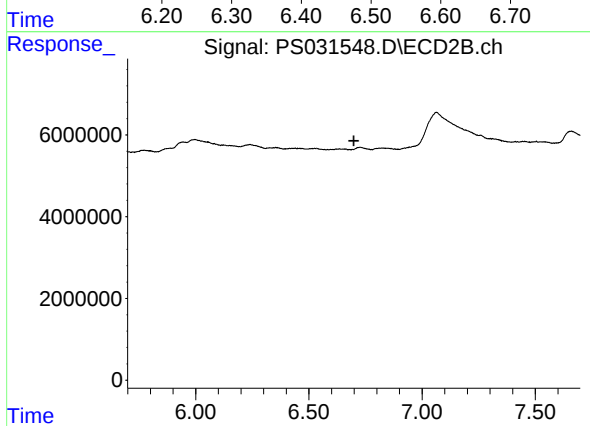

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.699 min
Response: 0
Conc: N.D.

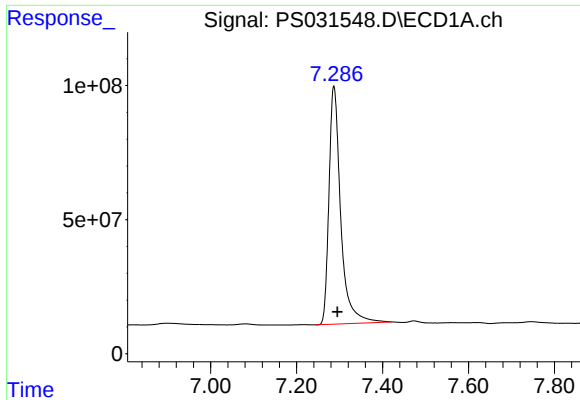

#4 2,4-DCAA


R.T.: 7.287 min
Delta R.T.: -0.008 min
Response: 1685732565
Conc: 531.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

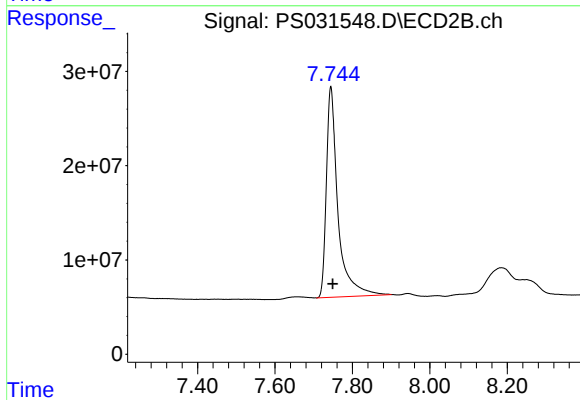


#4 2,4-DCAA

R.T.: 7.744 min
Delta R.T.: -0.005 min
Response: 462444310
Conc: 547.05 ng/ml

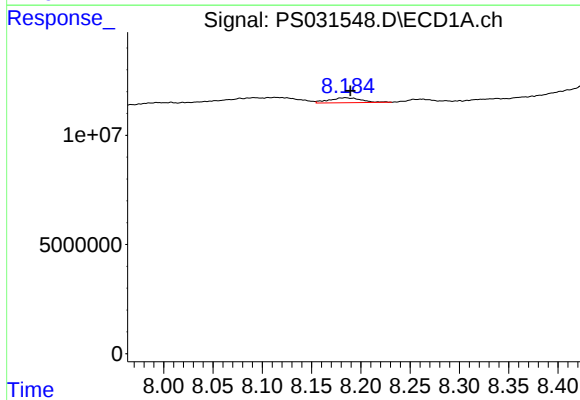


#8 DICHLORPROP

R.T.: 8.184 min
Delta R.T.: -0.005 min
Response: 5050083
Conc: 1.59 ng/ml

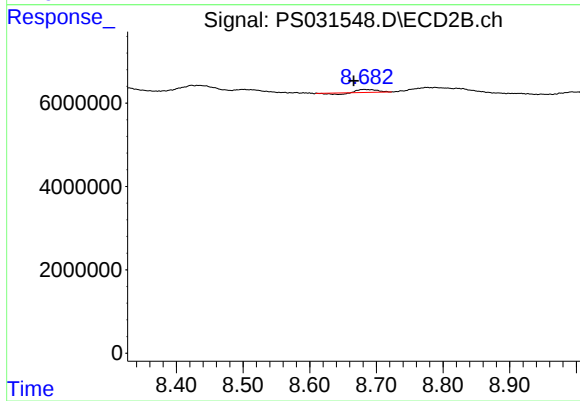

#8 DICHLORPROP


R.T.: 8.682 min
Delta R.T.: 0.016 min
Response: 967109
Conc: N.D.

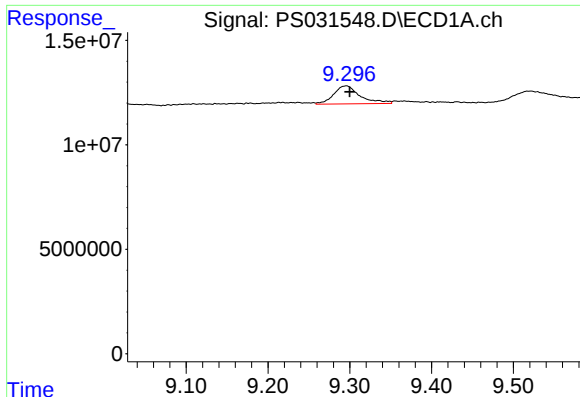

#11 2,4,5-TP (SILVEX)


R.T.: 9.296 min
Delta R.T.: -0.004 min
Response: 19256339
Conc: 1.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

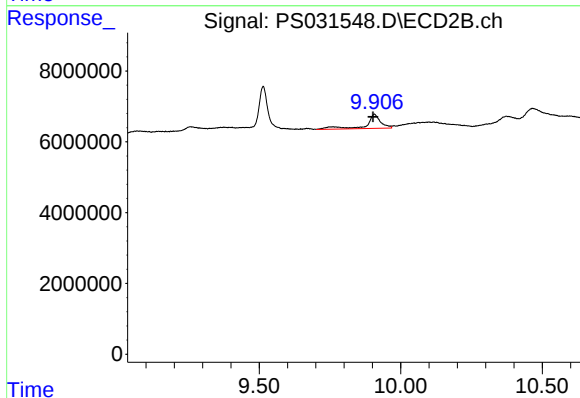


#11 2,4,5-TP (SILVEX)

R.T.: 9.907 min
Delta R.T.: 0.004 min
Response: 14458318
Conc: 1.10 ng/ml

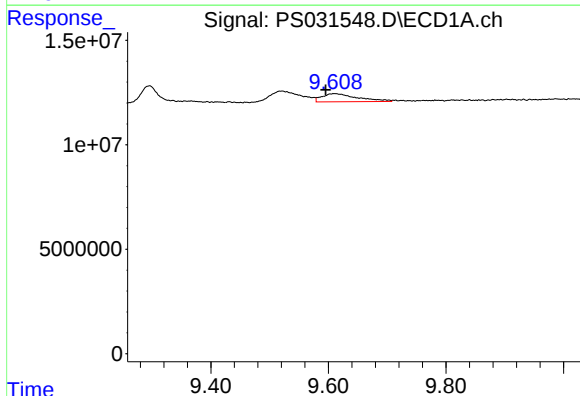


#12 2,4,5-T

R.T.: 9.610 min
Delta R.T.: 0.015 min
Response: 16170374
Conc: 1.10 ng/ml

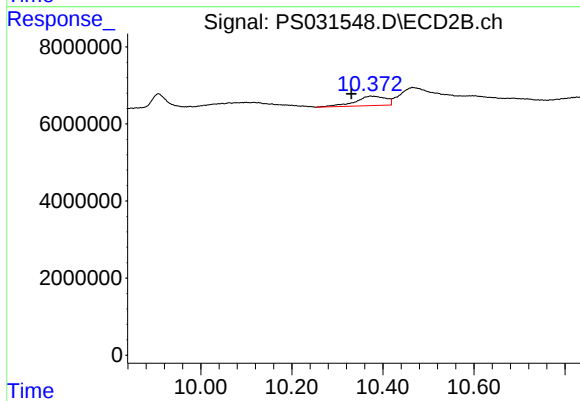

#12 2,4,5-T


R.T.: 10.374 min
Delta R.T.: 0.043 min
Response: 11699847
Conc: N.D.

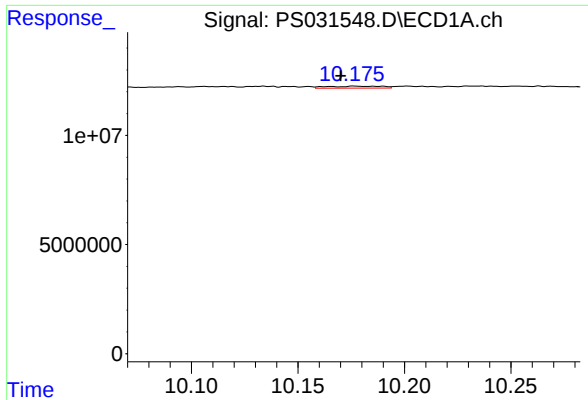

#13 2,4-DB


R.T.: 10.177 min
Delta R.T.: 0.006 min
Response: 1551677
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

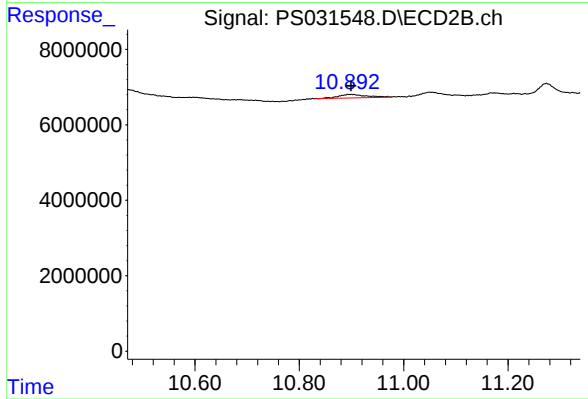


#13 2,4-DB

R.T.: 10.896 min
Delta R.T.: -0.003 min
Response: 3494935
Conc: 3.62 ng/ml

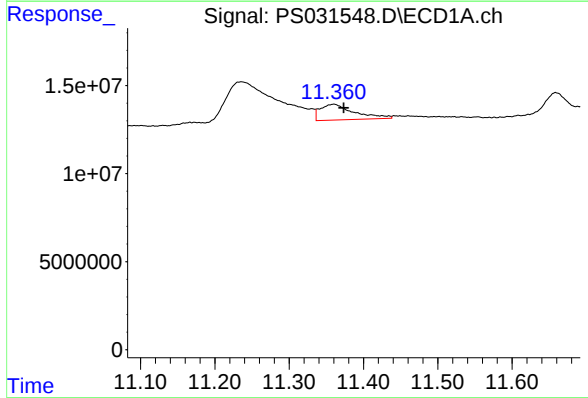

#14 DINOSEB

R.T.: 11.360 min
Delta R.T.: -0.014 min
Response: 28336452
Conc: 2.24 ng/ml

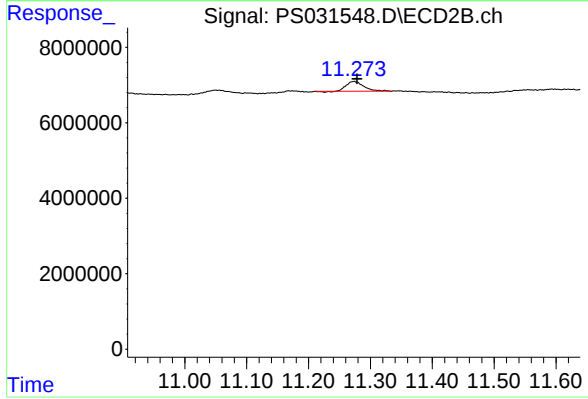

#14 DINOSEB

R.T.: 11.273 min
Delta R.T.: -0.005 min
Response: 5001281
Conc: N.D.