

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082718\
 Data File : PS001611.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2018 16:51
 Operator : UA
 Sample : J4629-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 00:51:06 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.489	10.964	52813969	56515797	286.099	279.049
Target Compounds							
2) T	3,5-DICHL...	0.000	9.203	0	35162823	N.D.	137.594 #
5) T	DICAMBA	0.000	11.208	0	1235509	N.D.	1.762 #
6) T	MCP	12.178	0.000	8626373	0	17.144	N.D. #
7) T	MCPA	0.000	11.825	0	450679	N.D.	0.618 #
10) T	Pentachlo...	13.735	0.000	7025334	0	2.817	N.D. #
11) T	2,4,5-TP ...	0.000	14.001	0	3133908	N.D.	2.949 #
13) T	2,4-DB	15.803	15.283	14011522	2990205	104.312	22.549 #
14) T	DINOSEB	0.000	15.659	0	4463934	N.D.	6.036 #
15) T	Picloram	17.002	16.902	6496019	24549086	4.638	18.827 #
16) T	DCPA	0.000	16.902	0	24549086	N.D.	17.194 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082718\
Data File : PS001611.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2018 16:51
Operator : UA
Sample : J4629-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 00:51:06 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

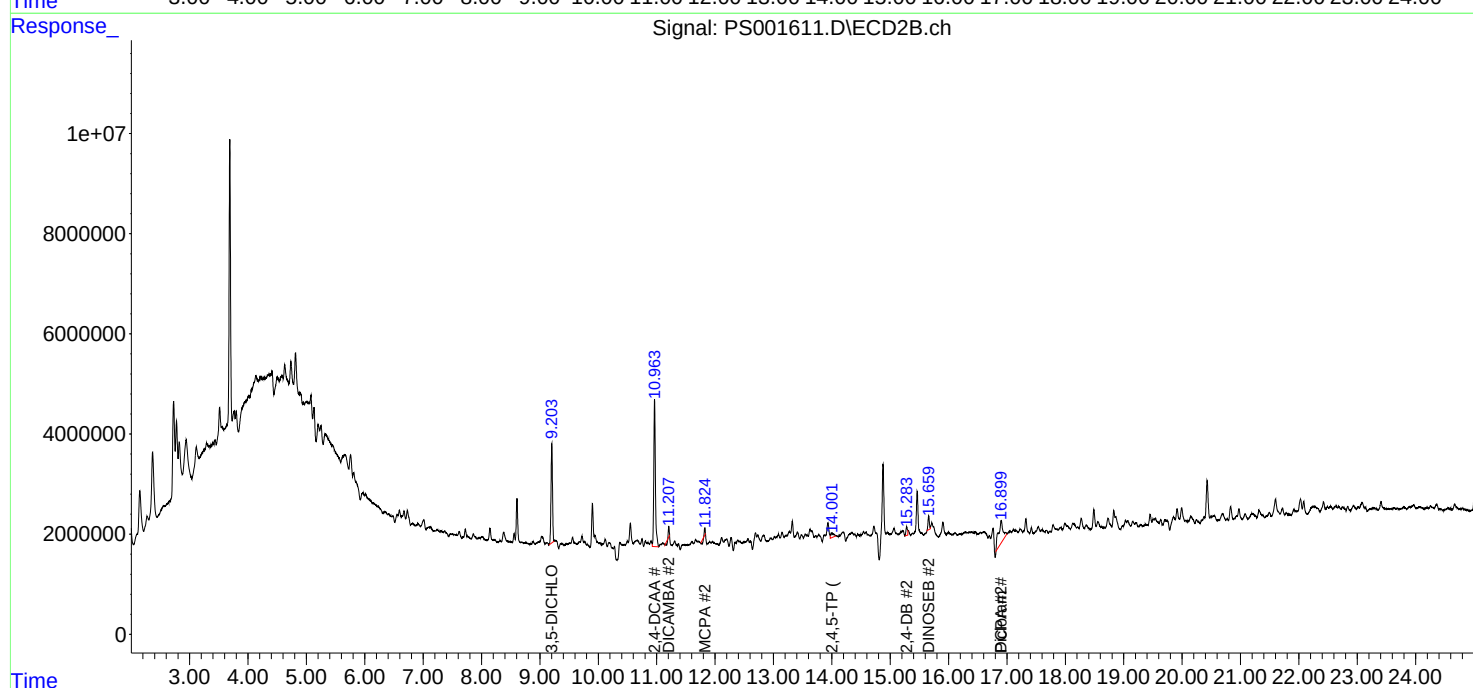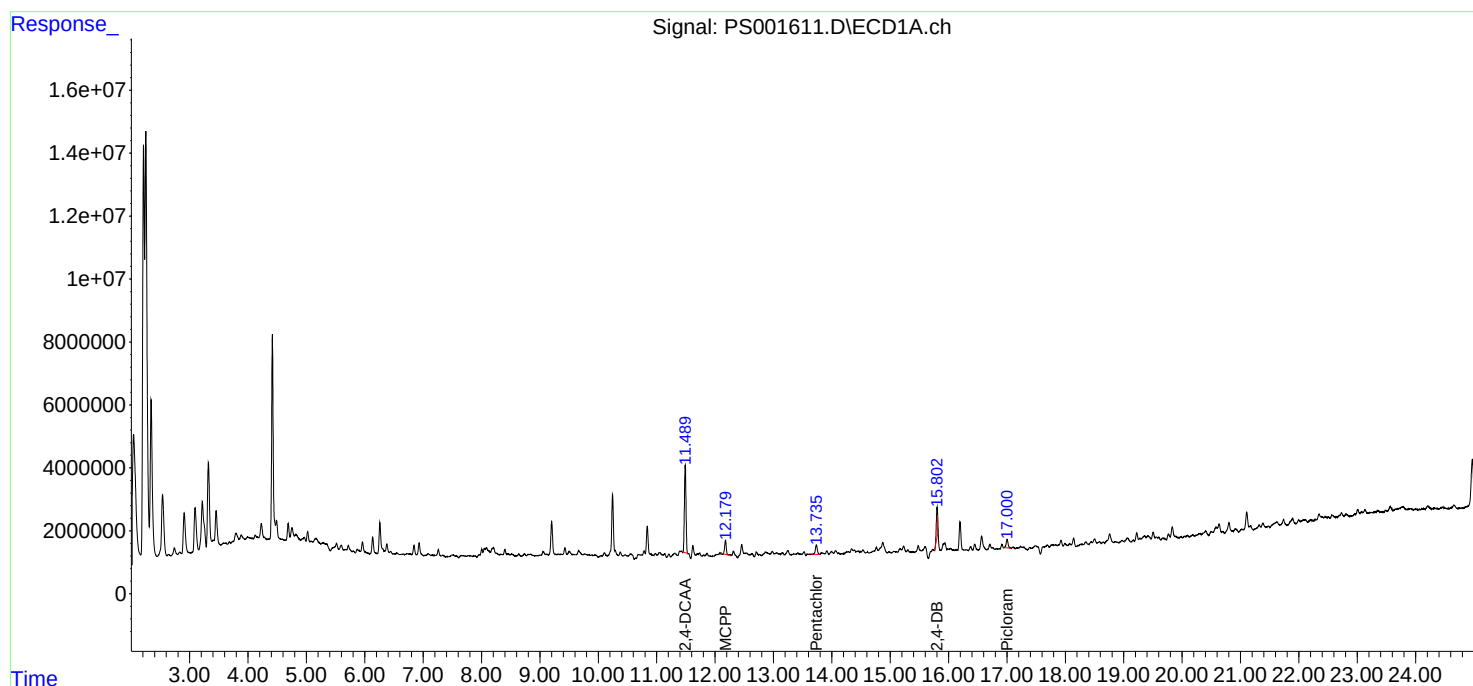


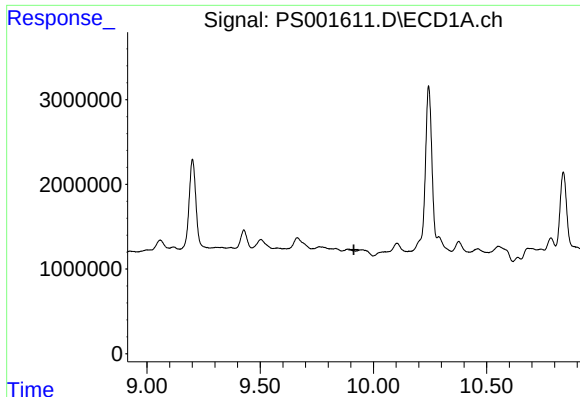

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

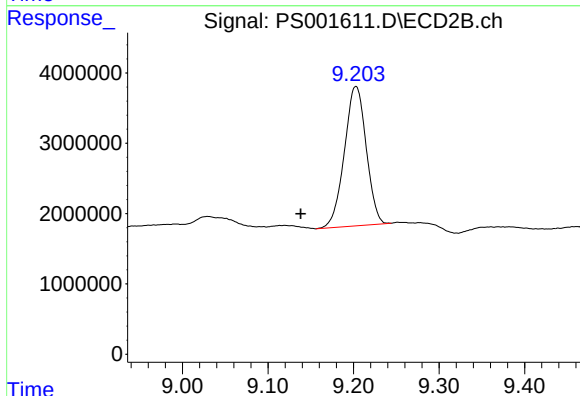


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.203 min
Delta R.T.: 0.065 min
Response: 35162823
Conc: 137.59 ng/ml

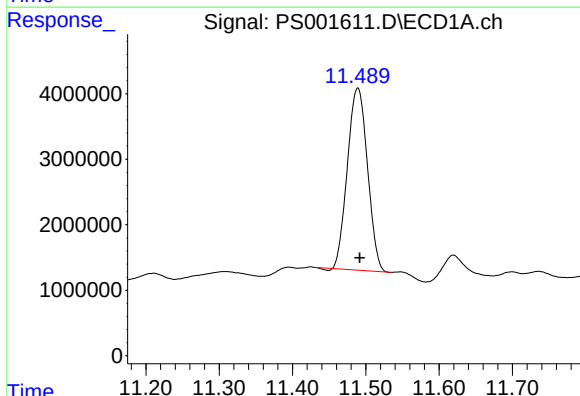


#4 2,4-DCAA

R.T.: 11.489 min
Delta R.T.: -0.003 min
Response: 52813969
Conc: 286.10 ng/ml

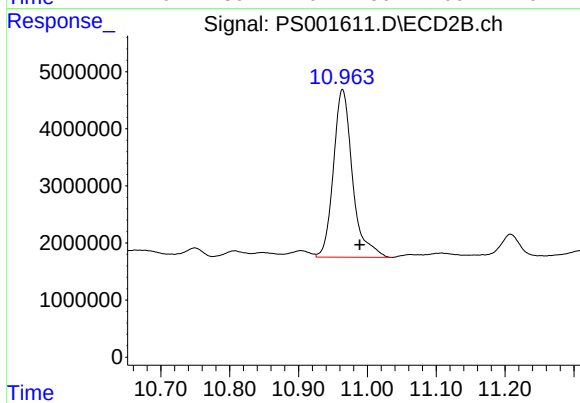

#4 2,4-DCAA


R.T.: 10.964 min
Delta R.T.: -0.025 min
Response: 56515797
Conc: 279.05 ng/ml

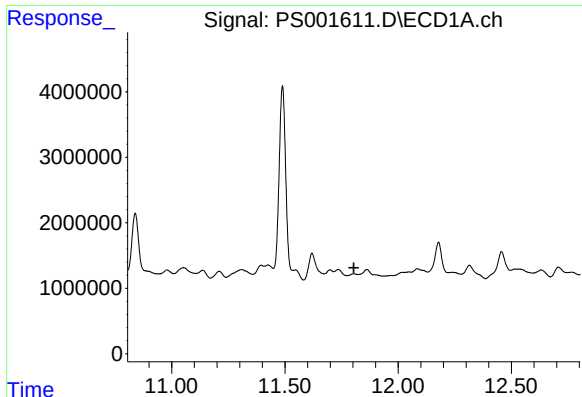

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.805 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

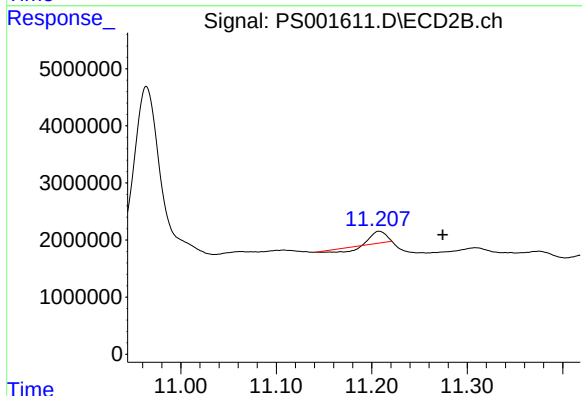


#5 DICAMBA

R.T.: 11.208 min
Delta R.T.: -0.067 min
Response: 1235509
Conc: 1.76 ng/ml

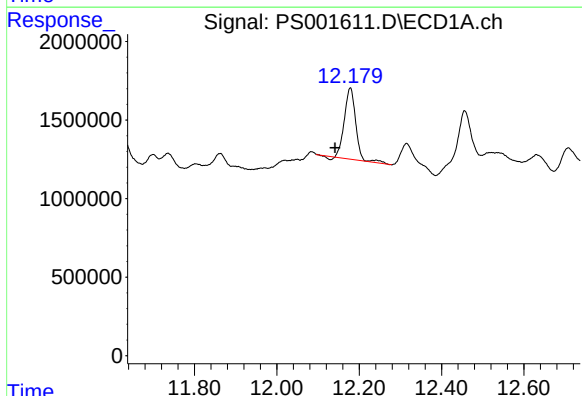


#6 MCP

R.T.: 12.178 min
Delta R.T.: 0.037 min
Response: 8626373
Conc: 17.14 ug/ml

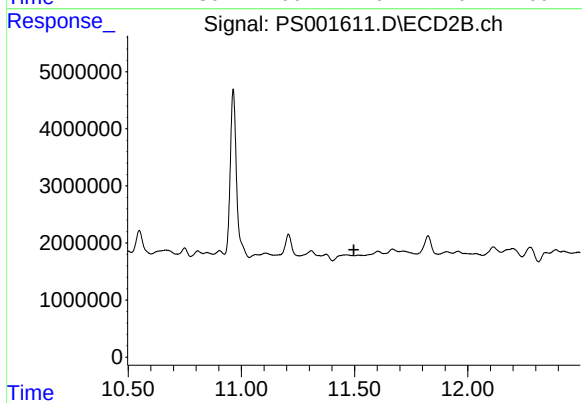

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.497 min
Response: 0
Conc: N.D.

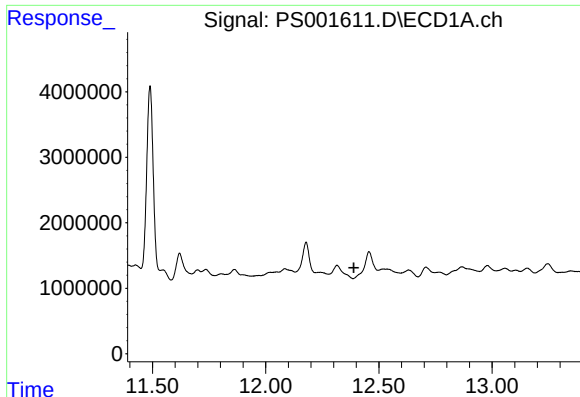

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.390 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

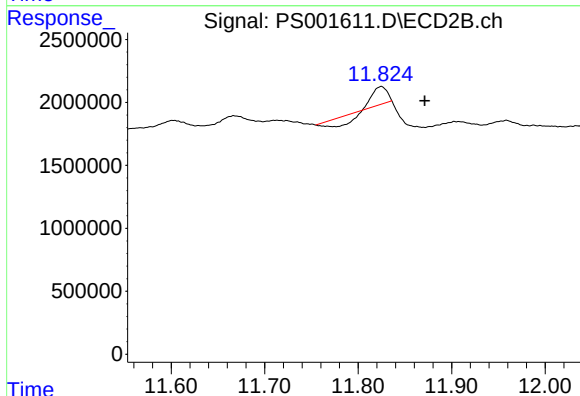


#7 MCPA

R.T.: 11.825 min
Delta R.T.: -0.047 min
Response: 450679
Conc: 0.62 ug/ml

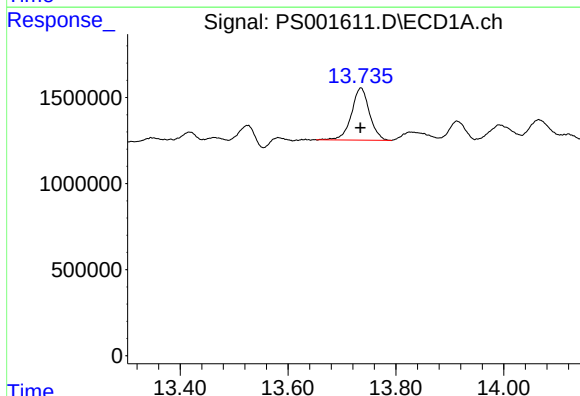


#10 Pentachlorophenol

R.T.: 13.735 min
Delta R.T.: 0.001 min
Response: 7025334
Conc: 2.82 ng/ml

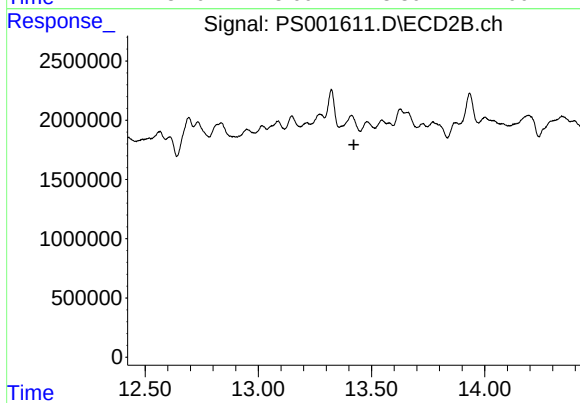

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.422 min
Response: 0
Conc: N.D.

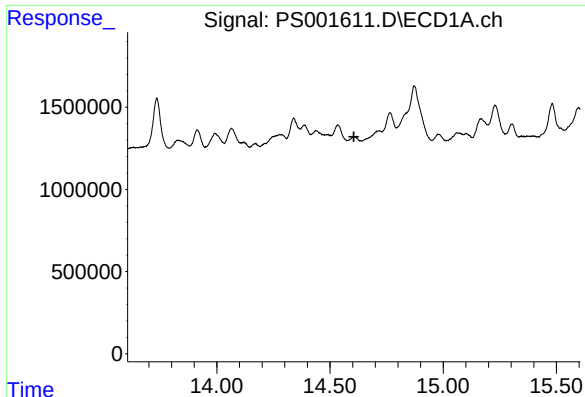

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.606 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

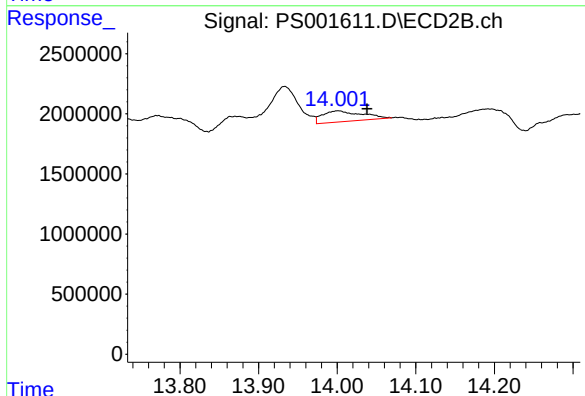


#11 2,4,5-TP (SILVEX)

R.T.: 14.001 min
Delta R.T.: -0.037 min
Response: 3133908
Conc: 2.95 ng/ml

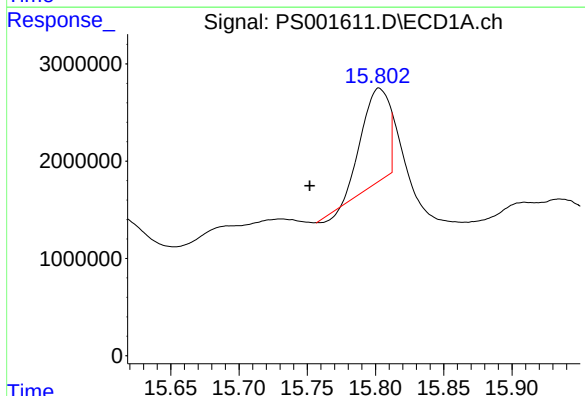


#13 2,4-DB

R.T.: 15.803 min
Delta R.T.: 0.051 min
Response: 14011522
Conc: 104.31 ng/ml

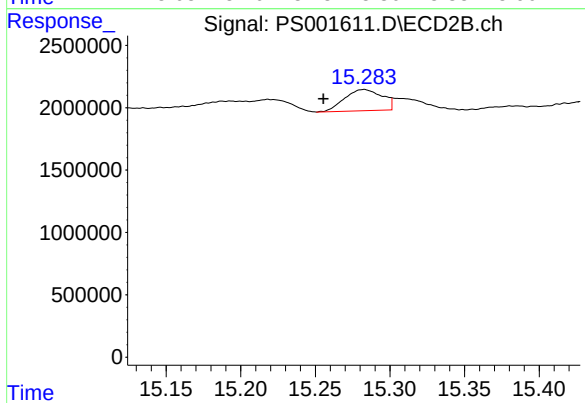

#13 2,4-DB


R.T.: 15.283 min
Delta R.T.: 0.027 min
Response: 2990205
Conc: 22.55 ng/ml

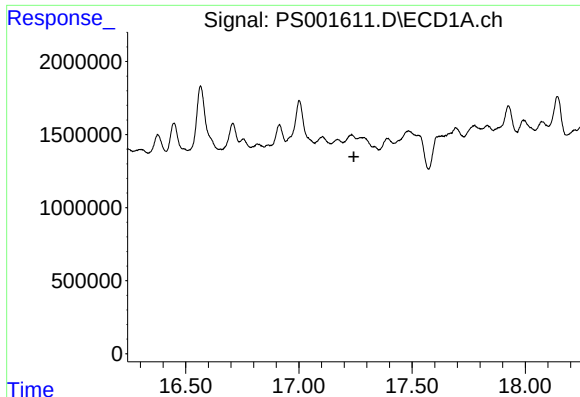

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.243 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

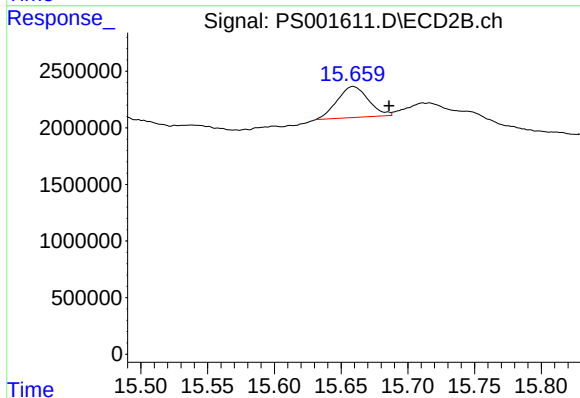


#14 DINOSEB

R.T.: 15.659 min
Delta R.T.: -0.027 min
Response: 4463934
Conc: 6.04 ng/ml

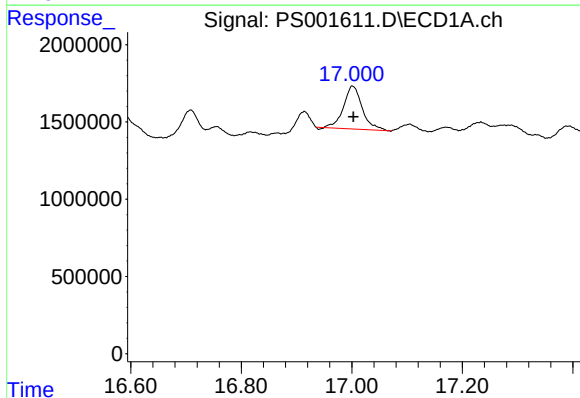


#15 Picloram

R.T.: 17.002 min
Delta R.T.: -0.001 min
Response: 6496019
Conc: 4.64 ng/ml

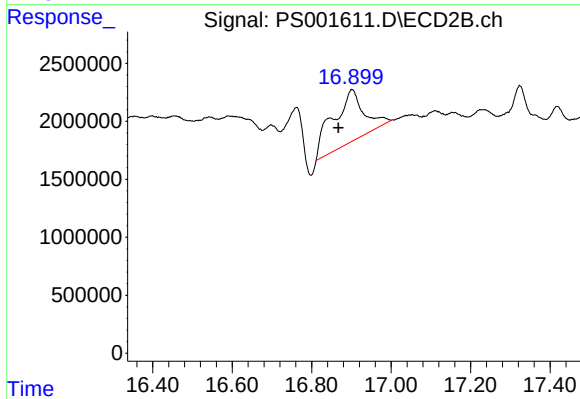

#15 Picloram


R.T.: 16.902 min
Delta R.T.: 0.034 min
Response: 24549086
Conc: 18.83 ng/ml

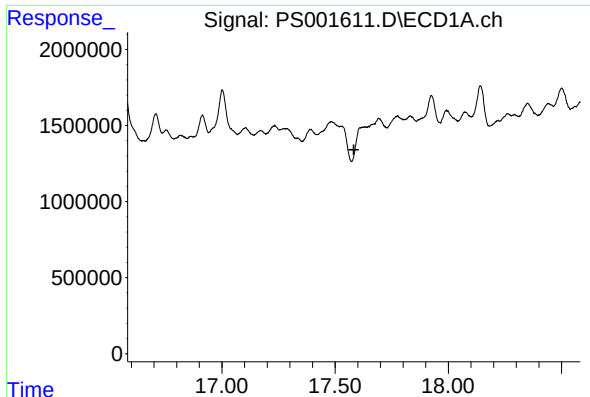

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.583 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

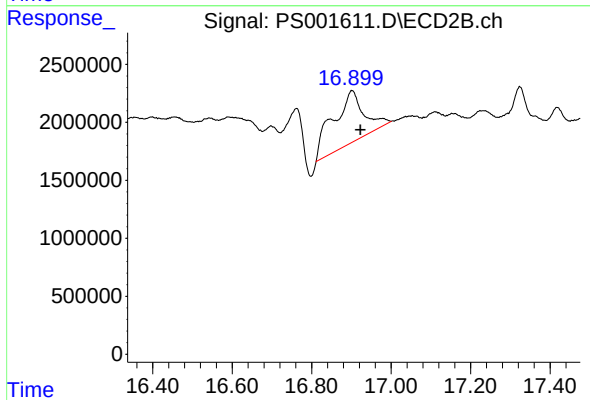

#16 DCPA

R.T.: 16.902 min
Delta R.T.: -0.021 min
Response: 24549086
Conc: 17.19 ng/ml