

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082718\
 Data File : PS001613.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2018 17:53
 Operator : UA
 Sample : J4636-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 00:51:51 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.468	10.966	54885070	55541765	297.318	274.240
Target Compounds							
1) T	Dalapon	2.888	0.000	5255806	0	20.908	N.D. #
2) T	3,5-DICHL...	0.000	9.206	0	29946346	N.D.	117.182 #
6) T	MCP	12.157	0.000	6394123	0	12.708	N.D. #
8) T	DICHLORPROP	0.000	12.388	0	2669770	N.D.	14.333 #
10) T	Pentachlo...	13.713	13.476	3649636	2024642	1.464	0.749 #
11) T	2,4,5-TP ...	0.000	14.088	0	2120745	N.D.	1.995 #
12) T	2,4,5-T	15.045	0.000	2731720	0	2.887	N.D. #
14) T	DINOSEB	0.000	15.696	0	9741486	N.D.	13.172 #
15) T	Picloram	17.031	16.845	9960656	12328300	7.112	9.455 #
16) T	DCPA	17.587	16.912	-3183139	11280196	N.D.	7.901



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082718\
Data File : PS001613.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2018 17:53
Operator : UA
Sample : J4636-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 00:51:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

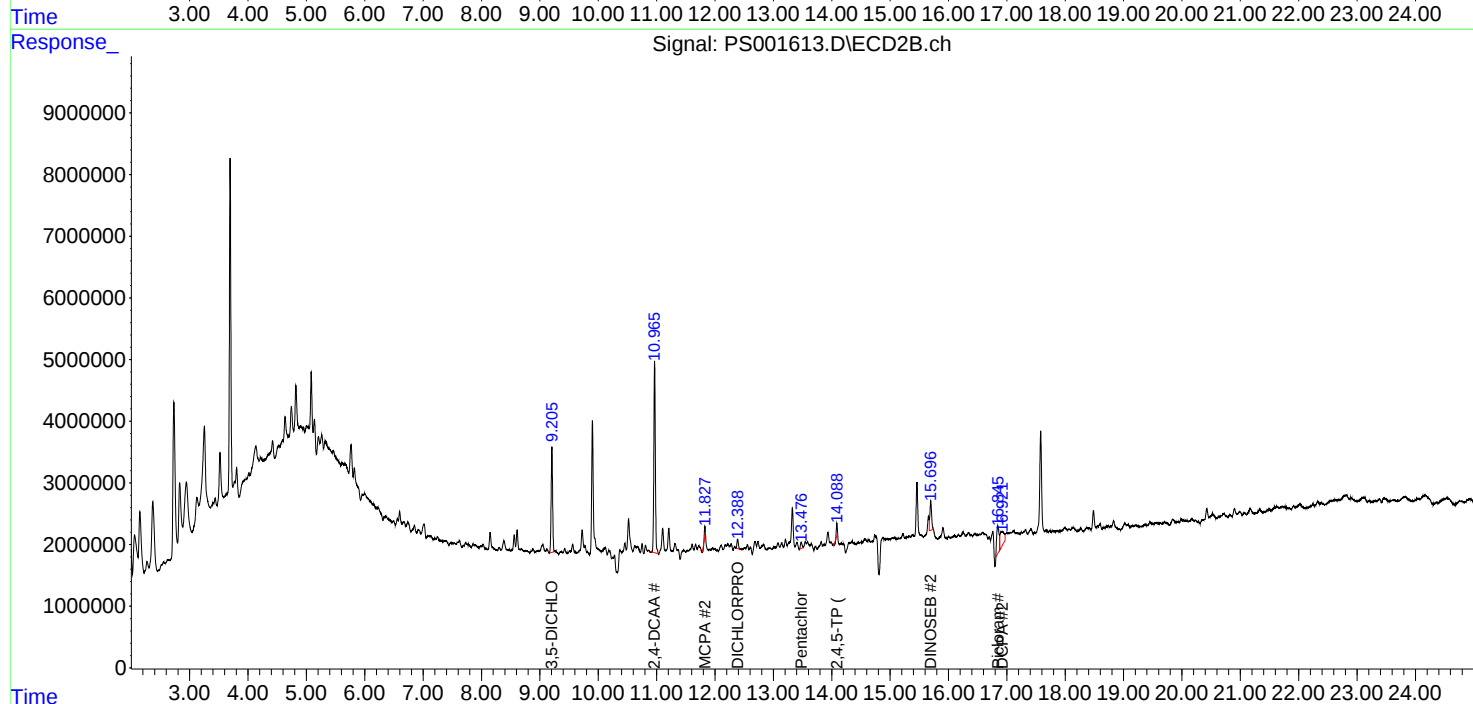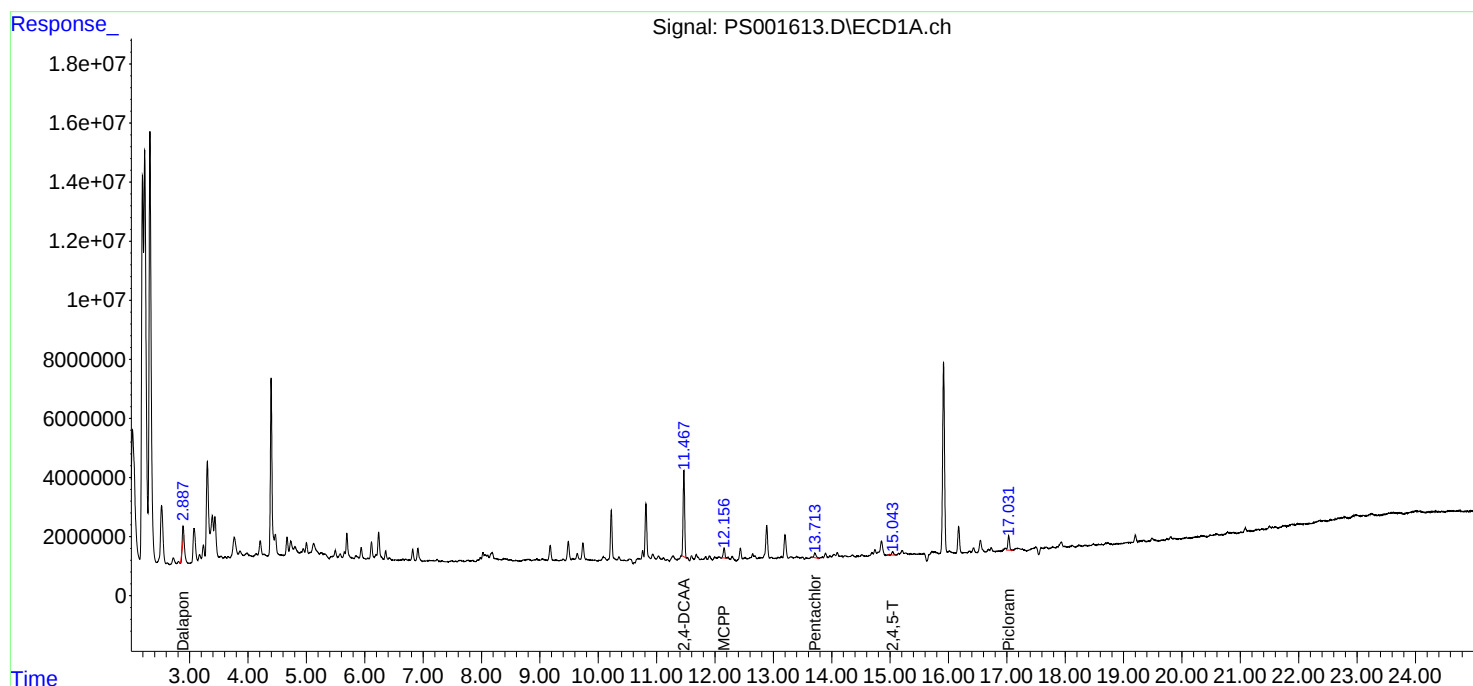


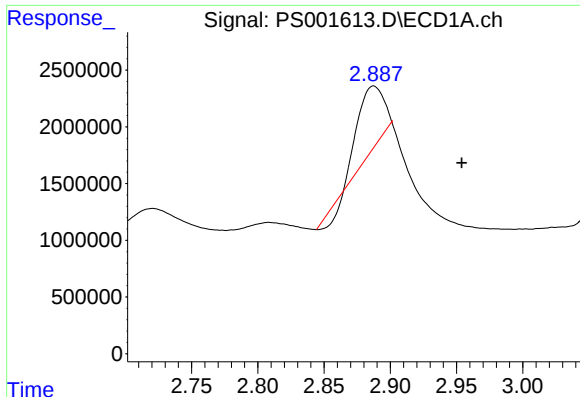

#1 Dalapon


R.T.: 2.888 min
Delta R.T.: -0.066 min
Response: 5255806
Conc: 20.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

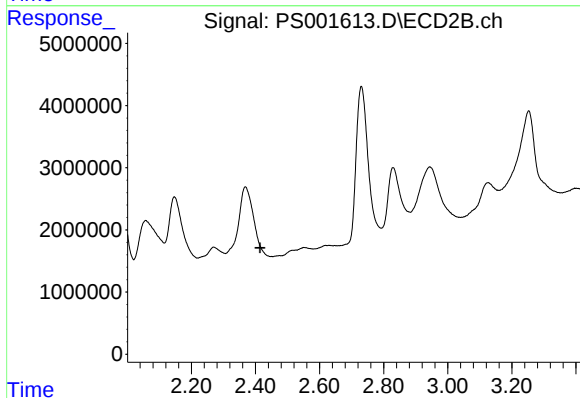


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.414 min
Response: 0
Conc: N.D.

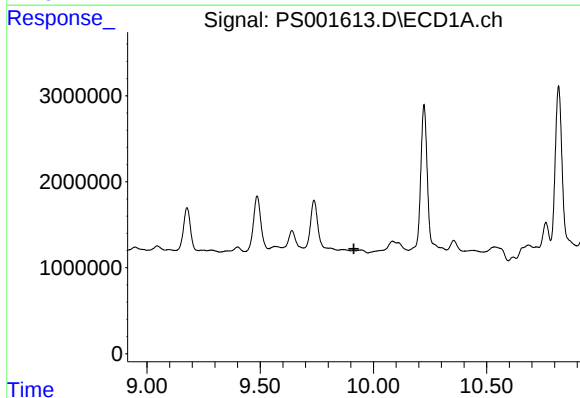


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.914 min
Response: 0
Conc: N.D.

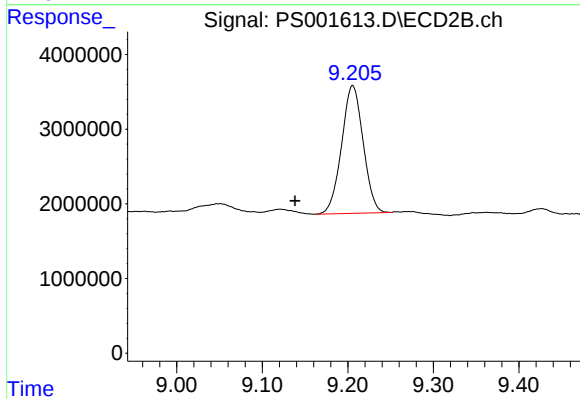

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.206 min
Delta R.T.: 0.068 min
Response: 29946346
Conc: 117.18 ng/ml

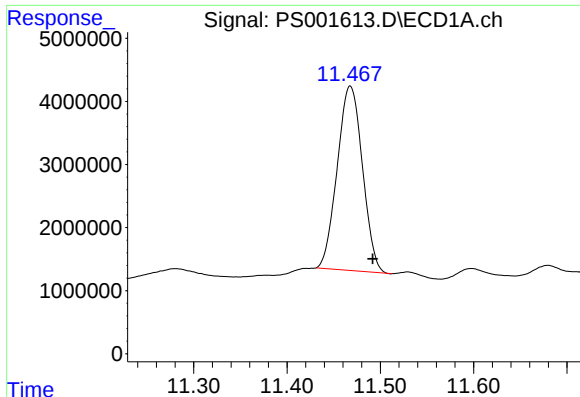

#4 2,4-DCAA


R.T.: 11.468 min
Delta R.T.: -0.024 min
Response: 54885070
Conc: 297.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

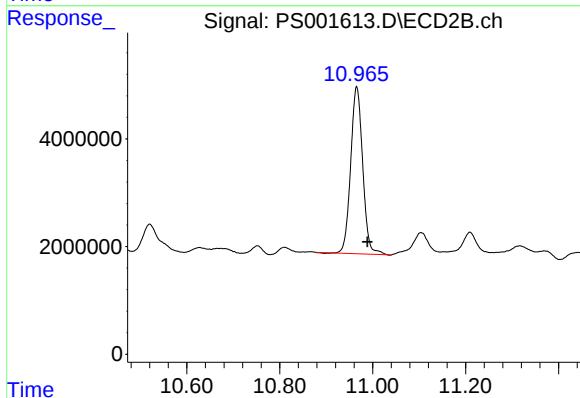


#4 2,4-DCAA

R.T.: 10.966 min
Delta R.T.: -0.023 min
Response: 55541765
Conc: 274.24 ng/ml

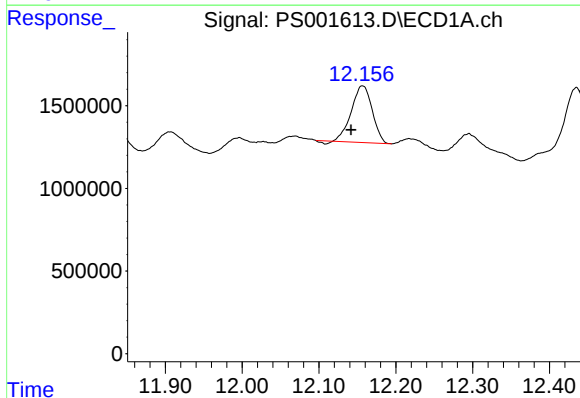


#6 MCP

R.T.: 12.157 min
Delta R.T.: 0.015 min
Response: 6394123
Conc: 12.71 ug/ml

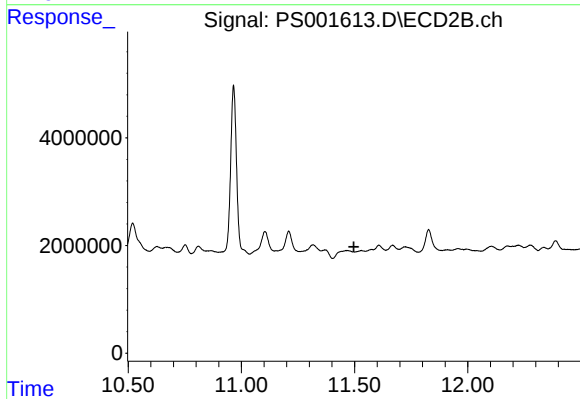

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.497 min
Response: 0
Conc: N.D.

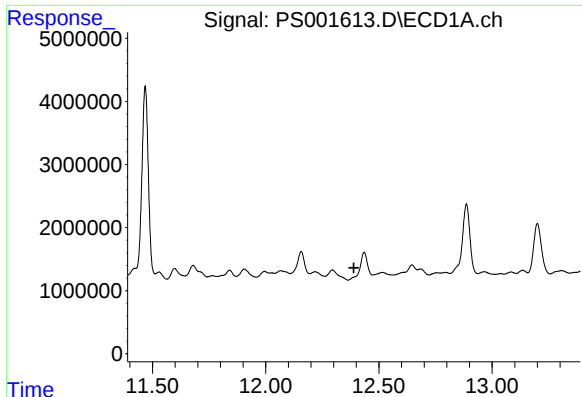

#7 MCPA


R.T.: 12.435 min
Delta R.T.: 0.045 min
Response: -5395255
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

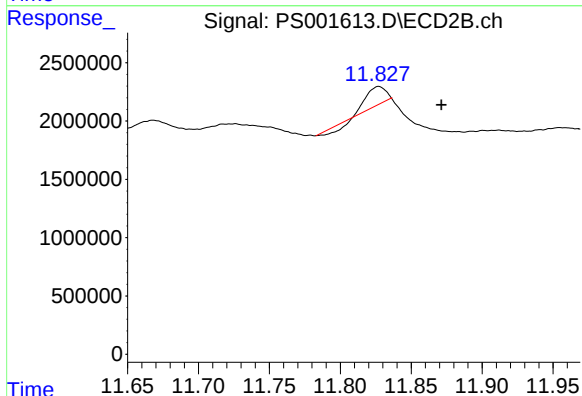


#7 MCPA

R.T.: 11.827 min
Delta R.T.: -0.044 min
Response: 1169048
Conc: 1.60 ug/ml

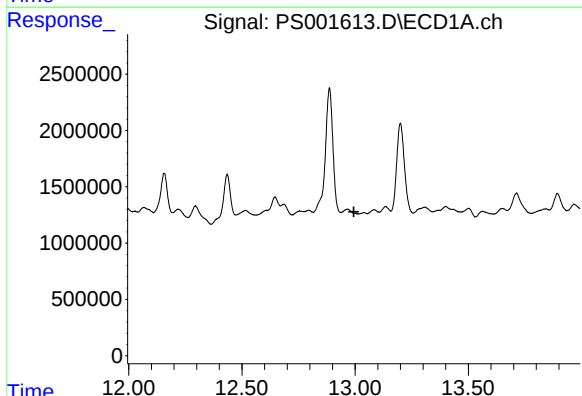


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.995 min
Response: 0
Conc: N.D.

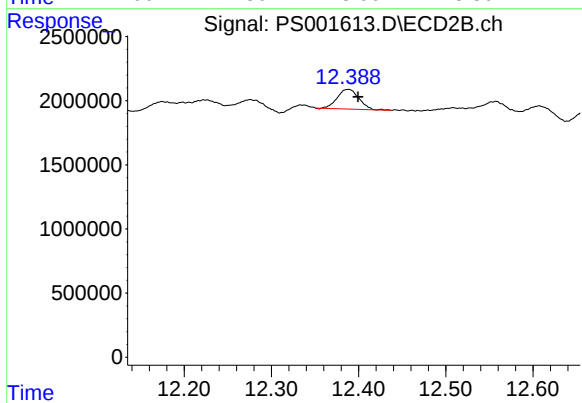

#8 DICHLORPROP


R.T.: 12.388 min
Delta R.T.: -0.011 min
Response: 2669770
Conc: 14.33 ng/ml

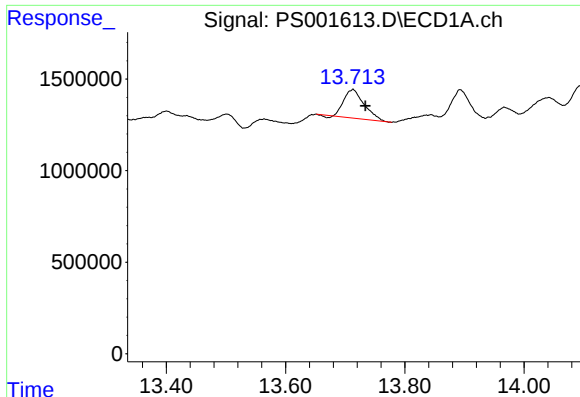

#10 Pentachlorophenol


R.T.: 13.713 min
Delta R.T.: -0.021 min
Response: 3649636
Conc: 1.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

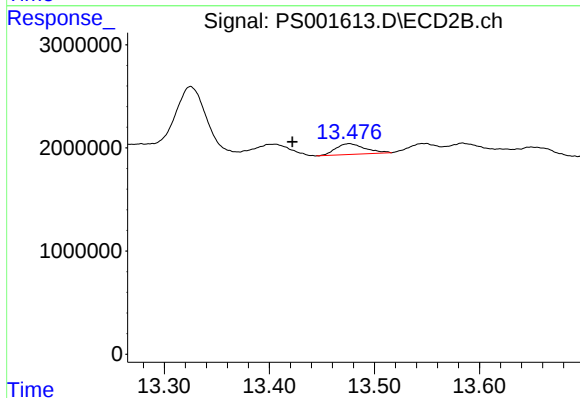


#10 Pentachlorophenol

R.T.: 13.476 min
Delta R.T.: 0.054 min
Response: 2024642
Conc: 0.75 ng/ml

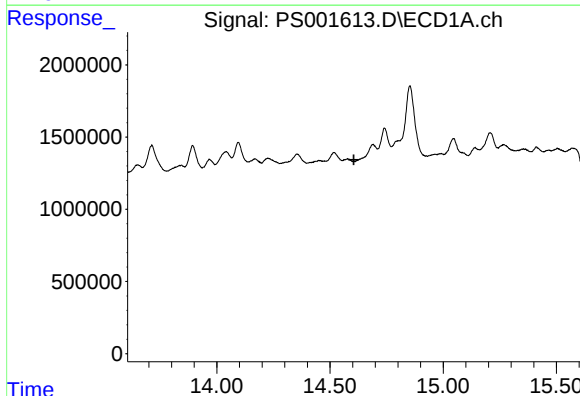


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.606 min
Response: 0
Conc: N.D.

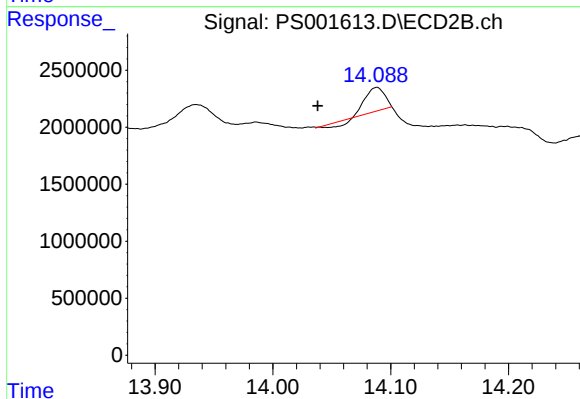

#11 2,4,5-TP (SILVEX)


R.T.: 14.088 min
Delta R.T.: 0.050 min
Response: 2120745
Conc: 2.00 ng/ml

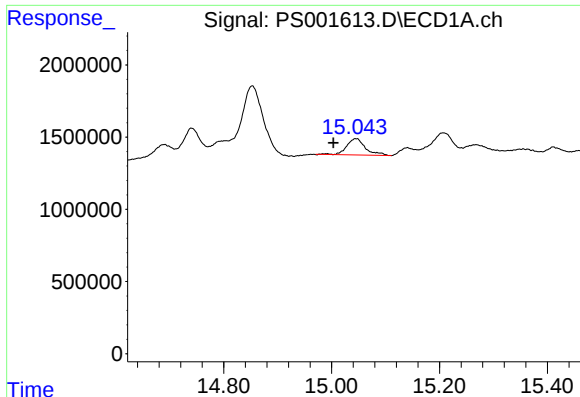

#12 2,4,5-T


R.T.: 15.045 min
Delta R.T.: 0.042 min
Response: 2731720
Conc: 2.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

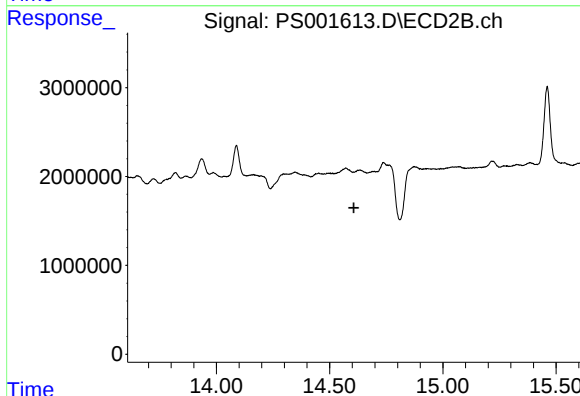


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.607 min
Response: 0
Conc: N.D.

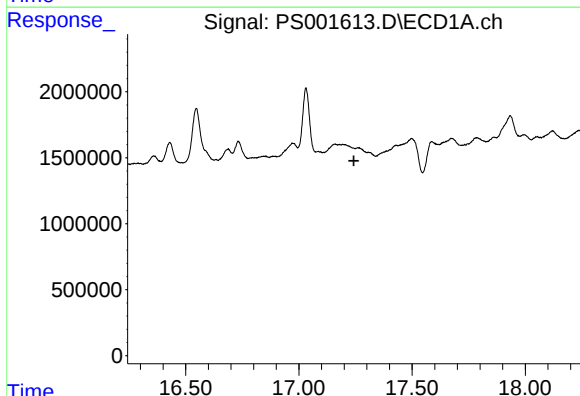


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.243 min
Response: 0
Conc: N.D.

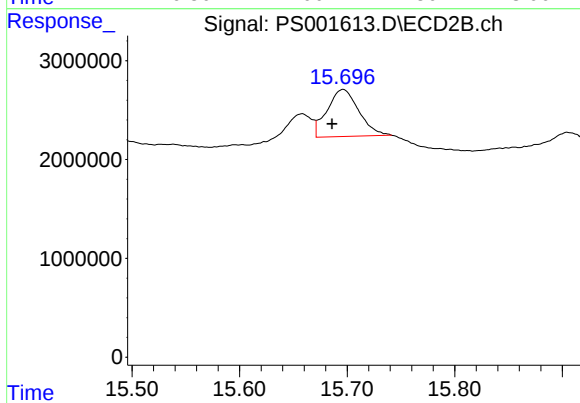

#14 DINOSEB


R.T.: 15.696 min
Delta R.T.: 0.010 min
Response: 9741486
Conc: 13.17 ng/ml

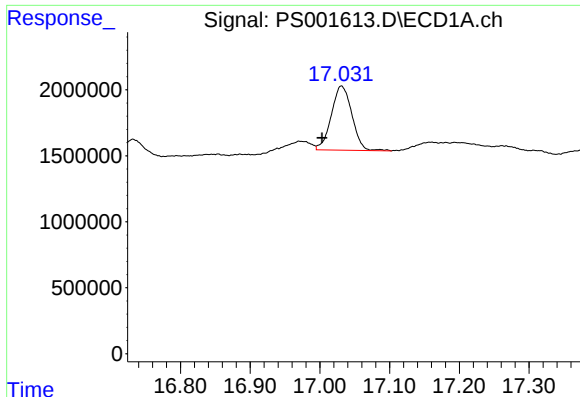

#15 Picloram


R.T.: 17.031 min
Delta R.T.: 0.028 min
Response: 9960656
Conc: 7.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

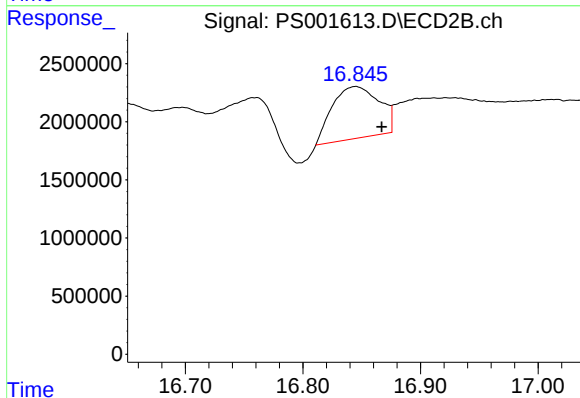


#15 Picloram

R.T.: 16.845 min
Delta R.T.: -0.023 min
Response: 12328300
Conc: 9.45 ng/ml

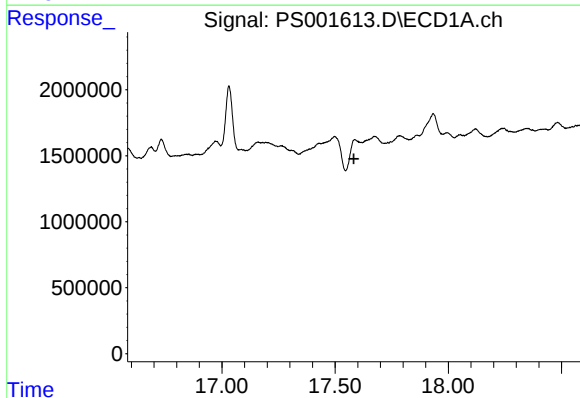

#16 DCPA

R.T.: 17.587 min
Delta R.T.: 0.004 min
Response: -3183139
Conc: N.D.

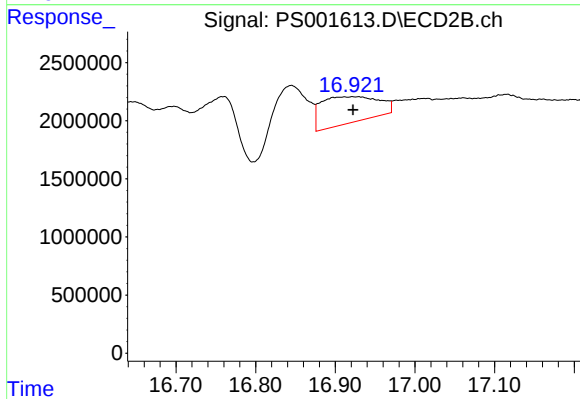

#16 DCPA

R.T.: 16.912 min
Delta R.T.: -0.011 min
Response: 11280196
Conc: 7.90 ng/ml