

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082718\
 Data File : PS001617.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2018 19:58
 Operator : UA
 Sample : J4606-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 00:53:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.487	10.969	47477252	50854944	257.189	251.098
Target Compounds							
3) T	4-Nitroph...	0.000	10.123	0	2825644	N.D.	26.808 #
5) T	DICAMBA	0.000	11.317	0	832918	N.D.	1.188 #
6) T	MCP	12.175	0.000	10935258	0	21.733	N.D. #
7) T	MCPA	0.000	11.829	0	1010445	N.D.	1.386 #
9) T	2,4-D	13.332	0.000	3253994	0	13.723	N.D. #
10) T	Pentachlo...	13.729	0.000	4459925	0	1.788	N.D. #
14) T	DINOSEB	0.000	15.661	0	6149236	N.D.	8.314 #
15) T	Picloram	16.999	16.849	6770265	10045390	4.834	7.704 #
16) T	DCPA	0.000	16.903	0	18218819	N.D.	12.761 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082718\
Data File : PS001617.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2018 19:58
Operator : UA
Sample : J4606-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 00:53:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

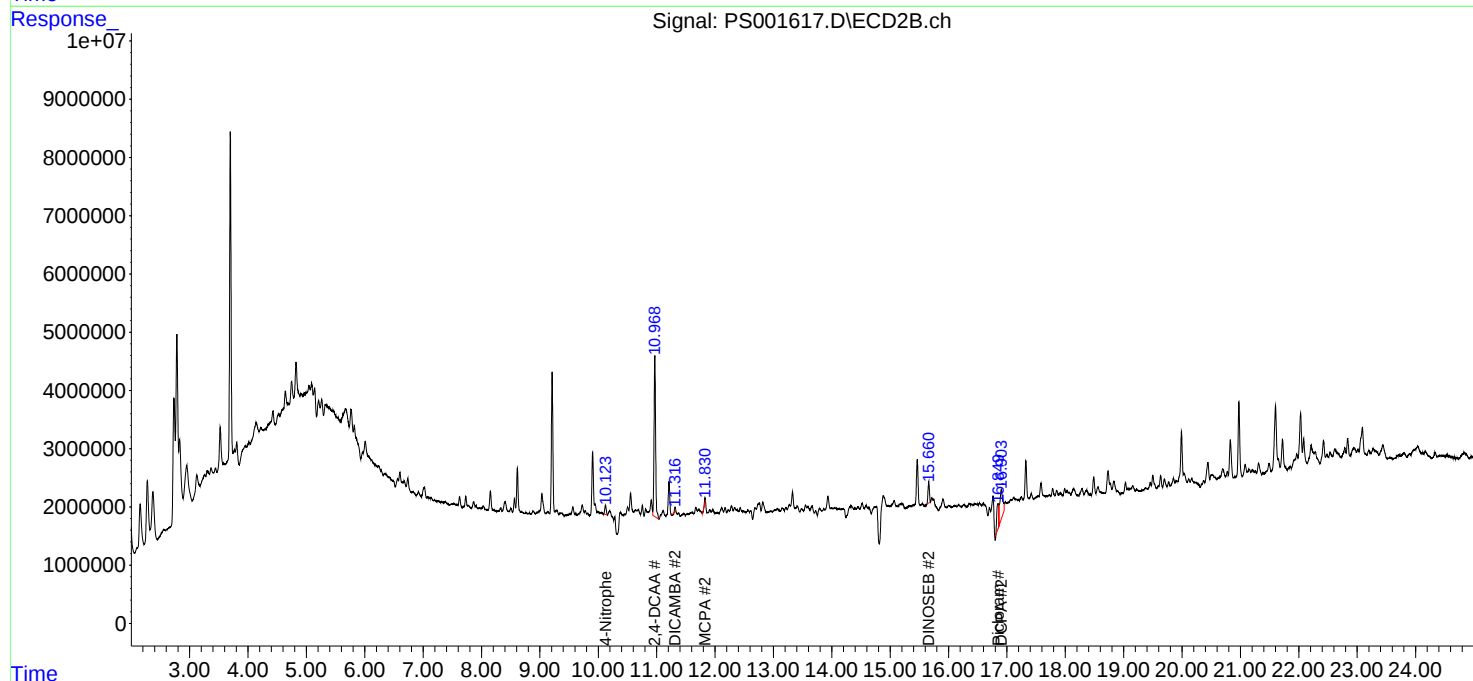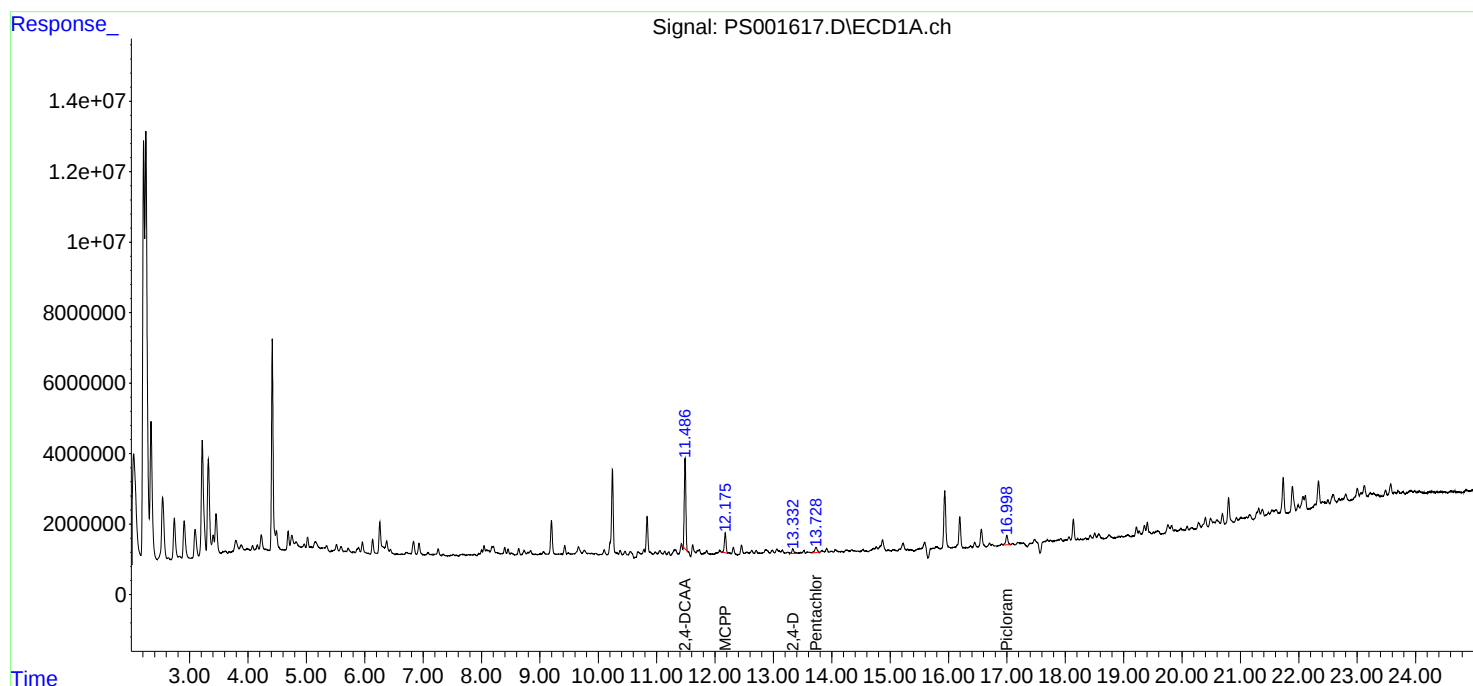


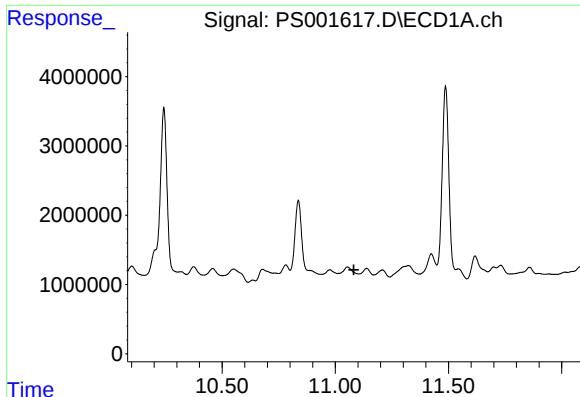

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.082 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

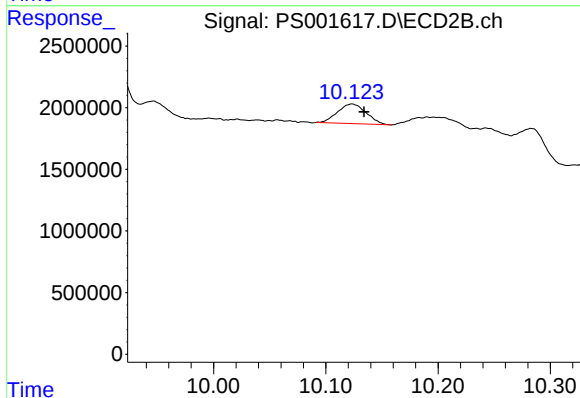


#3 4-Nitrophenol

R.T.: 10.123 min
Delta R.T.: -0.011 min
Response: 2825644
Conc: 26.81 ng/ml

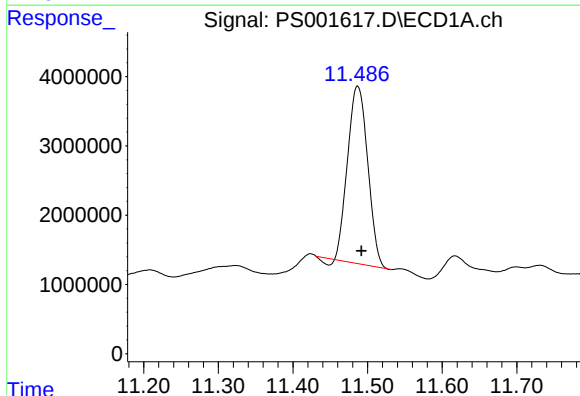


#4 2,4-DCAA

R.T.: 11.487 min
Delta R.T.: -0.005 min
Response: 47477252
Conc: 257.19 ng/ml

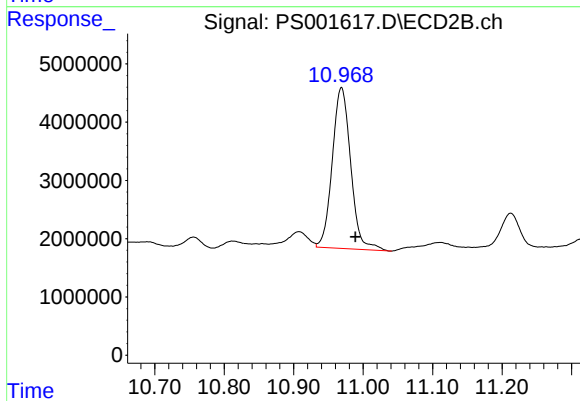

#4 2,4-DCAA


R.T.: 10.969 min
Delta R.T.: -0.020 min
Response: 50854944
Conc: 251.10 ng/ml

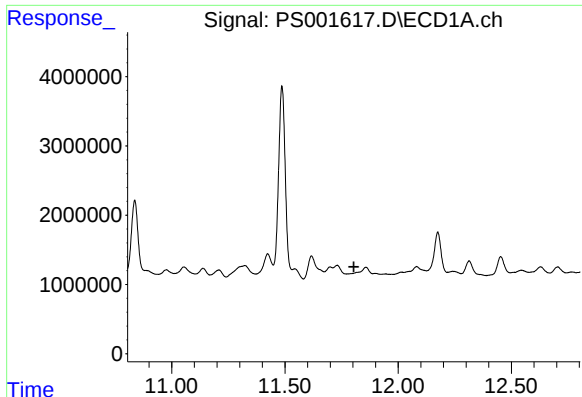

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.805 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

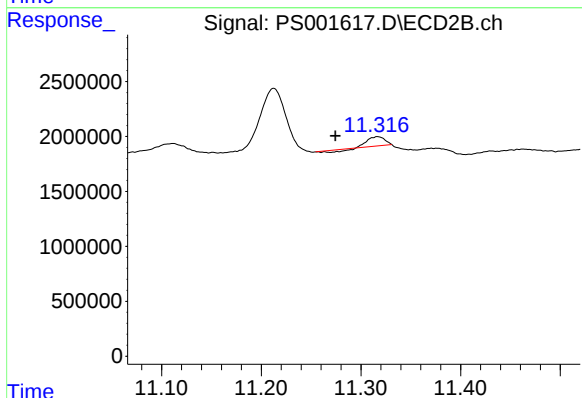


#5 DICAMBA

R.T.: 11.317 min
Delta R.T.: 0.042 min
Response: 832918
Conc: 1.19 ng/ml

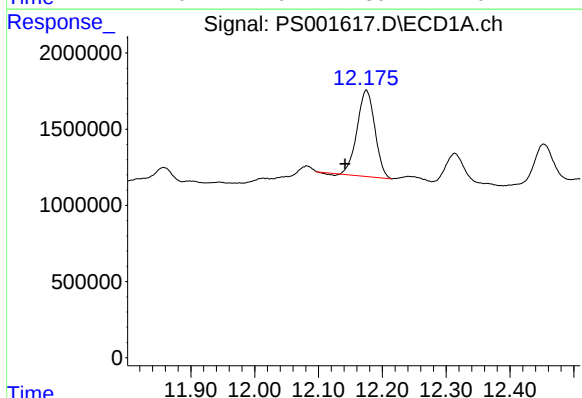


#6 MCP

R.T.: 12.175 min
Delta R.T.: 0.033 min
Response: 10935258
Conc: 21.73 ug/ml

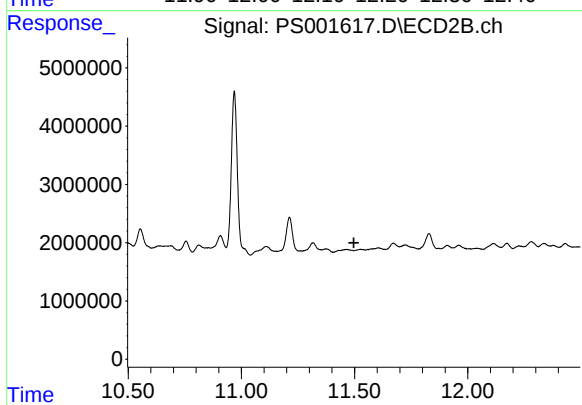

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.497 min
Response: 0
Conc: N.D.

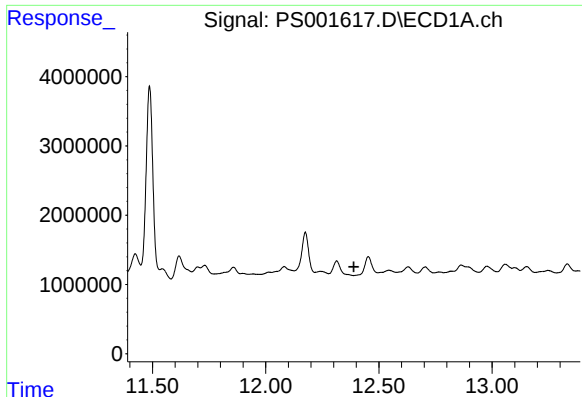

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.390 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

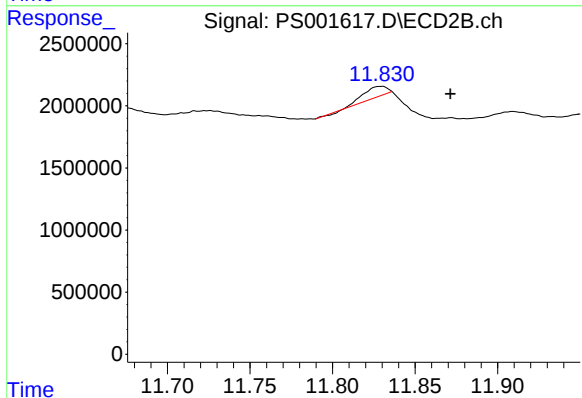


#7 MCPA

R.T.: 11.829 min
Delta R.T.: -0.042 min
Response: 1010445
Conc: 1.39 ug/ml

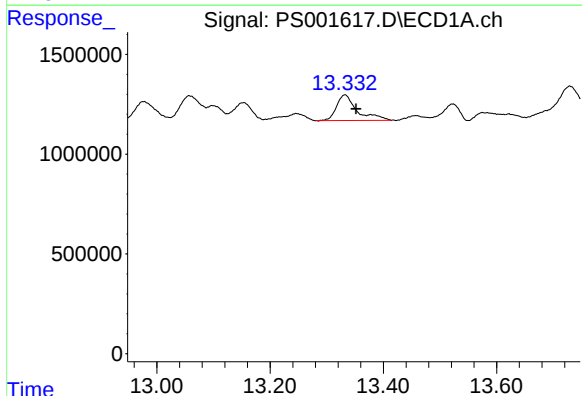


#9 2,4-D

R.T.: 13.332 min
Delta R.T.: -0.019 min
Response: 3253994
Conc: 13.72 ng/ml

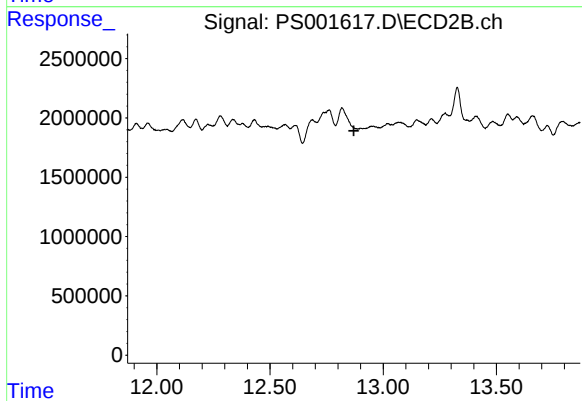

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 12.871 min
Response: 0
Conc: N.D.

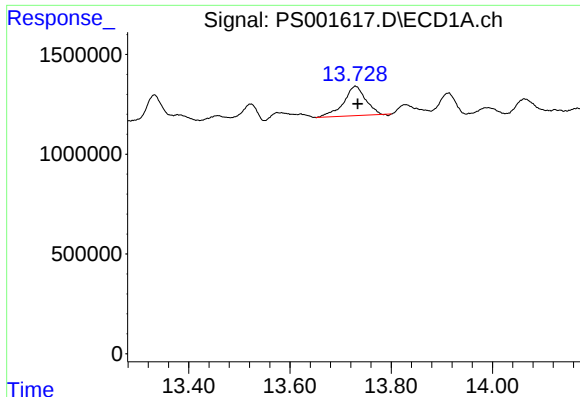

#10 Pentachlorophenol


R.T.: 13.729 min
Delta R.T.: -0.005 min
Response: 4459925
Conc: 1.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

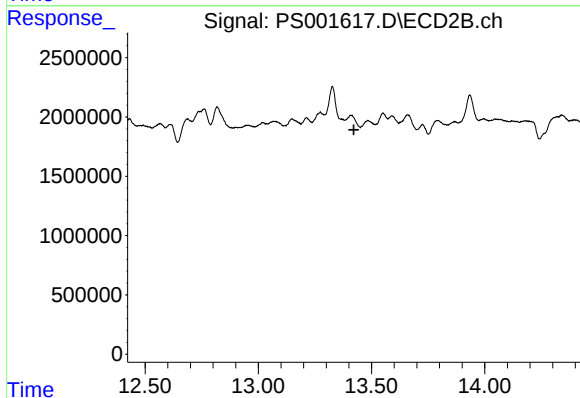


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.422 min
Response: 0
Conc: N.D.

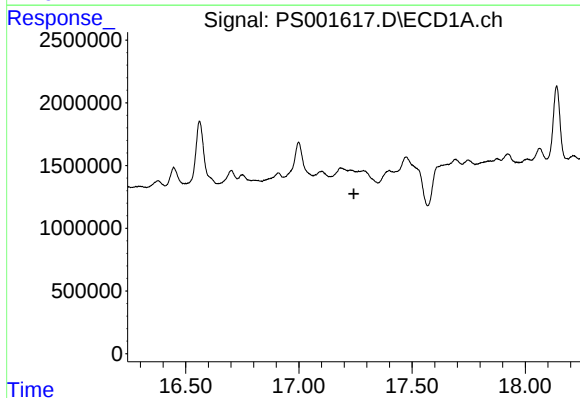


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.243 min
Response: 0
Conc: N.D.

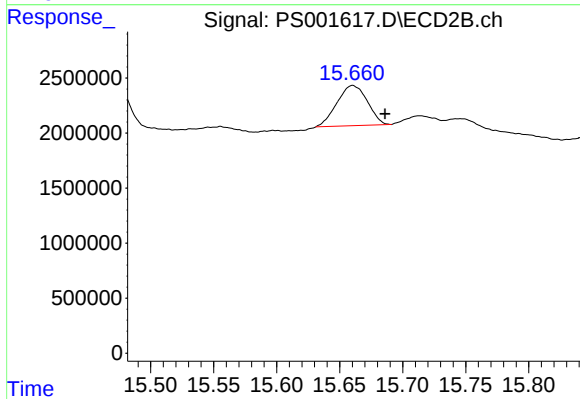

#14 DINOSEB


R.T.: 15.661 min
Delta R.T.: -0.025 min
Response: 6149236
Conc: 8.31 ng/ml

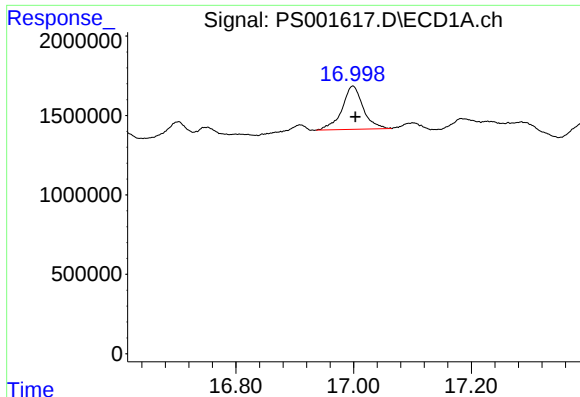

#15 Picloram


R.T.: 16.999 min
Delta R.T.: -0.004 min
Response: 6770265
Conc: 4.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

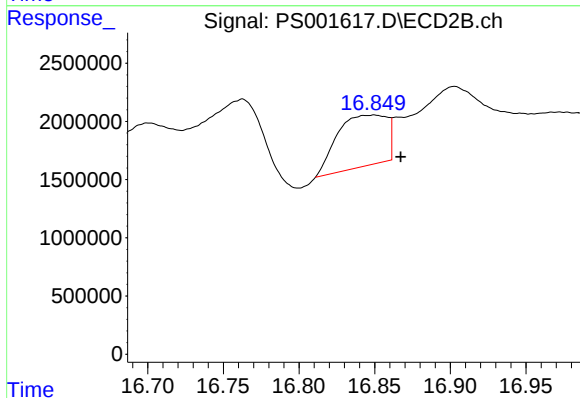


#15 Picloram

R.T.: 16.849 min
Delta R.T.: -0.018 min
Response: 10045390
Conc: 7.70 ng/ml

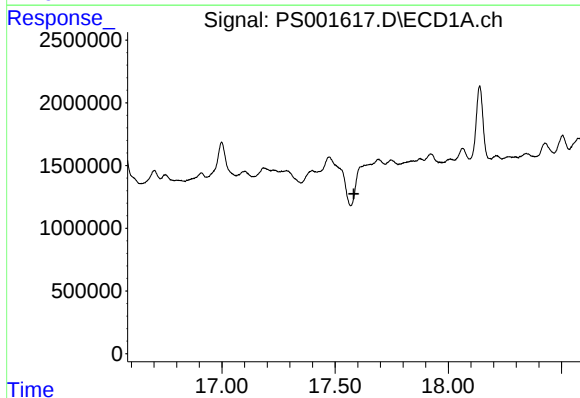

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.583 min
Response: 0
Conc: N.D.

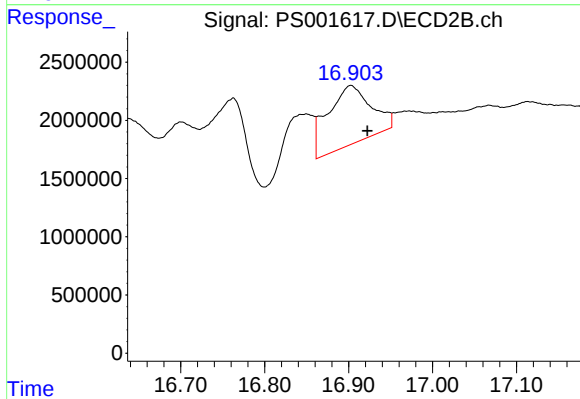

#16 DCPA

R.T.: 16.903 min
Delta R.T.: -0.020 min
Response: 18218819
Conc: 12.76 ng/ml