

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082719\
 Data File : PS006358.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2019 14:33
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 04:49:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.511	5.234	337.3E6	169.0E6	390.761	343.661
Target Compounds							
5) T	DICAMBA	0.000	5.386	0	178.5E6	N.D.	96.792
6) T	MCPD	0.000	5.386	0	178.5E6	N.D.	144.316
9) T	2,4-D	6.467	0.000	923.5E6	0	1133.478	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082719\
Data File : PS006358.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2019 14:33
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 04:49:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

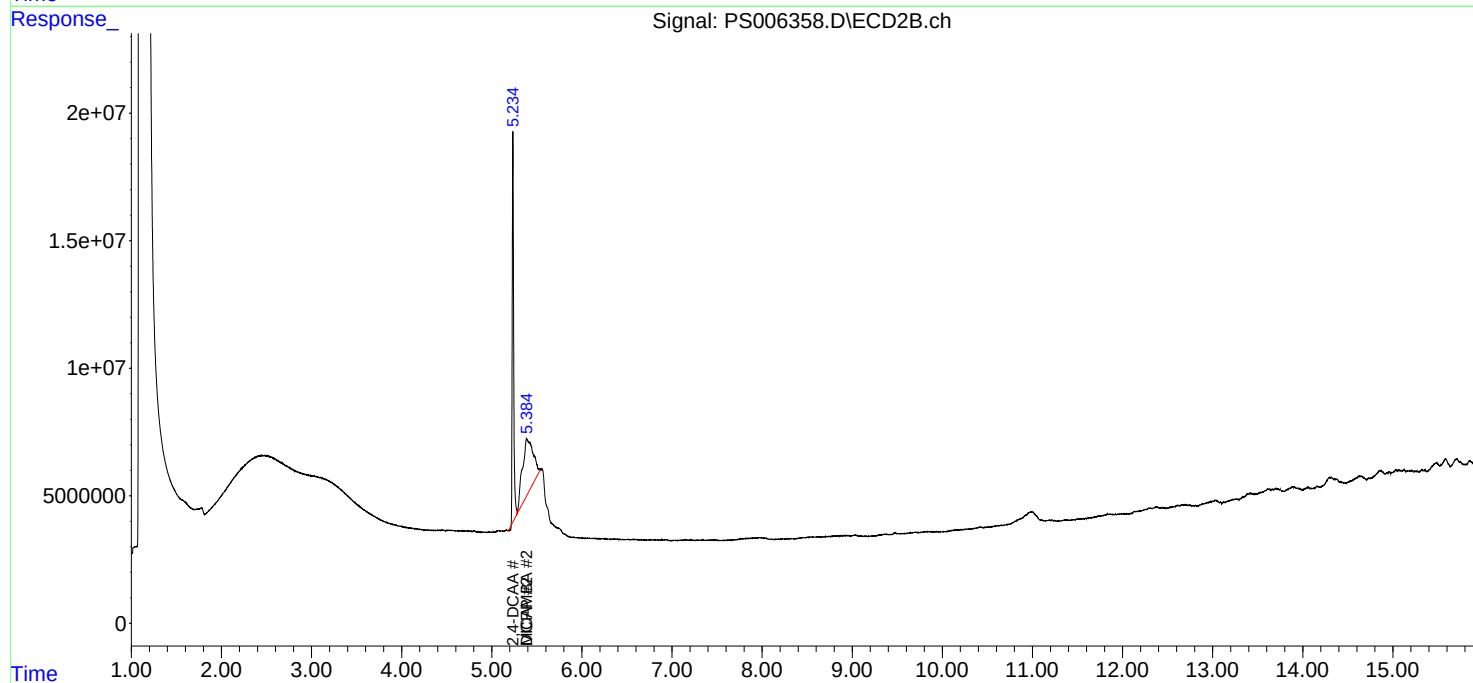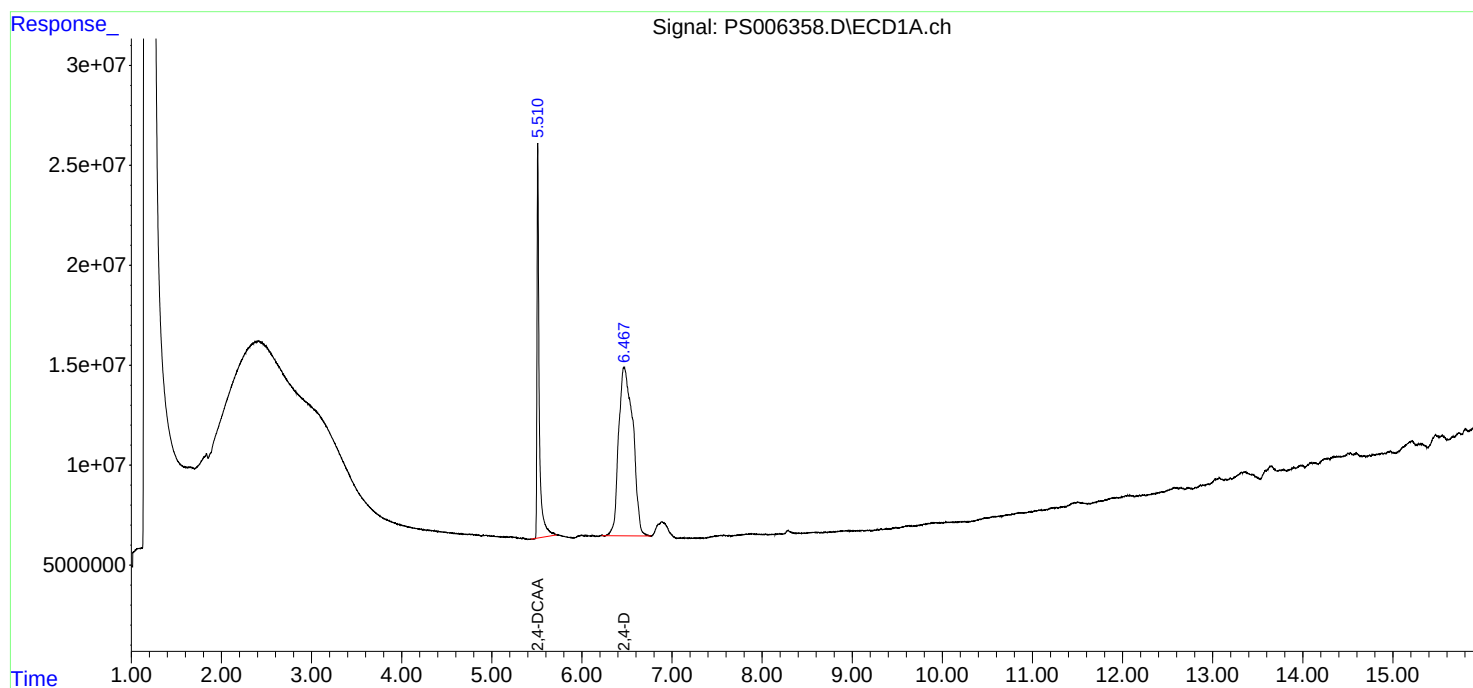


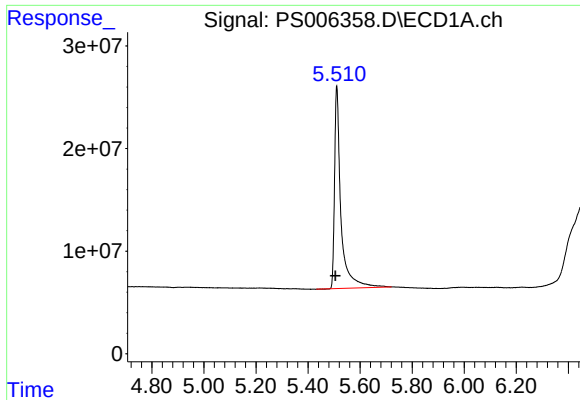

#4 2,4-DCAA


R.T.: 5.511 min
Delta R.T.: 0.006 min
Response: 337305265
Conc: 390.76 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

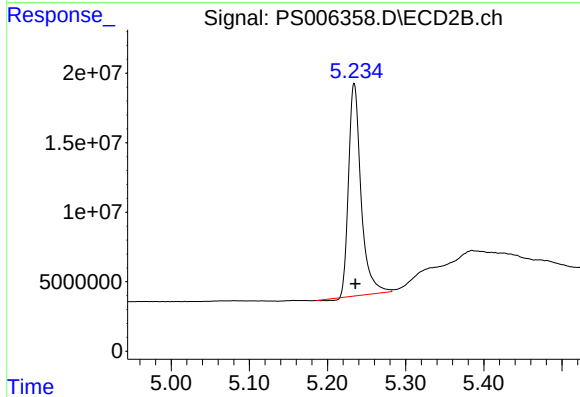


#4 2,4-DCAA

R.T.: 5.234 min
Delta R.T.: -0.001 min
Response: 169030383
Conc: 343.66 ng/ml

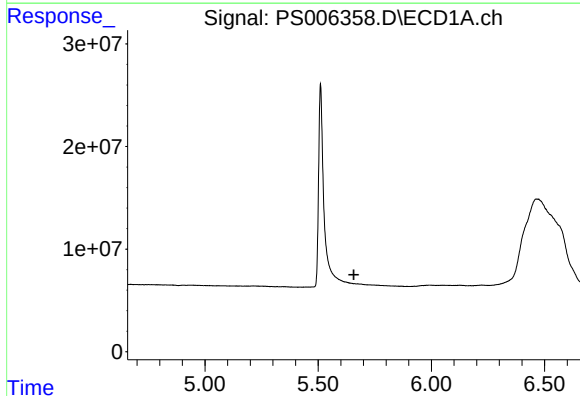


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.658 min
Response: 0
Conc: N.D.

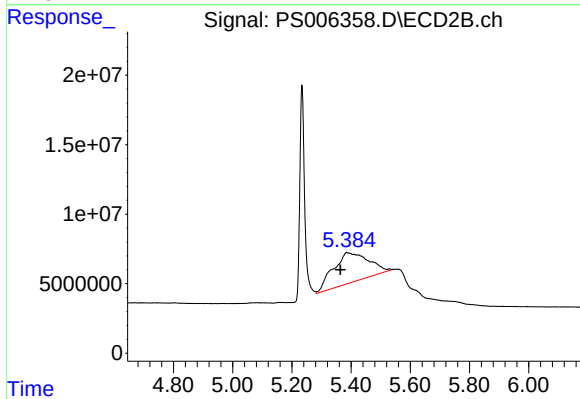

#5 DICAMBA


R.T.: 5.386 min
Delta R.T.: 0.022 min
Response: 178534174
Conc: 96.79 ng/ml

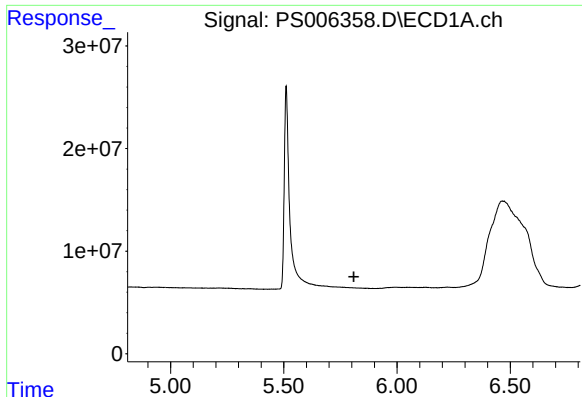

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.810 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

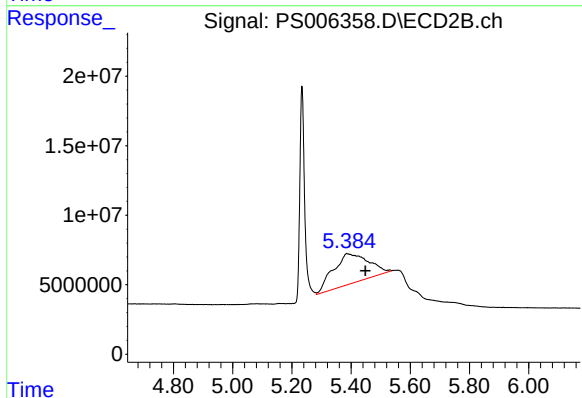


#6 MCP

R.T.: 5.386 min
Delta R.T.: -0.062 min
Response: 178534174
Conc: 144.32 ug/ml

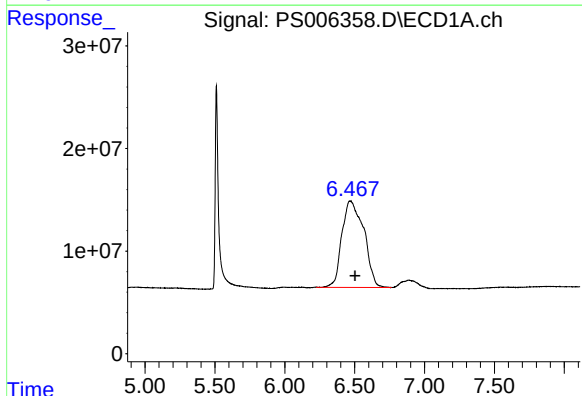

#9 2,4-D

R.T.: 6.467 min
Delta R.T.: -0.035 min
Response: 923540255
Conc: 1133.48 ng/ml

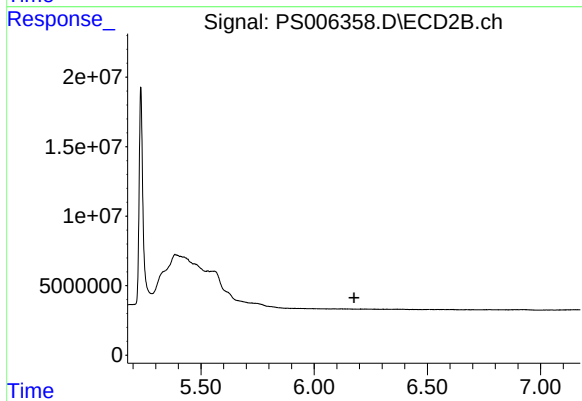

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.176 min
Response: 0
Conc: N.D.