

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082720\
 Data File : PS011960.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2020 11:13
 Operator : DD\AJ
 Sample : L3784-14RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 12:18:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.914	635.3E6	392.8E6	582.440	734.491 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	90589245	N.D.	110.123
3) T	4-Nitroph...	7.057	6.506	3778428	16174641	6.415	44.362 #
5) T	DICAMBA	7.397	7.049	8427295	15034908	2.057	6.959 #
6) T	MCP	7.630	0.000	7624761	0	2.386	N.D. #
7) T	MCPA	7.695	7.467	205.9E6	139.7E6	45.269	50.976
8) T	DICHLORPROP	0.000	7.739	0	29246958	N.D.	51.798
9) T	2,4-D	8.400	0.000	100.1E6	0	88.621	N.D. #
11) T	2,4,5-TP ...	0.000	8.763	0	21883103	N.D.	7.485
12) T	2,4,5-T	9.413	0.000	19365168	0	3.268	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082720\
Data File : PS011960.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2020 11:13
Operator : DD\AJ
Sample : L3784-14RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 12:18:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

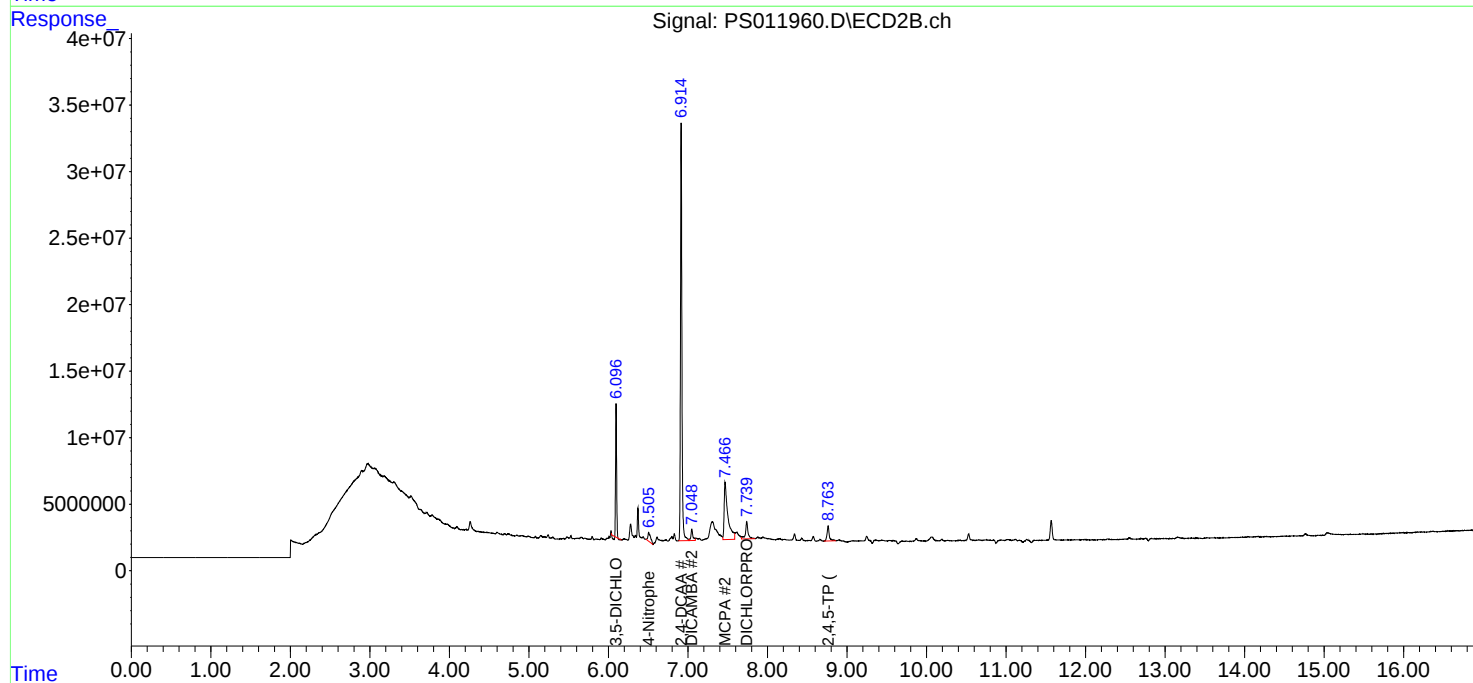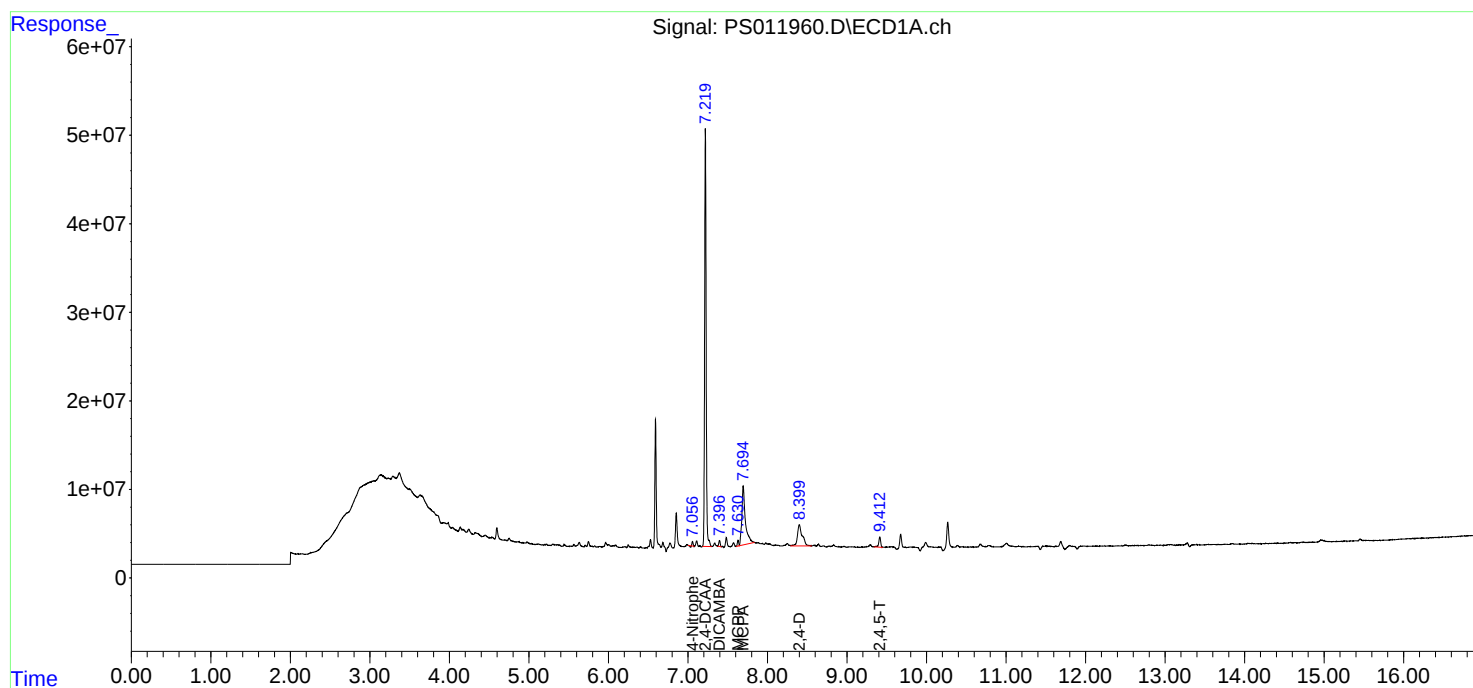


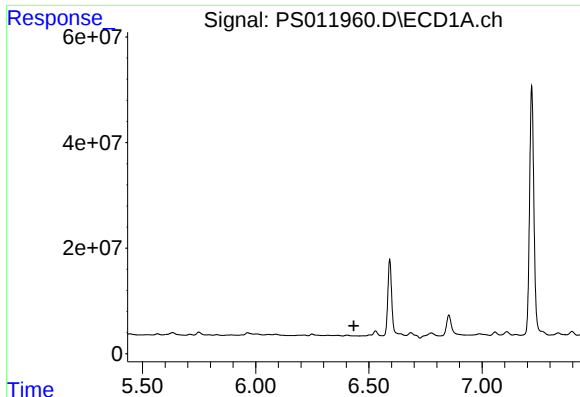

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

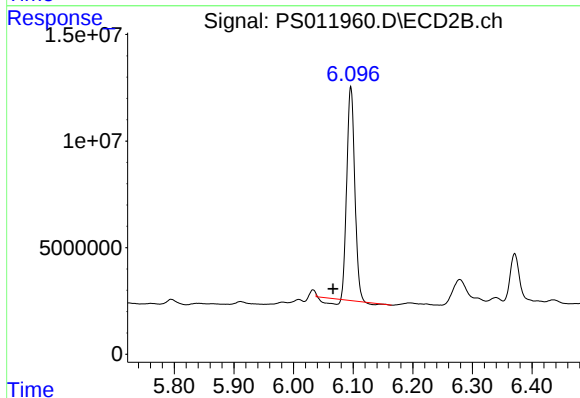


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.030 min
Response: 90589245
Conc: 110.12 ng/ml

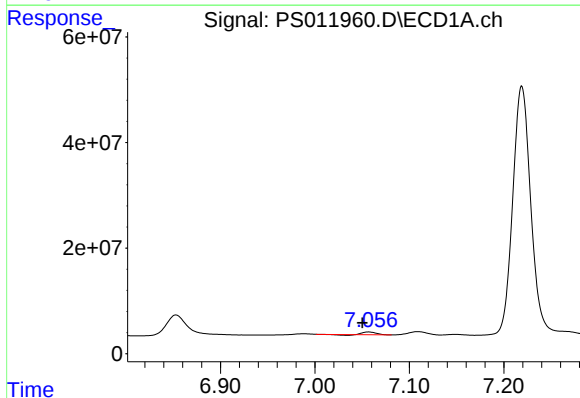


#3 4-Nitrophenol

R.T.: 7.057 min
Delta R.T.: 0.007 min
Response: 3778428
Conc: 6.41 ng/ml

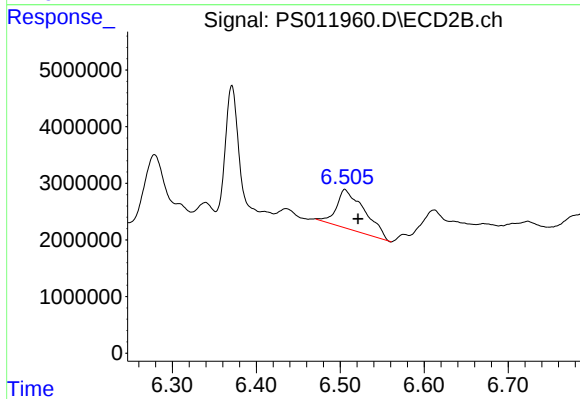

#3 4-Nitrophenol


R.T.: 6.506 min
Delta R.T.: -0.015 min
Response: 16174641
Conc: 44.36 ng/ml

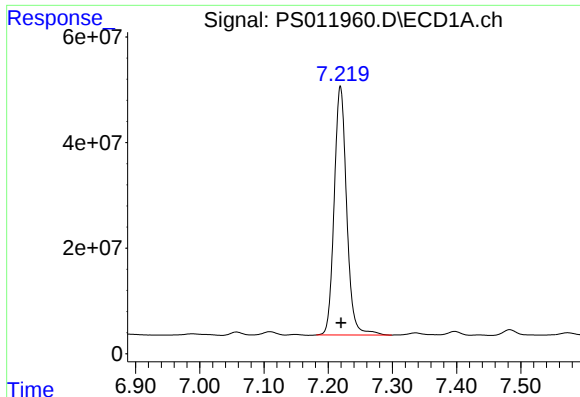

#4 2,4-DCAA


R.T.: 7.219 min
Delta R.T.: -0.001 min
Response: 635306672
Conc: 582.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

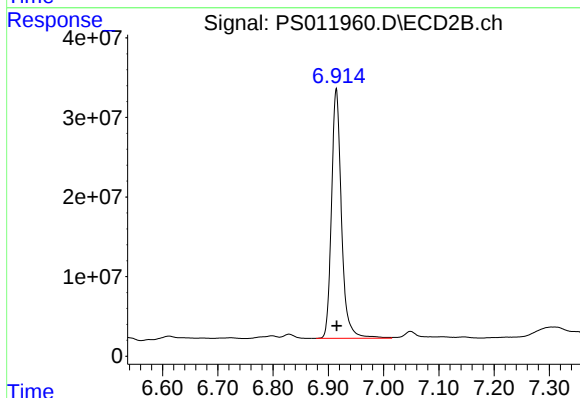


#4 2,4-DCAA

R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 392795810
Conc: 734.49 ng/ml

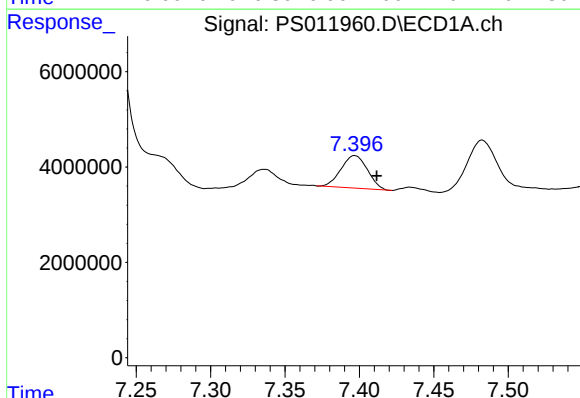


#5 DICAMBA

R.T.: 7.397 min
Delta R.T.: -0.015 min
Response: 8427295
Conc: 2.06 ng/ml

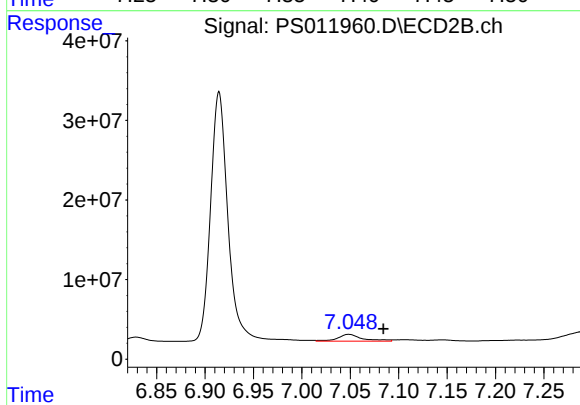

#5 DICAMBA


R.T.: 7.049 min
Delta R.T.: -0.036 min
Response: 15034908
Conc: 6.96 ng/ml

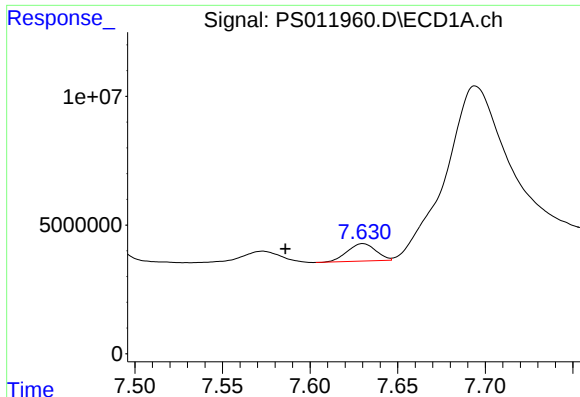

#6 MCPP


R.T.: 7.630 min
Delta R.T.: 0.044 min
Response: 7624761
Conc: 2.39 ug/ml

Instrument :
ECD_S
ClientSampleId :

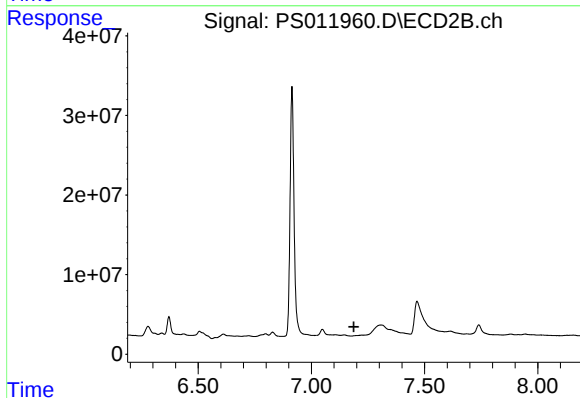


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

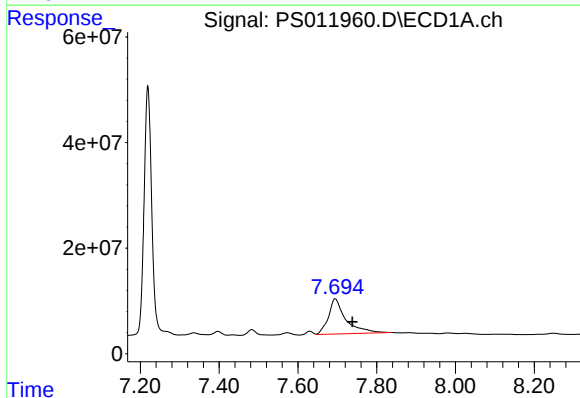


#7 MCPA

R.T.: 7.695 min
Delta R.T.: -0.044 min
Response: 205906672
Conc: 45.27 ug/ml

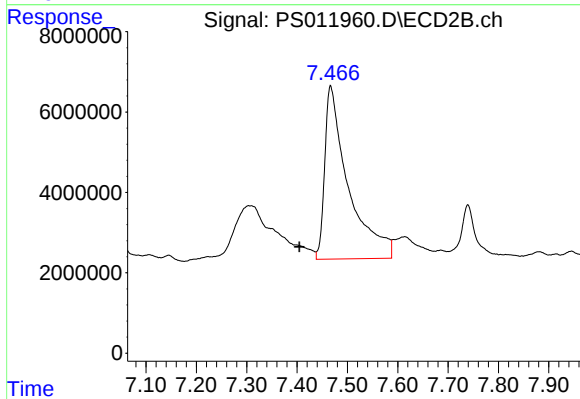

#7 MCPA


R.T.: 7.467 min
Delta R.T.: 0.062 min
Response: 139682830
Conc: 50.98 ug/ml

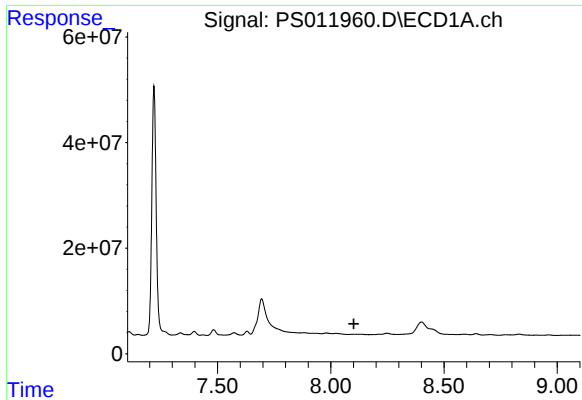

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

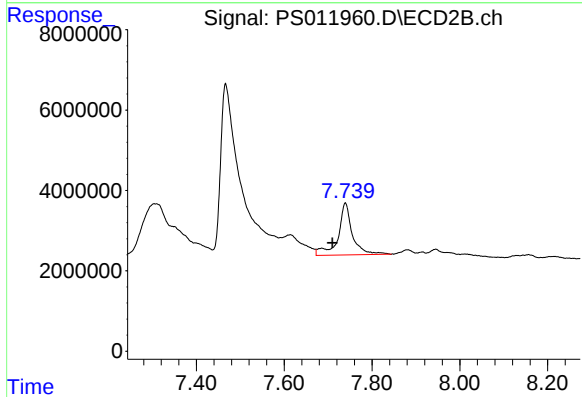


#8 DICHLORPROP

R.T.: 7.739 min
Delta R.T.: 0.030 min
Response: 29246958
Conc: 51.80 ng/ml

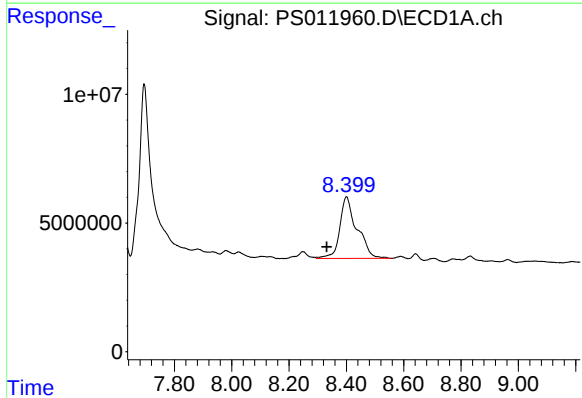


#9 2,4-D

R.T.: 8.400 min
Delta R.T.: 0.068 min
Response: 100060823
Conc: 88.62 ng/ml

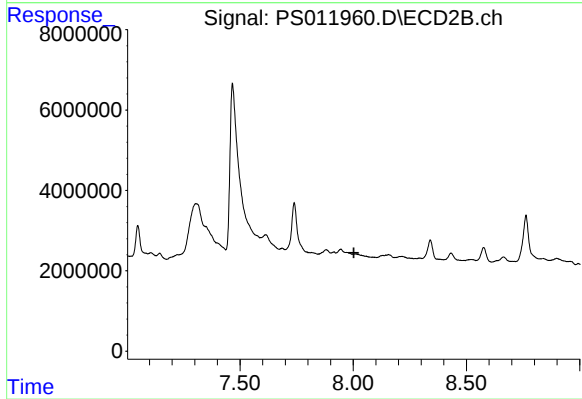

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

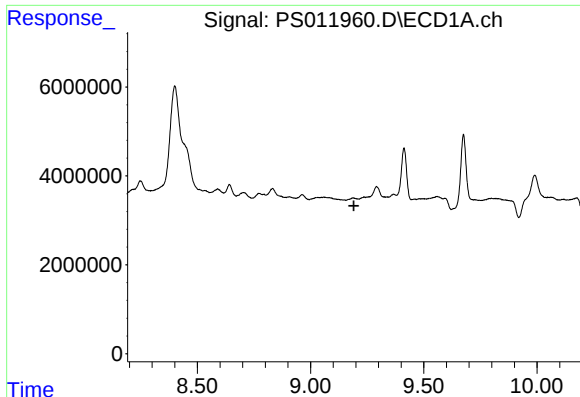

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

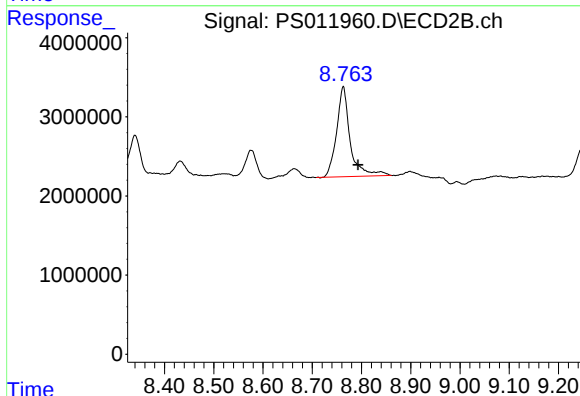


#11 2,4,5-TP (SILVEX)

R.T.: 8.763 min
Delta R.T.: -0.030 min
Response: 21883103
Conc: 7.48 ng/ml

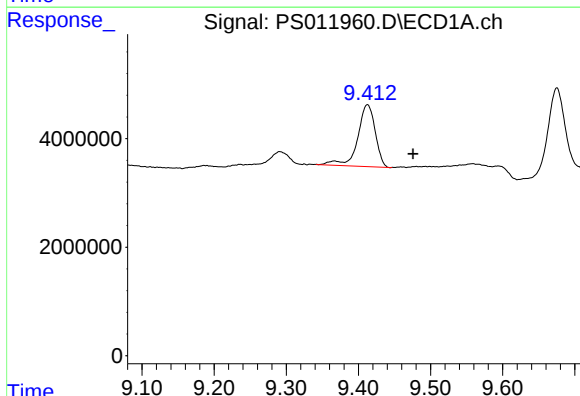

#12 2,4,5-T

R.T.: 9.413 min
Delta R.T.: -0.063 min
Response: 19365168
Conc: 3.27 ng/ml

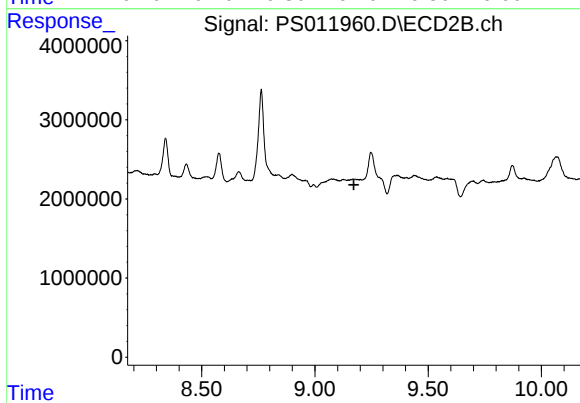

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.