

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082720\
 Data File : PS011961.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2020 11:36
 Operator : DD\AJ
 Sample : L3784-17RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 12:18:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.218	6.914	836.7E6	512.1E6	767.098	957.515
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	95800246	N.D.	116.457
3) T	4-Nitroph...	7.056	6.506	4158640	16156378	7.060	44.311 #
5) T	DICAMBA	7.396	7.049	8504468	15203948	2.076	7.037 #
6) T	MCP	7.629	0.000	8913754	0	2.790	N.D. #
7) T	MCPA	7.692	7.466	233.2E6	158.5E6	51.273	57.860
8) T	DICHLORPROP	0.000	7.739	0	30079149	N.D.	53.272
9) T	2,4-D	8.401	0.000	98040677	0	86.831	N.D. #
11) T	2,4,5-TP ...	0.000	8.763	0	17862834	N.D.	6.110
12) T	2,4,5-T	9.412	0.000	20645104	0	3.484	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082720\
Data File : PS011961.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2020 11:36
Operator : DD\AJ
Sample : L3784-17RE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 12:18:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

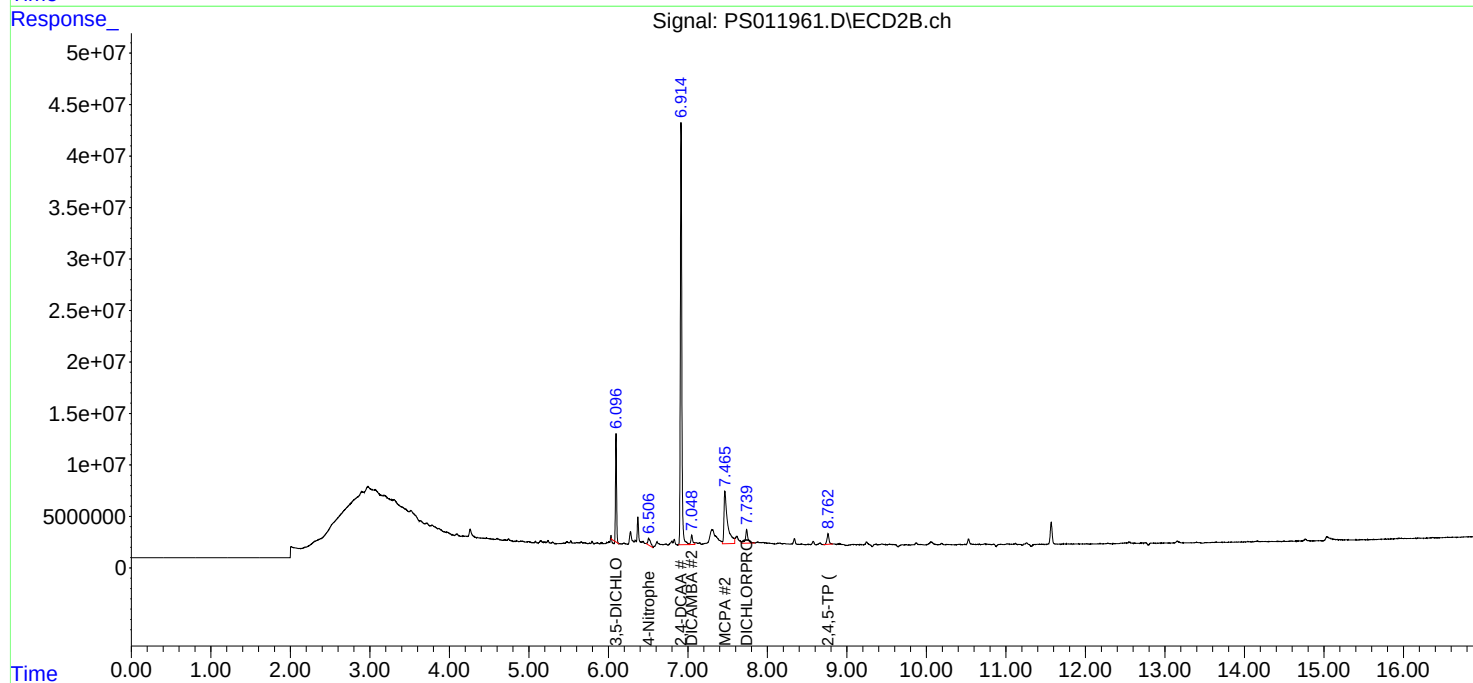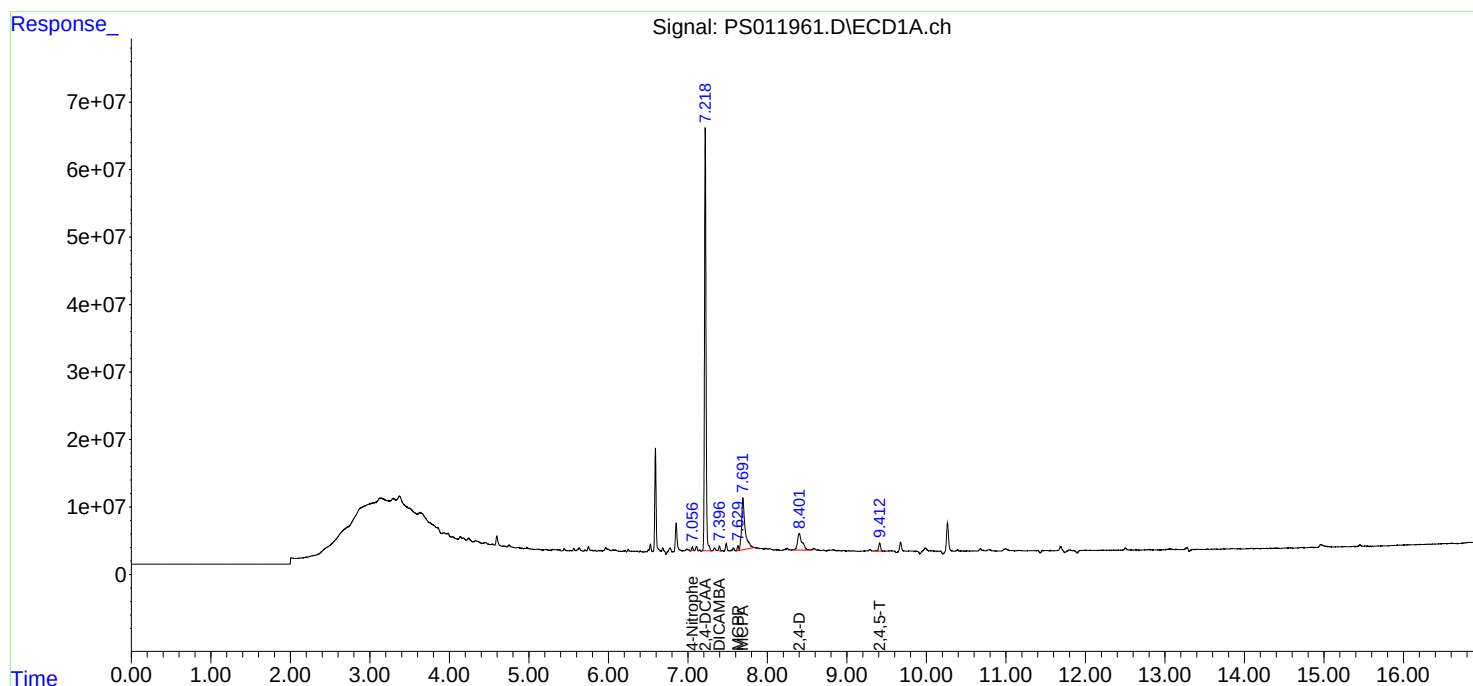


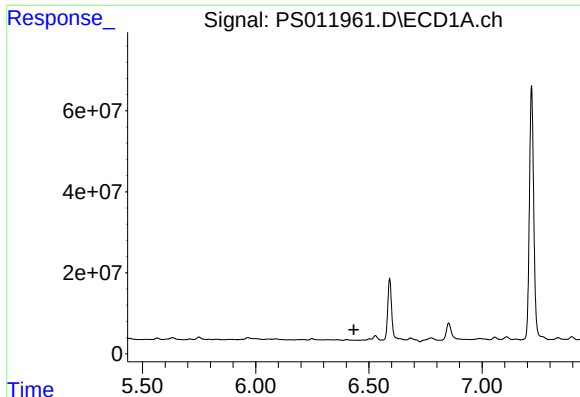

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

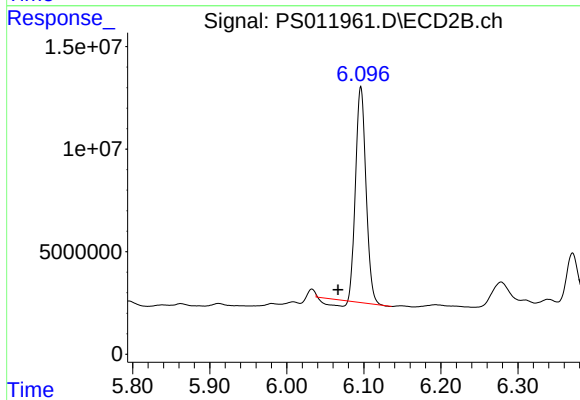


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.030 min
Response: 95800246
Conc: 116.46 ng/ml

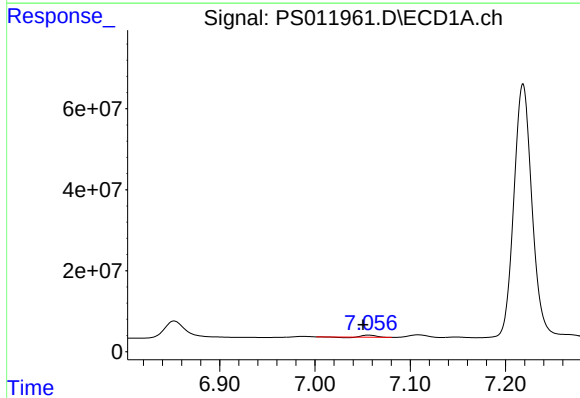


#3 4-Nitrophenol

R.T.: 7.056 min
Delta R.T.: 0.006 min
Response: 4158640
Conc: 7.06 ng/ml

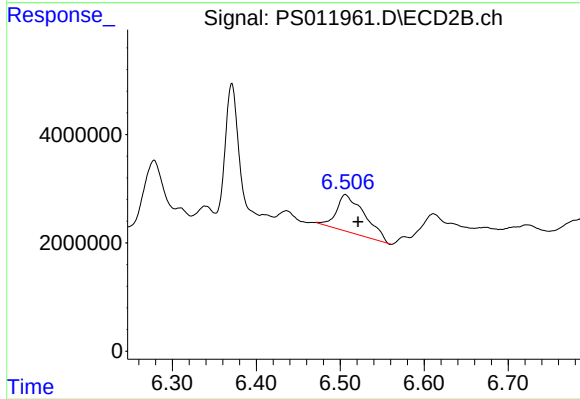

#3 4-Nitrophenol


R.T.: 6.506 min
Delta R.T.: -0.015 min
Response: 16156378
Conc: 44.31 ng/ml

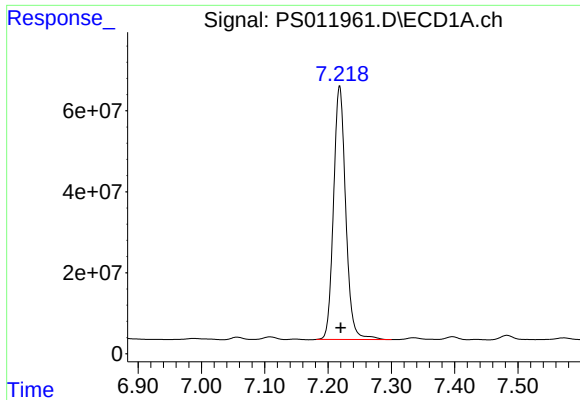

#4 2,4-DCAA


R.T.: 7.218 min
Delta R.T.: -0.002 min
Response: 836726718
Conc: 767.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

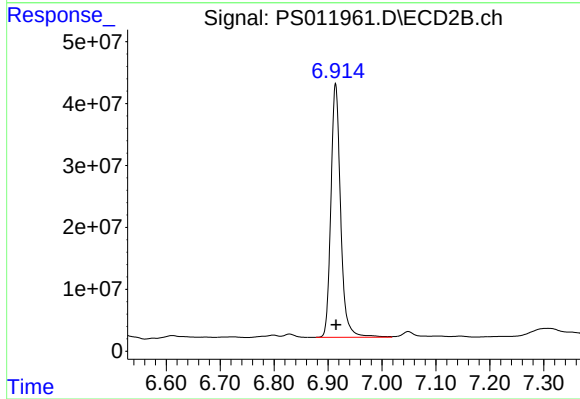


#4 2,4-DCAA

R.T.: 6.914 min
Delta R.T.: -0.001 min
Response: 512066543
Conc: 957.52 ng/ml

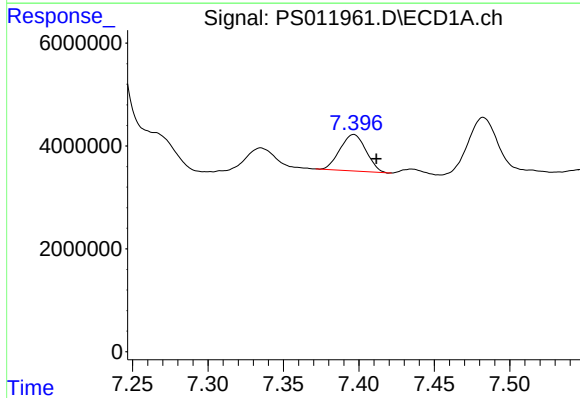


#5 DICAMBA

R.T.: 7.396 min
Delta R.T.: -0.015 min
Response: 8504468
Conc: 2.08 ng/ml

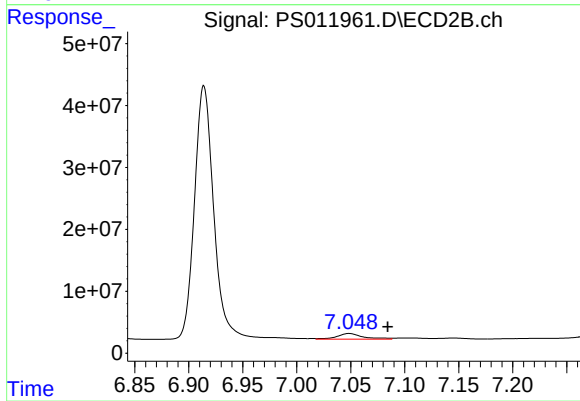

#5 DICAMBA


R.T.: 7.049 min
Delta R.T.: -0.036 min
Response: 15203948
Conc: 7.04 ng/ml

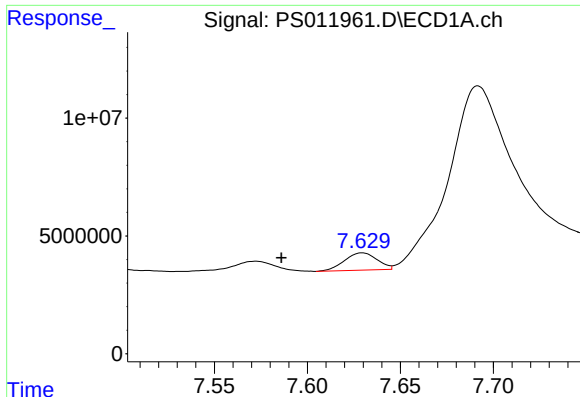

#6 MCPP


R.T.: 7.629 min
Delta R.T.: 0.043 min
Response: 8913754
Conc: 2.79 ug/ml

Instrument :
ECD_S
ClientSampleId :

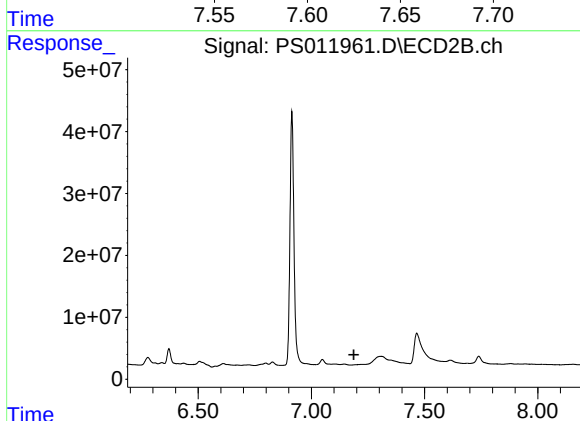


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

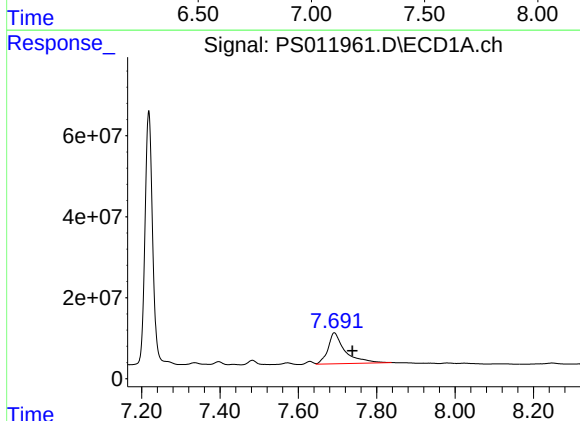


#7 MCPA

R.T.: 7.692 min
Delta R.T.: -0.046 min
Response: 233214672
Conc: 51.27 ug/ml

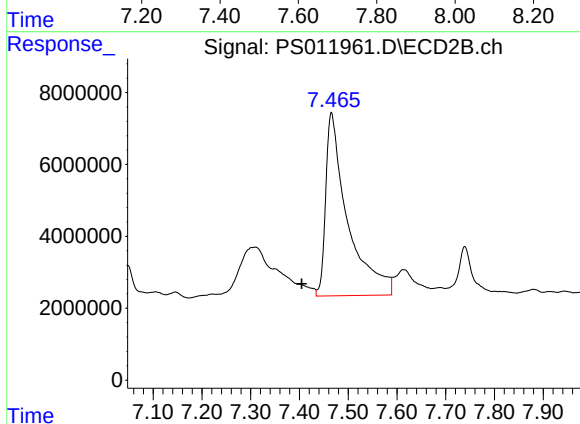

#7 MCPA


R.T.: 7.466 min
Delta R.T.: 0.061 min
Response: 158543664
Conc: 57.86 ug/ml

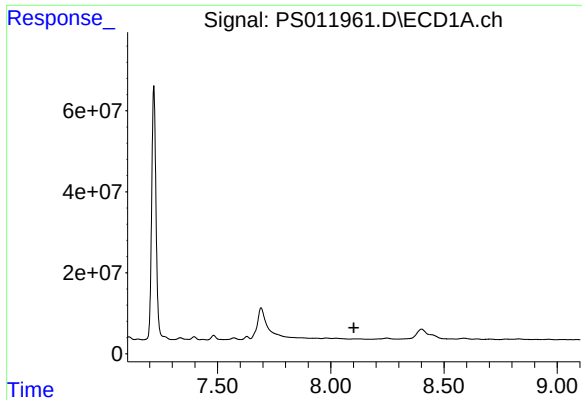

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

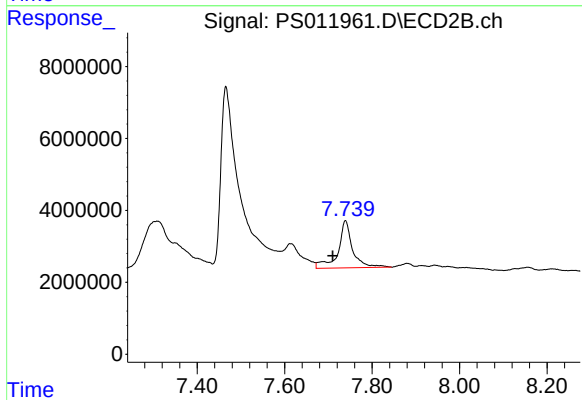


#8 DICHLORPROP

R.T.: 7.739 min
Delta R.T.: 0.030 min
Response: 30079149
Conc: 53.27 ng/ml

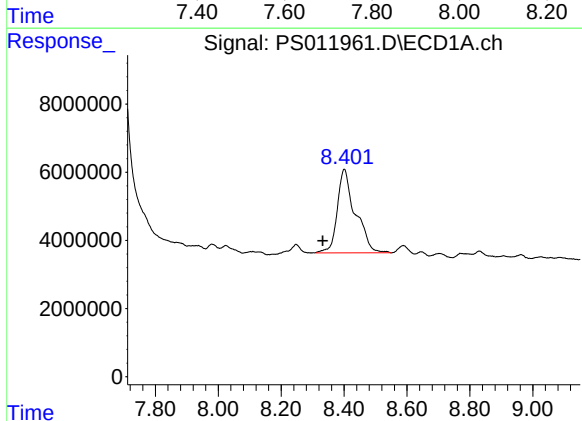


#9 2,4-D

R.T.: 8.401 min
Delta R.T.: 0.069 min
Response: 98040677
Conc: 86.83 ng/ml

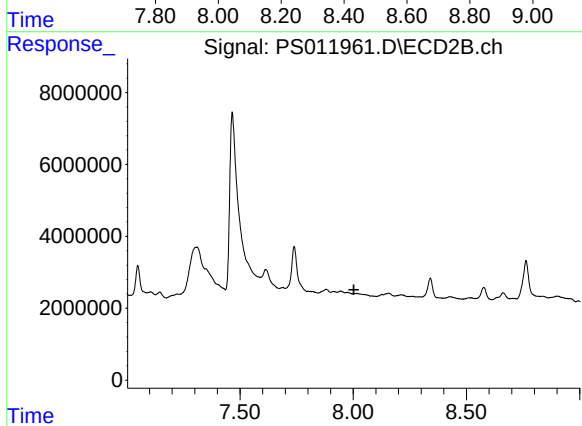

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

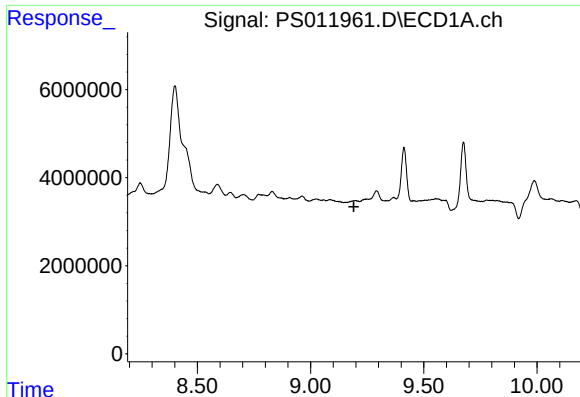

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

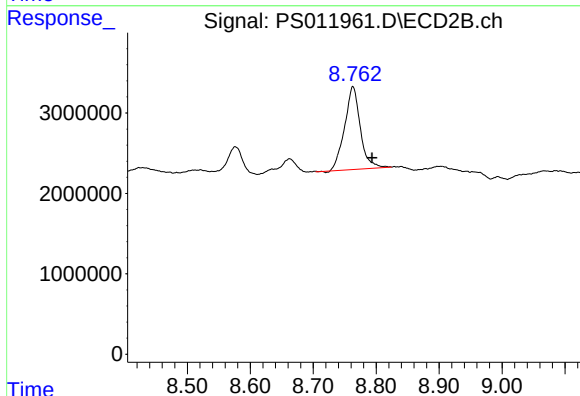


#11 2,4,5-TP (SILVEX)

R.T.: 8.763 min
Delta R.T.: -0.030 min
Response: 17862834
Conc: 6.11 ng/ml

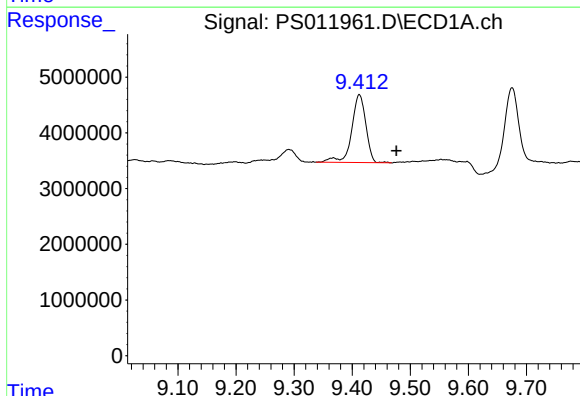

#12 2,4,5-T

R.T.: 9.412 min
Delta R.T.: -0.064 min
Response: 20645104
Conc: 3.48 ng/ml

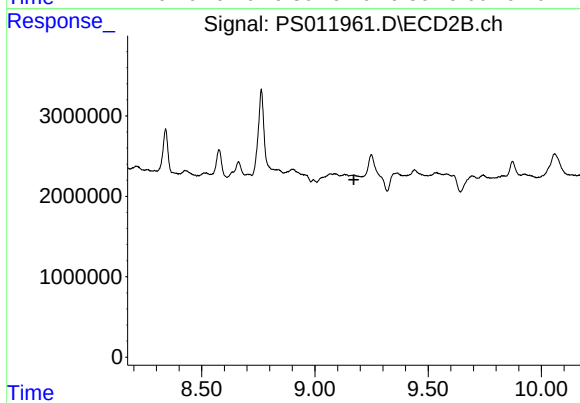

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.