

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082720\
 Data File : PS011962.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2020 11:59
 Operator : DD\AJ
 Sample : PB131211BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 12:18:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.220	6.916	460.0E6	277.7E6	421.761	519.227
Target Compounds							
2) T	3,5-DICHL...	0.000	6.097	0	89847182	N.D.	109.221
3) T	4-Nitroph...	7.057	6.508	3630350	20690795	6.163	56.748 #
5) T	DICAMBA	7.397	7.050	9397955	9055756	2.294	4.191 #
6) T	MCP	7.630	0.000	7894576	0	2.471	N.D. #
7) T	MCPA	7.766	7.376	23575450	31810119	5.183	11.609 #
8) T	DICHLORPROP	0.000	7.747	0	12205217	N.D.	21.616
9) T	2,4-D	8.399	0.000	112.1E6	0	99.287	N.D. #
11) T	2,4,5-TP ...	0.000	8.767	0	17645235	N.D.	6.035
12) T	2,4,5-T	9.414	0.000	16992960	0	2.868	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082720\
Data File : PS011962.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2020 11:59
Operator : DD\AJ
Sample : PB131211BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 12:18:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

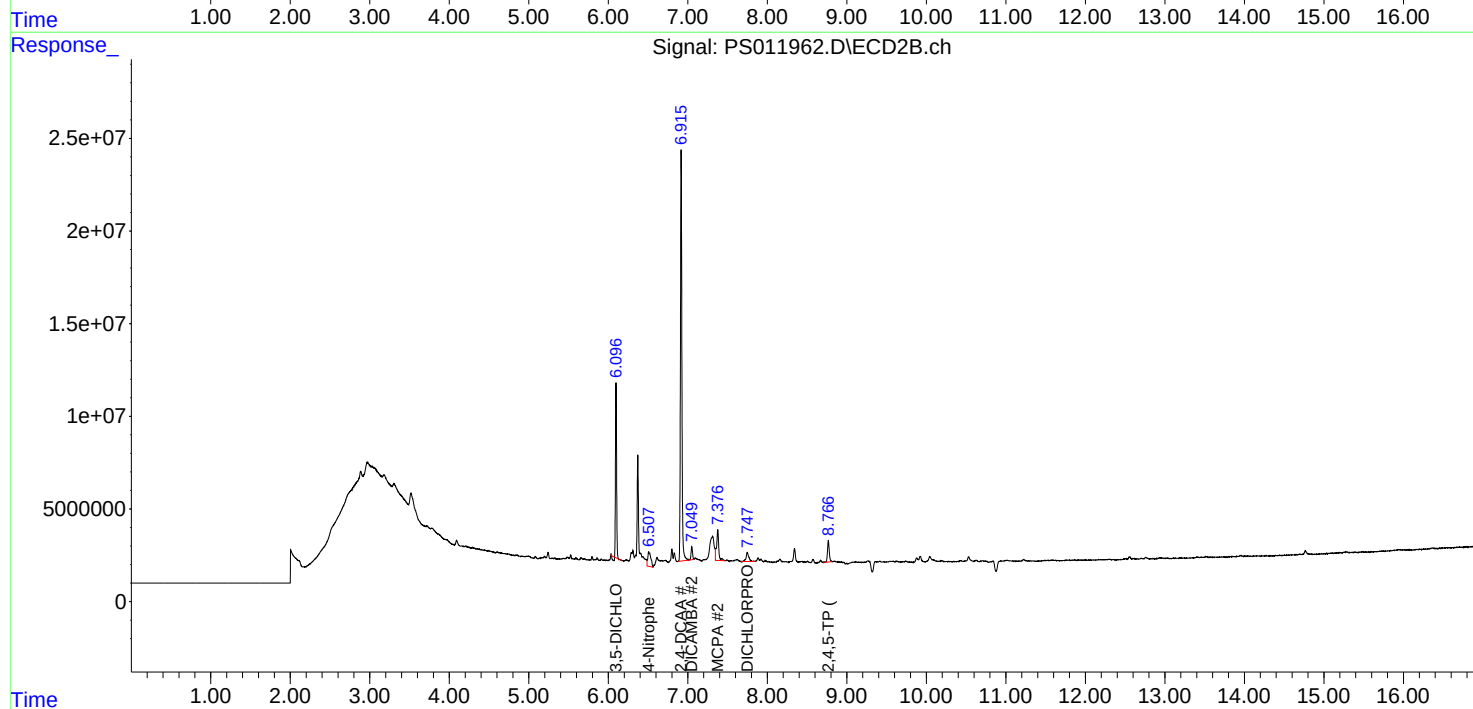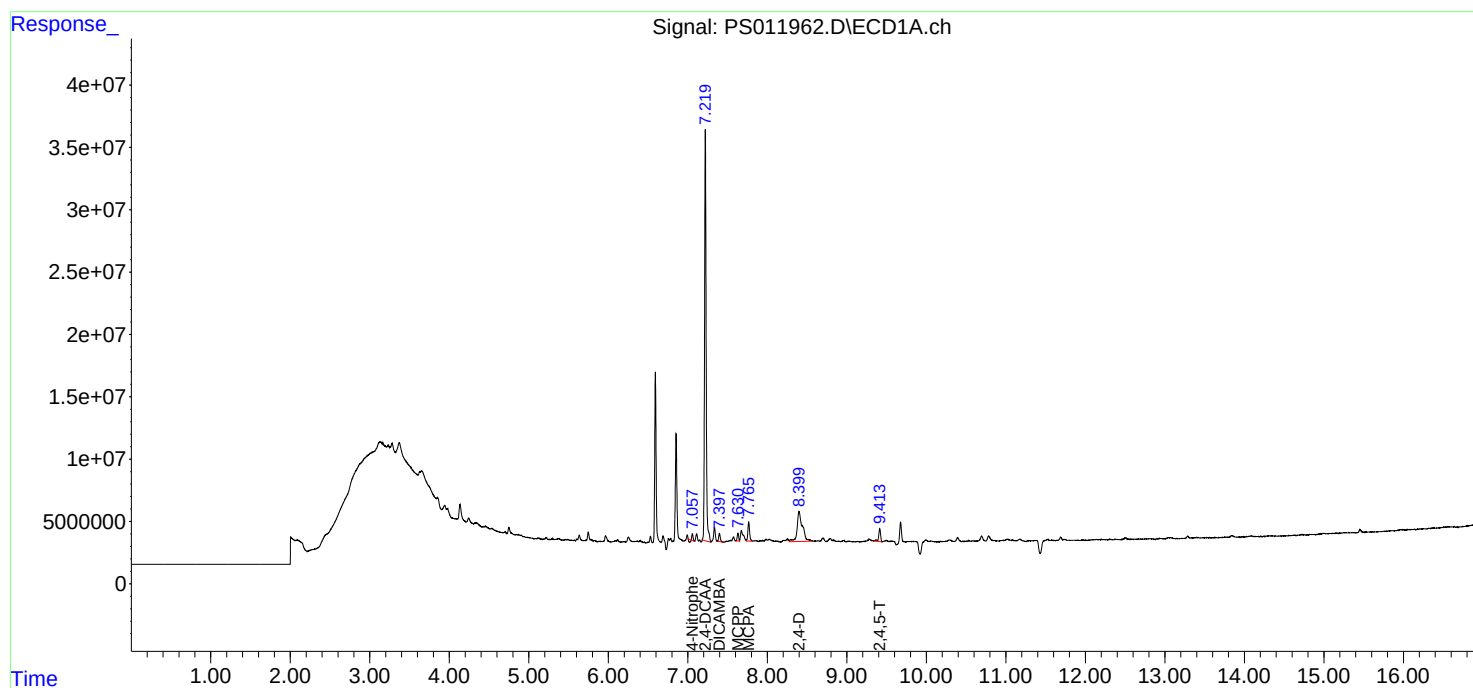


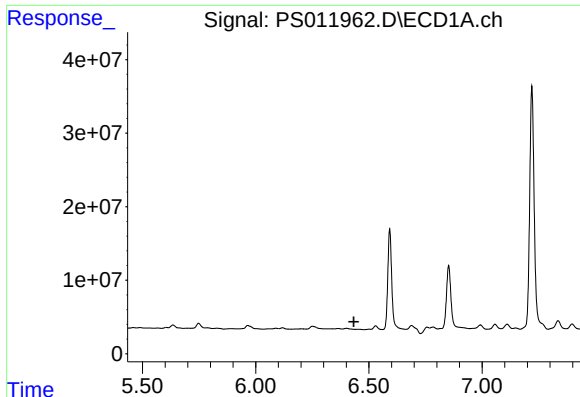

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

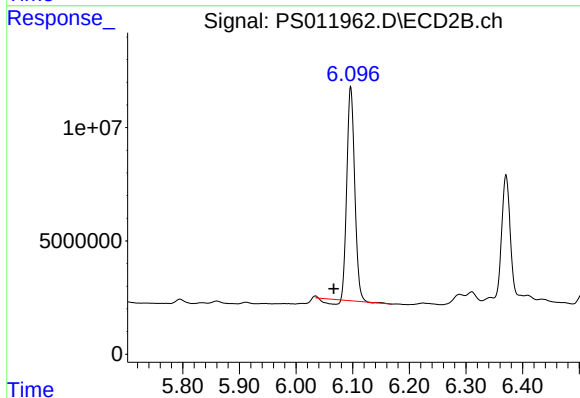


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.097 min
Delta R.T.: 0.030 min
Response: 89847182
Conc: 109.22 ng/ml

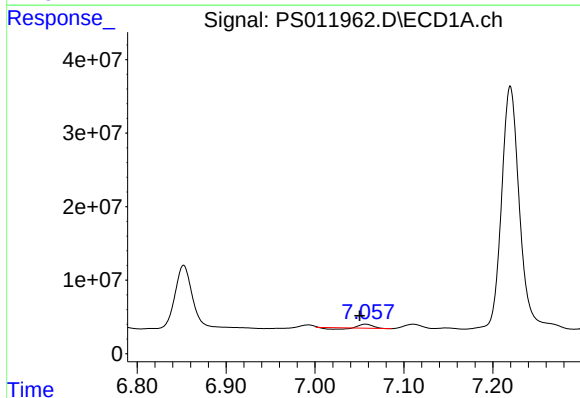


#3 4-Nitrophenol

R.T.: 7.057 min
Delta R.T.: 0.007 min
Response: 3630350
Conc: 6.16 ng/ml

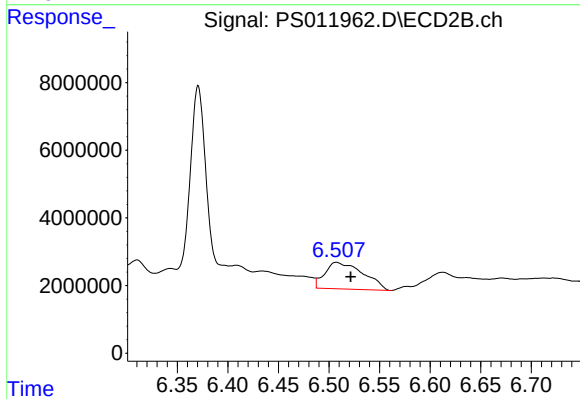

#3 4-Nitrophenol


R.T.: 6.508 min
Delta R.T.: -0.013 min
Response: 20690795
Conc: 56.75 ng/ml

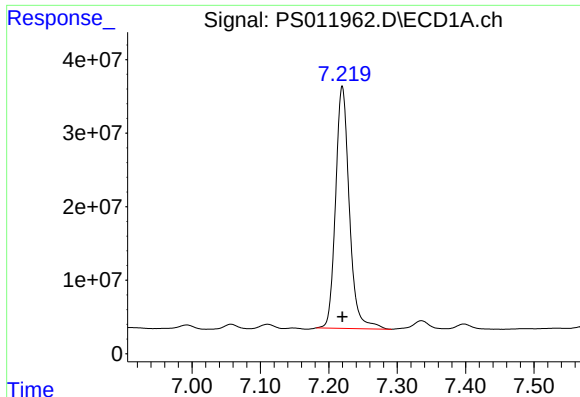

#4 2,4-DCAA


R.T.: 7.220 min
Delta R.T.: 0.000 min
Response: 460043648
Conc: 421.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

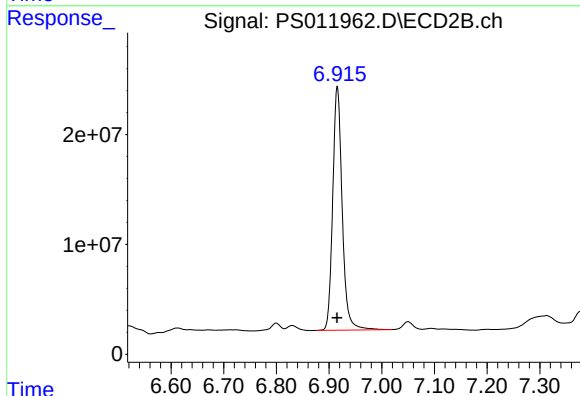


#4 2,4-DCAA

R.T.: 6.916 min
Delta R.T.: 0.000 min
Response: 277675910
Conc: 519.23 ng/ml

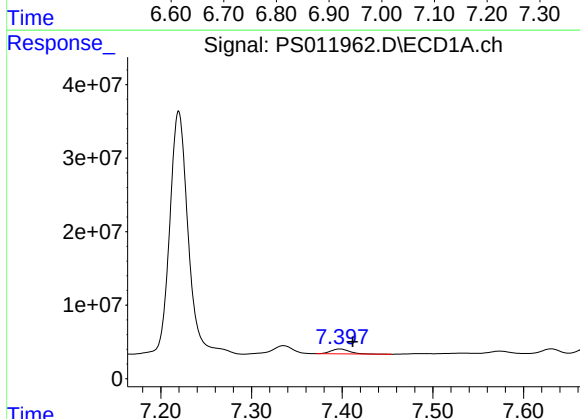


#5 DICAMBA

R.T.: 7.397 min
Delta R.T.: -0.014 min
Response: 9397955
Conc: 2.29 ng/ml

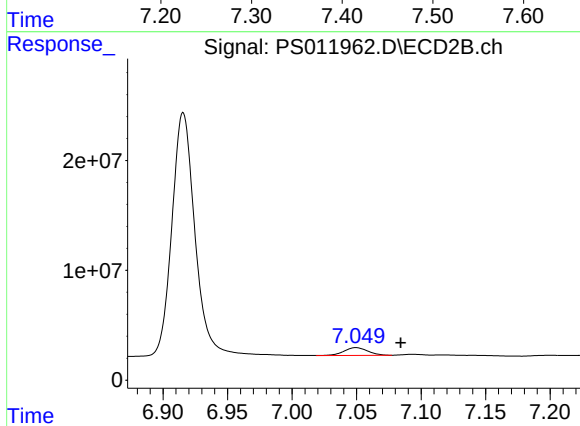

#5 DICAMBA


R.T.: 7.050 min
Delta R.T.: -0.035 min
Response: 9055756
Conc: 4.19 ng/ml

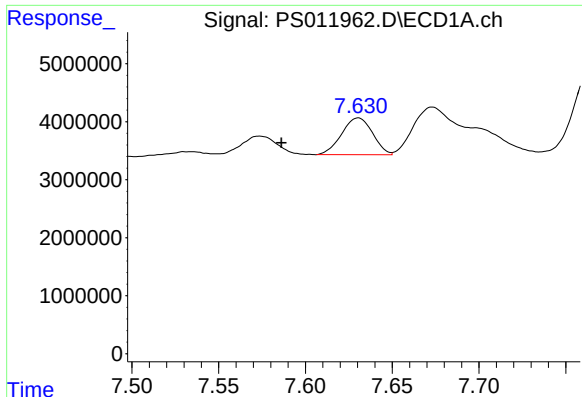

#6 MCPP


R.T.: 7.630 min
Delta R.T.: 0.044 min
Response: 7894576
Conc: 2.47 ug/ml

Instrument :
ECD_S
ClientSampleId :

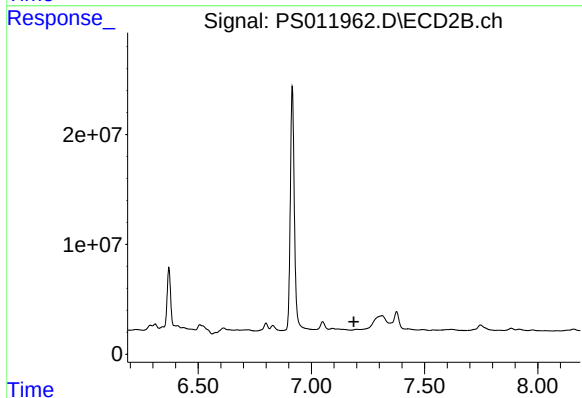


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

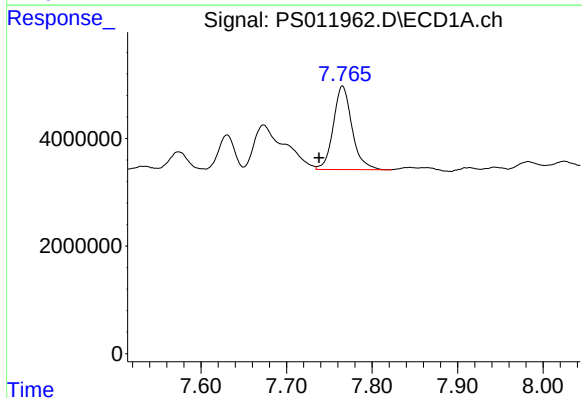


#7 MCPA

R.T.: 7.766 min
Delta R.T.: 0.027 min
Response: 23575450
Conc: 5.18 ug/ml

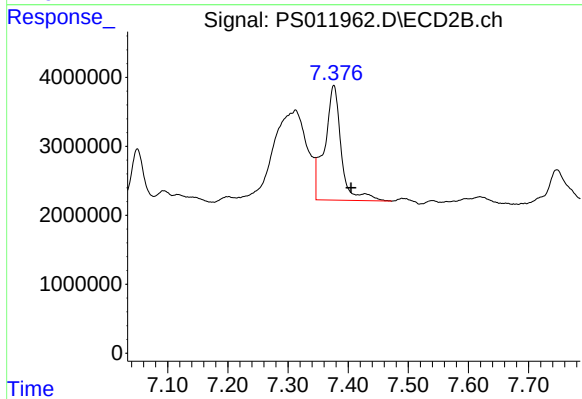

#7 MCPA


R.T.: 7.376 min
Delta R.T.: -0.029 min
Response: 31810119
Conc: 11.61 ug/ml

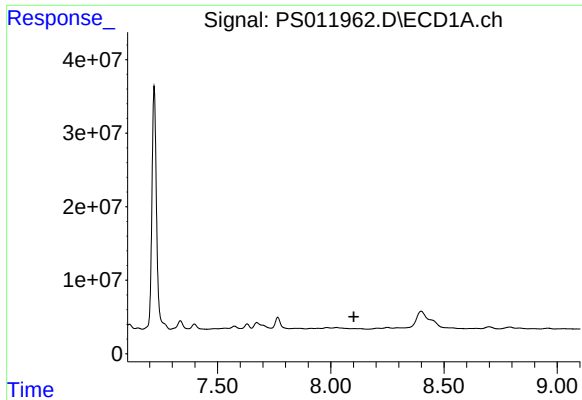

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

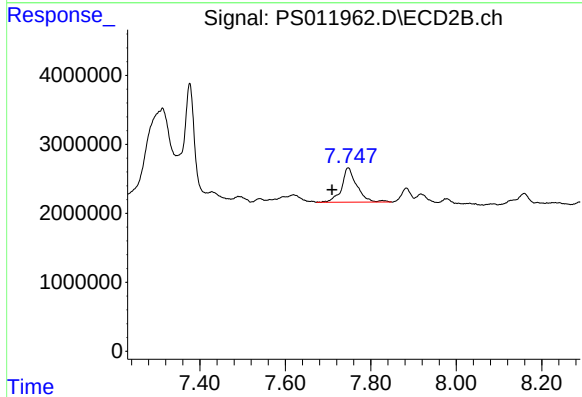


#8 DICHLORPROP

R.T.: 7.747 min
Delta R.T.: 0.038 min
Response: 12205217
Conc: 21.62 ng/ml

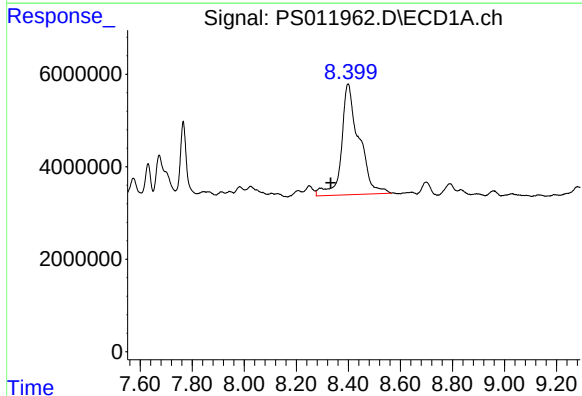


#9 2,4-D

R.T.: 8.399 min
Delta R.T.: 0.067 min
Response: 112104210
Conc: 99.29 ng/ml

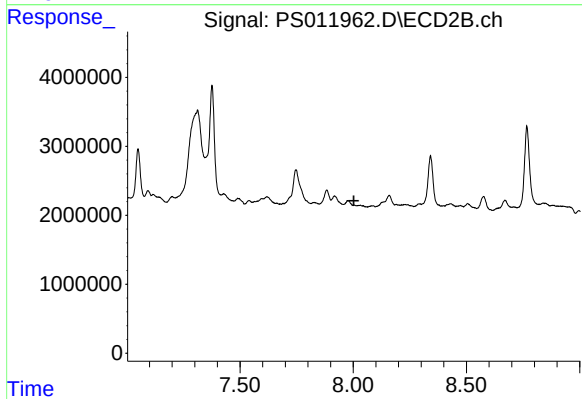

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

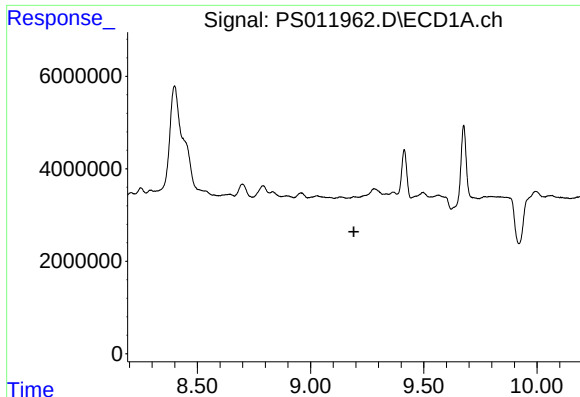

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

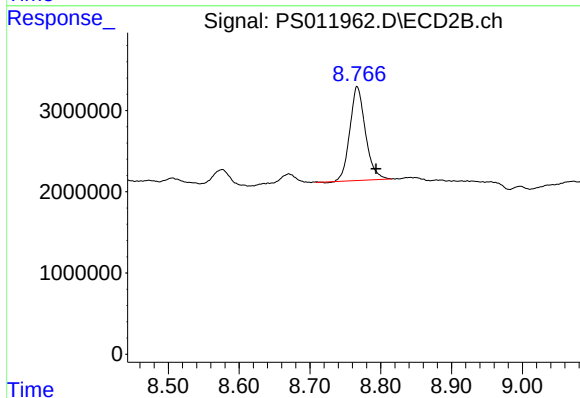


#11 2,4,5-TP (SILVEX)

R.T.: 8.767 min
Delta R.T.: -0.026 min
Response: 17645235
Conc: 6.04 ng/ml

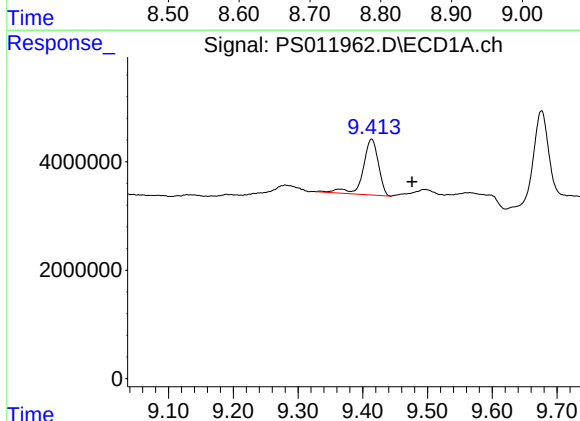

#12 2,4,5-T

R.T.: 9.414 min
Delta R.T.: -0.062 min
Response: 16992960
Conc: 2.87 ng/ml

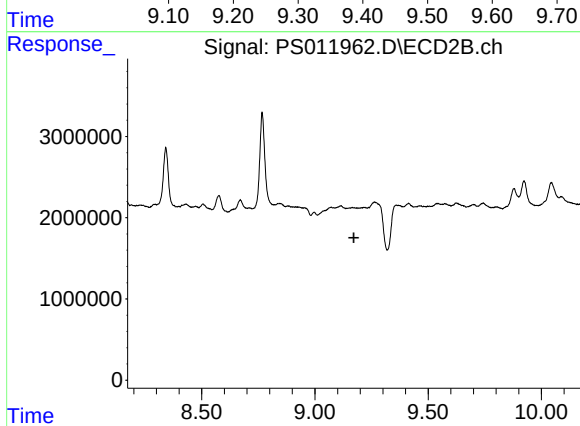

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.