

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082819\
 Data File : PS006364.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2019 12:47
 Operator : SM\AJ
 Sample : PB122601BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB122601BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 15:16:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.513	5.231	255.2E6	145.8E6	295.647	296.440
Target Compounds							
7) T	MCPA	0.000	5.558	0	98240249	N.D.	48.069
9) T	2,4-D	6.563	0.000	261.5E6	0	320.982	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082819\
Data File : PS006364.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2019 12:47
Operator : SM\AJ
Sample : PB122601BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB122601BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 15:16:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

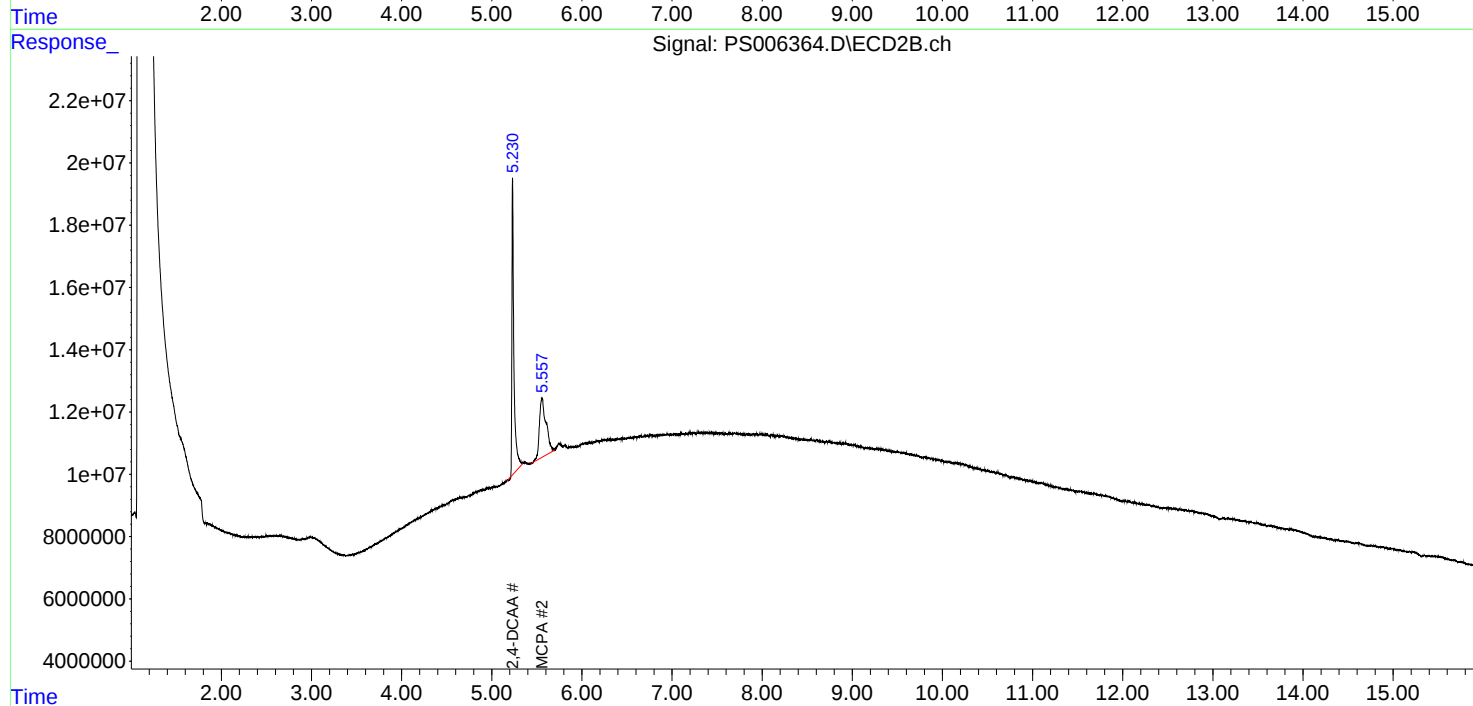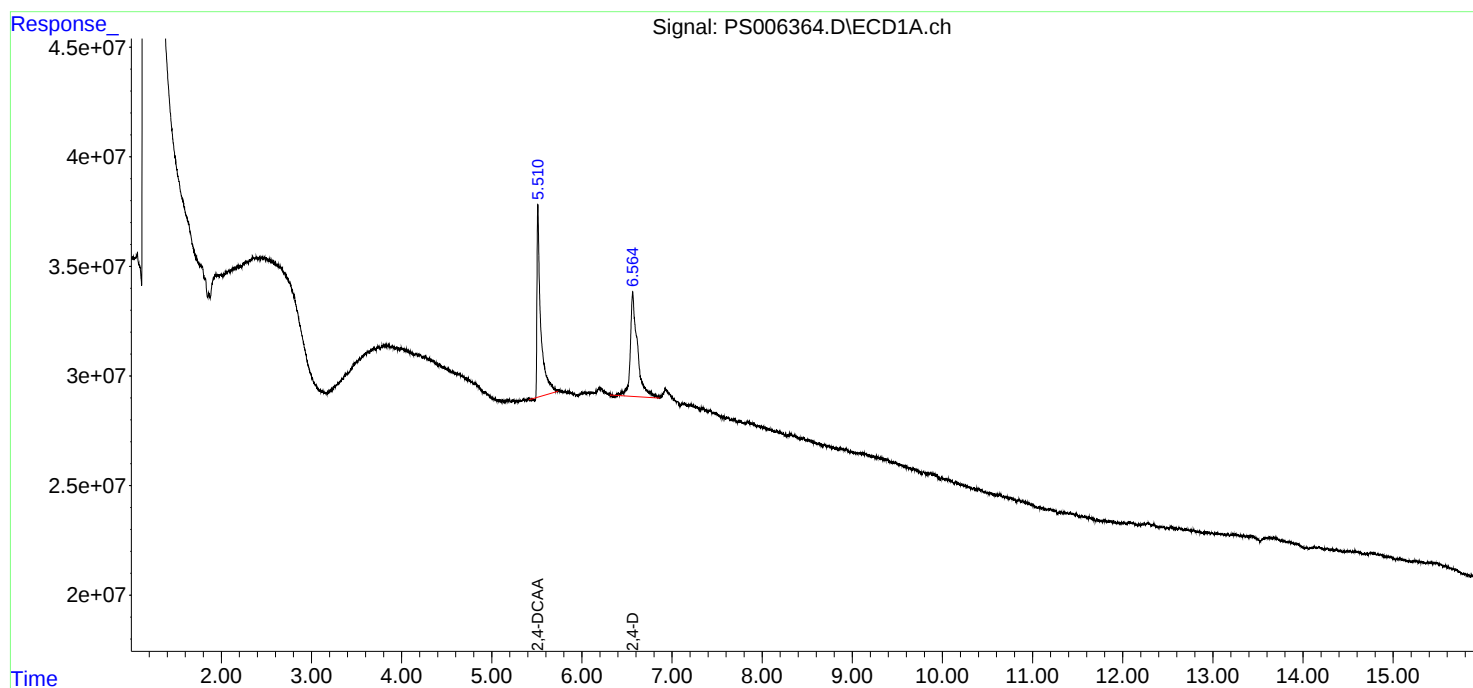


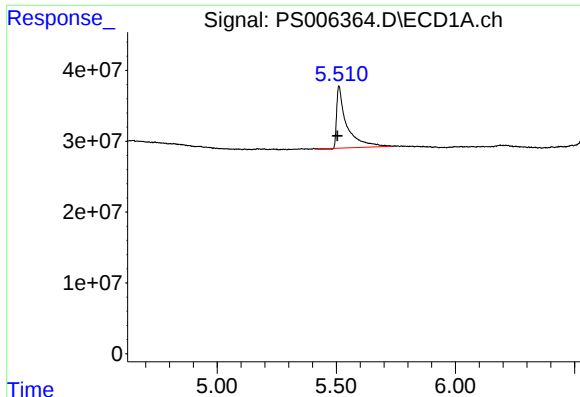

#4 2,4-DCAA


R.T.: 5.513 min
Delta R.T.: 0.008 min
Response: 255202903
Conc: 295.65 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB122601BL

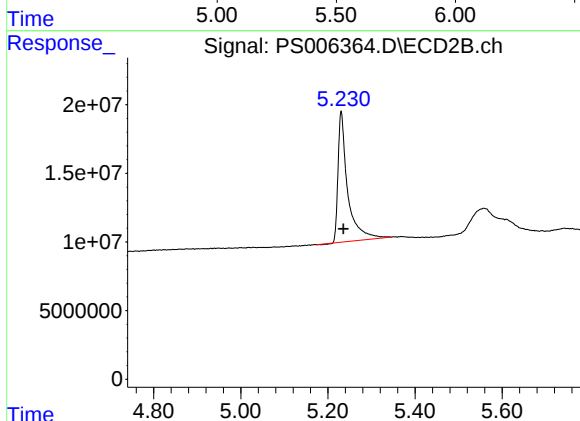


#4 2,4-DCAA

R.T.: 5.231 min
Delta R.T.: -0.005 min
Response: 145804794
Conc: 296.44 ng/ml

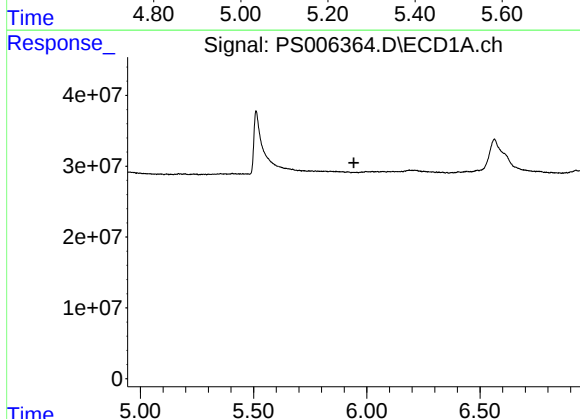


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.943 min
Response: 0
Conc: N.D.

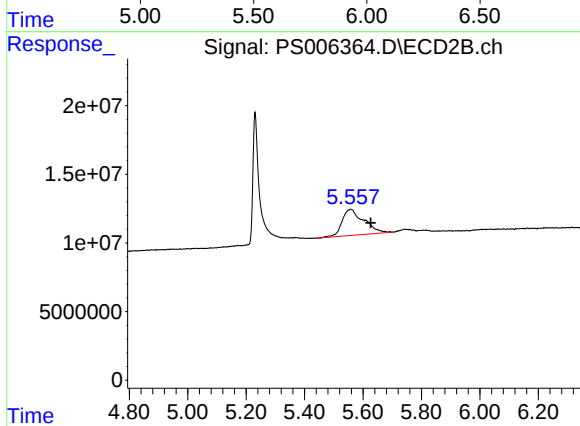

#7 MCPA


R.T.: 5.558 min
Delta R.T.: -0.068 min
Response: 98240249
Conc: 48.07 ug/ml

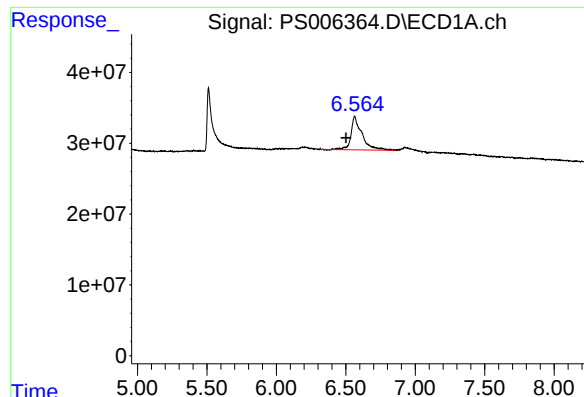

#9 2,4-D

R.T.: 6.563 min
Delta R.T.: 0.060 min
Response: 261531199
Conc: 320.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB122601BL

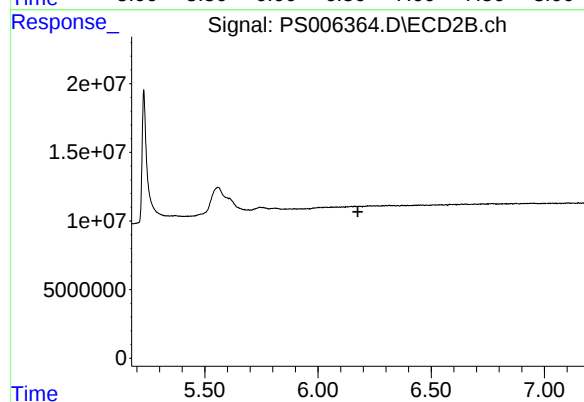

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.