

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082820\
 Data File : PS011984.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2020 18:00
 Operator : DD\AJ
 Sample : PB131270TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 18:59:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.915	294.5E6	186.3E6	270.007	348.280 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	94097526	N.D.	114.388
3) T	4-Nitroph...	7.056	6.506	8366729	14144492	14.204	38.794 #
5) T	DICAMBA	7.396	7.049	9997204	25131474	2.441	11.632 #
6) T	MCP	7.570	0.000	8389178	0	2.626	N.D. #
7) T	MCPA	7.701	0.000	53746616	0	11.816	N.D. #
8) T	DICHLORPROP	0.000	7.739	0	24816178	N.D.	43.951
9) T	2,4-D	8.398	0.000	146.8E6	0	130.007	N.D. #
11) T	2,4,5-TP ...	0.000	8.763	0	13604696	N.D.	4.653
12) T	2,4,5-T	9.412	0.000	23603894	0	3.983	N.D. #
15) T	Picloram	11.038	11.021	17457434	8750295	2.234	1.931



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082820\
Data File : PS011984.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2020 18:00
Operator : DD\AJ
Sample : PB131270TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 18:59:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

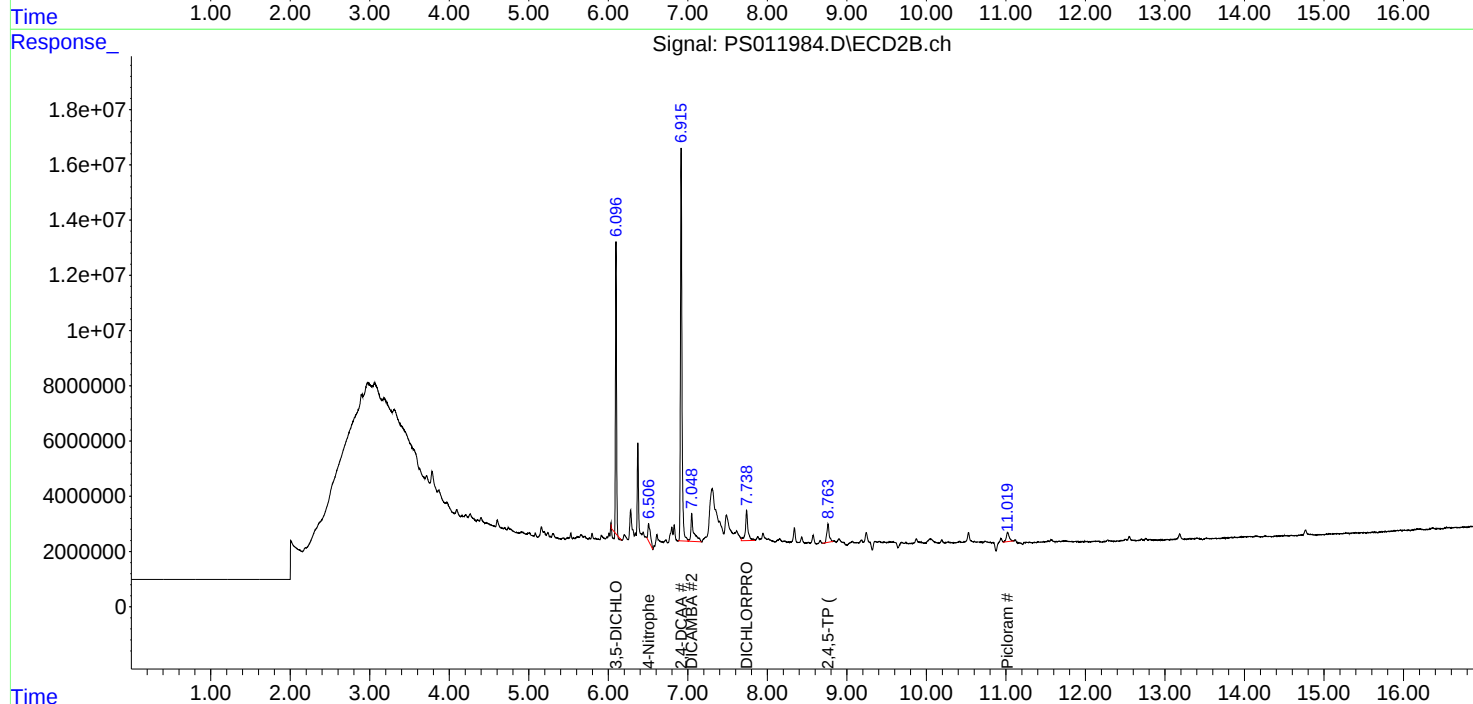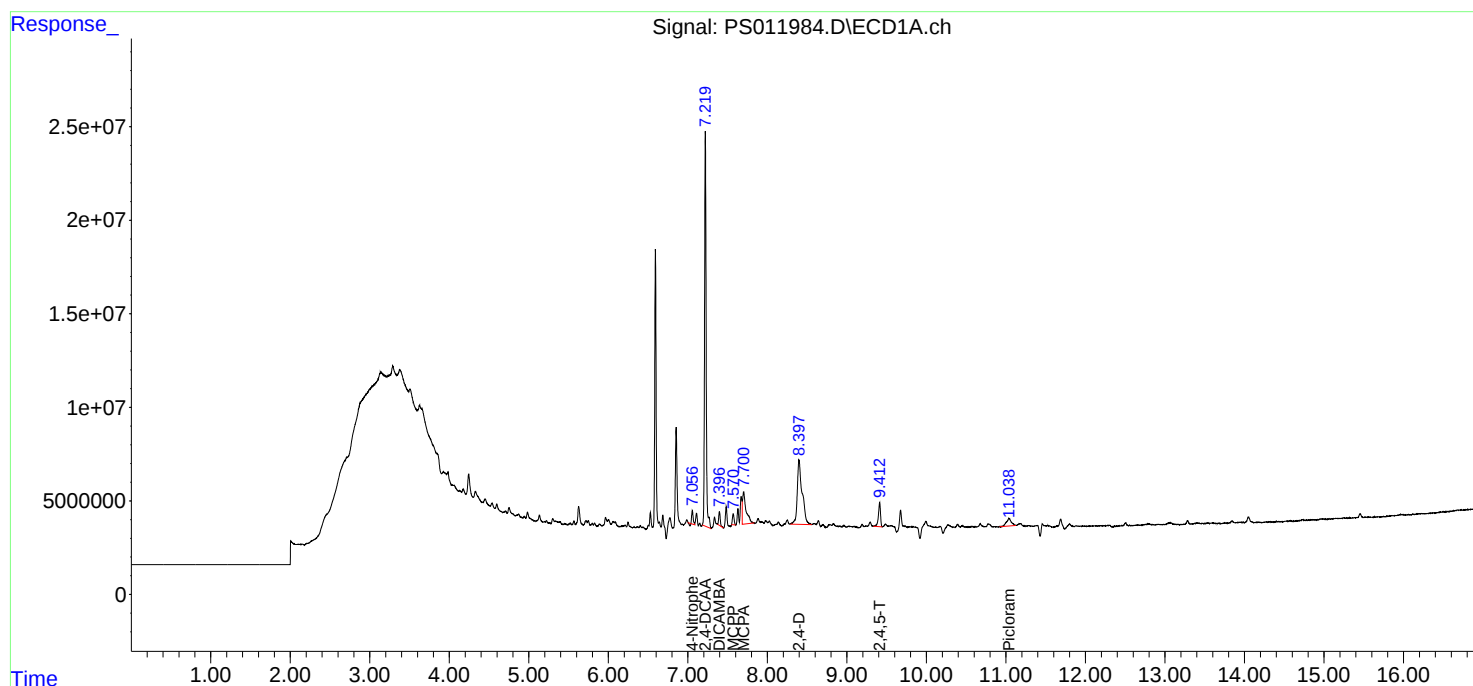


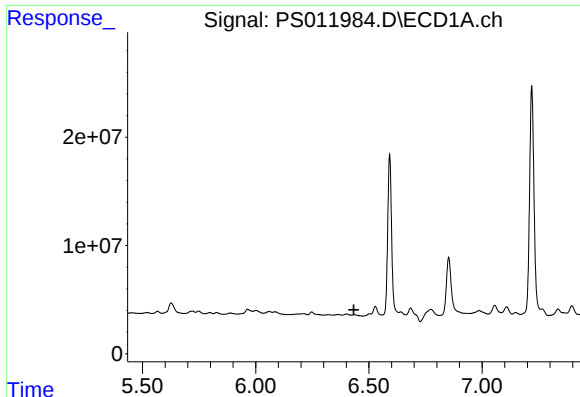

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

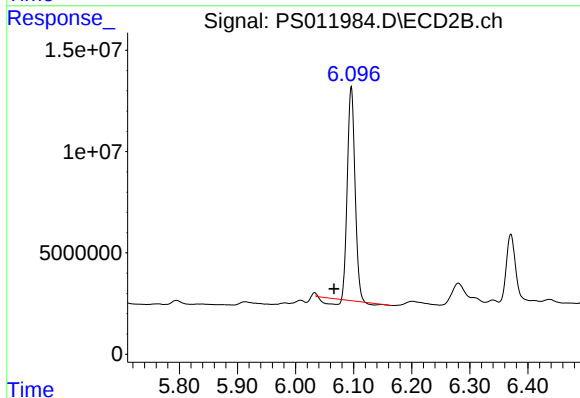


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.029 min
Response: 94097526
Conc: 114.39 ng/ml

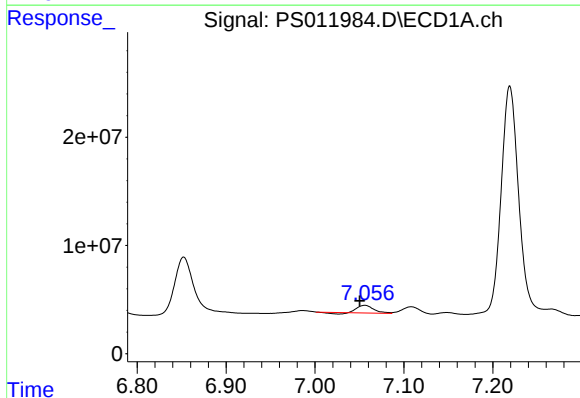


#3 4-Nitrophenol

R.T.: 7.056 min
Delta R.T.: 0.006 min
Response: 8366729
Conc: 14.20 ng/ml

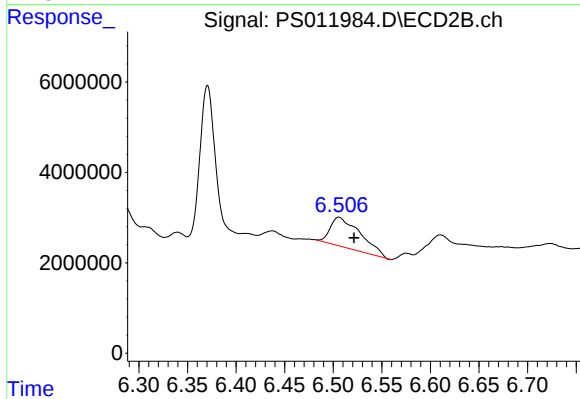

#3 4-Nitrophenol


R.T.: 6.506 min
Delta R.T.: -0.015 min
Response: 14144492
Conc: 38.79 ng/ml

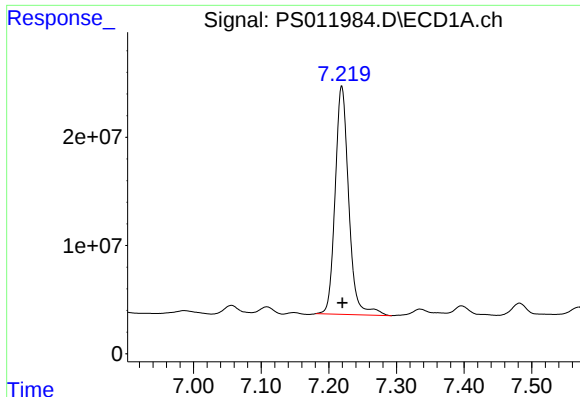

#4 2,4-DCAA


R.T.: 7.219 min
Delta R.T.: 0.000 min
Response: 294515058
Conc: 270.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

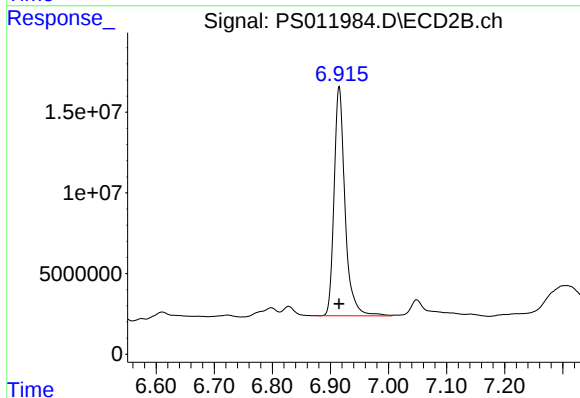


#4 2,4-DCAA

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 186255281
Conc: 348.28 ng/ml

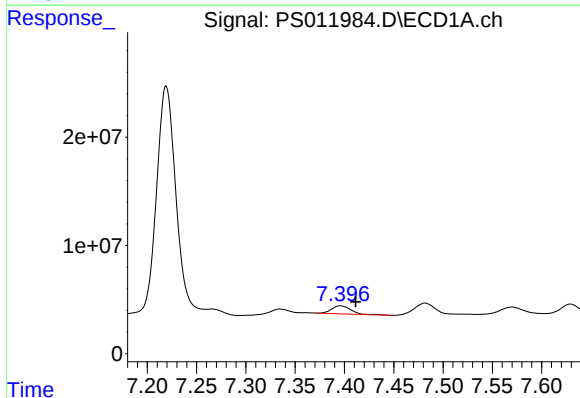


#5 DICAMBA

R.T.: 7.396 min
Delta R.T.: -0.015 min
Response: 9997204
Conc: 2.44 ng/ml

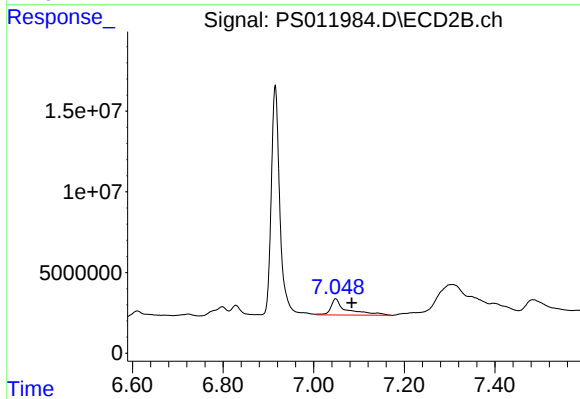

#5 DICAMBA


R.T.: 7.049 min
Delta R.T.: -0.036 min
Response: 25131474
Conc: 11.63 ng/ml

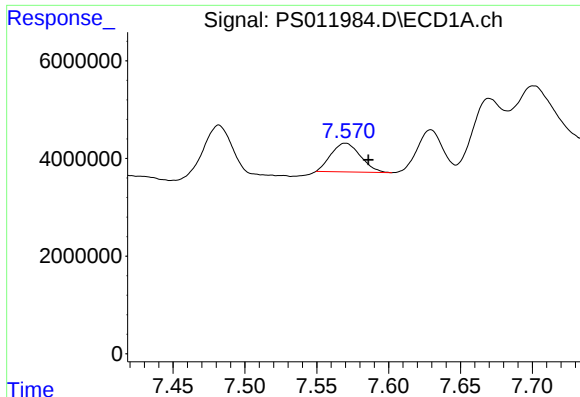

#6 MCPP


R.T.: 7.570 min
Delta R.T.: -0.016 min
Response: 8389178
Conc: 2.63 ug/ml

Instrument :
ECD_S
ClientSampleId :

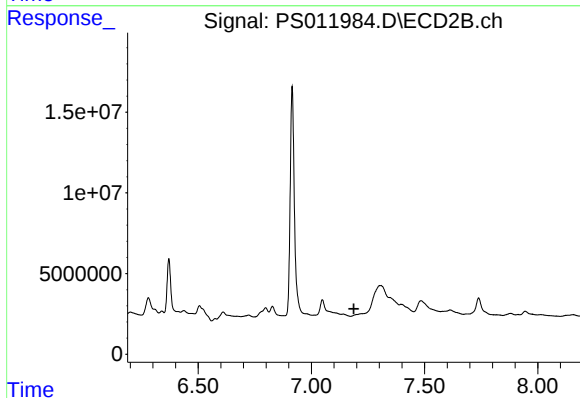


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

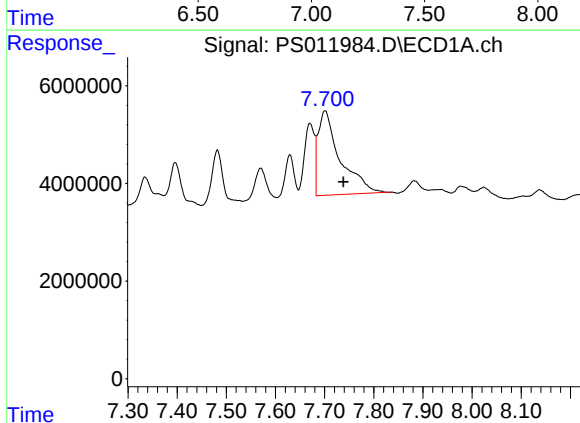


#7 MCPA

R.T.: 7.701 min
Delta R.T.: -0.037 min
Response: 53746616
Conc: 11.82 ug/ml

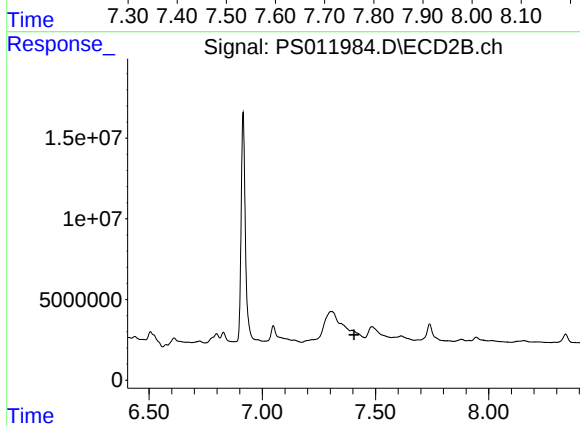

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.405 min
Response: 0
Conc: N.D.

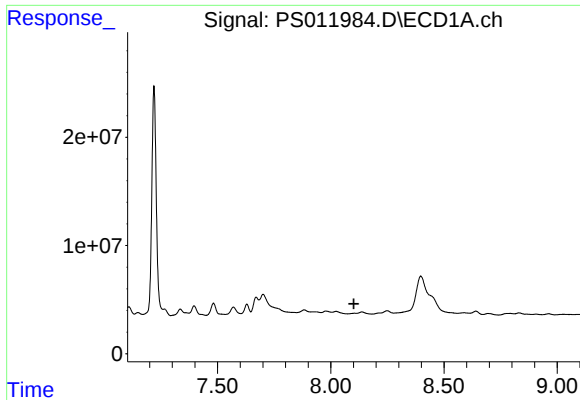

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

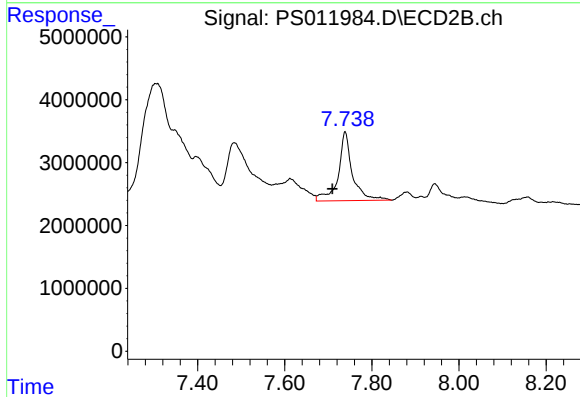


#8 DICHLORPROP

R.T.: 7.739 min
Delta R.T.: 0.029 min
Response: 24816178
Conc: 43.95 ng/ml

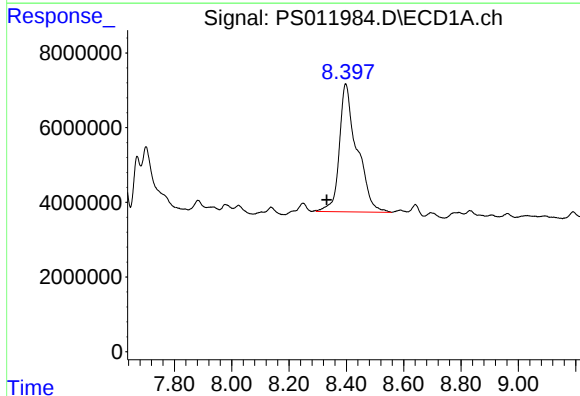


#9 2,4-D

R.T.: 8.398 min
Delta R.T.: 0.066 min
Response: 146790056
Conc: 130.01 ng/ml

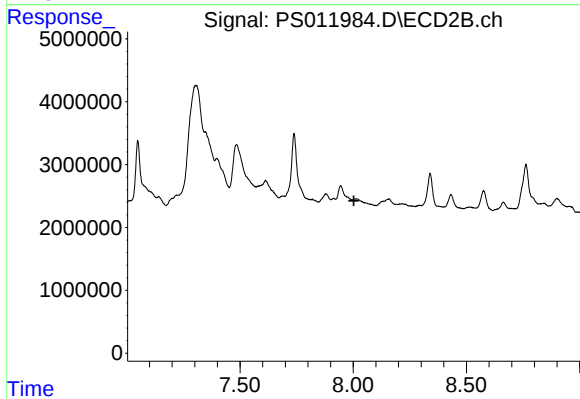

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

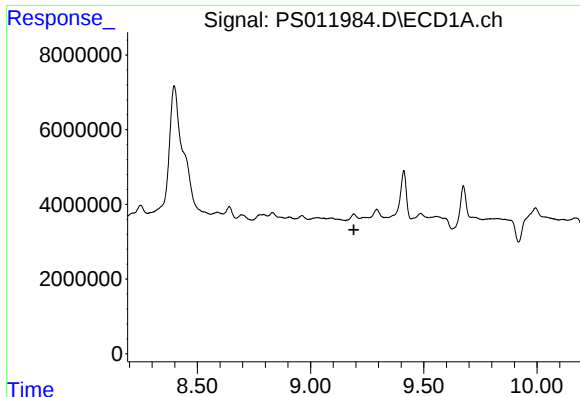

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

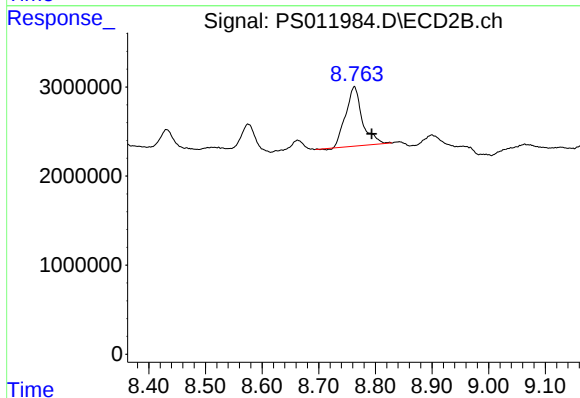


#11 2,4,5-TP (SILVEX)

R.T.: 8.763 min
Delta R.T.: -0.031 min
Response: 13604696
Conc: 4.65 ng/ml

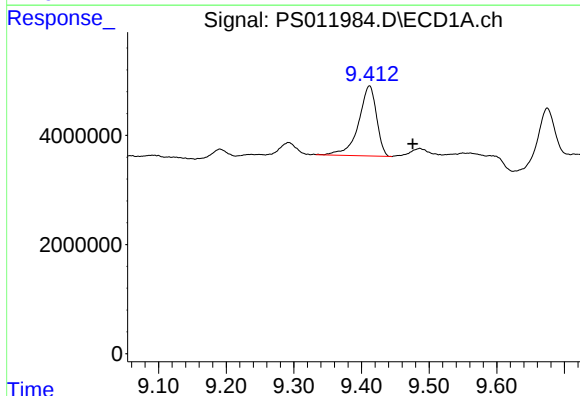


#12 2,4,5-T

R.T.: 9.412 min
Delta R.T.: -0.064 min
Response: 23603894
Conc: 3.98 ng/ml

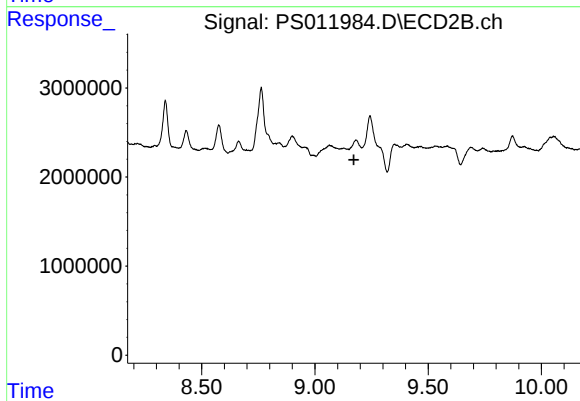

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.

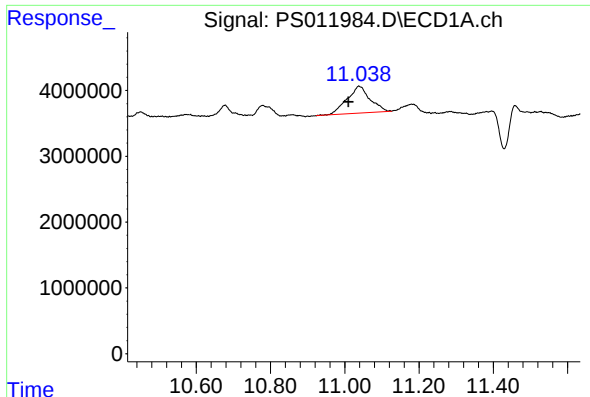

#15 Picloram

R.T.: 11.038 min
Delta R.T.: 0.029 min
Response: 17457434
Conc: 2.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

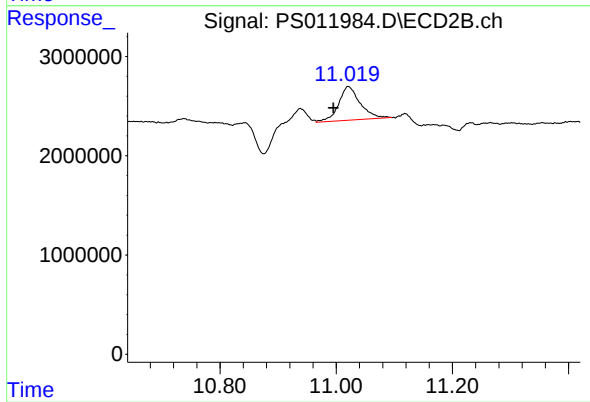

#15 Picloram

R.T.: 11.021 min
Delta R.T.: 0.026 min
Response: 8750295
Conc: 1.93 ng/ml