

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082820\
 Data File : PS011988.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2020 19:32
 Operator : DD\AJ
 Sample : L3507-17
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 01:02:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.914	370.0E6	227.3E6	339.241	425.075 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.096	0	75650544	N.D.	91.963
3) T	4-Nitroph...	7.055	0.000	2194800	0	3.726	N.D. #
5) T	DICAMBA	7.396	7.048	7649413	11976747	1.868	5.543 #
6) T	MCP	7.629	0.000	7062890	0	2.211	N.D. #
7) T	MCPA	7.692	7.467	209.0E6	163.1E6	45.952	59.527 #
8) T	DICHLORPROP	0.000	7.738	0	17743773	N.D.	31.425
9) T	2,4-D	8.399	0.000	151.6E6	0	134.262	N.D. #
11) T	2,4,5-TP ...	0.000	8.786	0	189.6E6	N.D.	64.842
12) T	2,4,5-T	9.412	0.000	29486639	0	4.976	N.D. #
15) T	Picloram	0.000	11.018	0	5906810	N.D.	1.303



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082820\
Data File : PS011988.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2020 19:32
Operator : DD\AJ
Sample : L3507-17
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 01:02:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

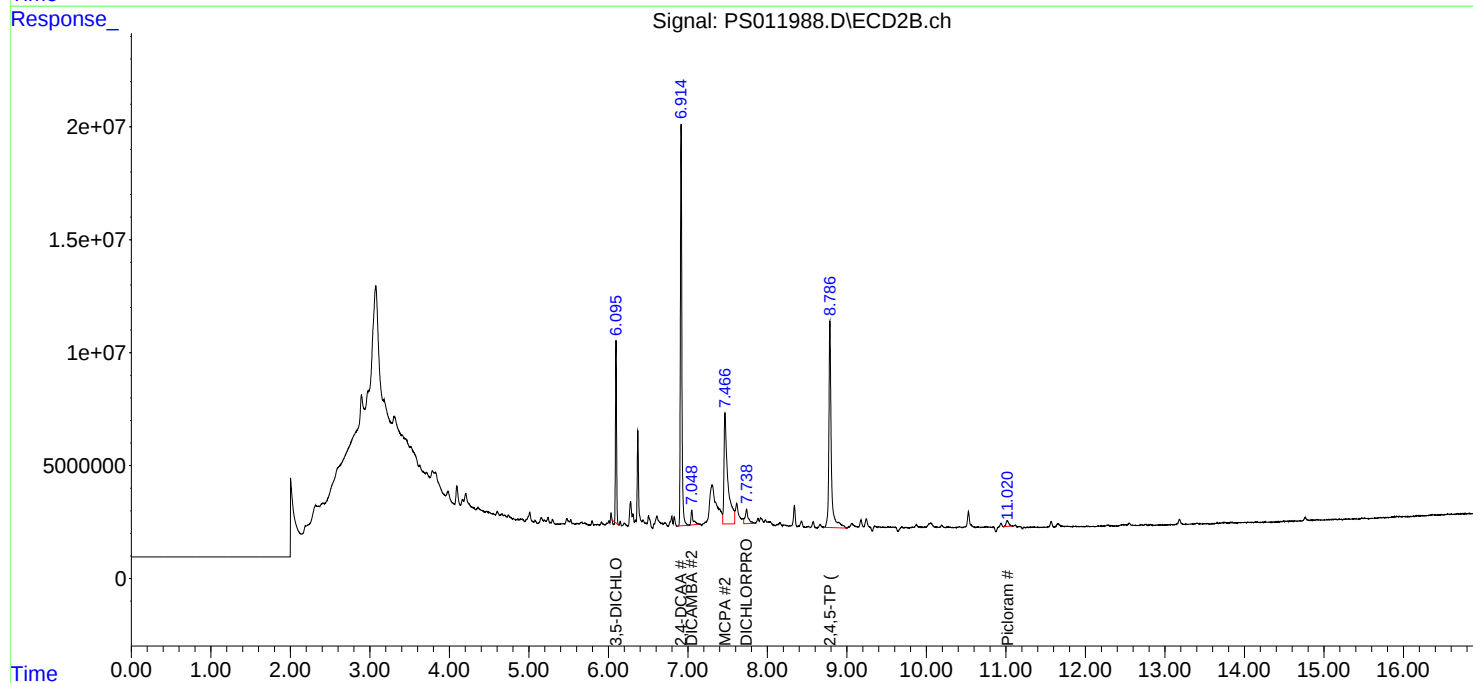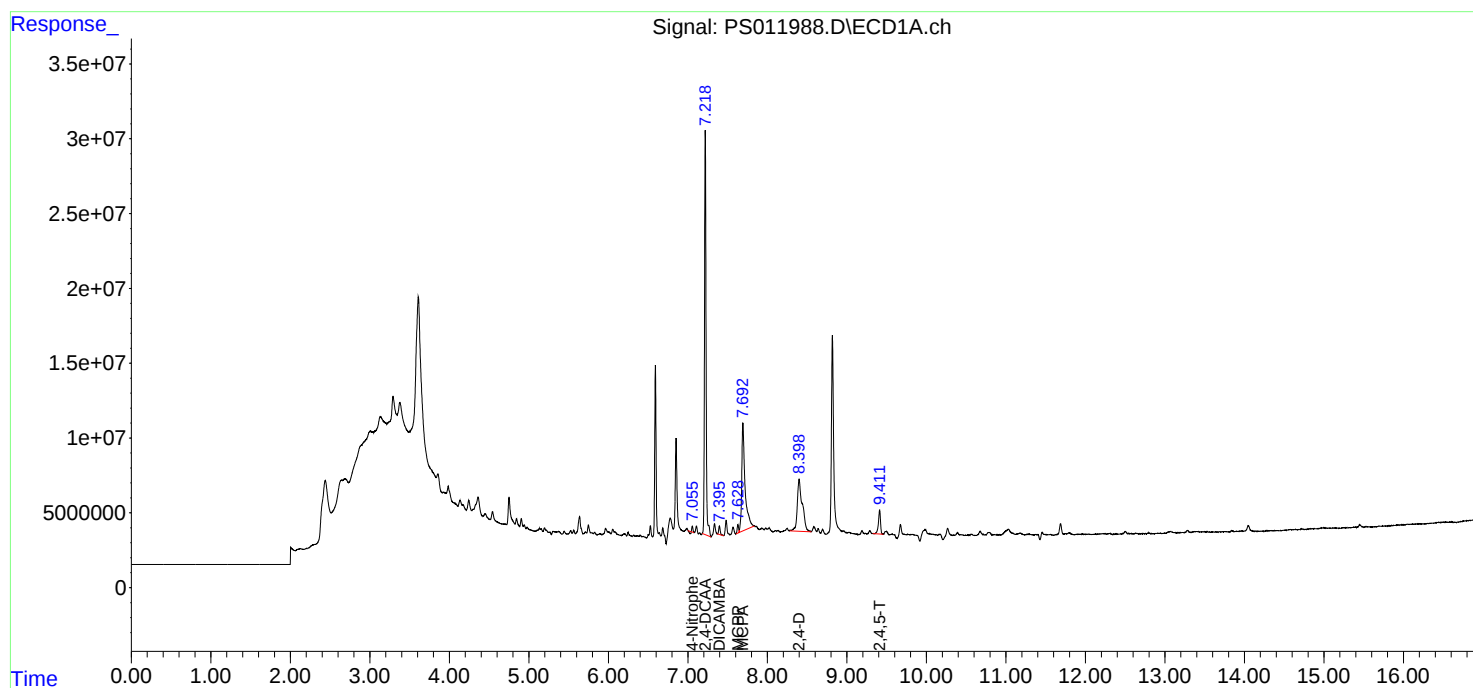


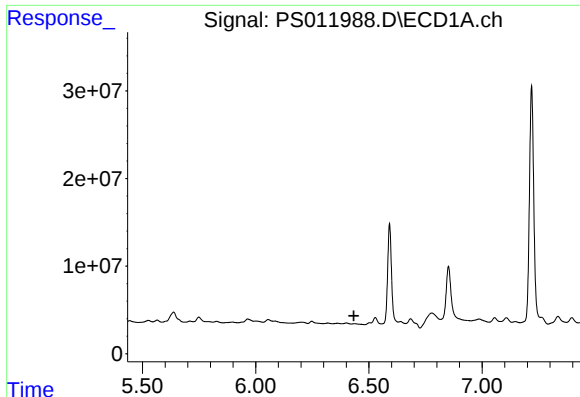

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

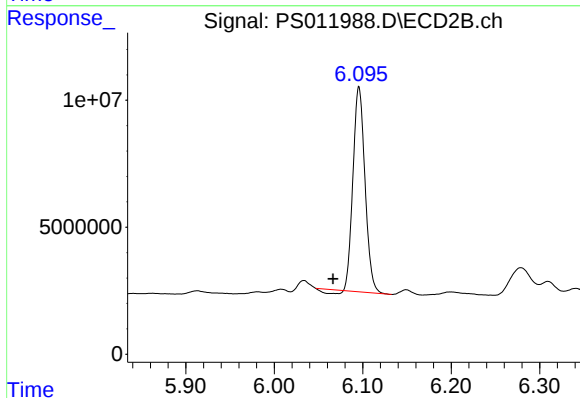


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.096 min
Delta R.T.: 0.029 min
Response: 75650544
Conc: 91.96 ng/ml

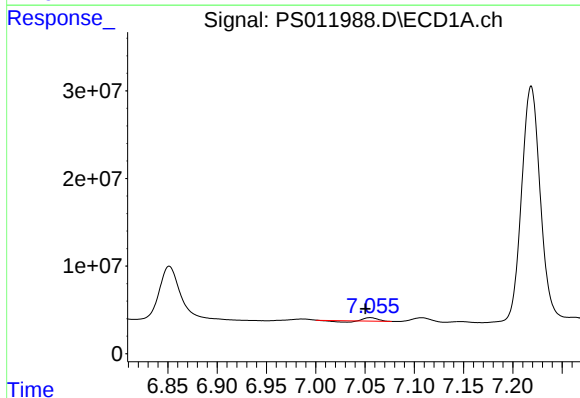


#3 4-Nitrophenol

R.T.: 7.055 min
Delta R.T.: 0.005 min
Response: 2194800
Conc: 3.73 ng/ml

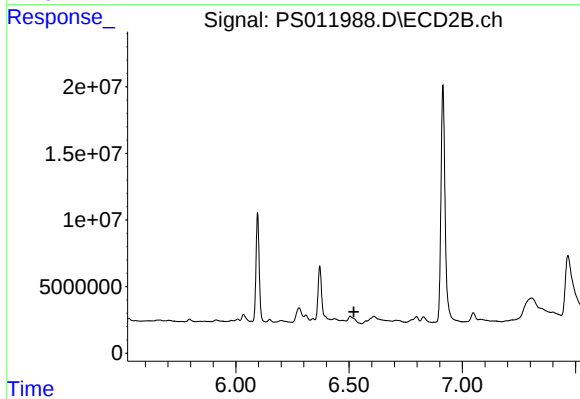

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.521 min
Response: 0
Conc: N.D.

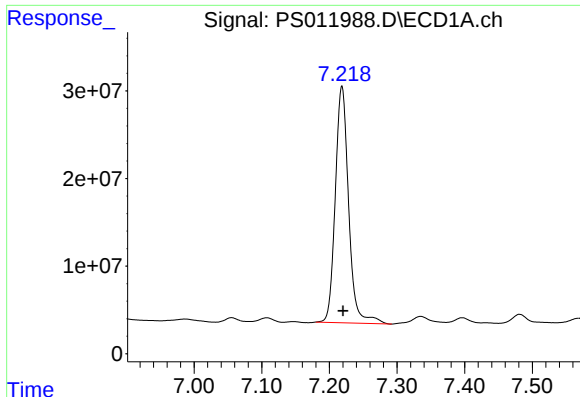

#4 2,4-DCAA


R.T.: 7.219 min
Delta R.T.: -0.002 min
Response: 370033037
Conc: 339.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

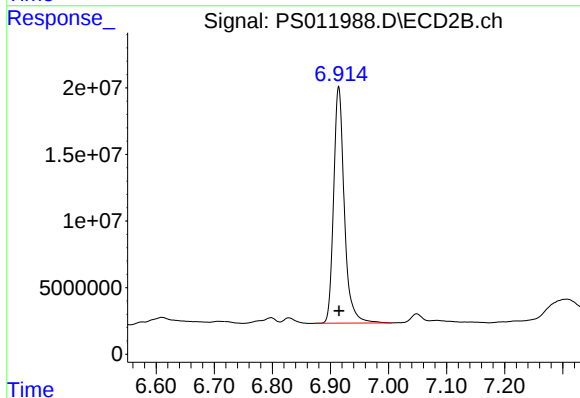


#4 2,4-DCAA

R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 227324468
Conc: 425.08 ng/ml

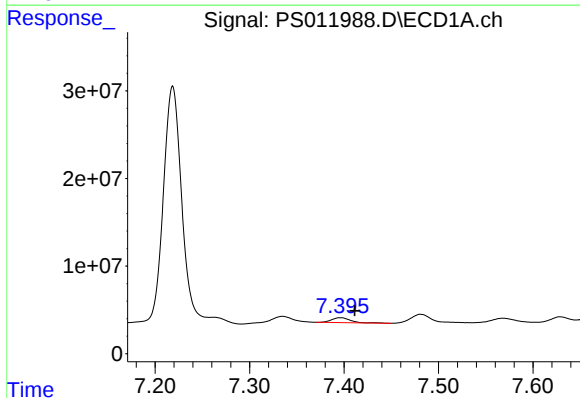


#5 DICAMBA

R.T.: 7.396 min
Delta R.T.: -0.015 min
Response: 7649413
Conc: 1.87 ng/ml

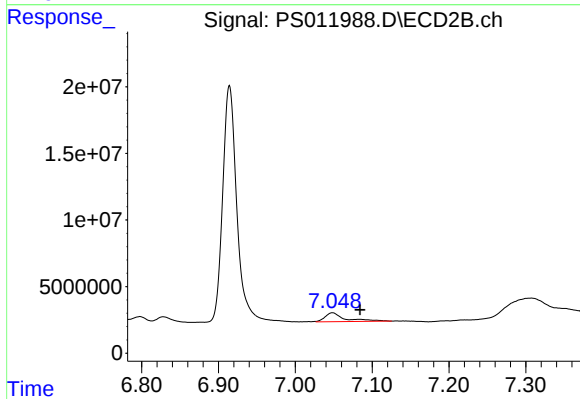

#5 DICAMBA


R.T.: 7.048 min
Delta R.T.: -0.036 min
Response: 11976747
Conc: 5.54 ng/ml

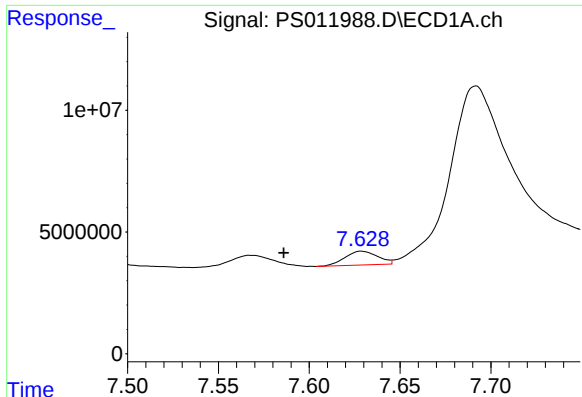

#6 MCPP


R.T.: 7.629 min
Delta R.T.: 0.043 min
Response: 7062890
Conc: 2.21 ug/ml

Instrument :
ECD_S
ClientSampleId :

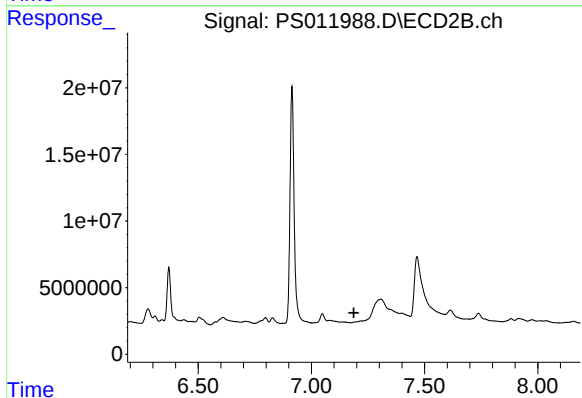


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

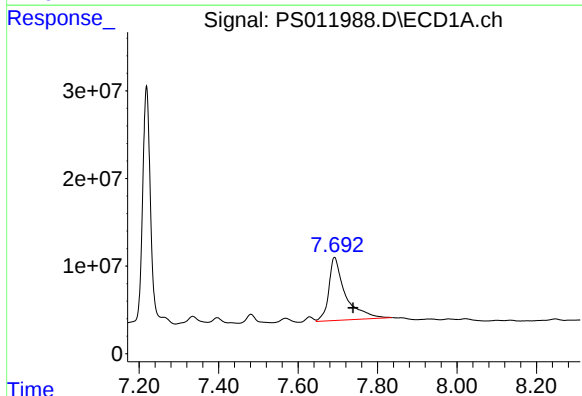


#7 MCPA

R.T.: 7.692 min
Delta R.T.: -0.046 min
Response: 209012218
Conc: 45.95 ug/ml

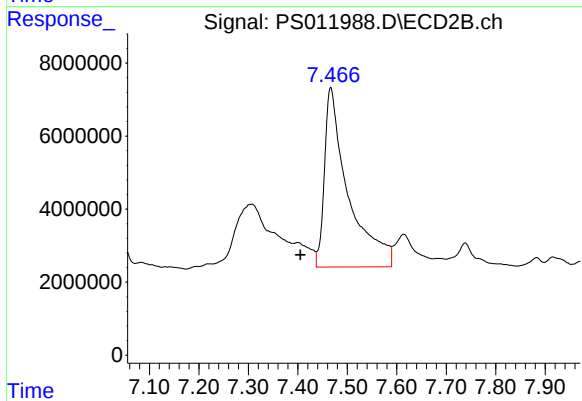

#7 MCPA


R.T.: 7.467 min
Delta R.T.: 0.062 min
Response: 163113792
Conc: 59.53 ug/ml

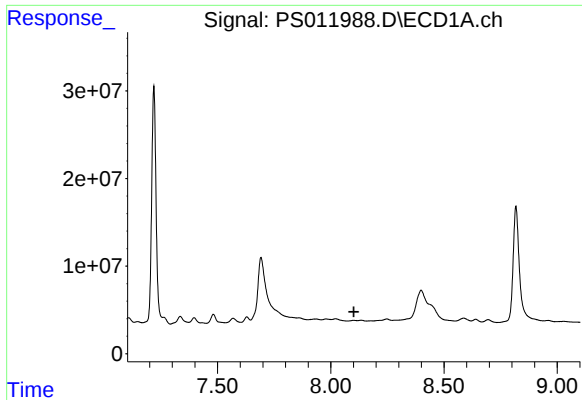

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

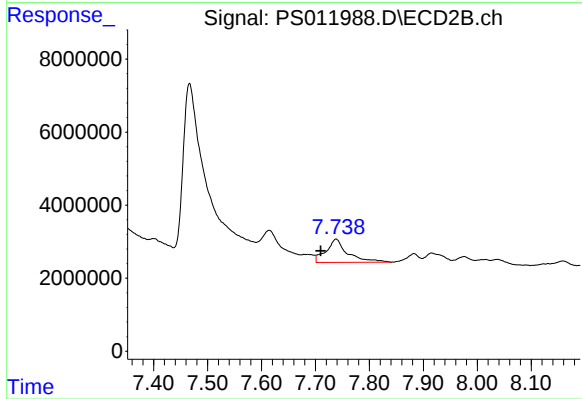


#8 DICHLORPROP

R.T.: 7.738 min
Delta R.T.: 0.029 min
Response: 17743773
Conc: 31.43 ng/ml

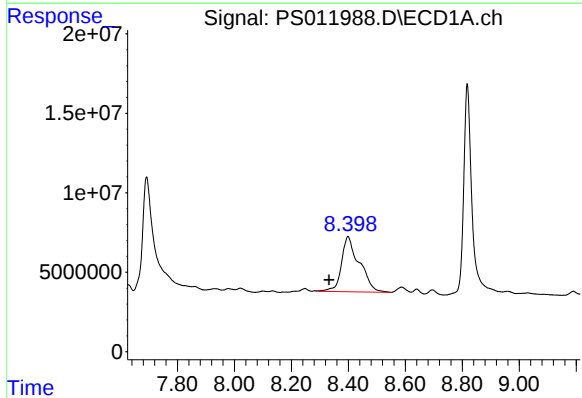


#9 2,4-D

R.T.: 8.399 min
Delta R.T.: 0.067 min
Response: 151594637
Conc: 134.26 ng/ml

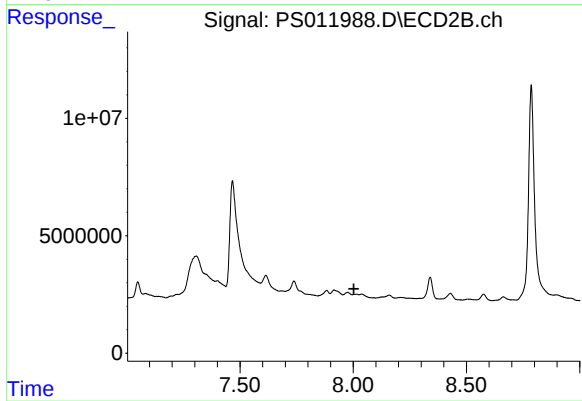

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.003 min
Response: 0
Conc: N.D.

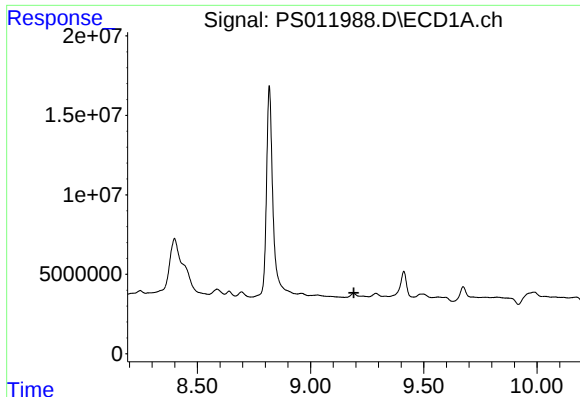

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

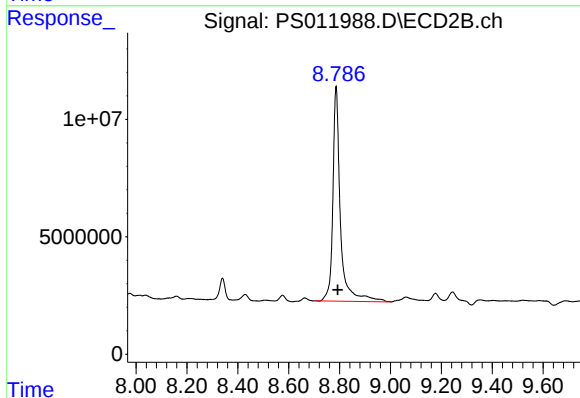


#11 2,4,5-TP (SILVEX)

R.T.: 8.786 min
Delta R.T.: -0.007 min
Response: 189573699
Conc: 64.84 ng/ml

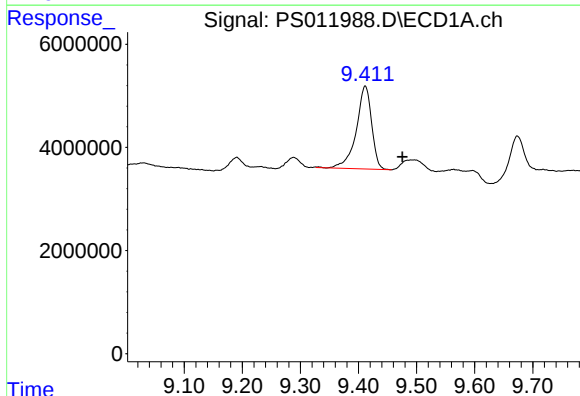


#12 2,4,5-T

R.T.: 9.412 min
Delta R.T.: -0.064 min
Response: 29486639
Conc: 4.98 ng/ml

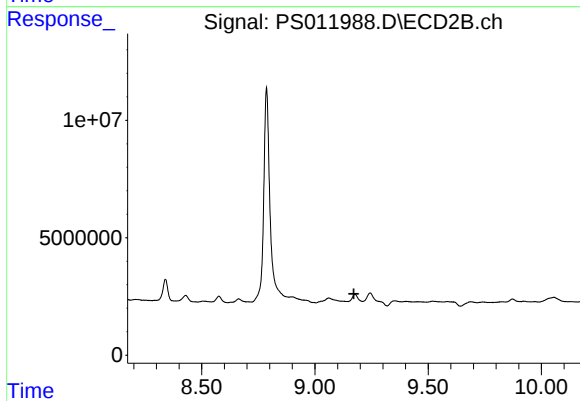

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.

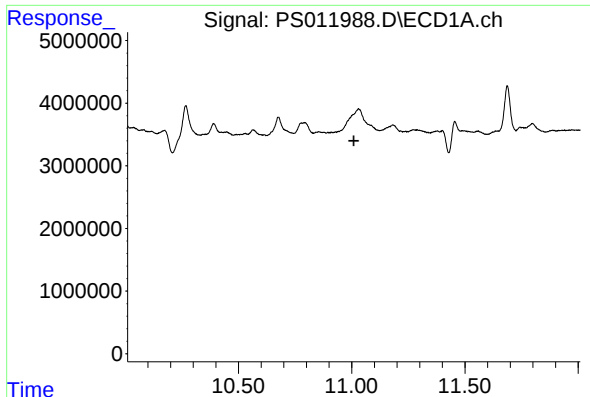

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

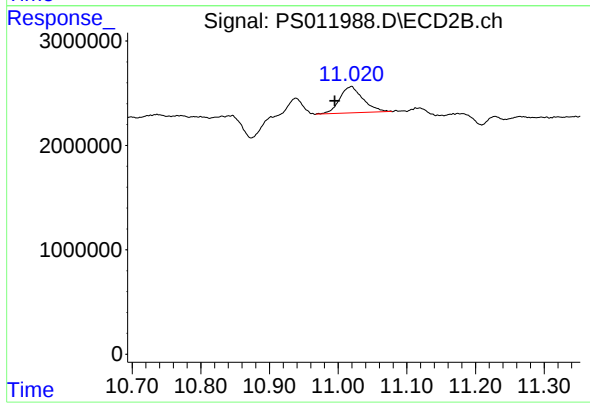

#15 Picloram

R.T.: 11.018 min
Delta R.T.: 0.023 min
Response: 5906810
Conc: 1.30 ng/ml