

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082918\
 Data File : PS001629.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2018 10:13
 Operator : UA
 Sample : J4280-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 11:19:53 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.472	10.963	97093061	99389965	525.963	490.742
Target Compounds							
1) T	Dalapon	2.890	0.000	18687223	0	74.340	N.D. #
2) T	3,5-DICHL...	0.000	9.116	0	1824229	N.D.	7.138 #
5) T	DICAMBA	0.000	11.206	0	6718766	N.D.	9.580 #
6) T	MCP	12.160	0.000	11098091	0	22.057	N.D. #
10) T	Pentachlo...	13.717	0.000	3188497	0	1.279	N.D. #
12) T	2,4,5-T	0.000	14.586	0	5012473	N.D.	5.802 #
15) T	Picloram	16.984	16.846	11897711	3952673	8.495	3.031 #
16) T	DCPA	0.000	16.901	0	15130590	N.D.	10.598 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082918\
Data File : PS001629.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2018 10:13
Operator : UA
Sample : J4280-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 11:19:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

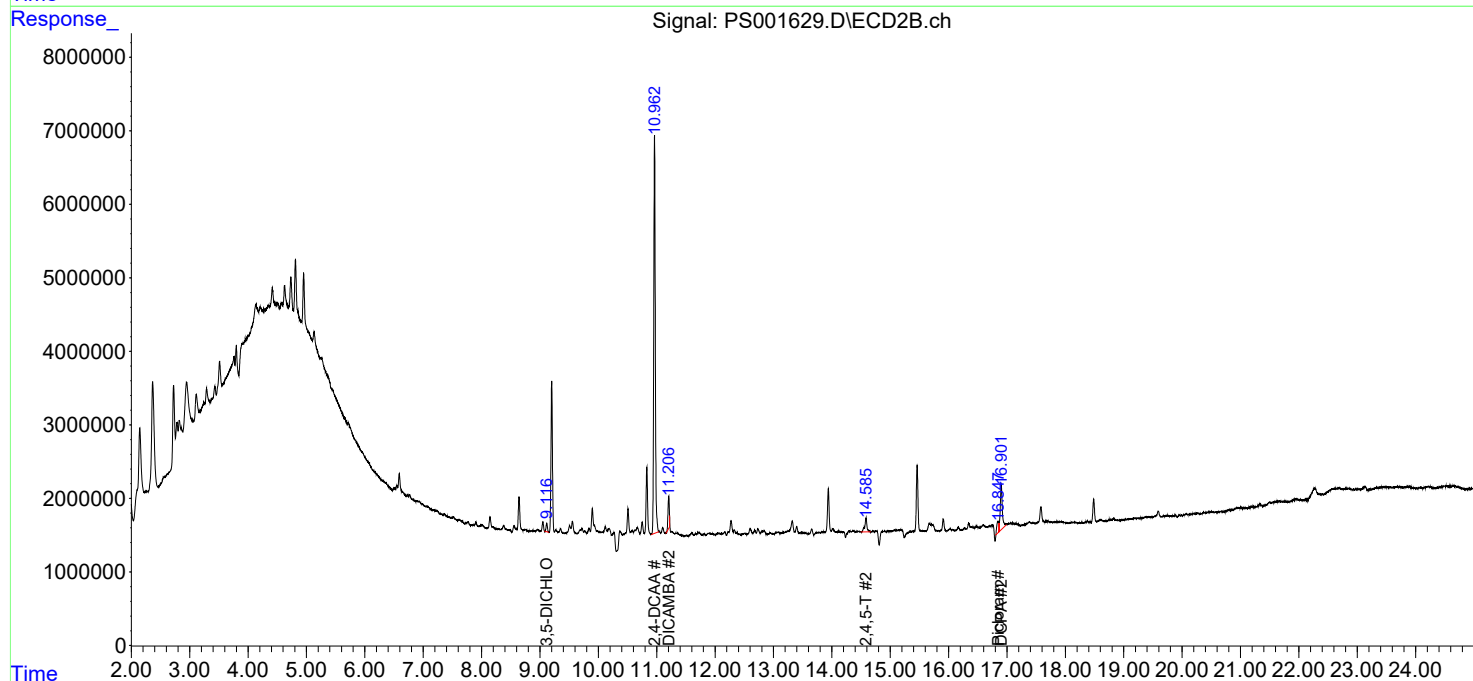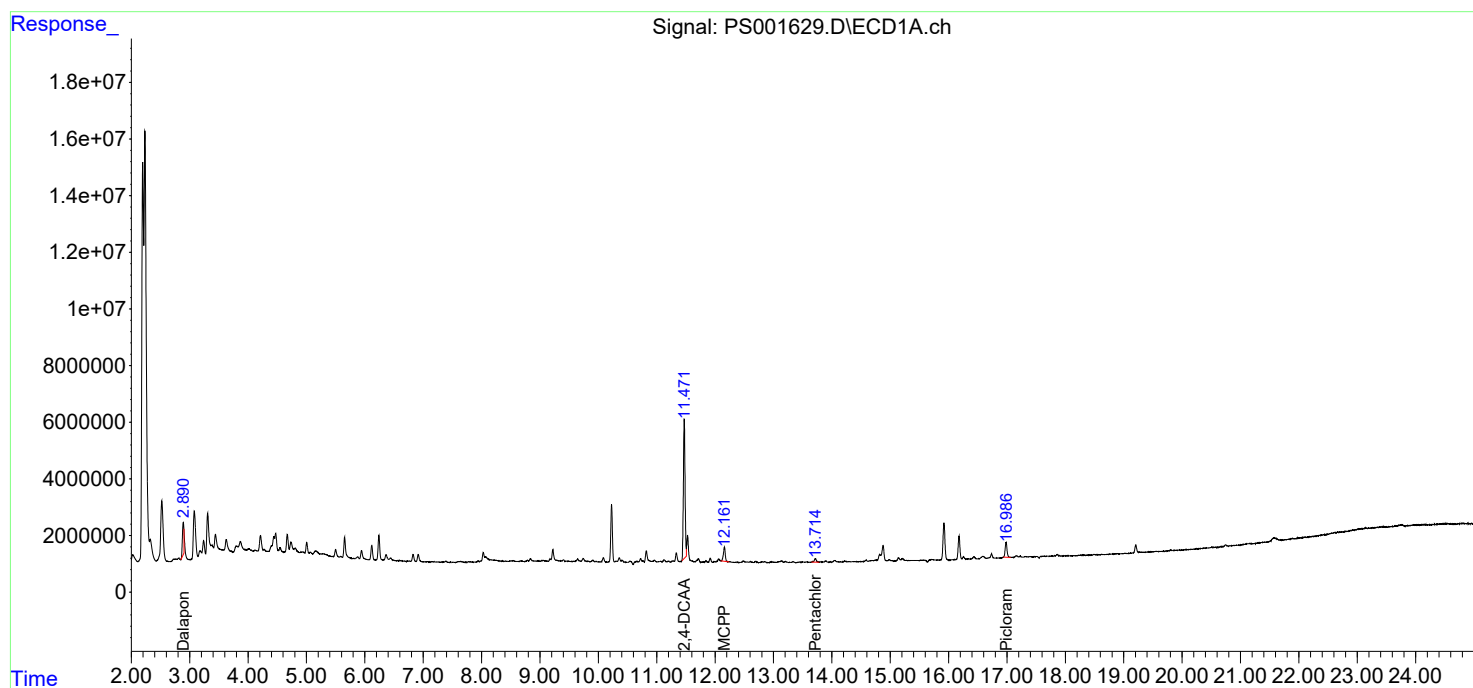


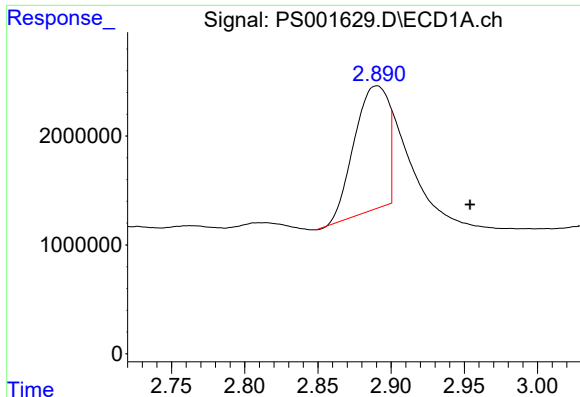

#1 Dalapon


R.T.: 2.890 min
Delta R.T.: -0.064 min
Response: 18687223
Conc: 74.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

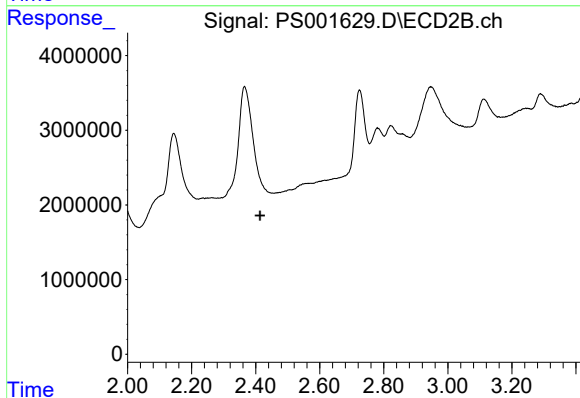


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.414 min
Response: 0
Conc: N.D.

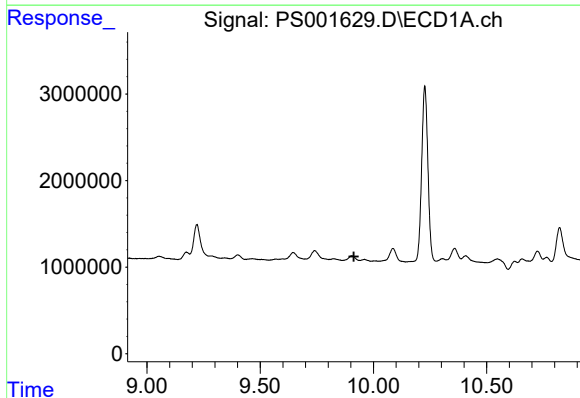


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.914 min
Response: 0
Conc: N.D.

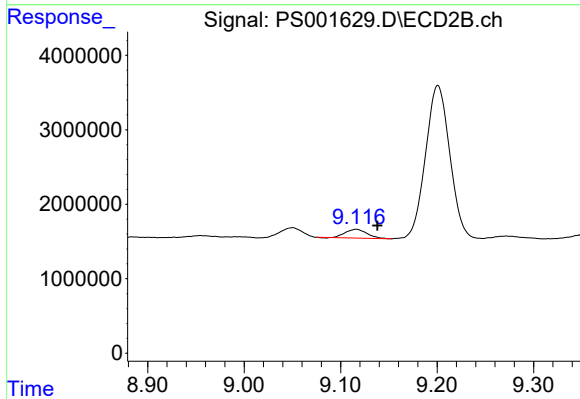

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.116 min
Delta R.T.: -0.022 min
Response: 1824229
Conc: 7.14 ng/ml

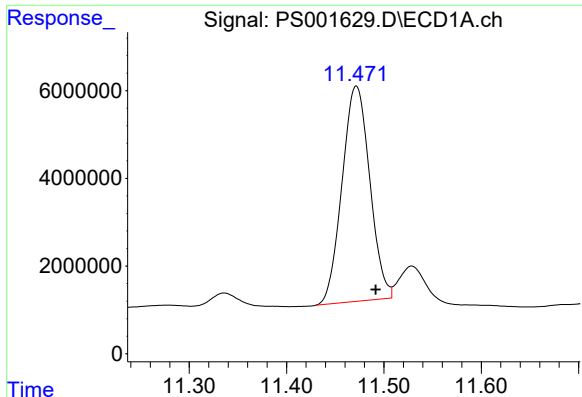

#4 2,4-DCAA


R.T.: 11.472 min
Delta R.T.: -0.020 min
Response: 97093061
Conc: 525.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

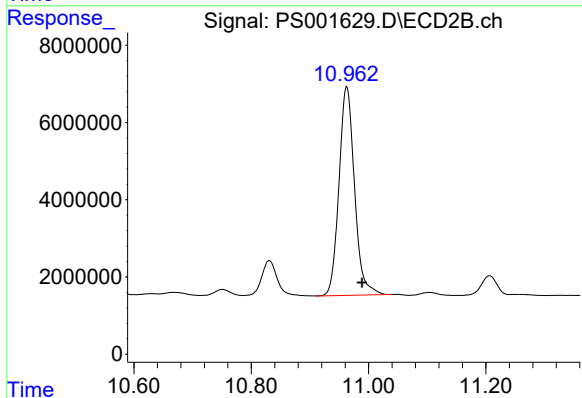


#4 2,4-DCAA

R.T.: 10.963 min
Delta R.T.: -0.026 min
Response: 99389965
Conc: 490.74 ng/ml

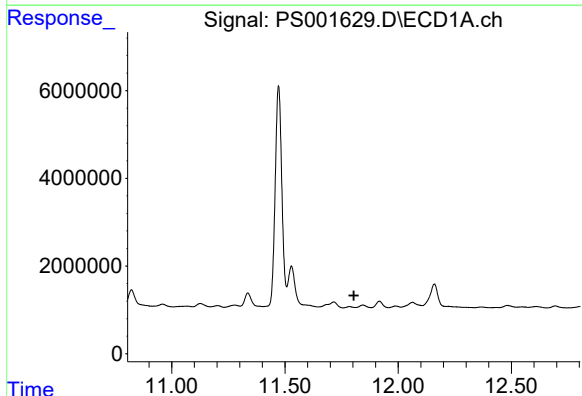


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.805 min
Response: 0
Conc: N.D.

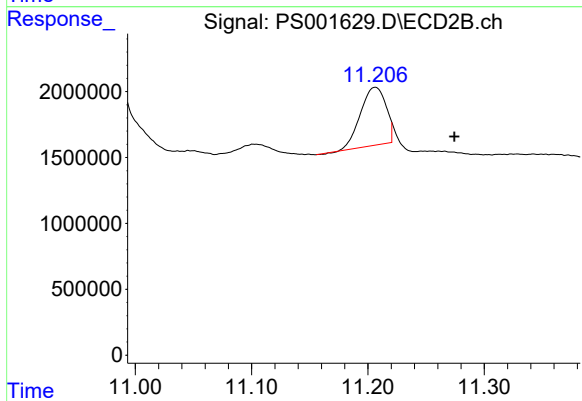

#5 DICAMBA


R.T.: 11.206 min
Delta R.T.: -0.068 min
Response: 6718766
Conc: 9.58 ng/ml

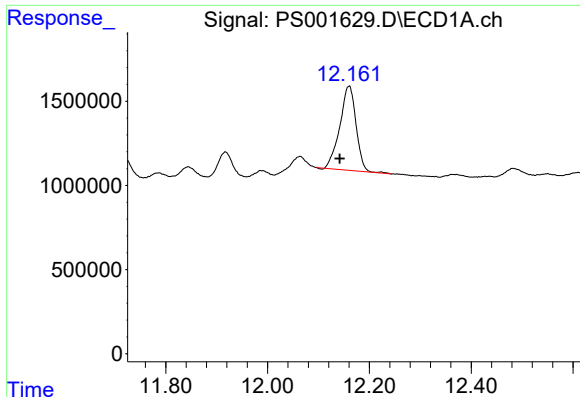

#6 MCPP


R.T.: 12.160 min
Delta R.T.: 0.018 min
Response: 11098091
Conc: 22.06 ug/ml

Instrument :
ECD_S
ClientSampleId :

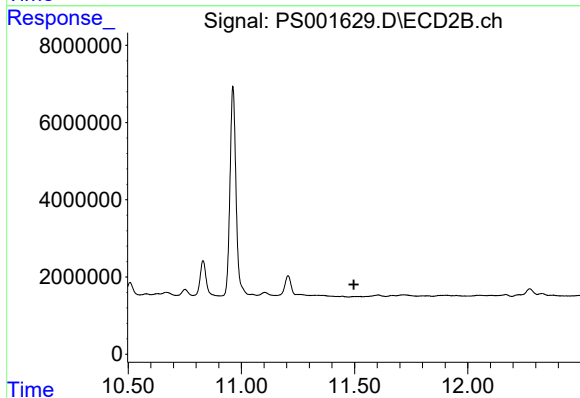


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.497 min
Response: 0
Conc: N.D.

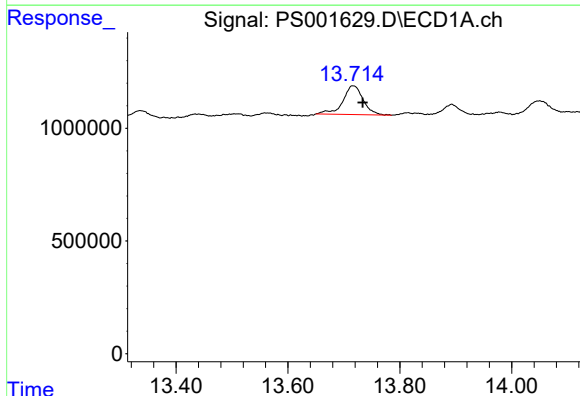


#10 Pentachlorophenol

R.T.: 13.717 min
Delta R.T.: -0.017 min
Response: 3188497
Conc: 1.28 ng/ml

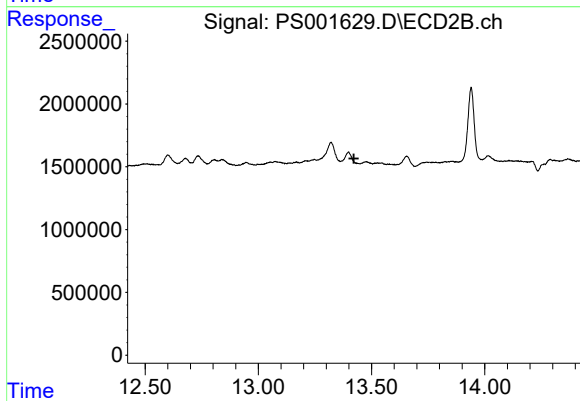

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 13.422 min
Response: 0
Conc: N.D.

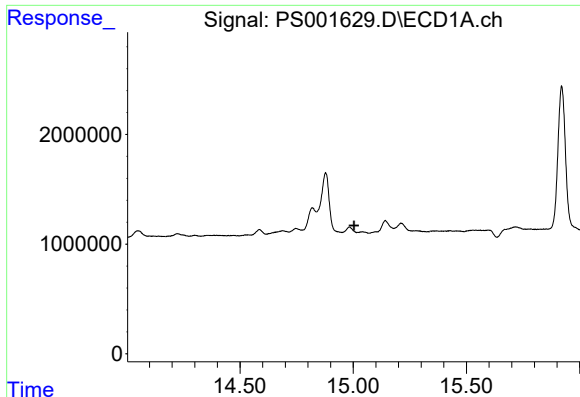

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.003 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

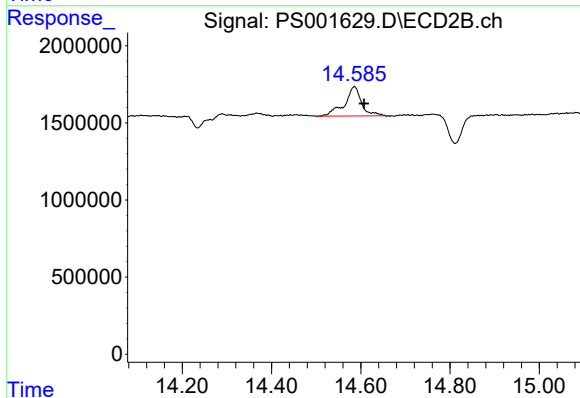


#12 2,4,5-T

R.T.: 14.586 min
Delta R.T.: -0.022 min
Response: 5012473
Conc: 5.80 ng/ml

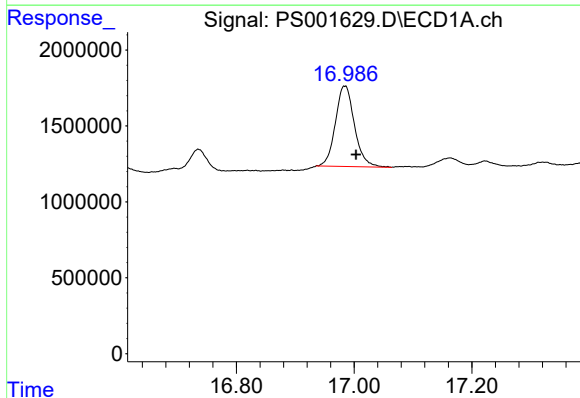


#15 Picloram

R.T.: 16.984 min
Delta R.T.: -0.019 min
Response: 11897711
Conc: 8.49 ng/ml

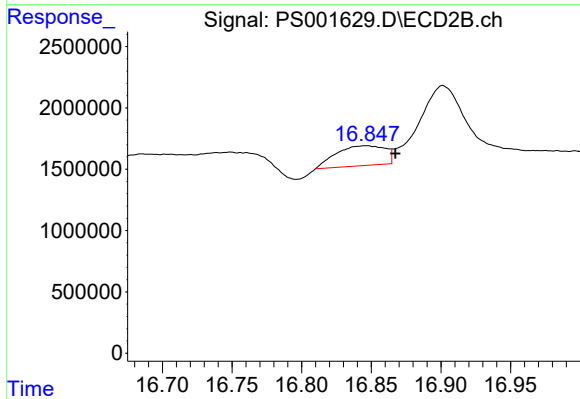

#15 Picloram


R.T.: 16.846 min
Delta R.T.: -0.021 min
Response: 3952673
Conc: 3.03 ng/ml

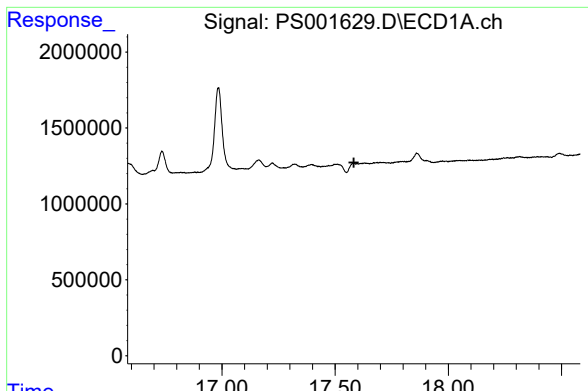

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.583 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

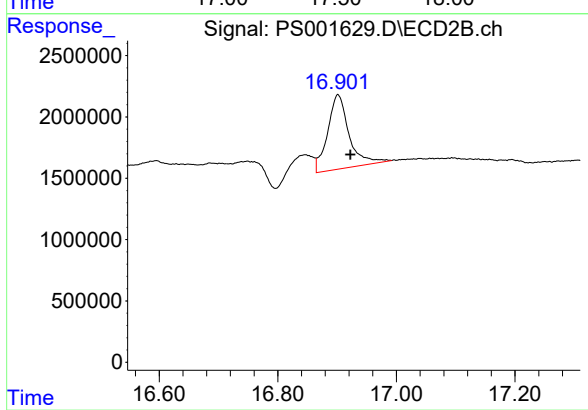

#16 DCPA

R.T.: 16.901 min
Delta R.T.: -0.021 min
Response: 15130590
Conc: 10.60 ng/ml