

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082918\
 Data File : PS001640.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2018 15:54
 Operator : UA
 Sample : J4671-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TL-SPEEDY-DRY

Manual Integrations
 APPROVED

Sohil
 8/30/2018 2:07:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 01:22:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	11.506	11.005	121.8E6	116.1E6	660.060m	573.334m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082918\
Data File : PS001640.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2018 15:54
Operator : UA
Sample : J4671-02
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
TL-SPEEDY-DRY


Manual Integrations
APPROVED

Sohil
8/30/2018 2:07:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 01:22:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

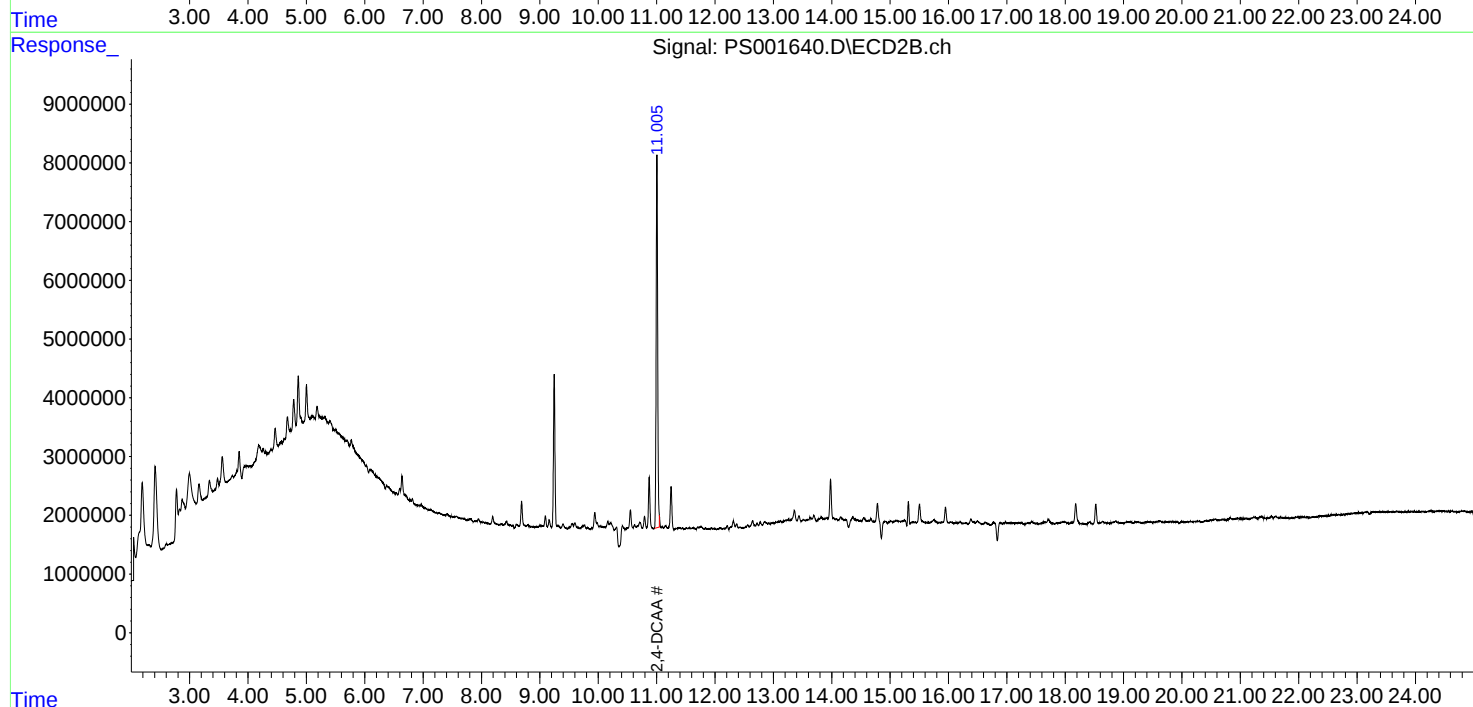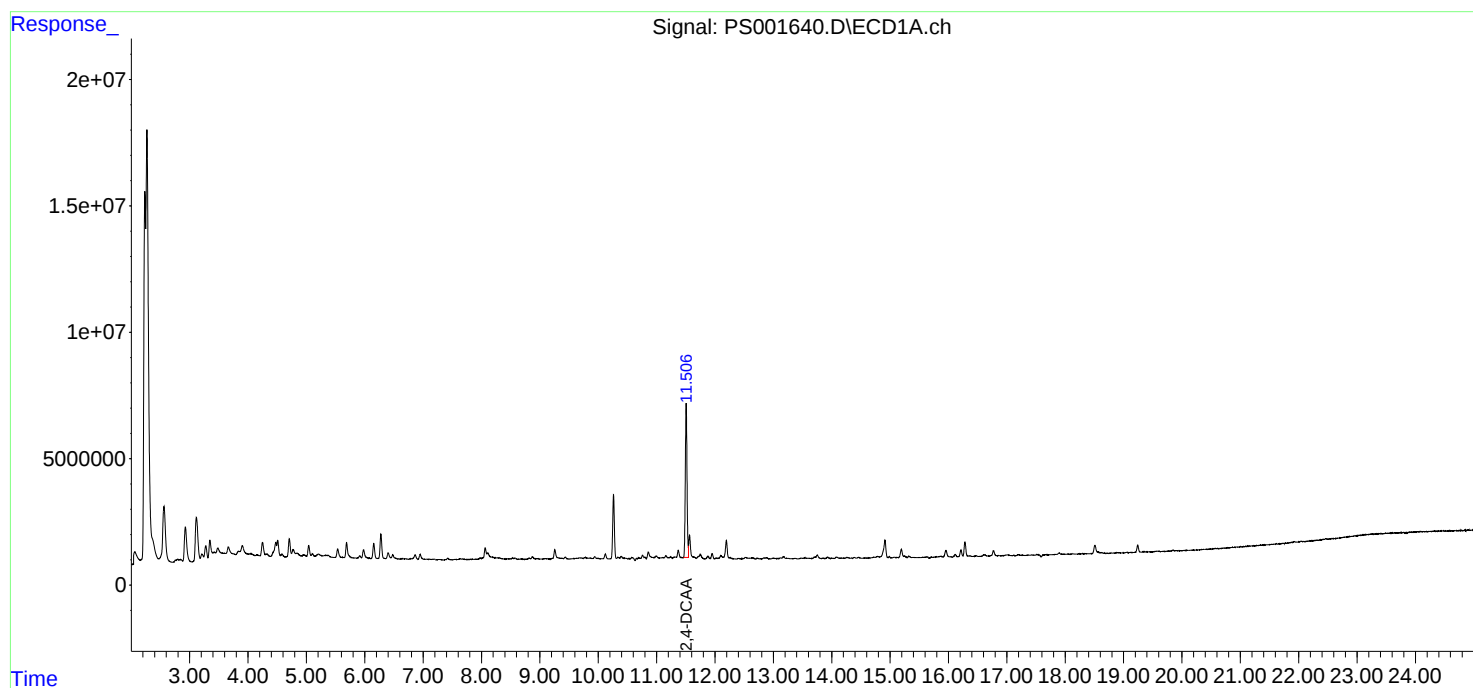

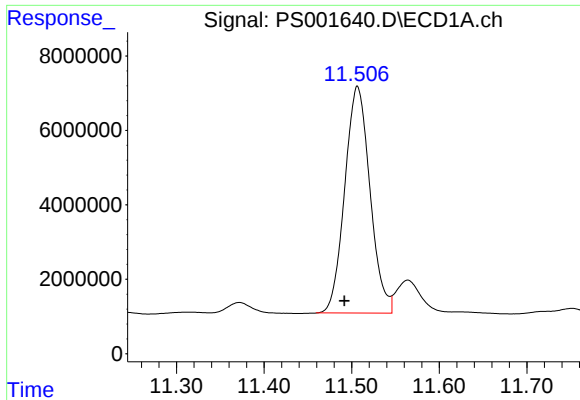


#4 2,4-DCAA

R.T.: 11.506 min
Delta R.T.: 0.014 min
Response: 121847455
Conc: 660.06 ng/ml m

Instrument :
ECD_S
ClientSampleId :
TL-SPEEDY-DRY

Manual Integrations
APPROVED

Sohil
8/30/2018 2:07:39 PM

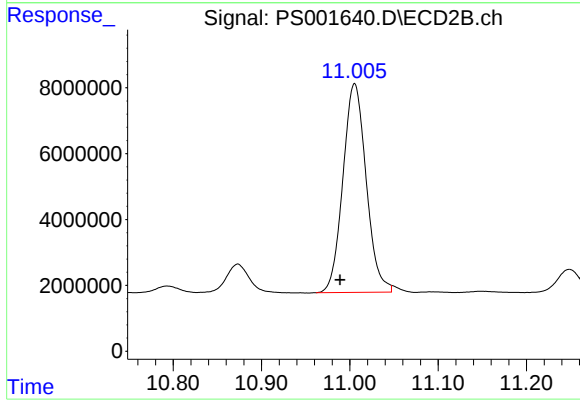

#4 2,4-DCAA

R.T.: 11.005 min
Delta R.T.: 0.016 min
Response: 116117276
Conc: 573.33 ng/ml m