

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082919\
 Data File : PS006406.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2019 15:30
 Operator : SM\AJ
 Sample : K4526-22
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 T9-12-13-D(0-1.9)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 04:59:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.489	5.216	908.7E6	523.3E6	1052.664	1064.004
Target Compounds							
1) T	Dalapon	2.122	1.745	6178760	31574102	5.671	50.318 #
2) T	3,5-DICHL...	4.925	4.544	44420886	64145708	41.202	105.902 #
6) T	MCP	0.000	5.513	0	243.6E6	N.D.	196.949
9) T	2,4-D	6.536	0.000	571.5E6	0	701.353	N.D. #
15) T	Picloram	9.047	8.998	29913677	36321587	4.020	8.052 #
16) T	DCPA	0.000	8.998	0	36321587	N.D.	10.416



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082919\
Data File : PS006406.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2019 15:30
Operator : SM\AJ
Sample : K4526-22
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
T9-12-13-D(0-1.9)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 04:59:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

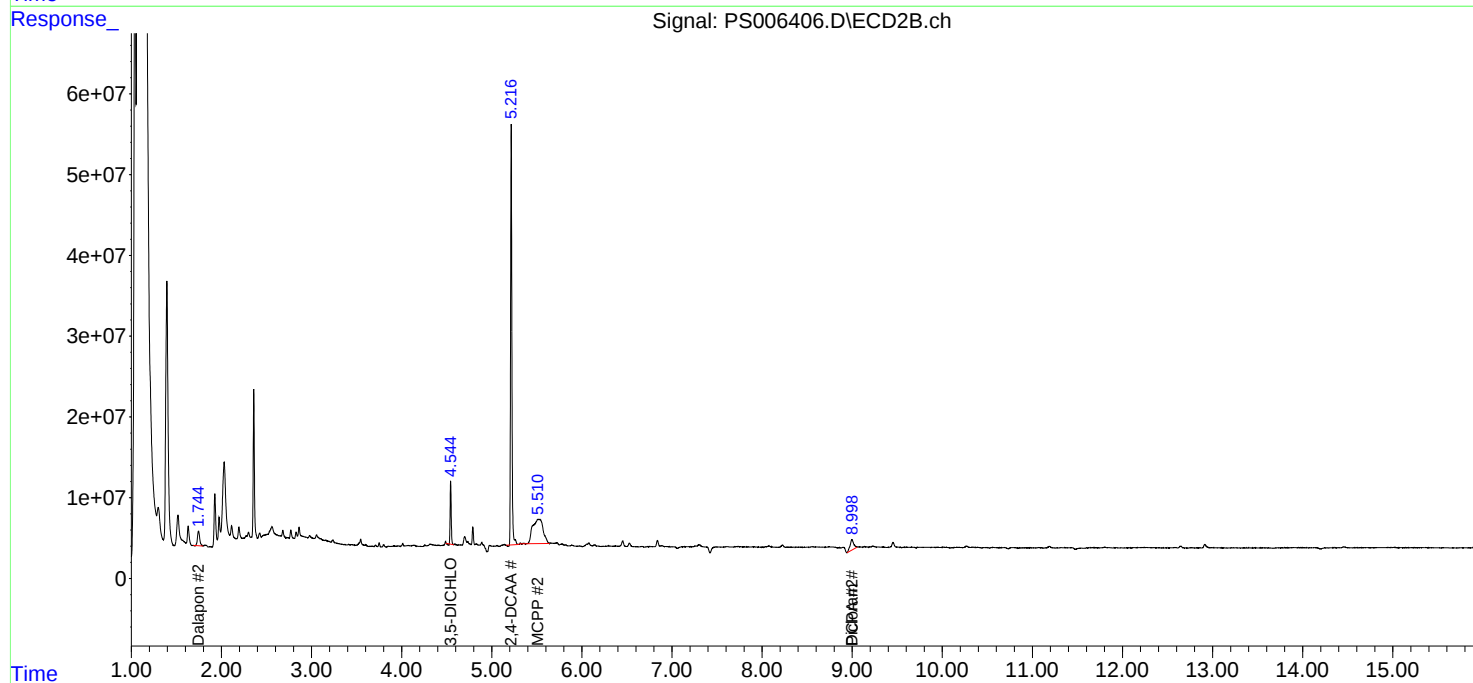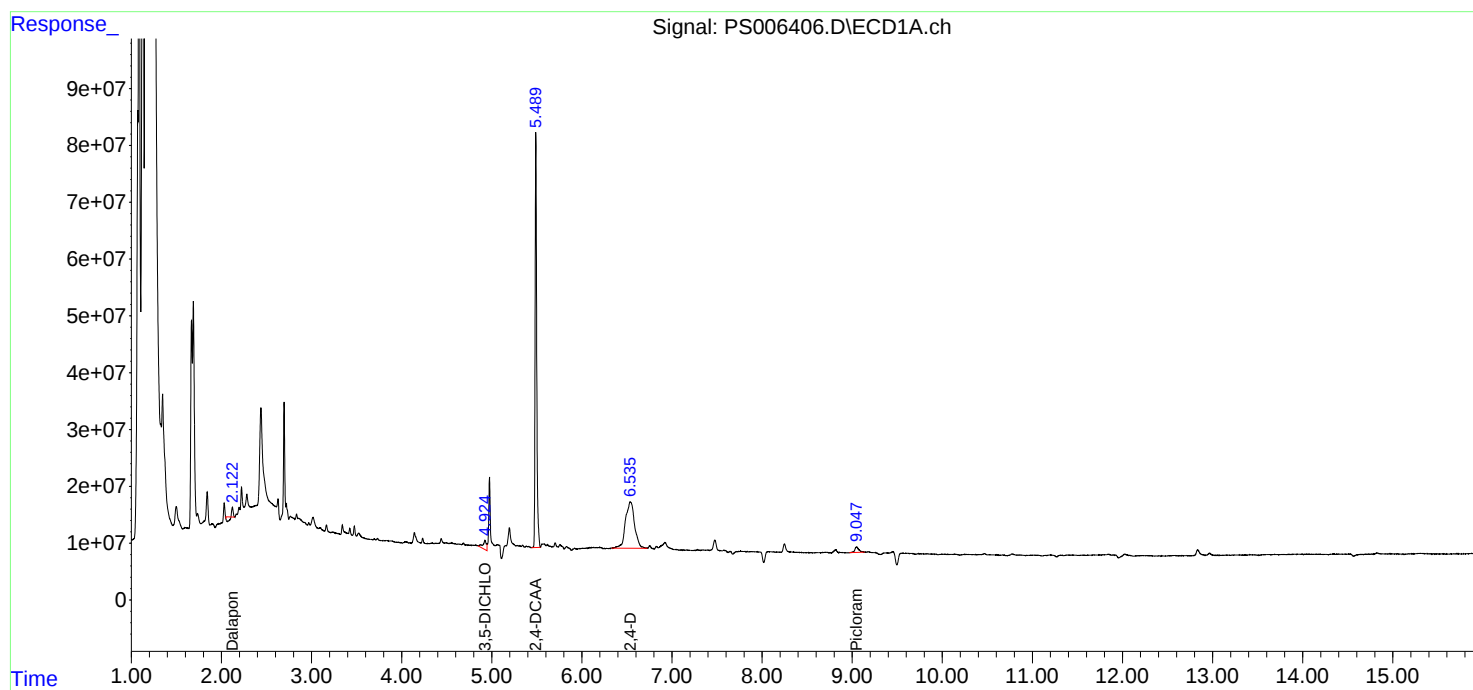


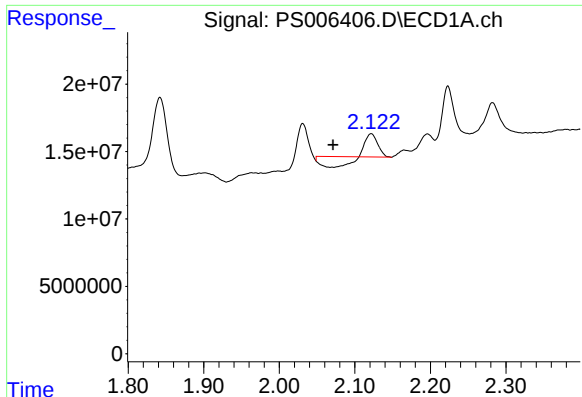

#1 Dalapon


R.T.: 2.122 min
Delta R.T.: 0.051 min
Response: 6178760
Conc: 5.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
T9-12-13-D(0-1.9)

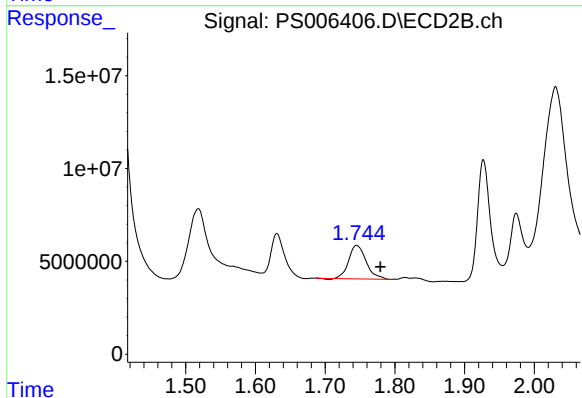


#1 Dalapon

R.T.: 1.745 min
Delta R.T.: -0.034 min
Response: 31574102
Conc: 50.32 ng/ml

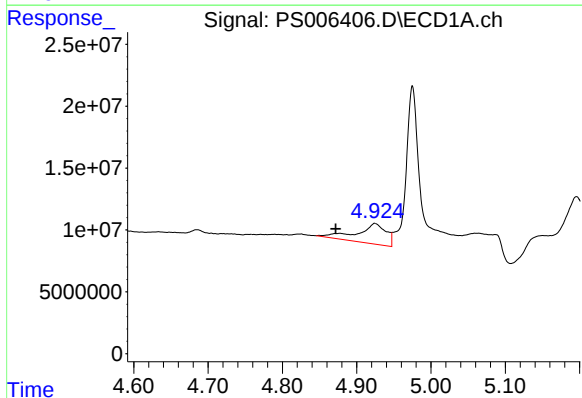


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.925 min
Delta R.T.: 0.053 min
Response: 44420886
Conc: 41.20 ng/ml

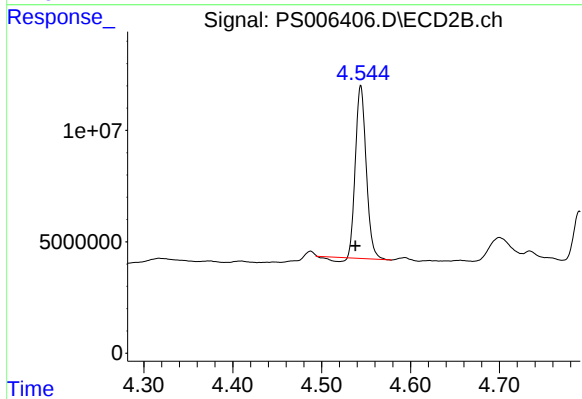

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.544 min
Delta R.T.: 0.006 min
Response: 64145708
Conc: 105.90 ng/ml

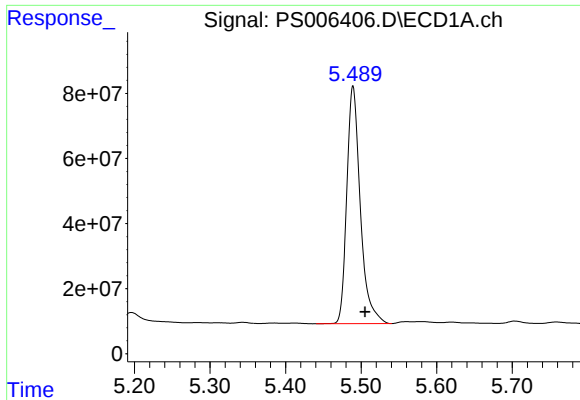

#4 2,4-DCAA


R.T.: 5.489 min
Delta R.T.: -0.016 min
Response: 908660979
Conc: 1052.66 ng/ml

Instrument :
ECD_S
ClientSampleId :
T9-12-13-D(0-1.9)

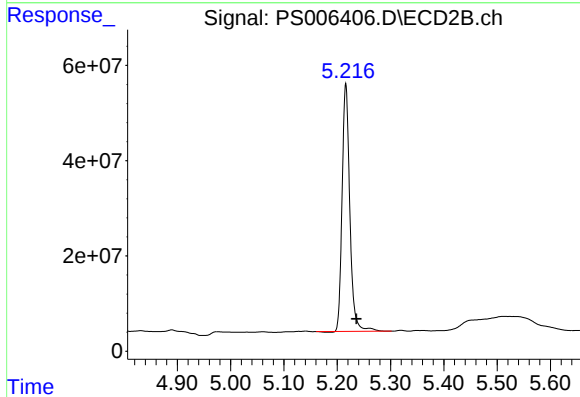


#4 2,4-DCAA

R.T.: 5.216 min
Delta R.T.: -0.020 min
Response: 523332532
Conc: 1064.00 ng/ml

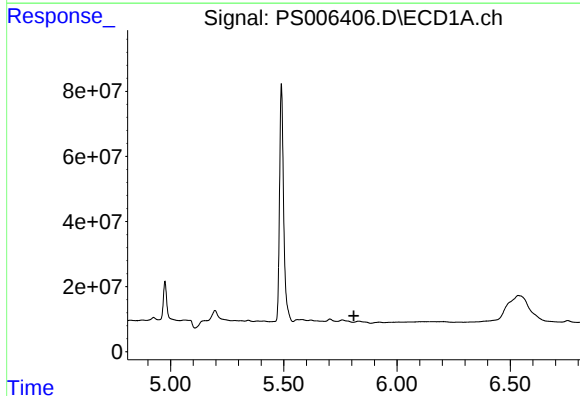


#6 MCP

R.T.: 0.000 min
Exp R.T. : 5.810 min
Response: 0
Conc: N.D.

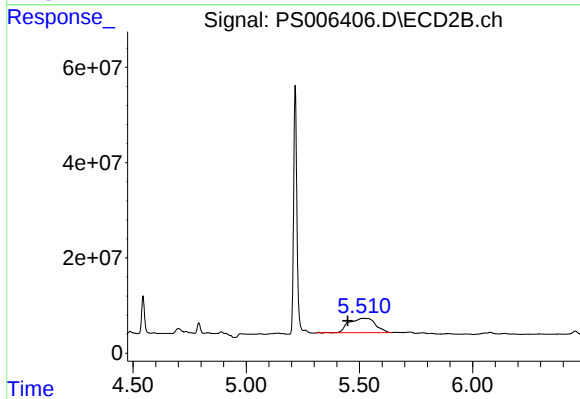

#6 MCP


R.T.: 5.513 min
Delta R.T.: 0.065 min
Response: 243646033
Conc: 196.95 ug/ml

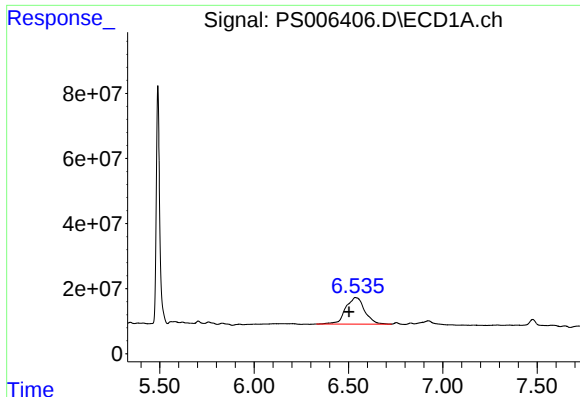

#9 2,4-D


R.T.: 6.536 min
Delta R.T.: 0.033 min
Response: 571451565
Conc: 701.35 ng/ml

Instrument :
ECD_S
ClientSampleId :
T9-12-13-D(0-1.9)

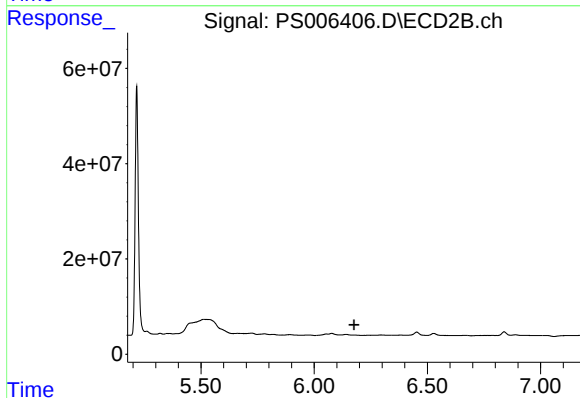


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.176 min
Response: 0
Conc: N.D.

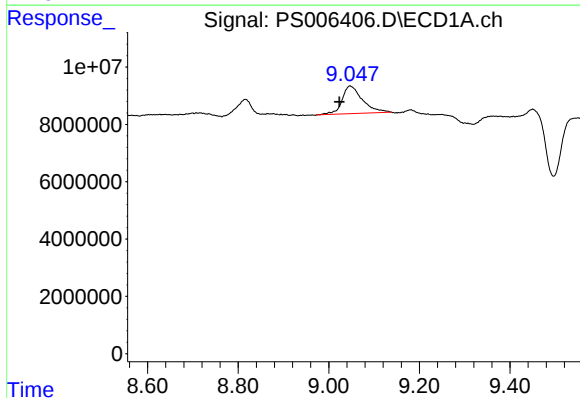


#15 Picloram

R.T.: 9.047 min
Delta R.T.: 0.024 min
Response: 29913677
Conc: 4.02 ng/ml

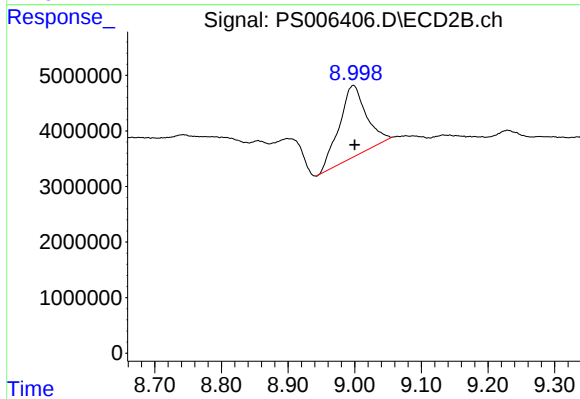

#15 Picloram


R.T.: 8.998 min
Delta R.T.: -0.002 min
Response: 36321587
Conc: 8.05 ng/ml

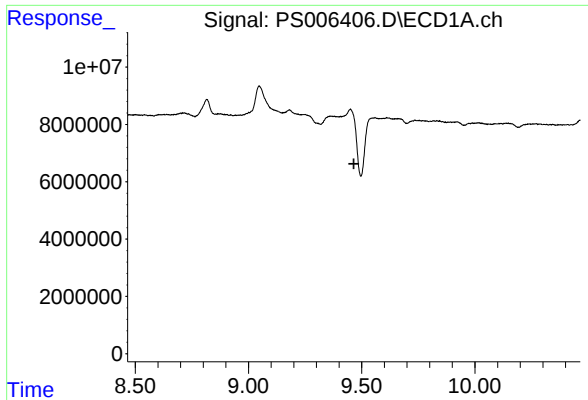

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
T9-12-13-D(0-1.9)

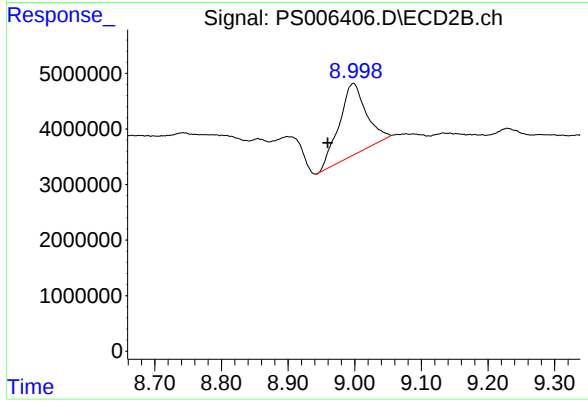

#16 DCPA

R.T.: 8.998 min
Delta R.T.: 0.038 min
Response: 36321587
Conc: 10.42 ng/ml