

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082924\
 Data File : PS027536.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2024 14:23
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 MH-21

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 06:14:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081924.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 19 14:50:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.153	7.731	1299.6E6	1019.2E6	502.486	516.243
Target Compounds							
1) T	Dalapon	2.618f	2.686	44855	4439238	<MDL	1.215 #
2) T	3,5-DICHL...	0.000	6.684	0	675407	N.D.	<MDL
3) T	4-Nitroph...	6.949	0.000	7968652	0	5.117	N.D. #
5) T	DICAMBA	0.000	7.928	0	61905159	N.D.	6.767
6) T	MCP	7.569f	8.040	20318327	71008089	2.652	11.665 #
8) T	DICHLORPROP	0.000	8.691f	0	11442618	N.D.	5.146
9) T	2,4-D	8.264	0.000	138.9E6	0	47.666	N.D. #
10) T	Pentachlo...	8.585f	0.000	8223352	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.164f	0.000	3422893	0	<MDL	N.D. #
12) T	2,4,5-T	9.435	10.275	990713	2626916	<MDL	<MDL #
13) T	2,4-DB	10.011f	10.861	12747995	68343	5.962	<MDL #
14) T	DINOSEB	11.125f	11.235	1098607	385481	<MDL	<MDL #
15) T	Picloram	10.949f	12.323	18832310	3829164	<MDL	<MDL #
16) T	DCPA	0.000	12.254	0	5361714	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082924\
Data File : PS027536.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2024 14:23
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
MH-21

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 06:14:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081924.M
Quant Title : 8080.M
QLast Update : Mon Aug 19 14:50:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

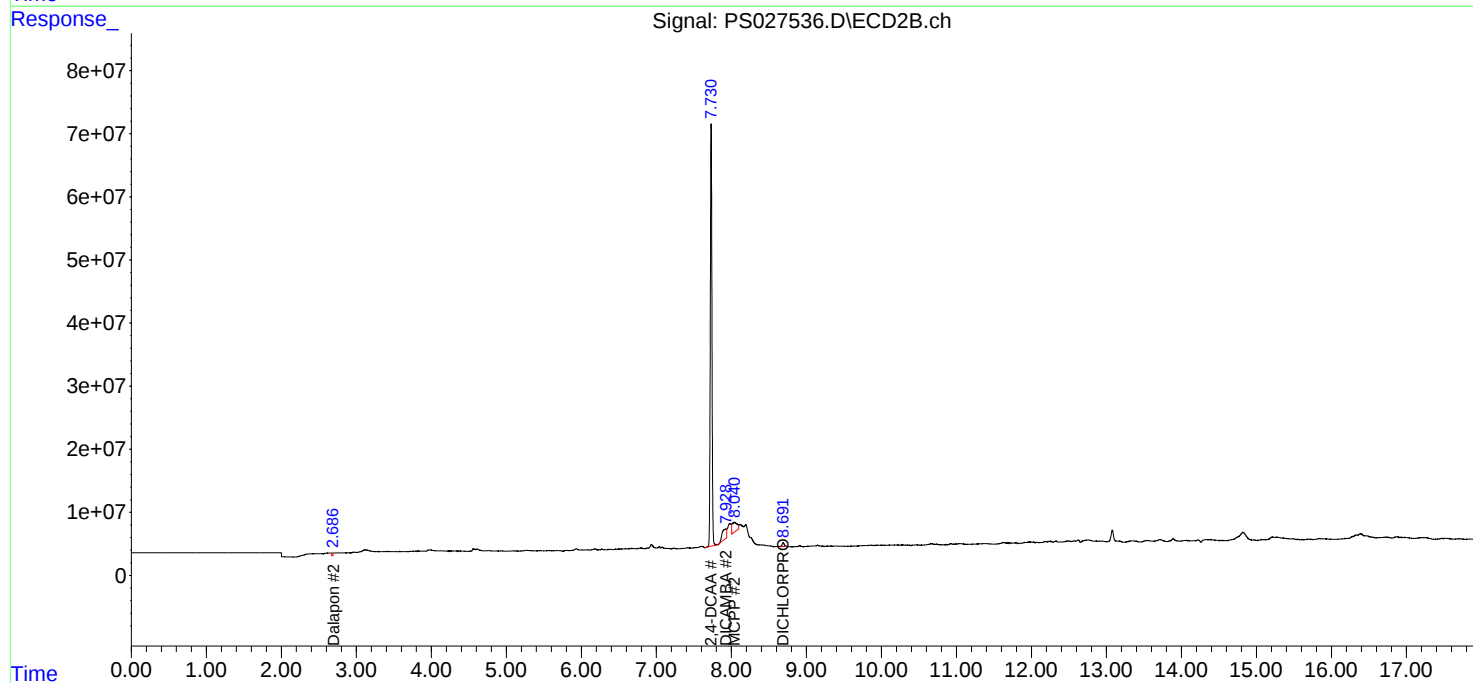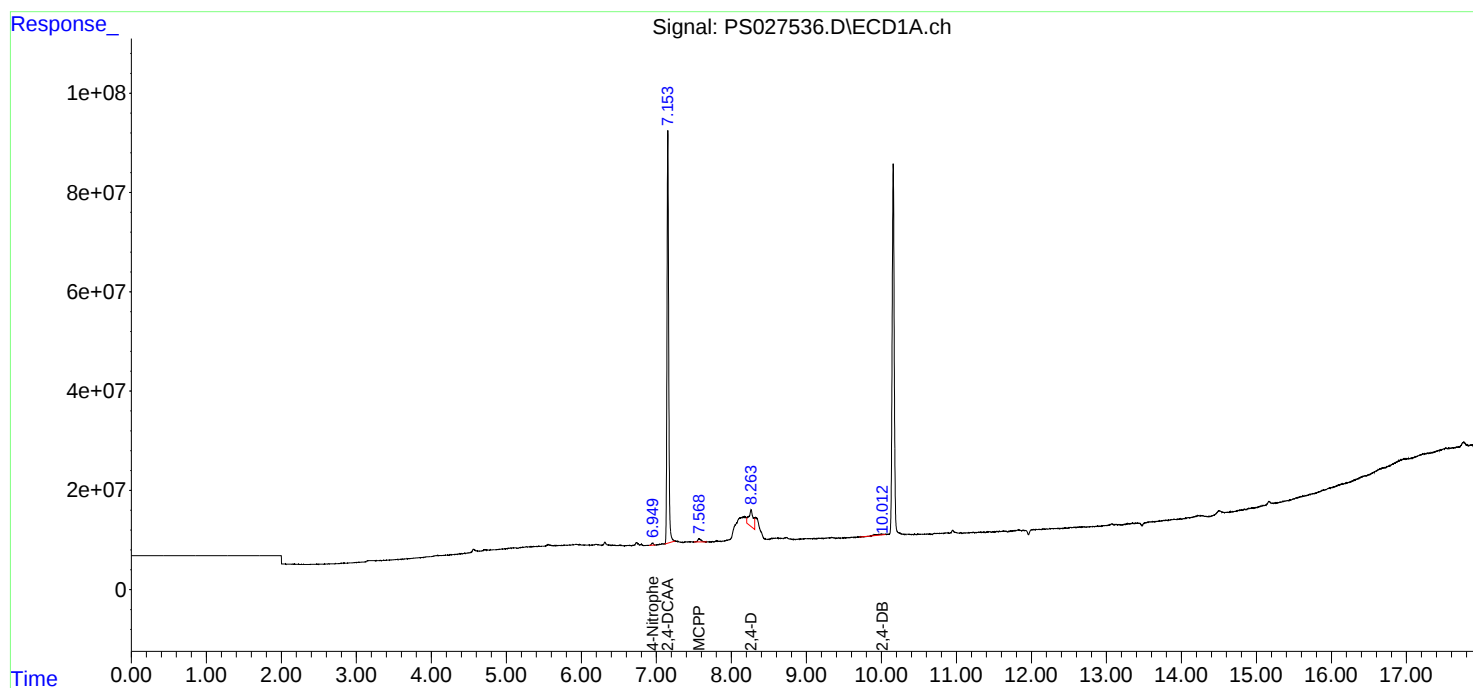


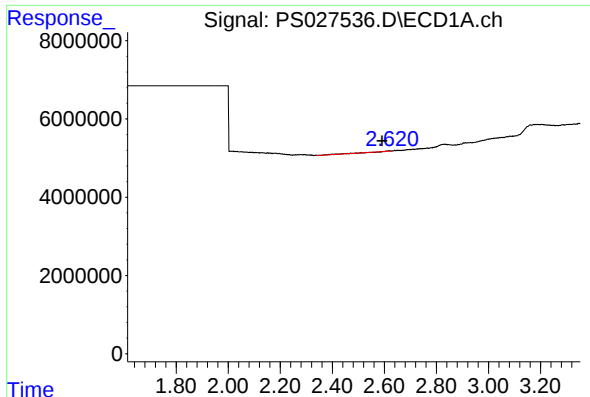

#1 Dalapon


R.T.: 2.618 min
Delta R.T.: 0.026 min
Response: 44855
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
MH-21

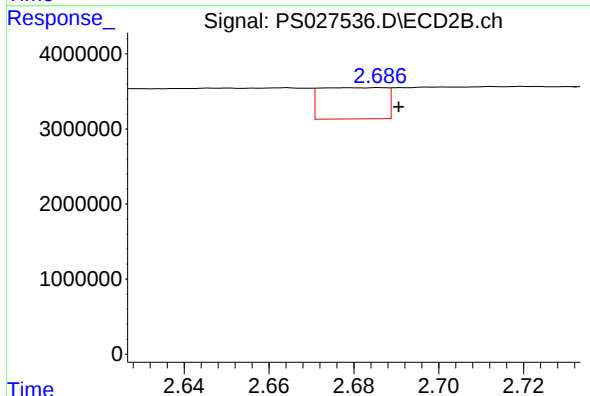


#1 Dalapon

R.T.: 2.686 min
Delta R.T.: -0.005 min
Response: 4439238
Conc: 1.22 ng/ml

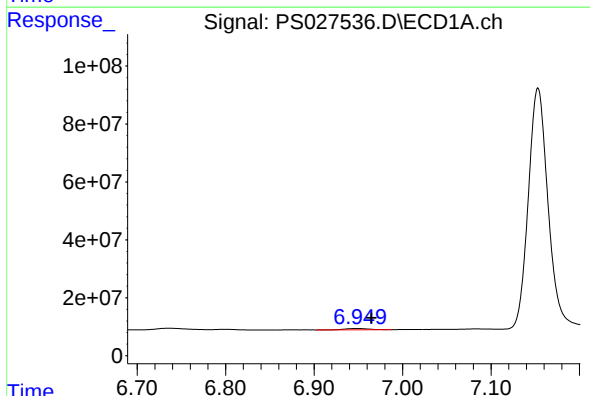


#3 4-Nitrophenol

R.T.: 6.949 min
Delta R.T.: -0.016 min
Response: 7968652
Conc: 5.12 ng/ml

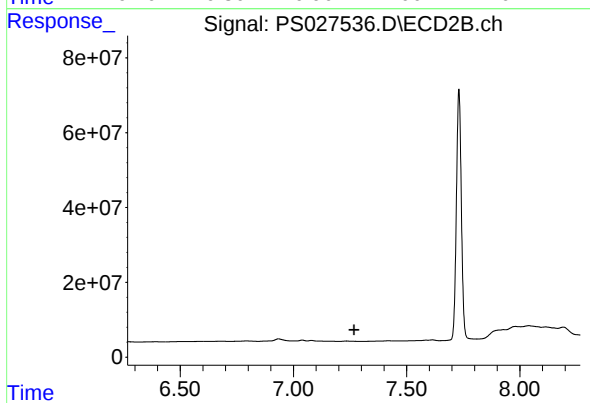

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.267 min
Response: 0
Conc: N.D.

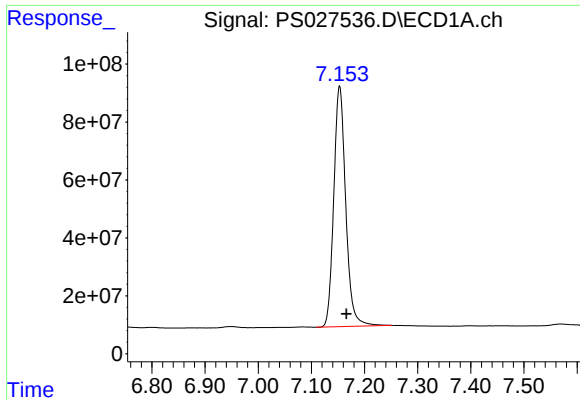

#4 2,4-DCAA


R.T.: 7.153 min
Delta R.T.: -0.013 min
Response: 1299559520
Conc: 502.49 ng/ml

Instrument :
ECD_S
ClientSampleId :
MH-21

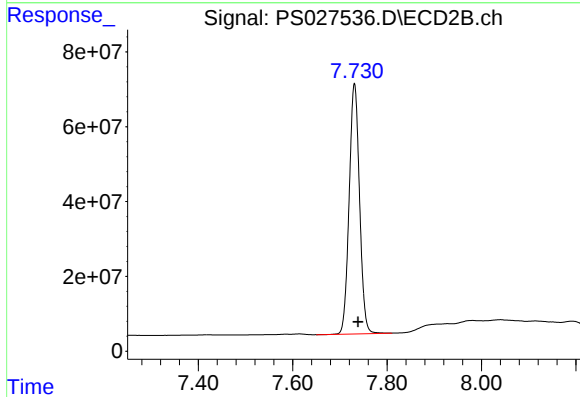


#4 2,4-DCAA

R.T.: 7.731 min
Delta R.T.: -0.008 min
Response: 1019184660
Conc: 516.24 ng/ml

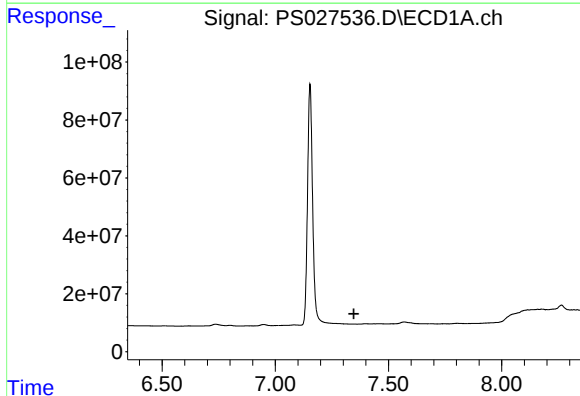


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.347 min
Response: 0
Conc: N.D.

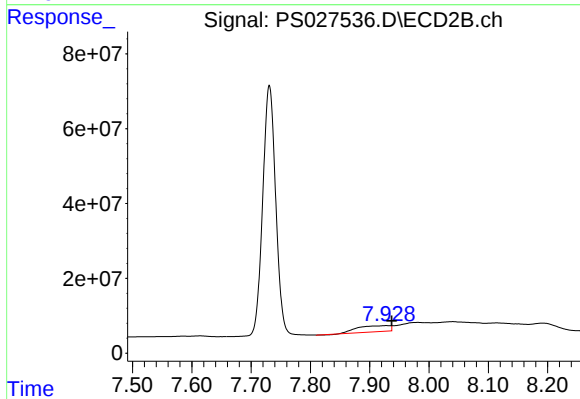

#5 DICAMBA


R.T.: 7.928 min
Delta R.T.: -0.009 min
Response: 61905159
Conc: 6.77 ng/ml

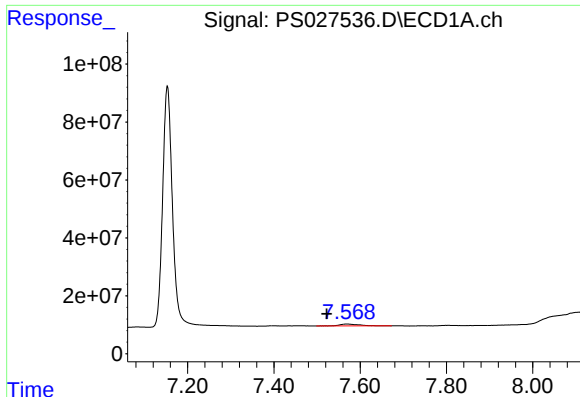

#6 MCP


R.T.: 7.569 min
Delta R.T.: 0.046 min
Response: 20318327
Conc: 2.65 ug/ml

Instrument :
ECD_S
ClientSampleId :
MH-21

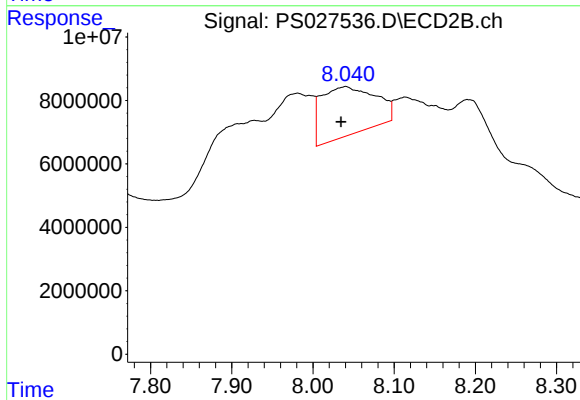


#6 MCP

R.T.: 8.040 min
Delta R.T.: 0.006 min
Response: 71008089
Conc: 11.66 ug/ml

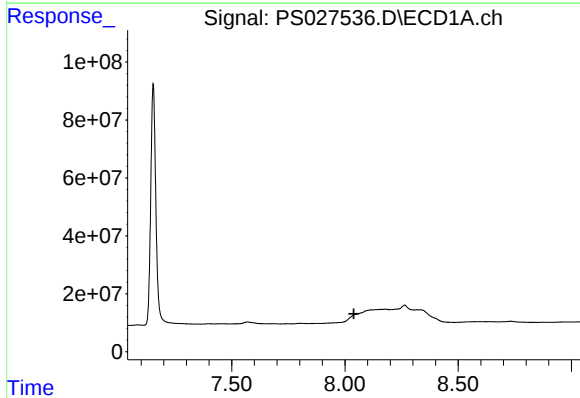


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.040 min
Response: 0
Conc: N.D.

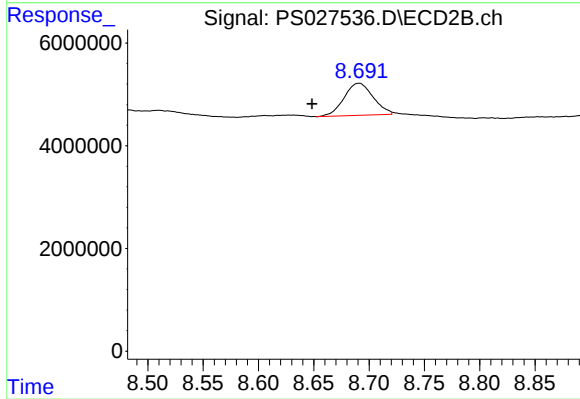

#8 DICHLORPROP


R.T.: 8.691 min
Delta R.T.: 0.042 min
Response: 11442618
Conc: 5.15 ng/ml

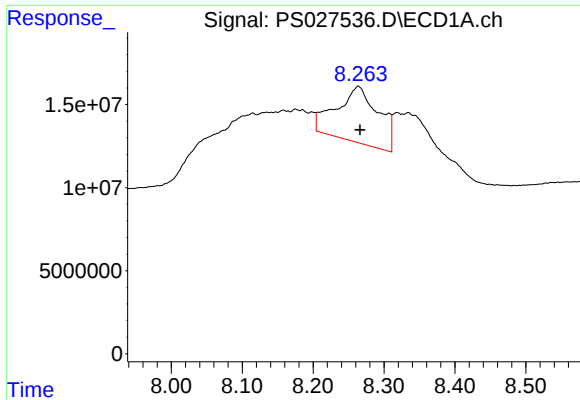

#9 2,4-D


R.T.: 8.264 min
Delta R.T.: -0.002 min
Response: 138926844
Conc: 47.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
MH-21

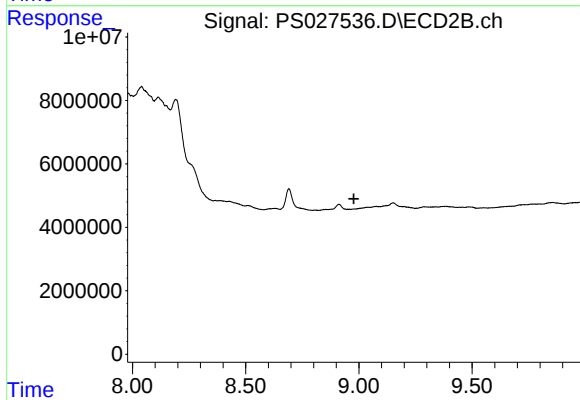


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.978 min
Response: 0
Conc: N.D.

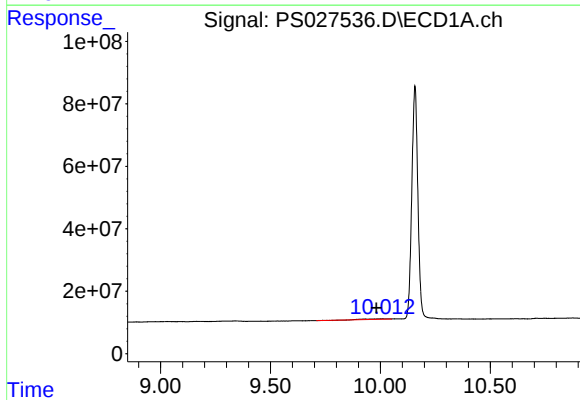

#13 2,4-DB

R.T.: 10.011 min
Delta R.T.: 0.029 min
Response: 12747995
Conc: 5.96 ng/ml

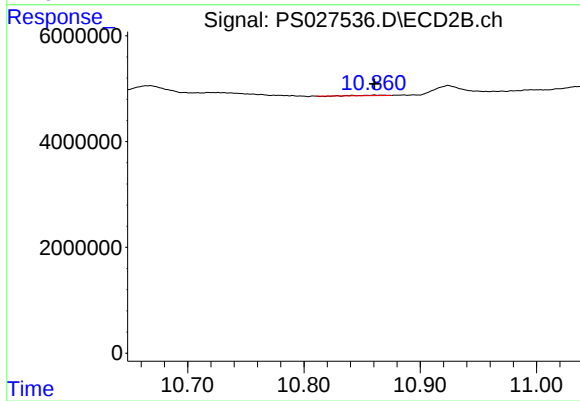

#13 2,4-DB

R.T.: 10.861 min
Delta R.T.: 0.000 min
Response: 68343
Conc: N.D.