

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083018\
 Data File : PS001644.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2018 09:16
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 00:58:44 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
10) T	Pentachlo...	13.717	0.000	2508951	0	1.006	N.D. #
12) T	2,4,5-T	14.986	14.584	3054741	4922988	3.228	5.699 #
15) T	Picloram	16.988	16.845	15714524	2334996	11.220	1.791 #
16) T	DCPA	17.565	16.903	3157894	12495738	2.783	8.752 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083018\
Data File : PS001644.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2018 09:16
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 00:58:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

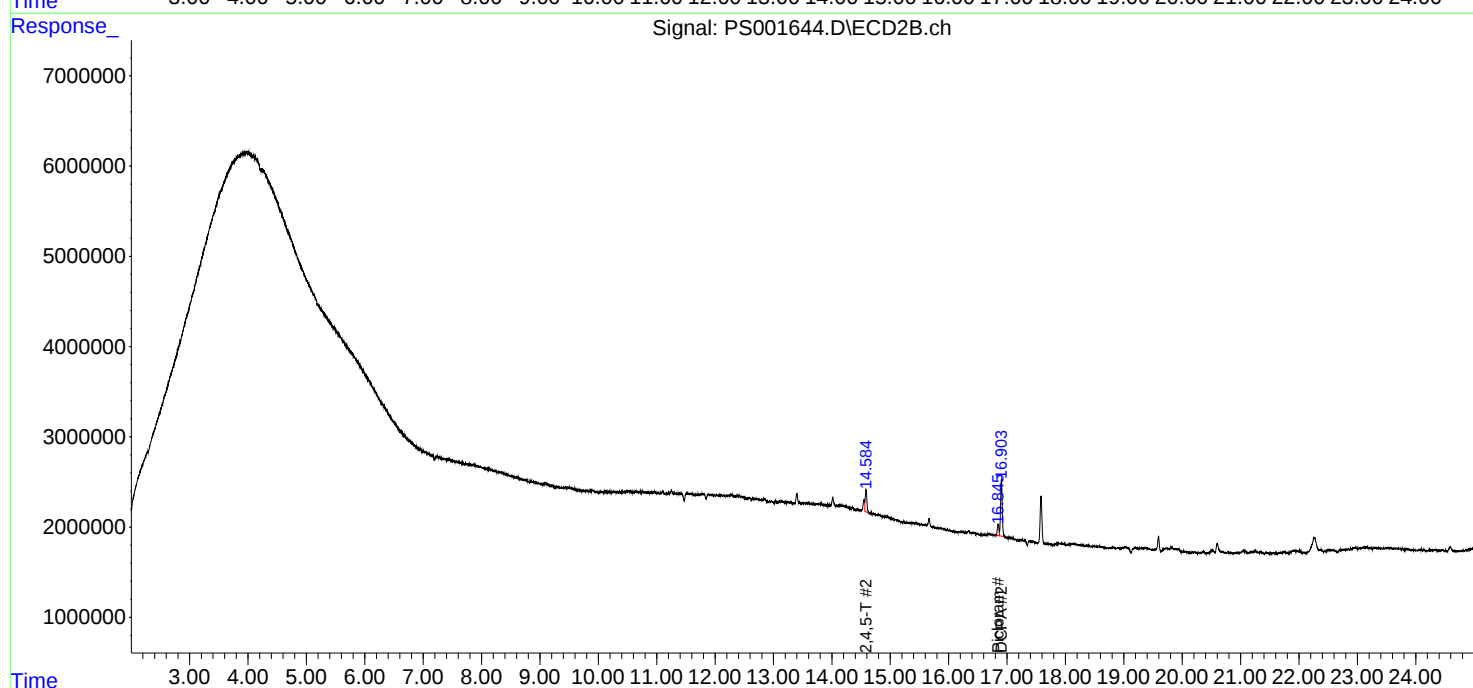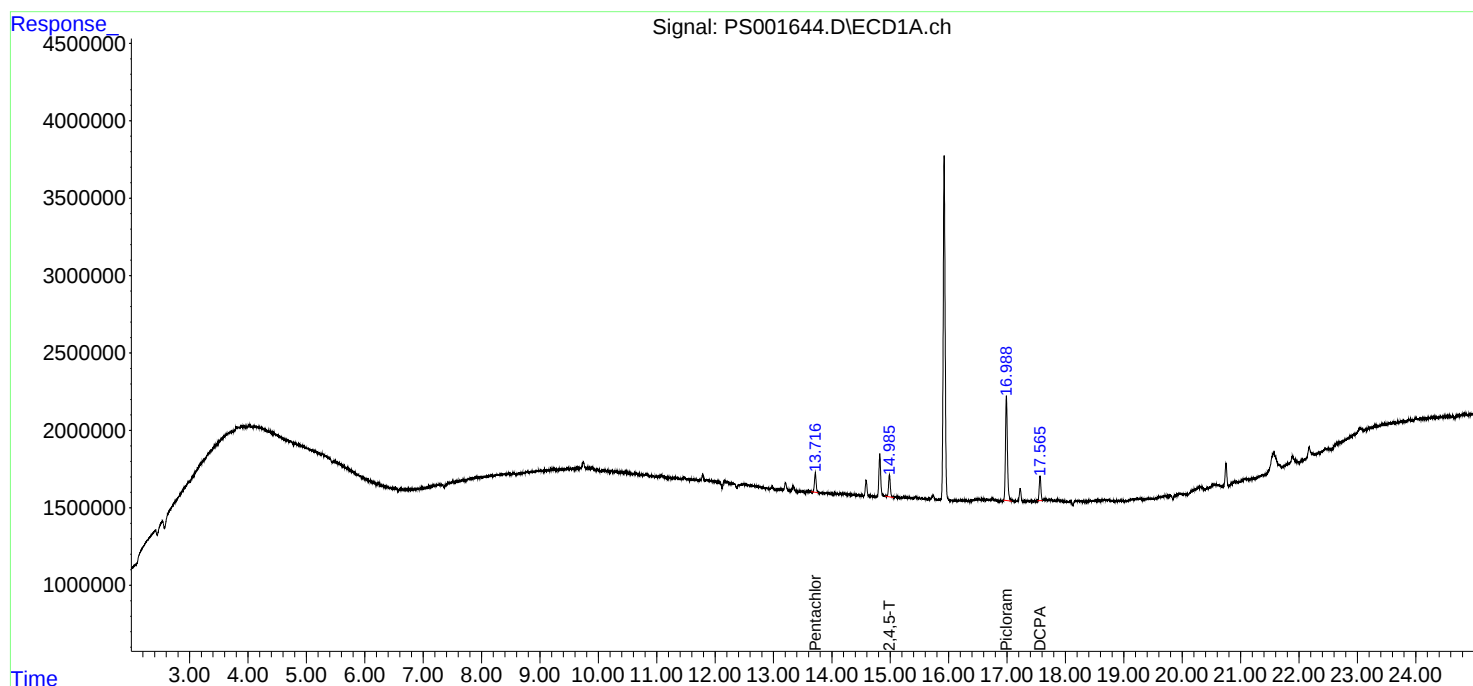


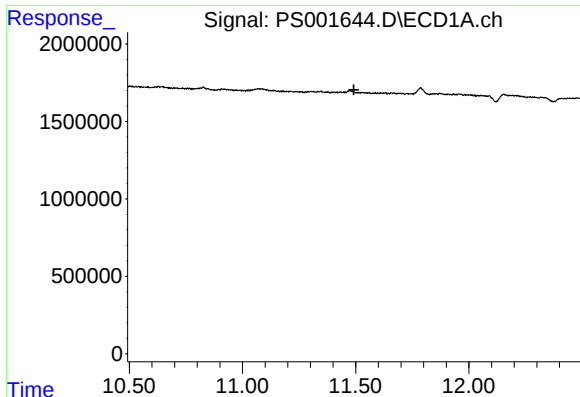

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 11.492 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

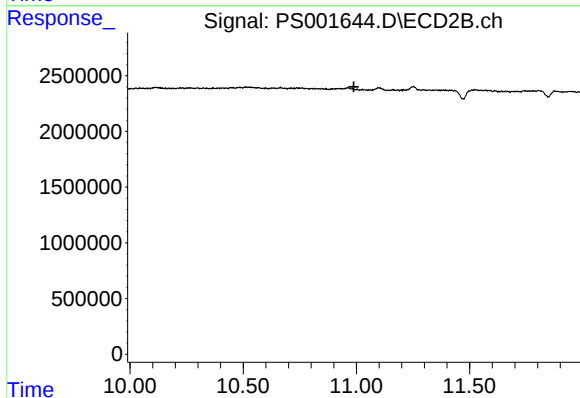


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 10.989 min
Response: 0
Conc: N.D.

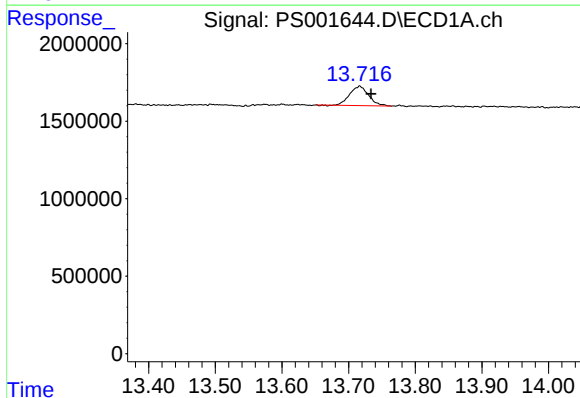


#10 Pentachlorophenol

R.T.: 13.717 min
Delta R.T.: -0.017 min
Response: 2508951
Conc: 1.01 ng/ml

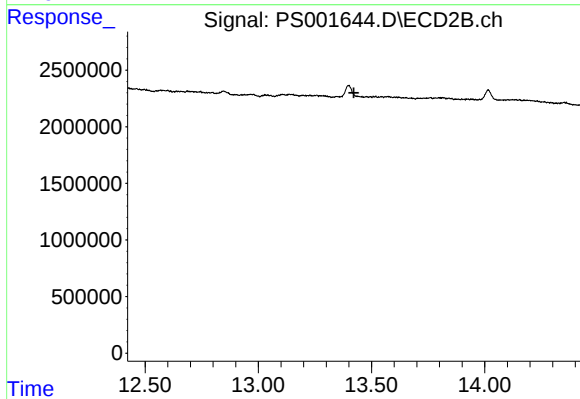

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 13.422 min
Response: 0
Conc: N.D.

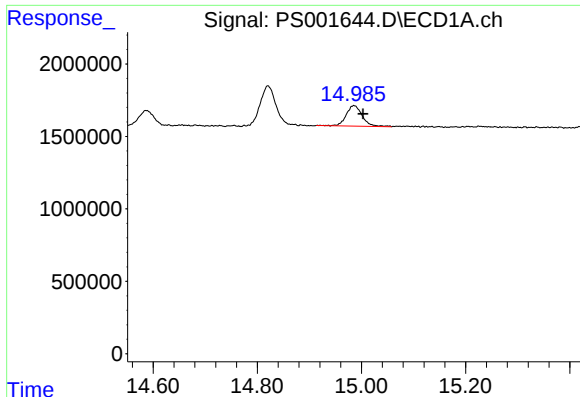

#12 2,4,5-T


R.T.: 14.986 min
Delta R.T.: -0.018 min
Response: 3054741
Conc: 3.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

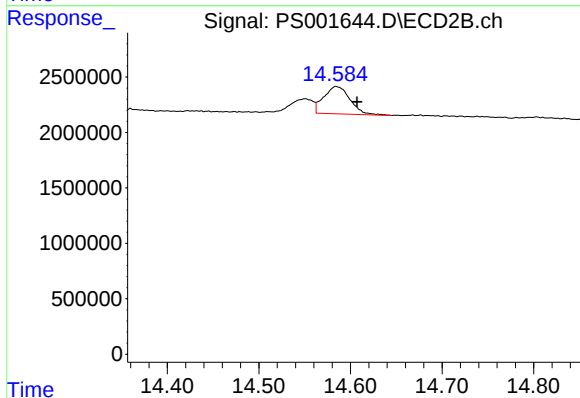


#12 2,4,5-T

R.T.: 14.584 min
Delta R.T.: -0.023 min
Response: 4922988
Conc: 5.70 ng/ml

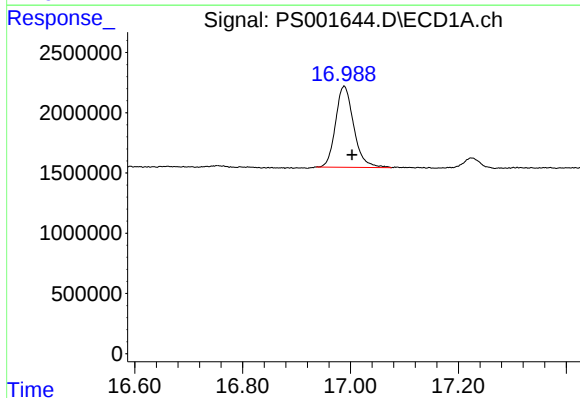


#15 Picloram

R.T.: 16.988 min
Delta R.T.: -0.015 min
Response: 15714524
Conc: 11.22 ng/ml

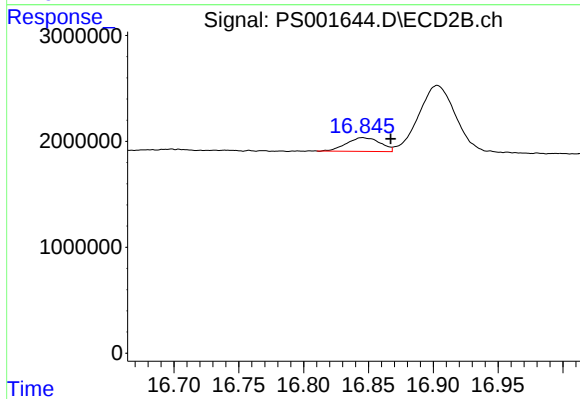

#15 Picloram


R.T.: 16.845 min
Delta R.T.: -0.022 min
Response: 2334996
Conc: 1.79 ng/ml

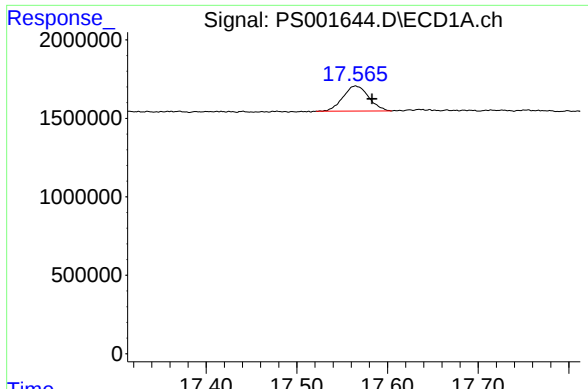

#16 DCPA

R.T.: 17.565 min
Delta R.T.: -0.018 min
Response: 3157894
Conc: 2.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

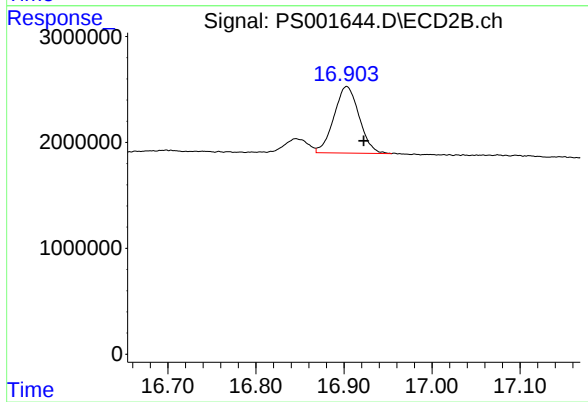

#16 DCPA

R.T.: 16.903 min
Delta R.T.: -0.019 min
Response: 12495738
Conc: 8.75 ng/ml