

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083018\
 Data File : PS001645.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2018 09:47
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 00:59:17 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.527	11.024	65202583	32693621	353.209	161.426 #
Target Compounds							
12) T	2,4,5-T	0.000	14.648	0	1993897	N.D.	2.308 #
15) T	Picloram	17.044	0.000	9749256	0	6.961	N.D. #
16) T	DCPA	0.000	16.961	0	8394079	N.D.	5.879 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083018\
Data File : PS001645.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2018 09:47
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 00:59:17 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

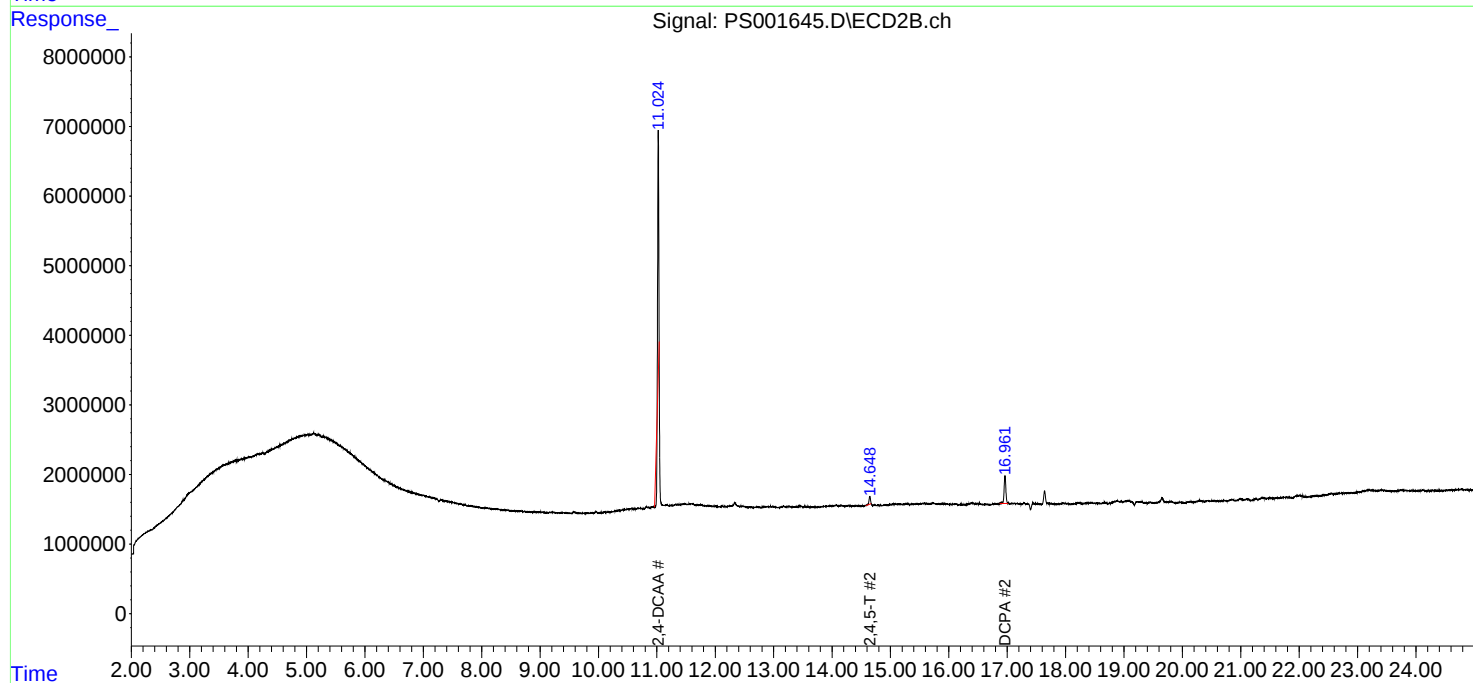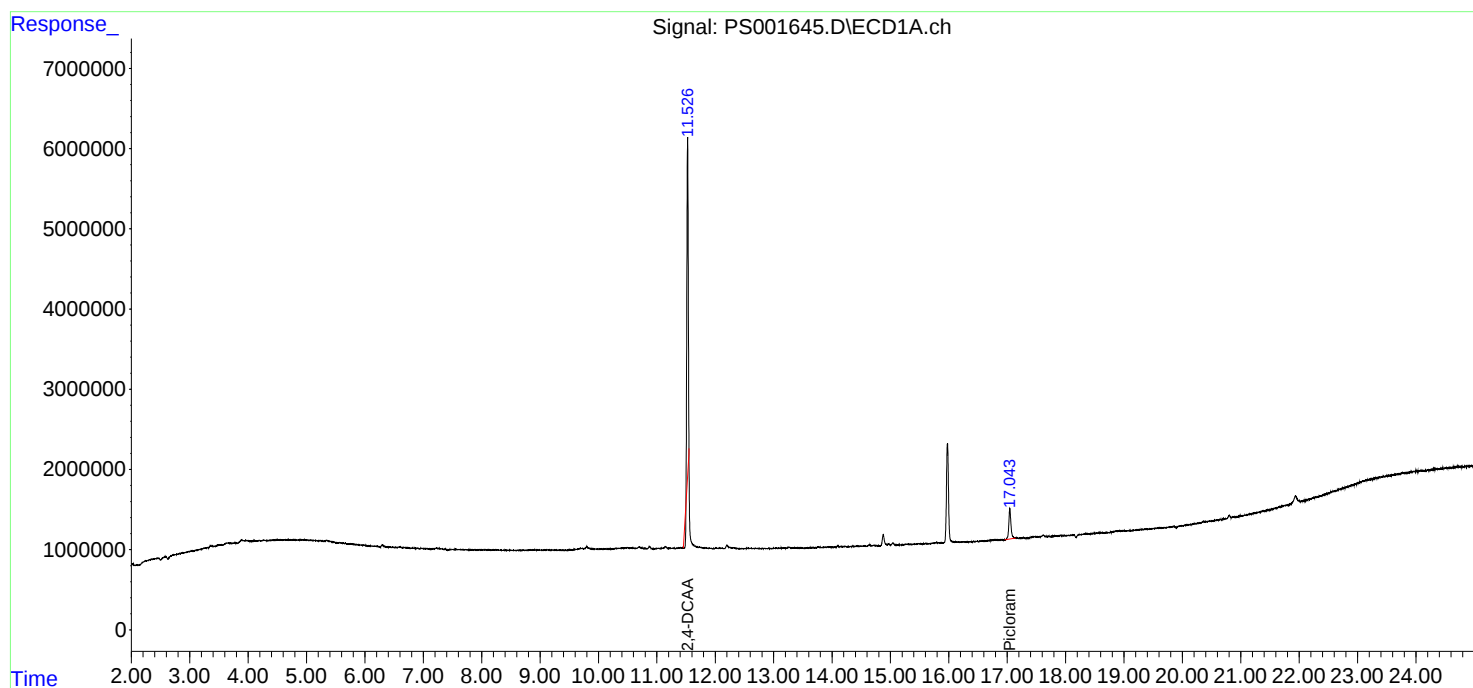


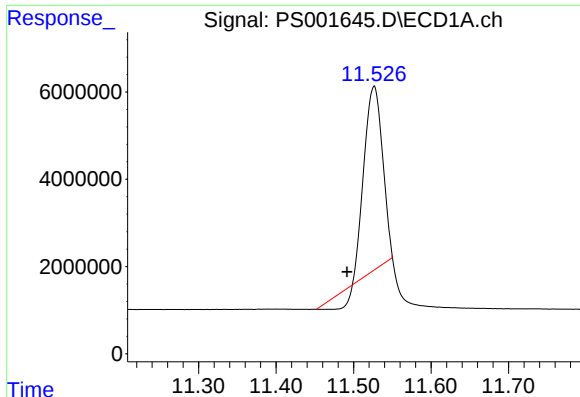

#4 2,4-DCAA


R.T.: 11.527 min
Delta R.T.: 0.035 min
Response: 65202583
Conc: 353.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

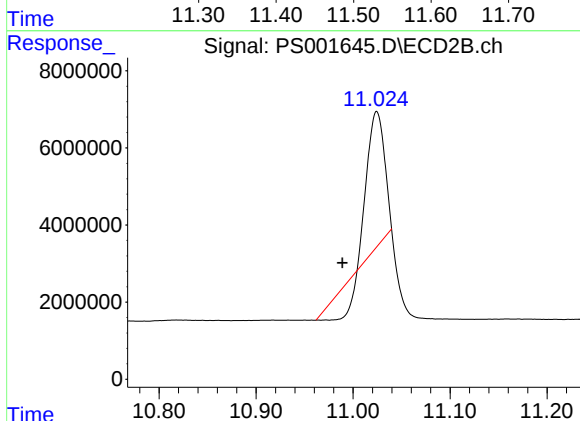


#4 2,4-DCAA

R.T.: 11.024 min
Delta R.T.: 0.035 min
Response: 32693621
Conc: 161.43 ng/ml

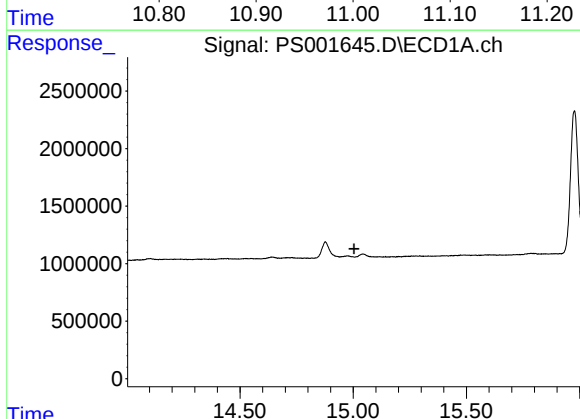


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 15.003 min
Response: 0
Conc: N.D.

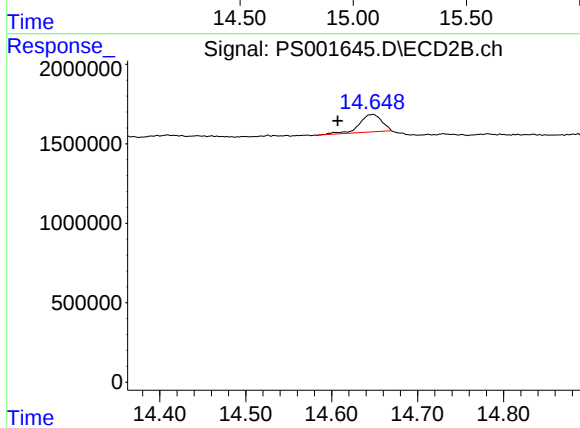

#12 2,4,5-T


R.T.: 14.648 min
Delta R.T.: 0.041 min
Response: 1993897
Conc: 2.31 ng/ml

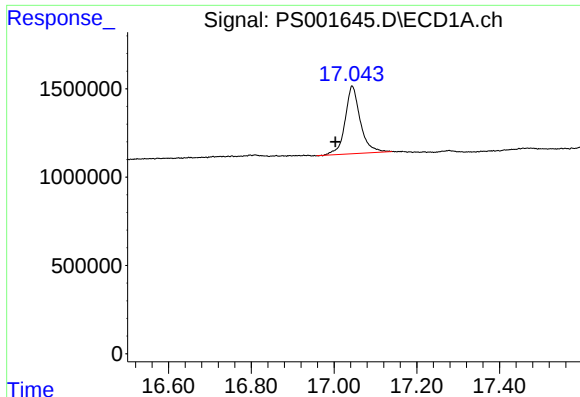

#15 Picloram


R.T.: 17.044 min
Delta R.T.: 0.041 min
Response: 9749256
Conc: 6.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

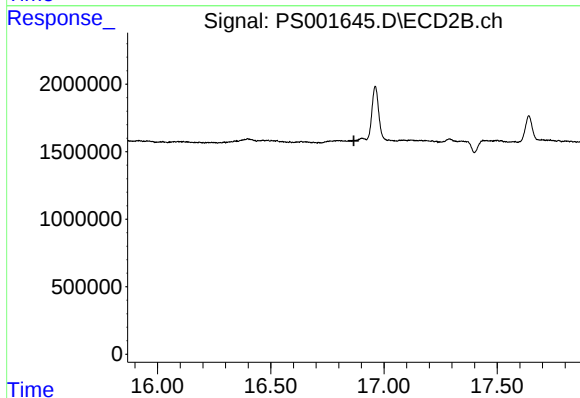


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.867 min
Response: 0
Conc: N.D.

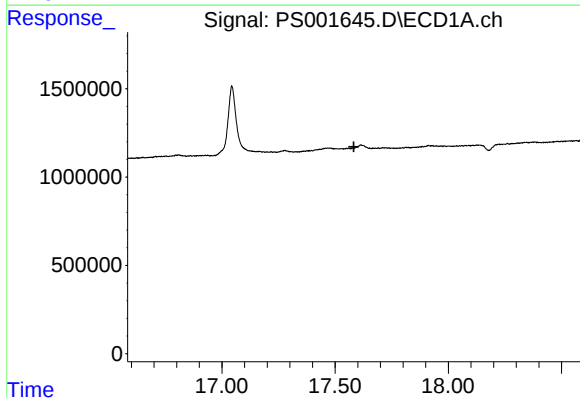

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.583 min
Response: 0
Conc: N.D.

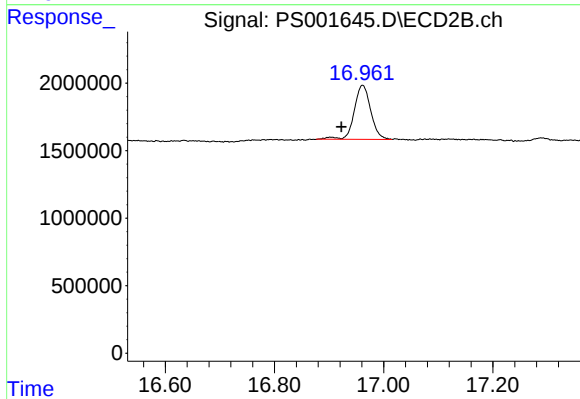

#16 DCPA

R.T.: 16.961 min
Delta R.T.: 0.039 min
Response: 8394079
Conc: 5.88 ng/ml