

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083018\
 Data File : PS001647.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2018 12:27
 Operator : EI\SJ
 Sample : IDOC 1 WATER
 Misc : HP
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 01:00:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.486	10.961	105.3E6	115.8E6	570.664	571.852
Target Compounds							
1) T	Dalapon	2.951	2.387	127.6E6	68496910	507.753	286.205 #
2) T	3,5-DICHL...	9.908	9.108	141.3E6	133.2E6	527.537	521.375
3) T	4-Nitroph...	11.076	10.105	64630632	6081634	524.206	57.699 #
5) T	DICAMBA	11.799	11.247	370.2E6	312.8E6	529.940	446.033
6) T	MCPD	12.137	0.000	27772529	0	55.196	N.D. #
7) T	MCPA	12.387	0.000	45962425	0	55.051	N.D. #
8) T	DICHLORPROP	12.988	12.373	101.7E6	69390936	538.376	372.538 #
9) T	2,4-D	13.346	12.845	127.3E6	101.2E6	536.889	408.450
10) T	Pentachlo...	13.729	13.396	1365.1E6	1494.3E6	547.427	552.567
11) T	2,4,5-TP ...	14.600	14.013	508.5E6	582.5E6	544.926	548.005
12) T	2,4,5-T	14.996	14.582	519.2E6	474.4E6	548.704	549.141
13) T	2,4-DB	15.745	15.231	72870755	59904362	542.503	451.732
14) T	DINOSEB	17.236	15.662	353.0E6	364.5E6	540.991	492.913
15) T	Picloram	16.997	16.844	753.6E6	691.2E6	538.050	530.084
16) T	DCPA	17.577	16.899	638.0E6	735.2E6	562.308	514.923



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083018\
Data File : PS001647.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2018 12:27
Operator : EI\SJ
Sample : IDOC 1 WATER
Misc : HP
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 01:00:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

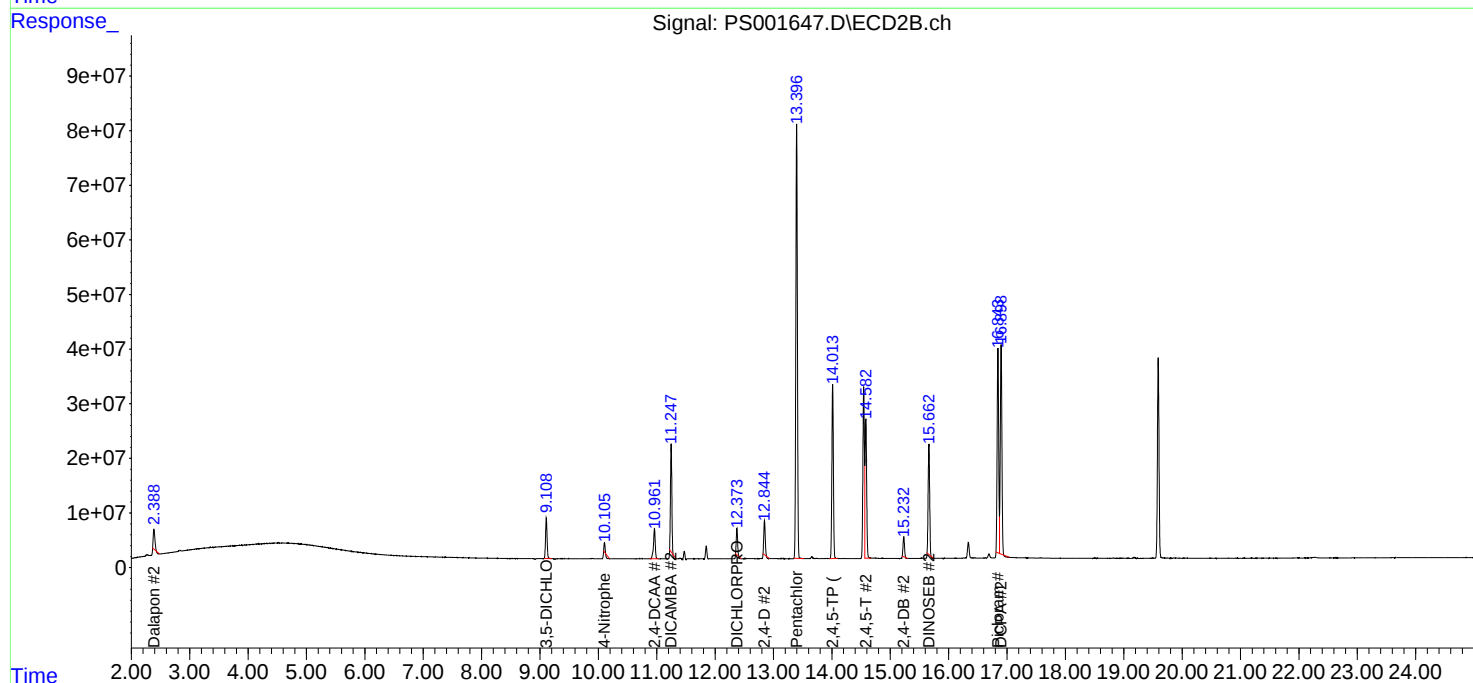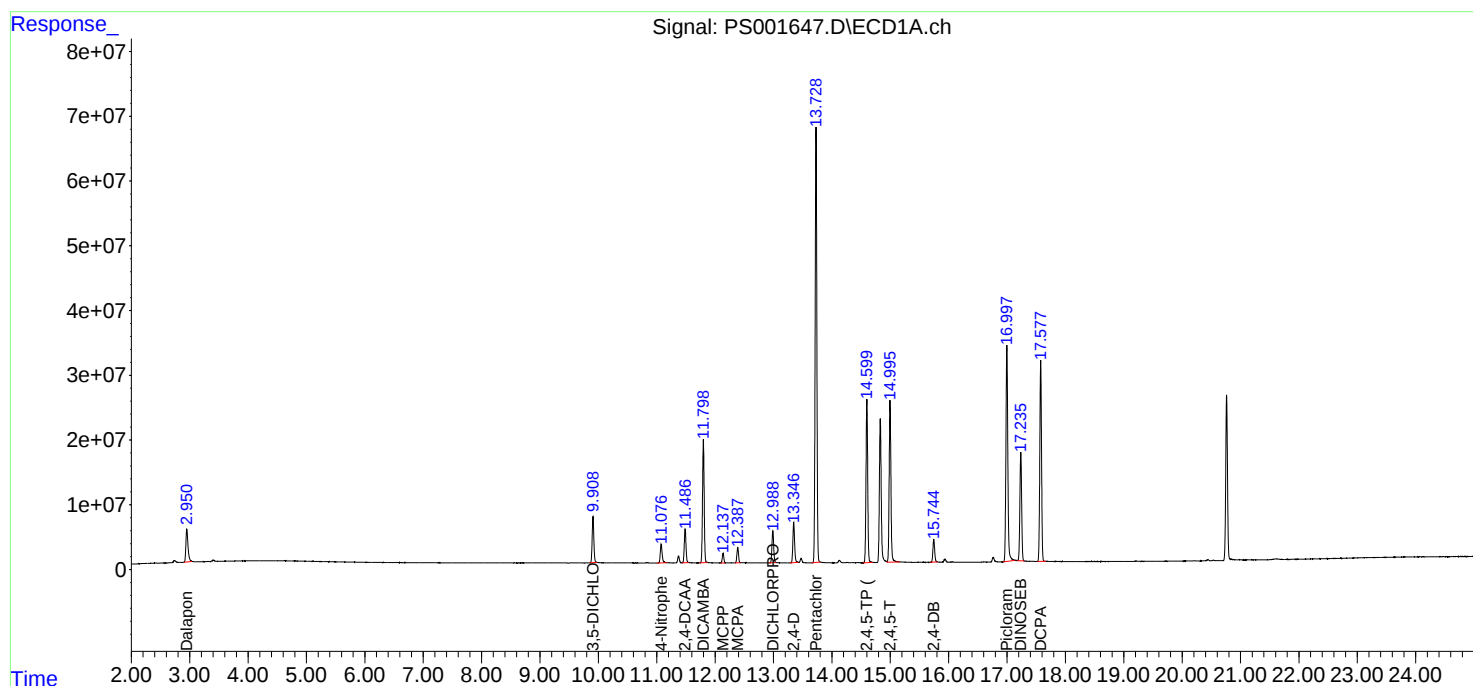


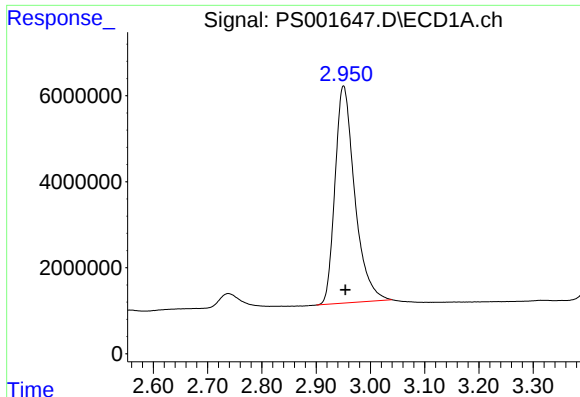

#1 Dalapon


R.T.: 2.951 min
Delta R.T.: -0.003 min
Response: 127636407
Conc: 507.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

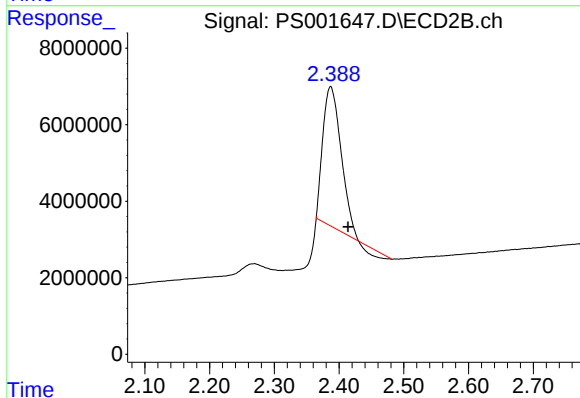


#1 Dalapon

R.T.: 2.387 min
Delta R.T.: -0.027 min
Response: 68496910
Conc: 286.20 ng/ml

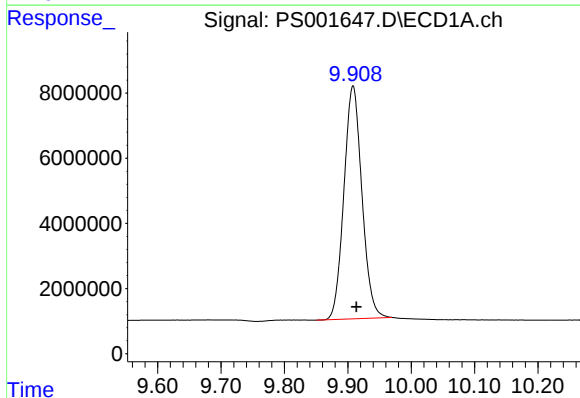


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.908 min
Delta R.T.: -0.005 min
Response: 141281520
Conc: 527.54 ng/ml

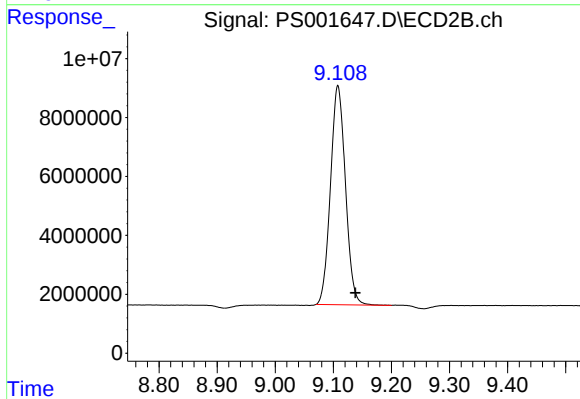

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.108 min
Delta R.T.: -0.030 min
Response: 133239912
Conc: 521.37 ng/ml

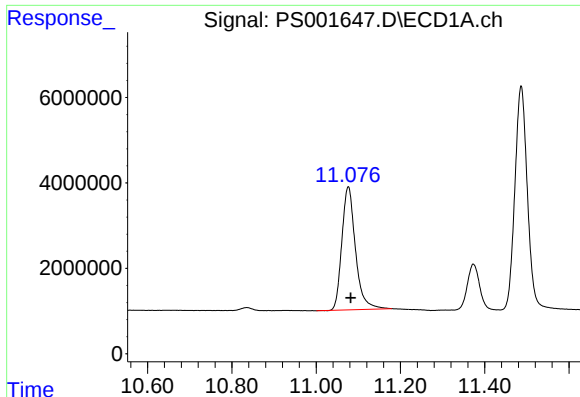

#3 4-Nitrophenol


R.T.: 11.076 min
Delta R.T.: -0.006 min
Response: 64630632
Conc: 524.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

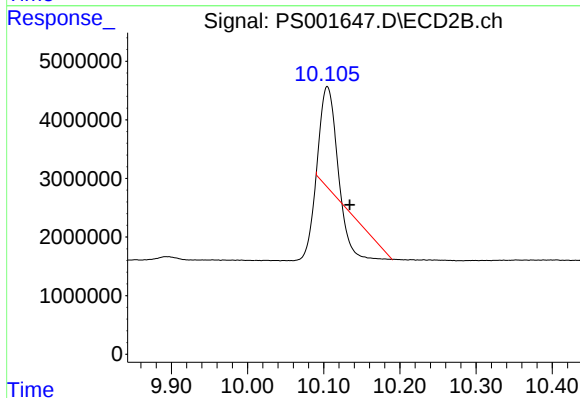


#3 4-Nitrophenol

R.T.: 10.105 min
Delta R.T.: -0.029 min
Response: 6081634
Conc: 57.70 ng/ml

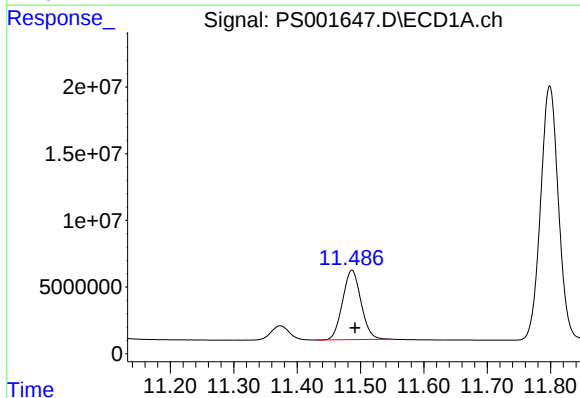


#4 2,4-DCAA

R.T.: 11.486 min
Delta R.T.: -0.005 min
Response: 105344759
Conc: 570.66 ng/ml

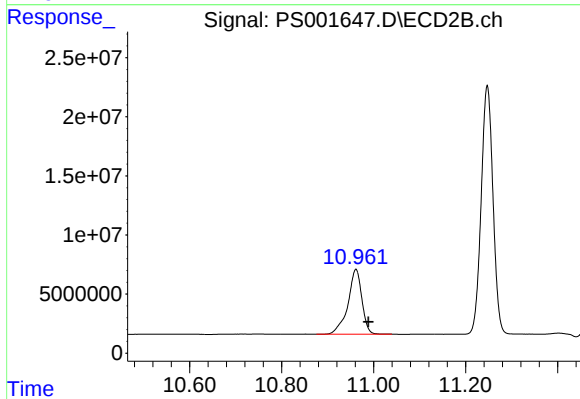

#4 2,4-DCAA


R.T.: 10.961 min
Delta R.T.: -0.027 min
Response: 115817072
Conc: 571.85 ng/ml

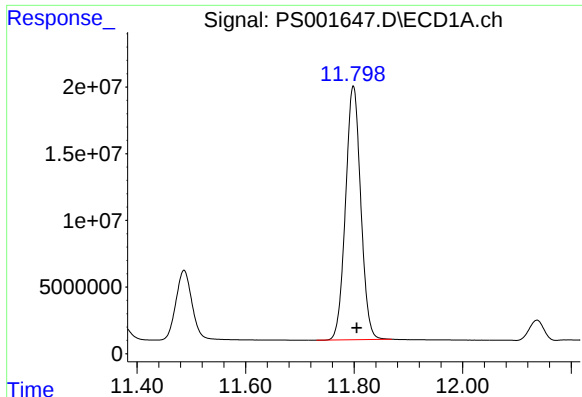

#5 DICAMBA


R.T.: 11.799 min
Delta R.T.: -0.006 min
Response: 370164357
Conc: 529.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

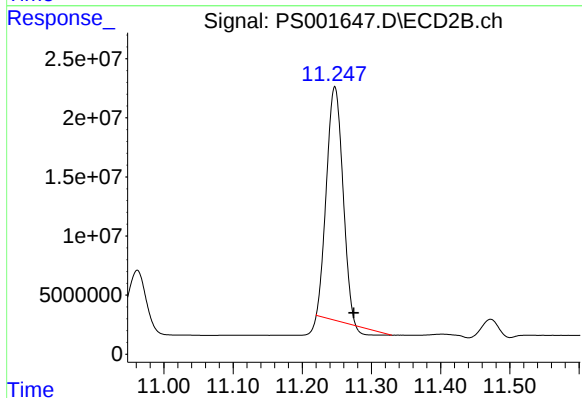


#5 DICAMBA

R.T.: 11.247 min
Delta R.T.: -0.027 min
Response: 312824092
Conc: 446.03 ng/ml

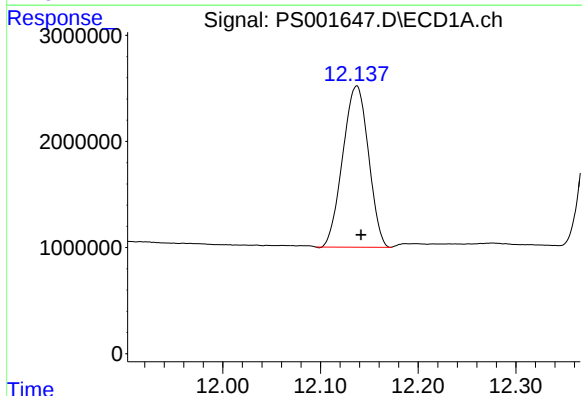


#6 MCP

R.T.: 12.137 min
Delta R.T.: -0.005 min
Response: 27772529
Conc: 55.20 ug/ml

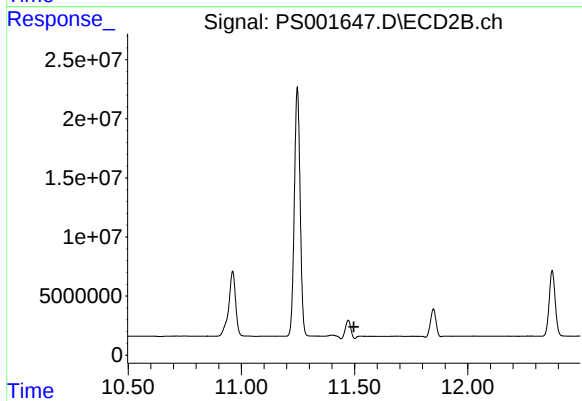

#6 MCP


R.T.: 0.000 min
Exp R.T. : 11.497 min
Response: 0
Conc: N.D.

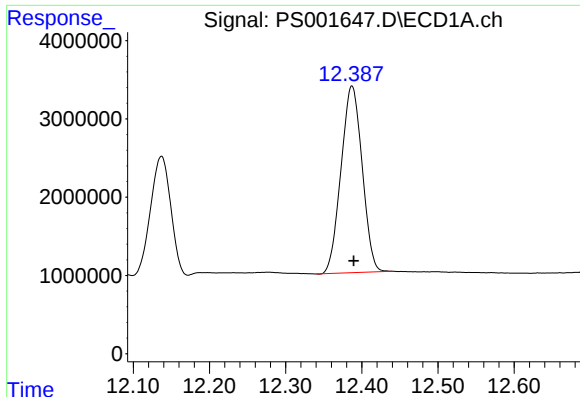

#7 MCPA


R.T.: 12.387 min
Delta R.T.: -0.003 min
Response: 45962425
Conc: 55.05 ug/ml

Instrument :
ECD_S
ClientSampleId :

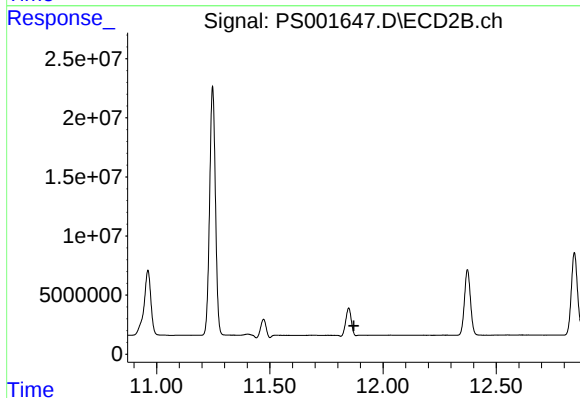


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.871 min
Response: 0
Conc: N.D.

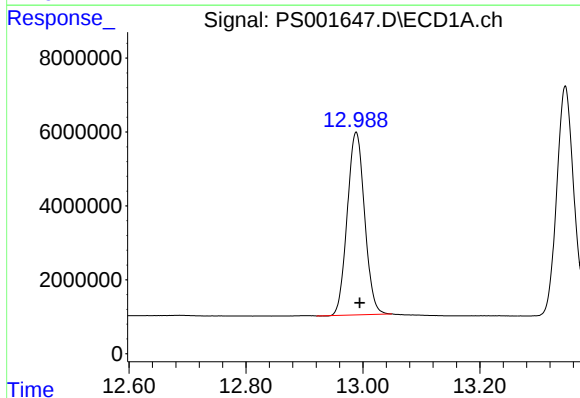


#8 DICHLORPROP

R.T.: 12.988 min
Delta R.T.: -0.006 min
Response: 101669333
Conc: 538.38 ng/ml

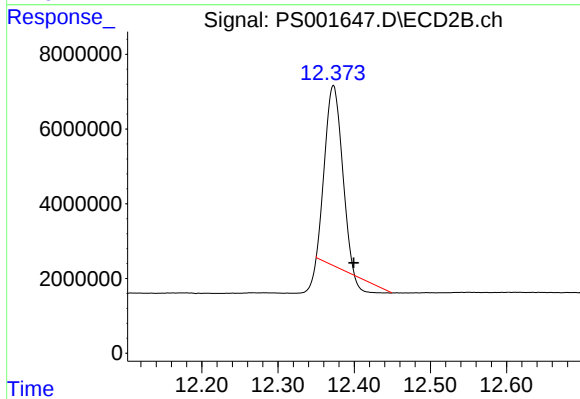

#8 DICHLORPROP


R.T.: 12.373 min
Delta R.T.: -0.027 min
Response: 69390936
Conc: 372.54 ng/ml

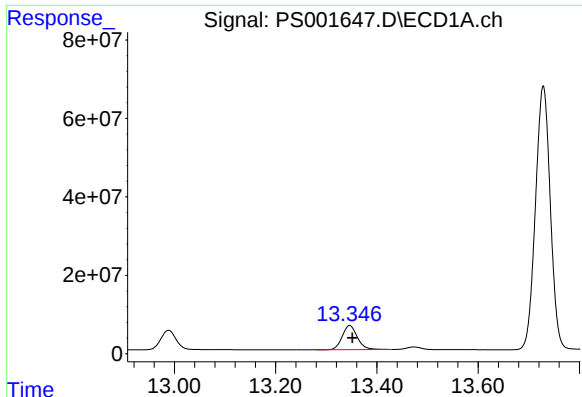

#9 2,4-D


R.T.: 13.346 min
Delta R.T.: -0.005 min
Response: 127307527
Conc: 536.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

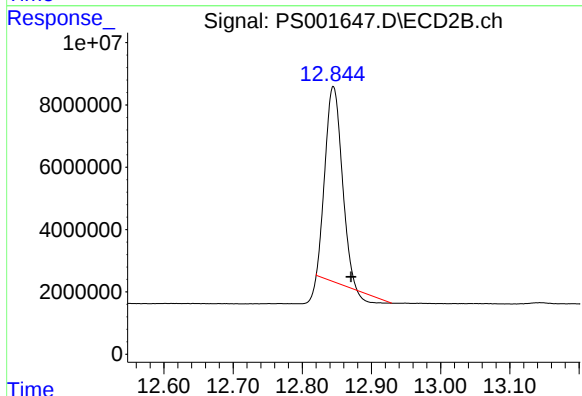


#9 2,4-D

R.T.: 12.845 min
Delta R.T.: -0.026 min
Response: 101180438
Conc: 408.45 ng/ml

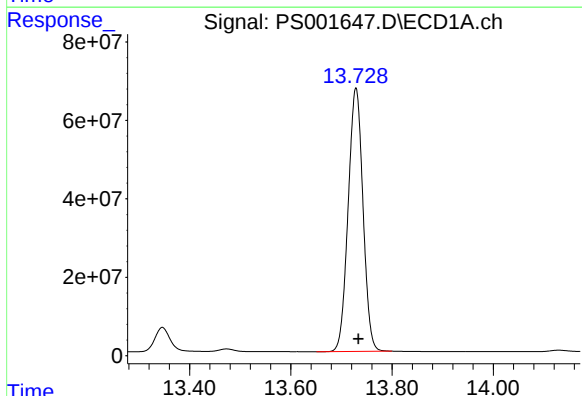


#10 Pentachlorophenol

R.T.: 13.729 min
Delta R.T.: -0.005 min
Response: 1365109892
Conc: 547.43 ng/ml

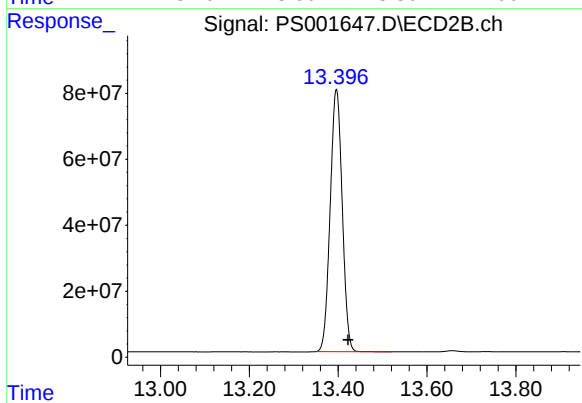

#10 Pentachlorophenol


R.T.: 13.396 min
Delta R.T.: -0.026 min
Response: 1494257455
Conc: 552.57 ng/ml

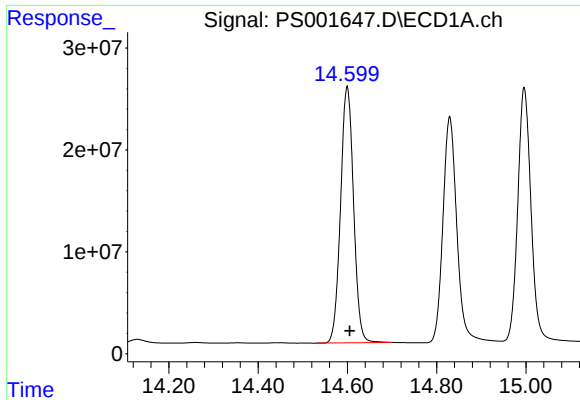

#11 2,4,5-TP (SILVEX)


R.T.: 14.600 min
Delta R.T.: -0.006 min
Response: 508517782
Conc: 544.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

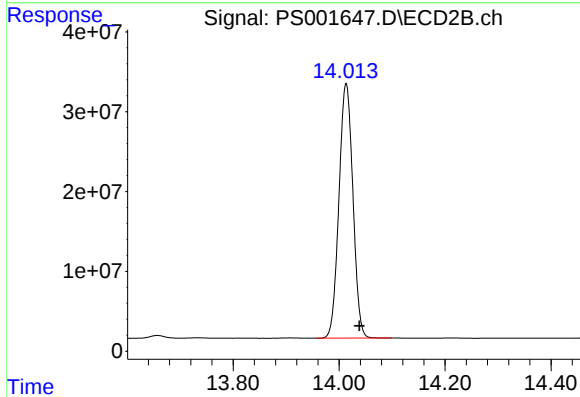


#11 2,4,5-TP (SILVEX)

R.T.: 14.013 min
Delta R.T.: -0.025 min
Response: 582451254
Conc: 548.01 ng/ml

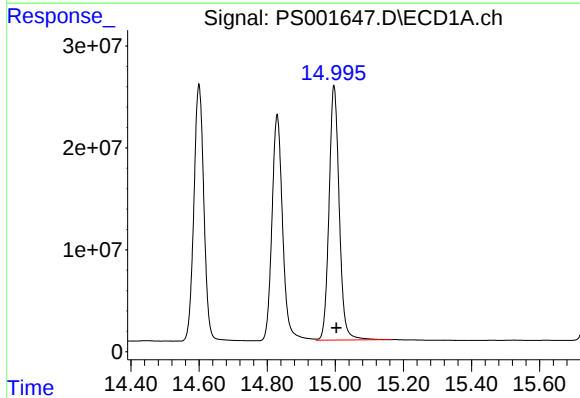


#12 2,4,5-T

R.T.: 14.996 min
Delta R.T.: -0.007 min
Response: 519248165
Conc: 548.70 ng/ml

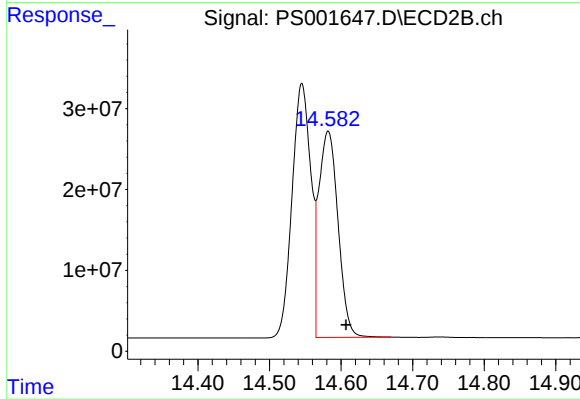

#12 2,4,5-T


R.T.: 14.582 min
Delta R.T.: -0.025 min
Response: 474376637
Conc: 549.14 ng/ml

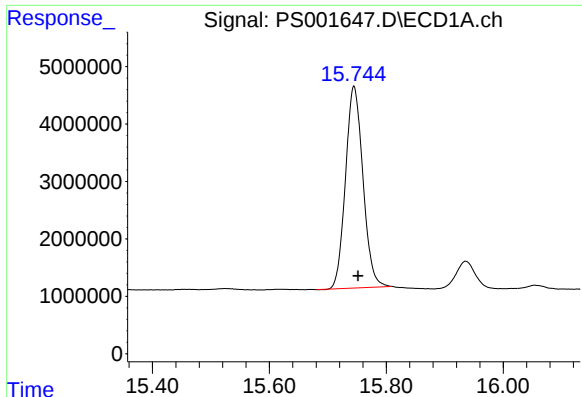

#13 2,4-DB


R.T.: 15.745 min
Delta R.T.: -0.007 min
Response: 72870755
Conc: 542.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

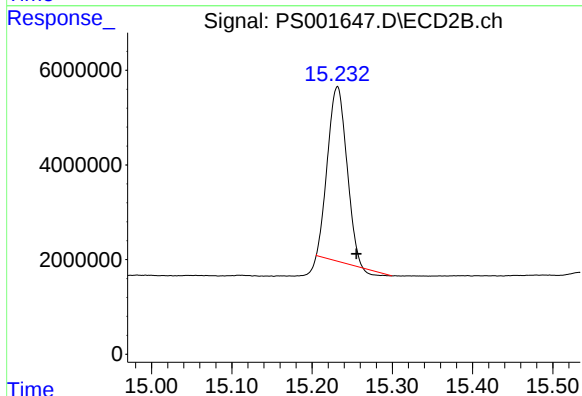


#13 2,4-DB

R.T.: 15.231 min
Delta R.T.: -0.024 min
Response: 59904362
Conc: 451.73 ng/ml

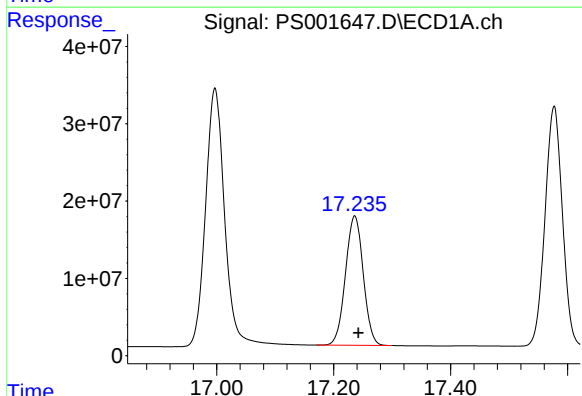


#14 DINOSEB

R.T.: 17.236 min
Delta R.T.: -0.007 min
Response: 353006564
Conc: 540.99 ng/ml

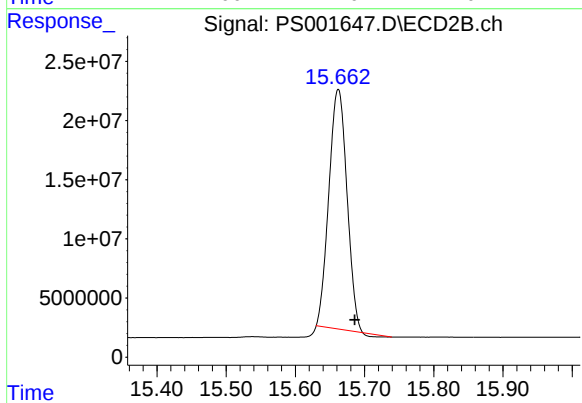

#14 DINOSEB


R.T.: 15.662 min
Delta R.T.: -0.024 min
Response: 364548727
Conc: 492.91 ng/ml

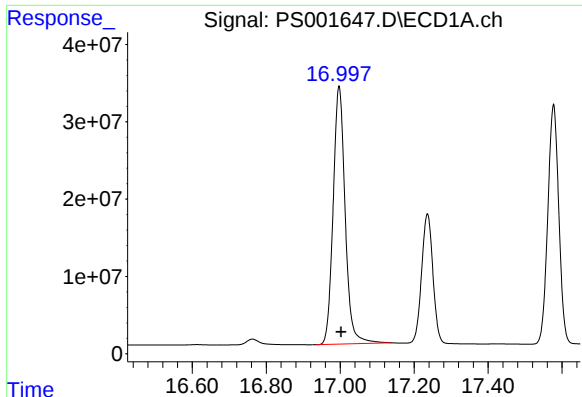

#15 Picloram


R.T.: 16.997 min
Delta R.T.: -0.006 min
Response: 753605203
Conc: 538.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

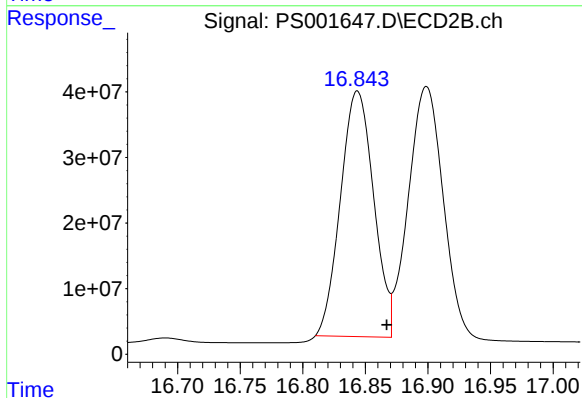


#15 Picloram

R.T.: 16.844 min
Delta R.T.: -0.024 min
Response: 691204906
Conc: 530.08 ng/ml

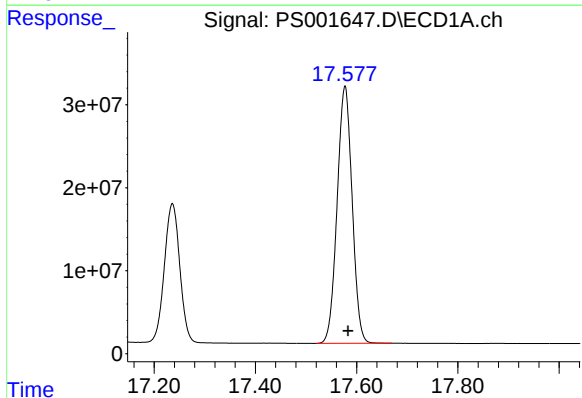

#16 DCPA

R.T.: 17.577 min
Delta R.T.: -0.006 min
Response: 638024391
Conc: 562.31 ng/ml

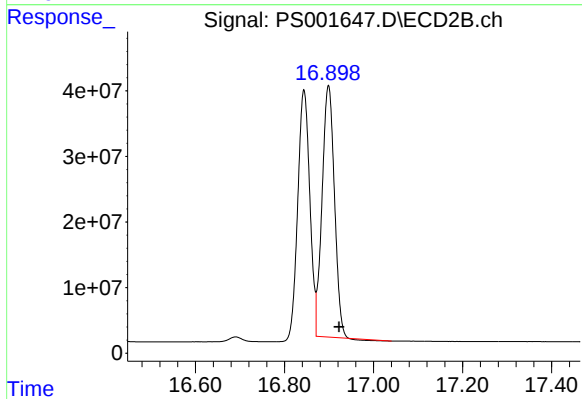

#16 DCPA

R.T.: 16.899 min
Delta R.T.: -0.024 min
Response: 735177496
Conc: 514.92 ng/ml