

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083018\
 Data File : PS001651.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2018 14:31
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 01:02:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.475	10.973	104.1E6	97031528	563.865	479.097
Target Compounds							
10) T	Pentachlo...	13.718	0.000	2485145	0	0.997	N.D. #
12) T	2,4,5-T	0.000	14.594	0	14662339	N.D.	16.973 #
15) T	Picloram	16.992	16.909	41337376	35695140	29.514	27.375
16) T	DCPA	0.000	16.909	0	35695140	N.D.	25.001 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083018\
Data File : PS001651.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2018 14:31
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 01:02:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

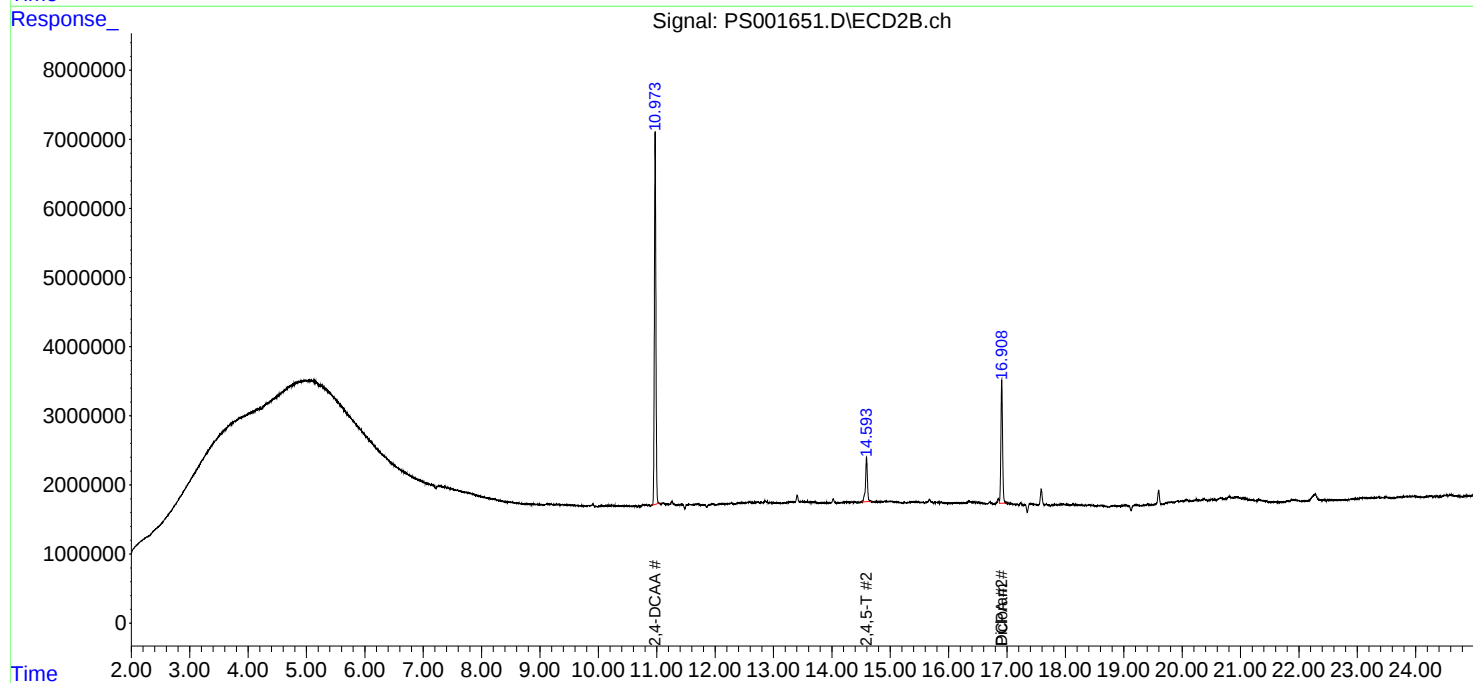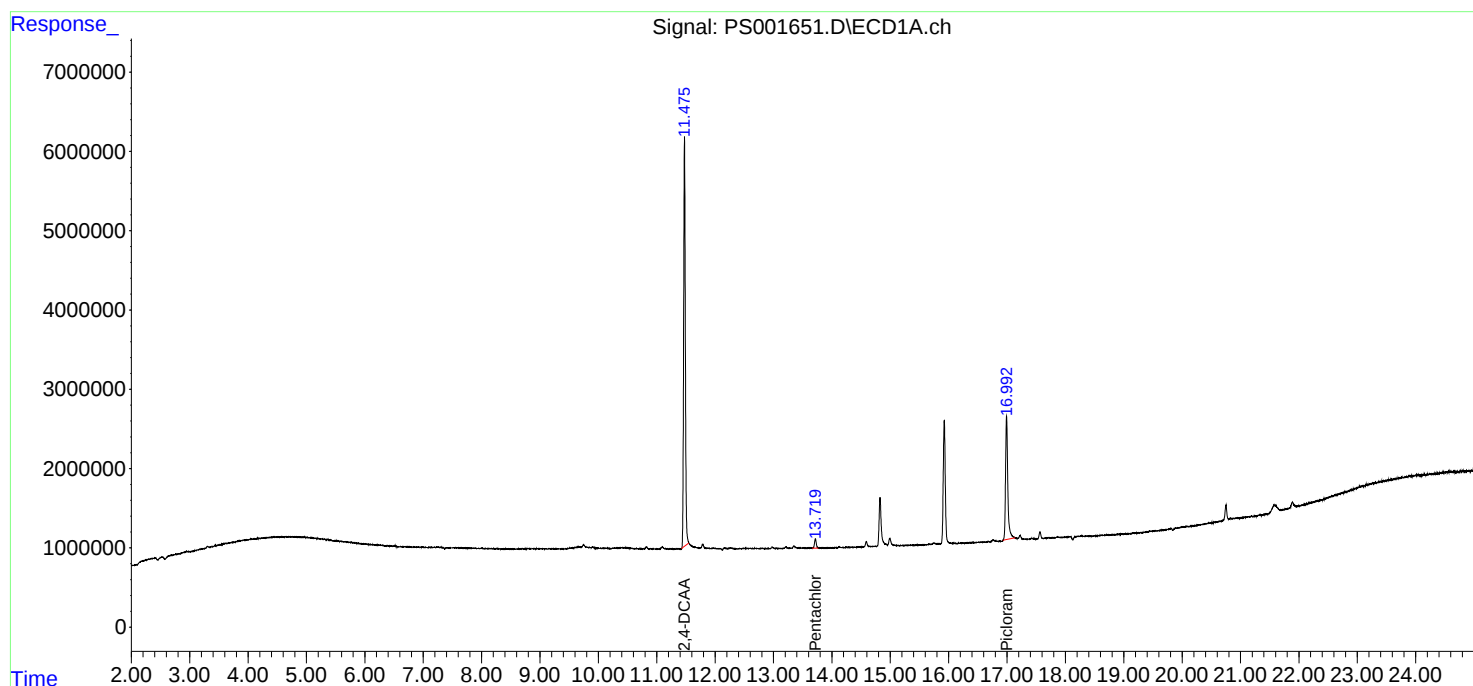


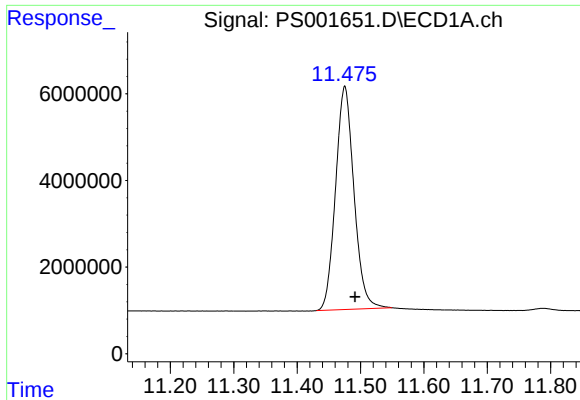

#4 2,4-DCAA


R.T.: 11.475 min
Delta R.T.: -0.016 min
Response: 104089678
Conc: 563.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

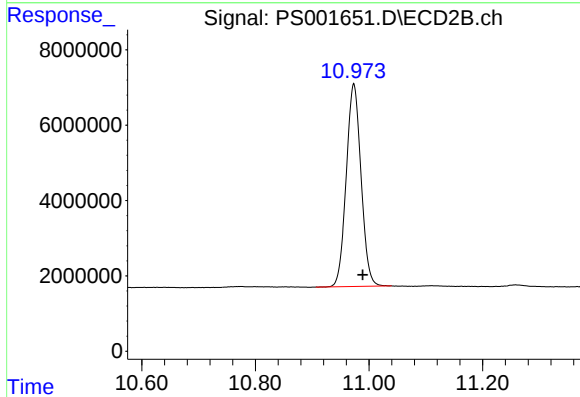


#4 2,4-DCAA

R.T.: 10.973 min
Delta R.T.: -0.016 min
Response: 97031528
Conc: 479.10 ng/ml

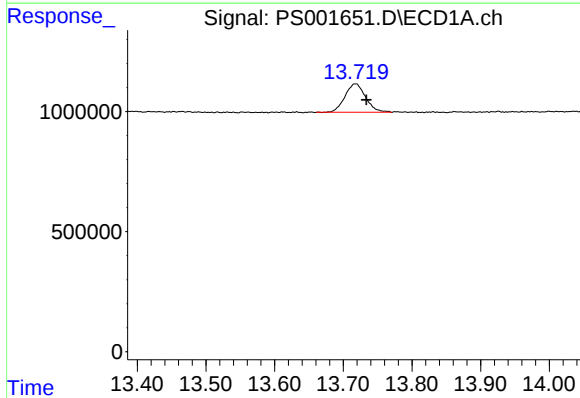


#10 Pentachlorophenol

R.T.: 13.718 min
Delta R.T.: -0.016 min
Response: 2485145
Conc: 1.00 ng/ml

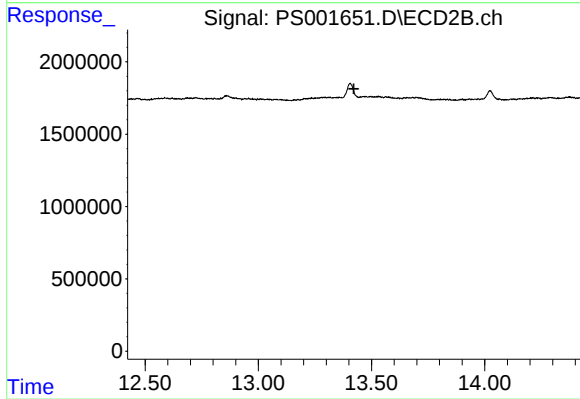

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.422 min
Response: 0
Conc: N.D.

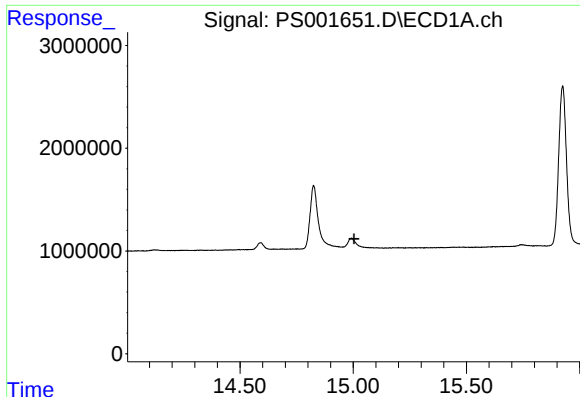

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.003 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

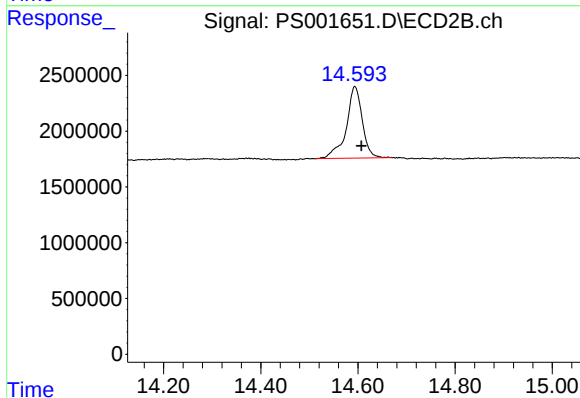


#12 2,4,5-T

R.T.: 14.594 min
Delta R.T.: -0.014 min
Response: 14662339
Conc: 16.97 ng/ml

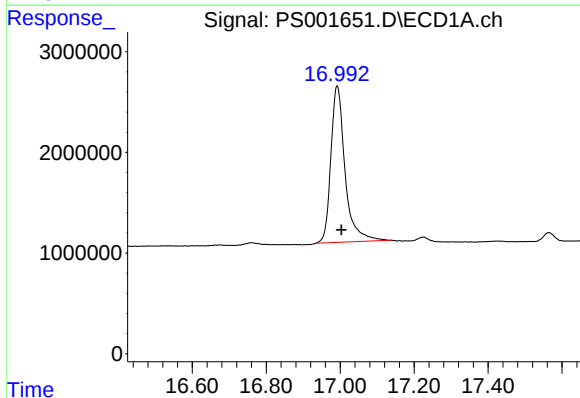


#15 Picloram

R.T.: 16.992 min
Delta R.T.: -0.011 min
Response: 41337376
Conc: 29.51 ng/ml

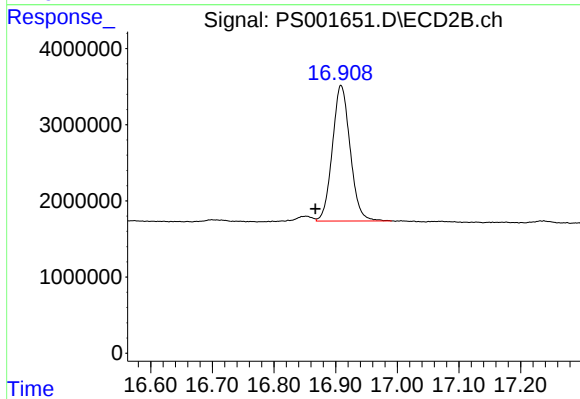

#15 Picloram


R.T.: 16.909 min
Delta R.T.: 0.041 min
Response: 35695140
Conc: 27.37 ng/ml

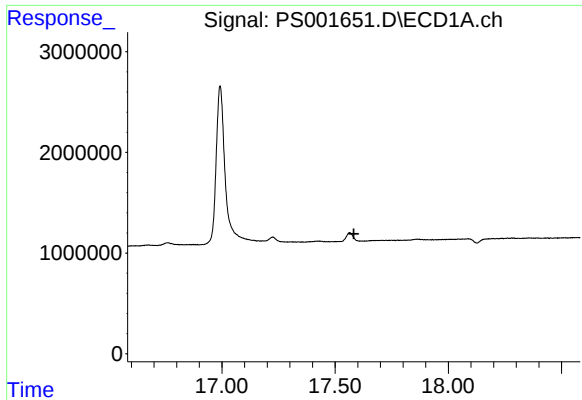

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.583 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

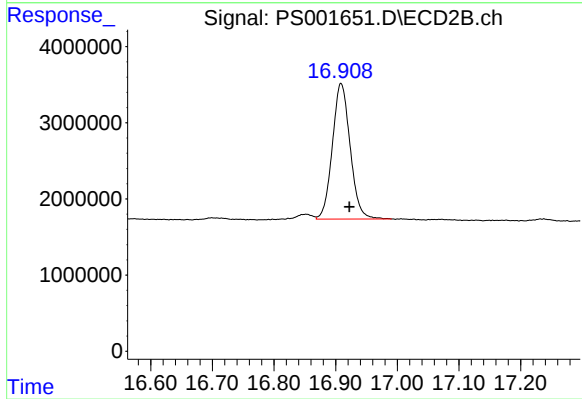

#16 DCPA

R.T.: 16.909 min
Delta R.T.: -0.014 min
Response: 35695140
Conc: 25.00 ng/ml