

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083019\
 Data File : PS006428.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2019 08:42
 Operator : SM\AJ
 Sample : K4526-22
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 T9-12-13-D-(0-1.9)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 00:13:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.482	5.211	530.0E6	316.3E6	614.003	643.153
Target Compounds							
1) T	Dalapon	2.115	1.742	26769189	44132389	24.567	70.331 #
2) T	3,5-DICHL...	0.000	4.540	0	40413384	N.D.	66.721
9) T	2,4-D	6.545	0.000	154.3E6	0	189.422	N.D. #
15) T	Picloram	9.039	8.991	28226031	19361385	3.794	4.292
16) T	DCPA	0.000	8.991	0	19361385	N.D.	5.552



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083019\
Data File : PS006428.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2019 08:42
Operator : SM\AJ
Sample : K4526-22
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
T9-12-13-D-(0-1.9)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 00:13:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

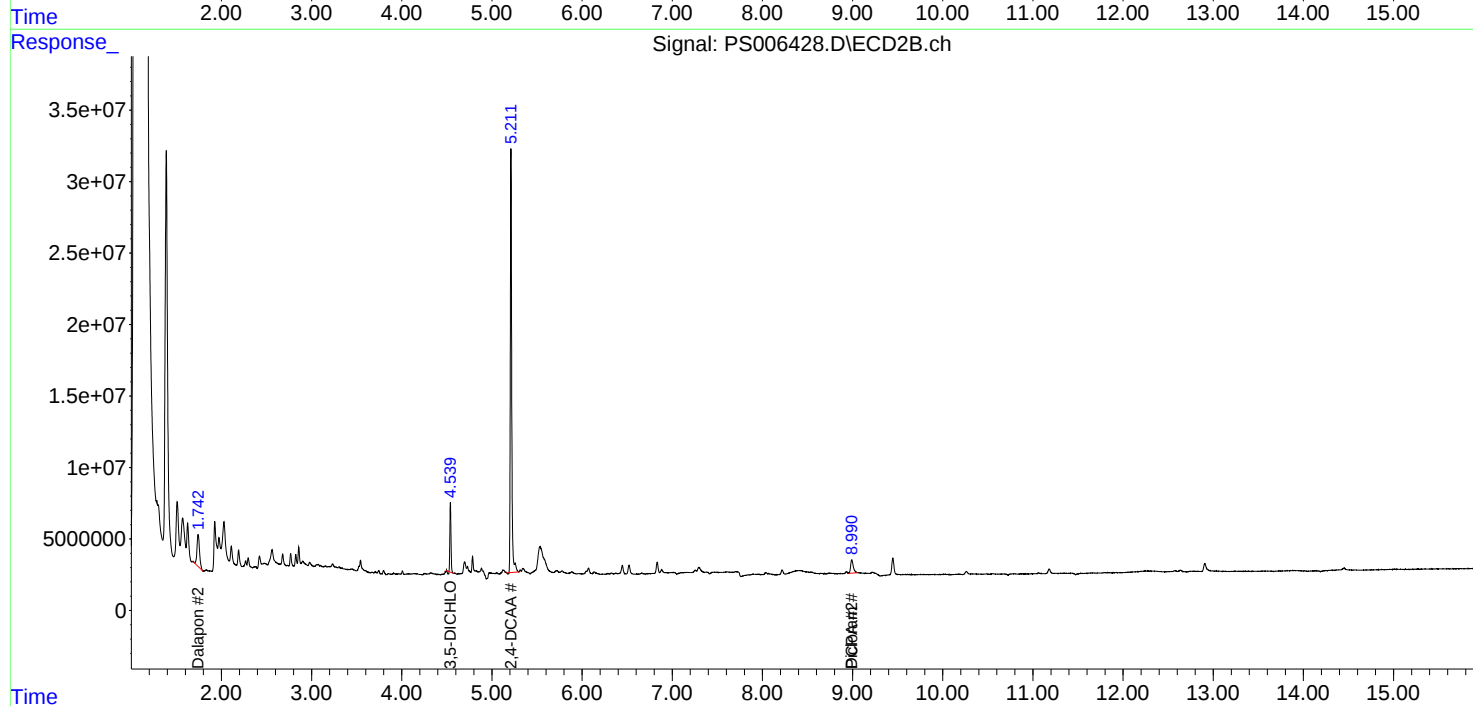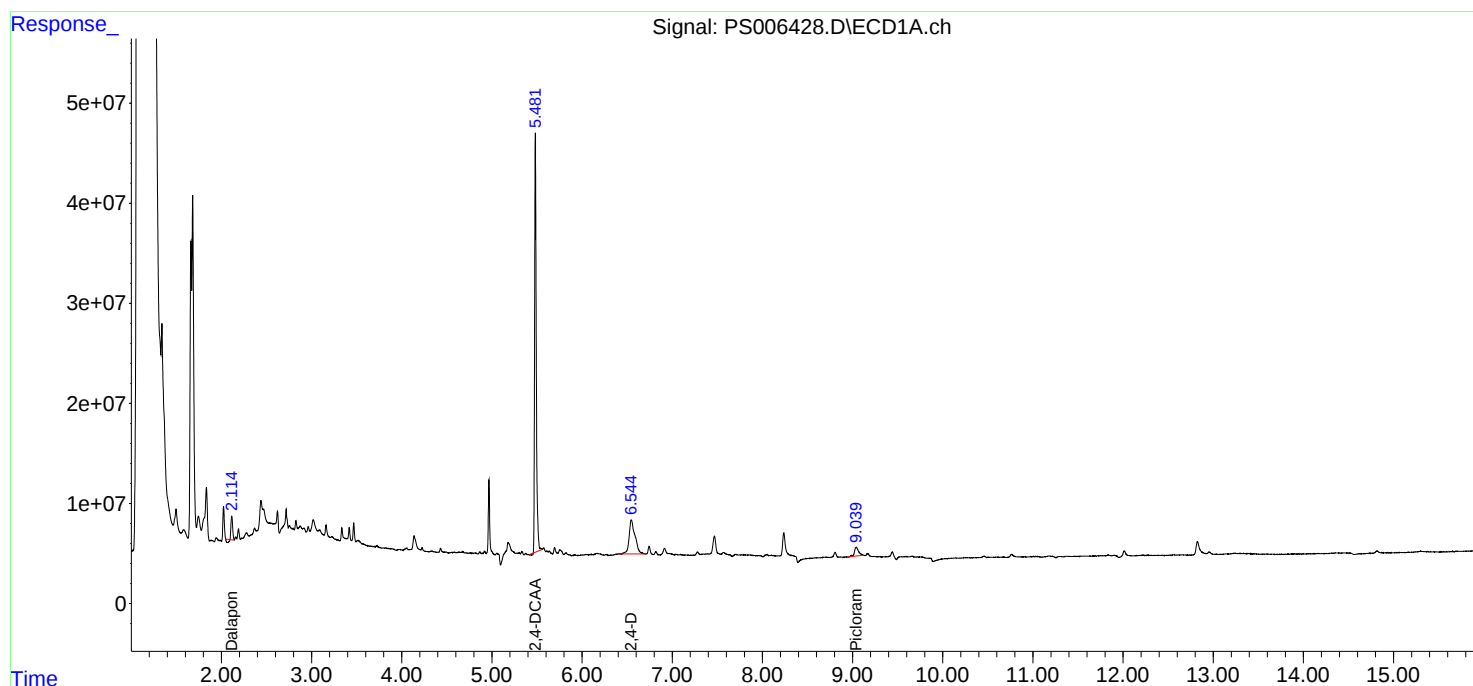


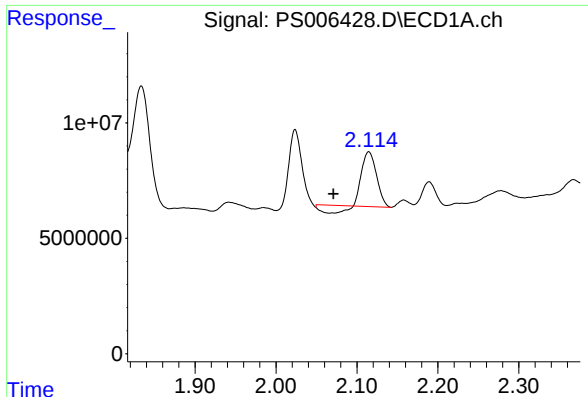

#1 Dalapon


R.T.: 2.115 min
Delta R.T.: 0.044 min
Response: 26769189
Conc: 24.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
T9-12-13-D-(0-1.9)

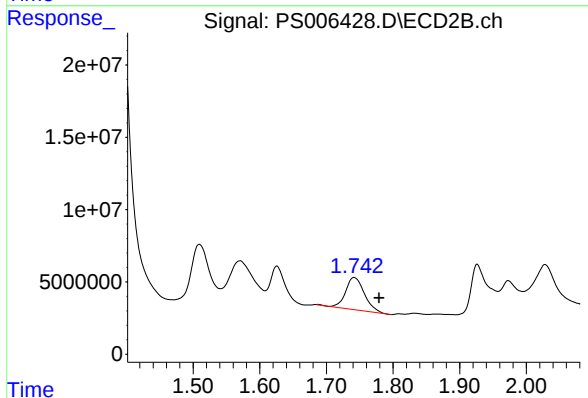


#1 Dalapon

R.T.: 1.742 min
Delta R.T.: -0.037 min
Response: 44132389
Conc: 70.33 ng/ml

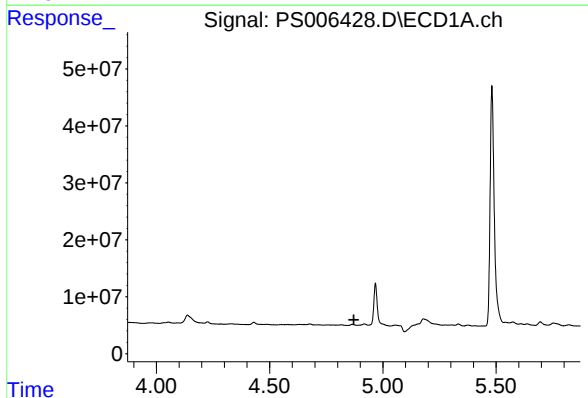


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.872 min
Response: 0
Conc: N.D.

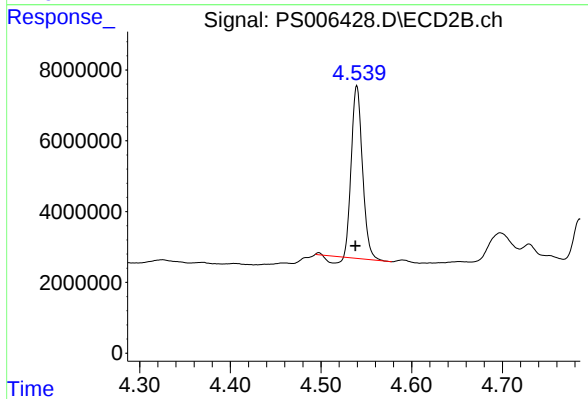

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.540 min
Delta R.T.: 0.002 min
Response: 40413384
Conc: 66.72 ng/ml

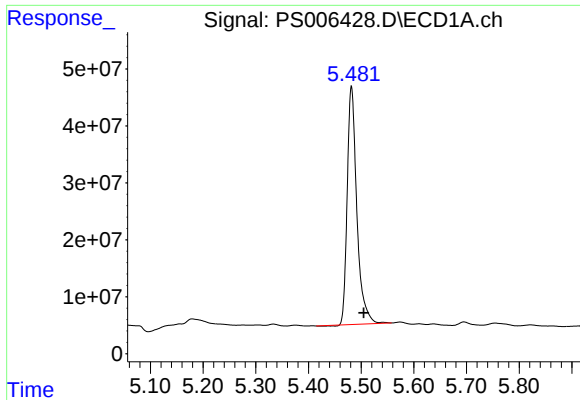

#4 2,4-DCAA


R.T.: 5.482 min
Delta R.T.: -0.023 min
Response: 530008236
Conc: 614.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
T9-12-13-D-(0-1.9)

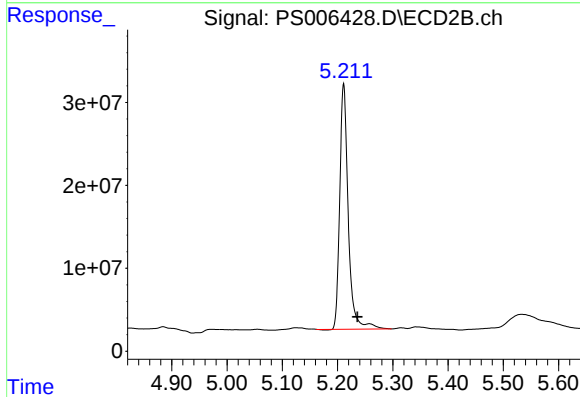


#4 2,4-DCAA

R.T.: 5.211 min
Delta R.T.: -0.025 min
Response: 316335783
Conc: 643.15 ng/ml

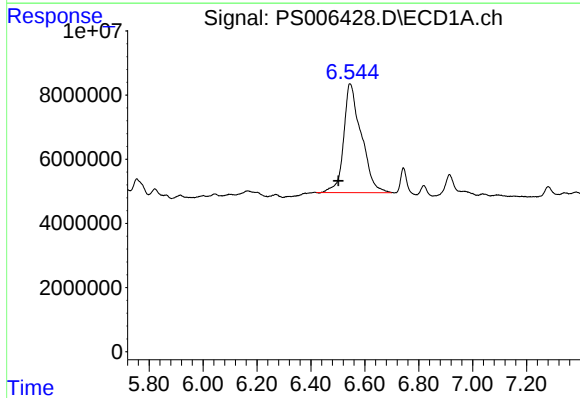


#9 2,4-D

R.T.: 6.545 min
Delta R.T.: 0.042 min
Response: 154337981
Conc: 189.42 ng/ml

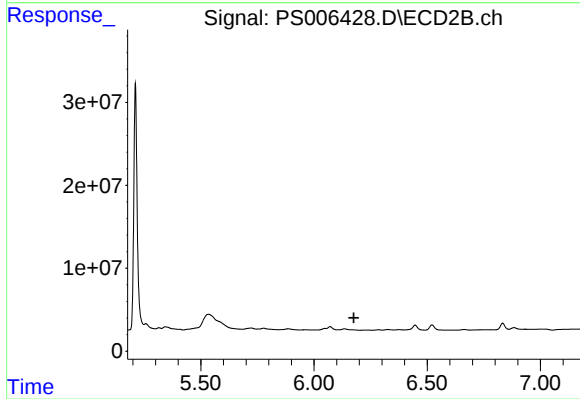

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.176 min
Response: 0
Conc: N.D.

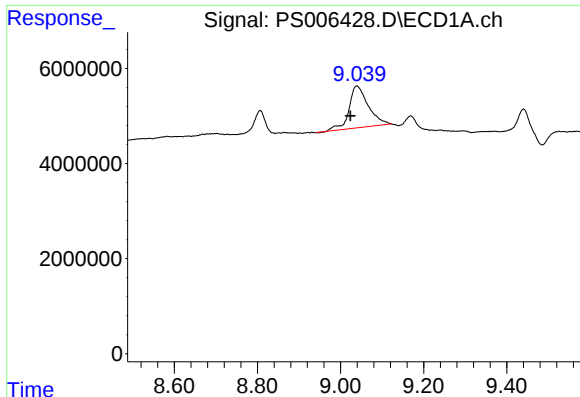

#15 Picloram


R.T.: 9.039 min
Delta R.T.: 0.016 min
Response: 28226031
Conc: 3.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
T9-12-13-D-(0-1.9)

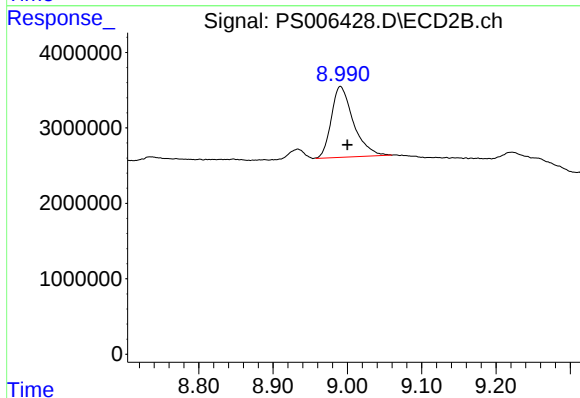


#15 Picloram

R.T.: 8.991 min
Delta R.T.: -0.009 min
Response: 19361385
Conc: 4.29 ng/ml

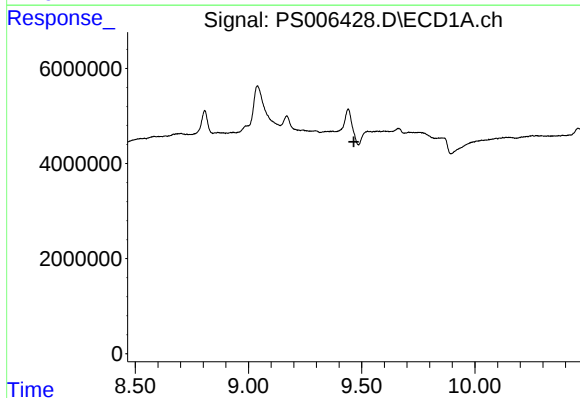

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.465 min
Response: 0
Conc: N.D.

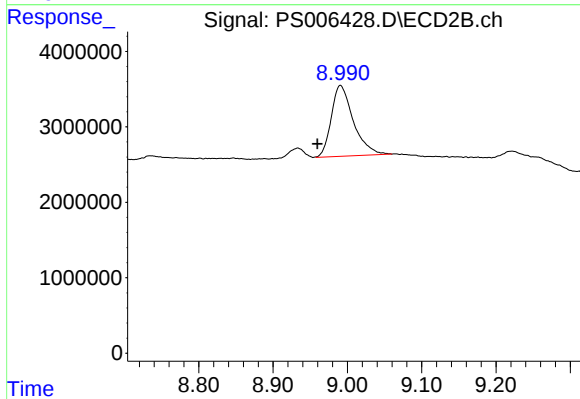

#16 DCPA

R.T.: 8.991 min
Delta R.T.: 0.031 min
Response: 19361385
Conc: 5.55 ng/ml