

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083019\
 Data File : PS006457.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2019 19:31
 Operator : SM\AJ
 Sample : K4439-06
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 S-3-(1-3)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 00:21:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.485	5.215	163.7E6	85846849	189.686	174.538
Target Compounds							
1) T	Dalapon	2.118	1.742	6526536	172.1E6	5.990	274.241 #
7) T	MCPA	5.961	5.591	16253168	34865754	5.148	17.060 #
9) T	2,4-D	6.550	0.000	218.8E6	0	268.485	N.D. #
10) T	Pentachlo...	6.822	0.000	17420751	0	1.474	N.D. #
13) T	2,4-DB	8.143	0.000	92154403	0	147.971	N.D. #
15) T	Picloram	0.000	9.029	0	27542229	N.D.	6.106
16) T	DCPA	0.000	9.029	0	27542229	N.D.	7.898



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083019\
Data File : PS006457.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2019 19:31
Operator : SM\AJ
Sample : K4439-06
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
S-3-(1-3)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 00:21:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

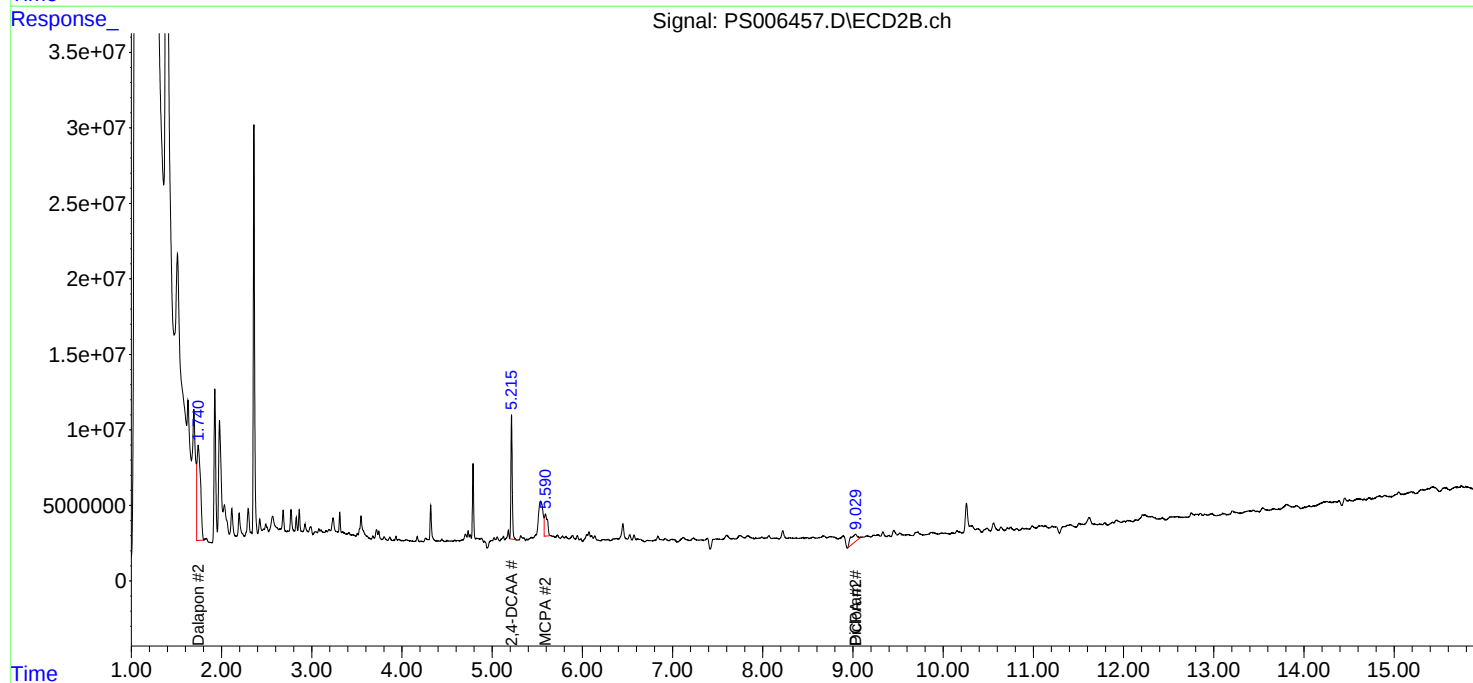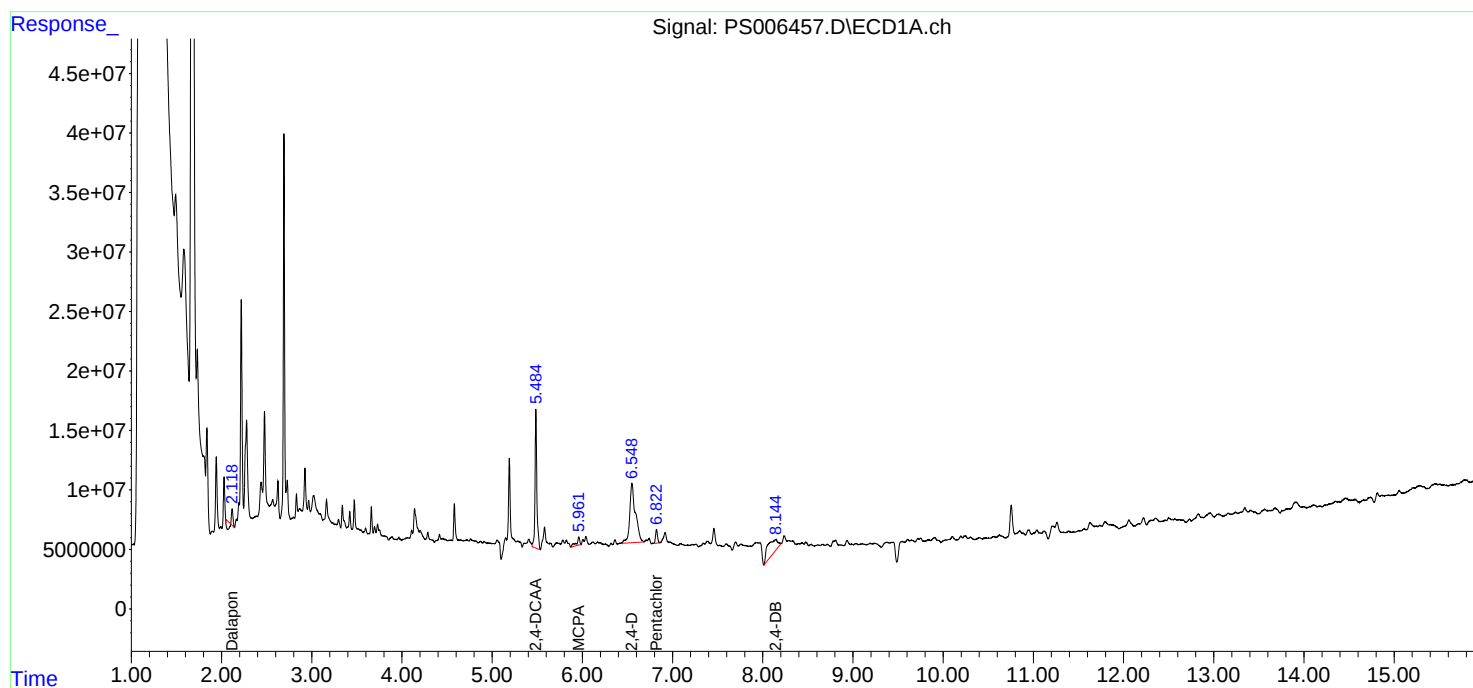


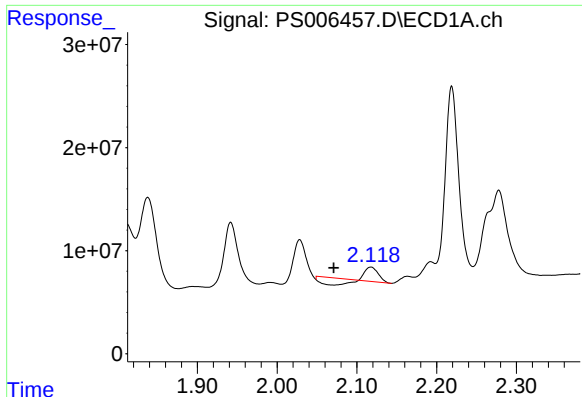

#1 Dalapon


R.T.: 2.118 min
Delta R.T.: 0.047 min
Response: 6526536
Conc: 5.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
S-3-(1-3)

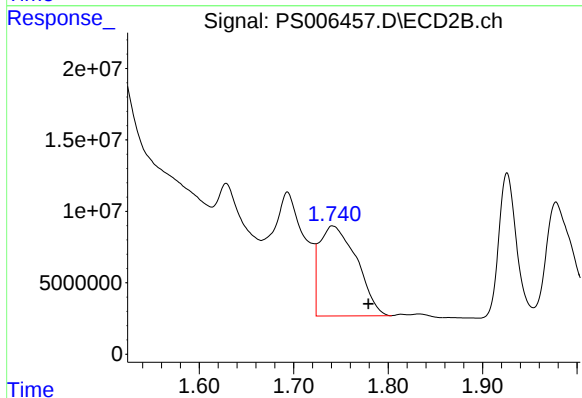


#1 Dalapon

R.T.: 1.742 min
Delta R.T.: -0.038 min
Response: 172084480
Conc: 274.24 ng/ml

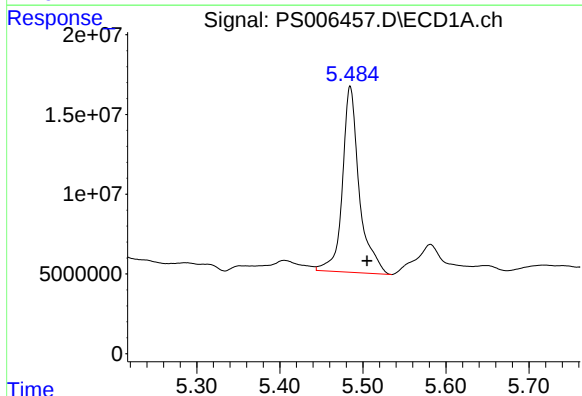


#4 2,4-DCAA

R.T.: 5.485 min
Delta R.T.: -0.020 min
Response: 163737343
Conc: 189.69 ng/ml

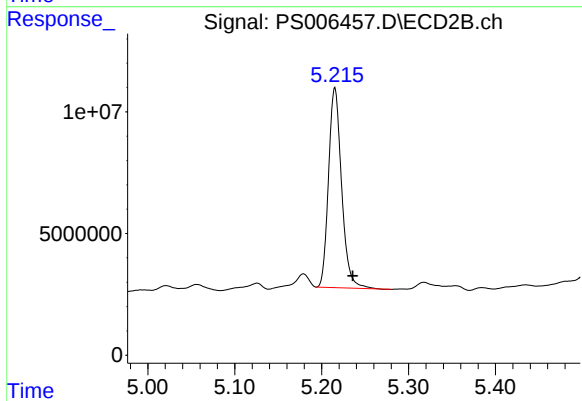

#4 2,4-DCAA


R.T.: 5.215 min
Delta R.T.: -0.020 min
Response: 85846849
Conc: 174.54 ng/ml

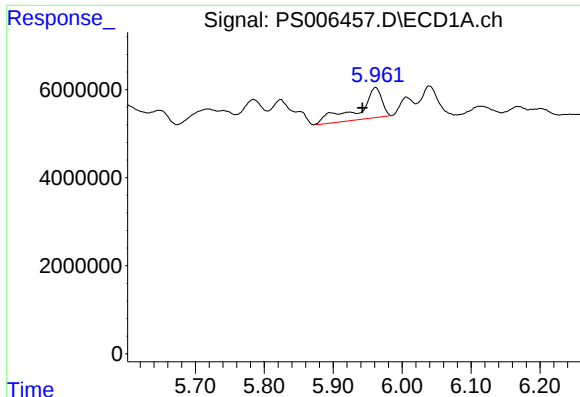

#7 MCPA


R.T.: 5.961 min
Delta R.T.: 0.019 min
Response: 16253168
Conc: 5.15 ug/ml

Instrument :
ECD_S
ClientSampleId :
S-3-(1-3)

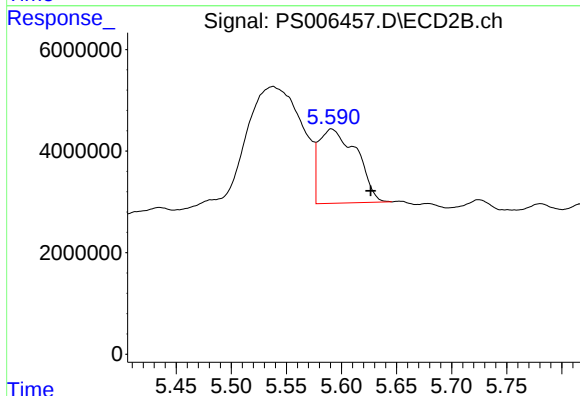


#7 MCPA

R.T.: 5.591 min
Delta R.T.: -0.035 min
Response: 34865754
Conc: 17.06 ug/ml

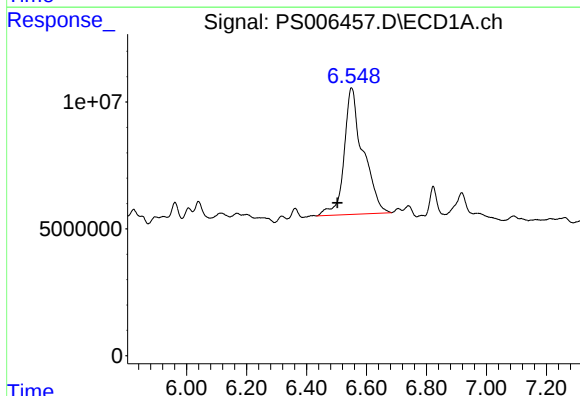


#9 2,4-D

R.T.: 6.550 min
Delta R.T.: 0.047 min
Response: 218757086
Conc: 268.48 ng/ml

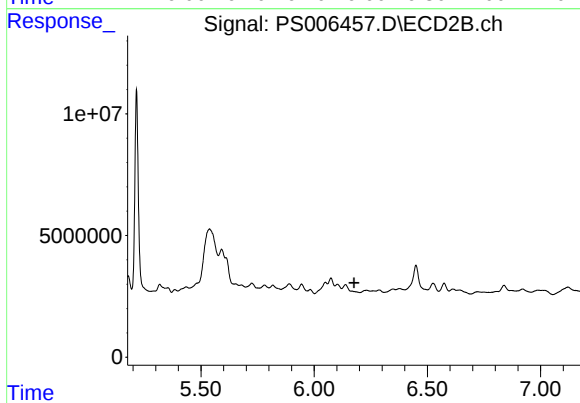

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.176 min
Response: 0
Conc: N.D.

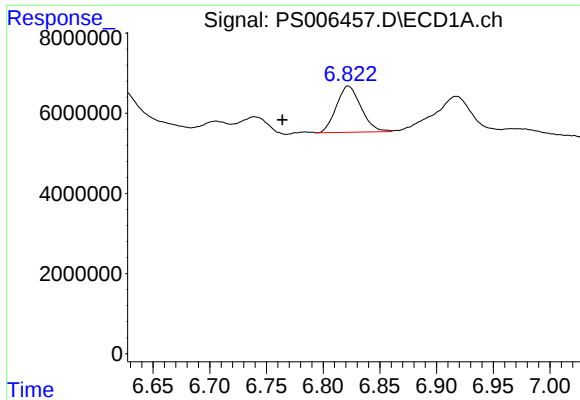

#10 Pentachlorophenol


R.T.: 6.822 min
Delta R.T.: 0.058 min
Response: 17420751
Conc: 1.47 ng/ml

Instrument :
ECD_S
ClientSampleId :
S-3-(1-3)

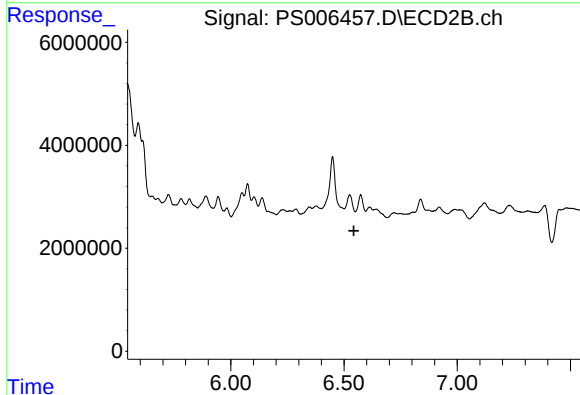


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.544 min
Response: 0
Conc: N.D.

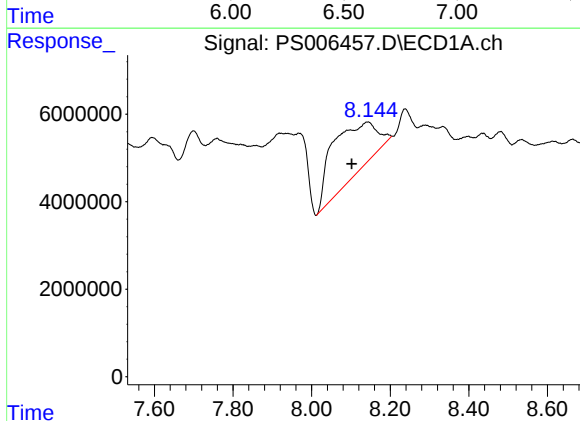


#13 2,4-DB

R.T.: 8.143 min
Delta R.T.: 0.040 min
Response: 92154403
Conc: 147.97 ng/ml

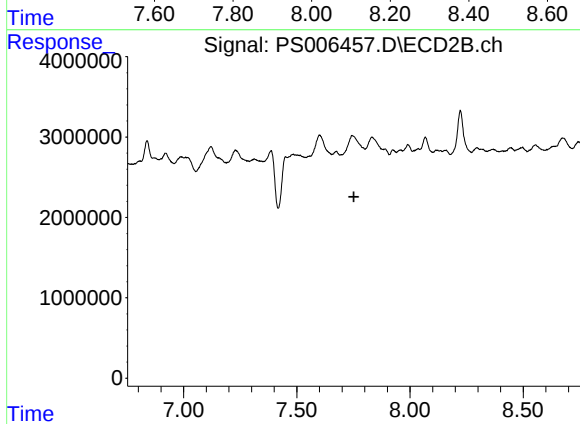

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 7.752 min
Response: 0
Conc: N.D.

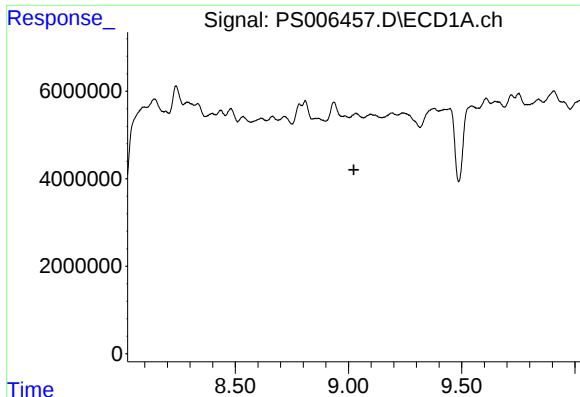

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 9.024 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S-3-(1-3)

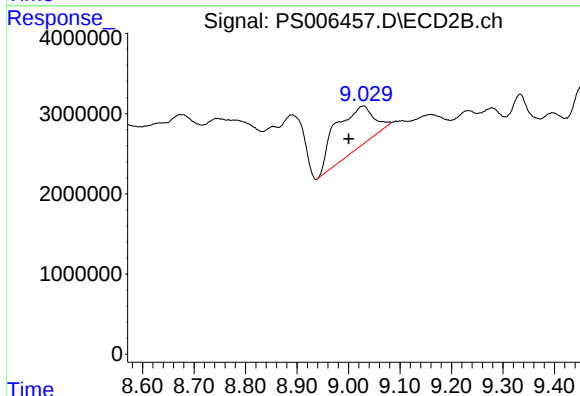


#15 Picloram

R.T.: 9.029 min
Delta R.T.: 0.028 min
Response: 27542229
Conc: 6.11 ng/ml

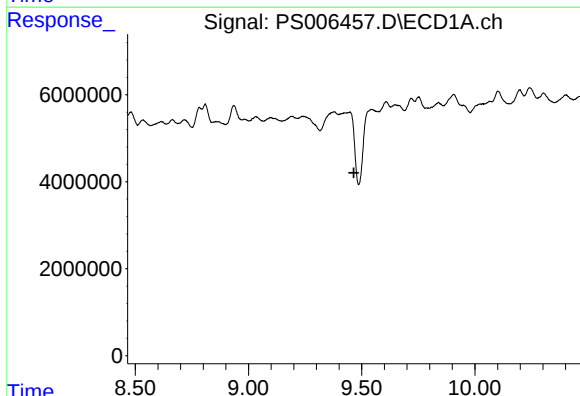

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.465 min
Response: 0
Conc: N.D.

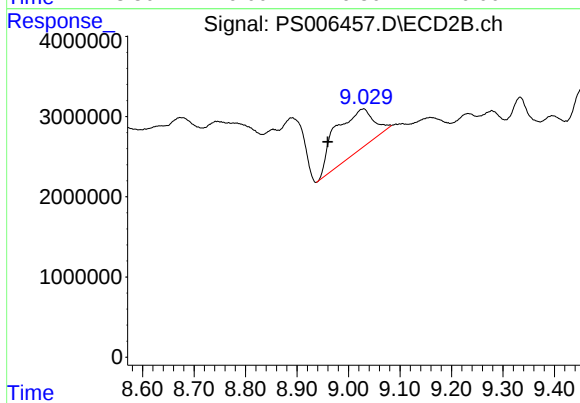

#16 DCPA

R.T.: 9.029 min
Delta R.T.: 0.069 min
Response: 27542229
Conc: 7.90 ng/ml