

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083024\
 Data File : PS027569.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2024 09:37
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 02:55:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081924.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 19 14:50:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.152	7.734	1294.5E6	1039.2E6	500.540	526.405
Target Compounds							
1) T	Dalapon	0.000	2.723f	0	223646	N.D.	<MDL
3) T	4-Nitroph...	6.946	0.000	10789439	0	6.929	N.D. #
5) T	DICAMBA	0.000	7.929	0	5575729	N.D.	<MDL
6) T	MCP	0.000	8.034	0	6278397	N.D.	1.031
8) T	DICHLORPROP	8.087f	8.635	2095668	615304	<MDL	<MDL #
9) T	2,4-D	8.261	0.000	32877875	0	11.280	N.D. #
10) T	Pentachlo...	0.000	9.501	0	1323618	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	9.881	0	2219496	N.D.	<MDL
12) T	2,4,5-T	9.405	10.293	6186696	1882640	<MDL	<MDL #
13) T	2,4-DB	10.027f	0.000	9657912	0	4.517	N.D. #
14) T	DINOSEB	0.000	11.234	0	294434	N.D.	<MDL
15) T	Picloram	10.987	12.330	75025317	50251420	3.734	2.567 #
16) T	DCPA	0.000	12.232f	0	3962684	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083024\
Data File : PS027569.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2024 09:37
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 02:55:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081924.M
Quant Title : 8080.M
QLast Update : Mon Aug 19 14:50:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

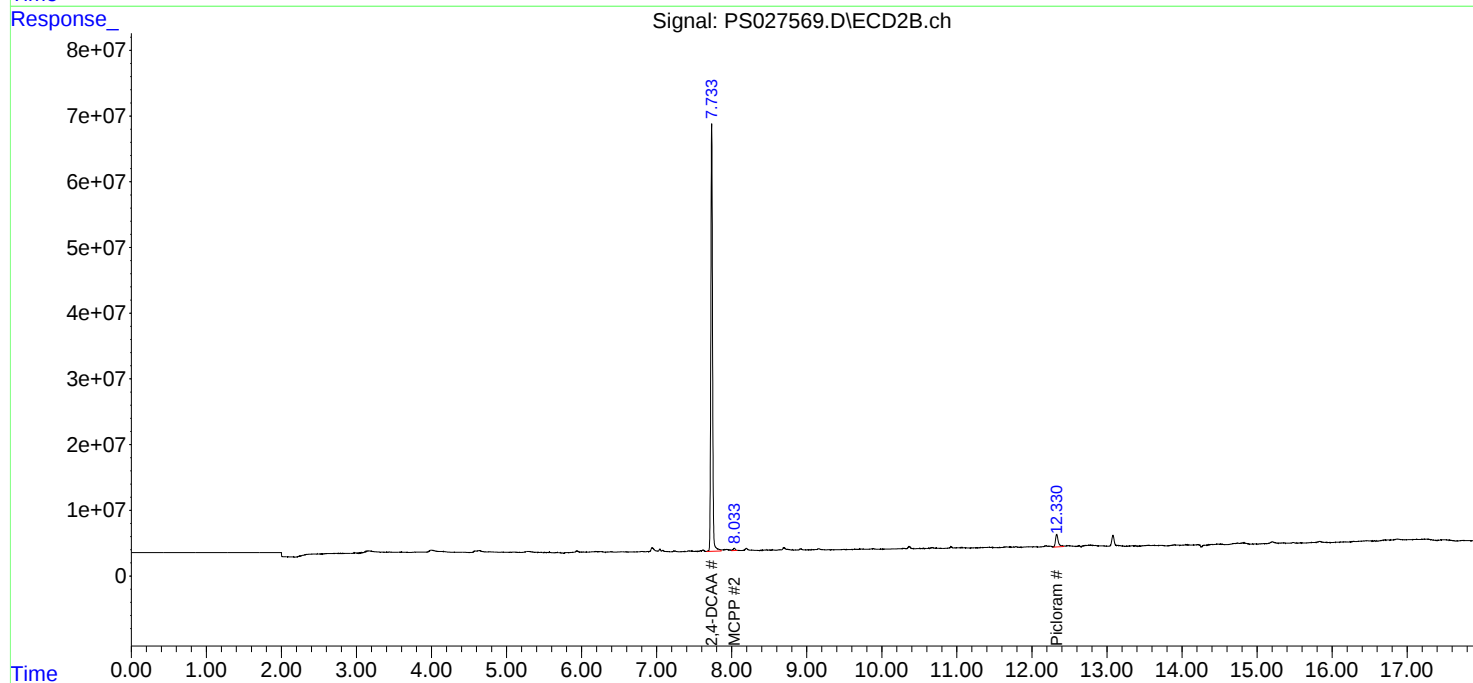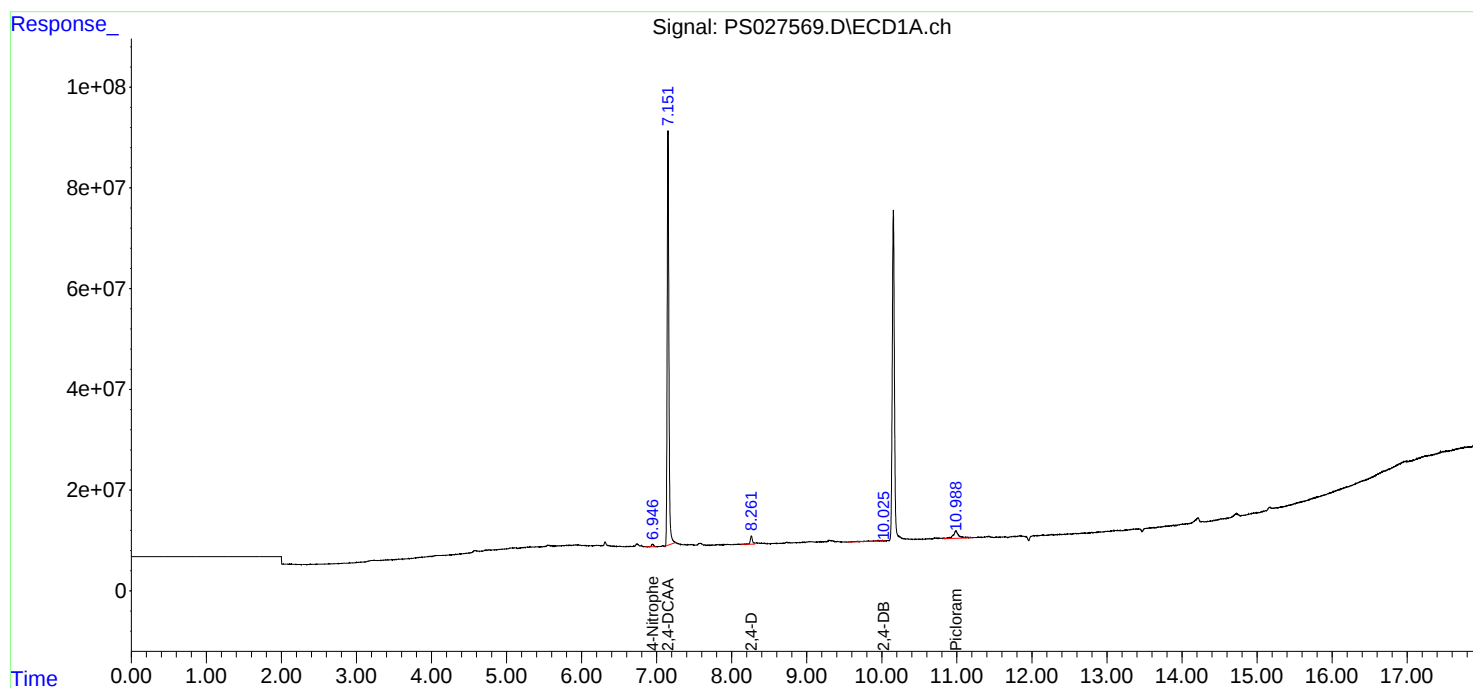


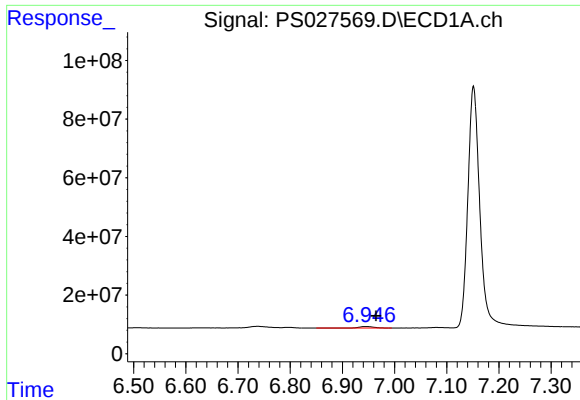

#3 4-Nitrophenol


R.T.: 6.946 min
Delta R.T.: -0.019 min
Response: 10789439
Conc: 6.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

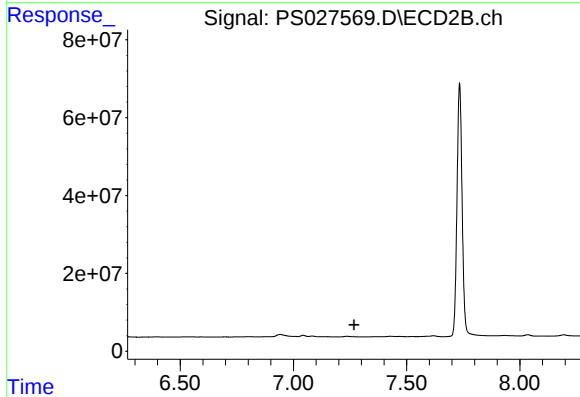


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.267 min
Response: 0
Conc: N.D.

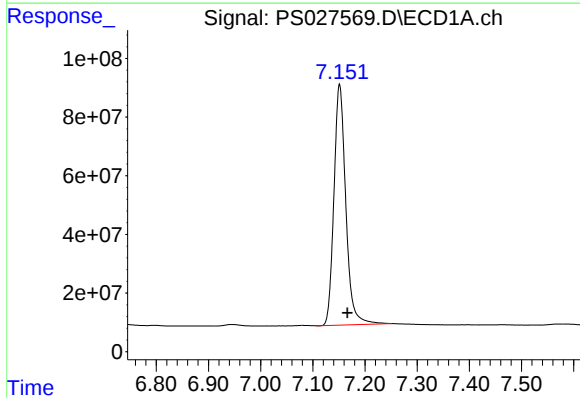


#4 2,4-DCAA

R.T.: 7.152 min
Delta R.T.: -0.014 min
Response: 1294526606
Conc: 500.54 ng/ml

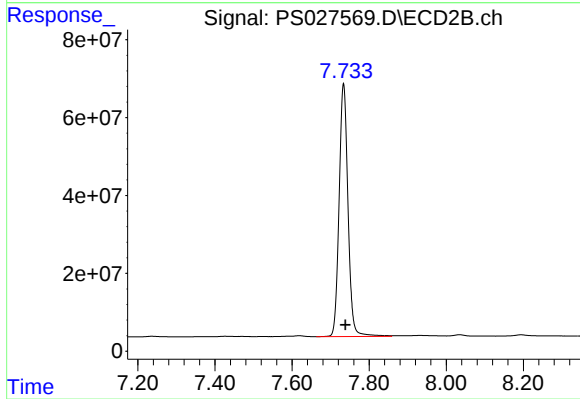

#4 2,4-DCAA


R.T.: 7.734 min
Delta R.T.: -0.005 min
Response: 1039246892
Conc: 526.41 ng/ml

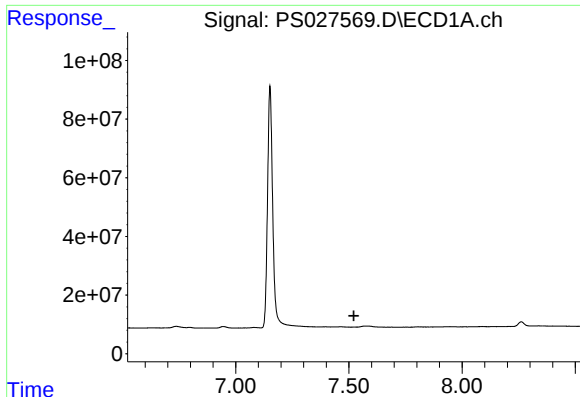

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.522 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

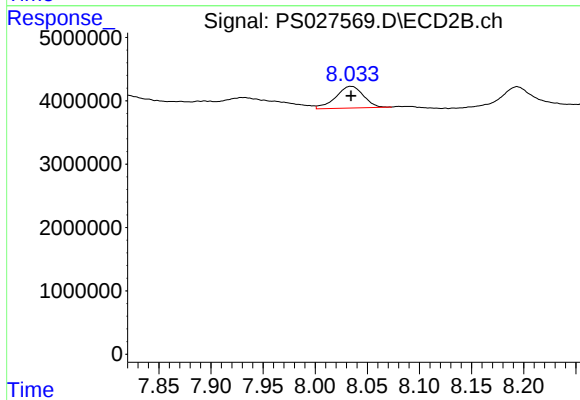


#6 MCPP

R.T.: 8.034 min
Delta R.T.: 0.000 min
Response: 6278397
Conc: 1.03 ug/ml

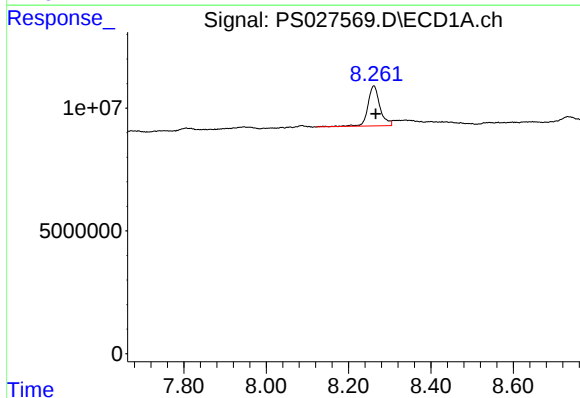


#9 2,4-D

R.T.: 8.261 min
Delta R.T.: -0.005 min
Response: 32877875
Conc: 11.28 ng/ml

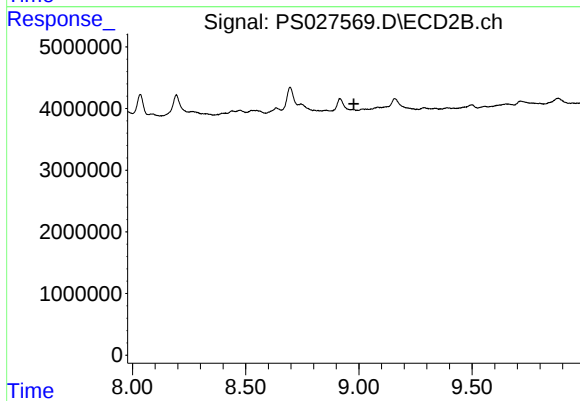

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.978 min
Response: 0
Conc: N.D.

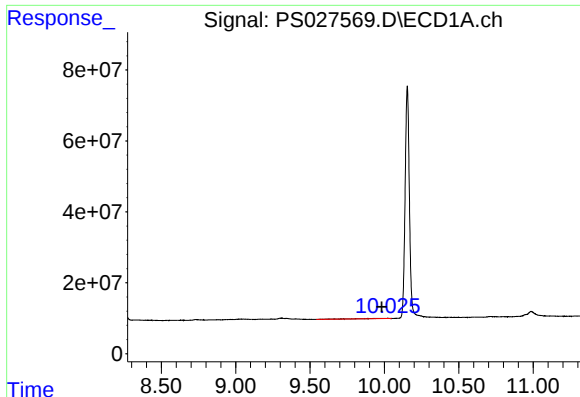

#13 2,4-DB


R.T.: 10.027 min
Delta R.T.: 0.044 min
Response: 9657912
Conc: 4.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

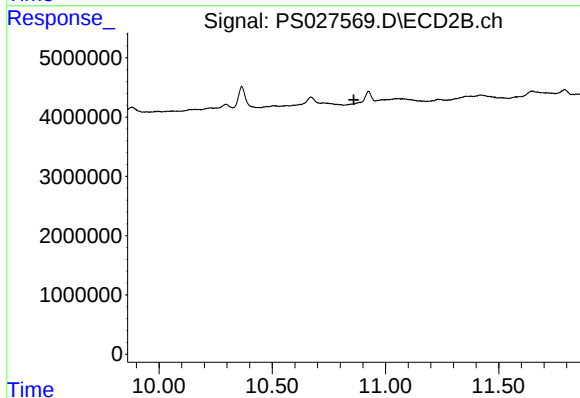


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.861 min
Response: 0
Conc: N.D.

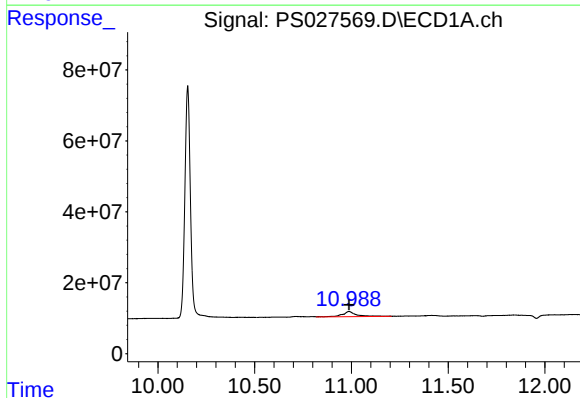

#15 Picloram

R.T.: 10.987 min
Delta R.T.: 0.000 min
Response: 75025317
Conc: 3.73 ng/ml

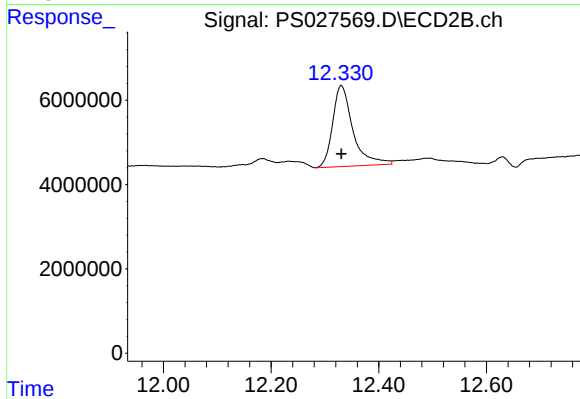

#15 Picloram

R.T.: 12.330 min
Delta R.T.: 0.000 min
Response: 50251420
Conc: 2.57 ng/ml